

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021723\
 Data File : VX034155.D
 Acq On : 17 Feb 2023 13:52
 Operator : JC/MD
 Sample : VX0217WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0217WBL01

Quant Time: Feb 17 14:18:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 17 12:33:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	399233	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	671044	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	578571	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	250598	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	254490	47.332	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.660%
35) Dibromofluoromethane	5.385	113	212489	48.634	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.260%
50) Toluene-d8	8.647	98	804696	51.298	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	102.600%
62) 4-Bromofluorobenzene	11.079	95	284086	47.346	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021723\
Data File : VX034155.D
Acq On : 17 Feb 2023 13:52
Operator : JC/MD
Sample : VX0217WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0217WBL01

Quant Time: Feb 17 14:18:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 17 12:33:35 2023
Response via : Initial Calibration




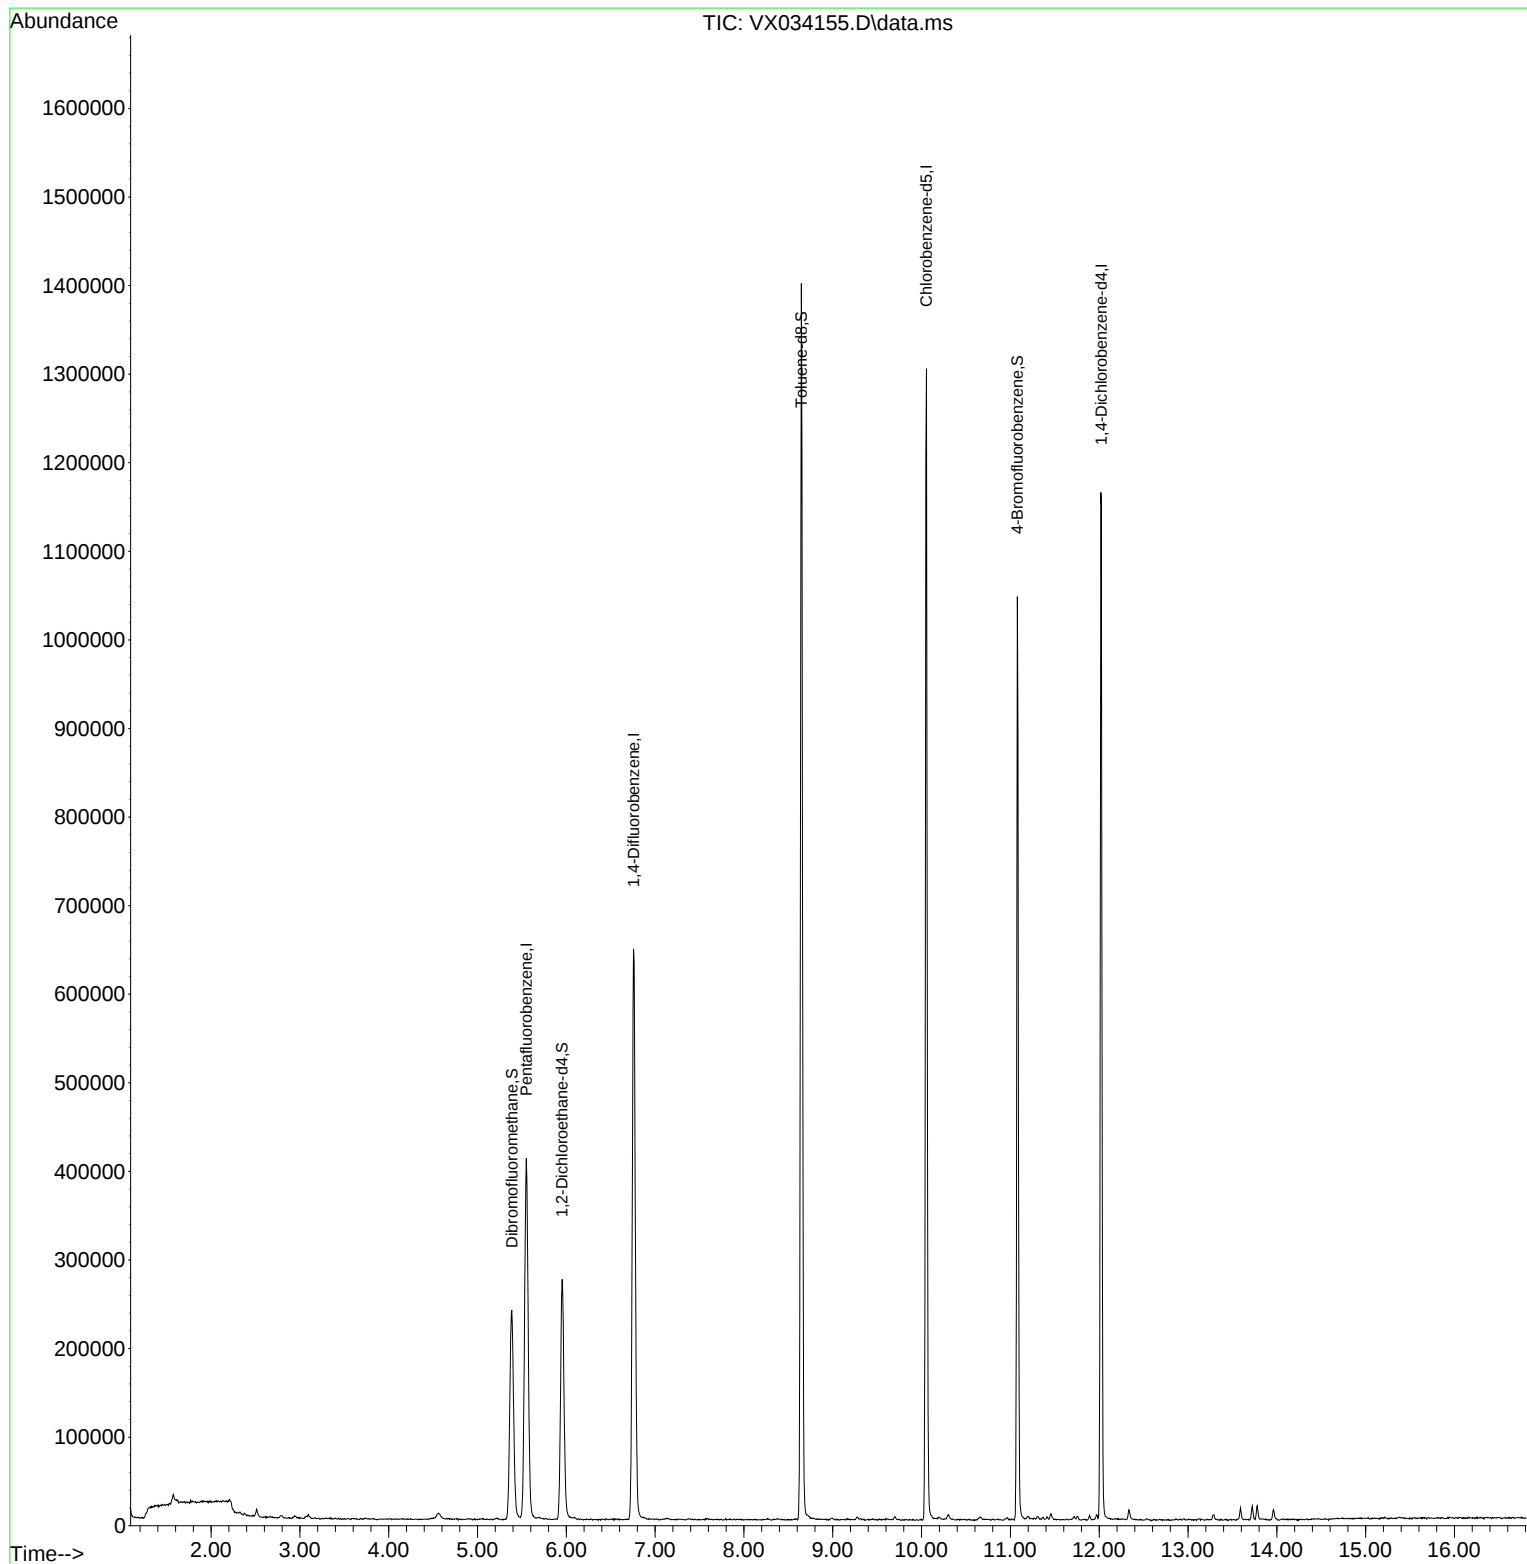


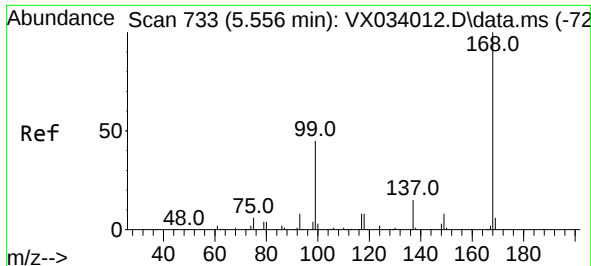

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.000 min
Lab File: VX034155.D
Acq: 17 Feb 2023 13:52




Instrument :
MSVOA_X
ClientSampleId :
VX0217WBL01


Tgt Ion:168 Resp: 399233
Ion Ratio Lower Upper
168 100
99 55.8 39.6 59.4

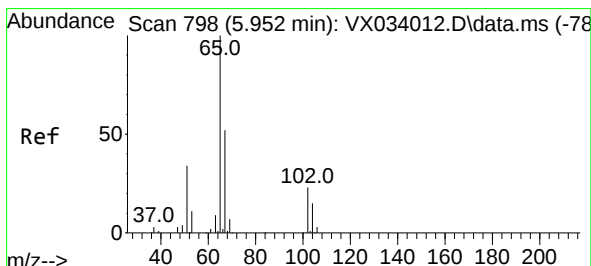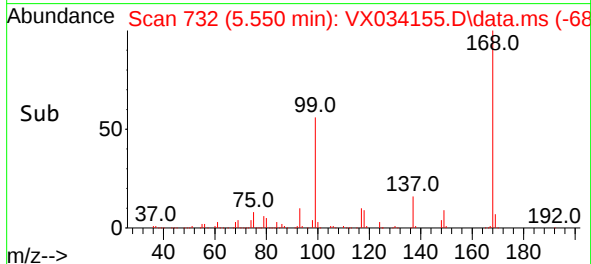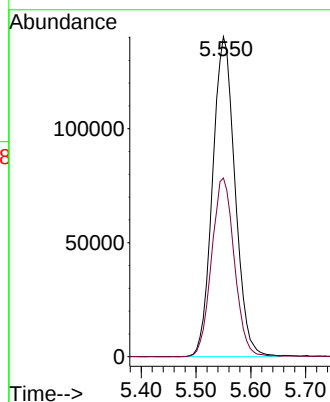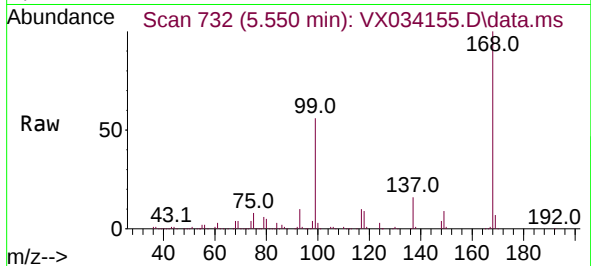

#33
1,2-Dichloroethane-d4
Concen: 47.332 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX034155.D
Acq: 17 Feb 2023 13:52

Tgt Ion: 65 Resp: 254490
Ion Ratio Lower Upper
65 100
67 53.1 0.0 104.8


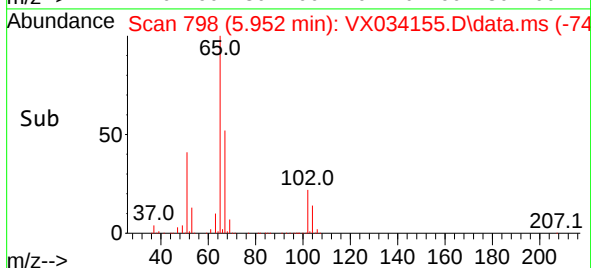
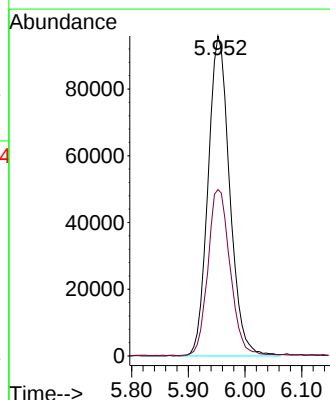
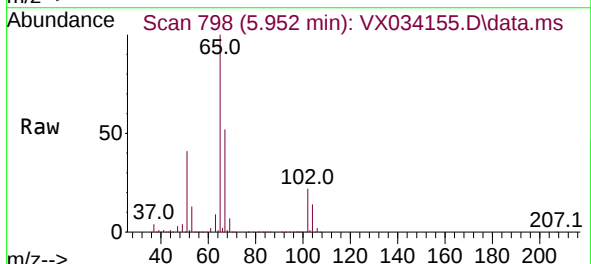


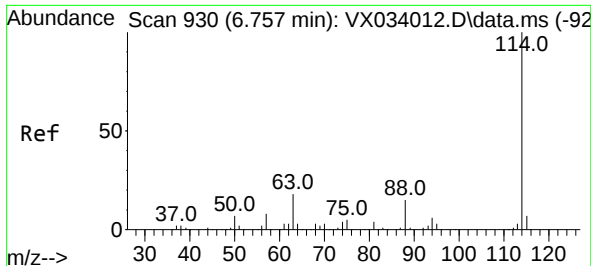

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX034155.D
Acq: 17 Feb 2023 13:52




Instrument :
MSVOA_X
ClientSampleId :
VX0217WBL01


Tgt Ion:114 Resp: 671044
Ion Ratio Lower Upper
114 100
63 22.3 0.0 37.4
88 16.9 0.0 30.6

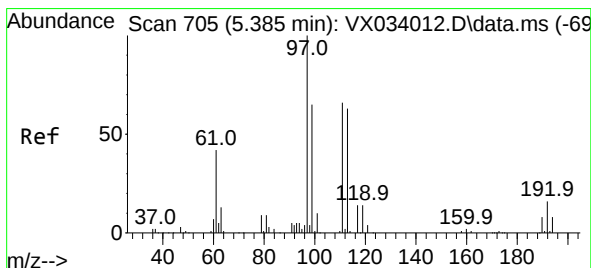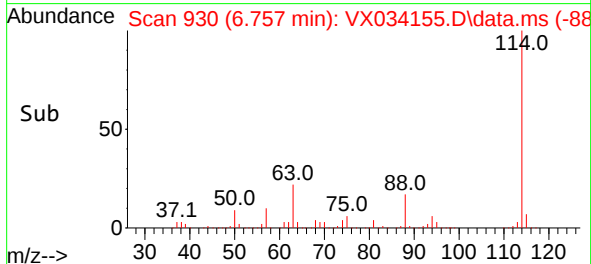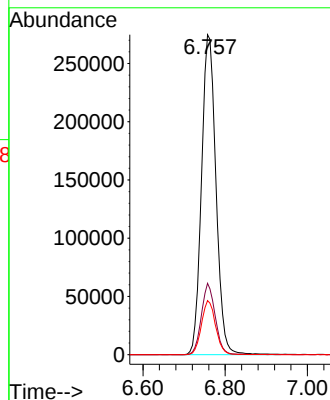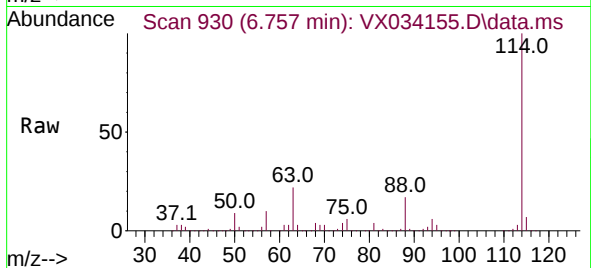

#35
Dibromofluoromethane
Concen: 48.634 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX034155.D
Acq: 17 Feb 2023 13:52

Tgt Ion:113 Resp: 212489
Ion Ratio Lower Upper
113 100
111 103.5 83.0 124.6
192 19.6 19.0 28.4


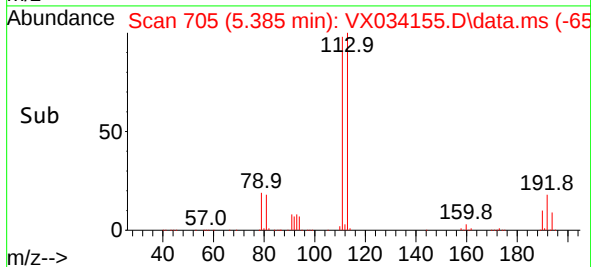
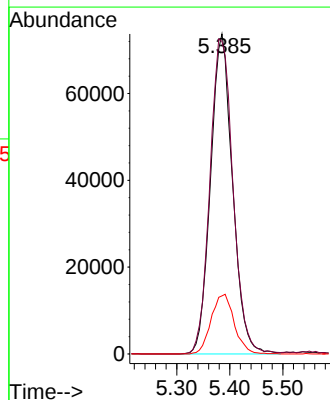
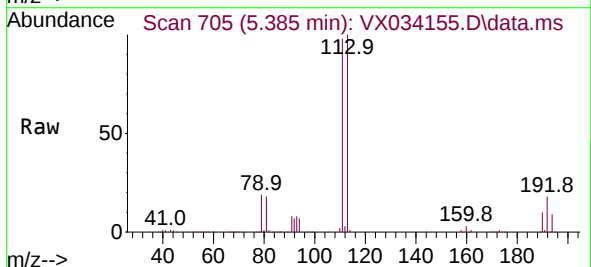


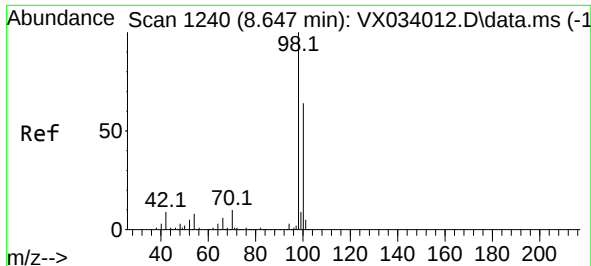

#50
Toluene-d8
Concen: 51.298 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034155.D
Acq: 17 Feb 2023 13:52




Instrument :
MSVOA_X
ClientSampleId :
VX0217WBL01


Tgt Ion: 98 Resp: 804696
Ion Ratio Lower Upper
98 100
100 66.2 53.6 80.4

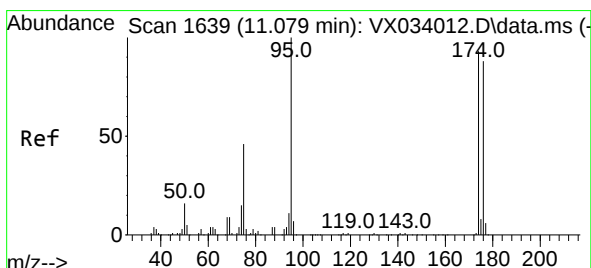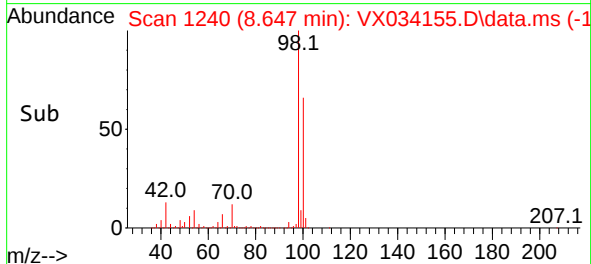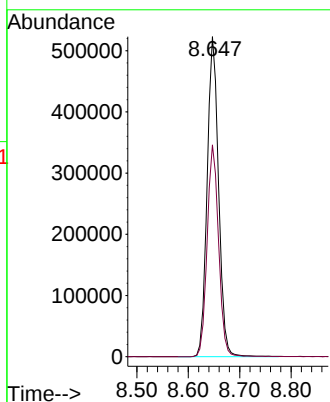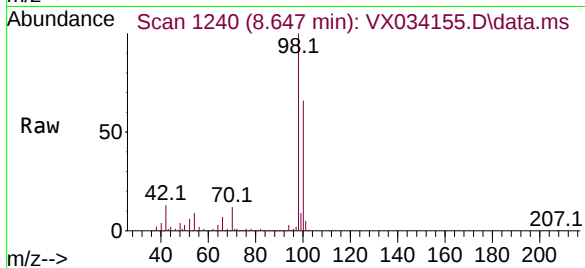

#62
4-Bromofluorobenzene
Concen: 47.346 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX034155.D
Acq: 17 Feb 2023 13:52

Tgt Ion: 95 Resp: 284086
Ion Ratio Lower Upper
95 100
174 74.3 0.0 184.4
176 72.5 0.0 178.8

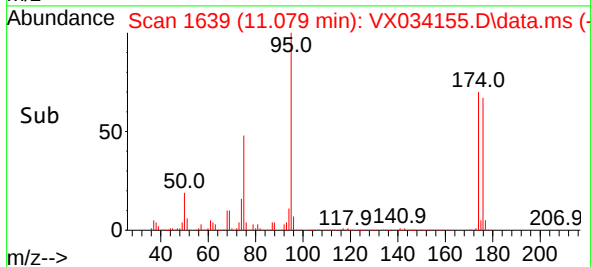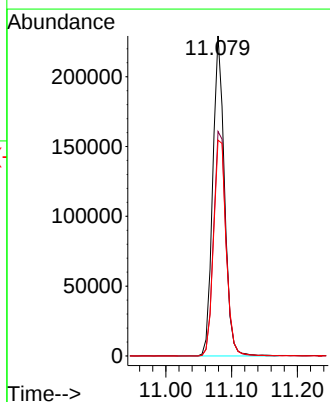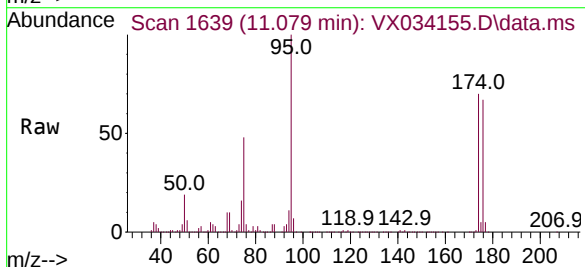

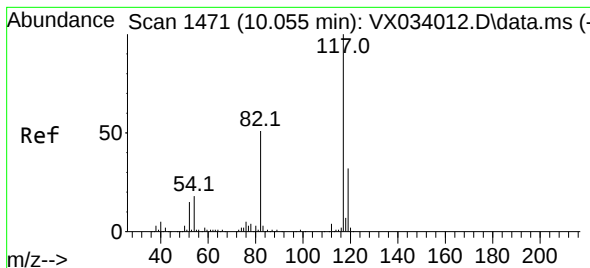

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX034155.D

Acq: 17 Feb 2023 13:52

Instrument :

MSVOA_X

ClientSampleId :

VX0217WBL01





Tgt Ion:117 Resp: 578571

Ion Ratio Lower Upper

117 100

82 57.1 40.6 60.8

119 32.2 25.6 38.4

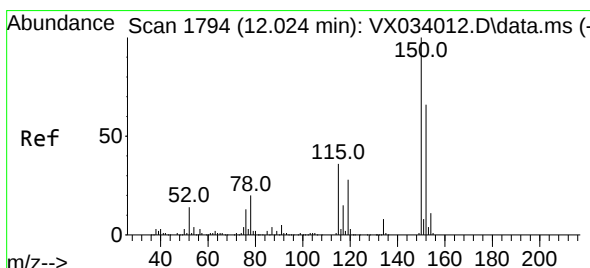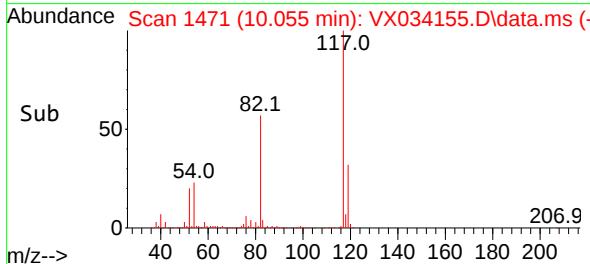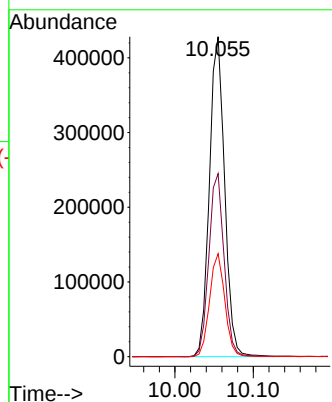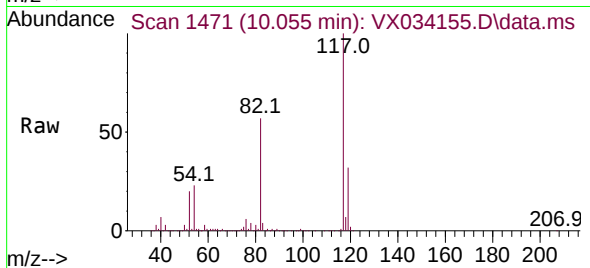

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX034155.D

Acq: 17 Feb 2023 13:52

Tgt Ion:152 Resp: 250598

Ion Ratio Lower Upper

152 100

115 60.7 38.7 116.1

150 156.9 0.0 348.2

