

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021723\
 Data File : VX034164.D
 Acq On : 17 Feb 2023 17:50
 Operator : JC/MD
 Sample : 01598-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M

Title : SW846 8260

Signal : TIC: VX034164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	23	28	31	rBV3	13135	25368	1.24%	0.242%
2	1.550	72	76	83	rBV9	9472	20867	1.02%	0.199%
3	5.385	695	705	721	rBV	226469	660710	32.31%	6.307%
4	5.556	721	733	748	rVB	377658	1091176	53.37%	10.417%
5	5.958	786	799	818	rBV	250280	680771	33.29%	6.499%
6	6.763	919	931	947	rBV	610743	1484246	72.59%	14.169%
7	8.647	1233	1240	1250	rBV	1312364	2044732	100.00%	19.519%
8	10.055	1465	1471	1482	rBV	1226434	1694980	82.89%	16.181%
9	11.079	1633	1639	1651	rBV	982710	1263781	61.81%	12.064%
10	12.018	1788	1793	1809	rVB	1111095	1487793	72.76%	14.203%
11	13.725	2069	2073	2078	rBV2	15557	20907	1.02%	0.200%




Sum of corrected areas: 10475331

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021723\
Data File : VX034164.D
Acq On : 17 Feb 2023 17:50
Operator : JC/MD
Sample : 01598-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

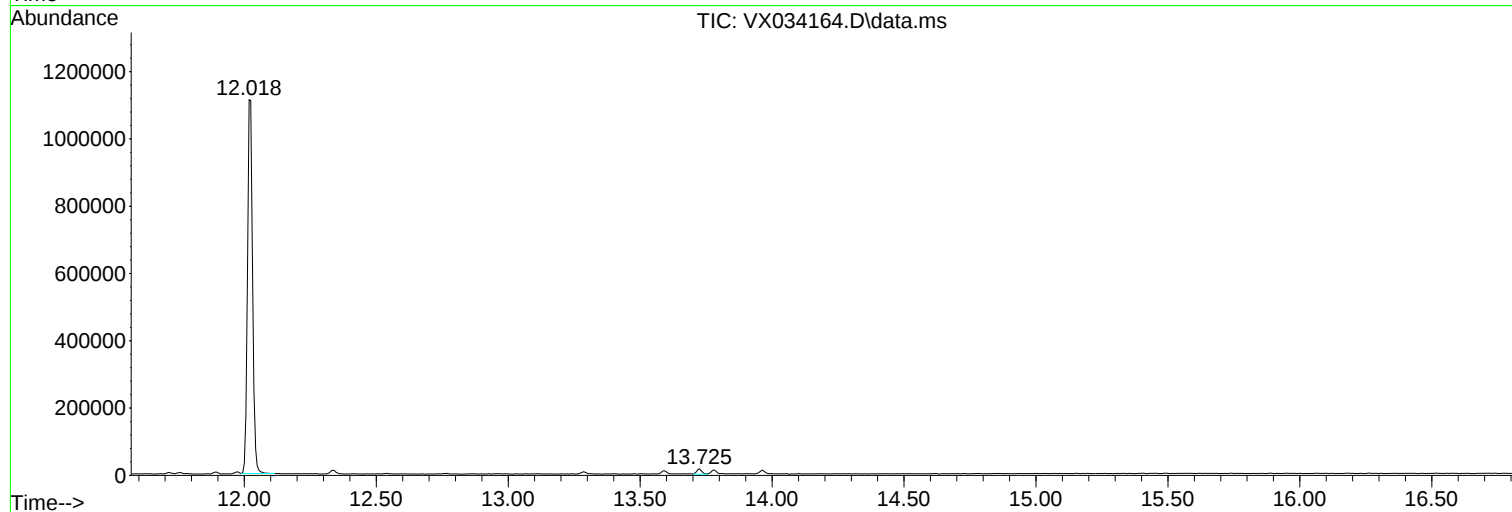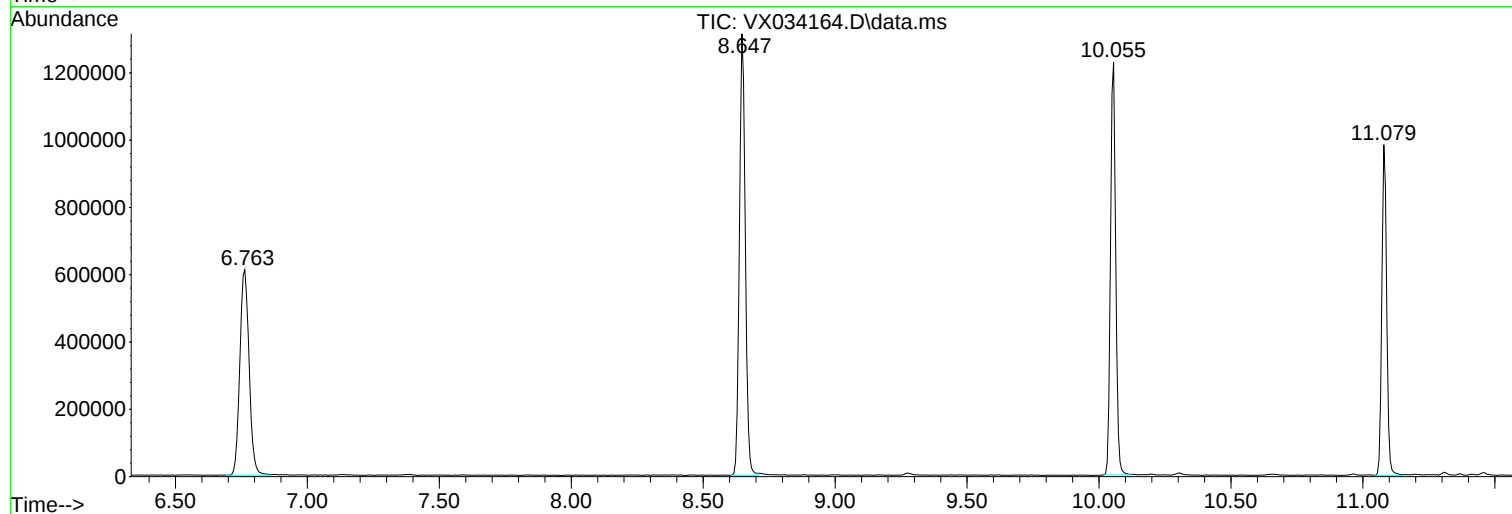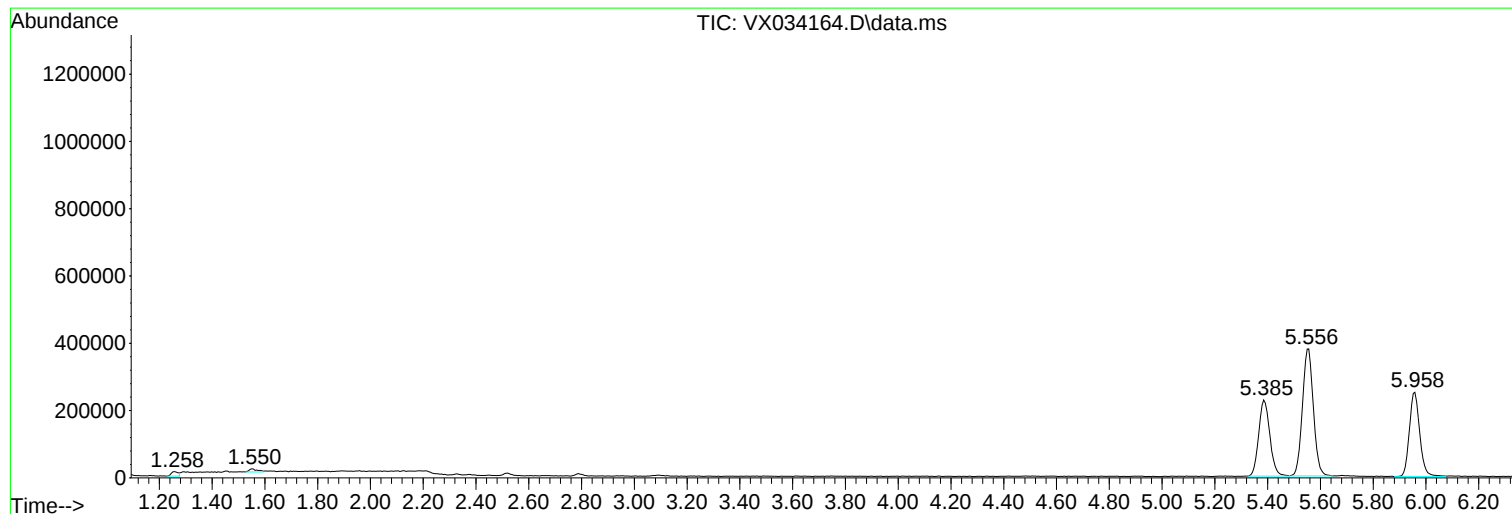

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021723\
Data File : VX034164.D
Acq On : 17 Feb 2023 17:50
Operator : JC/MD
Sample : 01598-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021723\
Data File : VX034164.D
Acq On : 17 Feb 2023 17:50
Operator : JC/MD
Sample : 01598-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------