

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX021819\
 Data File : VX007596.D
 Acq On : 18 Feb 2019 18:39
 Operator : JC/SP
 Sample : K1513-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WALL-ONE

Quant Time: Feb 19 04:14:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
 Quant Title : SW846 8260
 QLast Update : Sat Feb 02 01:32:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	459388	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	735034	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	697237	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	331192	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	258554	53.03	ug/l	0.00
Spiked Amount			Recovery	=	106.06%	
35) Dibromofluoromethane	5.51	113	242569	50.72	ug/l	0.00
Spiked Amount			Recovery	=	101.44%	
50) Toluene-d8	8.71	98	890412	50.18	ug/l	0.00
Spiked Amount			Recovery	=	100.36%	
62) 4-Bromofluorobenzene	11.13	95	308610	47.64	ug/l	0.00
Spiked Amount			Recovery	=	95.28%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.64	94	36	Below Cal	#	73
8) Diethyl Ether	2.19	74	1305	0.437	ug/l	60
11) Tert butyl alcohol	3.02	59	866	0.858	ug/l #	28
13) Acrolein	2.26	56	163	0.344	ug/l #	1
14) Allyl chloride	2.86	41	113259	15.847	ug/l #	26
16) Acetone	2.45	43	19319	8.649	ug/l	94
17) Carbon Disulfide	2.57	76	904	2.197	ug/l #	86
18) Methyl Acetate	2.78	43	10584	2.390	ug/l #	86
20) Methylene Chloride	2.86	84	3249973	717.612	ug/l	97
25) 2-Butanone	4.71	43	8275	2.603	ug/l	96
29) Tetrahydrofuran	5.17	42	1538	0.769	ug/l #	76
30) Chloroform	5.21	83	2495	0.317	ug/l #	69
36) 1,1-Dichloropropene	5.67	75	31896	4.836	ug/l #	48
38) Carbon Tetrachloride	5.67	117	41038	6.414	ug/l #	18
43) Isopropyl Acetate	6.46	43	3583	0.348	ug/l #	83
47) Bromodichloromethane	7.89	83	1373	0.229	ug/l	87
49) 1,4-Dioxane	7.75	88	351	9.857	ug/l #	1
51) 4-Methyl-2-Pentanone	8.62	43	28612	4.224	ug/l #	48
54) cis-1,3-Dichloropropene	8.62	75	12176	1.719	ug/l #	66
59) 2-Hexanone	9.44	43	14864	2.820	ug/l #	27
68) m/p-Xylenes	10.36	106	2269	0.233	ug/l	86
76) 1,2,3-Trichloropropane	11.13	75	149359	23.185	ug/l #	32
80) 1,3,5-Trimethylbenzene	11.51	105	4851	0.263	ug/l	94
81) trans-1,4-Dichloro-2-buten	11.13	75	149359	69.830	ug/l #	9
84) 1,2,4-Trimethylbenzene	11.80	105	12925	0.691	ug/l	99
90) Hexachloroethane	12.59	117	666	0.223	ug/l #	5
95) Naphthalene	13.83	128	35827	1.604	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX021819\
Data File : VX007596.D
Acq On : 18 Feb 2019 18:39
Operator : JC/SP
Sample : K1513-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WALL-ONE

Quant Time: Feb 19 04:14:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260
QLast Update : Sat Feb 02 01:32:36 2019
Response via : Initial Calibration

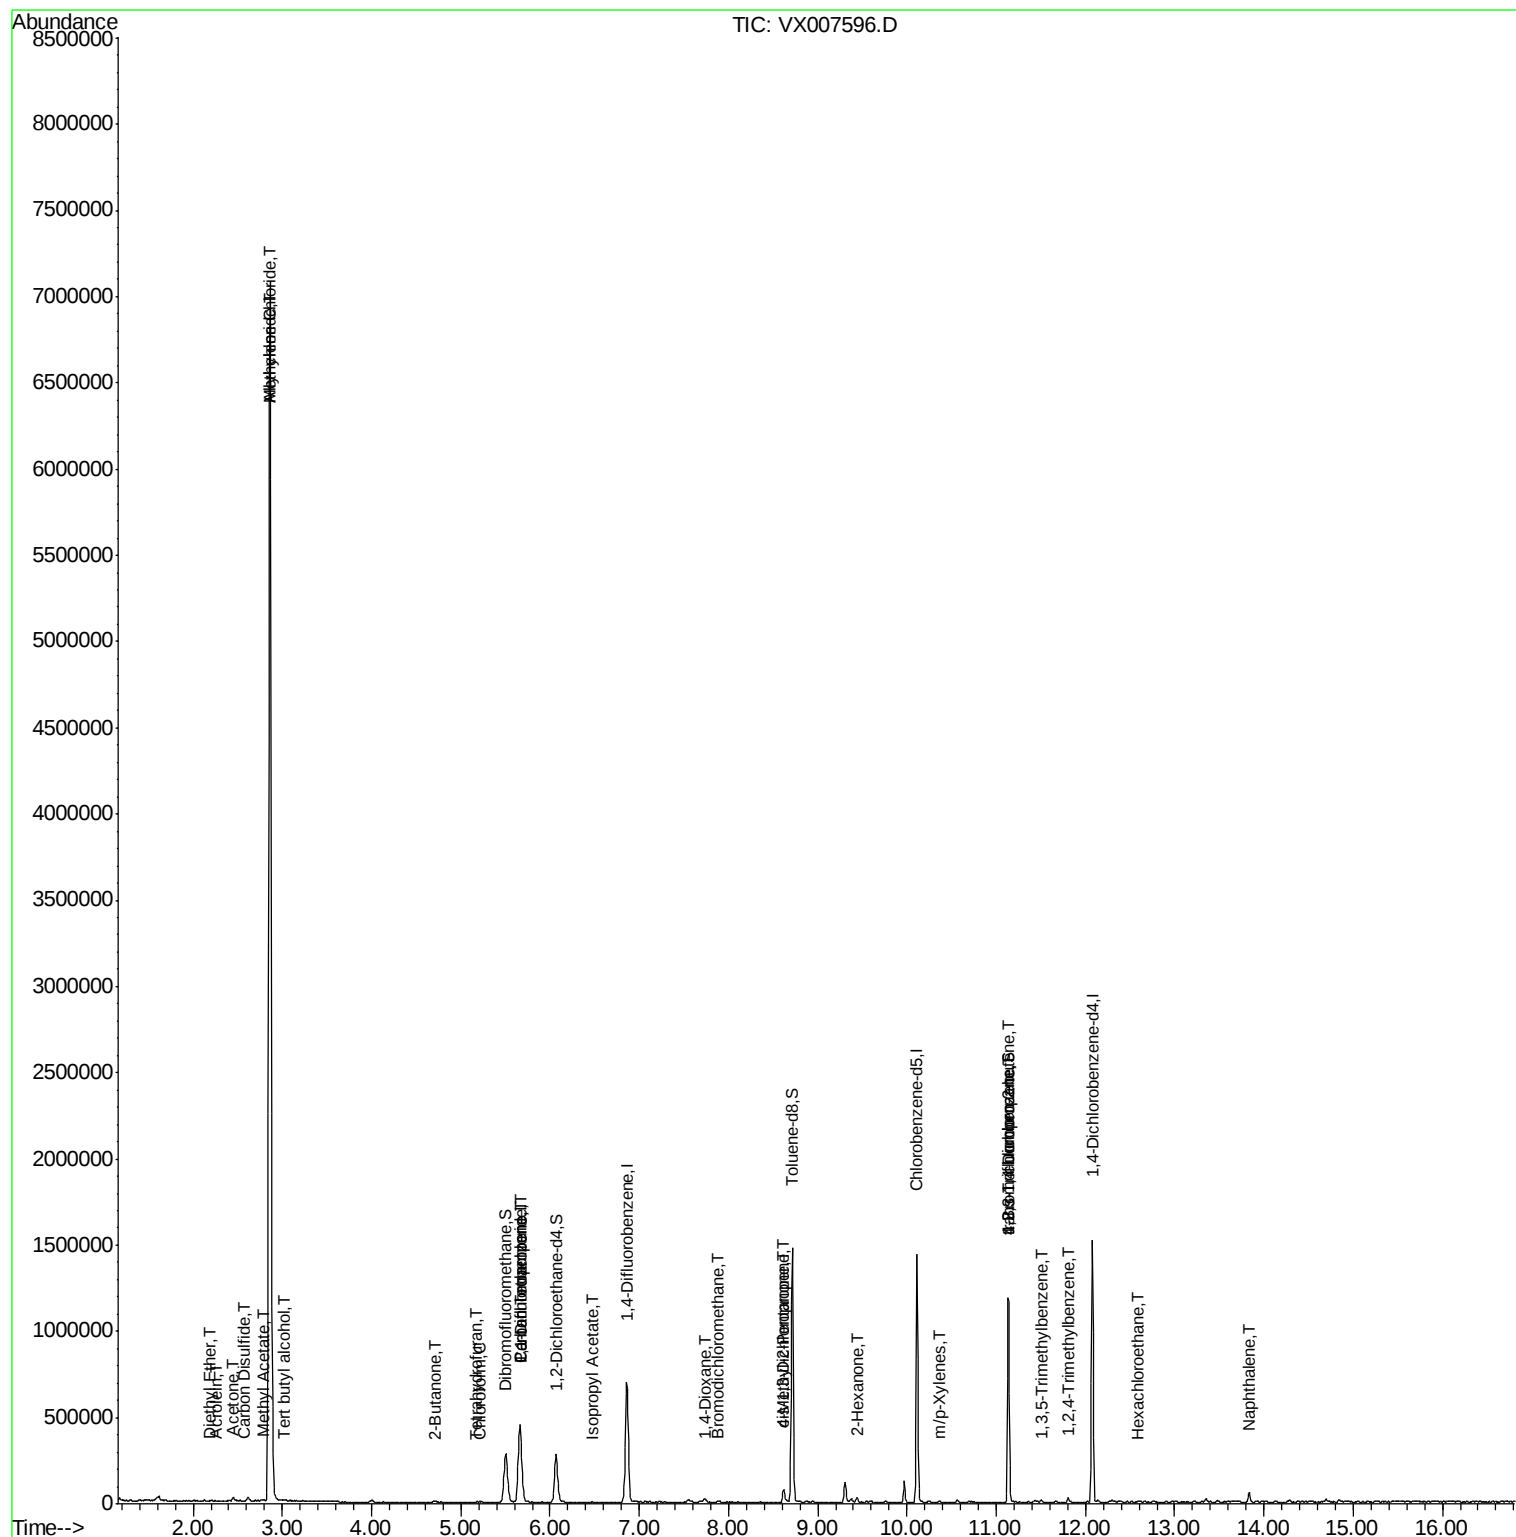

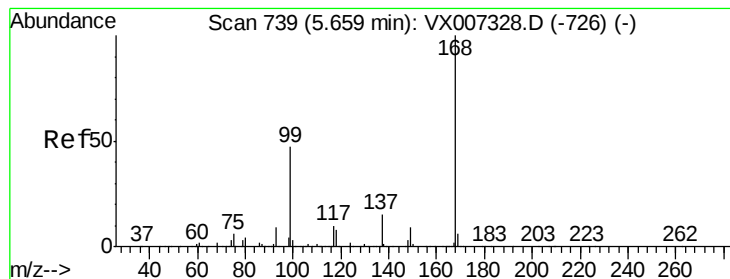

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39

Instrument :

MSVOA_X

ClientSampleId :


WALL-ONE

Tgt Ion:168 Resp: 459388

Ion Ratio Lower Upper

168 100

99 49.3 37.9 56.9



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67



150000

100000

50000

0

Time--> 5.50 5.60 5.70 5.80



#5

Bromomethane

Concen: Below Cal

RT: 1.64 min Scan# 80

Delta R.T. 0.00 min

Lab File: VX007596.D


Acq: 18 Feb 2019 18:39

Tgt Ion: 94 Resp: 36

Ion Ratio Lower Upper

94 100

96 118.7 73.9 110.9#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.64

300

250

200


150


100

50

0

Time--> 1.63 1.64 1.64 1.65 1.65



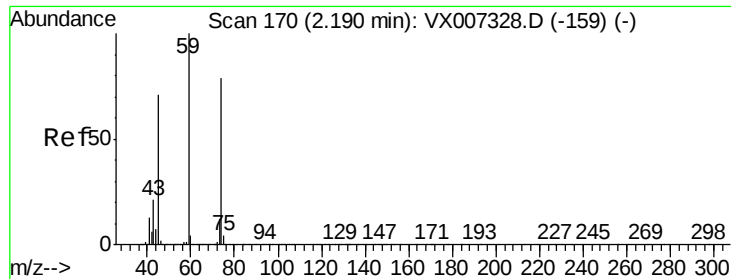

#8

Diethyl Ether

Concen: 0.437 ug/l

RT: 2.19 min Scan# 170

Delta R.T. -0.00 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39

Instrument :

MSVOA_X

ClientSampleId :


WALL-ONE

Tgt Ion: 74 Resp: 1305

Ion Ratio Lower Upper




74 100

45 53.0 45.7 137.1

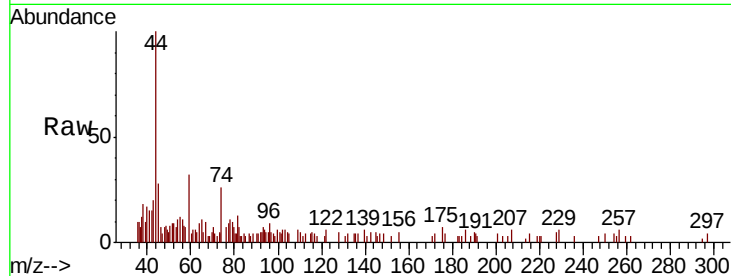

Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

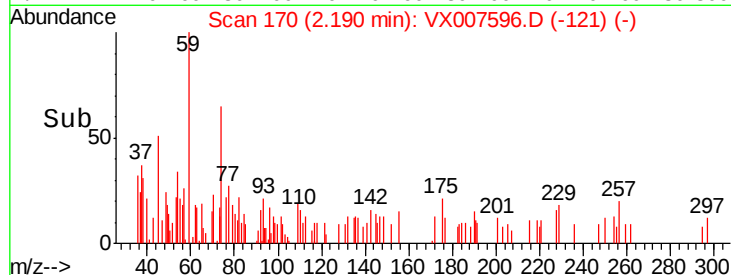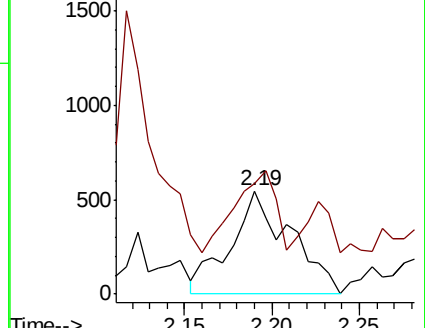

#11

Tert butyl alcohol

Concen: 0.858 ug/l

RT: 3.02 min Scan# 306

Delta R.T. -0.05 min

Lab File: VX007596.D


Acq: 18 Feb 2019 18:39

Tgt Ion: 59 Resp: 866

Ion Ratio Lower Upper



59 100


57 37.0 8.1 12.1#

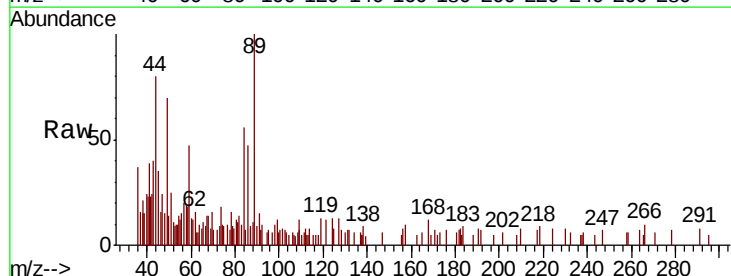

Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

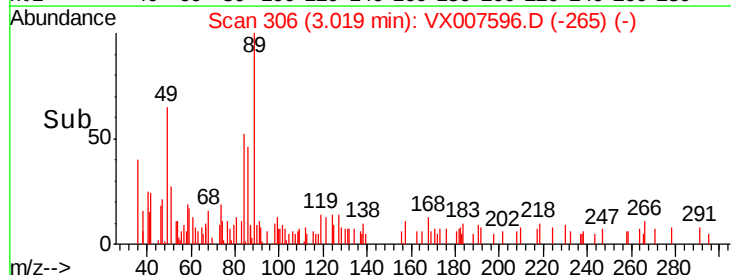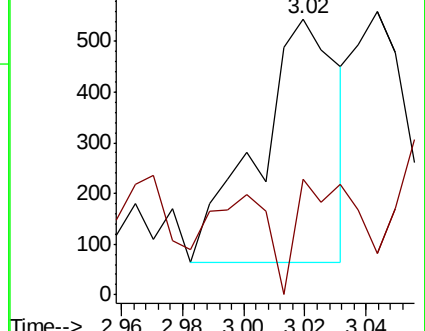



#13

Acrolein

Concen: 0.344 ug/l

RT: 2.26 min Scan# 181

Delta R.T. -0.04 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39

Instrument :

MSVOA_X

ClientSampled :





WALL-ONE

Tgt Ion: 56 Resp: 163

Ion Ratio Lower Upper

56 100

55 306.1 56.9 85.3#

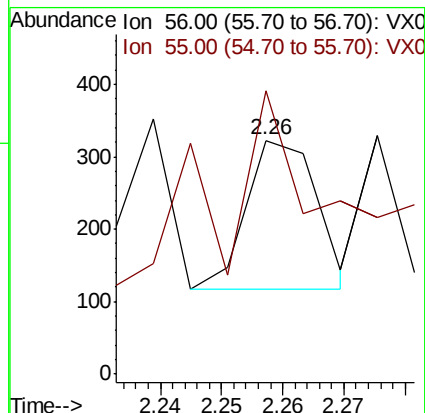

#14

Allyl chloride

Concen: 15.847 ug/l

RT: 2.86 min Scan# 280

Delta R.T. 0.13 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39




Tgt Ion: 41 Resp: 113259


Ion Ratio Lower Upper

41 100

39 1.8 54.1 81.1#

76 0.3 27.8 41.8#

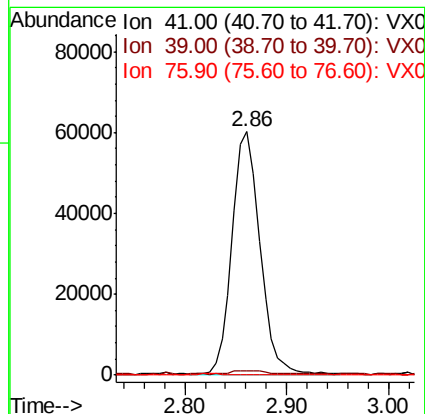

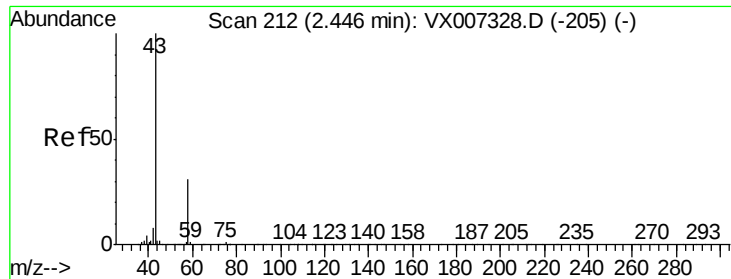

#16

Acetone

Concen: 8.649 ug/l

RT: 2.45 min Scan# 212

Delta R.T. -0.00 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39

Instrument :

MSVOA_X

ClientSampleId :


WALL-ONE

Tgt Ion: 43 Resp: 19319

Ion Ratio Lower Upper

43 100

58 34.5 24.9 37.3



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.45

12000

10000

8000

6000



4000

2000

0

Time-->

2.35 2.40 2.45 2.50 2.55

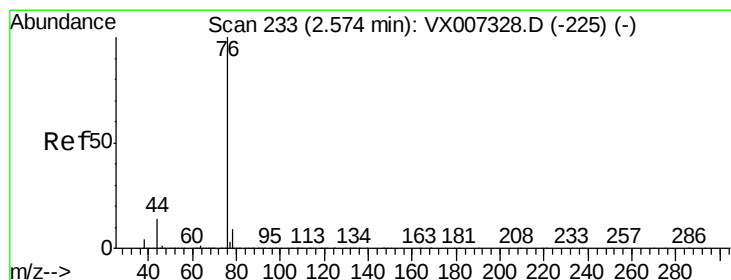

#17

Carbon Disulfide

Concen: 2.197 ug/l

RT: 2.57 min Scan# 233

Delta R.T. 0.00 min

Lab File: VX007596.D


Acq: 18 Feb 2019 18:39

Tgt Ion: 76 Resp: 904

Ion Ratio Lower Upper

76 100

78 4.0 7.1 10.7#

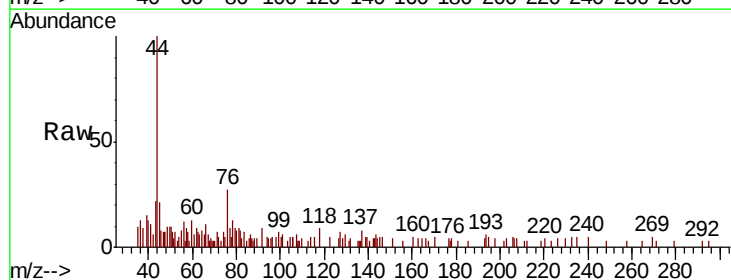

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

2.57

600

500

400

300


200


100

0

Time-->

2.55 2.60




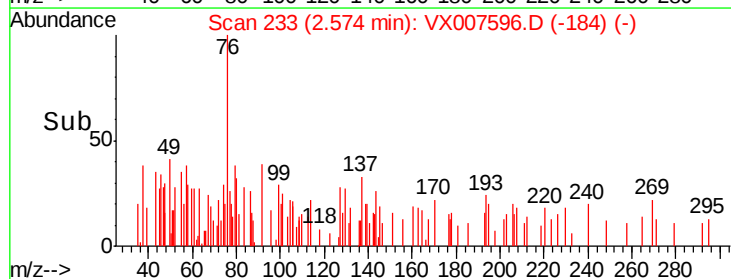


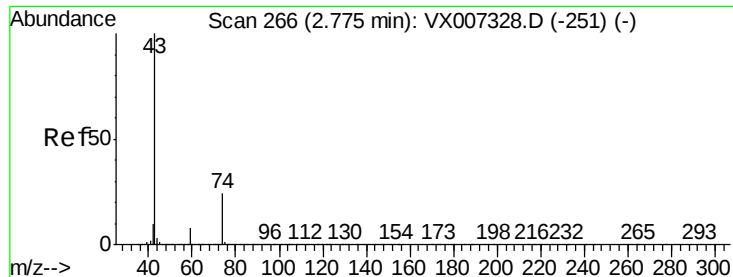

#18
Methyl Acetate
Concen: 2.390 ug/l
RT: 2.78 min Scan# 267
Delta R.T. 0.01 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39




Instrument :
MSVOA_X
ClientSampleId :
WALL-ONE


Tgt Ion: 43 Resp: 10584
Ion Ratio Lower Upper
43 100
74 31.2 19.4 29.2#

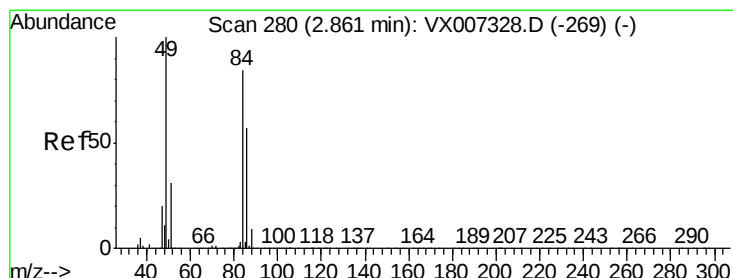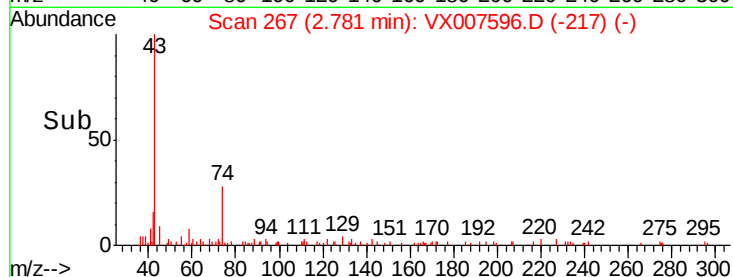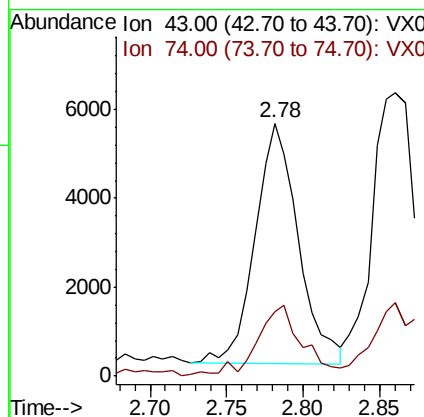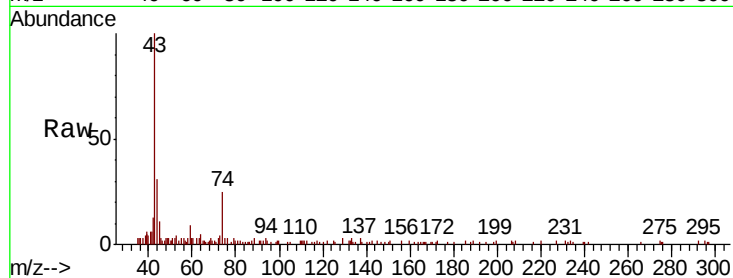

#20
Methylene Chloride
Concen: 717.612 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.00 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39

Tgt Ion: 84 Resp: 3249973
Ion Ratio Lower Upper
84 100
49 121.7 94.8 142.2
51 37.4 29.8 44.8
86 64.9 54.1 81.1

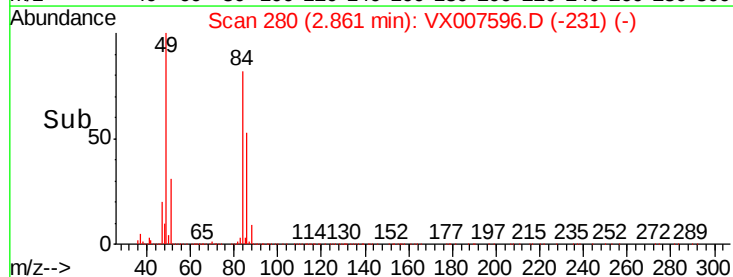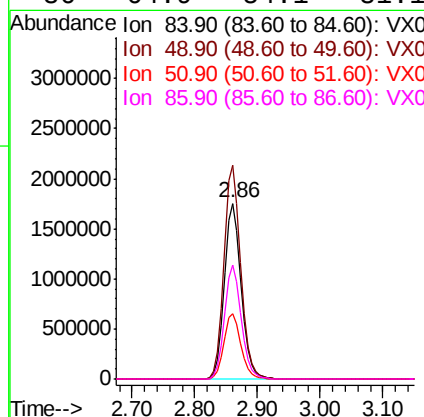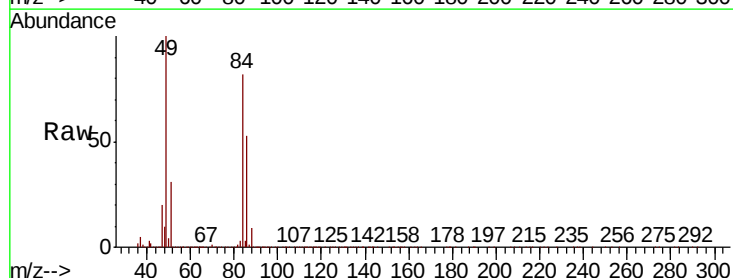

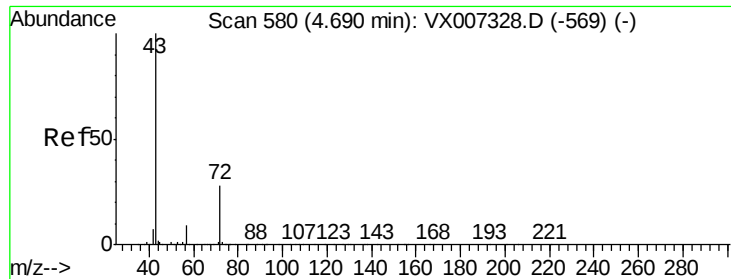

#25

2-Butanone

Concen: 2.603 ug/l

RT: 4.71 min Scan# 584

Delta R.T. 0.02 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39

Instrument :

MSVOA_X

ClientSampleId :


WALL-ONE

Tgt Ion: 43 Resp: 8275

Ion Ratio Lower Upper




43 100

72 25.4 22.2 33.2

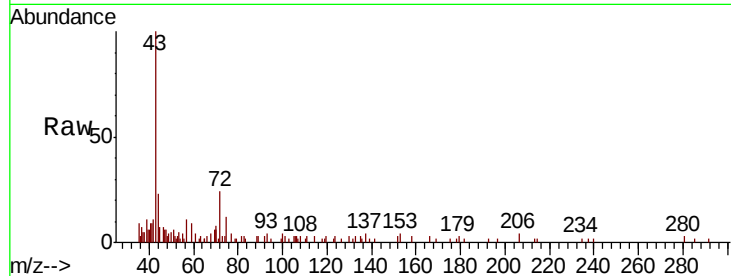

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

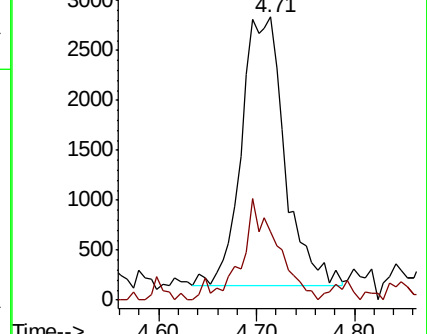

#29

Tetrahydrofuran

Concen: 0.769 ug/l

RT: 5.17 min Scan# 658

Delta R.T. 0.02 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39


Tgt Ion: 42 Resp: 1538

Ion Ratio Lower Upper

42 100

72 26.2 37.6 56.4#



71 32.3 34.6 51.8#




Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0




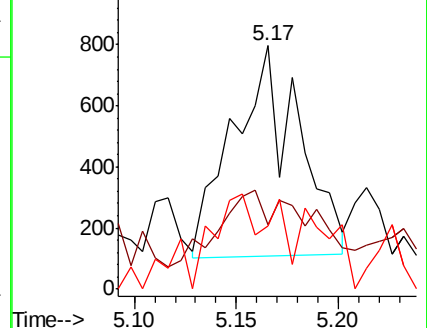


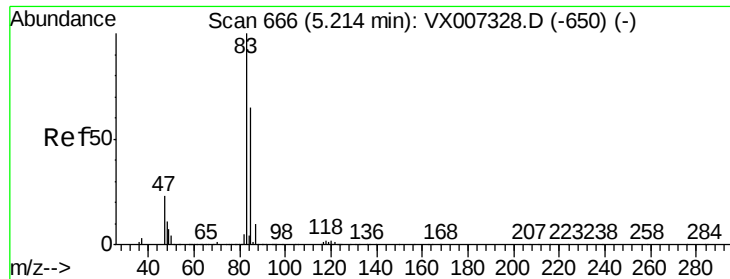

#30
Chloroform
Concen: 0.317 ug/l
RT: 5.21 min Scan# 666
Delta R.T. -0.00 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39




Instrument :
MSVOA_X
ClientSampleId :
WALL-ONE


Tgt Ion: 83 Resp: 2495
Ion Ratio Lower Upper
83 100
85 40.4 51.6 77.4#

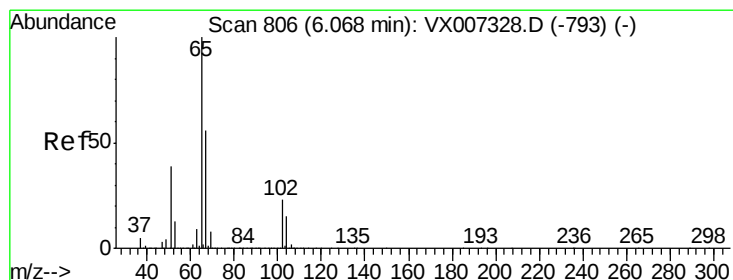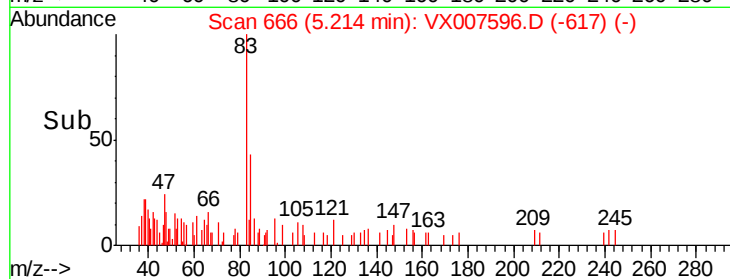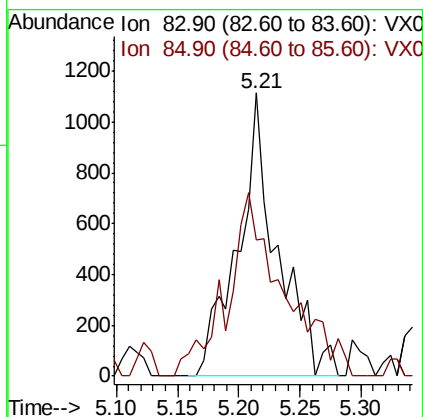

#33
1,2-Dichloroethane-d4
Concen: 53.025 ug/l
RT: 6.07 min Scan# 806
Delta R.T. -0.00 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39

Tgt Ion: 65 Resp: 258554
Ion Ratio Lower Upper
65 100
67 53.0 0.0 108.8

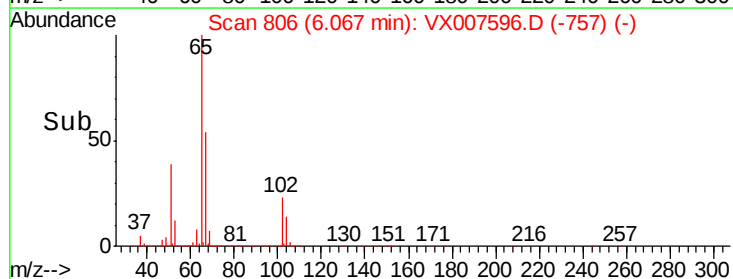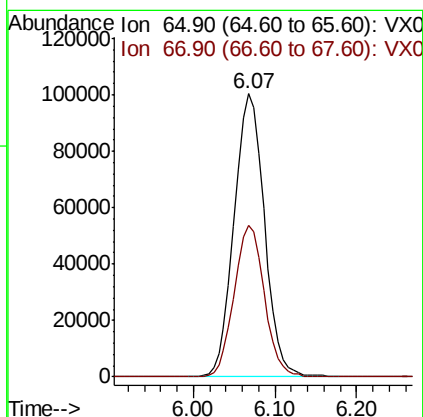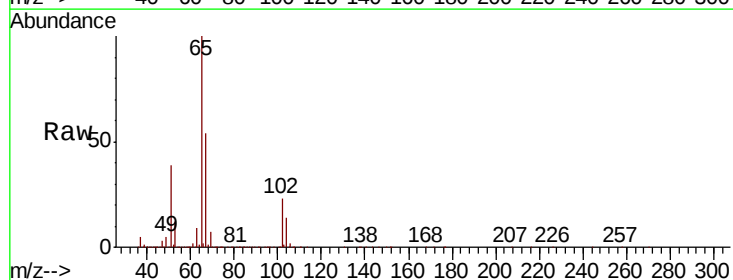



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39

Instrument :

MSVOA_X

ClientSampleId :

WALL-ONE


Tgt Ion:114 Resp: 735034

Ion Ratio Lower Upper

114 100

63 18.3 0.0 35.6

88 14.0 0.0 29.6

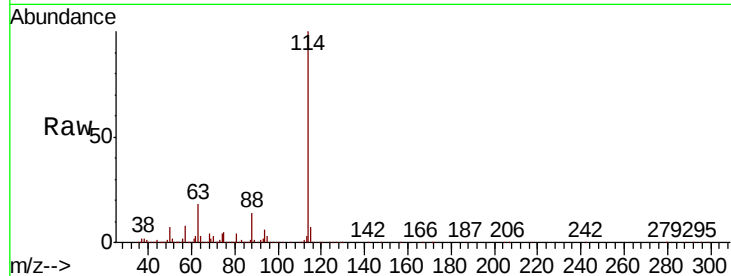



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

6.86

Time-->

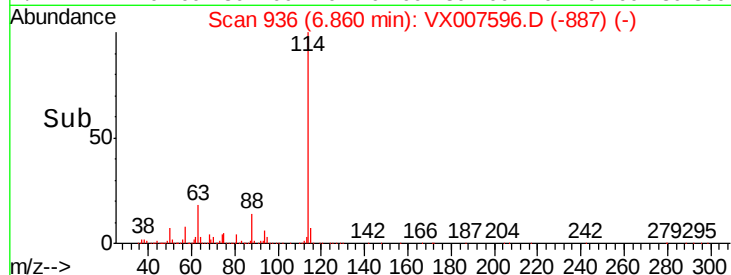

#35

Dibromofluoromethane

Concen: 50.719 ug/l

RT: 5.51 min Scan# 714

Delta R.T. -0.00 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39


Tgt Ion:113 Resp: 242569

Ion Ratio Lower Upper

113 100

111 102.4 81.8 122.8

192 21.4 18.5 27.7

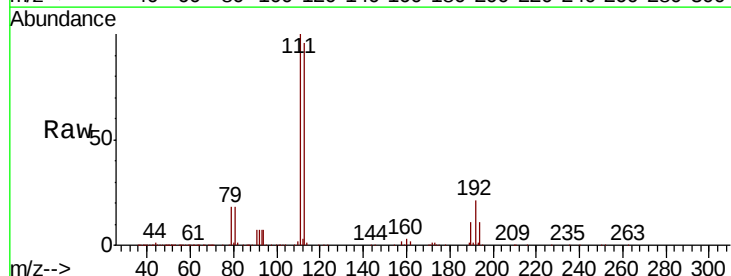


Abundance Ion 112.80 (112.50 to 113.50): V


Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

5.51

Time-->

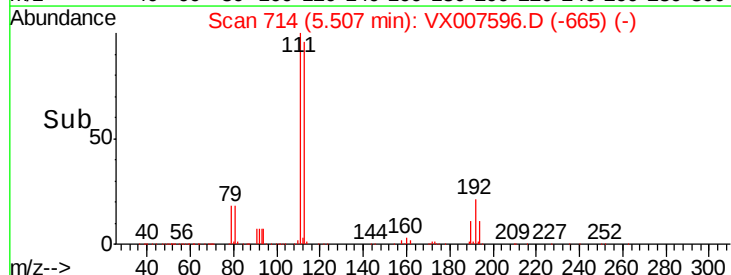

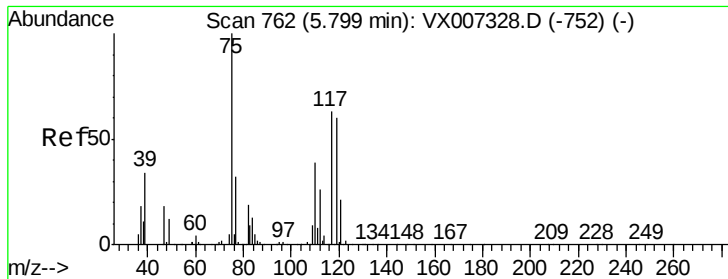

#36

1,1-Dichloropropene

Concen: 4.836 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.13 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39

Instrument :

MSVOA_X

ClientSampled :

WALL-ONE


Tgt Ion: 75 Resp: 31896

Ion Ratio Lower Upper

75 100

110 9.4 20.0 59.9#




77 0.6 24.7 37.1#

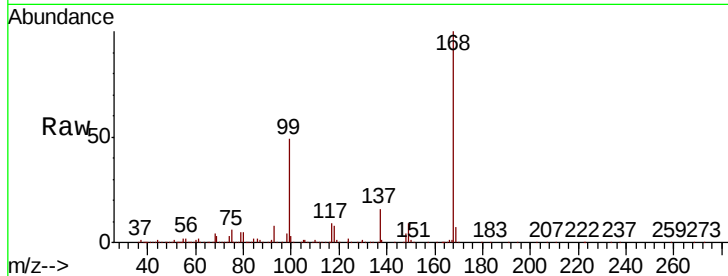

Abundance Ion 74.90 (74.60 to 75.60): VX007596.D (-713) (-)

Ion 109.90 (109.60 to 110.60): VX007596.D (-713) (-)

Ion 76.90 (76.60 to 77.60): VX007596.D (-713) (-)

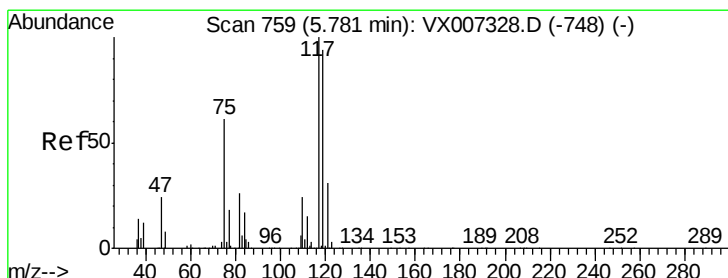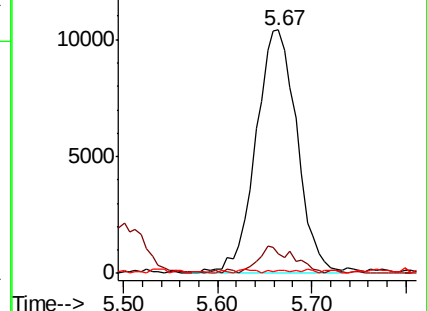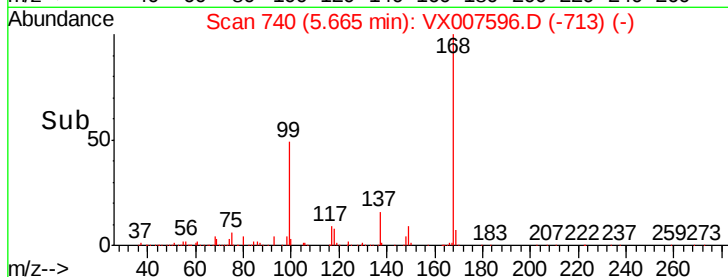

#38

Carbon Tetrachloride

Concen: 6.414 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.12 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39


Tgt Ion: 117 Resp: 41038

Ion Ratio Lower Upper

117 100

119 7.0 75.3 112.9#



121 0.0 25.0 37.4#

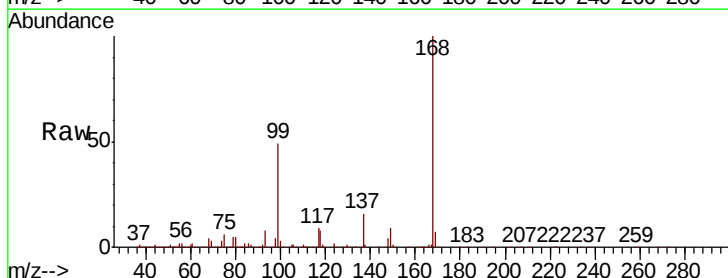


Abundance Ion 116.80 (116.50 to 117.50): VX007596.D (-710) (-)

Ion 118.80 (118.50 to 119.50): VX007596.D (-710) (-)

Ion 120.80 (120.50 to 121.50): VX007596.D (-710) (-)

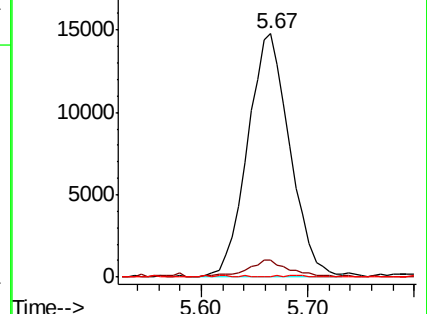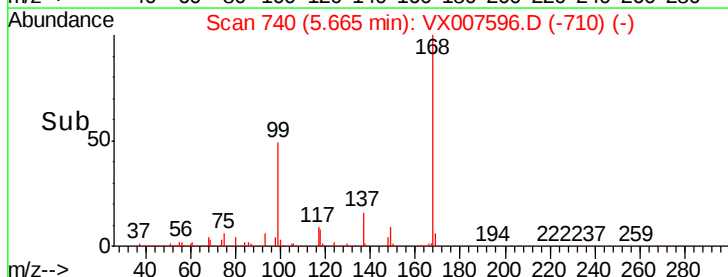



#43

Isopropyl Acetate

Concen: 0.348 ug/l

RT: 6.46 min Scan# 871

Delta R.T. 0.01 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39

Instrument :

MSVOA_X

ClientSampled :

WALL-ONE





Tgt Ion: 43 Resp: 3583

Ion Ratio Lower Upper

43 100

61 10.3 16.1 24.1#

87 18.5 11.5 17.3#

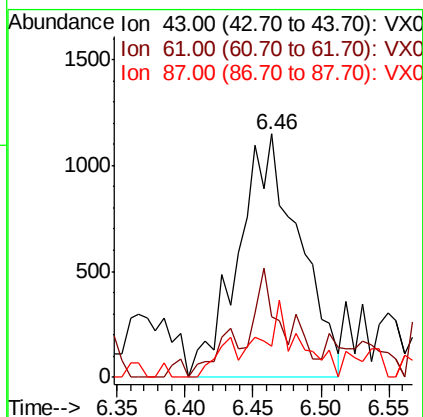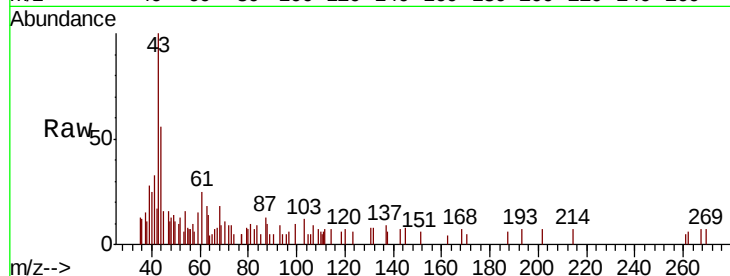

#47

Bromodichloromethane

Concen: 0.229 ug/l

RT: 7.89 min Scan# 1105

Delta R.T. -0.01 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39




Tgt Ion: 83 Resp: 1373


Ion Ratio Lower Upper

83 100

85 52.4 51.4 77.0

127 9.5 8.1 12.1



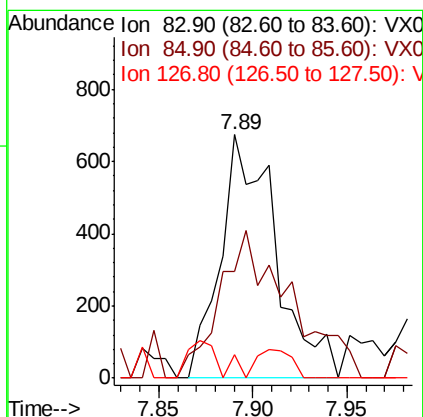





#49
1,4-Dioxane
Concen: 9.857 ug/l
RT: 7.75 min Scan# 1082
Delta R.T. 0.00 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39




Instrument :
MSVOA_X
ClientSampleId :
WALL-ONE


Tgt Ion: 88 Resp: 351
Ion Ratio Lower Upper
88 100
43 266.4 24.2 36.4#
58 364.1 53.0 79.4#

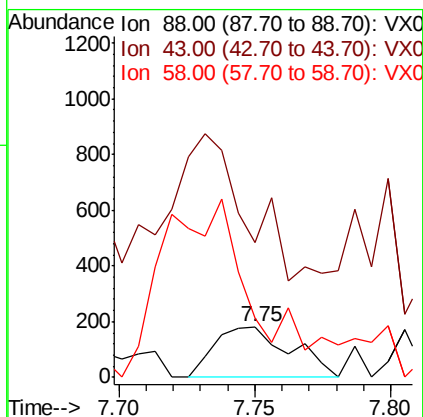

#50
Toluene-d8
Concen: 50.180 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39

Tgt Ion: 98 Resp: 890412
Ion Ratio Lower Upper
98 100
100 64.2 51.6 77.4



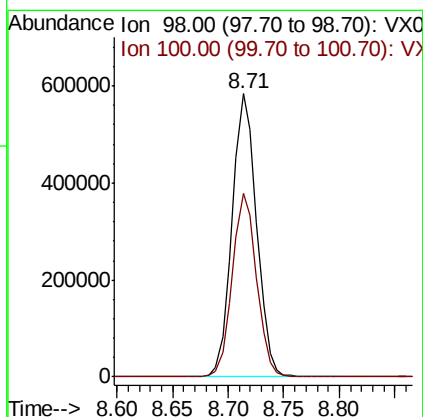



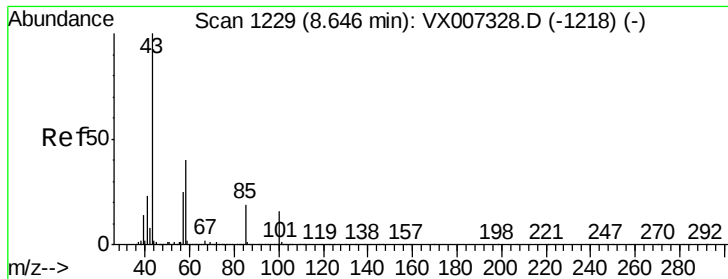

#51
 4-Methyl-2-Pentanone
 Concen: 4.224 ug/l
 RT: 8.62 min Scan# 1224
 Delta R.T. -0.03 min
 Lab File: VX007596.D
 Acq: 18 Feb 2019 18:39




Instrument :
 MSVOA_X
 ClientSampleId :
 WALL-ONE


Tgt Ion: 43 Resp: 28612
 Ion Ratio Lower Upper
 43 100
 58 7.1 31.2 46.8#

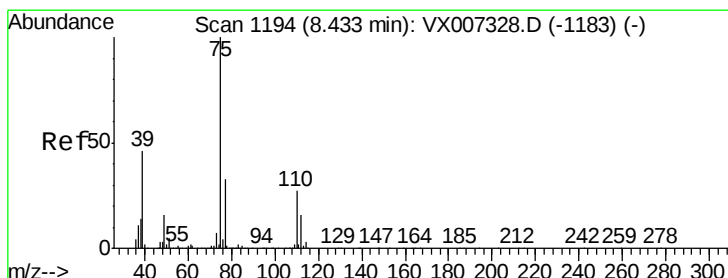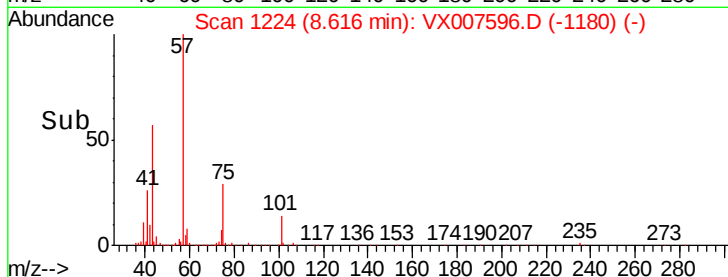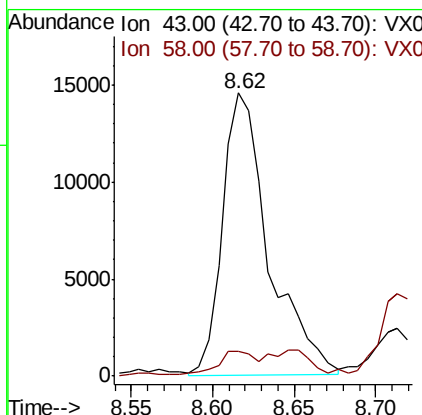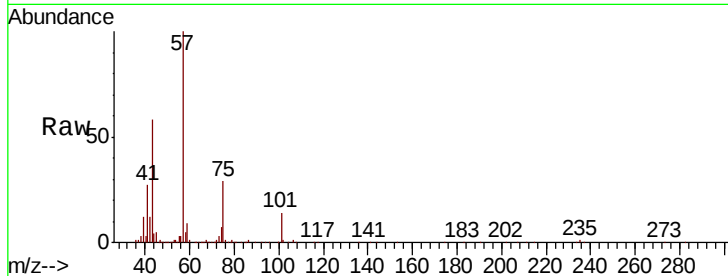

#54
 cis-1,3-Dichloropropene
 Concen: 1.719 ug/l
 RT: 8.62 min Scan# 1225
 Delta R.T. 0.19 min
 Lab File: VX007596.D
 Acq: 18 Feb 2019 18:39

Tgt Ion: 75 Resp: 12176
 Ion Ratio Lower Upper
 75 100
 77 1.5 26.2 39.4#
 39 33.6 37.1 55.7#


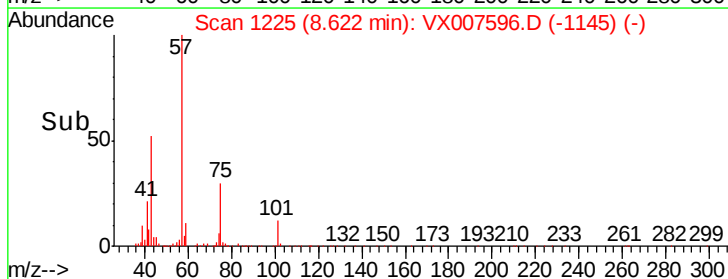
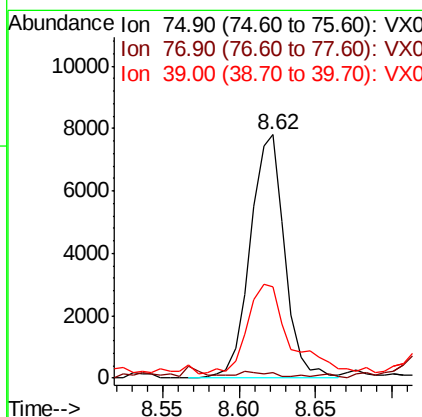
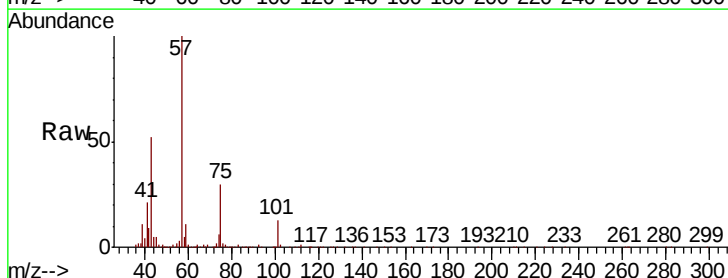


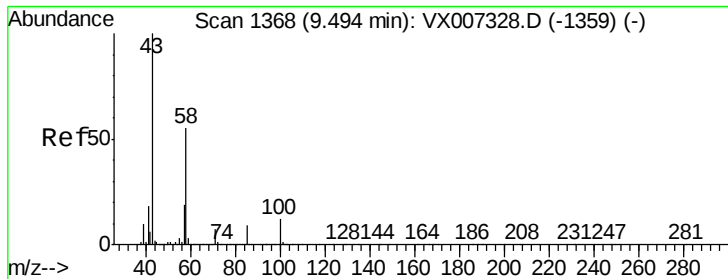

#59
2-Hexanone
Concen: 2.820 ug/l
RT: 9.44 min Scan# 1359
Delta R.T. -0.05 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39




Instrument :
MSVOA_X
ClientSampleId :
WALL-ONE


Tgt Ion: 43 Resp: 14864
Ion Ratio Lower Upper
43 100
58 1.5 27.1 81.3#

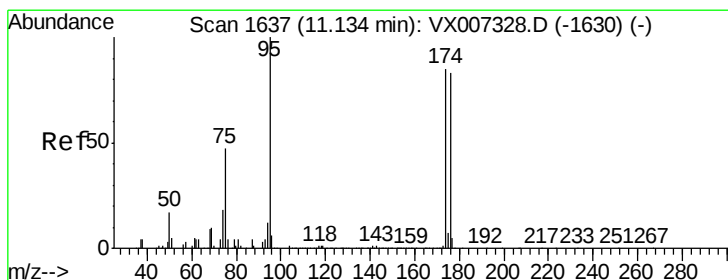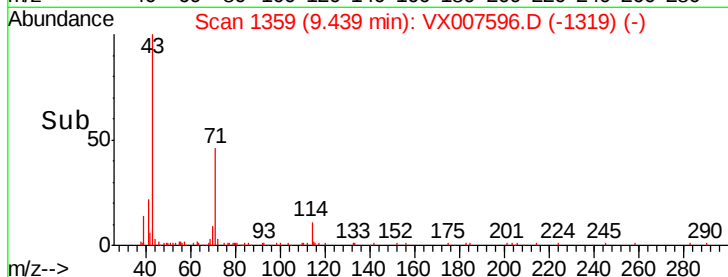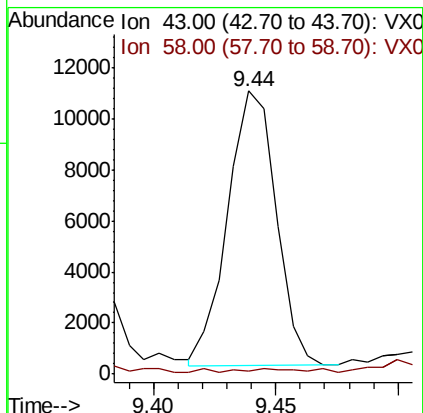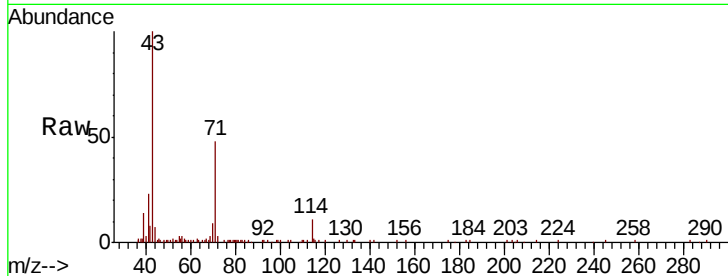

#62
4-Bromofluorobenzene
Concen: 47.636 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39

Tgt Ion: 95 Resp: 308610
Ion Ratio Lower Upper
95 100
174 92.7 0.0 189.2
176 89.7 0.0 186.2


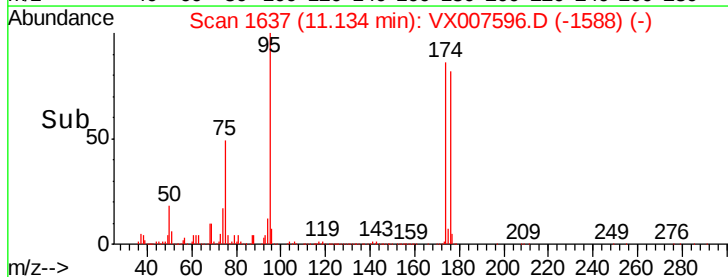
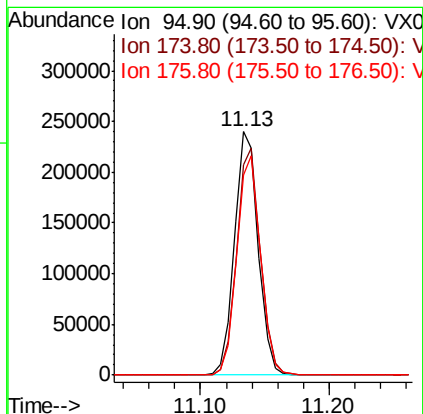
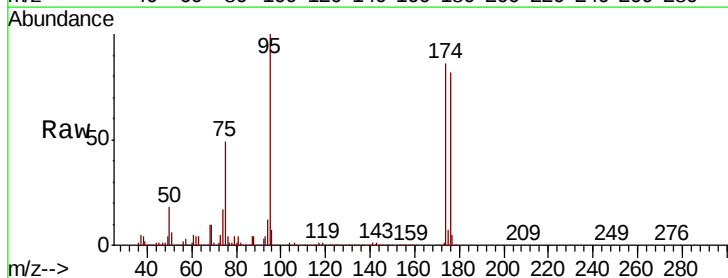




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.01 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39




Instrument :
MSVOA_X
ClientSampleId :
WALL-ONE


Tgt Ion:117 Resp: 697237
Ion Ratio Lower Upper
117 100
82 49.9 42.1 63.1
119 32.6 26.5 39.7

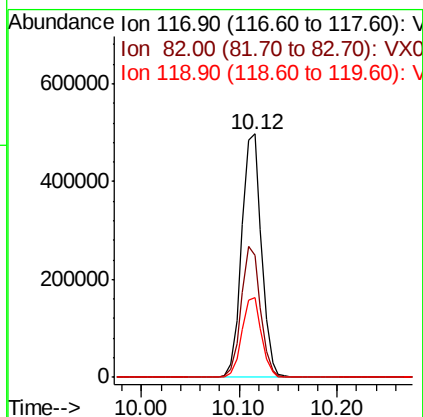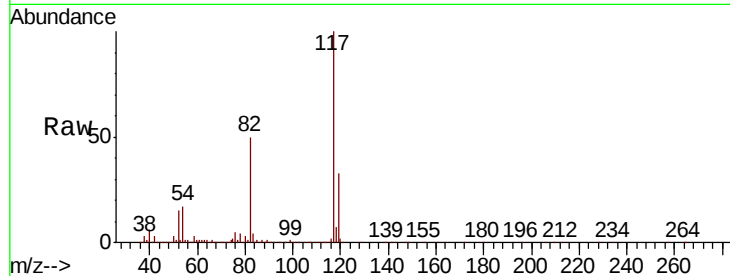

#68
m/p-Xylenes
Concen: 0.233 ug/l
RT: 10.36 min Scan# 1510
Delta R.T. -0.00 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39

Tgt Ion:106 Resp: 2269
Ion Ratio Lower Upper
106 100
91 174.8 156.6 234.8

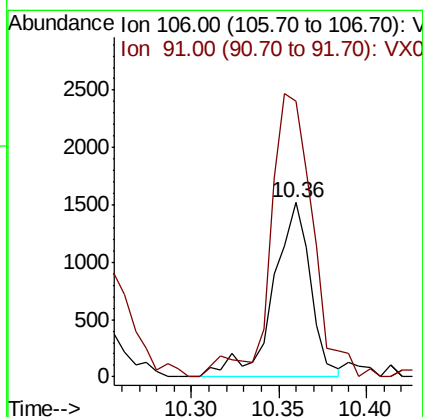



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39

Instrument :

MSVOA_X

ClientSampled :

WALL-ONE


Tgt Ion: 152 Resp: 331192

Ion Ratio Lower Upper

152 100

115 55.3 38.0 114.0




150 158.5 0.0 346.4

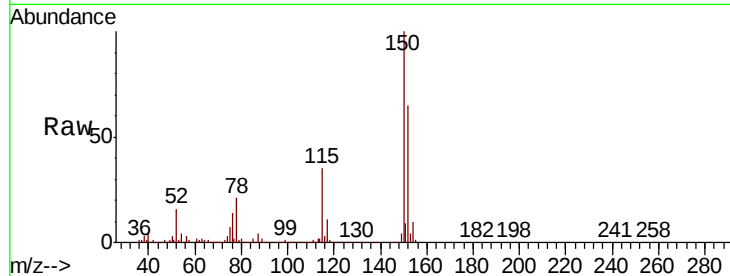

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

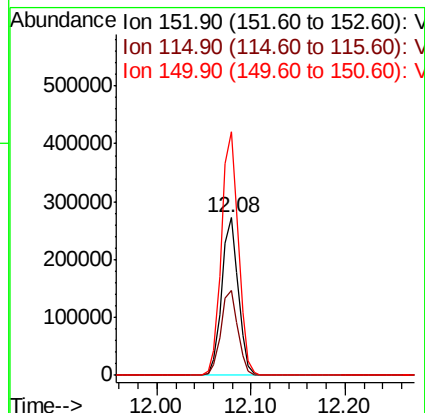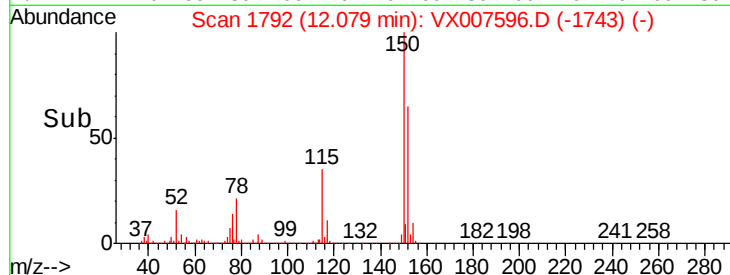

#76

1,2,3-Trichloropropane

Concen: 23.185 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX007596.D


Acq: 18 Feb 2019 18:39

Tgt Ion: 75 Resp: 149359

Ion Ratio Lower Upper



75 100


77 1.3 23.0 69.0#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

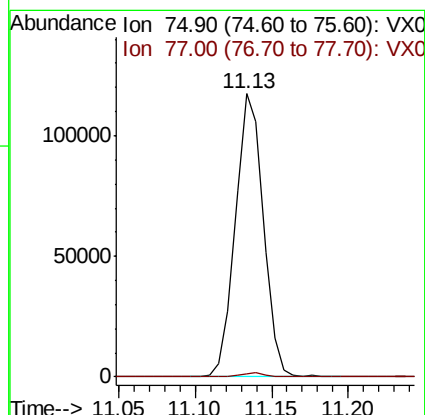



#80

1,3,5-Trimethylbenzene

Concen: 0.263 ug/l

RT: 11.51 min Scan# 1698

Delta R.T. -0.00 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39

Instrument :

MSVOA_X

ClientSampleId :


WALL-ONE

Tgt Ion: 105 Resp: 4851

Ion Ratio Lower Upper




105 100

120 54.8 25.3 75.8



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

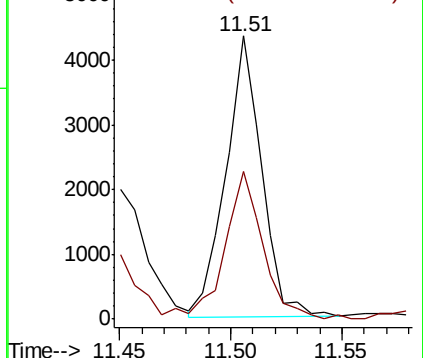

#81

trans-1,4-Dichloro-2-butene

Concen: 69.830 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX007596.D

Acq: 18 Feb 2019 18:39


Tgt Ion: 75 Resp: 149359

Ion Ratio Lower Upper

75 100

53 0.2 81.0 121.6#



89 0.1 41.4 62.0#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0



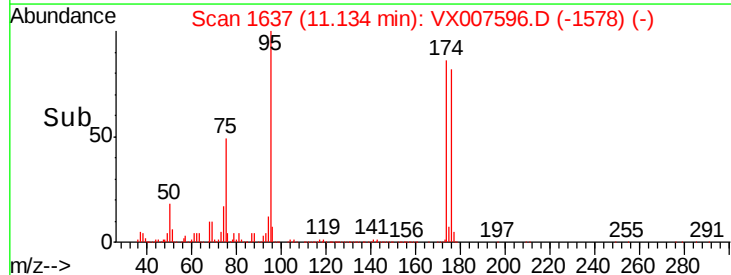
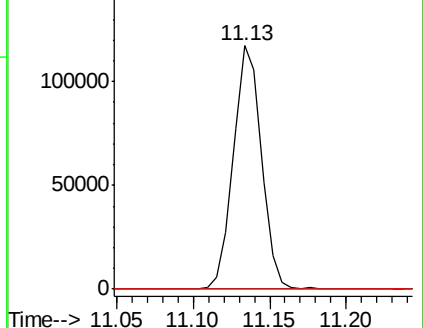




#84
1,2,4-Trimethylbenzene
Concen: 0.691 ug/l
RT: 11.80 min Scan# 1747
Delta R.T. -0.00 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39




Instrument :
MSVOA_X
ClientSampled :
WALL-ONE


Tgt Ion:105 Resp: 12925
Ion Ratio Lower Upper
105 100
120 45.5 23.1 69.3

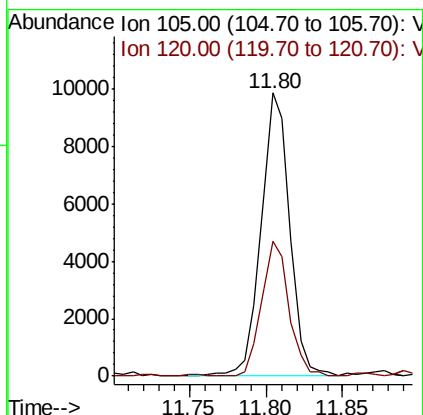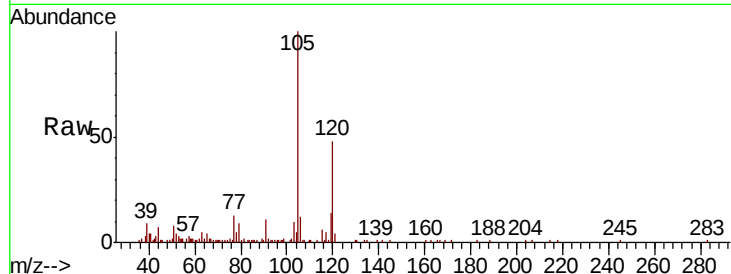

#90
Hexachloroethane
Concen: 0.223 ug/l
RT: 12.59 min Scan# 1876
Delta R.T. -0.01 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39

Tgt Ion:117 Resp: 666
Ion Ratio Lower Upper
117 100
201 0.0 44.9 134.7#

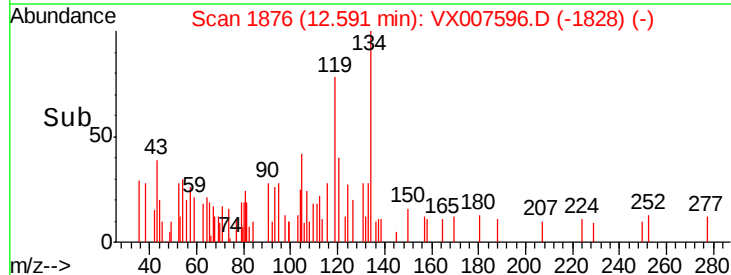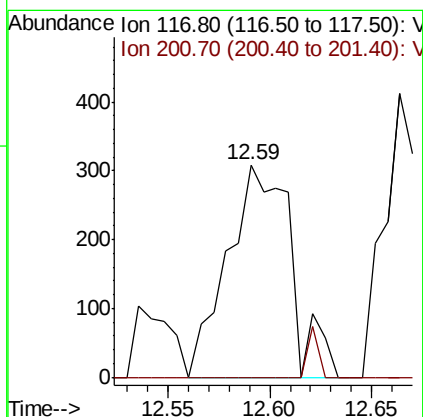


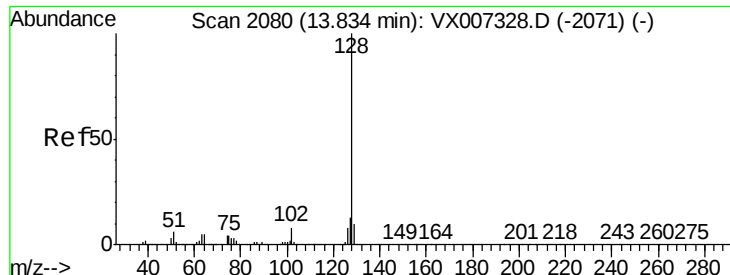

#95
Naphthalene
Concen: 1.604 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. -0.00 min
Lab File: VX007596.D
Acq: 18 Feb 2019 18:39

Instrument :
MSVOA_X
ClientSampleId :
WALL-ONE

Tgt Ion	Ratio	Lower	Upper
128	100		
127	13.3	10.5	15.7
129	11.2	8.7	13.1



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

