

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021822\
 Data File : VX027118.D
 Acq On : 18 Feb 2022 18:25
 Operator : JC/MD
 Sample : N1465-07ME
 Misc : 6.42g/5.0mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 A5-7-6.5

Quant Time: Feb 21 00:42:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 08 07:07:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	102522	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	170024	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	154701	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	74988	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	61796	50.213	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 100.420%	
35) Dibromofluoromethane	5.391	113	49517	48.883	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 97.760%	
50) Toluene-d8	8.653	98	194821	52.395	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 104.780%	
62) 4-Bromofluorobenzene	11.085	95	74998	57.290	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 114.580%	
Target Compounds						
						Qvalue
5) Bromomethane	1.605	94	202	0.438	ug/l	88
6) Chloroethane	1.806	64	20	Below Cal	#	43
10) Methyl Iodide	2.447	142	220	2.399	ug/l #	48
14) Allyl chloride	2.764	41	411	0.221	ug/l #	56
16) Acetone	2.404	43	397	0.734	ug/l #	46
18) Methyl Acetate	2.727	43	358	0.230	ug/l #	53
25) 2-Butanone	4.593	43	188	0.216	ug/l #	50
31) Cyclohexane	5.476	56	1393	0.712	ug/l	94
36) 1,1-Dichloropropene	5.556	75	7527	4.710	ug/l #	49
38) Carbon Tetrachloride	5.556	117	10180	6.075	ug/l #	17
39) Methylcyclohexane	7.379	83	1492	0.761	ug/l	89
43) Isopropyl Acetate	6.245	43	610	0.218	ug/l #	62
51) 4-Methyl-2-Pentanone	8.653	43	969	0.572	ug/l #	1
53) t-1,3-Dichloropropene	8.903	75	258	1.498	ug/l #	43
55) 1,1,2-Trichloroethane	9.104	97	224	0.201	ug/l #	15
67) Ethyl Benzene	10.195	91	20587	3.636	ug/l	100
68) m/p-Xylenes	10.305	106	8614	3.954	ug/l	95
69) o-Xylene	10.652	106	456	0.214	ug/l	97
73) Isopropylbenzene	10.963	105	2477	0.419	ug/l	98
76) 1,2,3-Trichloropropane	11.085	75	36775	22.403	ug/l #	40
78) n-propylbenzene	11.311	91	6845	1.045	ug/l	98
80) 1,3,5-Trimethylbenzene	11.457	105	2346	0.483	ug/l	95
81) trans-1,4-Dichloro-2-b...	11.085	75	36775	68.687	ug/l #	3
84) 1,2,4-Trimethylbenzene	11.756	105	3492	0.712	ug/l	100
89) n-Butylbenzene	12.335	91	1005	0.247	ug/l #	56
90) Hexachloroethane	12.615	117	363	0.505	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	12.762	75	85	0.216	ug/l #	3
95) Naphthalene	13.780	128	9716	1.771	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021822\
Data File : VX027118.D
Acq On : 18 Feb 2022 18:25
Operator : JC/MD
Sample : N1465-07ME
Misc : 6.42g/5.0mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5

Quant Time: Feb 21 00:42:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration




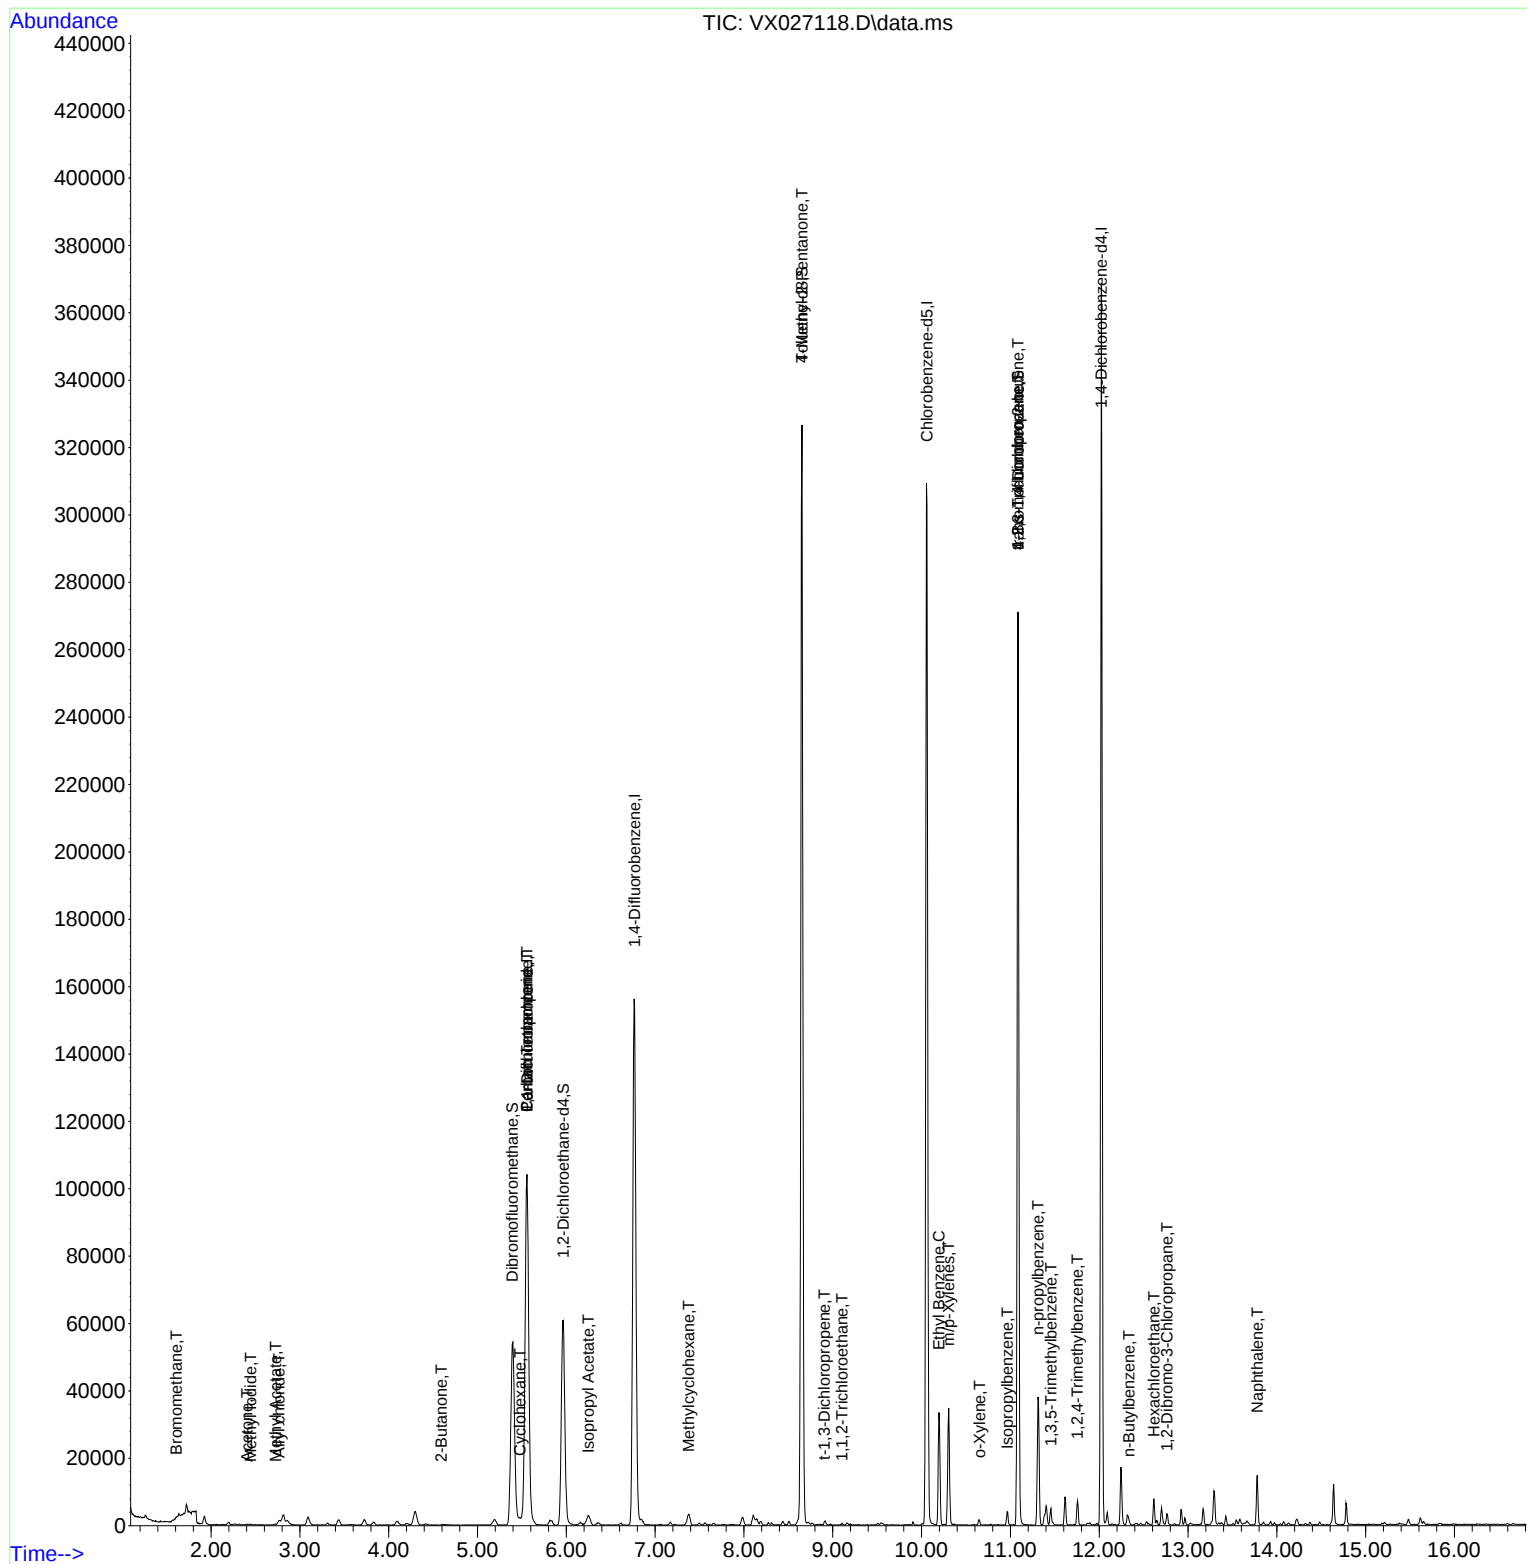


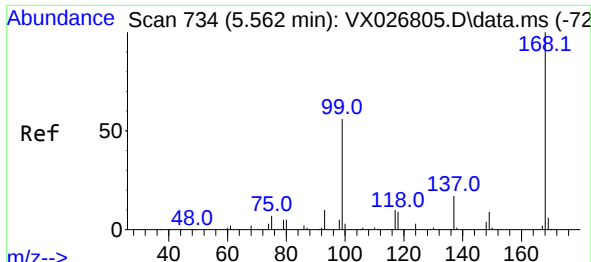

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25




Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5

Tgt Ion:168 Resp: 102522
Ion Ratio Lower Upper
168 100
99 57.0 50.3 75.5

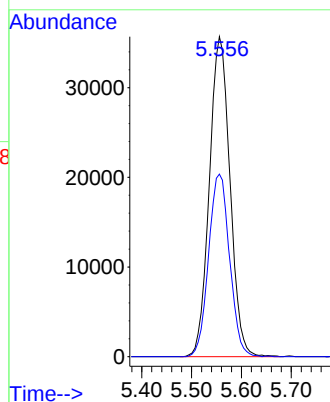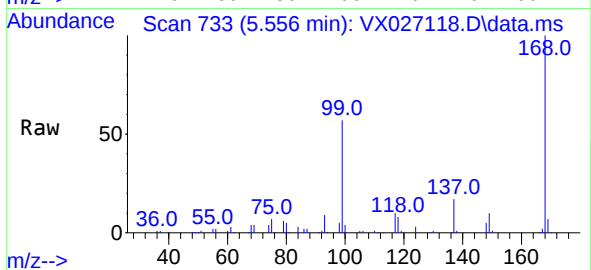


#5
Bromomethane
Concen: 0.438 ug/l
RT: 1.605 min Scan# 85
Delta R.T. -0.006 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25

Tgt Ion: 94 Resp: 202
Ion Ratio Lower Upper
94 100
96 83.2 75.9 113.9

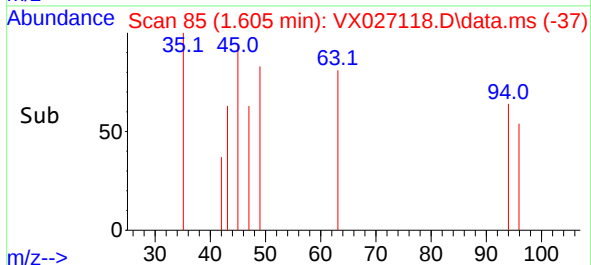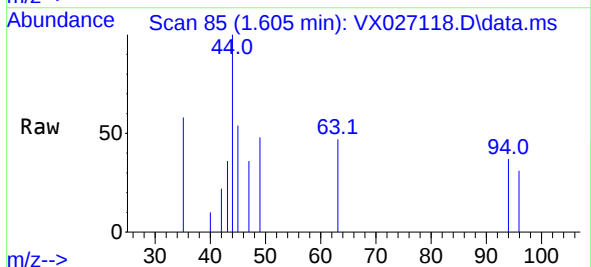

Abundance Scan 99 (1.691 min): VX026805.D\data.ms (-93)


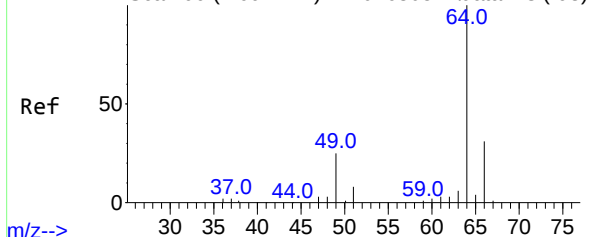


#6
Chloroethane
Concen: Below Cal
RT: 1.806 min Scan# 11
Delta R.T. 0.115 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25


Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5

Tgt Ion: 64 Resp: 20
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#


Abundance Scan 118 (1.806 min): VX027118.D\data.ms

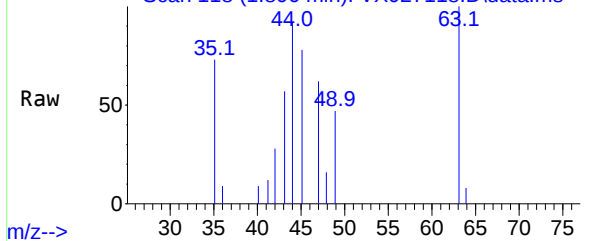

Abundance Scan 118 (1.806 min): VX027118.D\data.ms (-50)

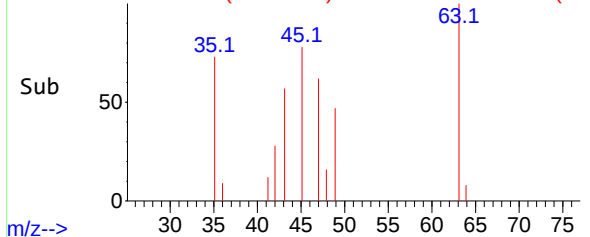



Abundance Scan 225 (2.459 min): VX026805.D\data.ms (-21)

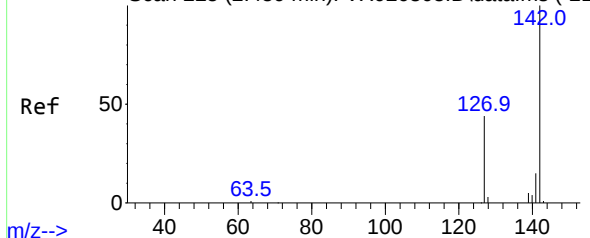


#10
Methyl Iodide
Concen: 2.399 ug/l
RT: 2.447 min Scan# 223
Delta R.T. -0.012 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25


Tgt Ion: 142 Resp: 220
Ion Ratio Lower Upper
142 100
127 9.1 38.1 57.1#
141 0.0 11.2 16.8#

Abundance Scan 223 (2.447 min): VX027118.D\data.ms

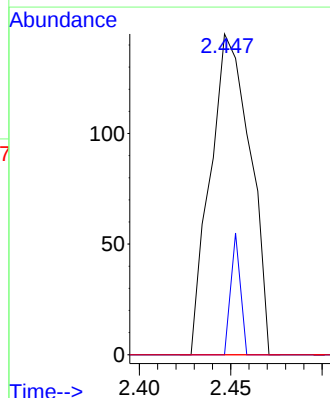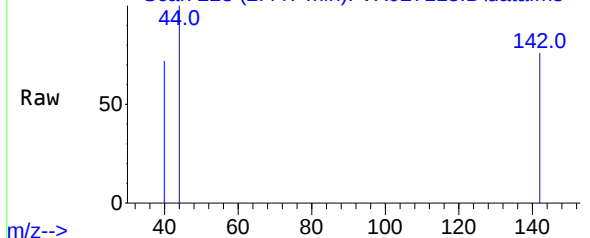

Abundance Scan 223 (2.447 min): VX027118.D\data.ms (-17)




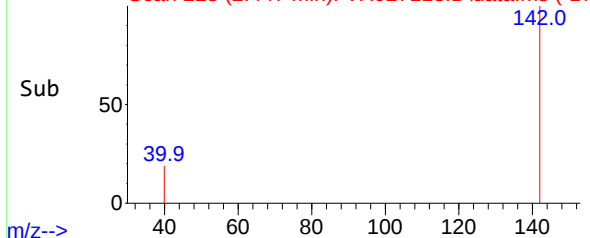




#14
 Allyl chloride
 Concen: 0.221 ug/l
 RT: 2.764 min Scan# 216
 Delta R.T. 0.098 min
 Lab File: VX027118.D
 Acq: 18 Feb 2022 18:25




Instrument :
 MSVOA_X
 ClientSampleId :
 A5-7-6.5


Tgt Ion:	41	Resp:	411
Ion	Ratio	Lower	Upper
41	100		
39	37.7	54.2	81.4#
76	0.0	25.2	37.8#

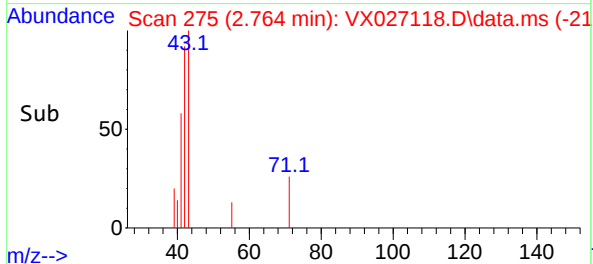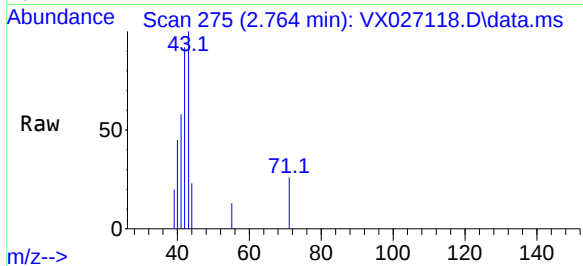

#16
 Acetone
 Concen: 0.734 ug/l
 RT: 2.404 min Scan# 216
 Delta R.T. 0.018 min
 Lab File: VX027118.D
 Acq: 18 Feb 2022 18:25

Tgt Ion:	43	Resp:	397
Ion	Ratio	Lower	Upper
43	100		
58	0.0	23.0	34.6#

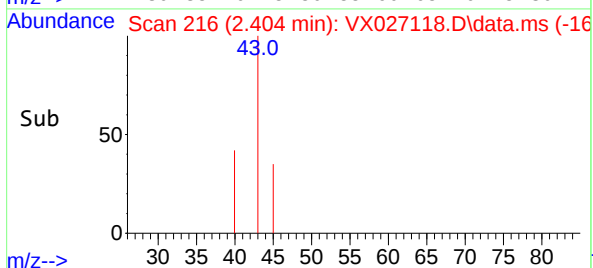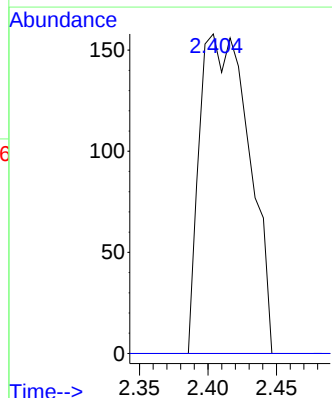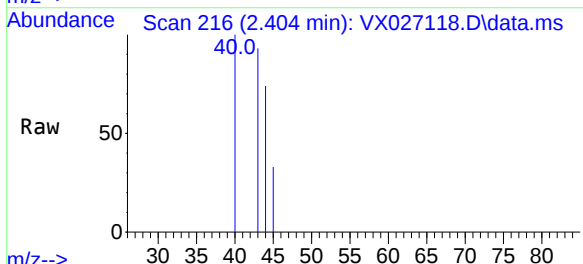



#18

Methyl Acetate

Concen: 0.230 ug/l

RT: 2.727 min Scan# 2

Delta R.T. 0.018 min

Lab File: VX027118.D

Acq: 18 Feb 2022 18:25

Instrument :

MSVOA_X

ClientSampleId :


A5-7-6.5

Tgt Ion: 43 Resp: 358




Ion Ratio Lower Upper

43 100

74 0.0 18.3 27.5#

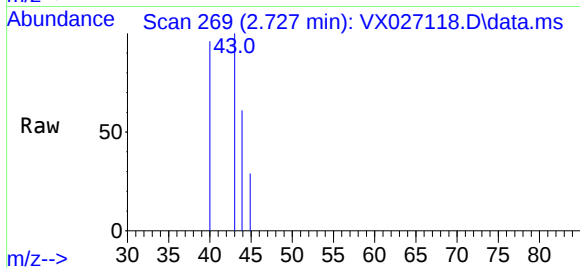

Abundance

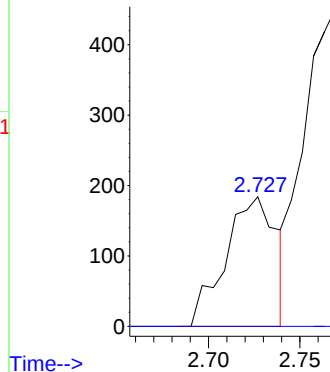

#25

2-Butanone

Concen: 0.216 ug/l

RT: 4.593 min Scan# 575

Delta R.T. 0.030 min

Lab File: VX027118.D


Acq: 18 Feb 2022 18:25

Tgt Ion: 43 Resp: 188



Ion Ratio Lower Upper


43 100

72 0.0 20.4 30.6#

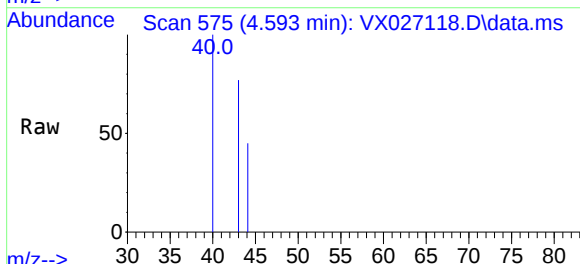

Abundance



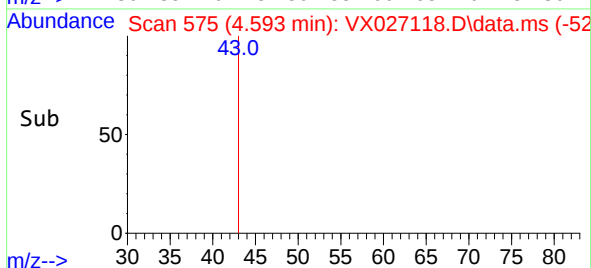
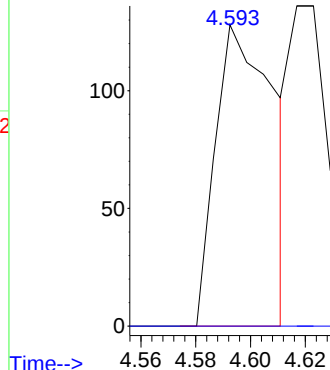




#31
Cyclohexane
Concen: 0.712 ug/l
RT: 5.476 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25




Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5


Tgt Ion: 56	Resp:	1393	
Ion	Ratio	Lower	Upper
56	100		
69	26.1	25.8	38.6
84	81.7	68.9	103.3

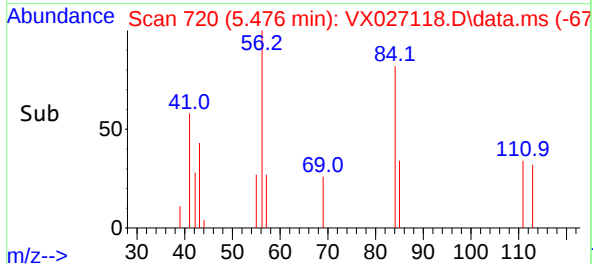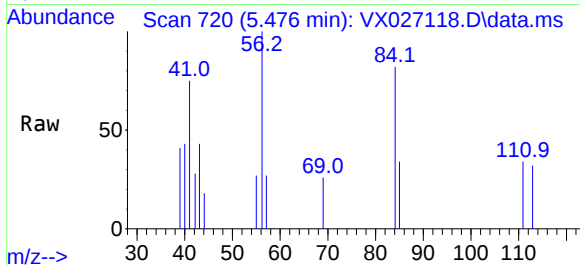

#33
1,2-Dichloroethane-d4
Concen: 50.213 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.000 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25

Tgt Ion: 65	Resp:	61796	
Ion	Ratio	Lower	Upper
65	100		
67	51.7	0.0	100.8

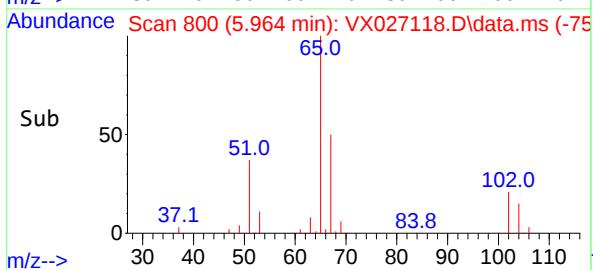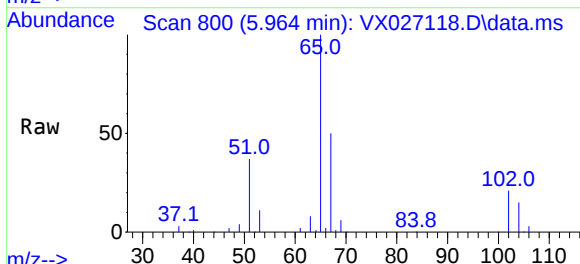

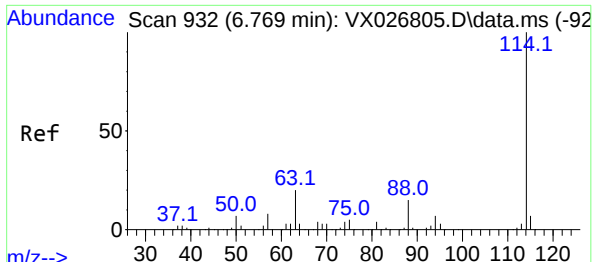

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 91

Delta R.T. -0.000 min

Lab File: VX027118.D

Acq: 18 Feb 2022 18:25

Instrument :

MSVOA_X

ClientSampleId :

A5-7-6.5





Tgt Ion:114 Resp: 170024

Ion Ratio Lower Upper

114 100

63 19.2 0.0 42.8

88 15.4 0.0 33.0

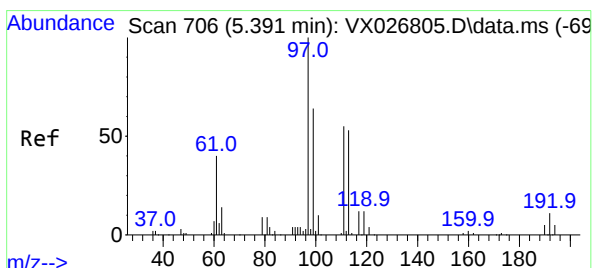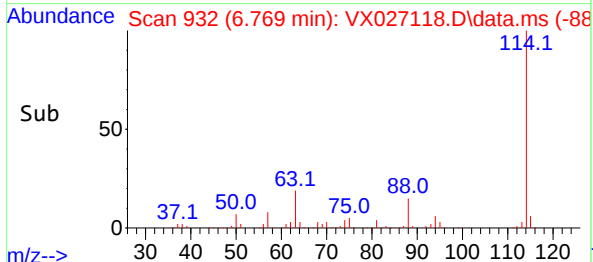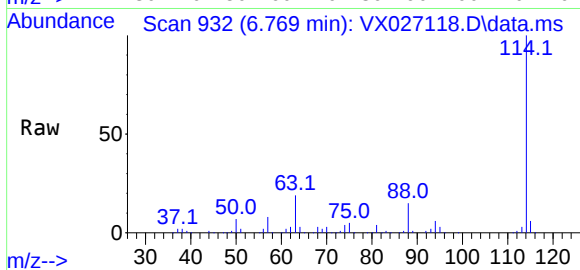

#35

Dibromofluoromethane

Concen: 48.883 ug/l

RT: 5.391 min Scan# 706

Delta R.T. -0.000 min

Lab File: VX027118.D

Acq: 18 Feb 2022 18:25




Tgt Ion:113 Resp: 49517


Ion Ratio Lower Upper

113 100

111 103.0 81.2 121.8

192 20.1 15.0 22.4


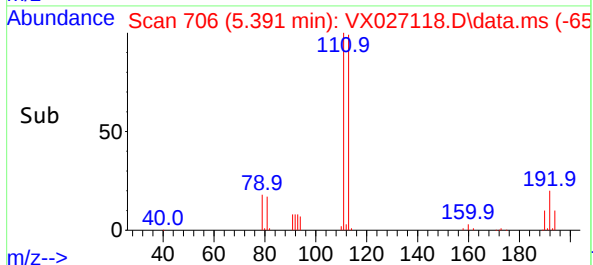

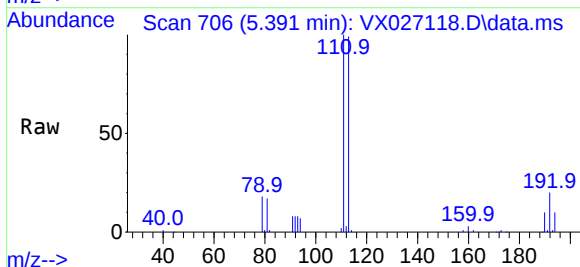




#36
1,1-Dichloropropene
Concen: 4.710 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.140 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25




Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5


Tgt Ion: 75 Resp: 7527
Ion Ratio Lower Upper
75 100
110 7.8 17.2 51.6#
77 0.0 24.6 36.8#

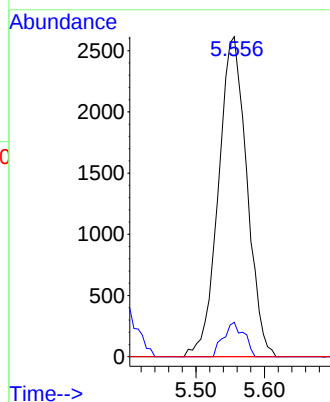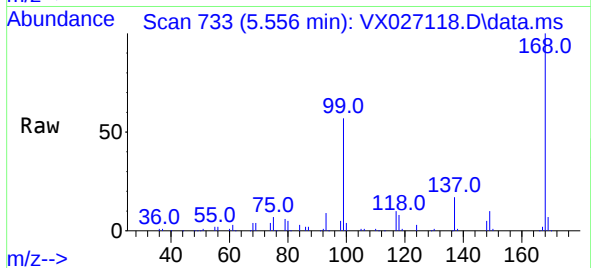

#38
Carbon Tetrachloride
Concen: 6.075 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.128 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25

Tgt Ion: 117 Resp: 10180
Ion Ratio Lower Upper
117 100
119 5.6 74.7 112.1#
121 0.0 25.4 38.0#

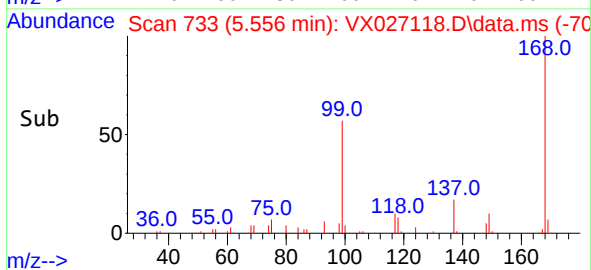



#39

Methylcyclohexane

Concen: 0.761 ug/l

RT: 7.379 min Scan# 1033

Delta R.T. -0.006 min

Lab File: VX027118.D

Acq: 18 Feb 2022 18:25

Instrument :

MSVOA_X

ClientSampleId :

A5-7-6.5





Tgt Ion: 83 Resp: 1492

Ion Ratio Lower Upper

83 100

55 89.3 63.6 95.4

98 55.5 38.4 57.6

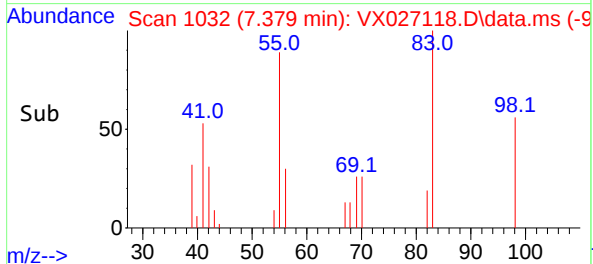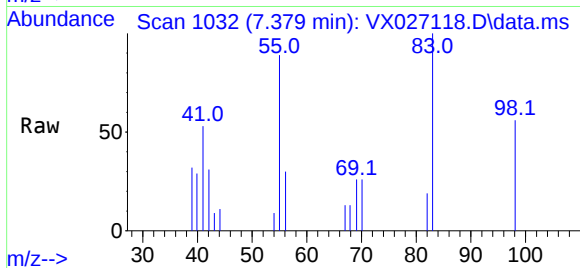

#43

Isopropyl Acetate

Concen: 0.218 ug/l

RT: 6.245 min Scan# 846

Delta R.T. -0.098 min

Lab File: VX027118.D

Acq: 18 Feb 2022 18:25




Tgt Ion: 43 Resp: 610


Ion Ratio Lower Upper

43 100

61 0.0 15.4 23.0#

87 0.0 10.2 15.2#


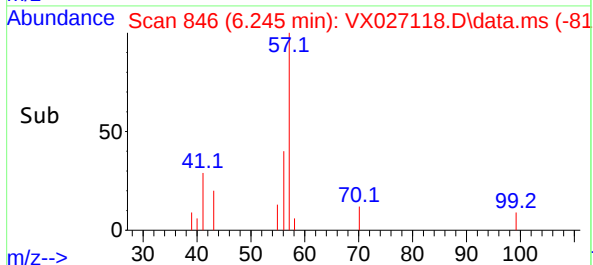
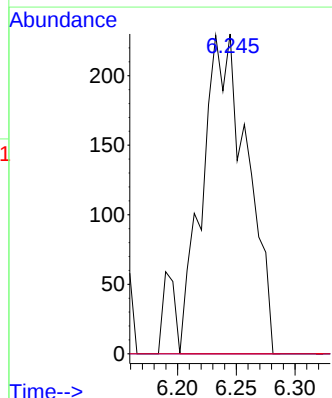
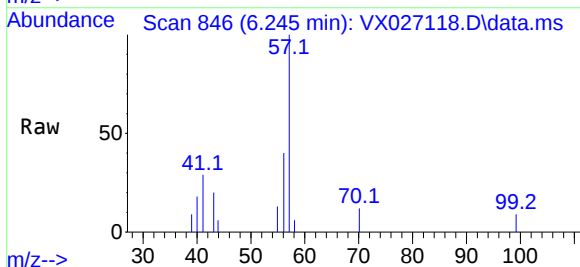




#50
Toluene-d8
Concen: 52.395 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25




Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5


Tgt Ion: 98 Resp: 194821
Ion Ratio Lower Upper
98 100
100 67.3 53.2 79.8

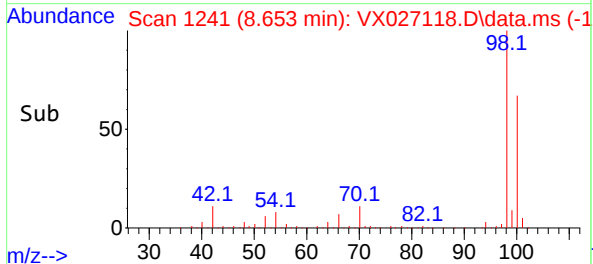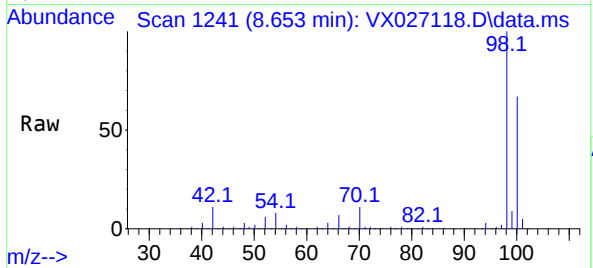

#51
4-Methyl-2-Pentanone
Concen: 0.572 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.079 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25

Tgt Ion: 43 Resp: 969
Ion Ratio Lower Upper
43 100
58 162.2 30.5 45.7#


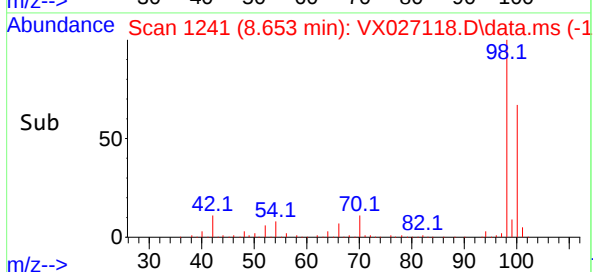

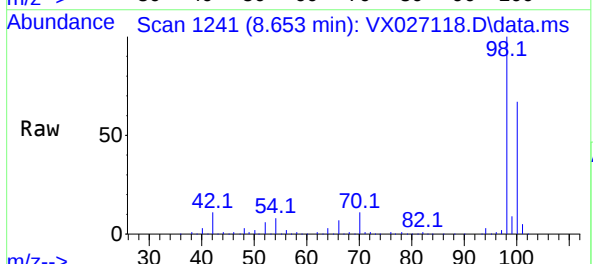




#53
t-1,3-Dichloropropene
Concen: 1.498 ug/l
RT: 8.903 min Scan# 1115
Delta R.T. -0.079 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25




Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5


Tgt Ion: 75 Resp: 258
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#

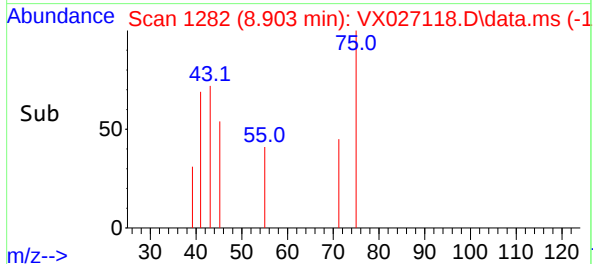

#55
1,1,2-Trichloroethane
Concen: 0.201 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.049 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25

Tgt Ion: 97 Resp: 224
Ion Ratio Lower Upper
97 100
83 0.0 68.4 102.6#
85 0.0 44.0 66.0#
99 0.0 49.8 74.6#


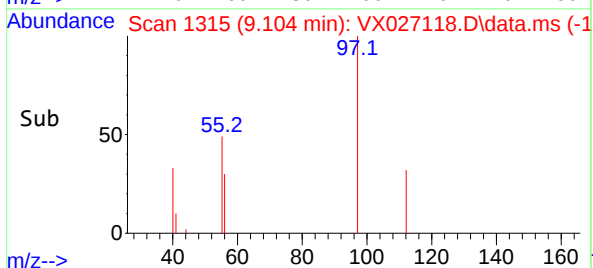
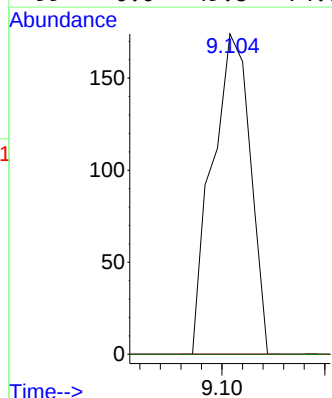
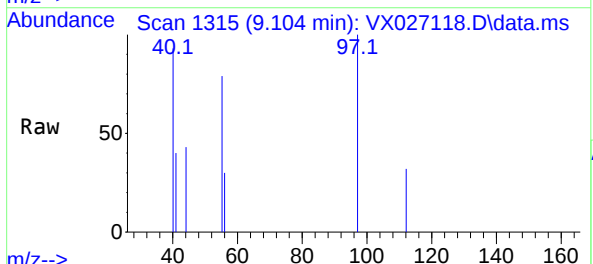




#62
4-Bromofluorobenzene
Concen: 57.290 ug/l
RT: 11.085 min Scan# 1639
Delta R.T. 0.006 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25




Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5


Tgt Ion: 95 Resp: 74998
Ion Ratio Lower Upper
95 100
174 78.6 0.0 148.6
176 75.3 0.0 141.4

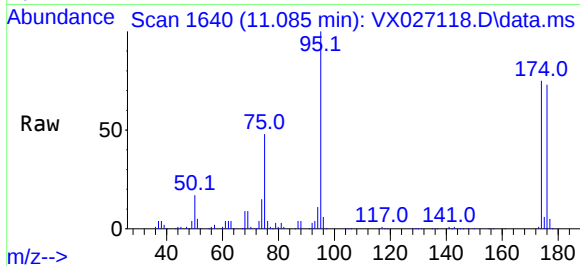

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.006 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25

Tgt Ion: 117 Resp: 154701
Ion Ratio Lower Upper
117 100
82 51.8 45.2 67.8
119 32.9 26.2 39.2

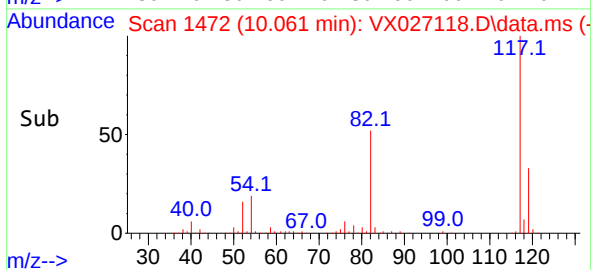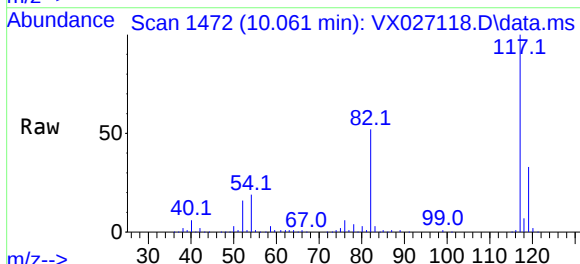



#67

Ethyl Benzene

Concen: 3.636 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. -0.000 min

Lab File: VX027118.D

Acq: 18 Feb 2022 18:25

Instrument :

MSVOA_X

ClientSampleId :





A5-7-6.5

Tgt Ion: 91 Resp: 20587

Ion Ratio Lower Upper

91 100

106 31.0 24.7 37.1

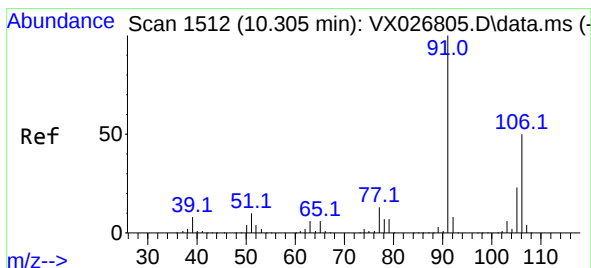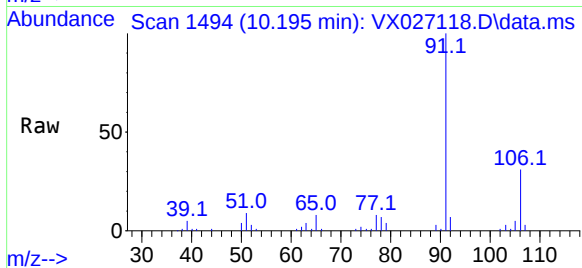

#68

m/p-Xylenes

Concen: 3.954 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. -0.000 min

Lab File: VX027118.D




Acq: 18 Feb 2022 18:25


Tgt Ion: 106 Resp: 8614

Ion Ratio Lower Upper

106 100

91 198.3 165.3 247.9


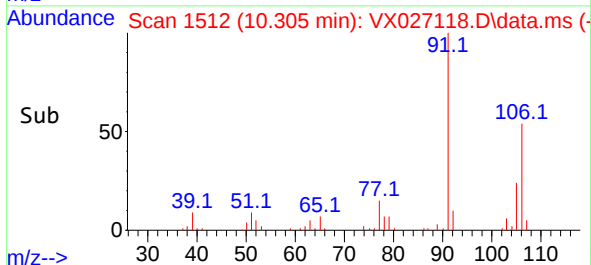
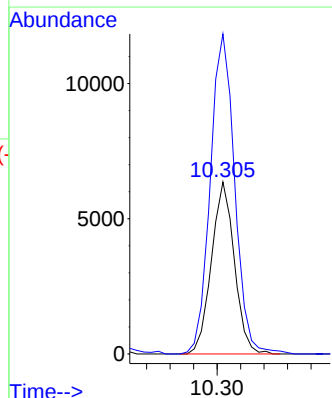
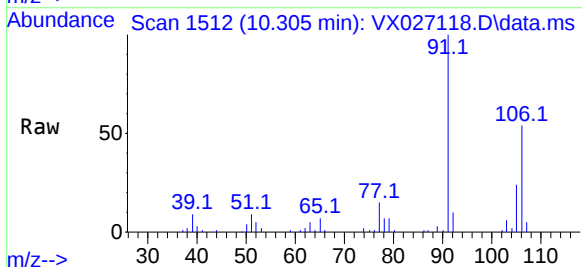




#69
o-Xylene
Concen: 0.214 ug/l
RT: 10.652 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25




Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5


Tgt Ion:106 Resp: 456
Ion Ratio Lower Upper
106 100
91 224.6 109.7 329.0

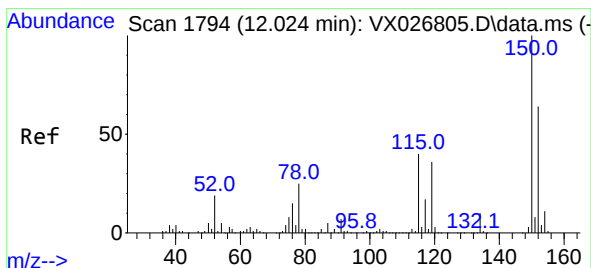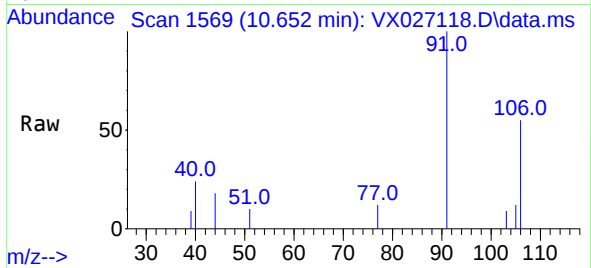

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25

Tgt Ion:152 Resp: 74988
Ion Ratio Lower Upper
152 100
115 59.4 44.2 132.6
150 158.4 0.0 348.2


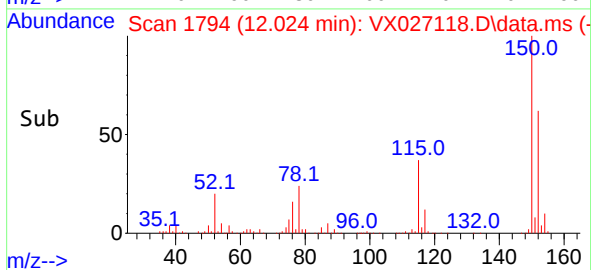

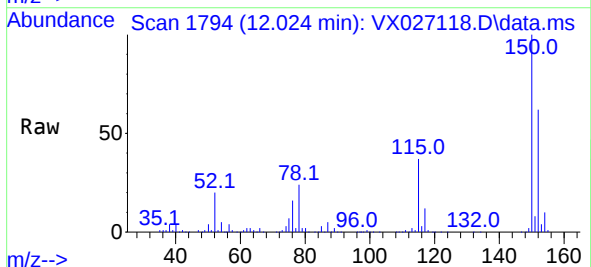




#73
Isopropylbenzene
Concen: 0.419 ug/l
RT: 10.963 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25




Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5


Tgt Ion:105 Resp: 2477
Ion Ratio Lower Upper
105 100
120 25.2 13.1 39.1

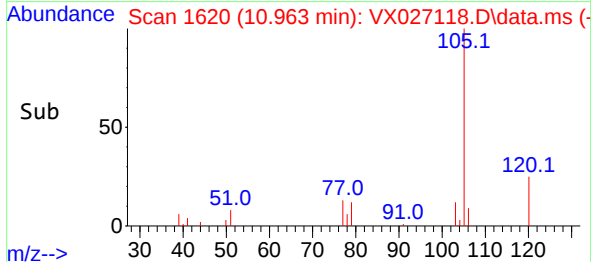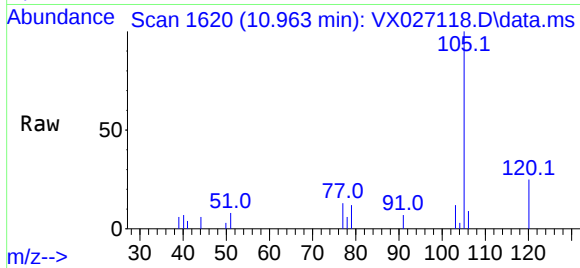

#76
1,2,3-Trichloropropane
Concen: 22.403 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25

Tgt Ion: 75 Resp: 36775
Ion Ratio Lower Upper
75 100
77 1.2 18.3 54.8#


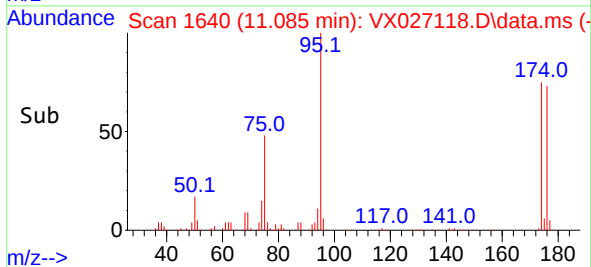

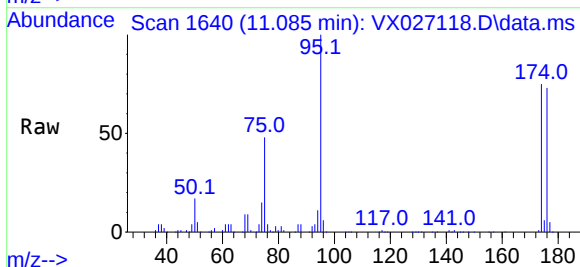




#78
n-propylbenzene
Concen: 1.045 ug/l
RT: 11.311 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25




Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5


Tgt Ion: 91 Resp: 6845
Ion Ratio Lower Upper
91 100
120 24.0 11.6 34.7

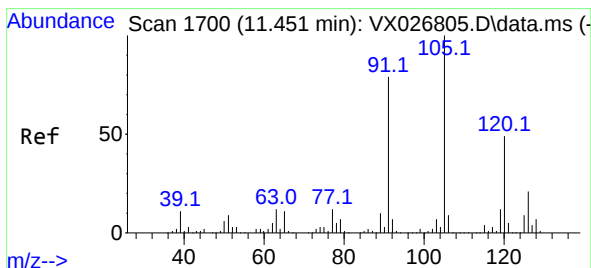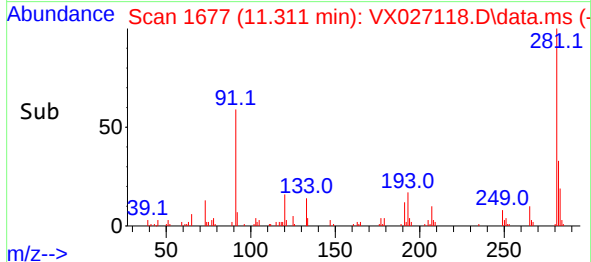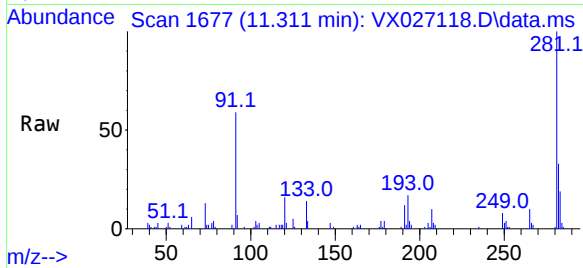

#80
1,3,5-Trimethylbenzene
Concen: 0.483 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25

Tgt Ion: 105 Resp: 2346
Ion Ratio Lower Upper
105 100
120 51.2 24.0 72.0


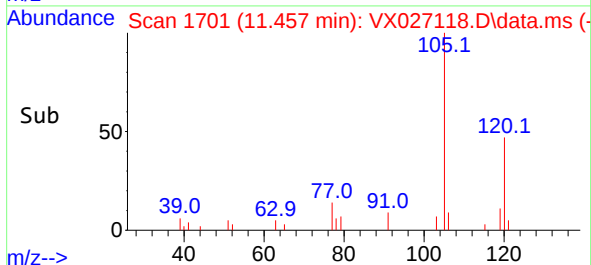
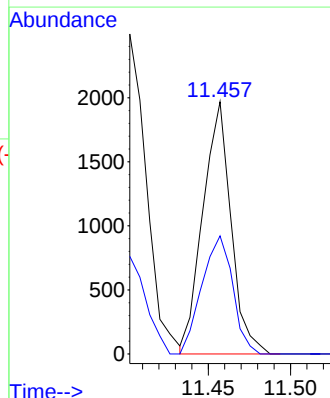
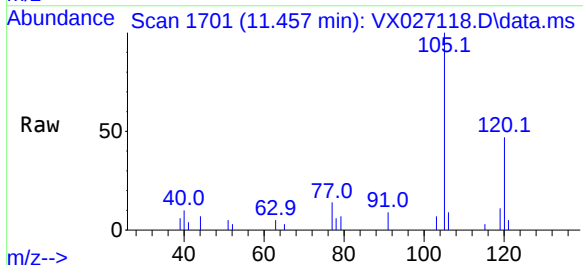




#81
trans-1,4-Dichloro-2-butene
Concen: 68.687 ug/l
RT: 11.085 min Scan# 1100
Delta R.T. 0.067 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25




Instrument :
MSVOA_X
ClientSampleId :
A5-7-6.5


Tgt Ion: 75 Resp: 36775
Ion Ratio Lower Upper
75 100
53 0.0 94.0 141.0#
89 0.0 37.0 55.4#

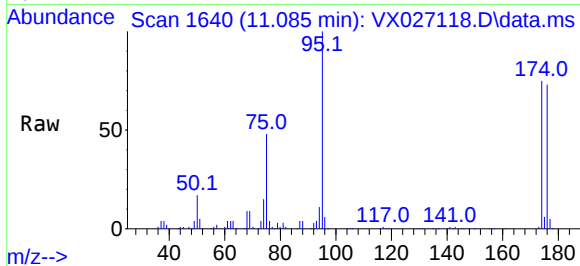

#84
1,2,4-Trimethylbenzene
Concen: 0.712 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX027118.D
Acq: 18 Feb 2022 18:25

Tgt Ion: 105 Resp: 3492
Ion Ratio Lower Upper
105 100
120 44.0 21.9 65.5

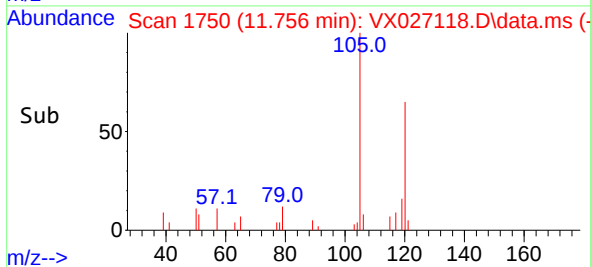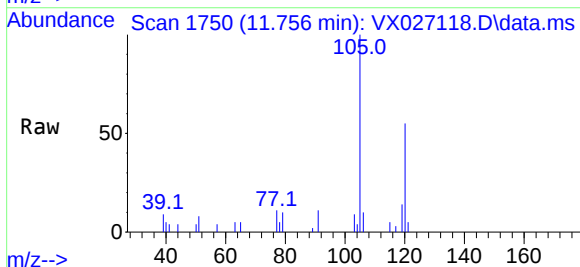



#89

n-Butylbenzene

Concen: 0.247 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. -0.000 min

Lab File: VX027118.D

Acq: 18 Feb 2022 18:25

Instrument :

MSVOA_X

ClientSampleId :

A5-7-6.5





Tgt Ion: 91 Resp: 1005

Ion Ratio Lower Upper

91 100

92 39.2 27.2 81.6

134 73.3 13.1 39.1#

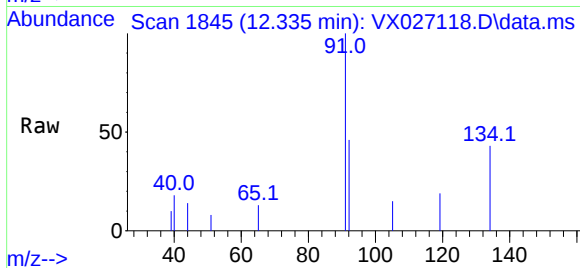

#90

Hexachloroethane

Concen: 0.505 ug/l

RT: 12.615 min Scan# 1891

Delta R.T. 0.073 min

Lab File: VX027118.D




Acq: 18 Feb 2022 18:25


Tgt Ion: 117 Resp: 363

Ion Ratio Lower Upper

117 100

201 0.0 35.6 106.8#


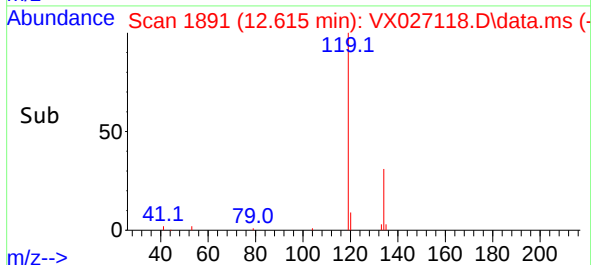
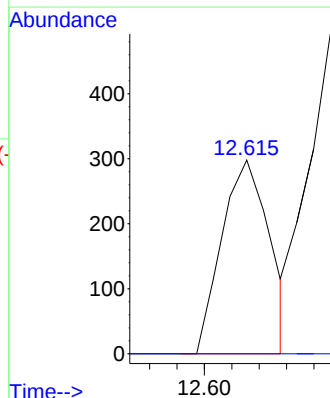
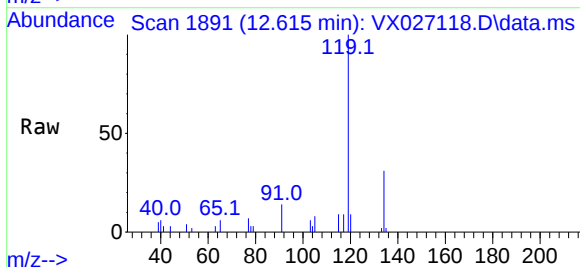




#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.216 ug/l
 RT: 12.762 min Scan# 1915
 Delta R.T. -0.183 min
 Lab File: VX027118.D
 Acq: 18 Feb 2022 18:25

Instrument :
 MSVOA_X
 ClientSampleId :
 A5-7-6.5

Tgt Ion: 75 Resp: 85
 Ion Ratio Lower Upper
 75 100
 155 0.0 40.0 119.9#
 157 0.0 51.6 154.8#

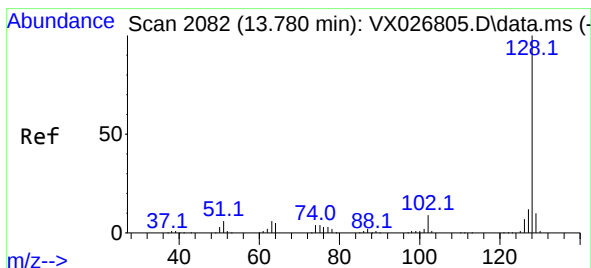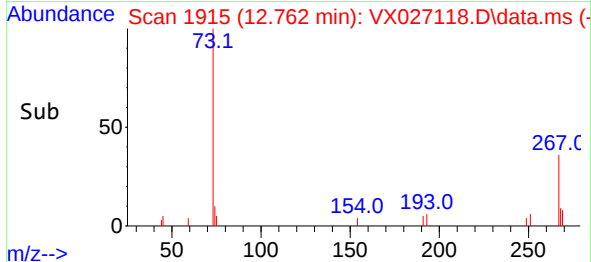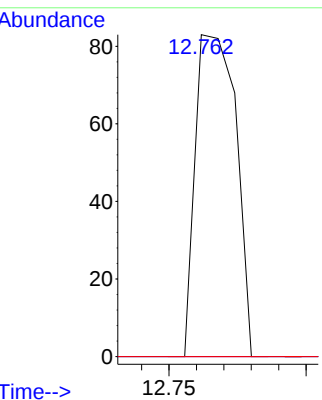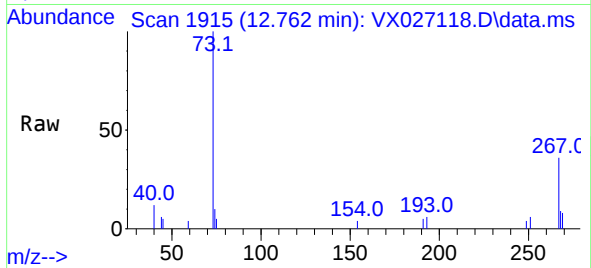

#95
 Naphthalene
 Concen: 1.771 ug/l
 RT: 13.780 min Scan# 2082
 Delta R.T. -0.000 min
 Lab File: VX027118.D
 Acq: 18 Feb 2022 18:25

Tgt Ion: 128 Resp: 9716
 Ion Ratio Lower Upper
 128 100
 127 12.4 10.3 15.5
 129 10.4 8.7 13.1

