


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021822\
Data File : VX027091.D
Acq On : 17 Feb 2022 20:48
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X021822W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Feb 18 05:14:00 2022

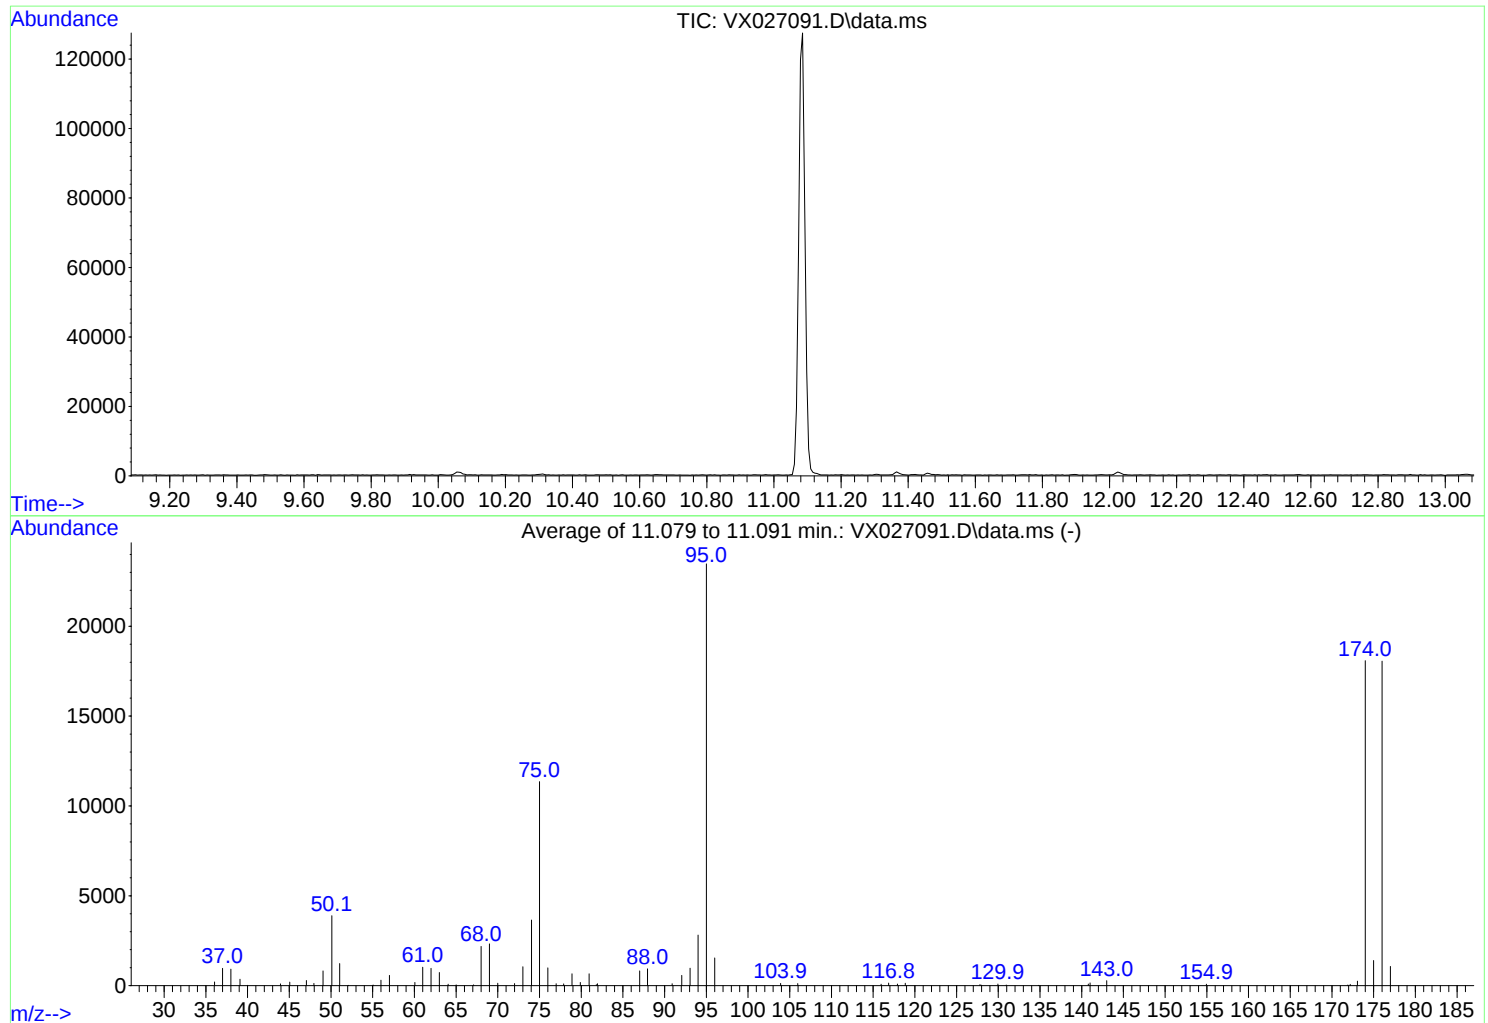

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	3891	PASS
75	95	30	60	48.4	11355	PASS
95	95	100	100	100.0	23473	PASS
96	95	5	9	6.5	1537	PASS
173	174	0.00	2	1.4	253	PASS
174	95	50	100	77.0	18085	PASS
175	174	5	9	7.7	1394	PASS
176	174	95	101	99.8	18054	PASS
177	176	5	9	5.9	1073	PASS