


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021822\
 Data File : VX027099.D
 Acq On : 18 Feb 2022 09:40
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X021822W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Feb 18 05:14:00 2022

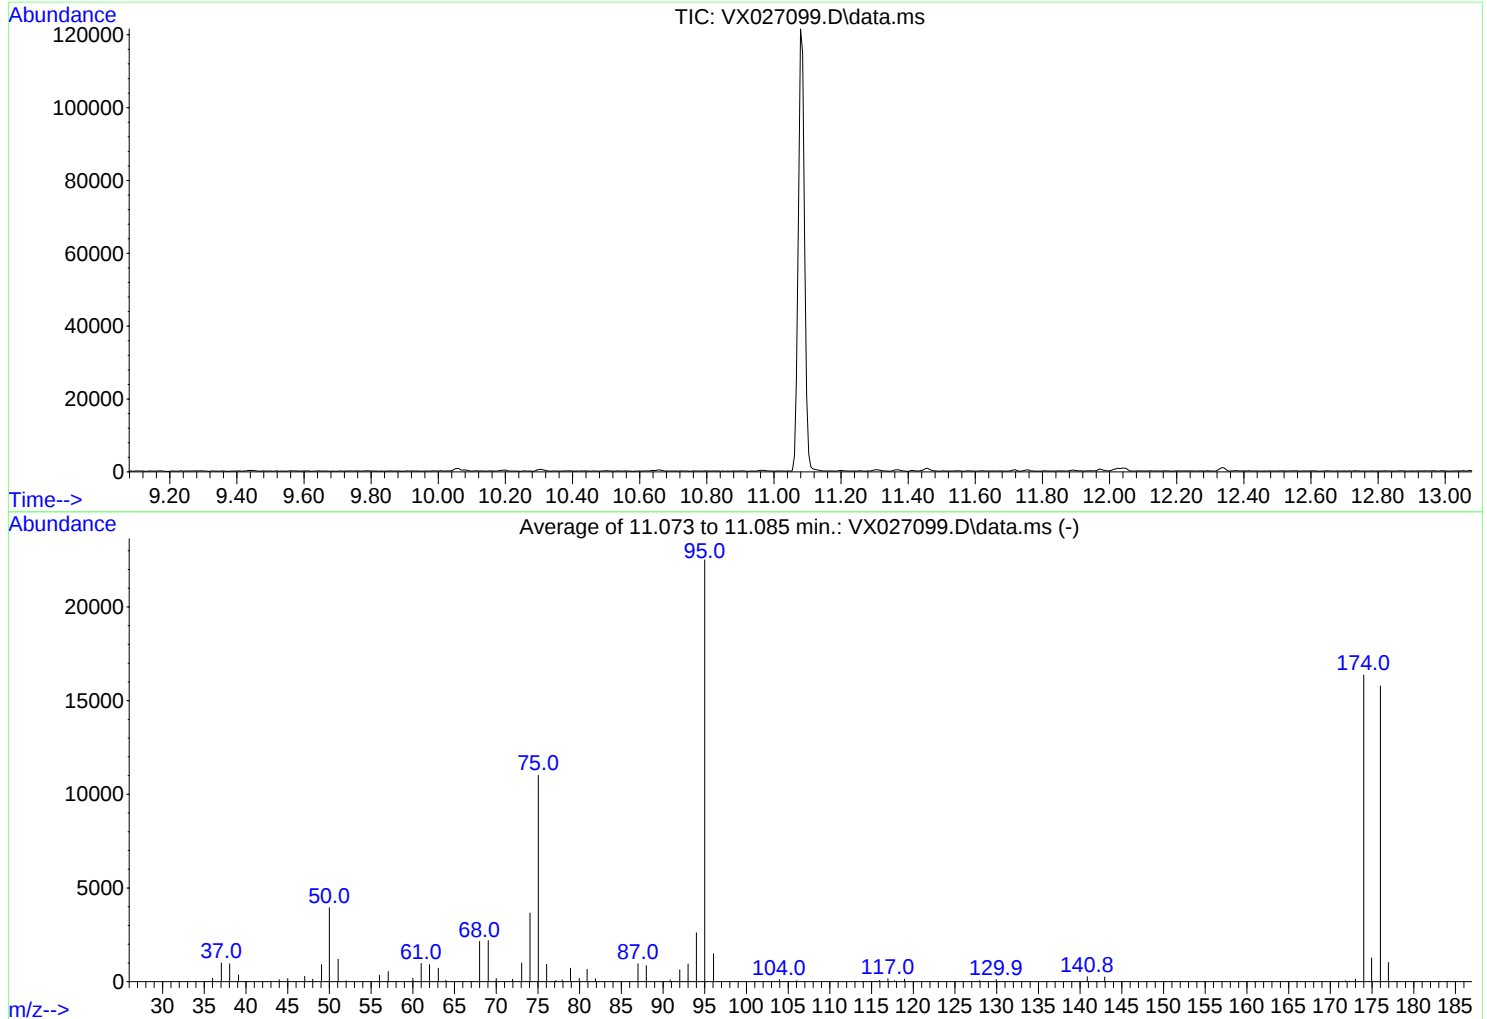

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	3947	PASS
75	95	30	60	48.9	11014	PASS
95	95	100	100	100.0	22514	PASS
96	95	5	9	6.6	1486	PASS
173	174	0.00	2	0.9	141	PASS
174	95	50	100	72.7	16363	PASS
175	174	5	9	7.7	1262	PASS
176	174	95	101	96.5	15785	PASS
177	176	5	9	6.5	1029	PASS