

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX021919\
 Data File : VX007603.D
 Acq On : 19 Feb 2019 10:44
 Operator : JC/SP
 Sample : VX0219MBL01
 Misc : 5.00µ/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0219MBL01

Quant Time: Feb 20 04:13:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
 Quant Title : SW846 8260
 QLast Update : Sat Feb 02 01:32:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	446956	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	714224	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	678799	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	322724	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	253196	53.37	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.74%	
35) Dibromofluoromethane	5.50	113	238509	51.32	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.64%	
50) Toluene-d8	8.71	98	874080	50.70	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.40%	
62) 4-Bromofluorobenzene	11.13	95	303031	48.14	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.28%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX021919\
Data File : VX007603.D
Acq On : 19 Feb 2019 10:44
Operator : JC/SP
Sample : VX0219MBL01
Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0219MBL01

Quant Time: Feb 20 04:13:34 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260
QLast Update : Sat Feb 02 01:32:36 2019
Response via : Initial Calibration

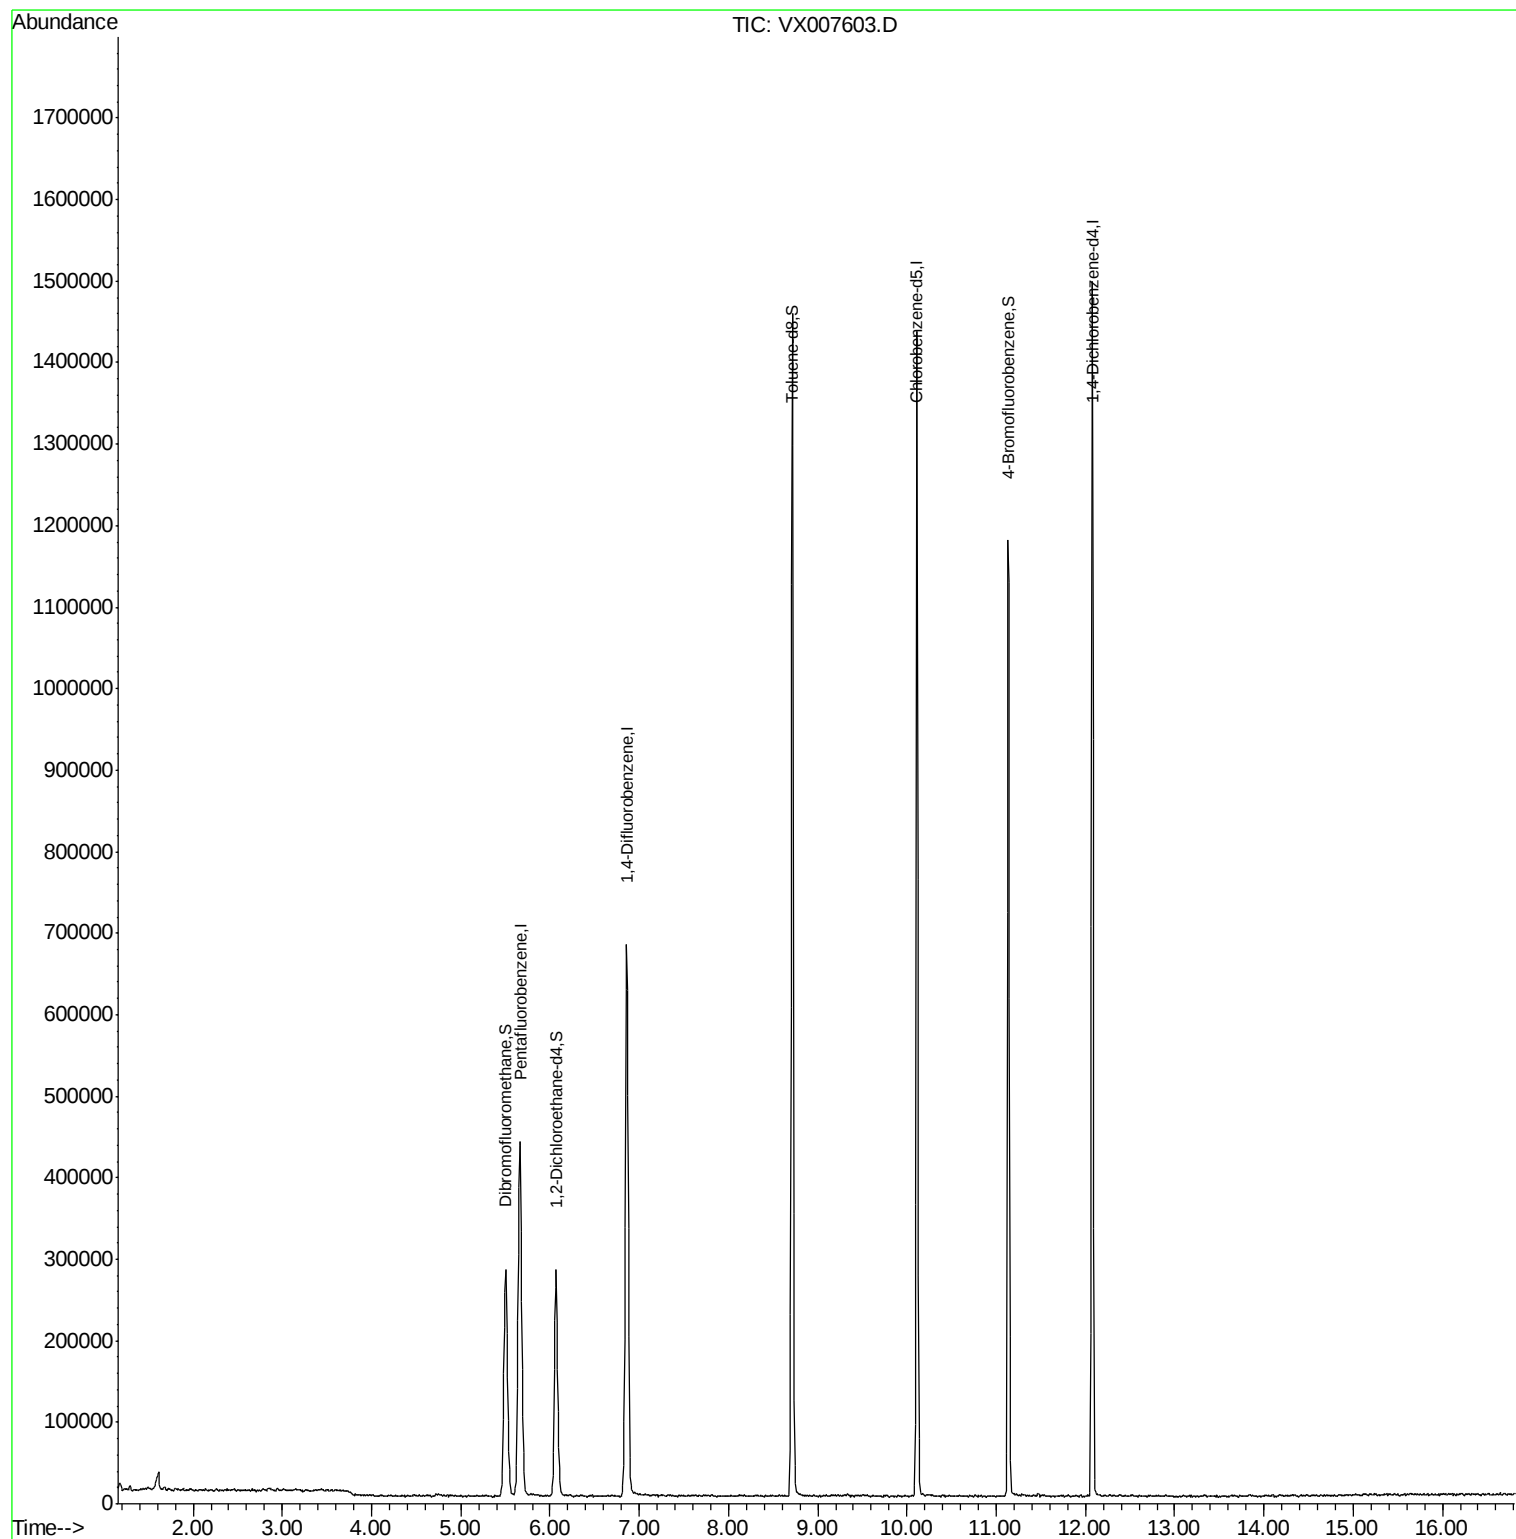

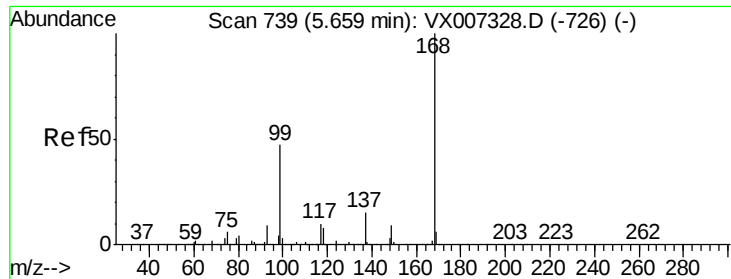

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX007603.D

Acq: 19 Feb 2019 10:44

Instrument :

MSVOA_X

ClientSampleId :


VX0219MBL01

Tot Ion:168 Resp: 446956

Ion Ratio Lower Upper

168 100

99 49.1 37.9 56.9

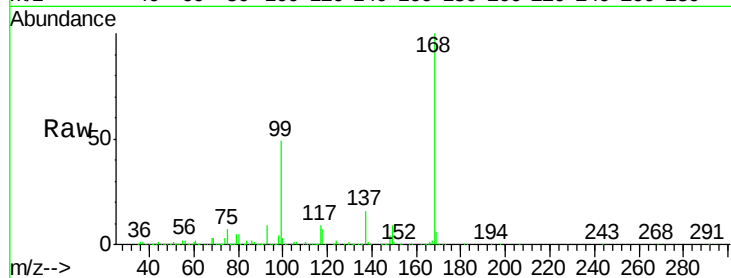

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67



150000

100000

50000

0

Time-->

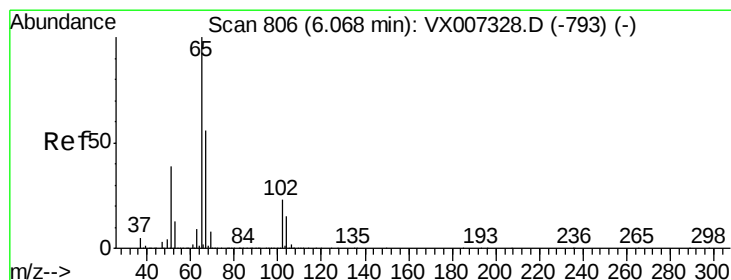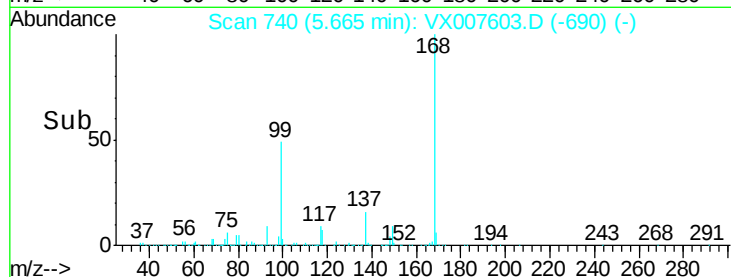

#33

1,2-Dichloroethane-d4

Concen: 53.371 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX007603.D


Acq: 19 Feb 2019 10:44

Tgt Ion: 65 Resp: 253196

Ion Ratio Lower Upper

65 100

67 53.8 0.0 108.8

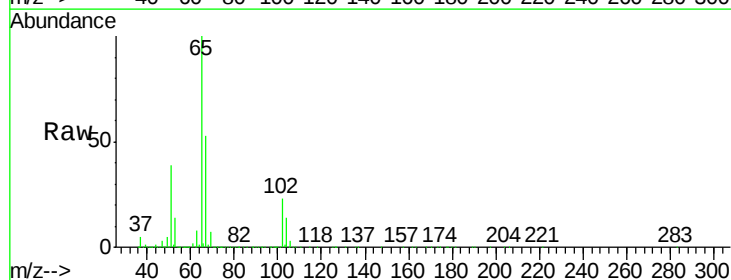

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

100000

80000


60000


40000

20000

0

Time-->

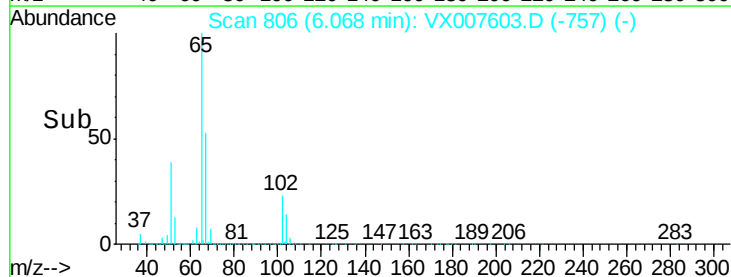

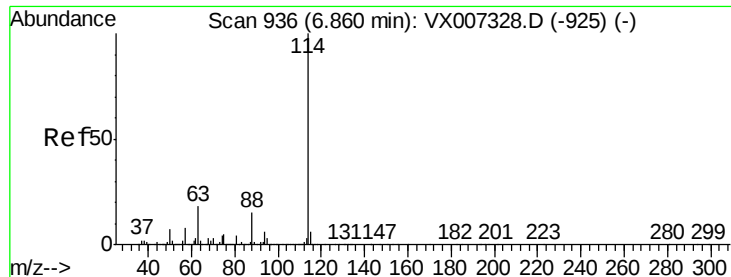

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX007603.D

Acq: 19 Feb 2019 10:44

Instrument :

MSVOA_X

ClientSampleId :

VX0219MBL01


Tot Ion:114 Resp: 714224

Ion Ratio Lower Upper

114 100

63 19.2 0.0 35.6




88 14.6 0.0 29.6

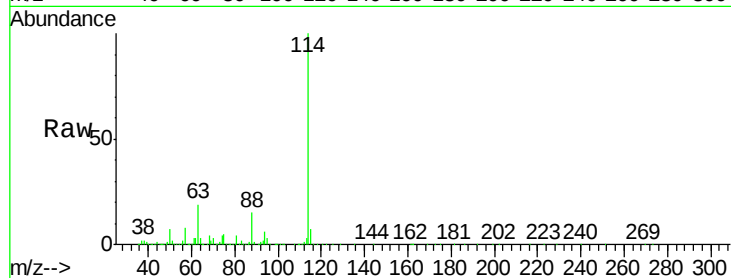

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

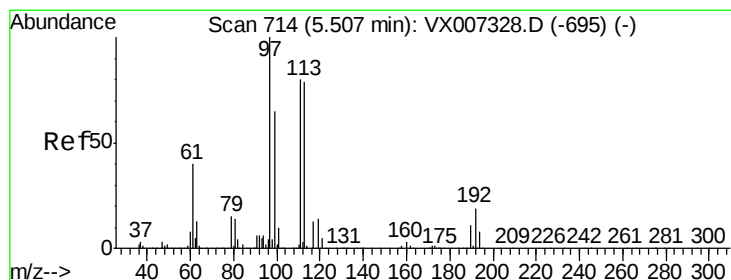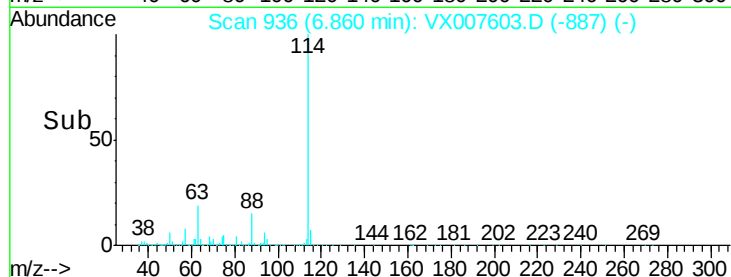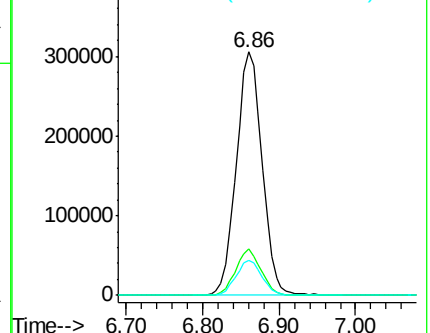

#35

Dibromofluoromethane

Concen: 51.323 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.01 min

Lab File: VX007603.D

Acq: 19 Feb 2019 10:44


Tgt Ion:113 Resp: 238509

Ion Ratio Lower Upper

113 100

111 101.3 81.8 122.8



192 21.7 18.5 27.7

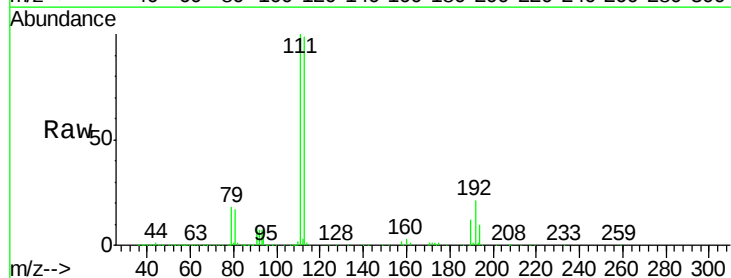


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

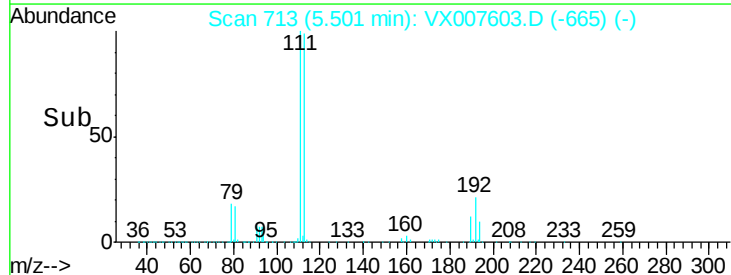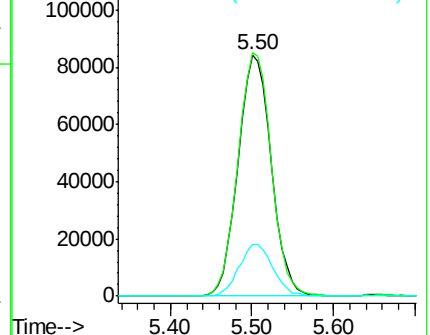

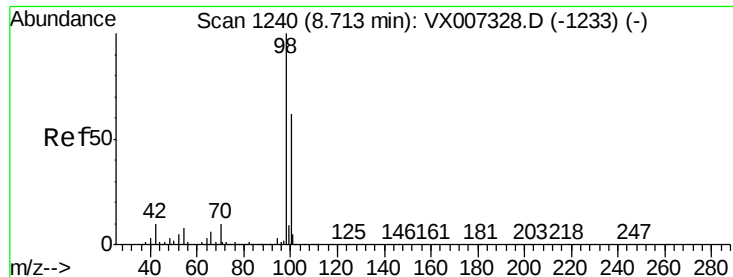

#50

Toluene-d8

Concen: 50.695 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX007603.D

Acq: 19 Feb 2019 10:44

Instrument :

MSVOA_X

ClientSampleId :





VX0219MBL01

Tot Ion: 98 Resp: 874080

Ion Ratio Lower Upper

98 100

100 63.8 51.6 77.4

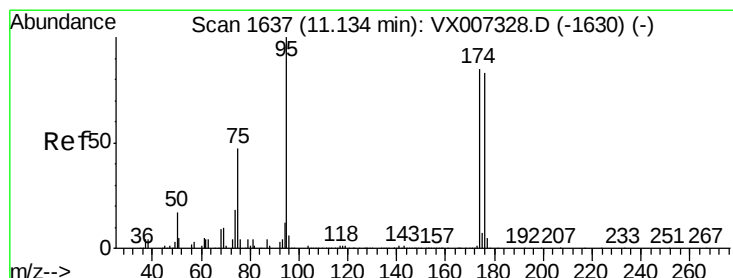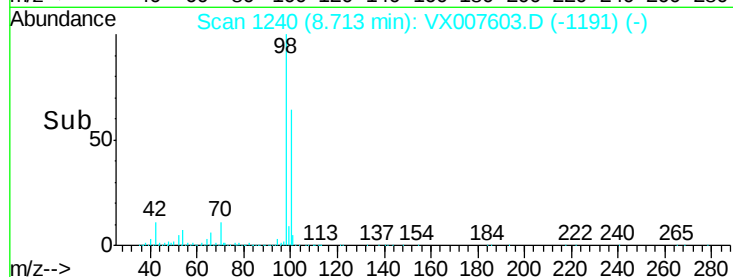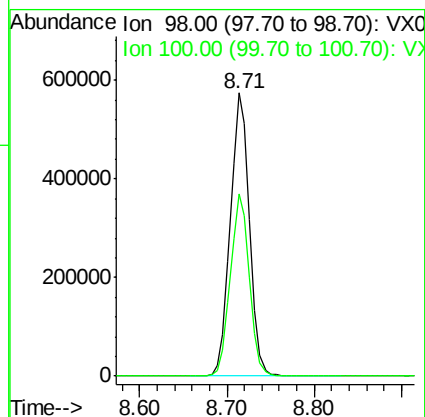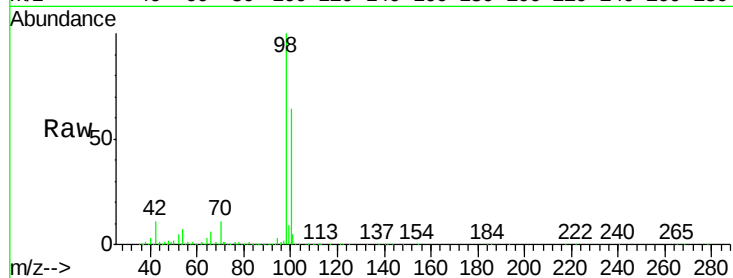

#62

4-Bromofluorobenzene

Concen: 48.138 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX007603.D

Acq: 19 Feb 2019 10:44




Tgt Ion: 95 Resp: 303031


Ion Ratio Lower Upper

95 100

174 93.2 0.0 189.2

176 88.8 0.0 186.2

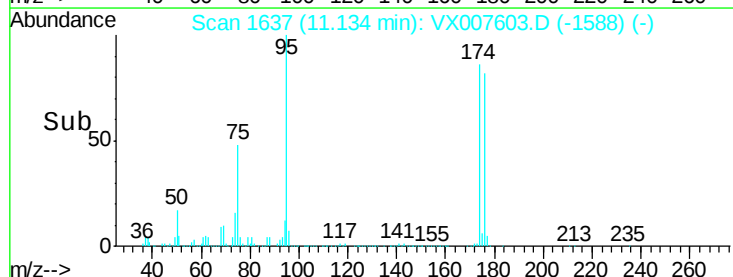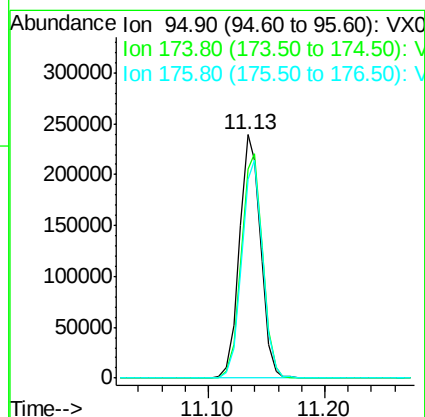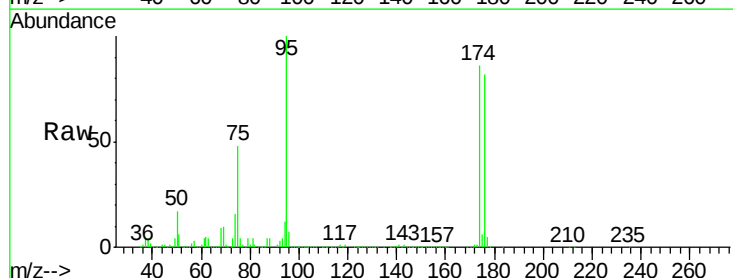

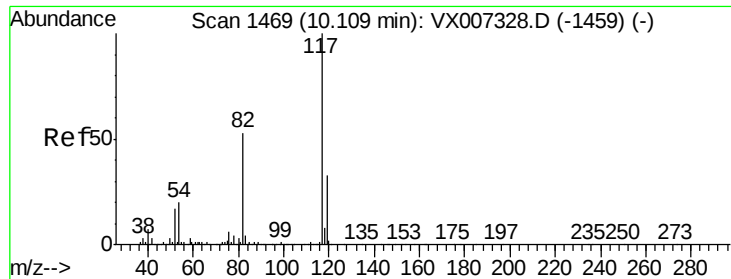

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VX007603.D

Acq: 19 Feb 2019 10:44

Instrument :

MSVOA_X

ClientSampleId :

VX0219MBL01


Tot Ion:117 Resp: 678799

Ion Ratio Lower Upper

117 100

82 52.6 42.1 63.1




119 32.2 26.5 39.7

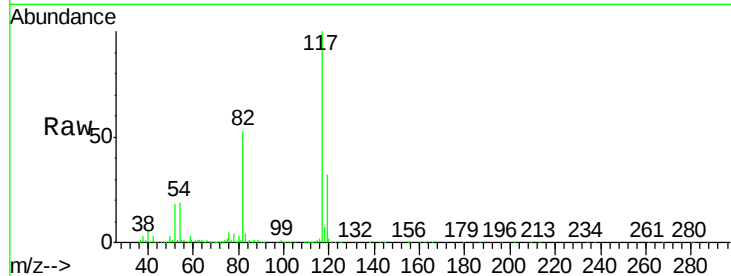

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

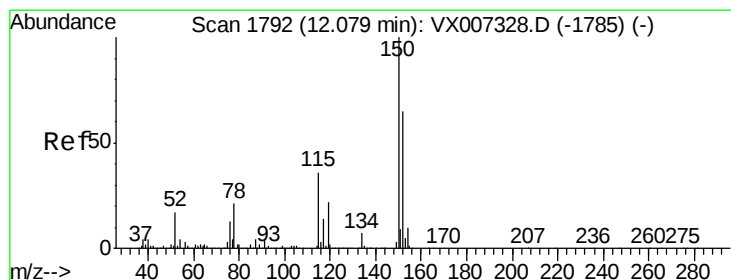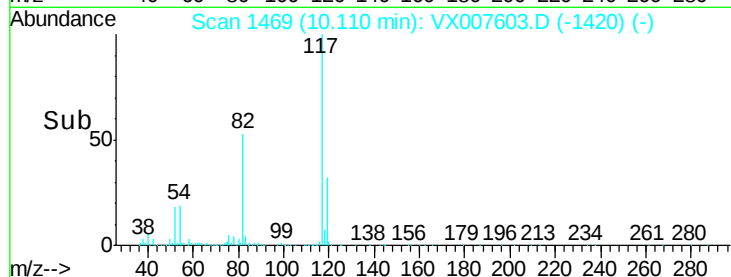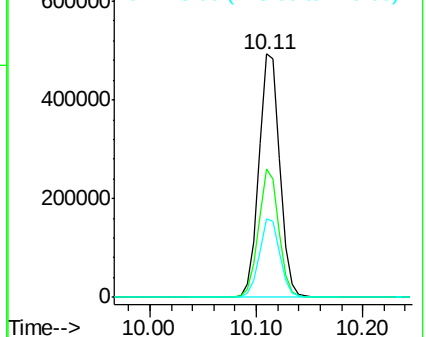

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX007603.D

Acq: 19 Feb 2019 10:44


Tgt Ion:152 Resp: 322724

Ion Ratio Lower Upper

152 100

115 55.7 38.0 114.0

150 157.4 0.0 346.4

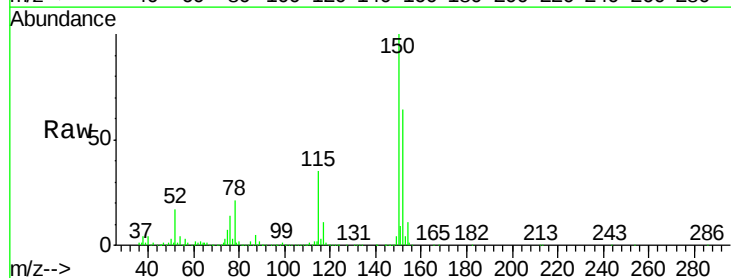

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

