


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX021919\
Data File : VX007600.D
Acq On : 19 Feb 2019 09:01
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Title : SW846 8260
Last Update : Sat Feb 02 01:32:36 2019

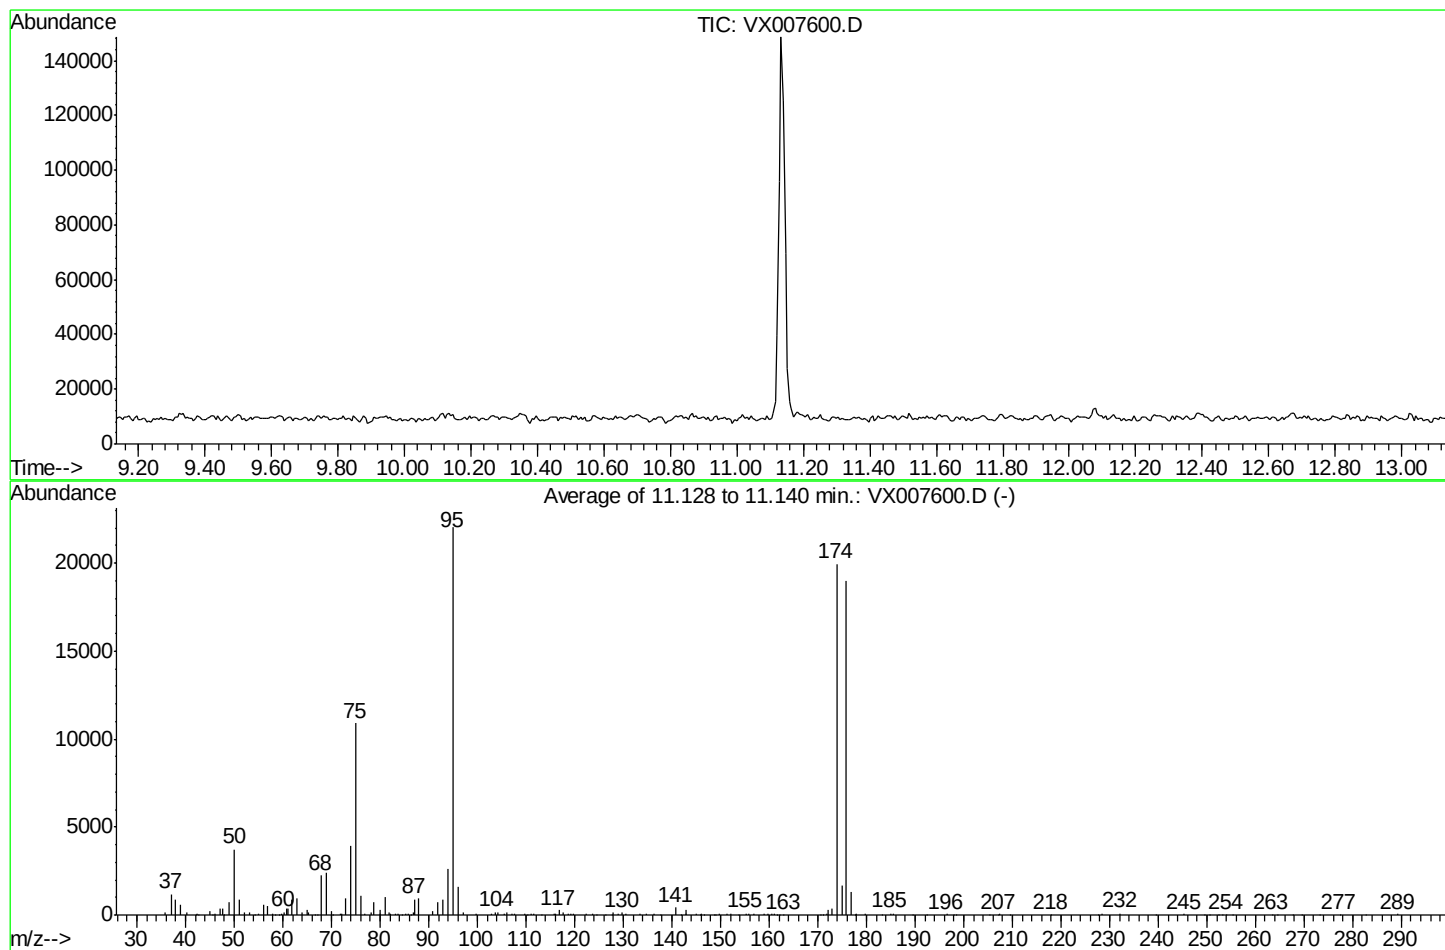

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	3749	PASS
75	95	30	60	49.4	10894	PASS
95	95	100	100	100.0	22040	PASS
96	95	5	9	7.2	1589	PASS
173	174	0.00	2	1.7	336	PASS
174	95	50	100	90.6	19968	PASS
175	174	5	9	8.5	1705	PASS
176	174	95	101	95.1	18999	PASS
177	176	5	9	7.0	1338	PASS