

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX021924\  
 Data File : VX040341.D  
 Acq On : 19 Feb 2024 19:16  
 Operator : JC/MD  
 Sample : P1507-24  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RE131D2-20240214

Quant Time: Feb 20 01:21:09 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X020924W.M  
 Quant Title : SW846 8260  
 QLast Update : Mon Feb 12 00:21:14 2024  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc      | Units      | Dev(Min) |
|-------------------------------|--------|-------|----------|-----------|------------|----------|
| -----                         |        |       |          |           |            |          |
| Internal Standards            |        |       |          |           |            |          |
| 1) Pentafluorobenzene         | 5.550  | 168   | 73339    | 50.000    | ug/l       | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.763  | 114   | 132390   | 50.000    | ug/l       | 0.00     |
| 63) Chlorobenzene-d5          | 10.055 | 117   | 126404   | 50.000    | ug/l       | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024 | 152   | 63423    | 50.000    | ug/l       | 0.00     |
| System Monitoring Compounds   |        |       |          |           |            |          |
| 33) 1,2-Dichloroethane-d4     | 5.952  | 65    | 57320    | 52.536    | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 78 - 117 | Recovery  | = 105.080% |          |
| 35) Dibromofluoromethane      | 5.385  | 113   | 43570    | 47.126    | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 75 - 124 | Recovery  | = 94.260%  |          |
| 50) Toluene-d8                | 8.647  | 98    | 160343   | 46.363    | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 92 - 112 | Recovery  | = 92.720%  |          |
| 62) 4-Bromofluorobenzene      | 11.079 | 95    | 60939    | 43.204    | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 83 - 123 | Recovery  | = 86.400%  |          |
| Target Compounds              |        |       |          |           |            |          |
|                               |        |       |          |           | Qvalue     |          |
| 2) Dichlorodifluoromethane    | 1.166  | 85    | 340      | 0.410     | ug/l       | 74       |
| 7) Trichlorofluoromethane     | 1.886  | 101   | 334      | 0.230     | ug/l #     | 80       |
| 9) 1,1,2-Trichlorotrifluo...  | 2.331  | 101   | 171608   | 220.669   | ug/l       | 99       |
| 12) 1,1-Dichloroethene        | 2.325  | 96    | 2341     | 3.126     | ug/l       | 92       |
| 16) Acetone                   | 2.380  | 43    | 846      | 1.888     | ug/l #     | 88       |
| 18) Methyl Acetate            | 2.526  | 43    | 293      | 0.244     | ug/l #     | 53       |
| 20) Methylene Chloride        | 2.788  | 84    | 722      | Below Cal | #          | 65       |
| 22) Diisopropyl ether         | 3.763  | 45    | 1340     | 0.508     | ug/l #     | 61       |
| 24) 1,1-Dichloroethane        | 3.611  | 63    | 774      | 0.504     | ug/l #     | 83       |
| 27) cis-1,2-Dichloroethene    | 4.489  | 96    | 5387     | 5.537     | ug/l       | 83       |
| 30) Chloroform                | 5.092  | 83    | 730      | 0.440     | ug/l #     | 75       |
| 31) Cyclohexane               | 5.556  | 56    | 1974     | 1.517     | ug/l #     | 12       |
| 36) 1,1-Dichloropropene       | 5.556  | 75    | 6734     | 5.199     | ug/l #     | 50       |
| 38) Carbon Tetrachloride      | 5.550  | 117   | 7957     | 6.462     | ug/l #     | 15       |
| 39) Methylcyclohexane         | 7.123  | 83    | 2495     | 1.658     | ug/l #     | 1        |
| 42) 1,2-Dichloroethane        | 6.086  | 62    | 476      | 0.336     | ug/l #     | 77       |
| 44) Trichloroethene           | 7.123  | 130   | 185947   | 186.128   | ug/l       | 95       |
| 49) 1,4-Dioxane               | 7.665  | 88    | 631      | 25.198    | ug/l #     | 92       |
| 51) 4-Methyl-2-Pentanone      | 8.647  | 43    | 846      | 0.551     | ug/l #     | 1        |
| 52) Toluene                   | 8.714  | 92    | 863      | 0.364     | ug/l       | 95       |
| 60) Dibromochloromethane      | 9.275  | 129   | 20080    | 19.479    | ug/l #     | 11       |
| 64) Tetrachloroethene         | 9.275  | 164   | 19523    | 22.040    | ug/l       | 96       |
| 76) 1,2,3-Trichloropropane    | 11.079 | 75    | 34237    | 26.657    | ug/l #     | 39       |
| 81) trans-1,4-Dichloro-2-b... | 11.079 | 75    | 34237    | 73.092    | ug/l #     | 5        |
| -----                         |        |       |          |           |            |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX021924\  
Data File : VX040341.D  
Acq On : 19 Feb 2024 19:16  
Operator : JC/MD  
Sample : P1507-24  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214

Quant Time: Feb 20 01:21:09 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X020924W.M  
Quant Title : SW846 8260  
QLast Update : Mon Feb 12 00:21:14 2024  
Response via : Initial Calibration




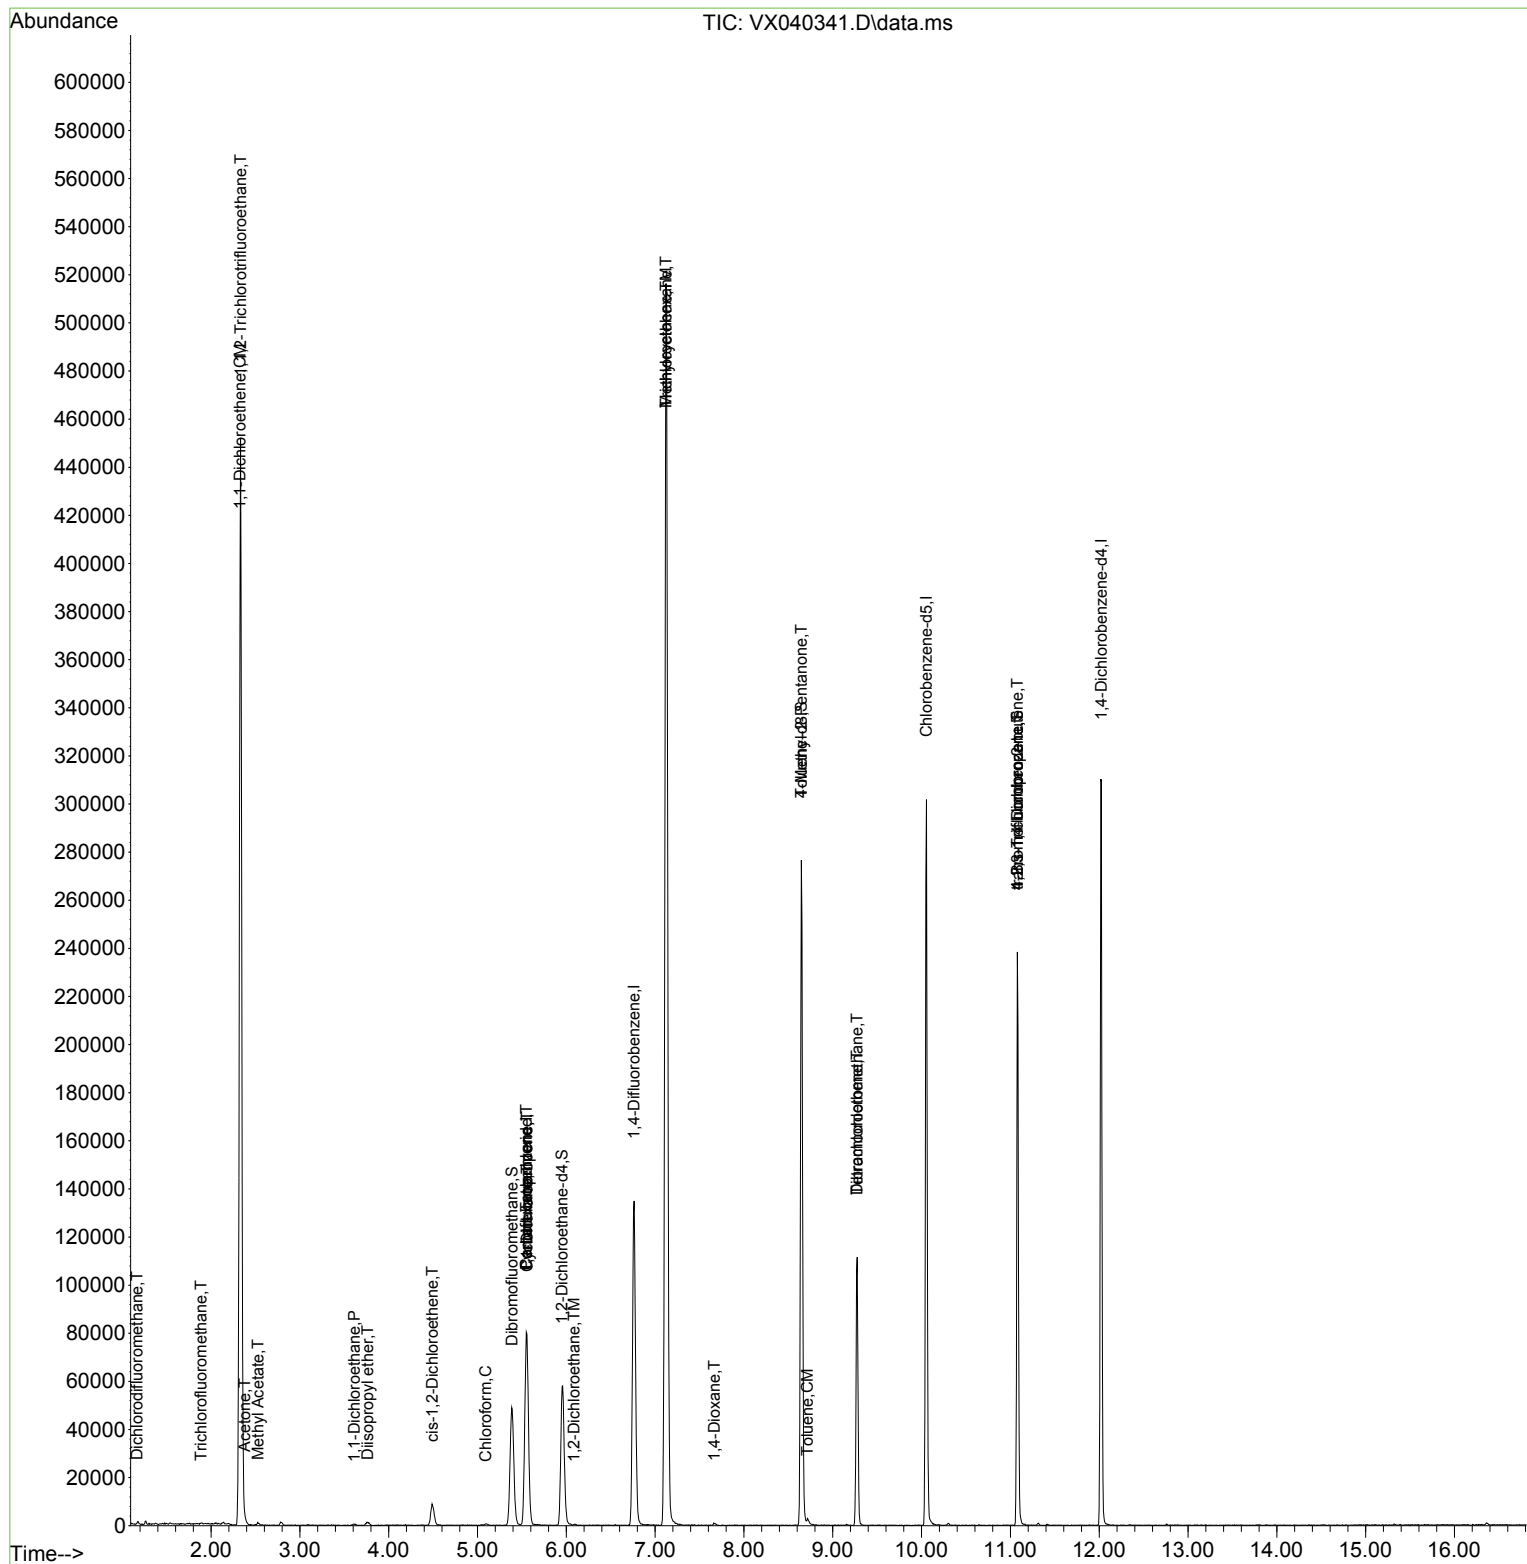




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 71  
Delta R.T. -0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214


Tgt Ion:168 Resp: 73339  
Ion Ratio Lower Upper  
168 100  
99 61.6 56.6 85.0



#2  
Dichlorodifluoromethane  
Concen: 0.410 ug/l  
RT: 1.166 min Scan# 13  
Delta R.T. 0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Tgt Ion: 85 Resp: 340  
Ion Ratio Lower Upper  
85 100  
87 48.0 16.7 50.1









#7  
 Trichlorofluoromethane  
 Concen: 0.230 ug/l  
 RT: 1.886 min Scan# 11  
 Delta R.T. 0.000 min  
 Lab File: VX040341.D  
 Acq: 19 Feb 2024 19:16




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RE131D2-20240214


Tgt Ion:101 Resp: 334  
 Ion Ratio Lower Upper  
 101 100  
 103 48.4 51.4 77.2#



#9  
 1,1,2-Trichlorotrifluoroethane  
 Concen: 220.669 ug/l  
 RT: 2.331 min Scan# 204  
 Delta R.T. 0.006 min  
 Lab File: VX040341.D  
 Acq: 19 Feb 2024 19:16

Tgt Ion:101 Resp: 171608  
 Ion Ratio Lower Upper  
 101 100  
 85 47.5 37.0 55.6  
 151 73.1 58.6 87.8



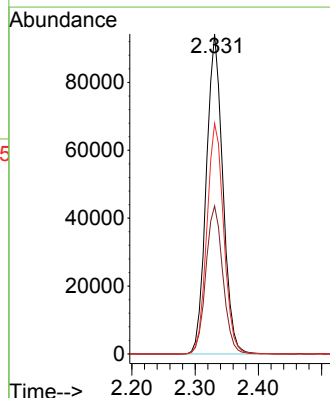



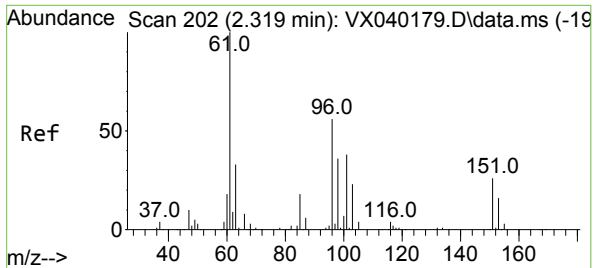

#12  
1,1-Dichloroethene  
Concen: 3.126 ug/l  
RT: 2.325 min Scan# 202  
Delta R.T. 0.006 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214


Tgt Ion: 96 Resp: 2341  
Ion Ratio Lower Upper  
96 100  
61 166.7 144.6 216.8  
98 61.6 50.4 75.6

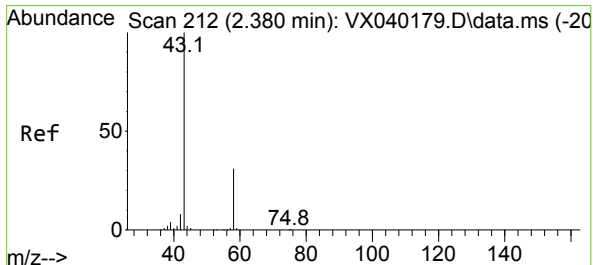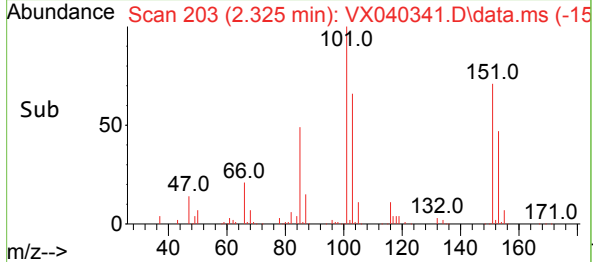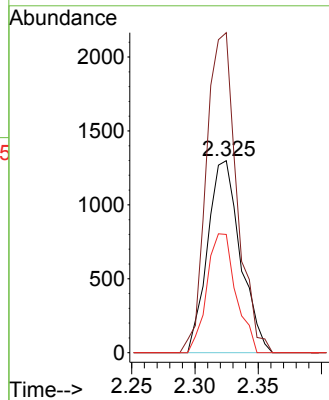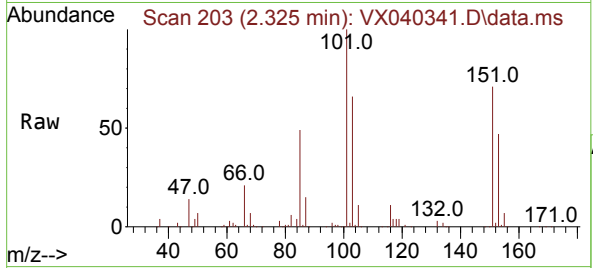

#16  
Acetone  
Concen: 1.888 ug/l  
RT: 2.380 min Scan# 212  
Delta R.T. 0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Tgt Ion: 43 Resp: 846  
Ion Ratio Lower Upper  
43 100  
58 21.4 21.9 32.9#


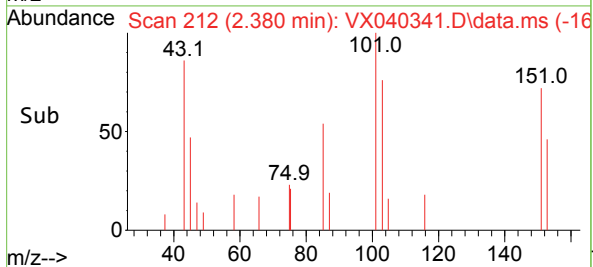
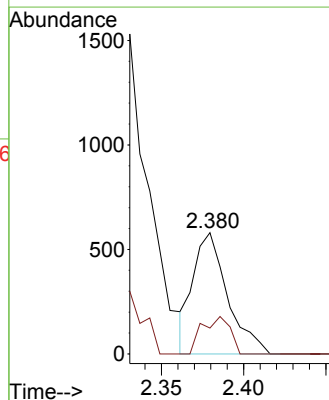
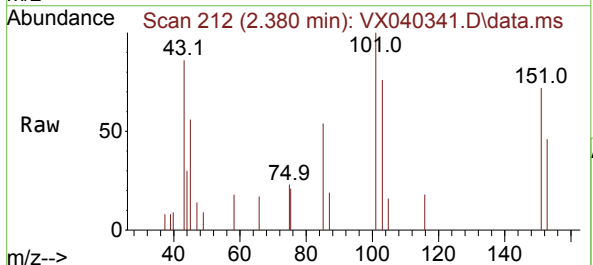




#18  
Methyl Acetate  
Concen: 0.244 ug/l  
RT: 2.526 min Scan# 21  
Delta R.T. -0.177 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214


Tgt Ion: 43 Resp: 293  
Ion Ratio Lower Upper  
43 100  
74 0.0 17.8 26.8#



#20  
Methylene Chloride  
Concen: Below Cal  
RT: 2.788 min Scan# 279  
Delta R.T. -0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16


Tgt Ion: 84 Resp: 722  
Ion Ratio Lower Upper  
84 100  
49 71.2 103.6 155.4#  
51 40.0 33.8 50.6  
86 44.0 49.4 74.0#

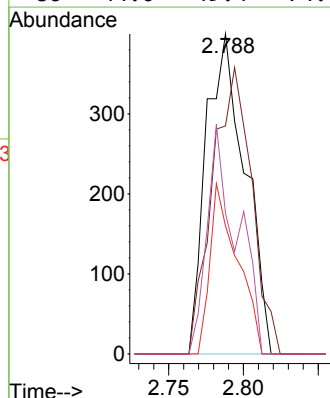






#22  
Diisopropyl ether  
Concen: 0.508 ug/l  
RT: 3.763 min Scan# 41  
Delta R.T. 0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214







|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 45    | Resp: | 1340   |
| Ion      | Ratio | Lower | Upper  |
| 45       | 100   |       |        |
| 43       | 40.6  | 69.7  | 104.5# |
| 87       | 18.6  | 20.8  | 31.2#  |
| 59       | 10.2  | 9.0   | 13.4   |

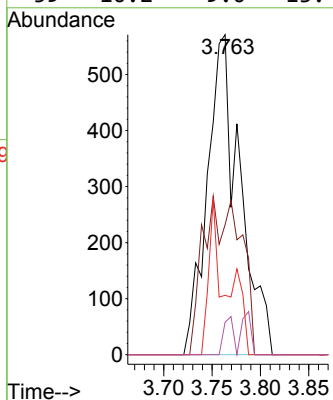

#24  
1,1-Dichloroethane  
Concen: 0.504 ug/l  
RT: 3.611 min Scan# 414  
Delta R.T. 0.006 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 63    | Resp: | 774   |
| Ion      | Ratio | Lower | Upper |
| 63       | 100   |       |       |
| 98       | 0.0   | 3.3   | 9.8#  |
| 100      | 0.0   | 2.1   | 6.5#  |

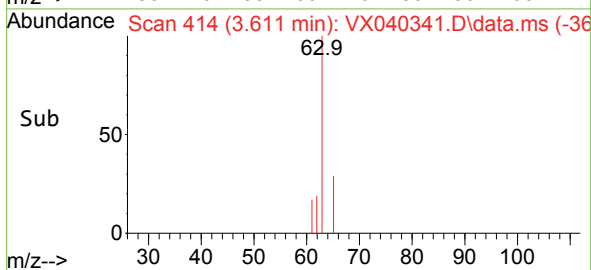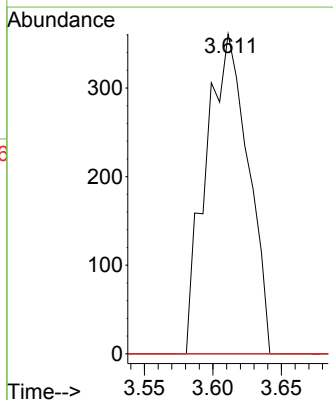



#27

cis-1,2-Dichloroethene

Concen: 5.537 ug/l

RT: 4.489 min Scan# 51

Delta R.T. -0.000 min

Lab File: VX040341.D

Acq: 19 Feb 2024 19:16

Instrument :

MSVOA\_X

ClientSampleId :

RE131D2-20240214





Tgt Ion: 96 Resp: 5387

Ion Ratio Lower Upper

96 100

61 128.0 0.0 312.2

98 68.6 0.0 129.0

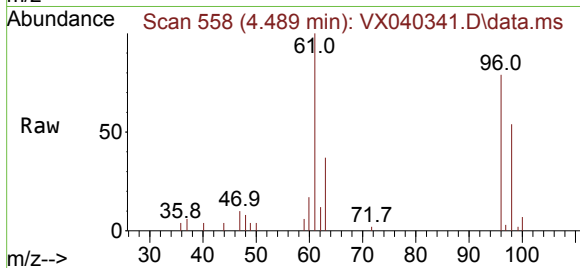

#30

Chloroform

Concen: 0.440 ug/l

RT: 5.092 min Scan# 657

Delta R.T. -0.006 min

Lab File: VX040341.D




Acq: 19 Feb 2024 19:16

Tgt Ion: 83 Resp: 730


Ion Ratio Lower Upper

83 100

85 43.4 50.3 75.5#

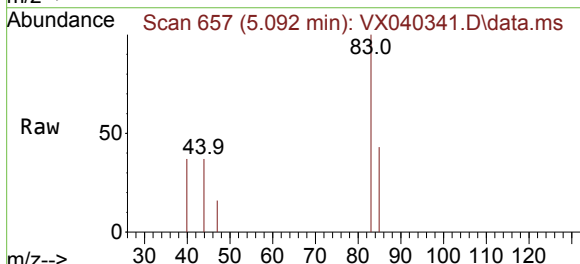









#31  
Cyclohexane  
Concen: 1.517 ug/l  
RT: 5.556 min Scan# 719  
Delta R.T. 0.085 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214







Tgt Ion: 56 Resp: 1974  
Ion Ratio Lower Upper  
56 100  
69 140.7 23.4 35.2#  
84 123.3 65.9 98.9#



#33  
1,2-Dichloroethane-d4  
Concen: 52.536 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. -0.006 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Tgt Ion: 65 Resp: 57320  
Ion Ratio Lower Upper  
65 100  
67 53.1 0.0 100.2


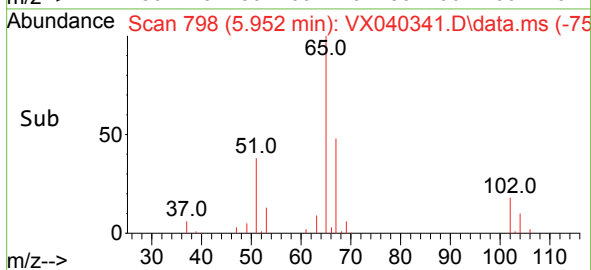






#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.763 min Scan# 91  
Delta R.T. -0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214


Tgt Ion:114 Resp: 132390  
Ion Ratio Lower Upper  
114 100  
63 21.7 0.0 45.0  
88 16.3 0.0 36.6



#35  
Dibromofluoromethane  
Concen: 47.126 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. 0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Tgt Ion:113 Resp: 43570  
Ion Ratio Lower Upper  
113 100  
111 100.8 82.9 124.3  
192 17.2 13.3 19.9

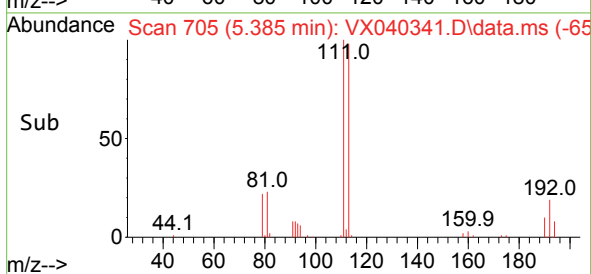



#36

1,1-Dichloropropene

Concen: 5.199 ug/l

RT: 5.556 min Scan# 71

Delta R.T. -0.140 min

Lab File: VX040341.D

Acq: 19 Feb 2024 19:16

Instrument :

MSVOA\_X

ClientSampleId :

RE131D2-20240214





Tgt Ion: 75 Resp: 6734

Ion Ratio Lower Upper

75 100

110 8.1 17.0 50.9#

77 0.0 24.7 37.1#

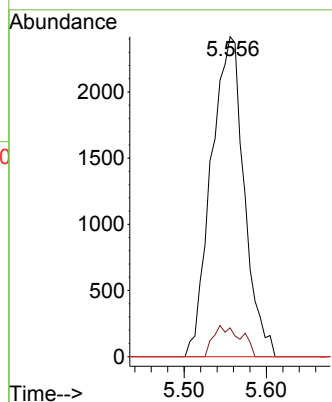

#38

Carbon Tetrachloride

Concen: 6.462 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.122 min

Lab File: VX040341.D

Acq: 19 Feb 2024 19:16




Tgt Ion: 117 Resp: 7957


Ion Ratio Lower Upper

117 100

119 4.4 78.2 117.2#

121 0.0 24.4 36.6#


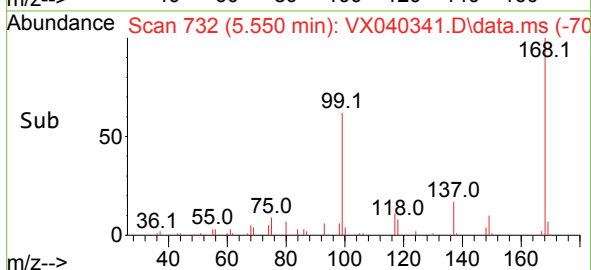






#39  
Methylcyclohexane  
Concen: 1.658 ug/l  
RT: 7.123 min Scan# 91  
Delta R.T. -0.256 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214


Tgt Ion: 83 Resp: 2495  
Ion Ratio Lower Upper  
83 100  
55 0.0 64.6 97.0#  
98 202.3 36.7 55.1#



#42  
1,2-Dichloroethane  
Concen: 0.336 ug/l  
RT: 6.086 min Scan# 820  
Delta R.T. 0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Tgt Ion: 62 Resp: 476  
Ion Ratio Lower Upper  
62 100  
98 0.0 0.0 16.0









#44  
Trichloroethene  
Concen: 186.128 ug/l  
RT: 7.123 min Scan# 990  
Delta R.T. -0.006 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214


Tgt Ion:130 Resp: 185947  
Ion Ratio Lower Upper  
130 100  
95 106.9 0.0 204.4

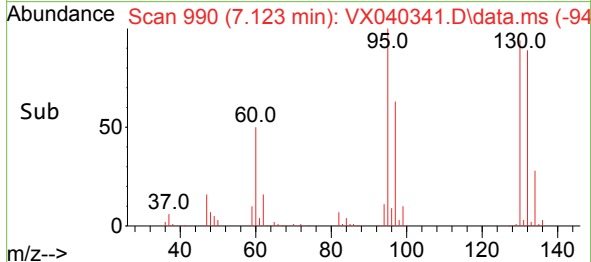

#49  
1,4-Dioxane  
Concen: 25.198 ug/l  
RT: 7.665 min Scan# 1079  
Delta R.T. 0.006 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Tgt Ion: 88 Resp: 631  
Ion Ratio Lower Upper  
88 100  
43 39.5 0.0 0.0#  
58 82.1 60.1 90.1


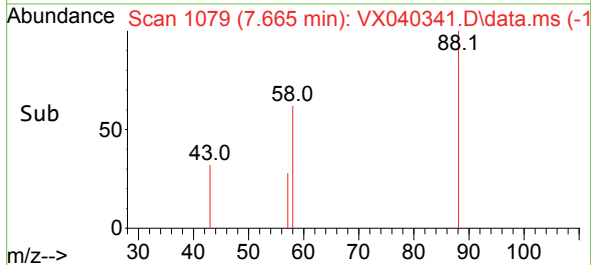






#50  
Toluene-d8  
Concen: 46.363 ug/l  
RT: 8.647 min Scan# 11  
Delta R.T. -0.006 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214


Tgt Ion: 98 Resp: 160343  
Ion Ratio Lower Upper  
98 100  
100 63.9 53.1 79.7

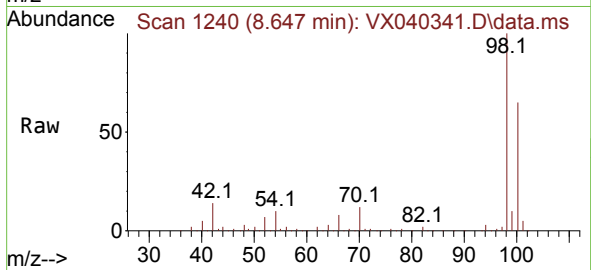

#51  
4-Methyl-2-Pentanone  
Concen: 0.551 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. 0.073 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Tgt Ion: 43 Resp: 846  
Ion Ratio Lower Upper  
43 100  
58 170.7 30.4 45.6#





#52

Toluene

Concen: 0.364 ug/l

RT: 8.714 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX040341.D

Acq: 19 Feb 2024 19:16

Instrument :

MSVOA\_X

ClientSampleId :





RE131D2-20240214

Tgt Ion: 92 Resp: 863

Ion Ratio Lower Upper

92 100

91 174.0 134.2 201.2

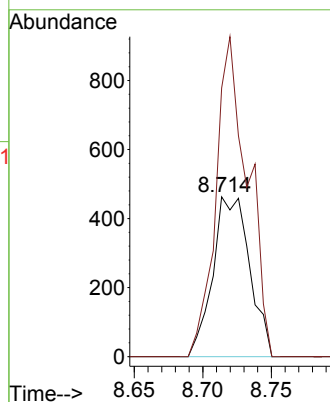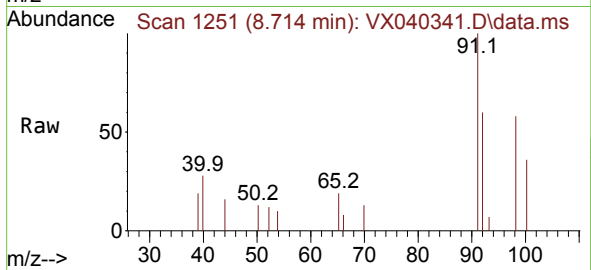

#60

Dibromochloromethane

Concen: 19.479 ug/l

RT: 9.275 min Scan# 1343

Delta R.T. -0.244 min

Lab File: VX040341.D




Acq: 19 Feb 2024 19:16


Tgt Ion: 129 Resp: 20080

Ion Ratio Lower Upper

129 100

127 0.0 38.8 116.4#


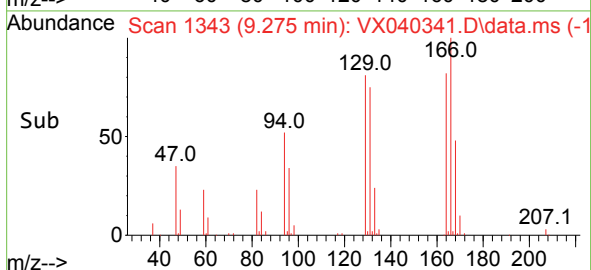






#62  
4-Bromofluorobenzene  
Concen: 43.204 ug/l  
RT: 11.079 min Scan# 1  
Delta R.T. 0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214

Tgt Ion: 95 Resp: 60939  
Ion Ratio Lower Upper  
95 100  
174 75.5 0.0 135.6  
176 71.7 0.0 131.0

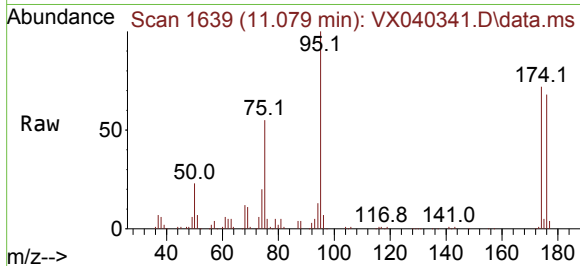


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Tgt Ion: 117 Resp: 126404  
Ion Ratio Lower Upper  
117 100  
82 57.3 46.2 69.4  
119 32.0 25.5 38.3

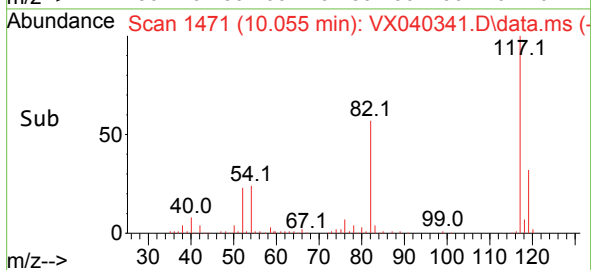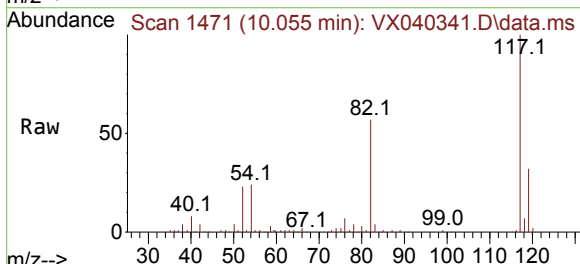









#64  
Tetrachloroethene  
Concen: 22.040 ug/l  
RT: 9.275 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214


|             |       |             |
|-------------|-------|-------------|
| Tgt Ion:164 | Resp: | 19523       |
| Ion         | Ratio | Lower Upper |
| 164         | 100   |             |
| 166         | 121.5 | 102.7 154.1 |
| 129         | 98.5  | 80.4 120.6  |
| 131         | 91.0  | 76.5 114.7  |

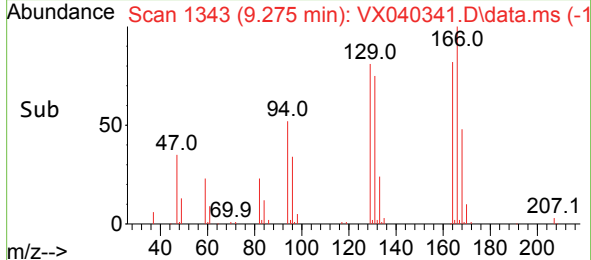

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 1794  
Delta R.T. -0.000 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

|             |       |             |
|-------------|-------|-------------|
| Tgt Ion:152 | Resp: | 63423       |
| Ion         | Ratio | Lower Upper |
| 152         | 100   |             |
| 115         | 61.0  | 43.3 129.9  |
| 150         | 156.3 | 0.0 345.0   |




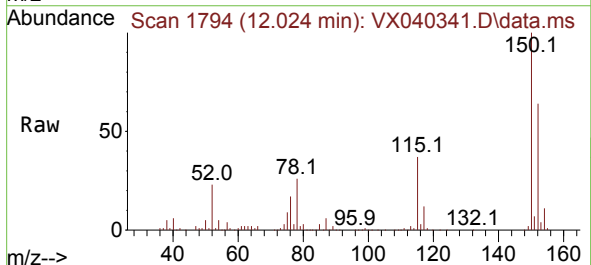




#76  
1,2,3-Trichloropropane  
Concen: 26.657 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.159 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE131D2-20240214

Tgt Ion: 75 Resp: 34237  
Ion Ratio Lower Upper  
75 100  
77 1.3 19.1 57.5#

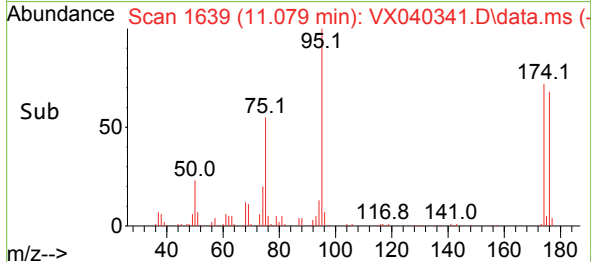

#81  
trans-1,4-Dichloro-2-butene  
Concen: 73.092 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.061 min  
Lab File: VX040341.D  
Acq: 19 Feb 2024 19:16

Tgt Ion: 75 Resp: 34237  
Ion Ratio Lower Upper  
75 100  
53 0.0 90.5 135.7#  
89 0.0 36.9 55.3#

