



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021924\
Data File : VX040317.D
Acq On : 19 Feb 2024 09:13
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
Title : SW846 8260
Last Update : Mon Feb 12 00:21:14 2024

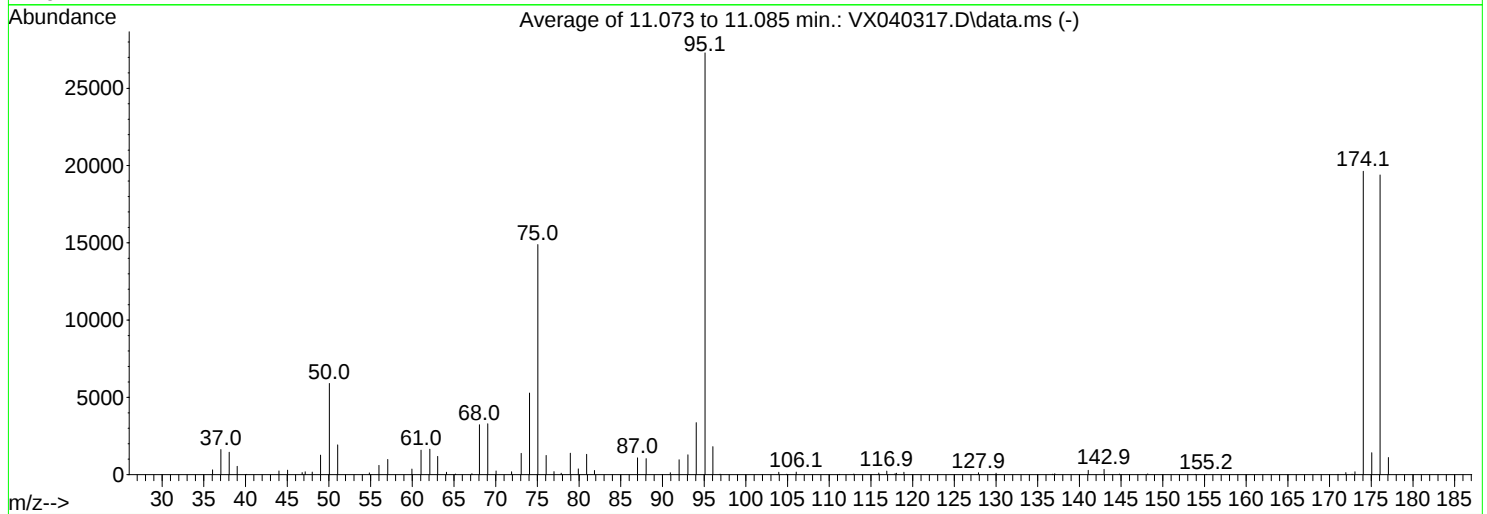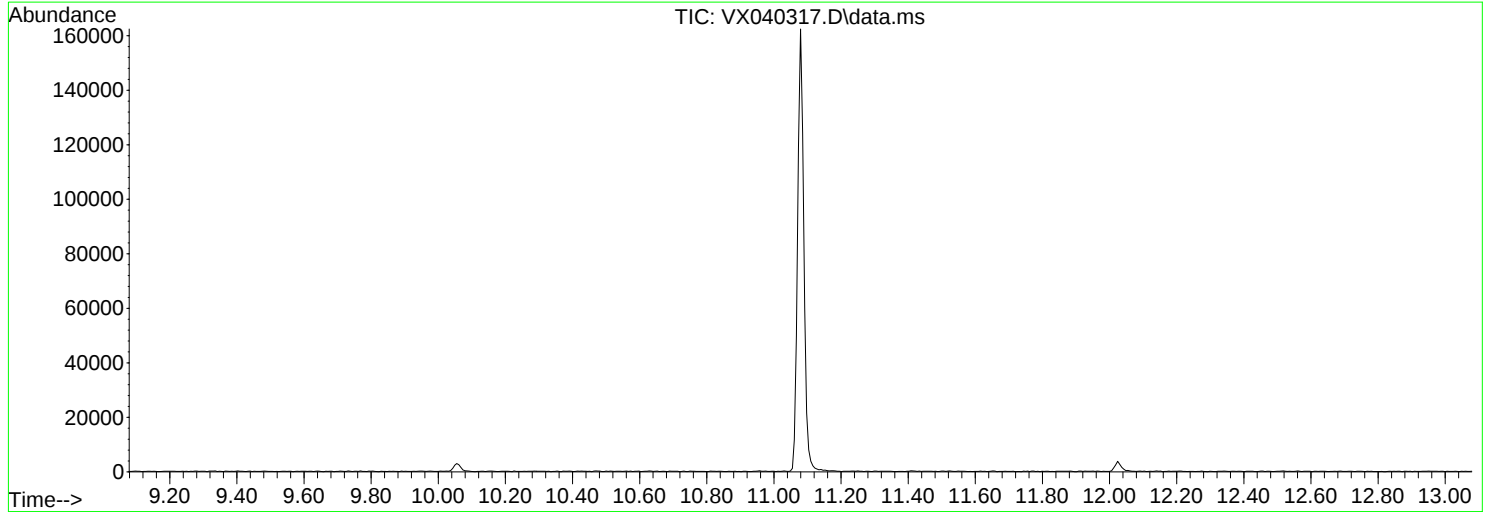

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.6	5900	PASS
75	95	30	60	54.6	14893	PASS
95	95	100	100	100.0	27296	PASS
96	95	5	9	6.6	1812	PASS
173	174	0.00	2	1.0	190	PASS
174	95	50	100	71.9	19631	PASS
175	174	5	9	7.2	1419	PASS
176	174	95	101	98.8	19393	PASS
177	176	5	9	5.7	1111	PASS