

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022023\
Data File : VX034183.D
Acq On : 20 Feb 2023 13:27
Operator : JC/MD
Sample : 01611-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-2-17

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Title : SW846 8260

Signal : TIC: VX034183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV	50355	80789	4.28%	0.831%
2	2.373	205	211	220	rVB	17853	32321	1.71%	0.332%
3	2.788	272	279	288	rBV	10260	20983	1.11%	0.216%
4	5.385	693	705	722	rBV	210769	617063	32.68%	6.344%
5	5.550	722	732	753	rVB	345039	1010341	53.52%	10.387%
6	5.958	787	799	817	rBV2	240465	629922	33.37%	6.476%
7	6.763	919	931	944	rBV	559508	1358070	71.93%	13.962%
8	8.647	1233	1240	1259	rBV	1173559	1887915	100.00%	19.409%
9	10.055	1465	1471	1487	rBV	1107763	1559255	82.59%	16.030%
10	11.079	1631	1639	1650	rBV	868584	1162710	61.59%	11.953%
11	12.024	1788	1794	1807	rBV	1053268	1367661	72.44%	14.060%




Sum of corrected areas: 9727030

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022023\
Data File : VX034183.D
Acq On : 20 Feb 2023 13:27
Operator : JC/MD
Sample : 01611-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-2-17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

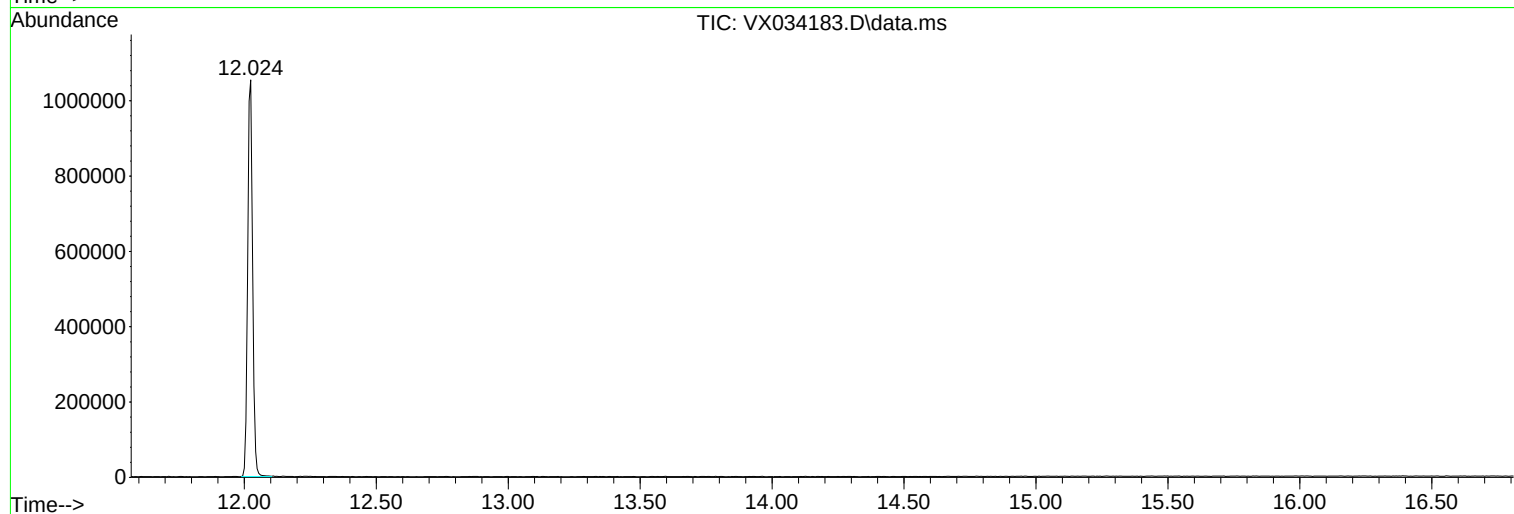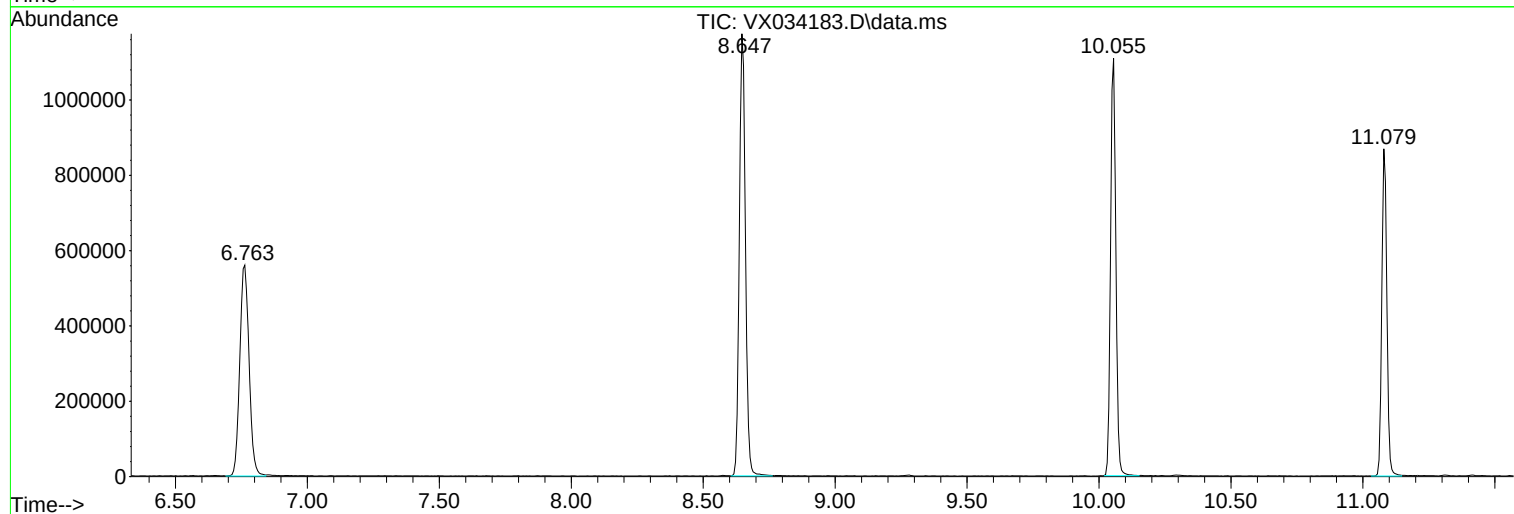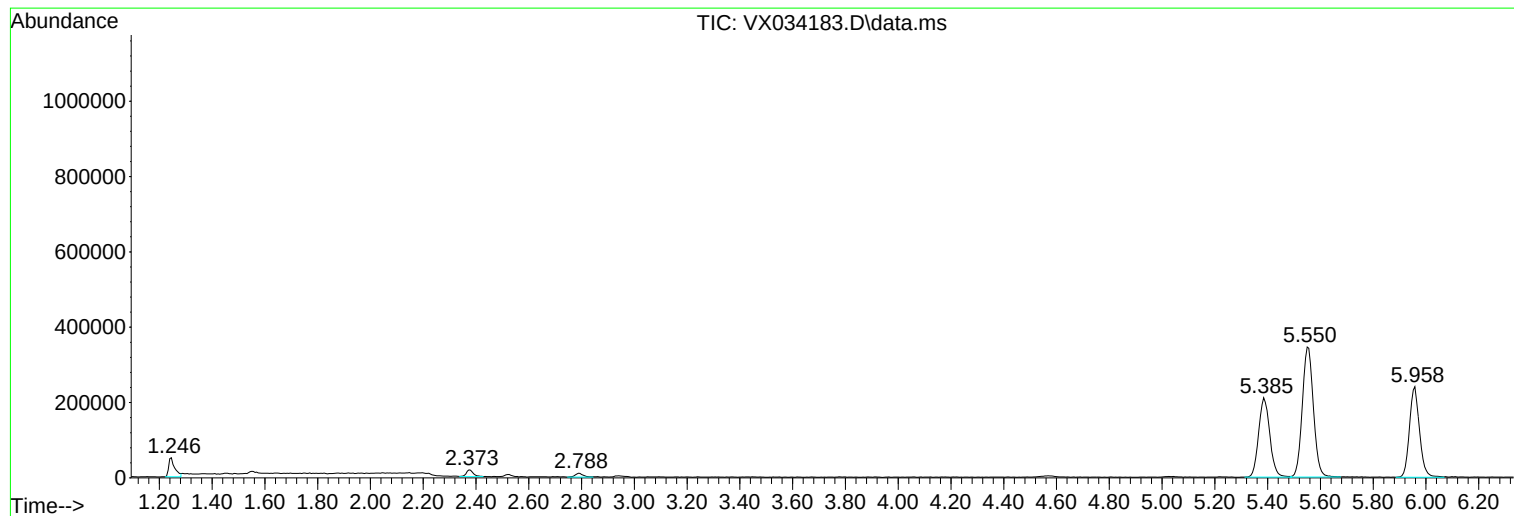

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022023\
Data File : VX034183.D
Acq On : 20 Feb 2023 13:27
Operator : JC/MD
Sample : 01611-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-2-17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022023\
Data File : VX034183.D
Acq On : 20 Feb 2023 13:27
Operator : JC/MD
Sample : 01611-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-2023-2-17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------