

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022023\
 Data File : VX034187.D
 Acq On : 20 Feb 2023 15:00
 Operator : JC/MD
 Sample : 01593-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M

Title : SW846 8260

Signal : TIC: VX034187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	33	rBV	17747	35582	1.94%	0.372%
2	2.288	193	197	206	rVB	29002	48963	2.67%	0.512%
3	2.374	206	211	220	rVB	15195	27943	1.52%	0.292%
4	4.239	509	517	529	rBV4	7135	18685	1.02%	0.195%
5	5.099	648	658	668	rBV3	6158	18461	1.01%	0.193%
6	5.385	694	705	722	rBV	204581	605957	33.06%	6.339%
7	5.550	722	732	750	rVB	343360	978112	53.36%	10.232%
8	5.952	788	798	811	rBV2	224060	606766	33.10%	6.347%
9	6.763	920	931	948	rBV	550686	1314515	71.72%	13.751%
10	8.647	1233	1240	1258	rBV	1161588	1832921	100.00%	19.173%
11	9.519	1378	1383	1394	rBV	57553	88980	4.85%	0.931%
12	10.055	1465	1471	1489	rBV	1101353	1523179	83.10%	15.933%
13	11.079	1634	1639	1655	rBV	866418	1127028	61.49%	11.789%
14	12.018	1788	1793	1807	rBV	1016479	1332642	72.71%	13.940%




Sum of corrected areas: 9559734

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022023\
Data File : VX034187.D
Acq On : 20 Feb 2023 15:00
Operator : JC/MD
Sample : 01593-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

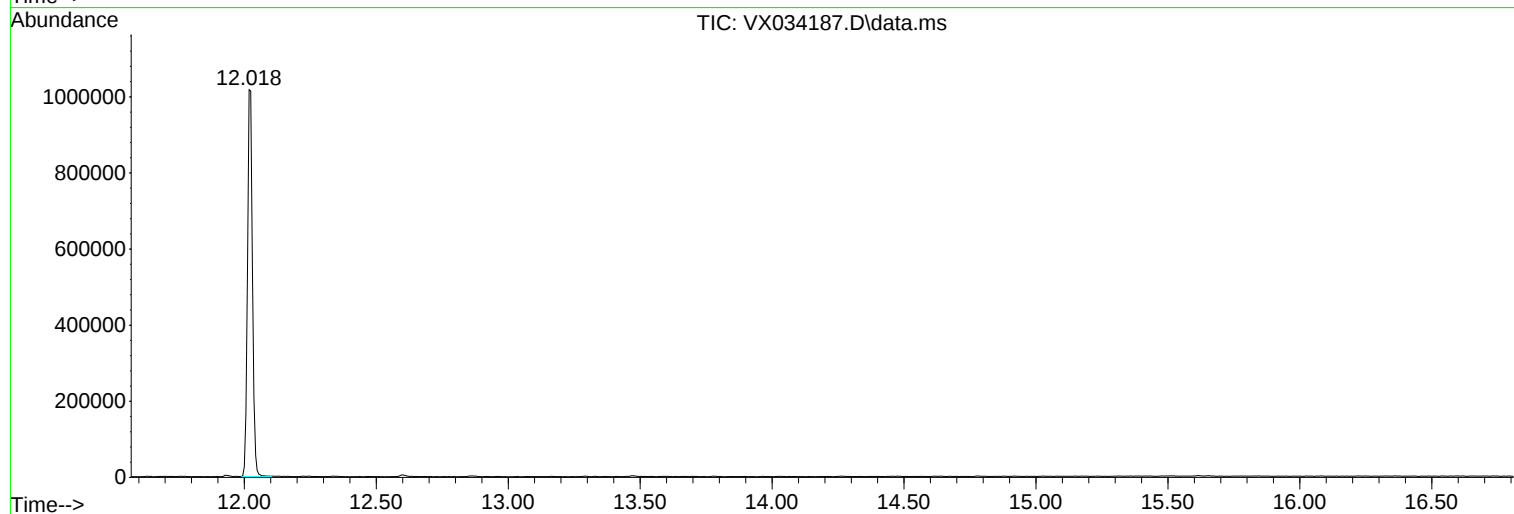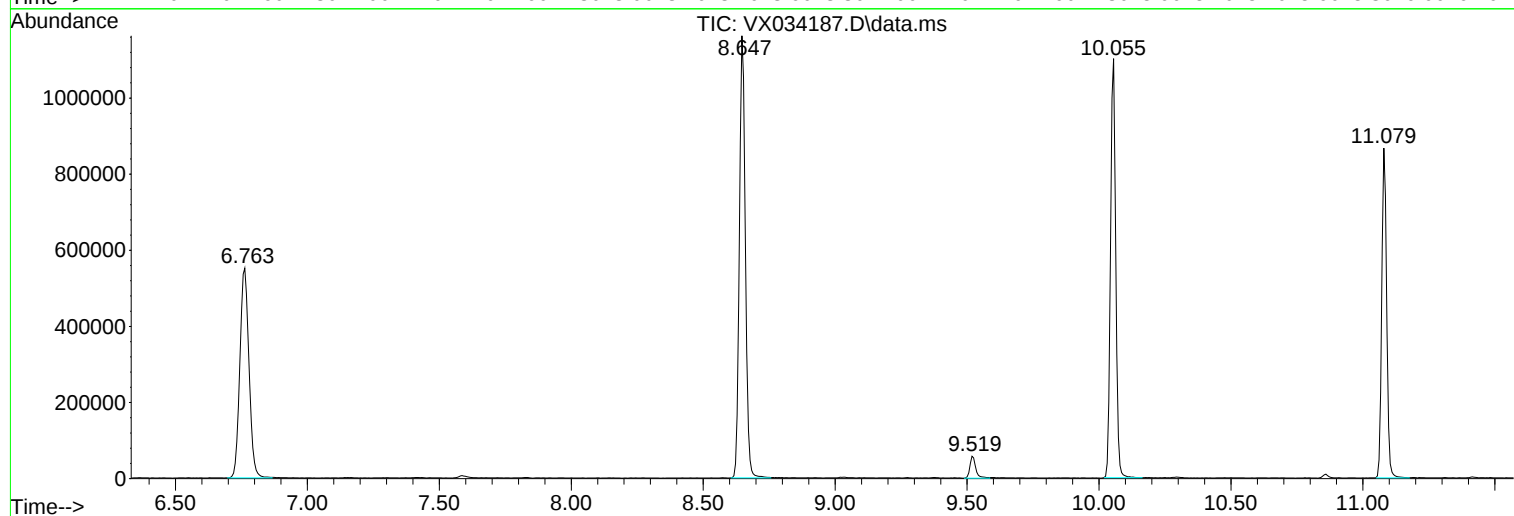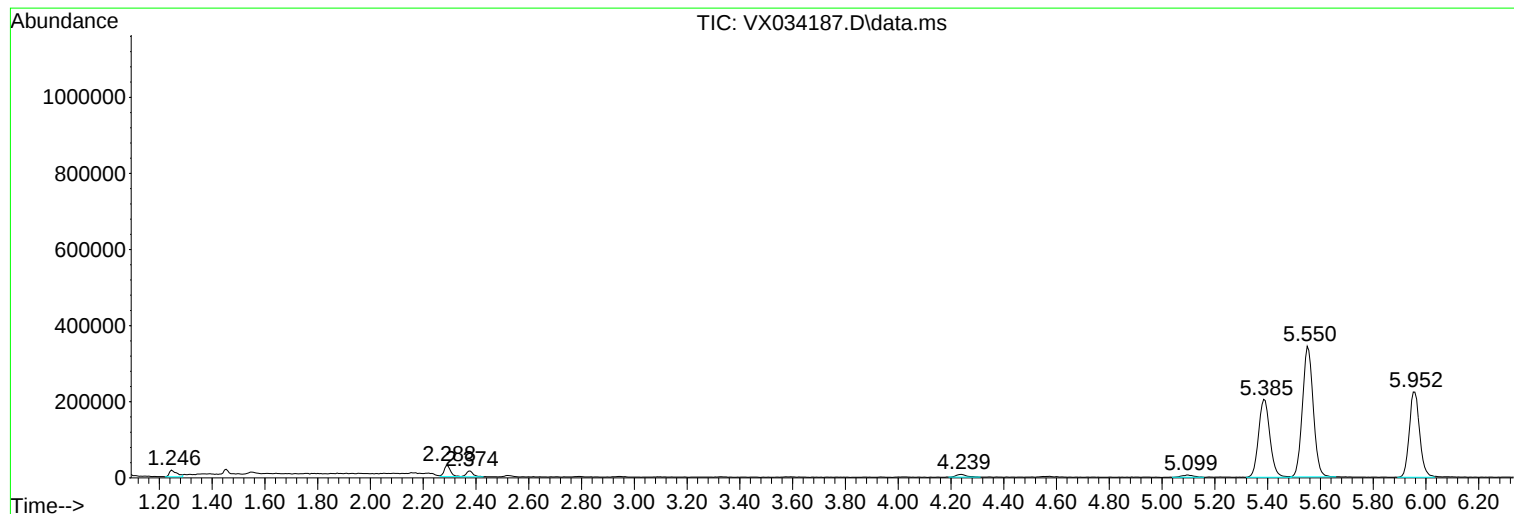

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022023\
Data File : VX034187.D
Acq On : 20 Feb 2023 15:00
Operator : JC/MD
Sample : 01593-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022023\
Data File : VX034187.D
Acq On : 20 Feb 2023 15:00
Operator : JC/MD
Sample : 01593-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------