

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022123\
 Data File : VX034209.D
 Acq On : 21 Feb 2023 15:07
 Operator : JC/MD
 Sample : 01627-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2023

Quant Time: Feb 22 02:57:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 22 02:40:46 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 02/22/2023
 Supervised By : Mahesh Dadoda 02/22/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	391194	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	622921	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	541197	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	253602	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	183074	34.749	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	69.500%#		
35) Dibromofluoromethane	5.385	113	154630	38.126	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	76.260%		
50) Toluene-d8	8.647	98	573808	39.405	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	78.820%#		
62) 4-Bromofluorobenzene	11.079	95	203198	36.481	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	72.960%#		
Target Compounds					Qvalue	
3) Chloromethane	1.301	50	1082	0.222	ug/l #	88
5) Bromomethane	1.605	94	922	0.524	ug/l #	57
8) Diethyl Ether	2.130	74	541	0.224	ug/l	99
11) Tert butyl alcohol	2.947	59	3187	2.705	ug/l #	89
13) Acrolein	2.233	56	566	1.052	ug/l #	14
15) Acrylonitrile	3.075	53	2117	0.824	ug/l	93
16) Acetone	2.380	43	2874	1.058	ug/l	91
17) Carbon Disulfide	2.514	76	2932	0.241	ug/l	97
20) Methylene Chloride	2.782	84	1719	0.351	ug/l	88
21) trans-1,2-Dichloroethene	3.093	96	937	0.211	ug/l #	82
23) Vinyl Acetate	3.733	43	9834	0.780	ug/l	96
25) 2-Butanone	4.593	43	3672m	0.934	ug/l	
28) Bromochloromethane	4.904	49	950	0.247	ug/l #	96
29) Tetrahydrofuran	5.032	42	2405	1.003	ug/l #	82
37) Ethyl Acetate	4.751	43	2177m	0.325	ug/l	
41) Methacrylonitrile	4.928	41	855m	0.229	ug/l	
42) 1,2-Dichloroethane	6.098	62	1286	0.206	ug/l	99
48) Methyl methacrylate	7.708	41	1450	0.258	ug/l #	62
49) 1,4-Dioxane	7.684	88	329	2.938	ug/l #	91
51) 4-Methyl-2-Pentanone	8.574	43	5337	0.820	ug/l	92
58) 2-Chloroethyl Vinyl ether	8.257	63	4187	1.314	ug/l	91
59) 2-Hexanone	9.439	43	3423	0.690	ug/l	93
68) m/p-Xylenes	10.305	106	2518	0.325	ug/l	94
93) 1,2,4-Trichlorobenzene	13.597	180	1136	0.207	ug/l	85
94) Hexachlorobutadiene	13.731	225	540	0.238	ug/l	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022123\
Data File : VX034209.D
Acq On : 21 Feb 2023 15:07
Operator : JC/MD
Sample : 01627-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023

Quant Time: Feb 22 02:57:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 22 02:40:46 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :John Carlone 02/22/2023
Supervised By :Mahesh Dadoda 02/22/2023

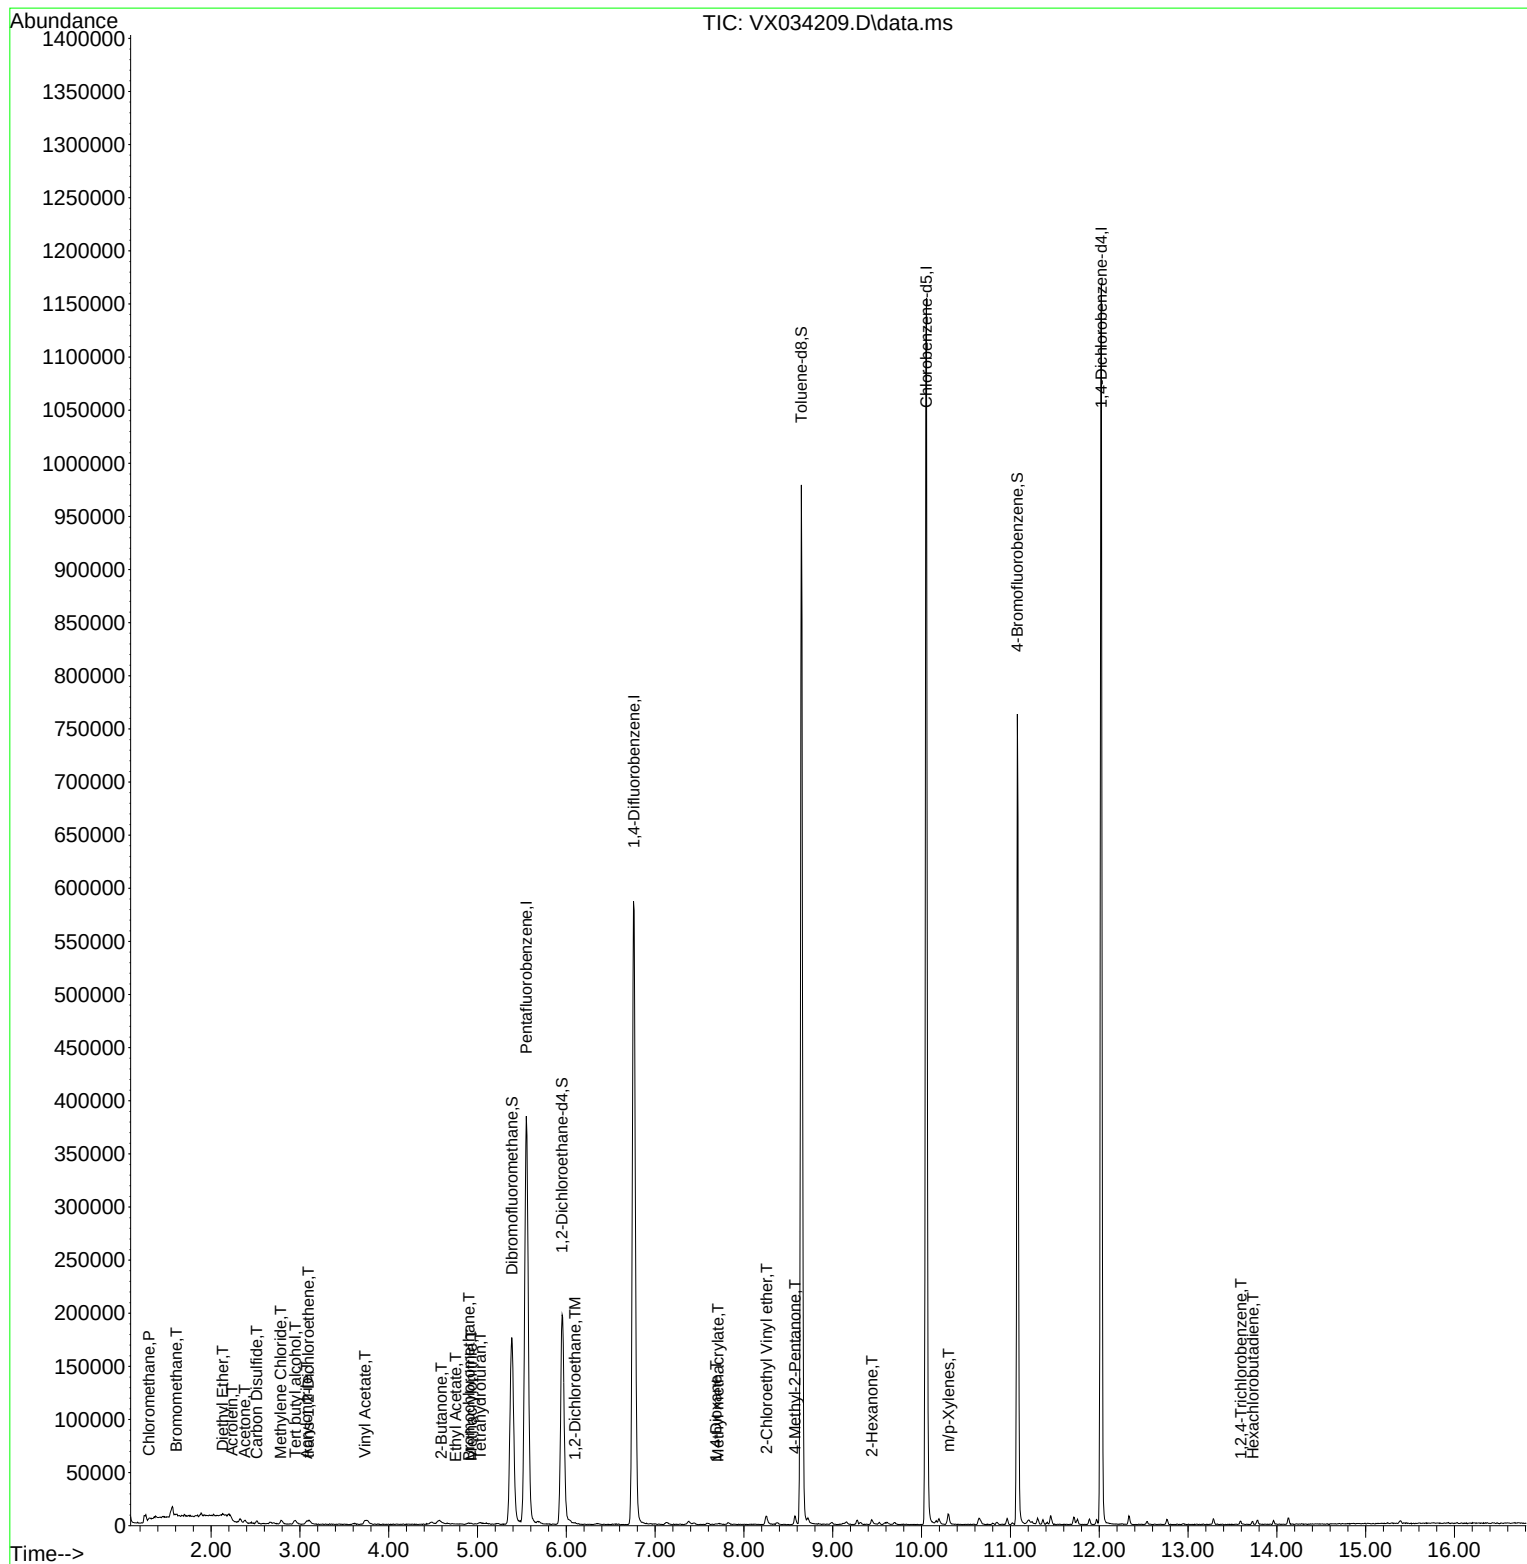



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07




Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023



Tgt Ion:168 Resp: 391194
Ion Ratio Lower Upper
168 100
99 53.7 39.6 59.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 02/22/2023
Supervised By :Mahesh Dadoda 02/22/2023

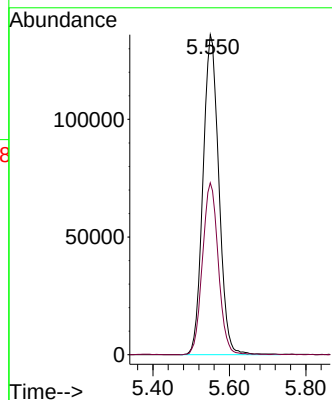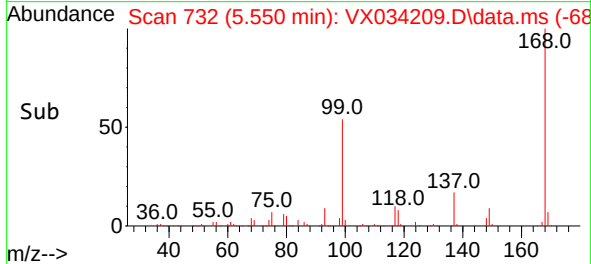

#3
Chloromethane
Concen: 0.222 ug/l
RT: 1.301 min Scan# 35
Delta R.T. 0.006 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07


Tgt Ion: 50 Resp: 1082
Ion Ratio Lower Upper
50 100
52 38.1 25.2 37.8#

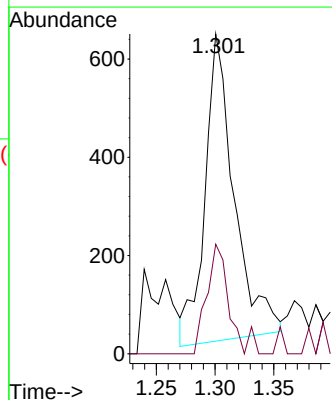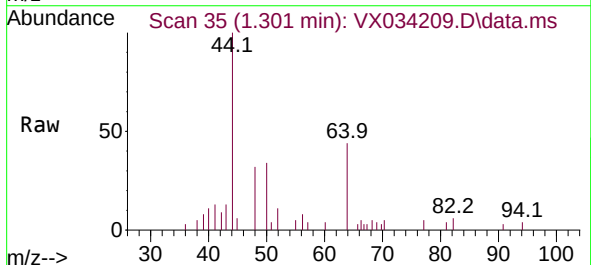

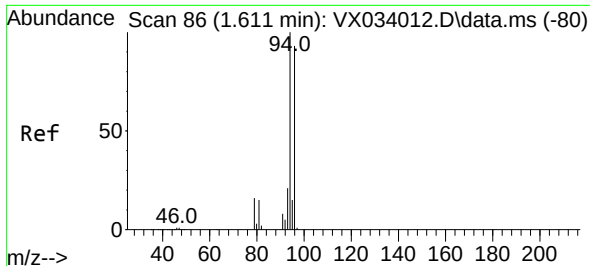

#5
Bromomethane
Concen: 0.524 ug/l
RT: 1.605 min Scan# 86
Delta R.T. 0.006 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07




Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023

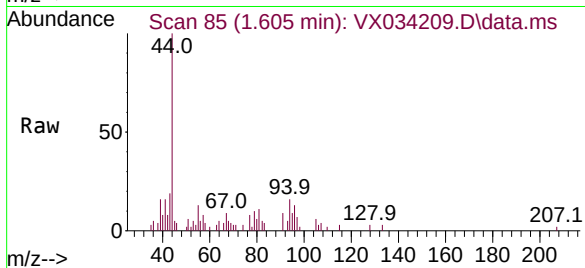

Tgt Ion: 94 Resp: 92
Ion Ratio Lower Upper
94 100
96 52.1 74.3 111.5




Manual Integrations
APPROVED


Reviewed By :John Carlone 02/22/2023
Supervised By :Mahesh Dadoda 02/22/2023

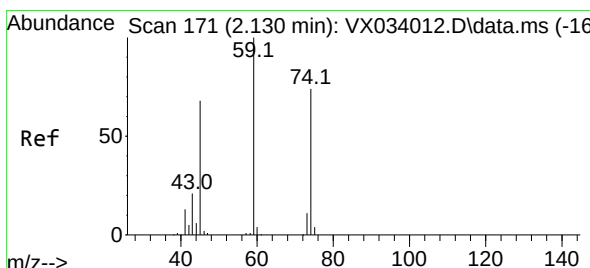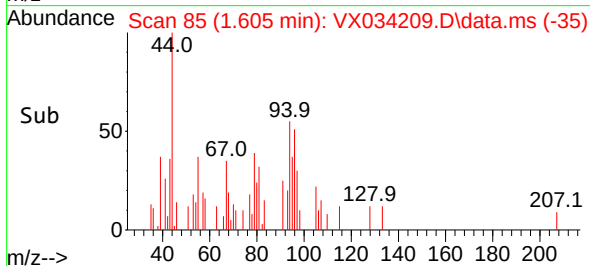

#8
Diethyl Ether
Concen: 0.224 ug/l
RT: 2.130 min Scan# 171
Delta R.T. 0.000 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07

Tgt Ion: 74 Resp: 541
Ion Ratio Lower Upper
74 100
45 103.9 51.5 154.5

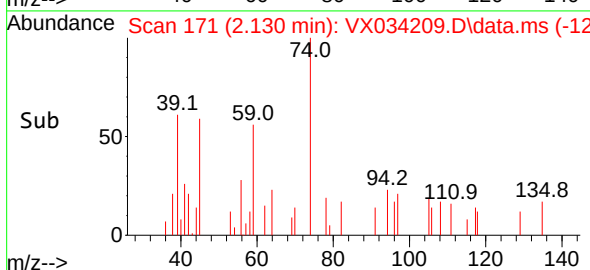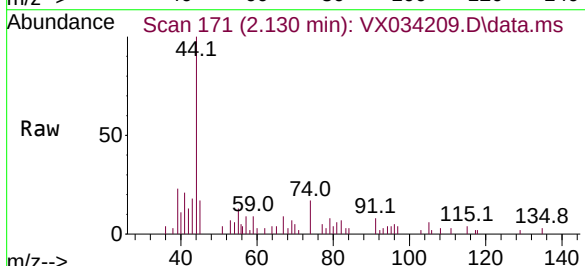



#11

Tert butyl alcohol

Concen: 2.705 ug/l

RT: 2.947 min Scan# 307

Delta R.T. -0.006 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07

Instrument :

MSVOA_X

ClientSampleId :

LOD-MDL-WATER-01-QT1-2023

Tgt Ion: 59 Resp: 318

Ion Ratio Lower Upper

59 100





57 8.1 3.7 5.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/22/2023

Supervised By :Mahesh Dadoda 02/22/2023



#13

Acrolein

Concen: 1.052 ug/l

RT: 2.233 min Scan# 188

Delta R.T. 0.000 min

Lab File: VX034209.D




Acq: 21 Feb 2023 15:07


Tgt Ion: 56 Resp: 566

Ion Ratio Lower Upper

56 100

55 0.0 56.3 84.5





#15

Acrylonitrile

Concen: 0.824 ug/l

RT: 3.075 min Scan# 311

Delta R.T. 0.018 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07

Instrument :

MSVOA_X

ClientSampleId :

LOD-MDL-WATER-01-QT1-2023





Tgt Ion: 53	Resp: 211
Ion Ratio	Lower Upper
53 100	
52 73.1	65.7 98.5
51 37.2	29.0 43.4

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/22/2023

Supervised By :Mahesh Dadoda 02/22/2023

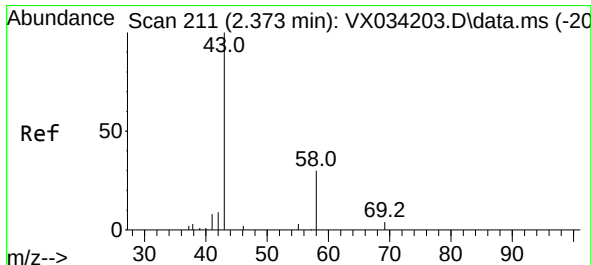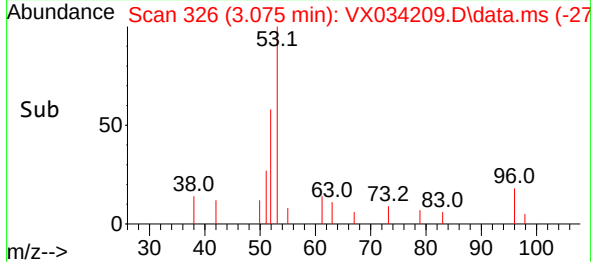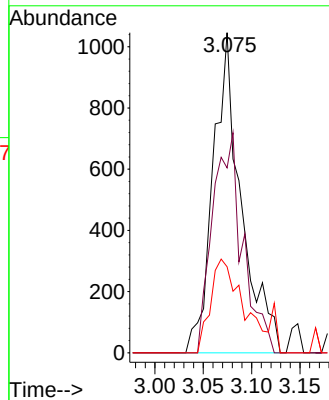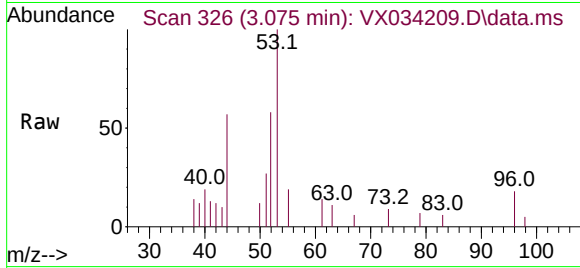

#16

Acetone

Concen: 1.058 ug/l




RT: 2.380 min Scan# 212


Delta R.T. 0.006 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07


Tgt Ion: 43	Resp: 2874
Ion Ratio	Lower Upper
43 100	
58 23.7	22.6 33.8

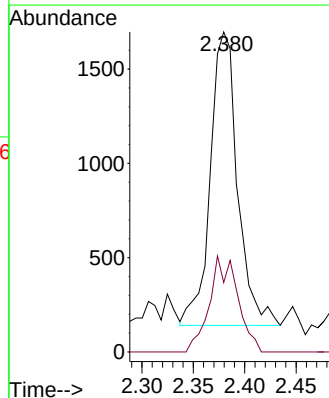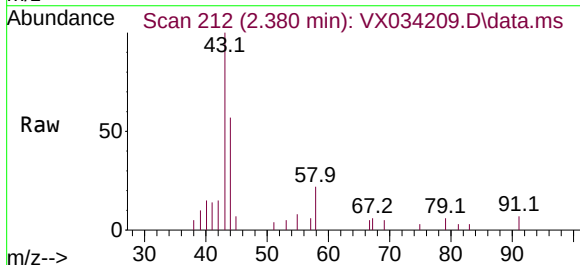



#17
Carbon Disulfide
Concen: 0.241 ug/l
RT: 2.514 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07




Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023



Tgt Ion: 76 Resp: 293
Ion Ratio Lower Upper
76 100
78 9.9 7.0 10.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 02/22/2023
Supervised By :Mahesh Dadoda 02/22/2023

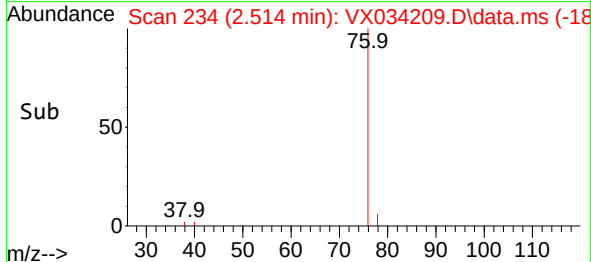

#20
Methylene Chloride
Concen: 0.351 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.006 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07


Tgt Ion: 84 Resp: 1719
Ion Ratio Lower Upper
84 100
49 105.4 101.1 151.7
51 36.2 31.0 46.6
86 61.3 52.6 79.0

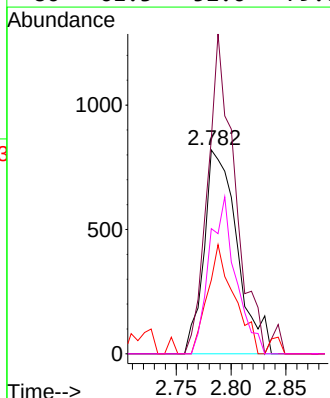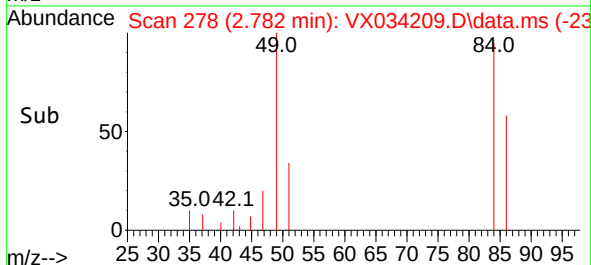



#21
trans-1,2-Dichloroethene
Concen: 0.211 ug/l
RT: 3.093 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07




Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023




Tgt Ion: 96 Resp: 93
Ion Ratio Lower Upper
96 100
61 115.8 106.7 160.1
98 44.5 50.0 75.0

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/22/2023
Supervised By :Mahesh Dadoda 02/22/2023

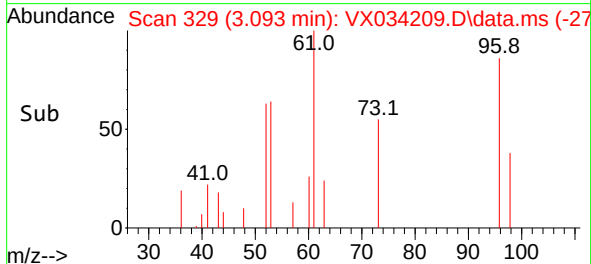


#23
Vinyl Acetate
Concen: 0.780 ug/l
RT: 3.733 min Scan# 434
Delta R.T. 0.018 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07




Tgt Ion: 43 Resp: 9834
Ion Ratio Lower Upper
43 100
86 9.2 8.4 12.6

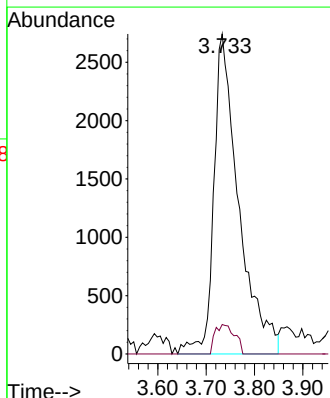



#25
2-Butanone
Concen: 0.934 ug/l m
RT: 4.593 min Scan# 51
Delta R.T. 0.049 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07




Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023




Tgt Ion: 43 Resp: 367
Ion Ratio Lower Upper
43 100
72 19.0 19.4 29.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/22/2023
Supervised By :Mahesh Dadoda 02/22/2023

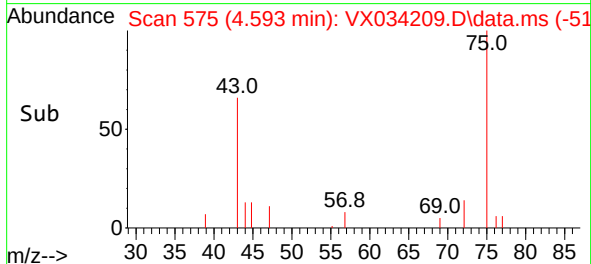


#28
Bromochloromethane
Concen: 0.247 ug/l
RT: 4.904 min Scan# 626
Delta R.T. 0.012 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07



Tgt Ion: 49 Resp: 950
Ion Ratio Lower Upper
49 100
129 0.0 0.0 4.6
130 82.2 68.5 102.7



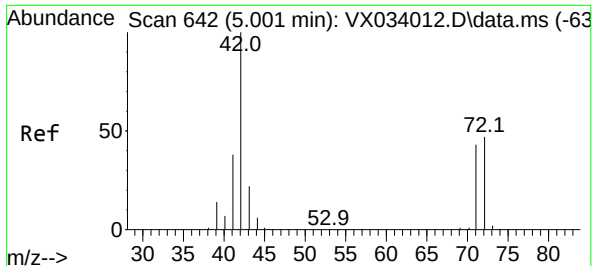

#29

Tetrahydrofuran

Concen: 1.003 ug/l

RT: 5.032 min Scan# 642

Delta R.T. 0.037 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07

Instrument :

MSVOA_X

ClientSampleId :

LOD-MDL-WATER-01-QT1-2023





Tgt Ion: 42	Resp: 240
Ion Ratio	Lower Upper
42 100	
72 32.9	34.8 52.2
71 28.6	32.2 48.2

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/22/2023

Supervised By :Mahesh Dadoda 02/22/2023

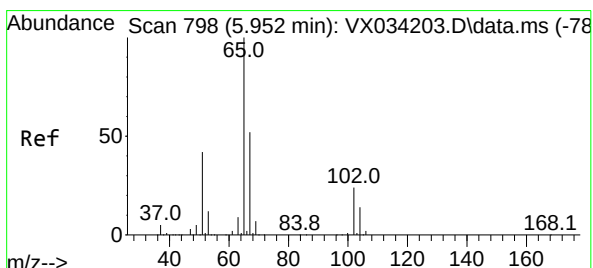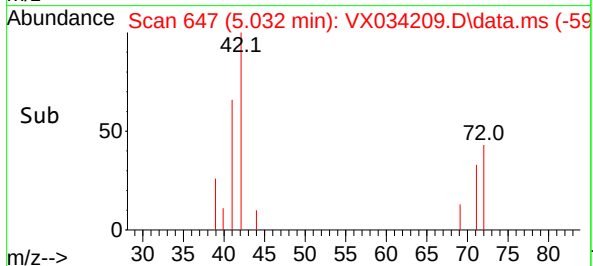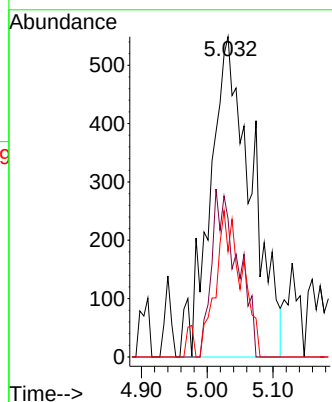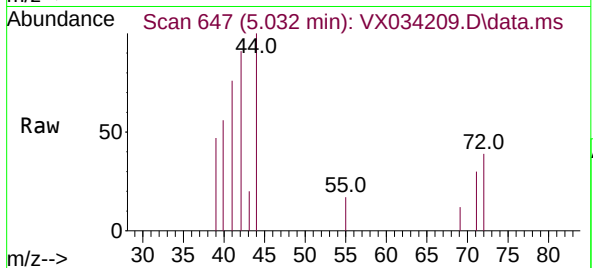

#33

1,2-Dichloroethane-d4

Concen: 34.749 ug/l




RT: 5.952 min Scan# 798


Delta R.T. 0.000 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07


Tgt Ion: 65	Resp: 183074
Ion Ratio	Lower Upper
65 100	
67 54.7	0.0 104.8

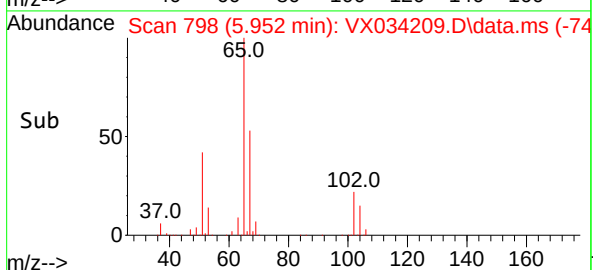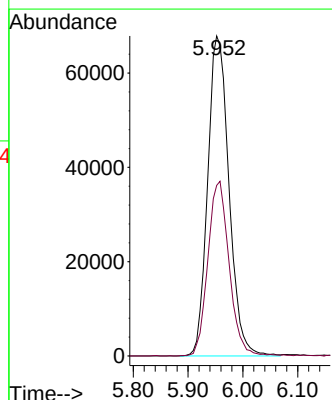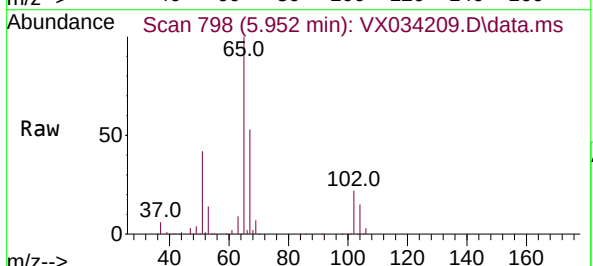



#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.006 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07




Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023




Tgt Ion:114 Resp: 62292
Ion Ratio Lower Upper
114 100
63 19.1 0.0 37.4
88 15.8 0.0 30.6

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/22/2023
Supervised By :Mahesh Dadoda 02/22/2023




#35
Dibromofluoromethane
Concen: 38.126 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07

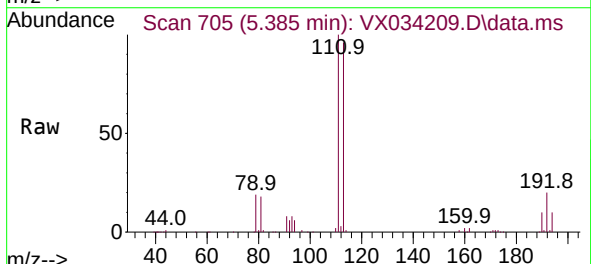

Tgt Ion:113 Resp: 154630
Ion Ratio Lower Upper
113 100
111 104.8 83.0 124.6
192 20.8 19.0 28.4

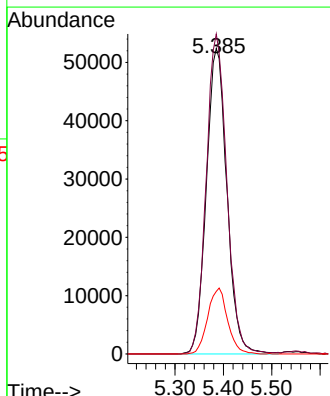



#37

Ethyl Acetate

Concen: 0.325 ug/l m

RT: 4.751 min Scan# 601

Delta R.T. 0.043 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07

Instrument :

MSVOA_X

ClientSampleId :

LOD-MDL-WATER-01-QT1-2023





Tgt Ion: 43	Resp: 217
Ion Ratio	Lower Upper
43 100	
61 0.0	11.1 16.7
70 0.0	8.5 12.7

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/22/2023

Supervised By :Mahesh Dadoda 02/22/2023

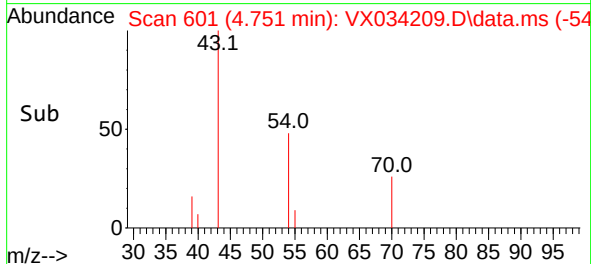

#41

Methacrylonitrile

Concen: 0.229 ug/l m




RT: 4.928 min Scan# 630


Delta R.T. 0.012 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07

Tgt Ion: 41	Resp: 855
Ion Ratio	Lower Upper
41 100	
39 18.4	43.8 65.6
67 0.0	54.8 82.2
52 3.4	23.0 34.6

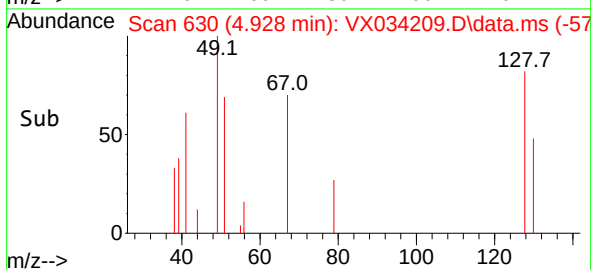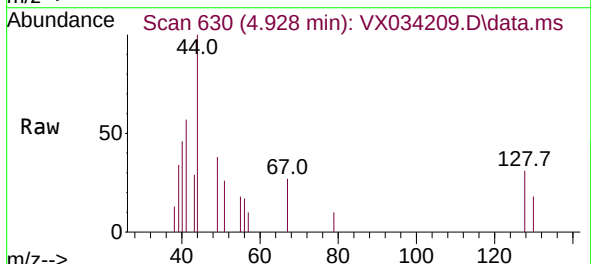



#42

1,2-Dichloroethane

Concen: 0.206 ug/l

RT: 6.098 min Scan# 81

Delta R.T. 0.012 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07

Instrument :

MSVOA_X

ClientSampleId :

LOD-MDL-WATER-01-QT1-2023





Tgt Ion: 62 Resp: 1280
 Ion Ratio Lower Upper
 62 100
 98 9.8 0.0 20.2

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/22/2023

Supervised By :Mahesh Dadoda 02/22/2023

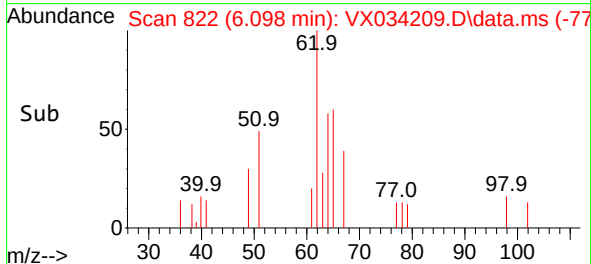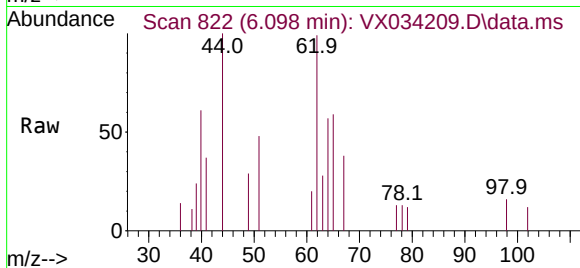

#48

Methyl methacrylate

Concen: 0.258 ug/l




RT: 7.708 min Scan# 1086


Delta R.T. 0.018 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07

Tgt Ion: 41 Resp: 1450
 Ion Ratio Lower Upper
 41 100
 69 25.2 63.1 94.7#
 39 56.0 43.2 64.8

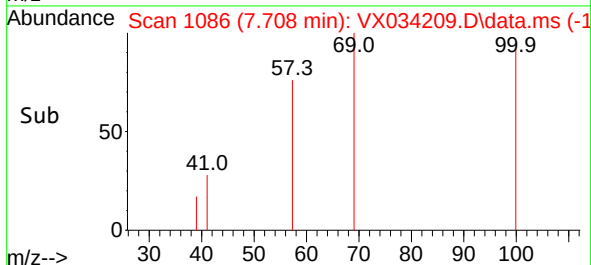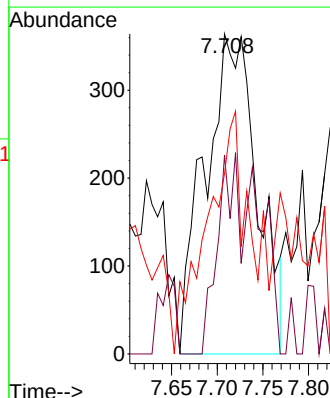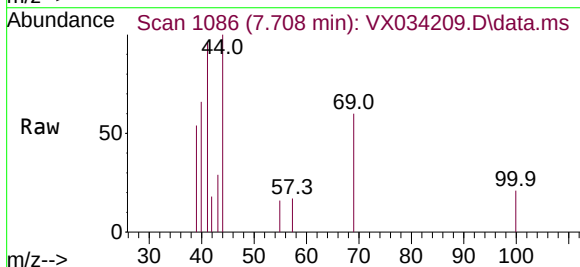







#49
1,4-Dioxane
Concen: 2.938 ug/l
RT: 7.684 min Scan# 1082
Delta R.T. 0.031 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07

Instrument : MSVOA_X
ClientSampleId : LOD-MDL-WATER-01-QT1-2023

Tgt Ion: 88 Resp: 329
Ion Ratio Lower Upper
88 100
43 0.0 0.0 0.0
58 63.5 56.5 84.7




Manual Integrations
APPROVED


Reviewed By :John Carlone 02/22/2023
Supervised By :Mahesh Dadoda 02/22/2023

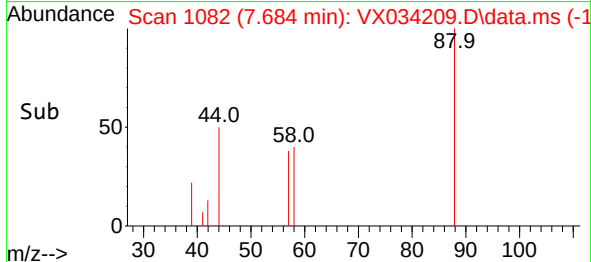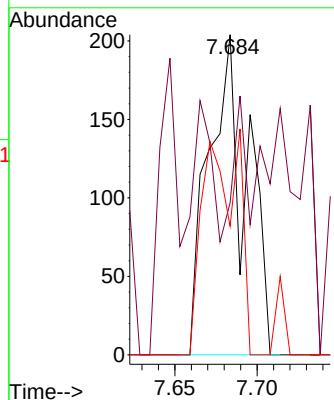

#50
Toluene-d8
Concen: 39.405 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07


Tgt Ion: 98 Resp: 573808
Ion Ratio Lower Upper
98 100
100 66.6 53.6 80.4

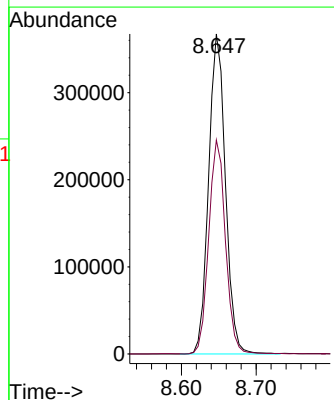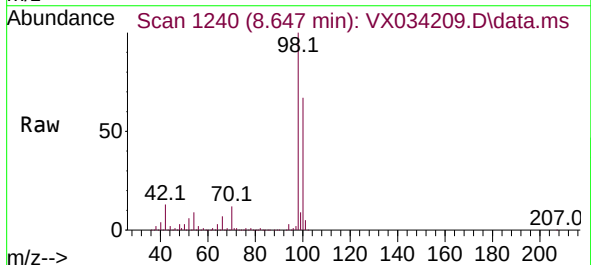

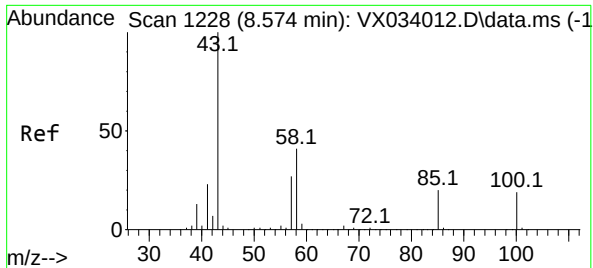

#51
4-Methyl-2-Pentanone
Concen: 0.820 ug/l
RT: 8.574 min Scan# 1176
Delta R.T. 0.006 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07




Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023

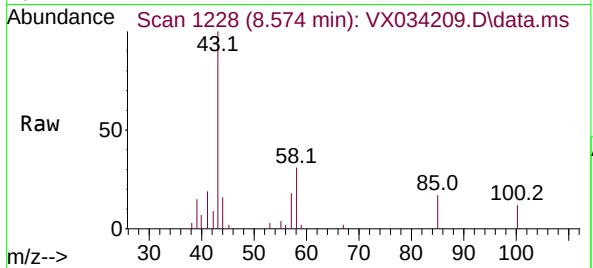

Tgt Ion: 43 Resp: 533
Ion Ratio Lower Upper
43 100
58 34.3 31.2 46.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 02/22/2023
Supervised By :Mahesh Dadoda 02/22/2023

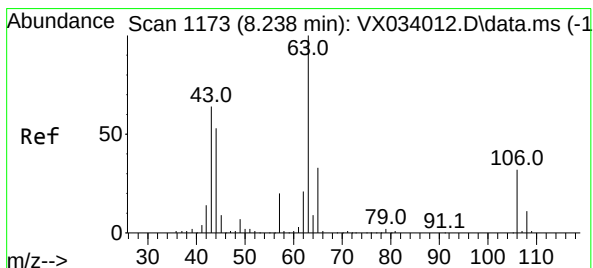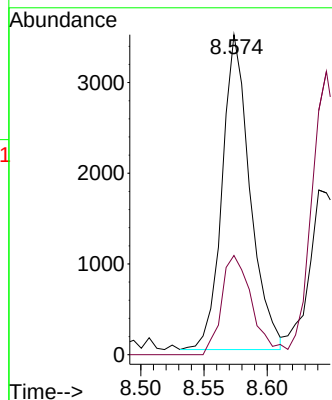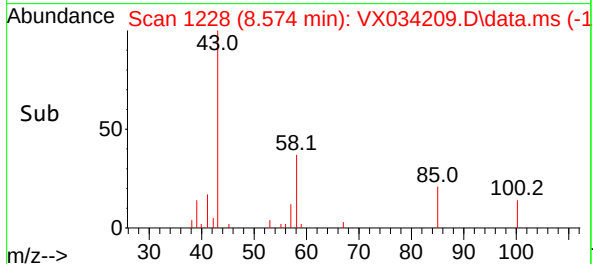

#58
2-Chloroethyl Vinyl ether
Concen: 1.314 ug/l
RT: 8.257 min Scan# 1176
Delta R.T. 0.018 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07

Tgt Ion: 63 Resp: 4187
Ion Ratio Lower Upper
63 100
106 25.9 24.5 36.7

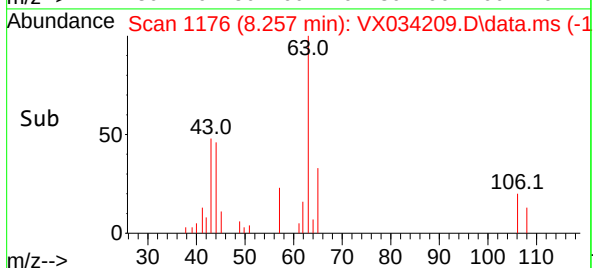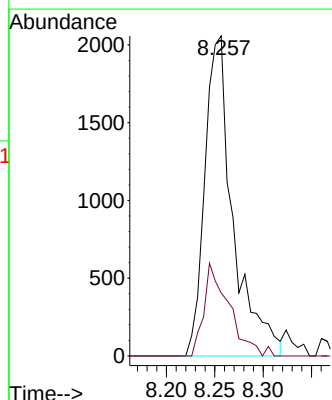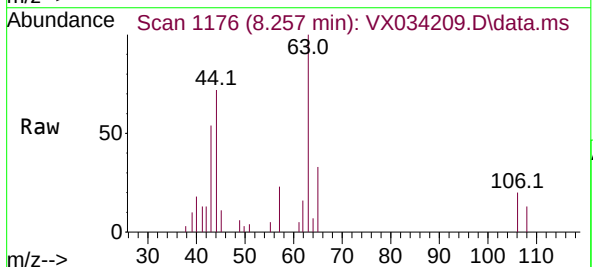



#59

2-Hexanone

Concen: 0.690 ug/l

RT: 9.439 min Scan# 1370

Delta R.T. 0.012 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07

Instrument :

MSVOA_X

ClientSampleId :

LOD-MDL-WATER-01-QT1-2023

Tgt Ion: 43 Resp: 342

Ion Ratio Lower Upper

43 100





58 49.8 27.4 82.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 02/22/2023

Supervised By :Mahesh Dadoda 02/22/2023

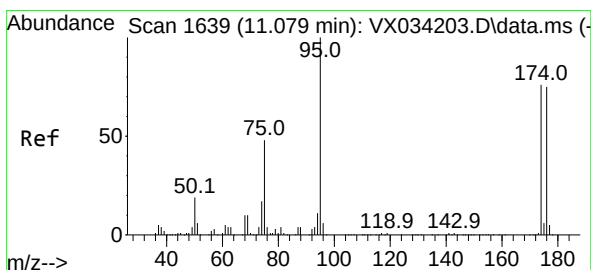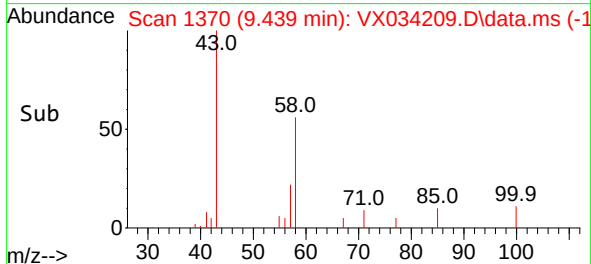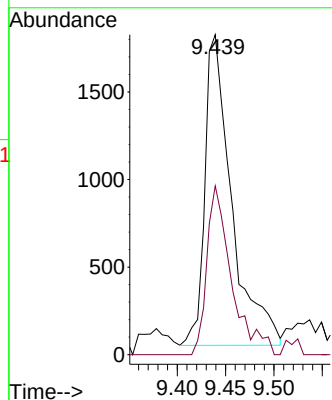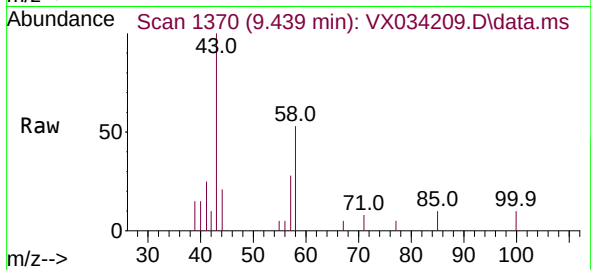

#62

4-Bromofluorobenzene

Concen: 36.481 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX034209.D

Acq: 21 Feb 2023 15:07




Tgt Ion: 95 Resp: 203198


Ion Ratio Lower Upper

95 100

174 80.9 0.0 184.4

176 78.5 0.0 178.8

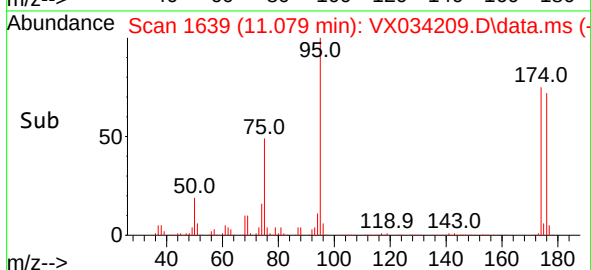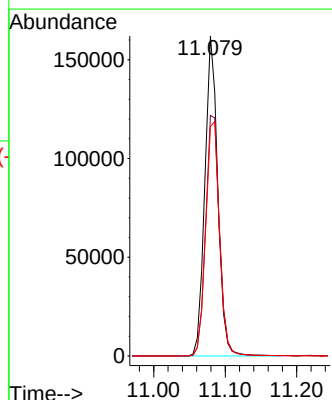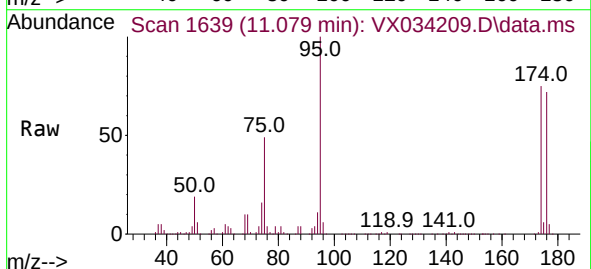







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07

Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT1-2023

Tgt Ion:117 Resp: 54119
Ion Ratio Lower Upper
117 100
82 54.9 40.6 60.8
119 32.5 25.6 38.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 02/22/2023
Supervised By :Mahesh Dadoda 02/22/2023

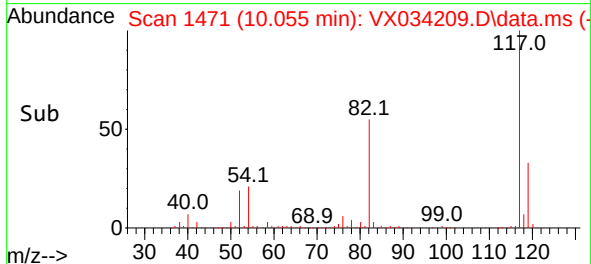

#68
m/p-Xylenes
Concen: 0.325 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX034209.D
Acq: 21 Feb 2023 15:07


Tgt Ion:106 Resp: 2518
Ion Ratio Lower Upper
106 100
91 204.2 156.4 234.6

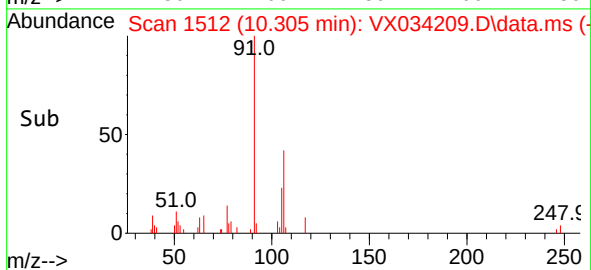



#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX034209.D
 Acq: 21 Feb 2023 15:07




Instrument :
 MSVOA_X
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2023




Tgt Ion:152 Resp: 253602
 Ion Ratio Lower Upper
 152 100
 115 58.1 38.7 116.1
 150 156.4 0.0 348.2

Manual Integrations
 APPROVED



Reviewed By :John Carlone 02/22/2023
 Supervised By :Mahesh Dadoda 02/22/2023




#93
 1,2,4-Trichlorobenzene
 Concen: 0.207 ug/l
 RT: 13.597 min Scan# 2052
 Delta R.T. 0.006 min
 Lab File: VX034209.D
 Acq: 21 Feb 2023 15:07




Tgt Ion:180 Resp: 1136
 Ion Ratio Lower Upper
 180 100
 182 83.9 47.9 143.6
 145 14.1 14.1 42.2

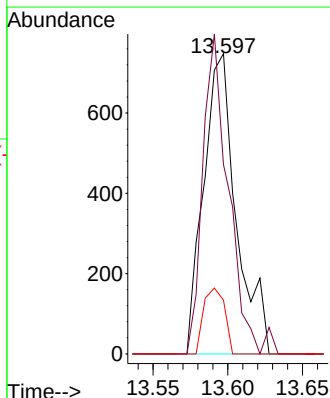



#94
 Hexachlorobutadiene
 Concen: 0.238 ug/l
 RT: 13.731 min Scan# 2074
 Delta R.T. 0.006 min
 Lab File: VX034209.D
 Acq: 21 Feb 2023 15:07

Instrument : MSVOA_X
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2023



Tgt Ion:225 Resp: 540
 Ion Ratio Lower Upper
 225 100
 223 52.4 31.3 93.9
 227 58.7 32.3 96.9

Manual Integrations
 APPROVED

Reviewed By :John Carlone 02/22/2023
 Supervised By :Mahesh Dadoda 02/22/2023

