
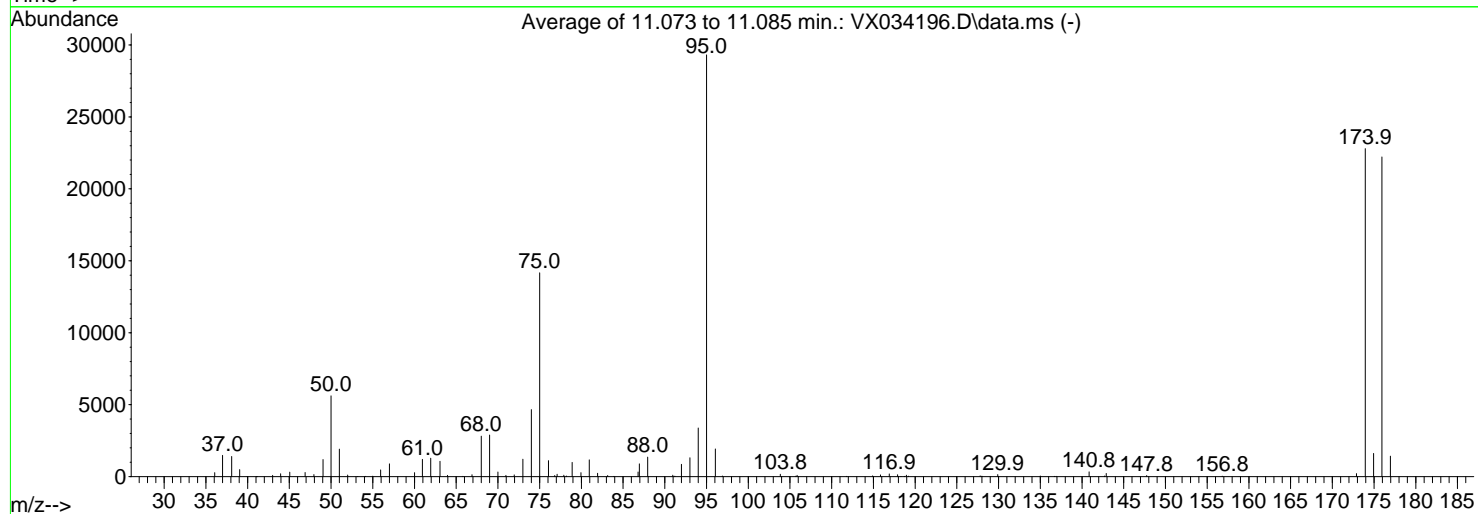


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX022123\  
 Data File : VX034196.D  
 Acq On : 21 Feb 2023 08:30  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X021723W.M  
 Title : SW846 8260  
 Last Update : Fri Feb 17 12:33:35 2023

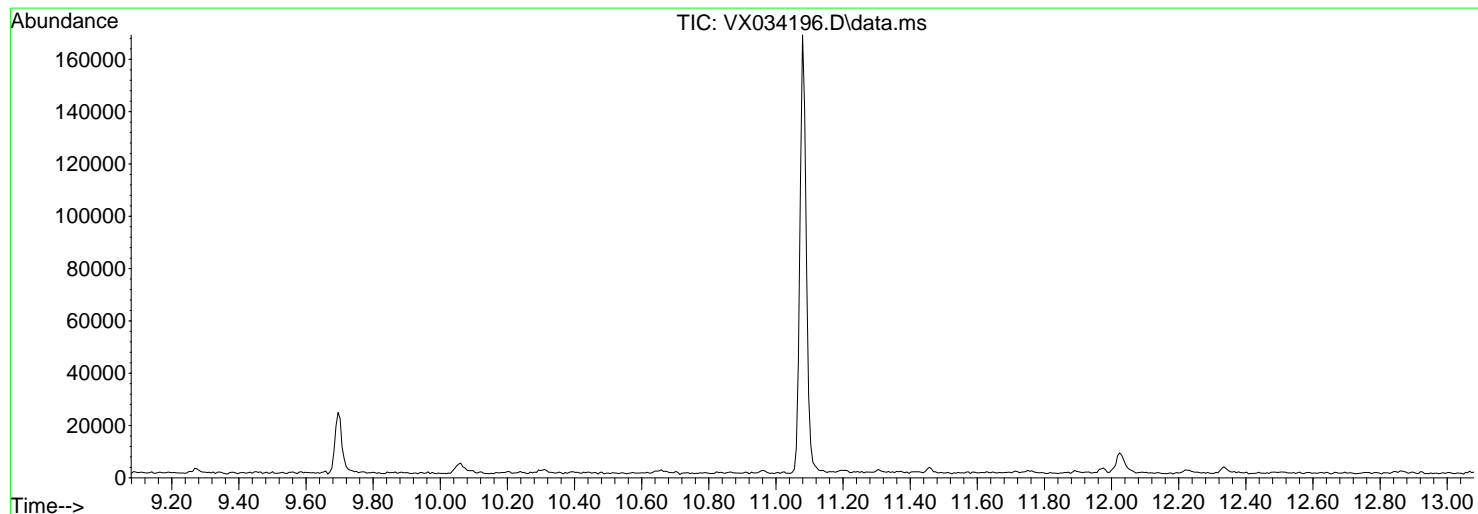

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
50	95	15	40	19.2	5614	PASS
75	95	30	60	48.3	14162	PASS
95	95	100	100	100.0	29312	PASS
96	95	5	9	6.6	1928	PASS
173	174	0.00	2	0.9	213	PASS
174	95	50	100	77.8	22792	PASS
175	174	5	9	7.1	1616	PASS
176	174	95	101	97.5	22214	PASS
177	176	5	9	6.4	1429	PASS