

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022124\
Data File : VX040377.D
Acq On : 21 Feb 2024 13:34
Operator : JC/MD
Sample : P1520-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178I-20240215

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M

Title : SW846 8260

Signal : TIC: VX040377.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	325	333	340	rBV3	2320	5512	1.23%	0.219%
2	5.385	693	705	718	rBV2	50975	149113	33.25%	5.922%
3	5.550	721	732	746	rBV2	80720	235918	52.60%	9.370%
4	5.952	789	798	811	rBV2	60650	161933	36.11%	6.431%
5	6.757	921	930	945	rBV	135084	326966	72.90%	12.986%
6	8.647	1233	1240	1252	rBV	282018	448493	100.00%	17.812%
7	9.275	1338	1343	1350	rBV2	7153	11379	2.54%	0.452%
8	10.055	1465	1471	1483	rBV	298544	416616	92.89%	16.546%
9	11.079	1634	1639	1649	rBV	249528	320308	71.42%	12.721%
10	11.311	1672	1677	1682	rVB2	7209	9822	2.19%	0.390%
11	12.018	1788	1793	1801	rBV	340403	431848	96.29%	17.151%




Sum of corrected areas: 2517908

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022124\
Data File : VX040377.D
Acq On : 21 Feb 2024 13:34
Operator : JC/MD
Sample : P1520-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178I-20240215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

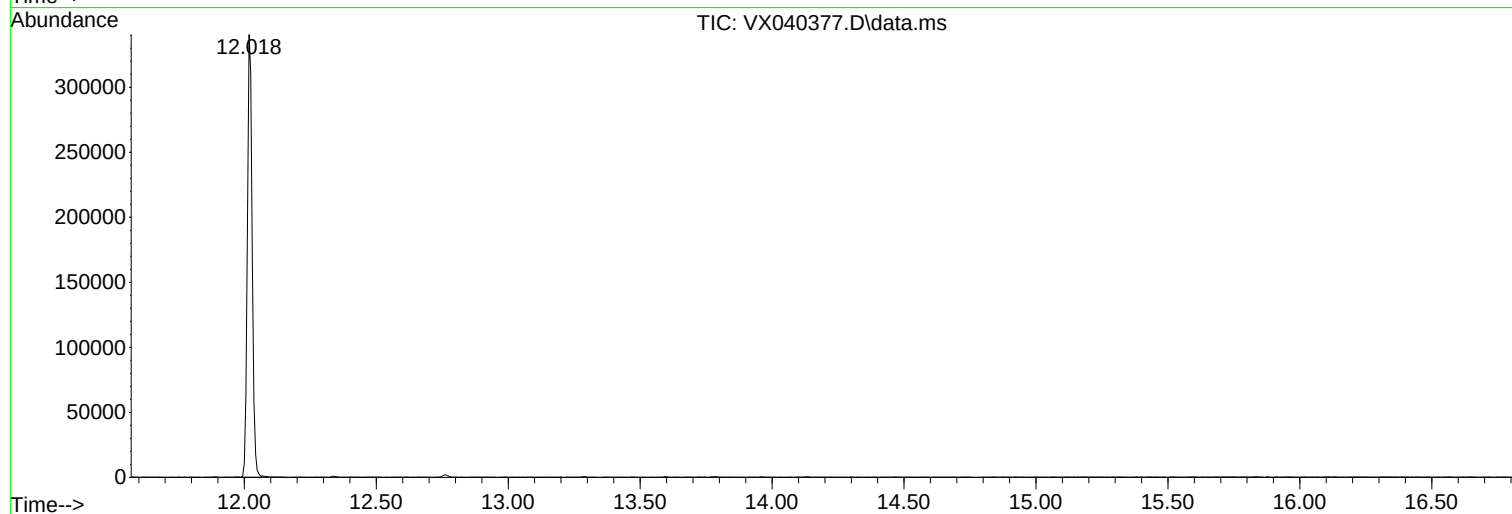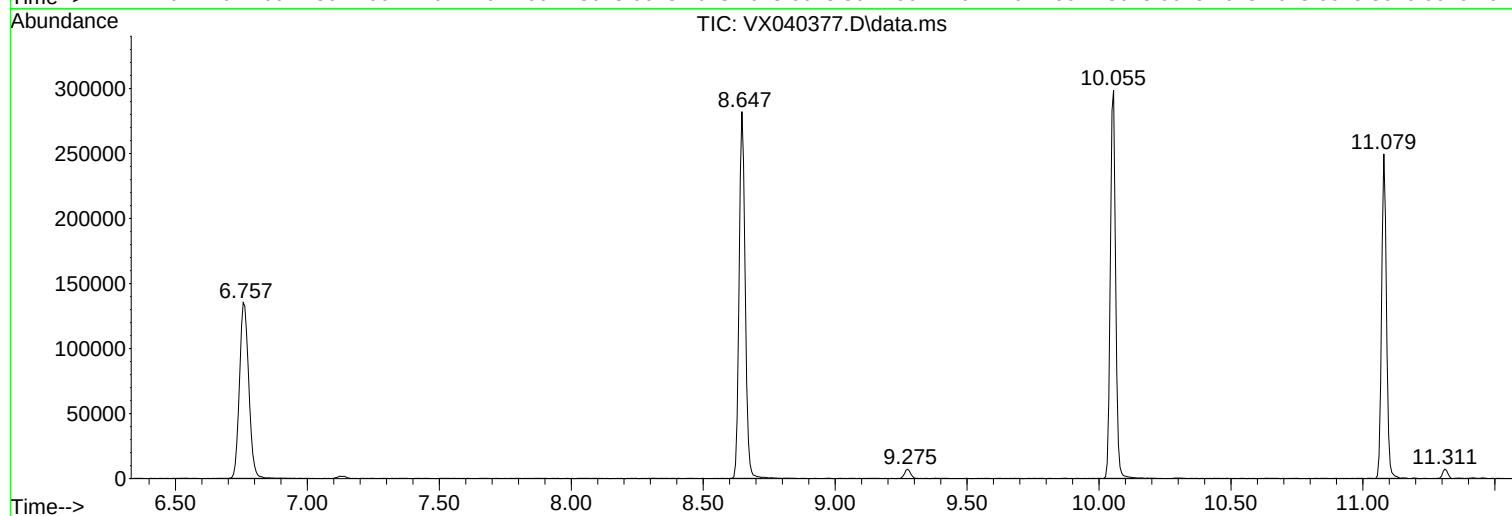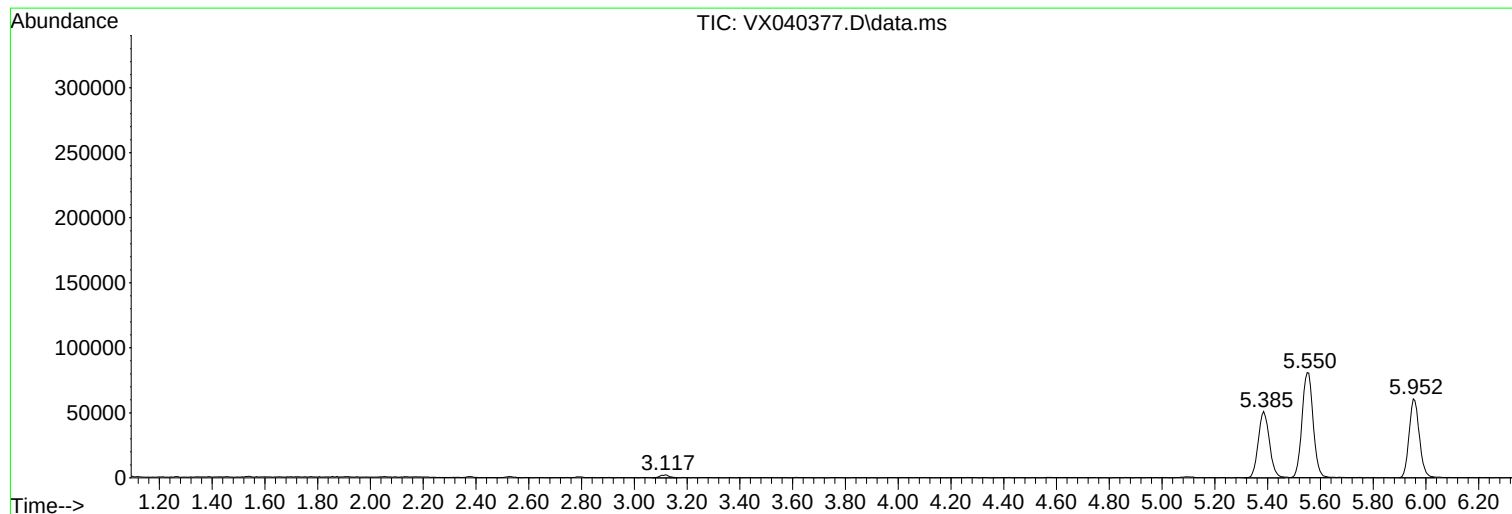

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022124\
Data File : VX040377.D
Acq On : 21 Feb 2024 13:34
Operator : JC/MD
Sample : P1520-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178I-20240215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022124\
Data File : VX040377.D
Acq On : 21 Feb 2024 13:34
Operator : JC/MD
Sample : P1520-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178I-20240215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------