

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022222\
 Data File : VX027130.D
 Acq On : 22 Feb 2022 13:34
 Operator : JC/MD
 Sample : N1600-08ME
 Misc : 4.52g/10.0mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AA9ME

Quant Time: Feb 22 15:17:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 08 07:07:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	97412	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	155737	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	146698	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	72973	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	56247	48.102	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	96.200%		
35) Dibromofluoromethane	5.397	113	46124	49.711	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.420%		
50) Toluene-d8	8.653	98	181222	53.209	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	106.420%		
62) 4-Bromofluorobenzene	11.085	95	73530	61.321	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	122.640%		
Target Compounds						Qvalue
5) Bromomethane	1.599	94	194	0.443	ug/l	99
10) Methyl Iodide	2.441	142	452	2.567	ug/l #	59
16) Acetone	2.422	43	172	0.335	ug/l #	46
29) Tetrahydrofuran	5.050	42	654	1.163	ug/l #	69
31) Cyclohexane	5.556	56	1791	0.964	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	7210	4.926	ug/l #	50
38) Carbon Tetrachloride	5.556	117	9461	6.164	ug/l #	17
39) Methylcyclohexane	7.379	83	2474	1.378	ug/l	89
41) Methacrylonitrile	5.050	41	301	0.334	ug/l #	25
43) Isopropyl Acetate	6.385	43	1178	0.460	ug/l #	62
51) 4-Methyl-2-Pentanone	8.598	43	448	0.289	ug/l #	37
55) 1,1,2-Trichloroethane	9.104	97	4394	4.297	ug/l #	18
56) Ethyl methacrylate	9.104	69	953	0.588	ug/l #	1
59) 2-Hexanone	9.385	43	6896	6.079	ug/l #	30
67) Ethyl Benzene	10.195	91	9452	1.760	ug/l	98
68) m/p-Xylenes	10.305	106	13556	6.562	ug/l	98
69) o-Xylene	10.647	106	11228	5.546	ug/l	98
73) Isopropylbenzene	10.964	105	10112	1.759	ug/l	99
74) N-amyl acetate	10.860	43	12814	5.579	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.220	83	10162	6.515	ug/l #	26
76) 1,2,3-Trichloropropane	11.384	75	1386	0.868	ug/l #	1
78) n-propylbenzene	11.305	91	41181	6.463	ug/l	99
79) 2-Chlorotoluene	11.384	91	20046	5.091	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.457	105	64289	13.590	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.085	75	34525	66.384	ug/l #	8
82) 4-Chlorotoluene	11.457	91	7581	1.716	ug/l #	52
83) tert-Butylbenzene	11.756	119	25588	5.675	ug/l #	62
84) 1,2,4-Trimethylbenzene	11.756	105	203944	42.741	ug/l	97
85) sec-Butylbenzene	11.896	105	35957	6.291	ug/l	84
86) p-Isopropyltoluene	12.012	119	24174	4.993	ug/l	98
89) n-Butylbenzene	12.335	91	91383	23.068	ug/l #	49
90) Hexachloroethane	12.536	117	9746	13.927	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	12.920	75	967	2.521	ug/l #	3
95) Naphthalene	13.780	128	40118	7.512	ug/l #	86
96) 1,2,3-Trichlorobenzene	13.975	180	3228	2.091	ug/l #	1

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022222\
Data File : VX027130.D
Acq On : 22 Feb 2022 13:34
Operator : JC/MD
Sample : N1600-08ME
Misc : 4.52g/10.0mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME

Quant Time: Feb 22 15:17:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022222\
Data File : VX027130.D
Acq On : 22 Feb 2022 13:34
Operator : JC/MD
Sample : N1600-08ME
Misc : 4.52g/10.0mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME

Quant Time: Feb 22 15:17:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration




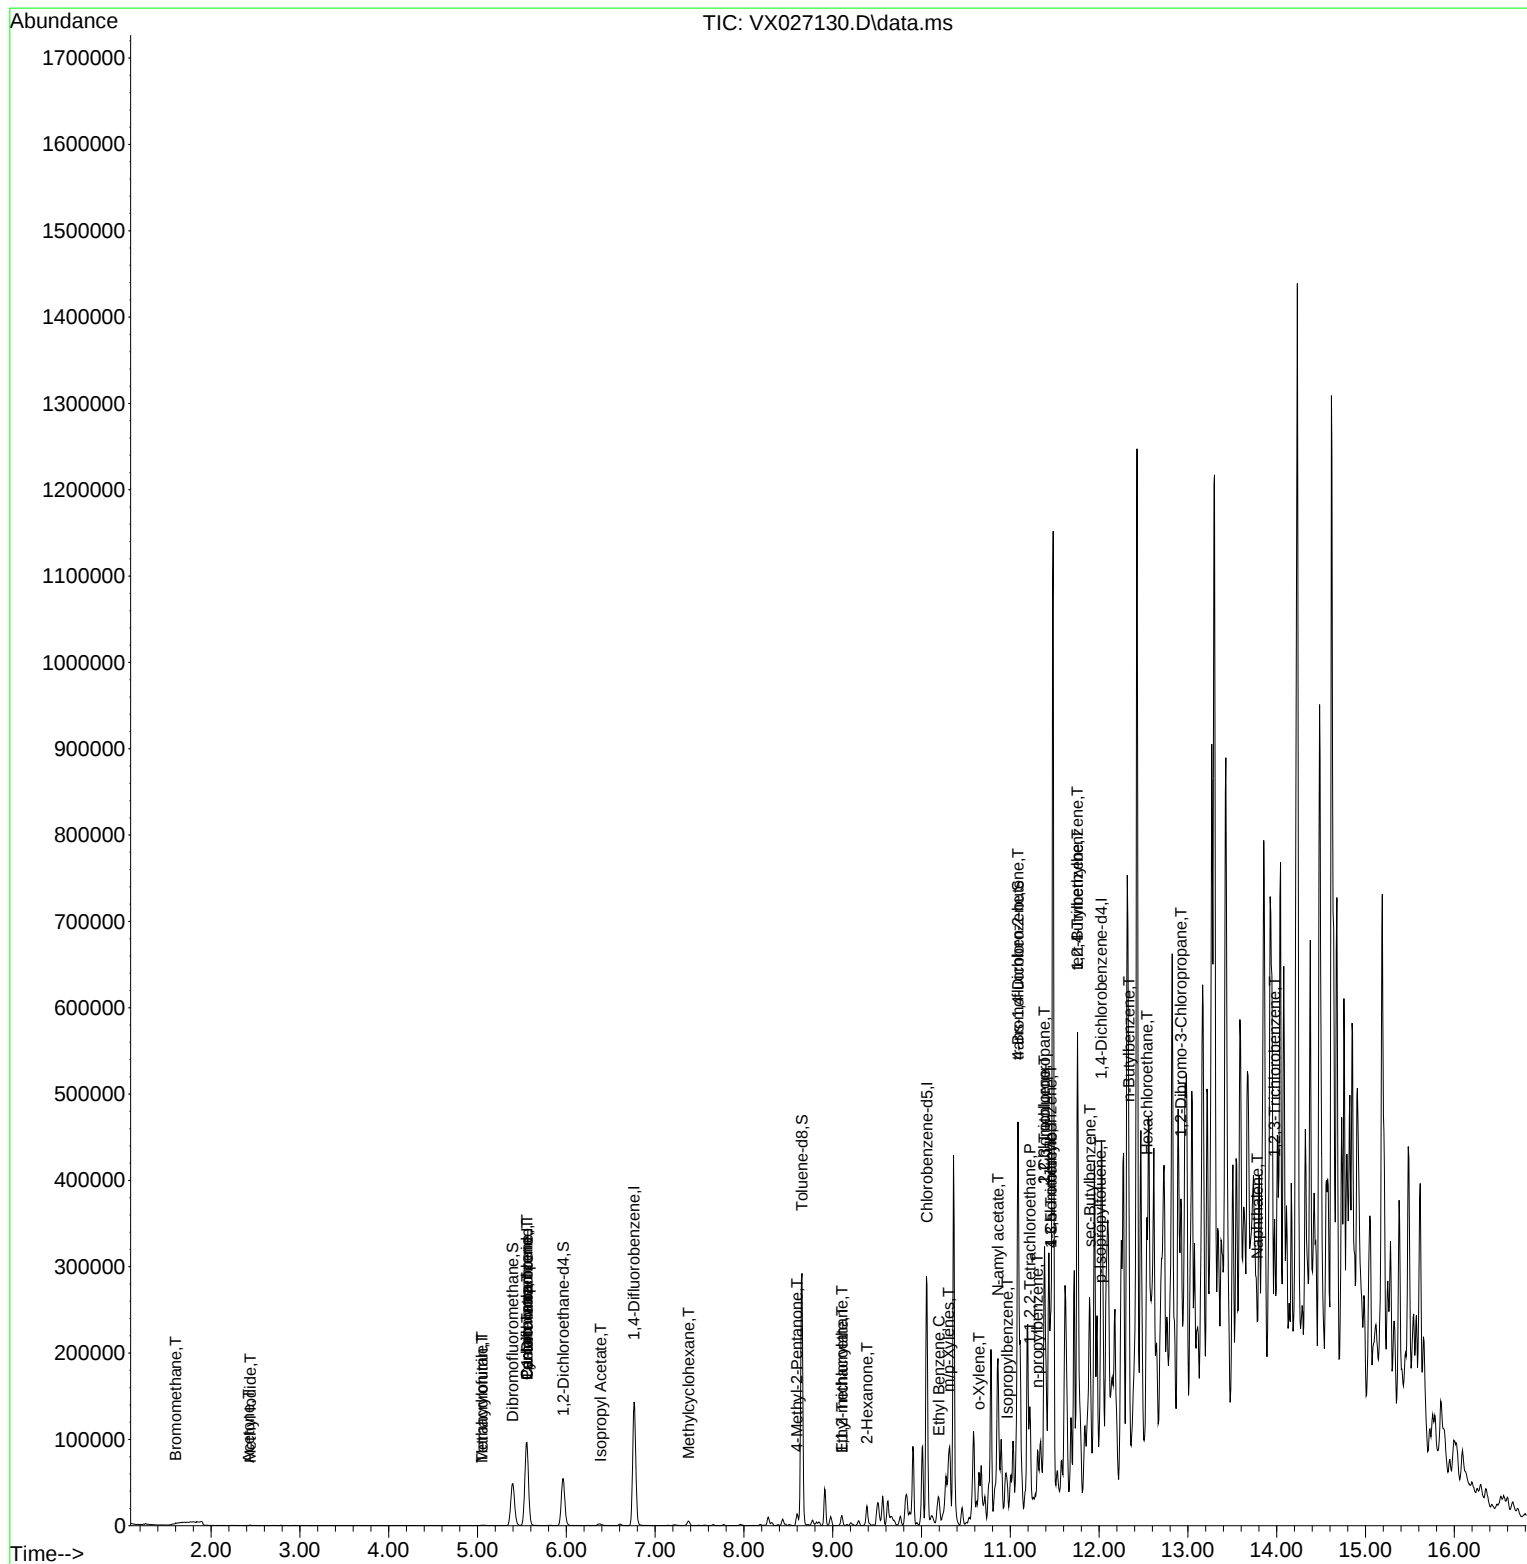




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion:168 Resp: 97412
Ion Ratio Lower Upper
168 100
99 57.4 50.3 75.5

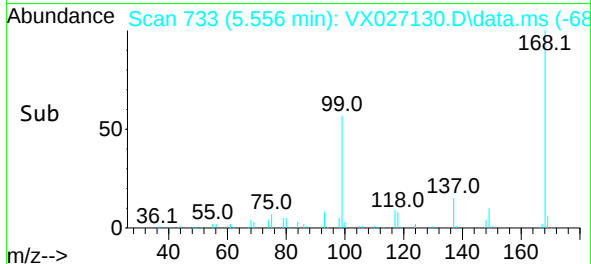

#5
Bromomethane
Concen: 0.443 ug/l
RT: 1.599 min Scan# 84
Delta R.T. -0.012 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion: 94 Resp: 194
Ion Ratio Lower Upper
94 100
96 94.4 75.9 113.9




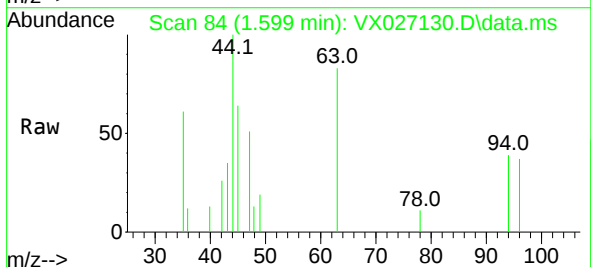




#10
Methyl Iodide
Concen: 2.567 ug/l
RT: 2.441 min Scan# 219
Delta R.T. -0.018 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion:142 Resp: 452
Ion Ratio Lower Upper
142 100
127 19.0 38.1 57.1#
141 0.0 11.2 16.8#

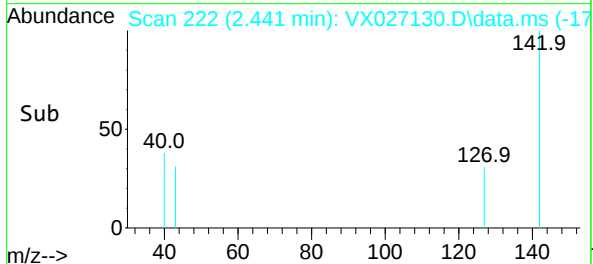

#16
Acetone
Concen: 0.335 ug/l
RT: 2.422 min Scan# 219
Delta R.T. 0.037 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion: 43 Resp: 172
Ion Ratio Lower Upper
43 100
58 0.0 23.0 34.6#

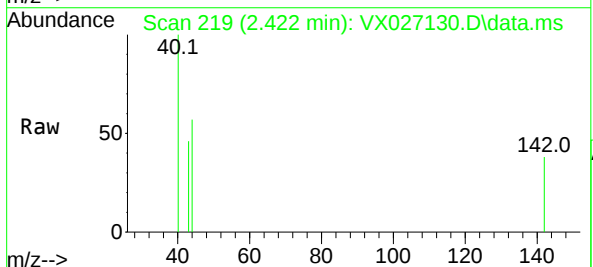



#29

Tetrahydrofuran

Concen: 1.163 ug/l

RT: 5.050 min Scan# 61

Delta R.T. 0.043 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34





Instrument :

MSVOA_X

ClientSampleId :

C0AA9ME

Tgt Ion:	42	Resp:	654
Ion	Ratio	Lower	Upper
42	100		
72	16.5	34.6	52.0#
71	27.7	31.8	47.8#

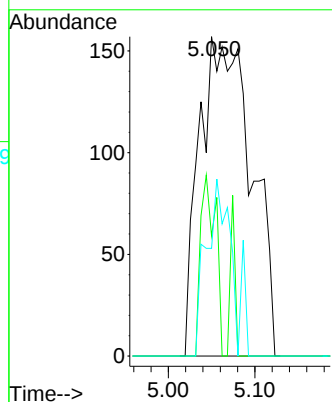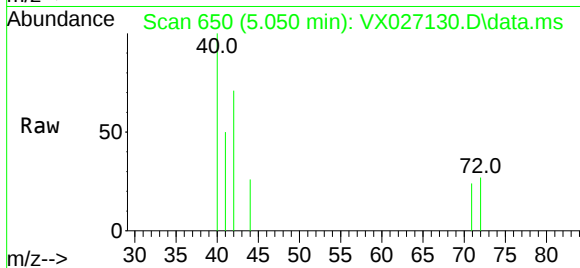

#31

Cyclohexane

Concen: 0.964 ug/l




RT: 5.556 min Scan# 733


Delta R.T. 0.079 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34

Tgt Ion:	56	Resp:	1791
Ion	Ratio	Lower	Upper
56	100		
69	161.0	25.8	38.6#
84	141.4	68.9	103.3#

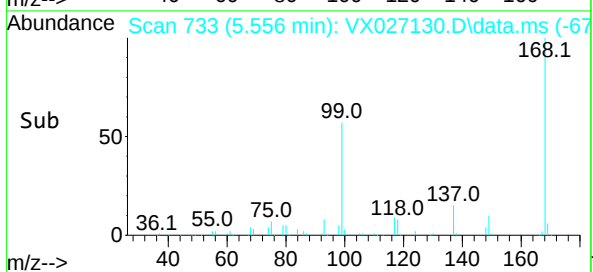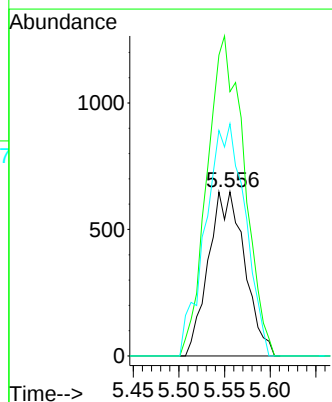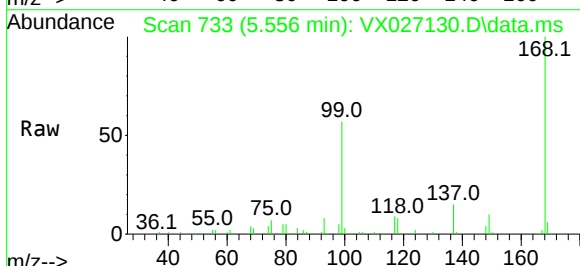



#33

1,2-Dichloroethane-d4

Concen: 48.102 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34

Instrument :

MSVOA_X

ClientSampleId :





C0AA9ME

Tgt Ion: 65 Resp: 56247

Ion Ratio Lower Upper

65 100

67 51.5 0.0 100.8

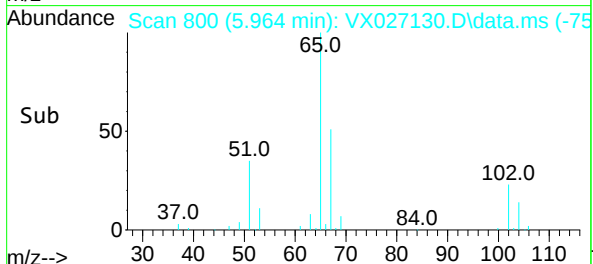

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34




Tgt Ion: 114 Resp: 155737


Ion Ratio Lower Upper

114 100

63 19.8 0.0 42.8

88 16.1 0.0 33.0

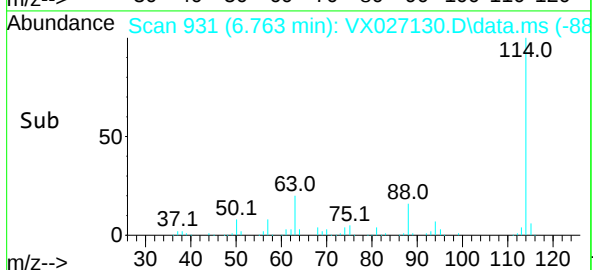



#35

Dibromofluoromethane

Concen: 49.711 ug/l

RT: 5.397 min Scan# 706

Delta R.T. 0.006 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34

Instrument :

MSVOA_X

ClientSampleId :

C0AA9ME





Tgt Ion:113 Resp: 46124

Ion Ratio Lower Upper

113 100

111 101.5 81.2 121.8

192 20.4 15.0 22.4

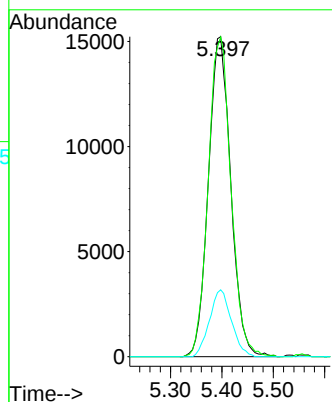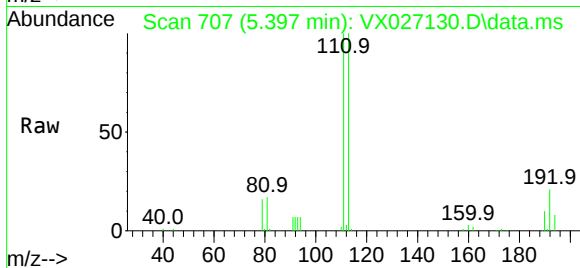

#36

1,1-Dichloropropene

Concen: 4.926 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34




Tgt Ion: 75 Resp: 7210


Ion Ratio Lower Upper

75 100

110 9.0 17.2 51.6#


77 0.0 24.6 36.8#

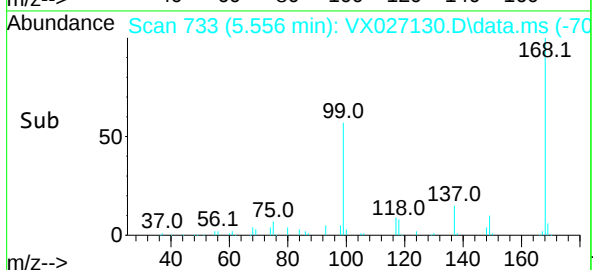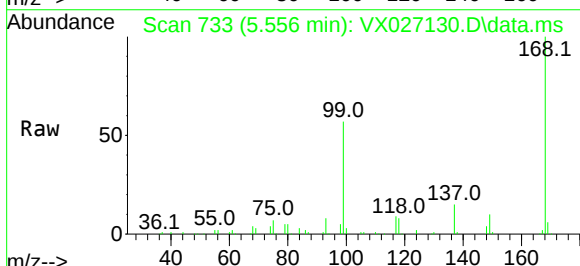






#38
Carbon Tetrachloride
Concen: 6.164 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME







Tgt Ion:117 Resp: 9461
Ion Ratio Lower Upper
117 100
119 4.5 74.7 112.1#
121 0.0 25.4 38.0#



#39
Methylcyclohexane
Concen: 1.378 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion: 83 Resp: 2474
Ion Ratio Lower Upper
83 100
55 89.2 63.6 95.4
98 40.2 38.4 57.6


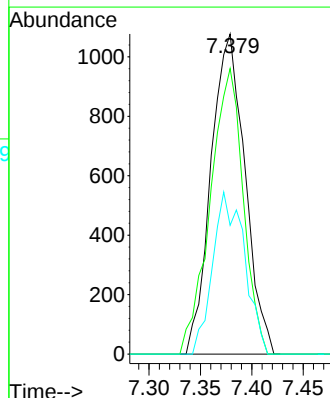

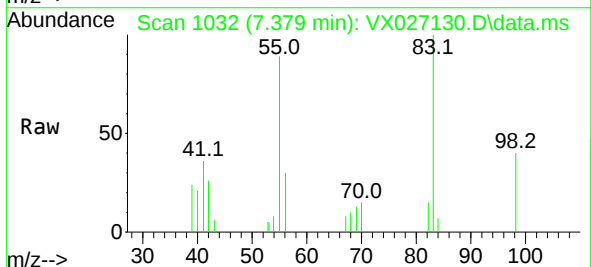




#41
Methacrylonitrile
Concen: 0.334 ug/l
RT: 5.050 min Scan# 61
Delta R.T. 0.128 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion: 41	Resp:	301
Ion	Ratio	Lower Upper
41	100	
39	0.0	45.4 68.0#
67	0.0	53.2 79.8#
52	0.0	23.0 34.6#

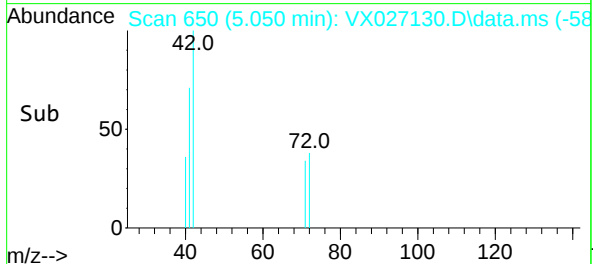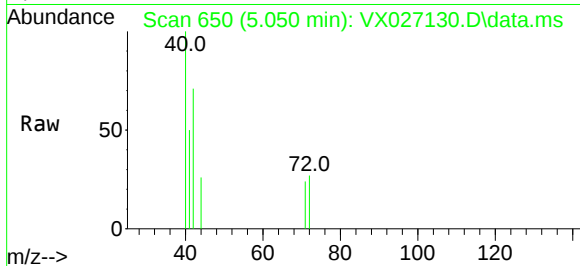

#43
Isopropyl Acetate
Concen: 0.460 ug/l
RT: 6.385 min Scan# 869
Delta R.T. 0.043 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion: 43	Resp:	1178
Ion	Ratio	Lower Upper
43	100	
61	0.0	15.4 23.0#
87	0.0	10.2 15.2#


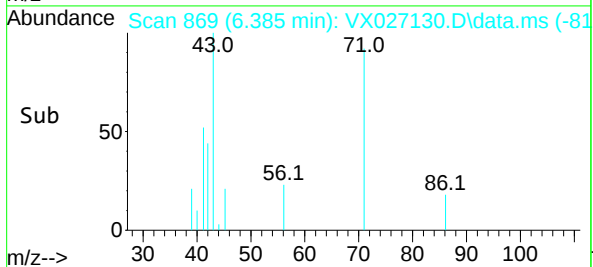

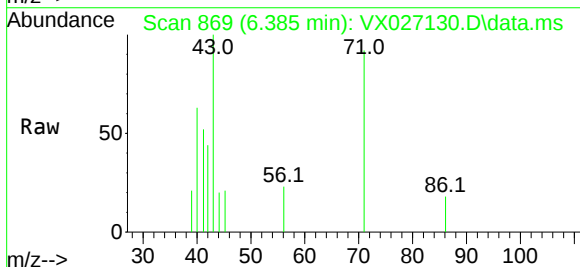




#50
Toluene-d8
Concen: 53.209 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion: 98 Resp: 181222
Ion Ratio Lower Upper
98 100
100 67.8 53.2 79.8

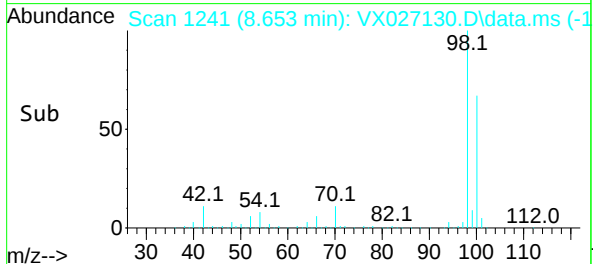

#51
4-Methyl-2-Pentanone
Concen: 0.289 ug/l
RT: 8.598 min Scan# 1232
Delta R.T. 0.025 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion: 43 Resp: 448
Ion Ratio Lower Upper
43 100
58 0.0 30.5 45.7#

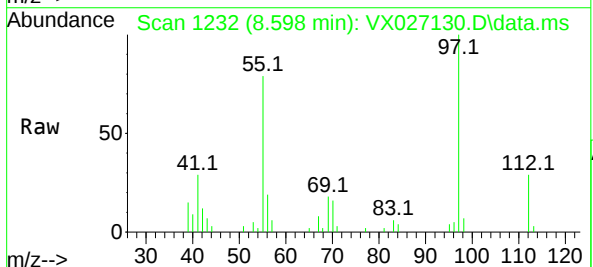



#55

1,1,2-Trichloroethane

Concen: 4.297 ug/l

RT: 9.104 min Scan# 1315

Delta R.T. -0.049 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34

Instrument :

MSVOA_X

ClientSampleId :

C0AA9ME

Tgt Ion: 97 Resp: 4394





Ion Ratio Lower Upper

97 100

83 5.7 68.4 102.6#

85 0.0 44.0 66.0#

99 0.0 49.8 74.6#

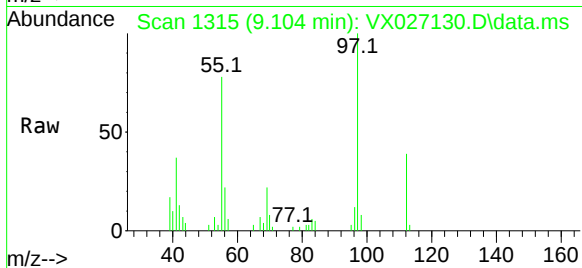

#56

Ethyl methacrylate

Concen: 0.588 ug/l

RT: 9.104 min Scan# 1315

Delta R.T. -0.012 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34




Tgt Ion: 69 Resp: 953


Ion Ratio Lower Upper

69 100

41 166.6 57.2 85.8#

39 86.6 30.9 46.3#

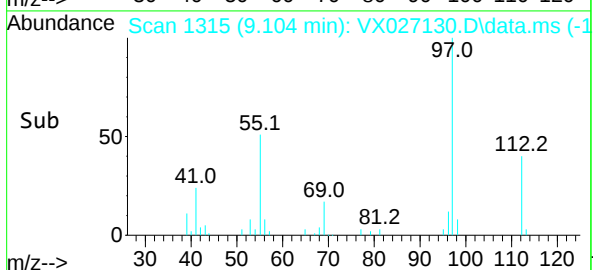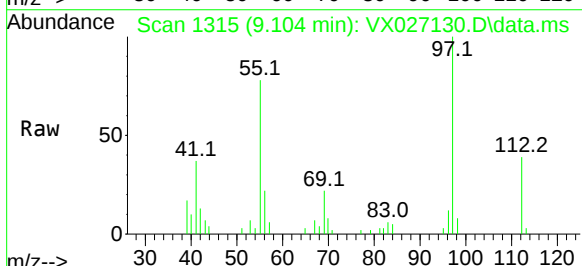



#59

2-Hexanone

Concen: 6.079 ug/l

RT: 9.385 min Scan# 11

Delta R.T. -0.049 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34

Instrument :

MSVOA_X

ClientSampleId :





C0AA9ME

Tgt Ion: 43 Resp: 6896

Ion Ratio Lower Upper

43 100

58 3.0 26.4 79.2#

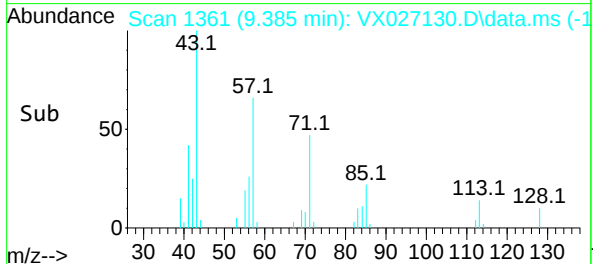

#62

4-Bromofluorobenzene

Concen: 61.321 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.006 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34




Tgt Ion: 95 Resp: 73530


Ion Ratio Lower Upper

95 100

174 77.2 0.0 148.6

176 74.2 0.0 141.4


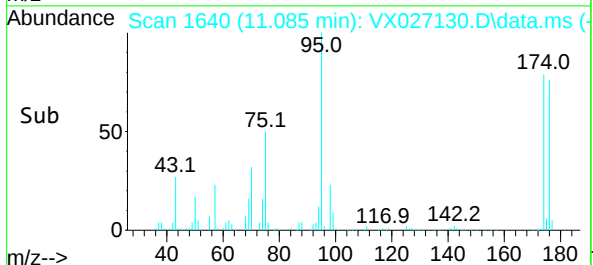
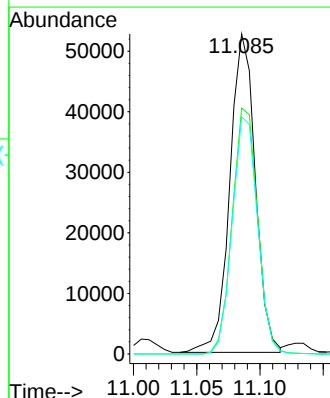
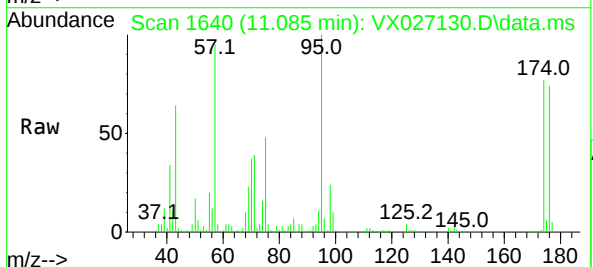




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion:117 Resp: 146698
Ion Ratio Lower Upper
117 100
82 52.4 45.2 67.8
119 32.4 26.2 39.2

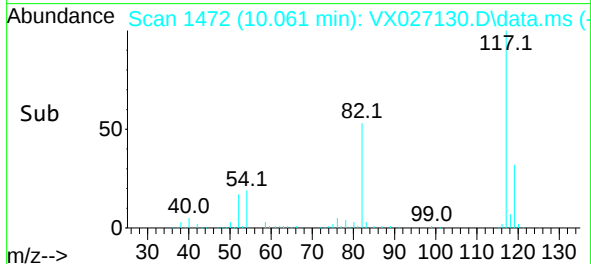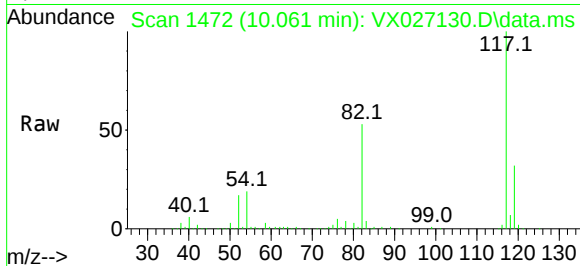

#67
Ethyl Benzene
Concen: 1.760 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion: 91 Resp: 9452
Ion Ratio Lower Upper
91 100
106 29.9 24.7 37.1


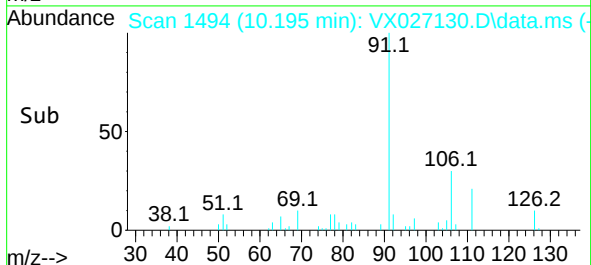
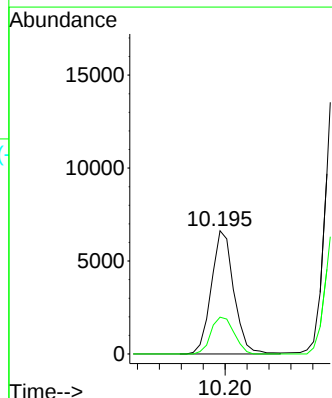
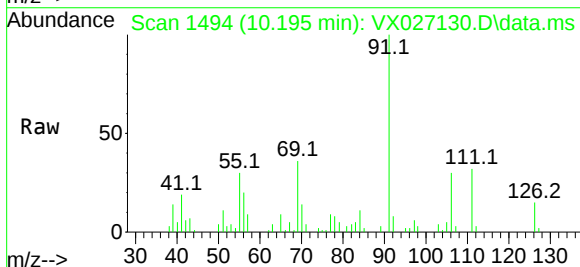




#68
m/p-Xylenes
Concen: 6.562 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion:106 Resp: 13556
Ion Ratio Lower Upper
106 100
91 203.1 165.3 247.9

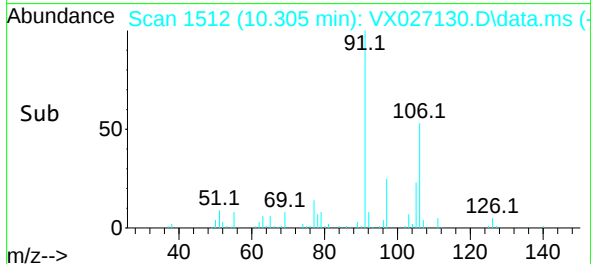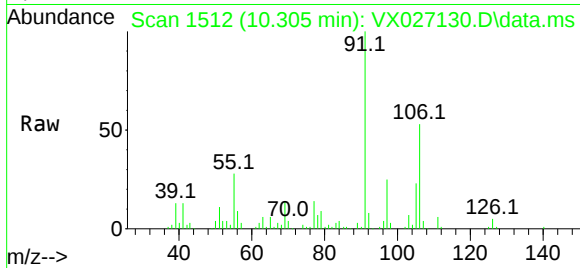

#69
o-Xylene
Concen: 5.546 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion:106 Resp: 11228
Ion Ratio Lower Upper
106 100
91 216.2 109.7 329.0




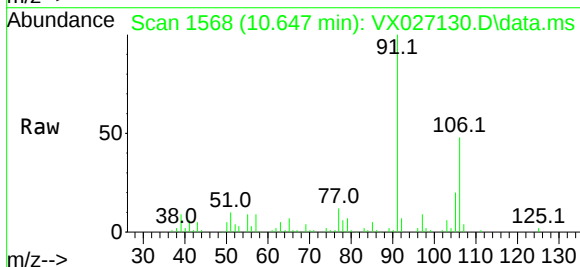




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion:152 Resp: 72973
Ion Ratio Lower Upper
152 100
115 61.3 44.2 132.6
150 155.4 0.0 348.2

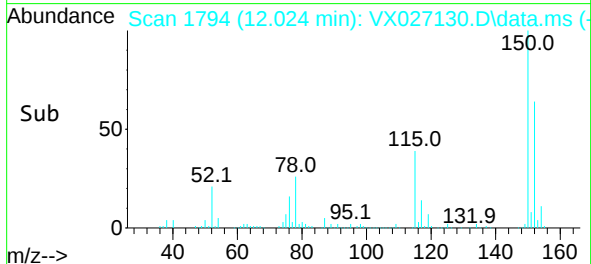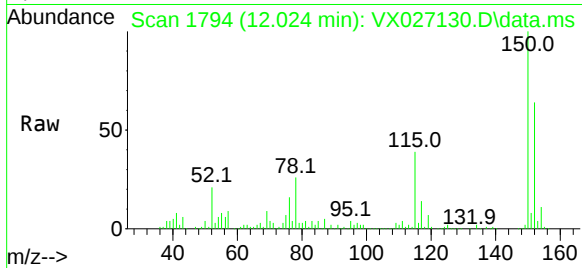

#73
Isopropylbenzene
Concen: 1.759 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion:105 Resp: 10112
Ion Ratio Lower Upper
105 100
120 26.5 13.1 39.1




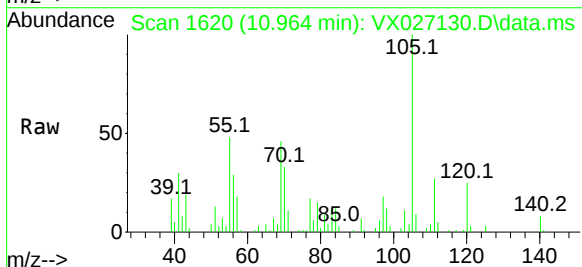




#74
N-amy1 acetate
Concen: 5.579 ug/l
RT: 10.860 min Scan# 1603
Delta R.T. 0.012 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion: 43	Resp: 12814
Ion Ratio	Lower Upper
43	100
70	112.0 32.9 49.3#
55	394.6 18.3 27.5#
61	0.0 18.9 28.3#

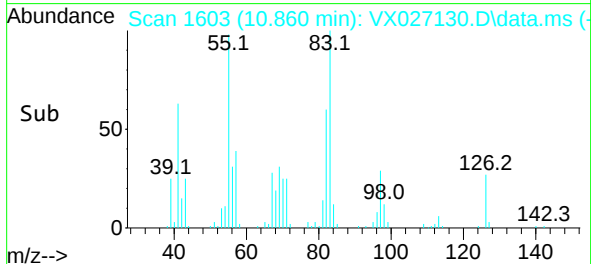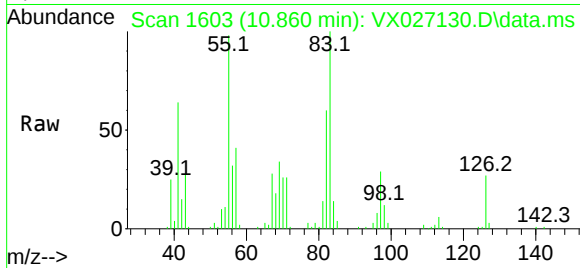

#75
1,1,2,2-Tetrachloroethane
Concen: 6.515 ug/l
RT: 11.220 min Scan# 1662
Delta R.T. 0.006 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion: 83	Resp: 10162
Ion Ratio	Lower Upper
83	100
131	0.0 5.3 15.9#
85	0.0 32.0 96.2#




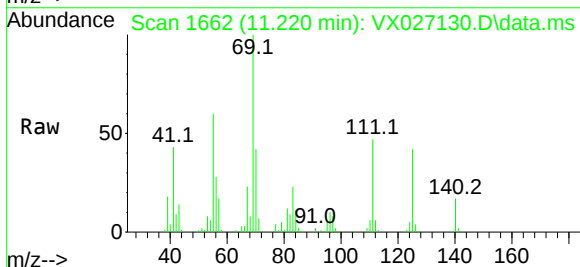




#76
1,2,3-Trichloropropane
Concen: 0.868 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.140 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion: 75 Resp: 1386
Ion Ratio Lower Upper
75 100
77 1415.7 18.3 54.8#

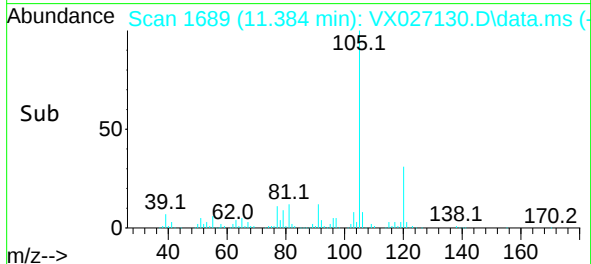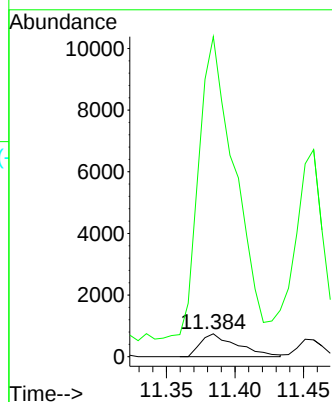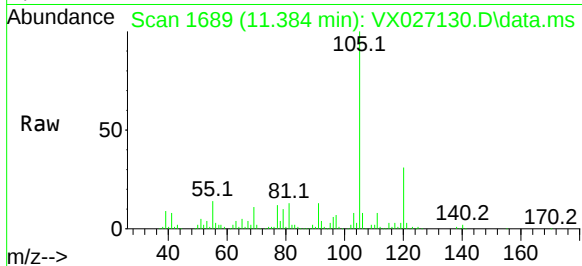

#78
n-propylbenzene
Concen: 6.463 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion: 91 Resp: 41181
Ion Ratio Lower Upper
91 100
120 23.4 11.6 34.7



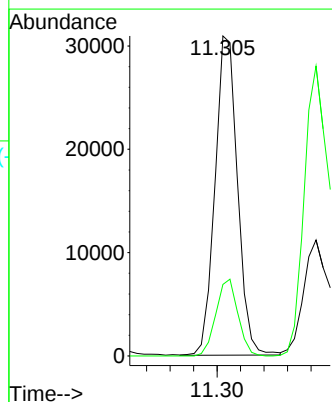
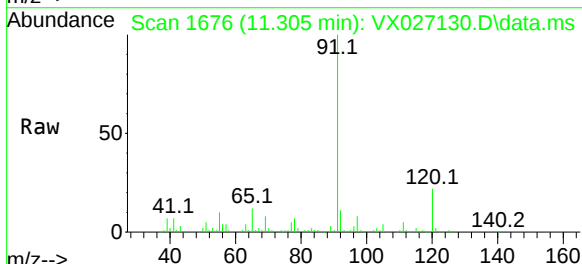




#79
2-Chlorotoluene
Concen: 5.091 ug/l
RT: 11.384 min Scan# 1
Delta R.T. 0.018 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion: 91 Resp: 20046
Ion Ratio Lower Upper
91 100
126 1.5 16.4 49.2#

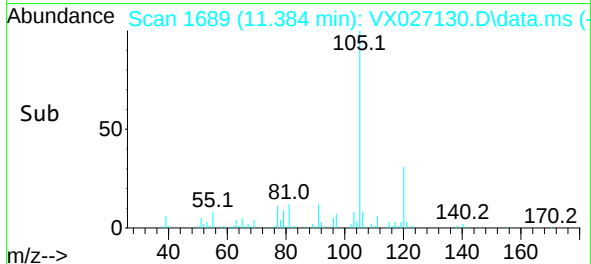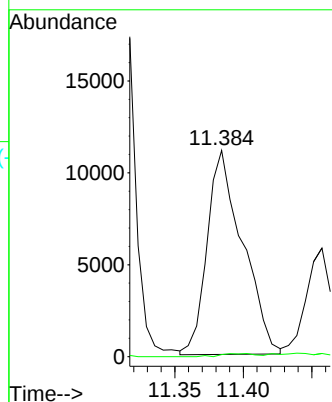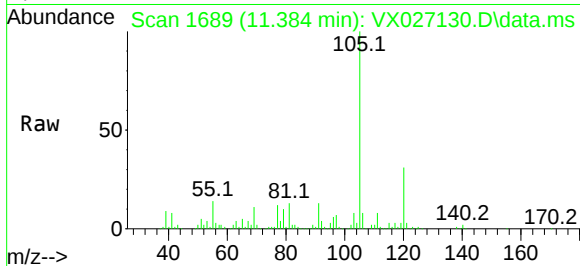

#80
1,3,5-Trimethylbenzene
Concen: 13.590 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion: 105 Resp: 64289
Ion Ratio Lower Upper
105 100
120 50.5 24.0 72.0


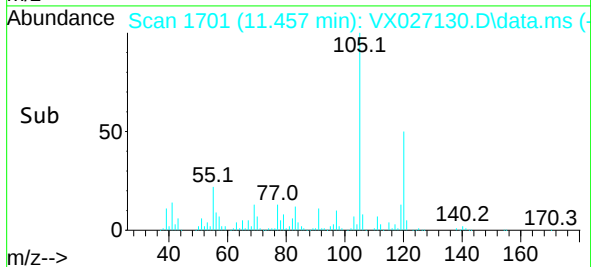
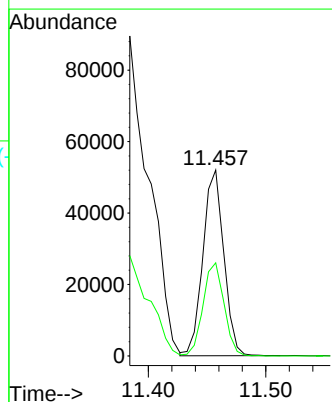
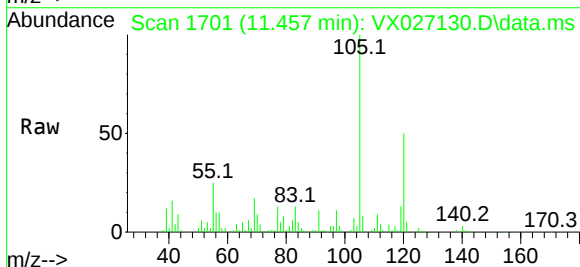




#81
trans-1,4-Dichloro-2-butene
Concen: 66.384 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.067 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion: 75 Resp: 34525
Ion Ratio Lower Upper
75 100
53 6.4 94.0 141.0#
89 0.0 37.0 55.4#

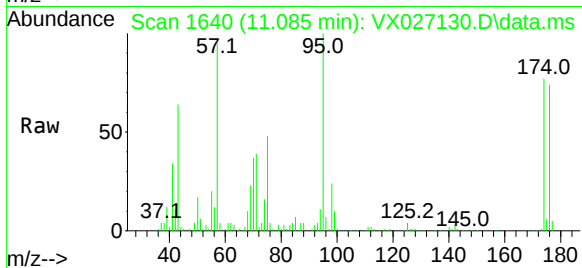

#82
4-Chlorotoluene
Concen: 1.716 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion: 91 Resp: 7581
Ion Ratio Lower Upper
91 100
126 2.9 14.1 42.4#




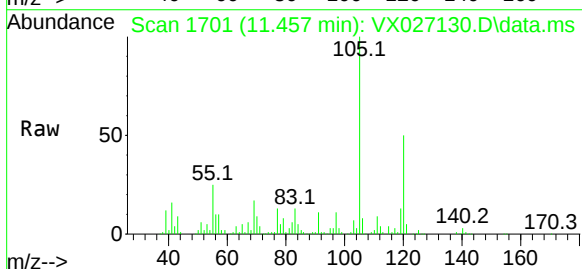




#83
tert-Butylbenzene
Concen: 5.675 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.043 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34




Instrument :
MSVOA_X
ClientSampleId :
C0AA9ME


Tgt Ion:119 Resp: 25588
Ion Ratio Lower Upper
119 100
91 89.2 31.4 94.0
134 0.0 11.8 35.3#

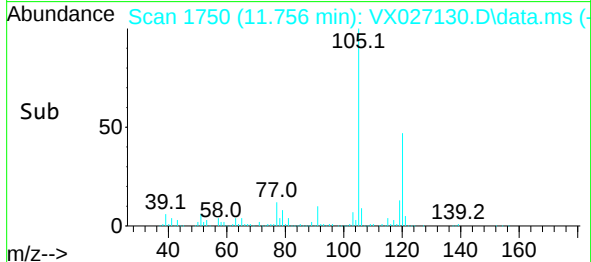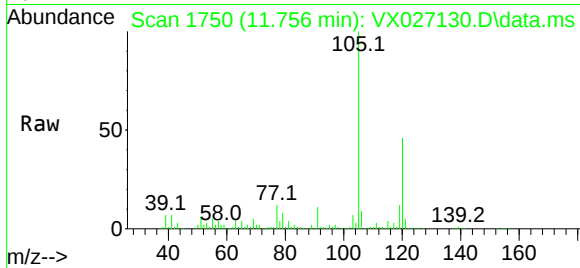

#84
1,2,4-Trimethylbenzene
Concen: 42.741 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX027130.D
Acq: 22 Feb 2022 13:34

Tgt Ion:105 Resp: 203944
Ion Ratio Lower Upper
105 100
120 45.7 21.9 65.5


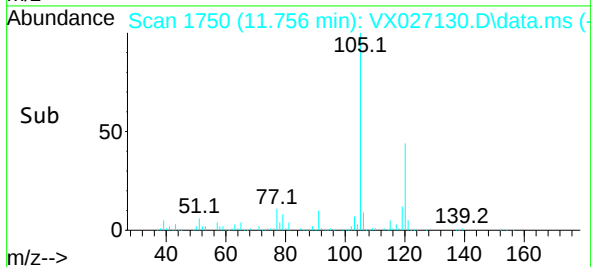

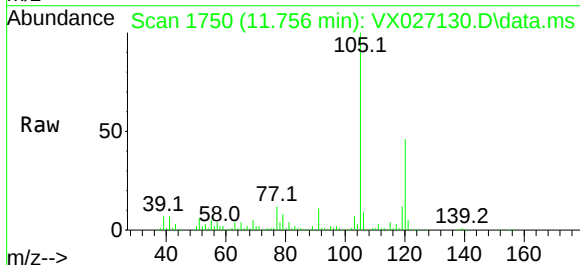




#85
 sec-Butylbenzene
 Concen: 6.291 ug/l
 RT: 11.896 min Scan# 1773
 Delta R.T. 0.006 min
 Lab File: VX027130.D
 Acq: 22 Feb 2022 13:34




Instrument :
 MSVOA_X
 ClientSampleId :
 C0AA9ME


Tgt Ion:105 Resp: 35957
 Ion Ratio Lower Upper
 105 100
 134 27.7 10.1 30.1

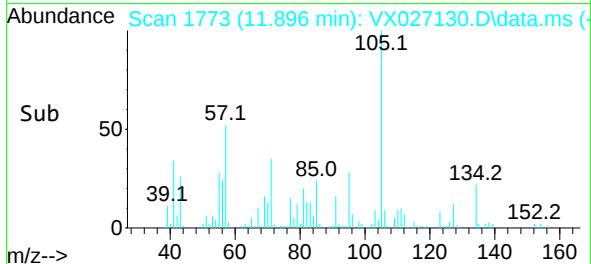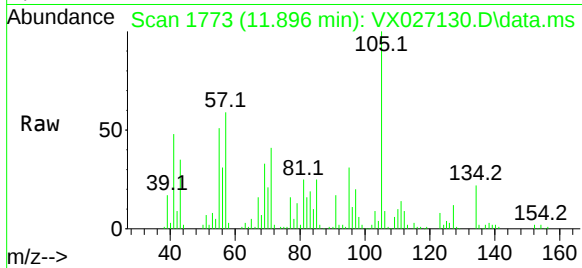

#86
 p-Isopropyltoluene
 Concen: 4.993 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.000 min
 Lab File: VX027130.D
 Acq: 22 Feb 2022 13:34

Tgt Ion:119 Resp: 24174
 Ion Ratio Lower Upper
 119 100
 134 26.5 13.0 39.0
 91 23.6 12.6 37.6

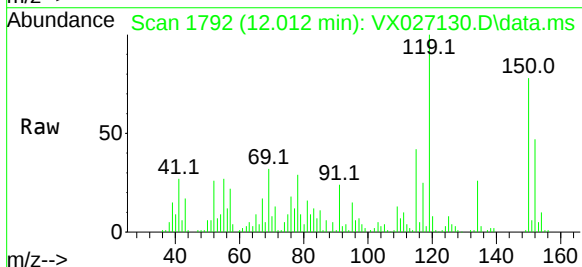



#89

n-Butylbenzene

Concen: 23.068 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34

Instrument :

MSVOA_X

ClientSampleId :

C0AA9ME





Tgt Ion: 91 Resp: 91383

Ion Ratio Lower Upper

91 100

92 39.3 27.2 81.6

134 84.4 13.1 39.1#

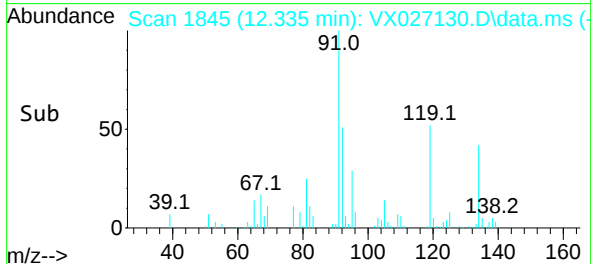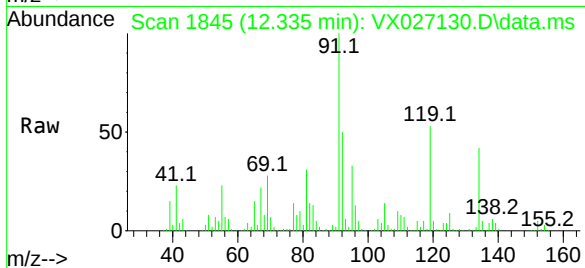

#90

Hexachloroethane

Concen: 13.927 ug/l

RT: 12.536 min Scan# 1878

Delta R.T. -0.006 min

Lab File: VX027130.D




Acq: 22 Feb 2022 13:34


Tgt Ion: 117 Resp: 9746

Ion Ratio Lower Upper

117 100

201 0.0 35.6 106.8#

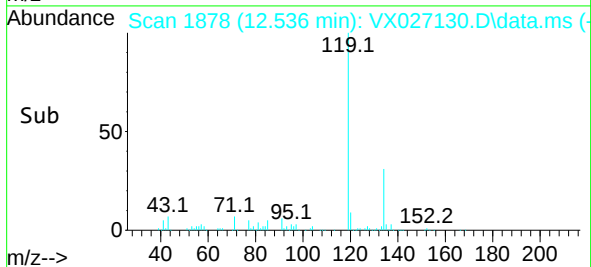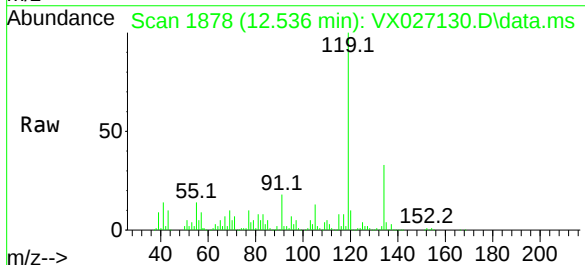



#92

1,2-Dibromo-3-Chloropropane

Concen: 2.521 ug/l

RT: 12.920 min Scan# 1941

Delta R.T. -0.024 min

Lab File: VX027130.D


Acq: 22 Feb 2022 13:34

Instrument :




MSVOA_X

ClientSampleId :

C0AA9ME

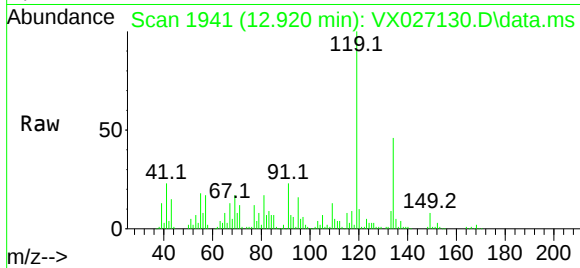

Tgt Ion:	75	Resp:	967
Ion	Ratio	Lower	Upper
75	100		
155	0.0	40.0	119.9#
157	0.0	51.6	154.8#

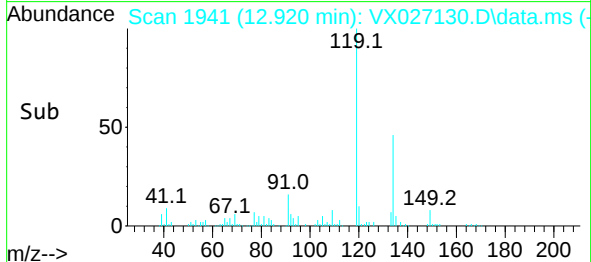

#95

Napthalene

Concen: 7.512 ug/l




RT: 13.780 min Scan# 2082


Delta R.T. 0.000 min

Lab File: VX027130.D

Acq: 22 Feb 2022 13:34


Tgt Ion:	128	Resp:	40118
Ion	Ratio	Lower	Upper
128	100		
127	14.6	10.3	15.5
129	20.7	8.7	13.1#

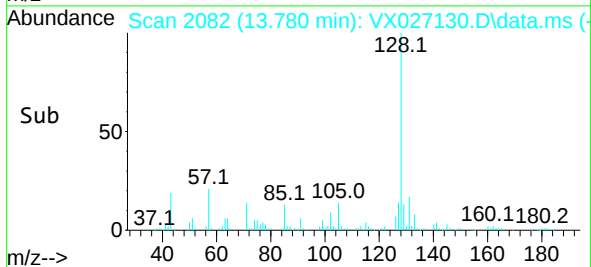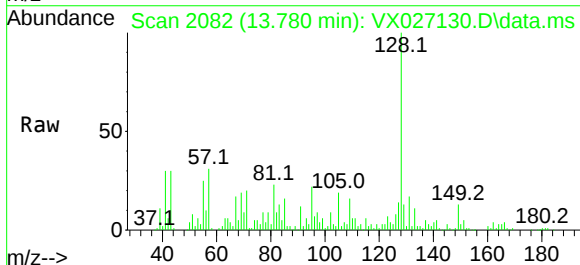



#96
 1,2,3-Trichlorobenzene
 Concen: 2.091 ug/l
 RT: 13.975 min Scan# 2114
 Delta R.T. 0.012 min
 Lab File: VX027130.D
 Acq: 22 Feb 2022 13:34

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AA9ME



Tgt Ion:180 Resp: 3228
 Ion Ratio Lower Upper
 180 100
 182 18.2 47.2 141.6#
 145 843.2 17.5 52.5#

