

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022223\
 Data File : VX034219.D
 Acq On : 22 Feb 2023 11:02
 Operator : JC/MD
 Sample : VX0222MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0222MBL01

Quant Time: Feb 23 01:26:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 17 12:33:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	297796	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	494348	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	432469	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	188720	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	177111	44.161	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	88.320%
35) Dibromofluoromethane	5.379	113	154837	48.106	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.220%
50) Toluene-d8	8.647	98	589013	50.970	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	101.940%
62) 4-Bromofluorobenzene	11.079	95	197595	44.702	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022223\
Data File : VX034219.D
Acq On : 22 Feb 2023 11:02
Operator : JC/MD
Sample : VX0222MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0222MBL01

Quant Time: Feb 23 01:26:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 17 12:33:35 2023
Response via : Initial Calibration




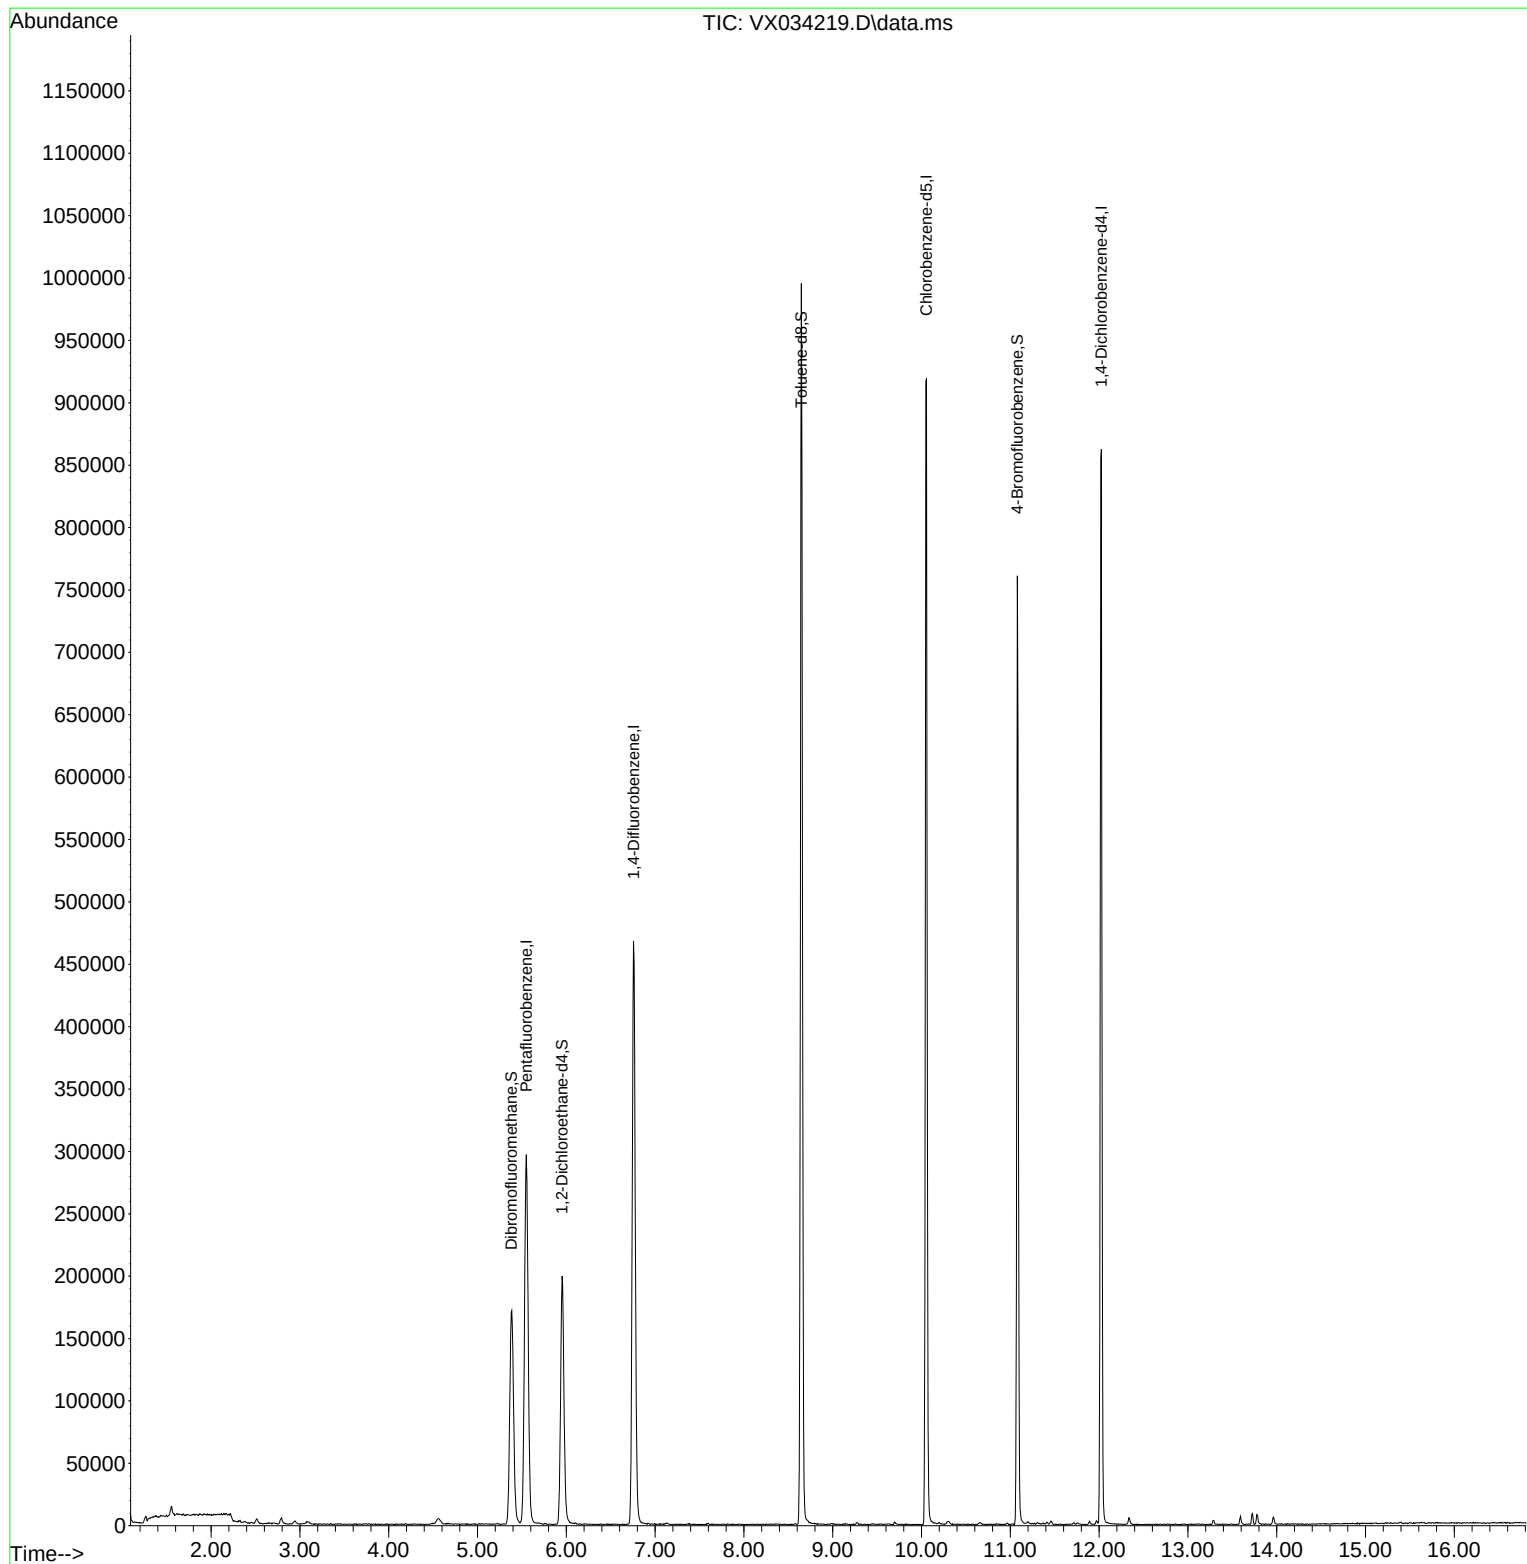


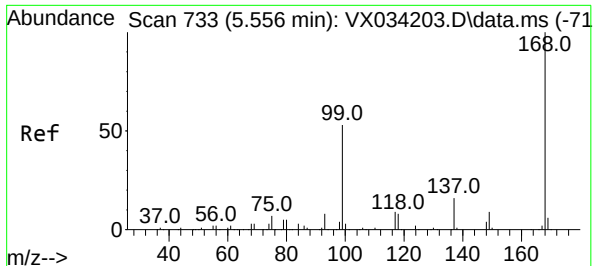

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX034219.D
Acq: 22 Feb 2023 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0222MBL01


Tgt Ion:168 Resp: 297796
Ion Ratio Lower Upper
168 100
99 55.5 39.6 59.4

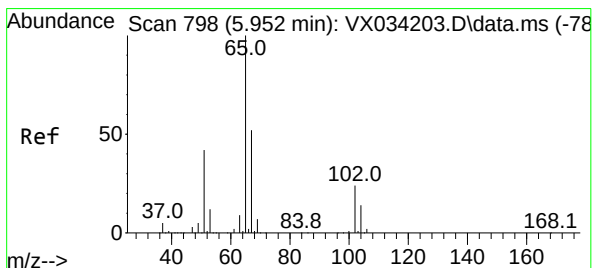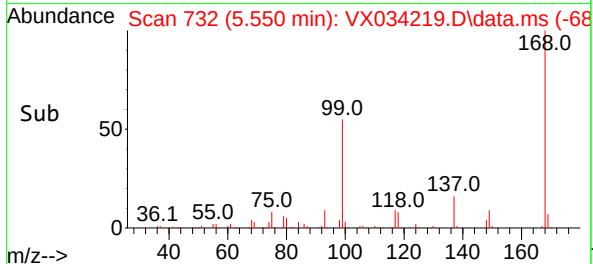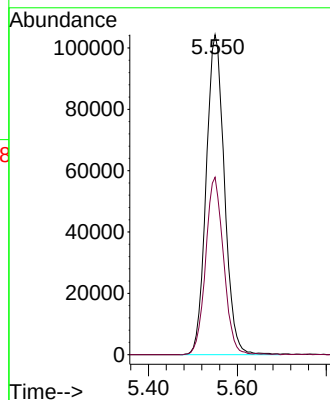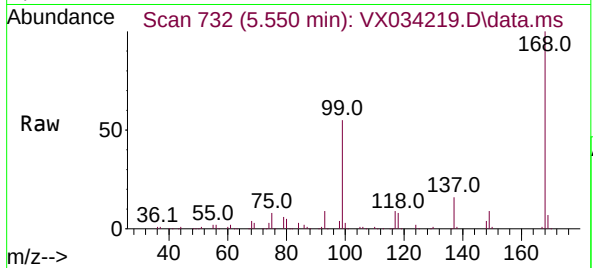

#33
1,2-Dichloroethane-d4
Concen: 44.161 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX034219.D
Acq: 22 Feb 2023 11:02

Tgt Ion: 65 Resp: 177111
Ion Ratio Lower Upper
65 100
67 53.4 0.0 104.8


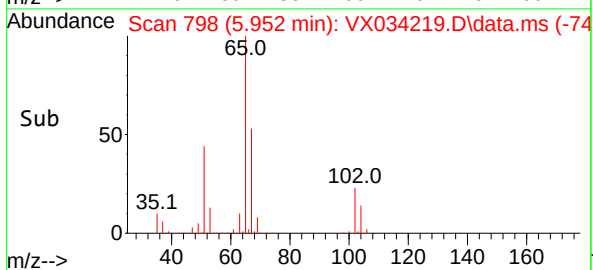
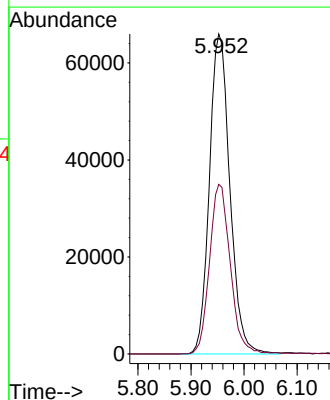
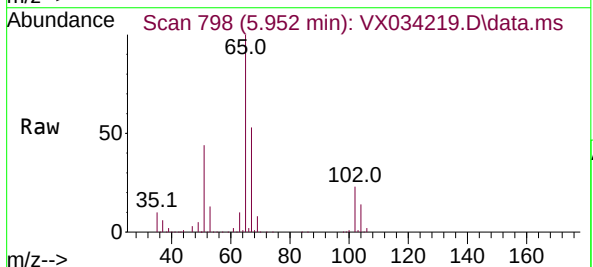


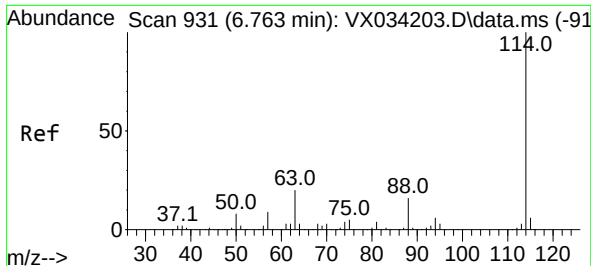

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX034219.D
Acq: 22 Feb 2023 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0222MBL01


Tgt Ion:114 Resp: 494348
Ion Ratio Lower Upper
114 100
63 19.9 0.0 37.4
88 15.8 0.0 30.6

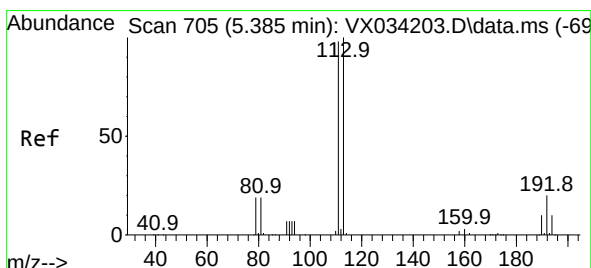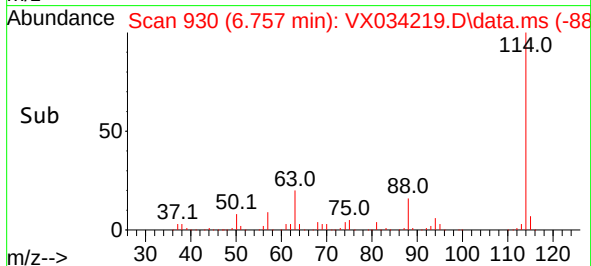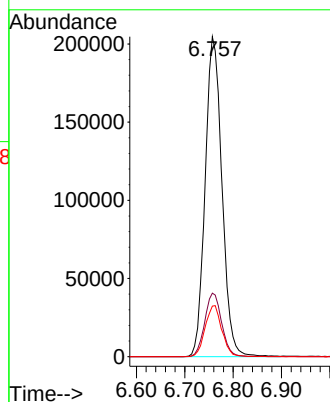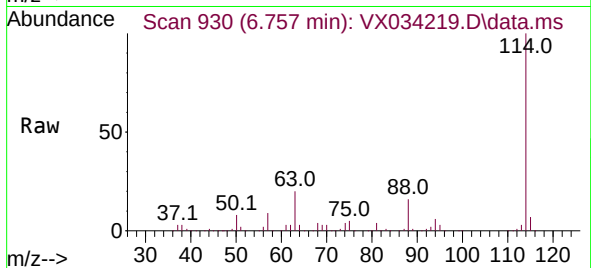

#35
Dibromofluoromethane
Concen: 48.106 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX034219.D
Acq: 22 Feb 2023 11:02

Tgt Ion:113 Resp: 154837
Ion Ratio Lower Upper
113 100
111 103.3 83.0 124.6
192 20.2 19.0 28.4


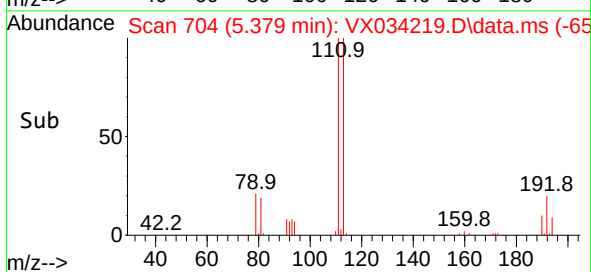
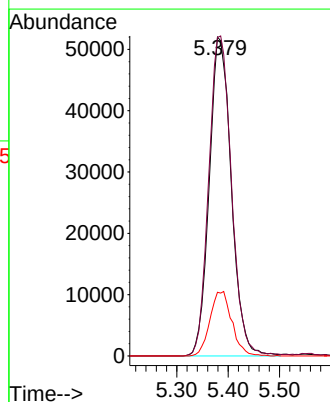
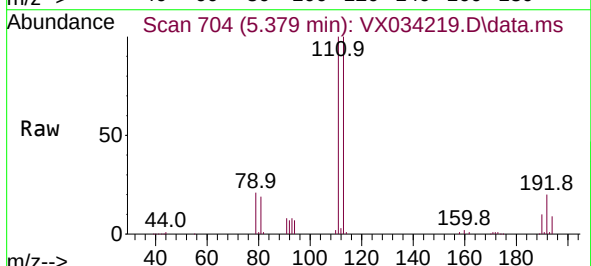


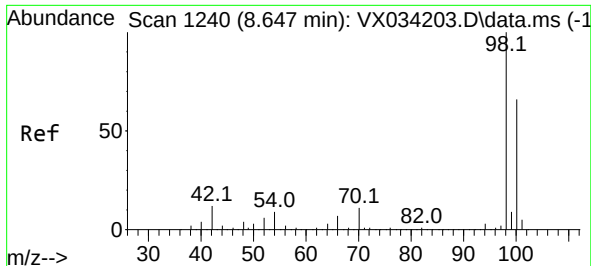

#50
Toluene-d8
Concen: 50.970 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034219.D
Acq: 22 Feb 2023 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0222MBL01


Tgt Ion: 98 Resp: 589013
Ion Ratio Lower Upper
98 100
100 66.0 53.6 80.4

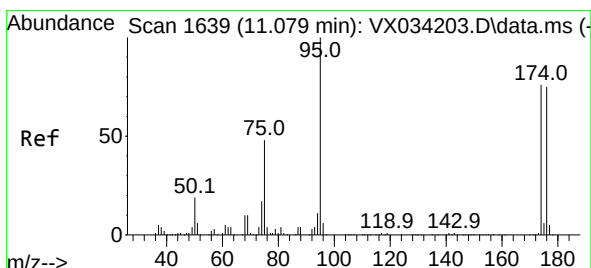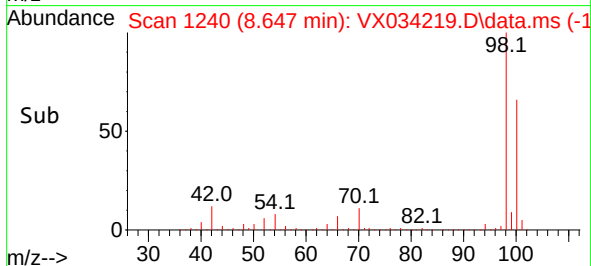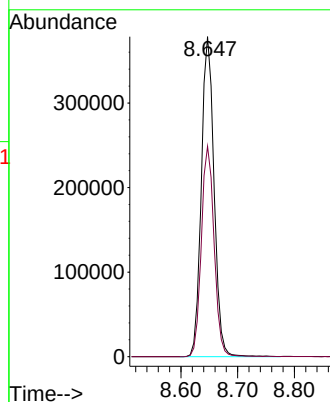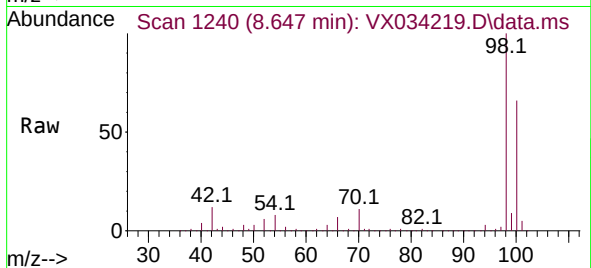

#62
4-Bromofluorobenzene
Concen: 44.702 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX034219.D
Acq: 22 Feb 2023 11:02

Tgt Ion: 95 Resp: 197595
Ion Ratio Lower Upper
95 100
174 81.5 0.0 184.4
176 78.8 0.0 178.8


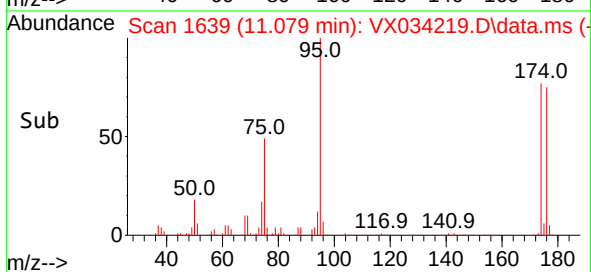
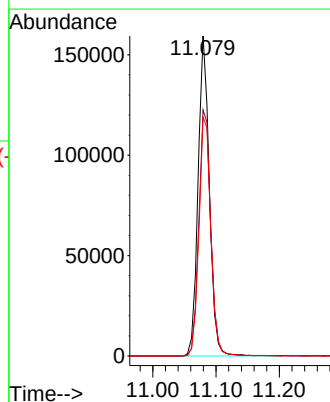
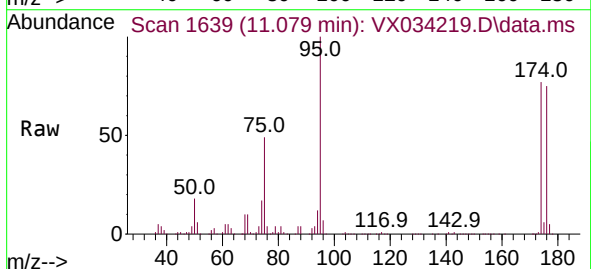


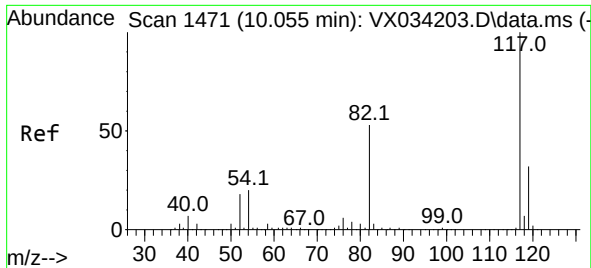

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034219.D
Acq: 22 Feb 2023 11:02

Instrument :
MSVOA_X
ClientSampleId :
VX0222MBL01

Tgt Ion:117 Resp: 432469
Ion Ratio Lower Upper
117 100
82 54.0 40.6 60.8
119 32.5 25.6 38.4

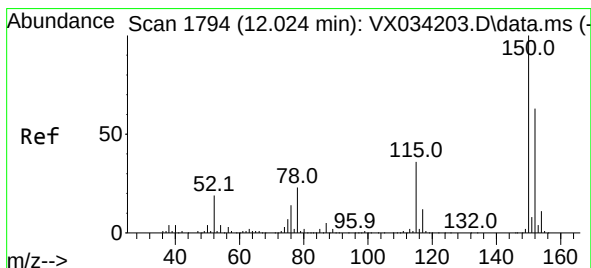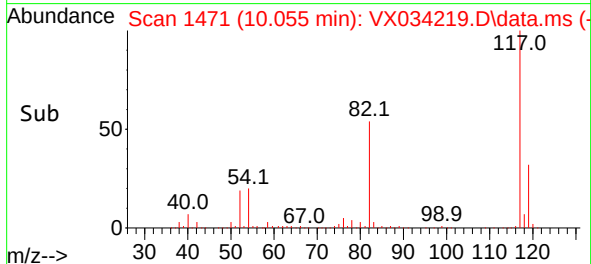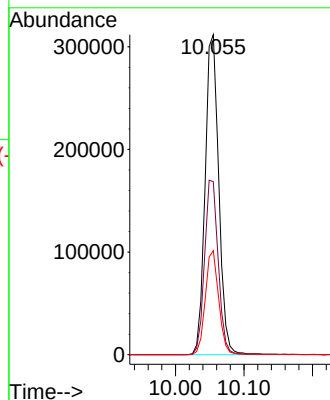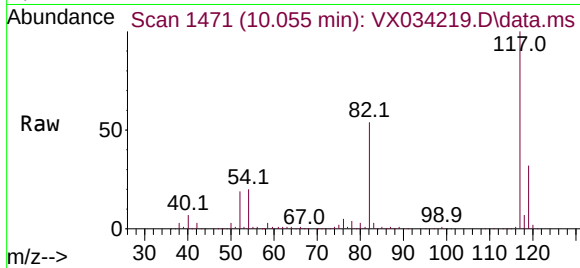

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX034219.D
Acq: 22 Feb 2023 11:02

Tgt Ion:152 Resp: 188720
Ion Ratio Lower Upper
152 100
115 58.8 38.7 116.1
150 158.3 0.0 348.2

