


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022223\
Data File : VX034217.D
Acq On : 22 Feb 2023 09:34
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Title : SW846 8260
Last Update : Fri Feb 17 12:33:35 2023

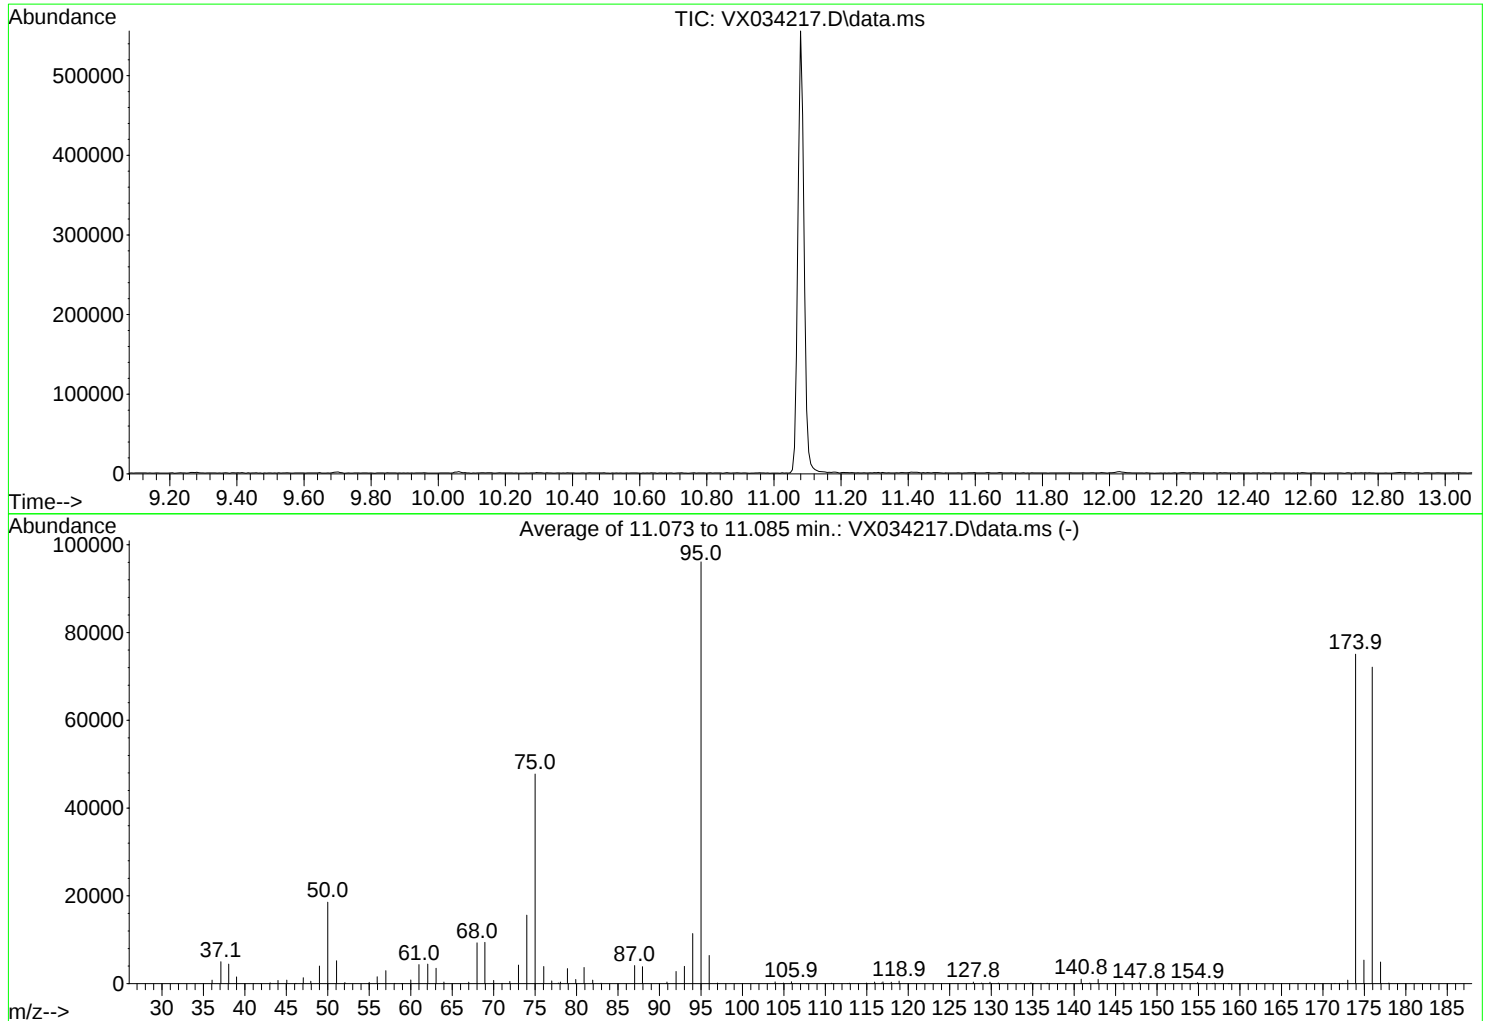

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	18553	PASS
75	95	30	60	49.7	47752	PASS
95	95	100	100	100.0	96104	PASS
96	95	5	9	6.7	6421	PASS
173	174	0.00	2	1.1	822	PASS
174	95	50	100	78.1	75080	PASS
175	174	5	9	7.2	5371	PASS
176	174	95	101	96.0	72109	PASS
177	176	5	9	6.9	4940	PASS