

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022224\
 Data File : VX040406.D
 Acq On : 22 Feb 2024 16:58
 Operator : JC/MD
 Sample : P1532-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE104D3-20240216

Quant Time: Feb 23 00:09:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 12 00:21:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	72886	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	131379	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	126641	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	61401	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	60153	55.475	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	110.940%
35) Dibromofluoromethane	5.385	113	43981	47.937	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.880%
50) Toluene-d8	8.647	98	160955	46.898	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	93.800%
62) 4-Bromofluorobenzene	11.079	95	61936	44.249	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	88.500%
Target Compounds						
					Qvalue	
16) Acetone	2.380	43	1673	3.757	ug/l #	84
44) Trichloroethene	7.129	130	895	0.903	ug/l	86
52) Toluene	8.720	92	2604	1.106	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022224\
Data File : VX040406.D
Acq On : 22 Feb 2024 16:58
Operator : JC/MD
Sample : P1532-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE104D3-20240216

Quant Time: Feb 23 00:09:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 12 00:21:14 2024
Response via : Initial Calibration




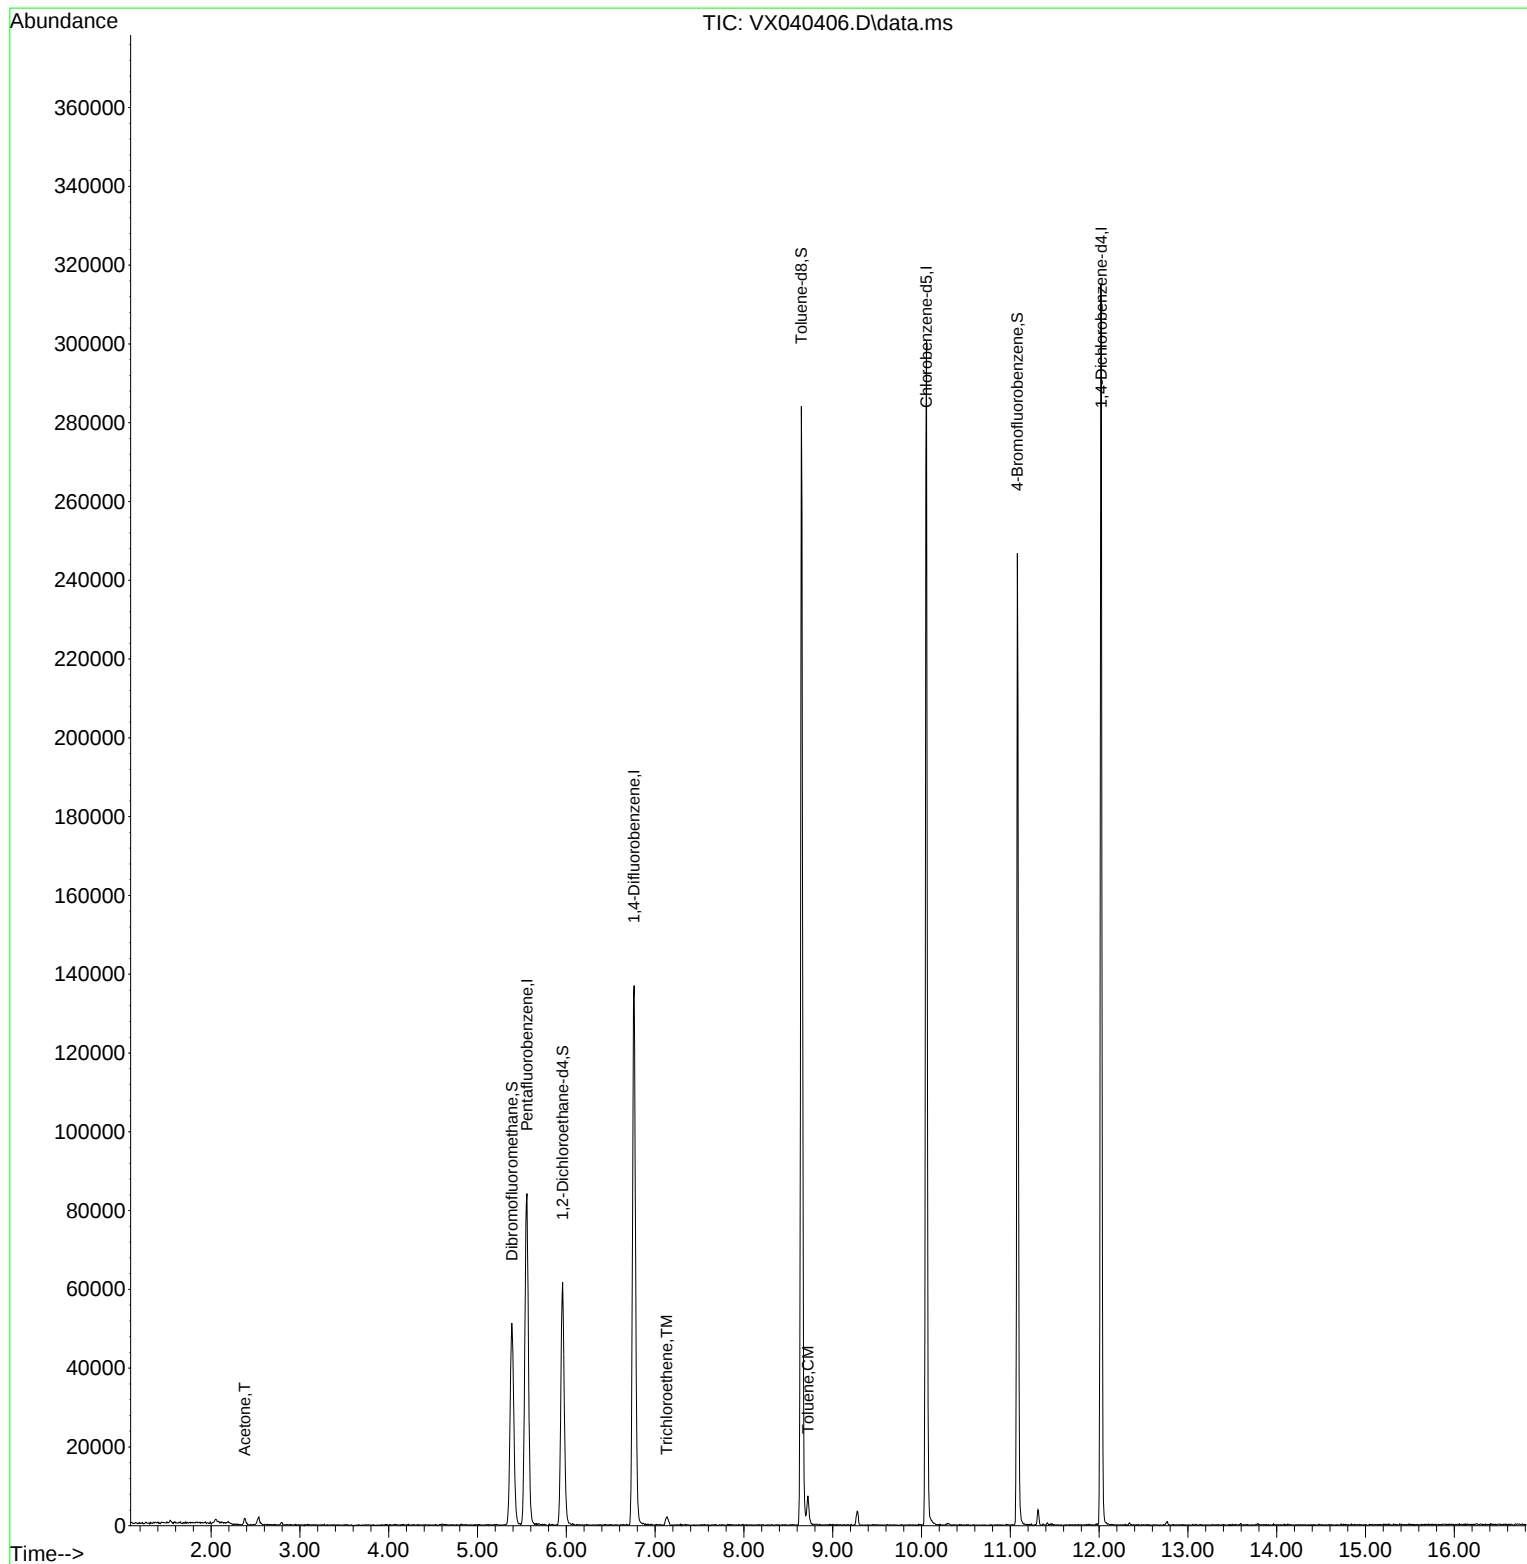


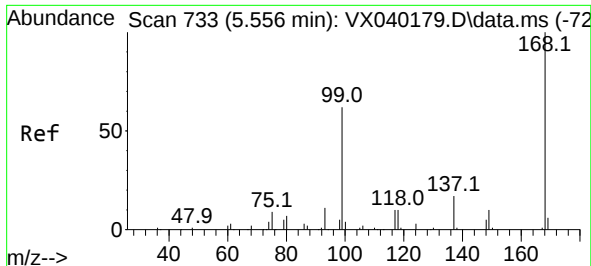

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX040406.D
Acq: 22 Feb 2024 16:58




Instrument :
MSVOA_X
ClientSampleId :
RE104D3-20240216

Tgt Ion:168 Resp: 72886
Ion Ratio Lower Upper
168 100
99 59.8 56.6 85.0

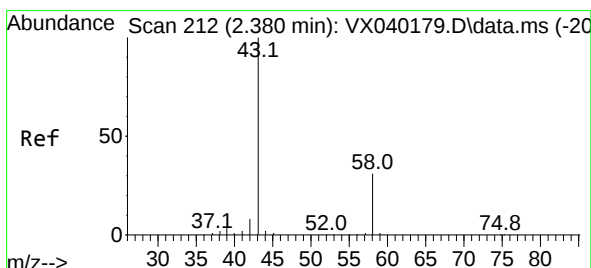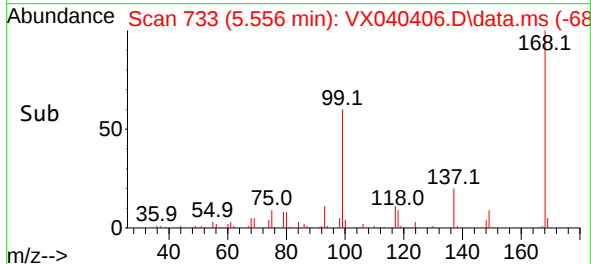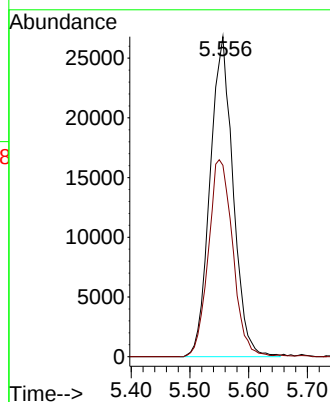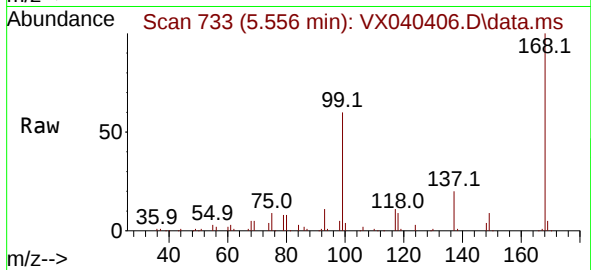

#16
Acetone
Concen: 3.757 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.000 min
Lab File: VX040406.D
Acq: 22 Feb 2024 16:58

Tgt Ion: 43 Resp: 1673
Ion Ratio Lower Upper
43 100
58 35.7 21.9 32.9#


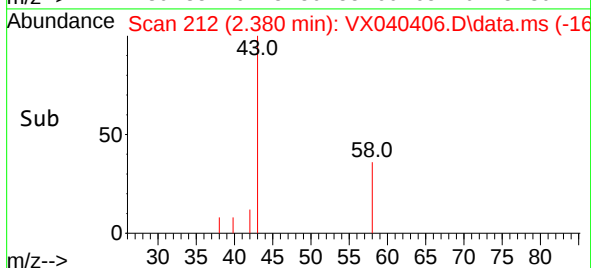
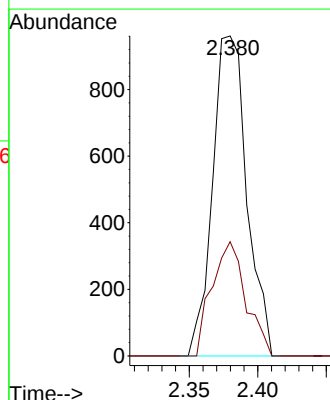
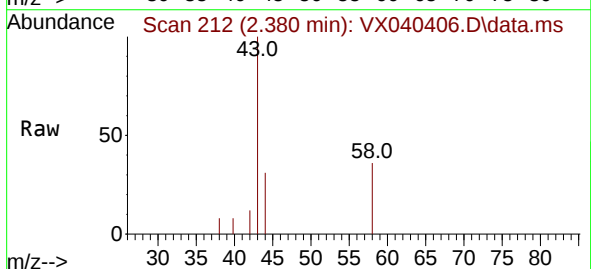




#33
1,2-Dichloroethane-d4
Concen: 55.475 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX040406.D
Acq: 22 Feb 2024 16:58




Instrument :
MSVOA_X
ClientSampleId :
RE104D3-20240216

Tgt Ion: 65 Resp: 60153
Ion Ratio Lower Upper
65 100
67 51.0 0.0 100.2

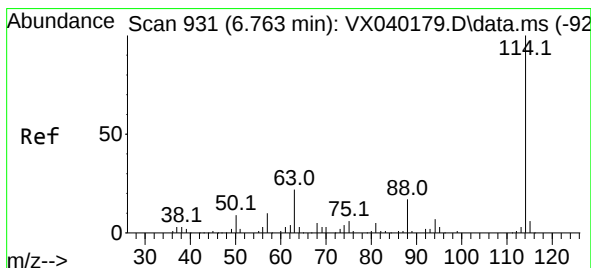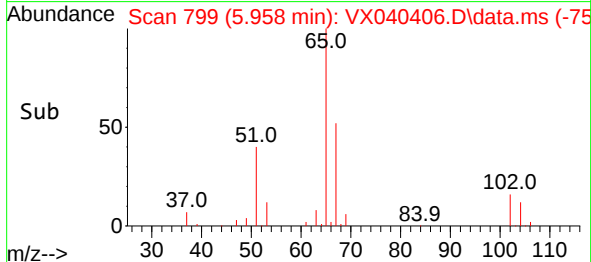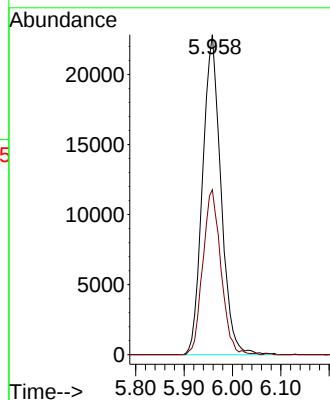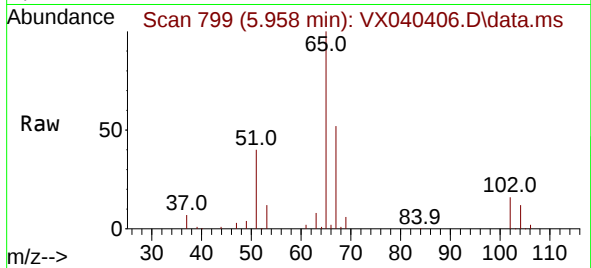

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX040406.D
Acq: 22 Feb 2024 16:58

Tgt Ion: 114 Resp: 131379
Ion Ratio Lower Upper
114 100
63 23.1 0.0 45.0
88 16.5 0.0 36.6

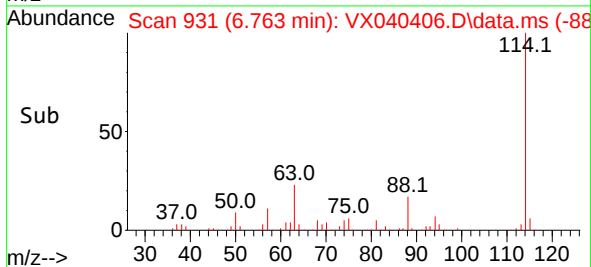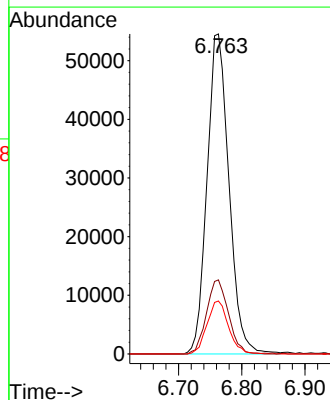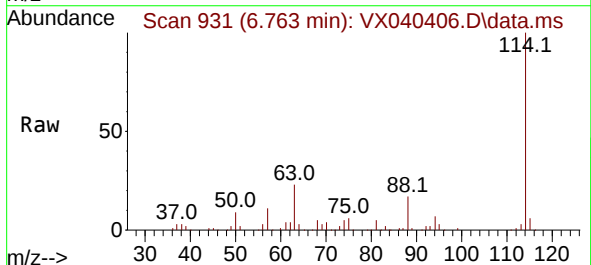



#35

Dibromofluoromethane

Concen: 47.937 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX040406.D


Acq: 22 Feb 2024 16:58

Instrument :

MSVOA_X

ClientSampleId :

RE104D3-20240216

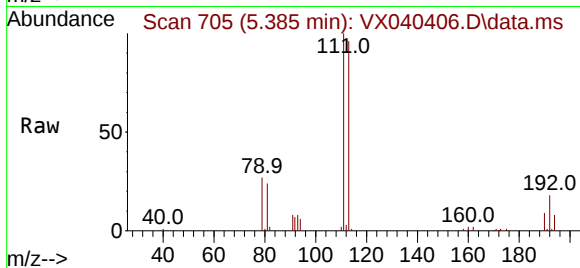




Tgt Ion:113 Resp: 43981

Ion Ratio Lower Upper

113 100

111 102.2 82.9 124.3

192 16.9 13.3 19.9

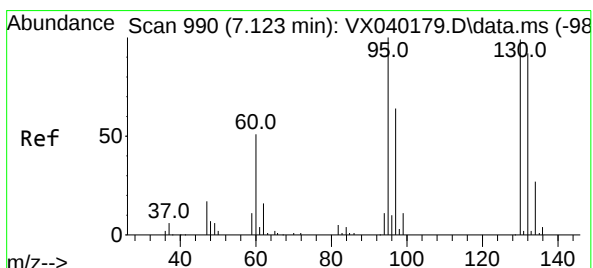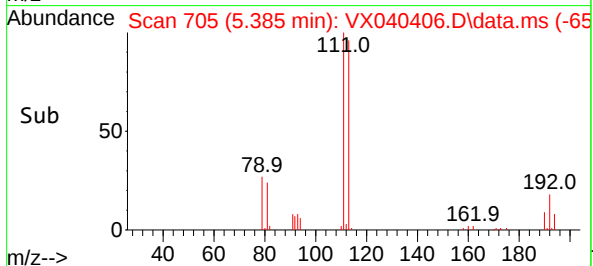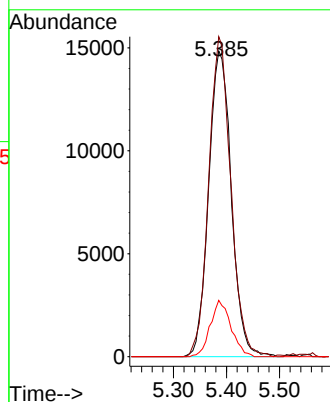

#44

Trichloroethene

Concen: 0.903 ug/l

RT: 7.129 min Scan# 991

Delta R.T. 0.000 min

Lab File: VX040406.D




Acq: 22 Feb 2024 16:58


Tgt Ion:130 Resp: 895

Ion Ratio Lower Upper

130 100

95 116.5 0.0 204.4


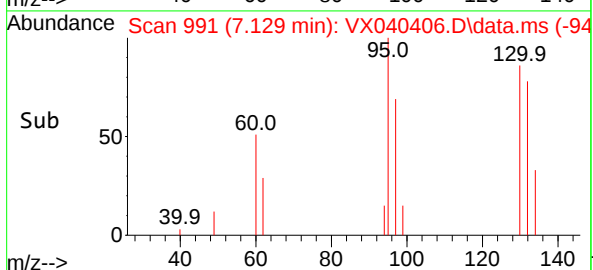
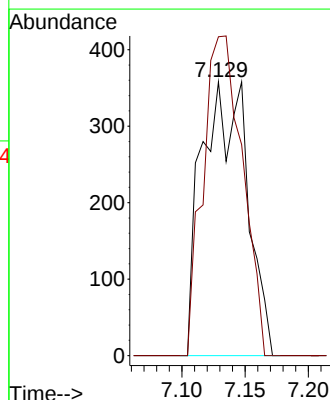
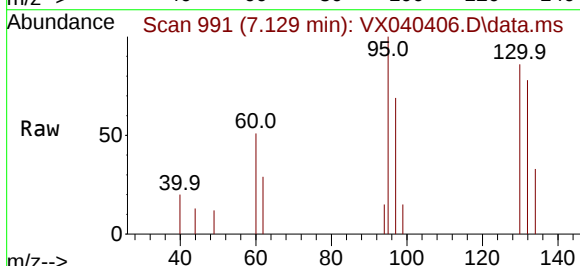


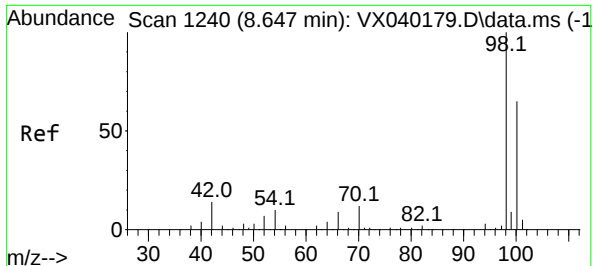

#50
Toluene-d8
Concen: 46.898 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX040406.D
Acq: 22 Feb 2024 16:58




Instrument :
MSVOA_X
ClientSampleId :
RE104D3-20240216


Tgt Ion: 98 Resp: 160955
Ion Ratio Lower Upper
98 100
100 64.8 53.1 79.7

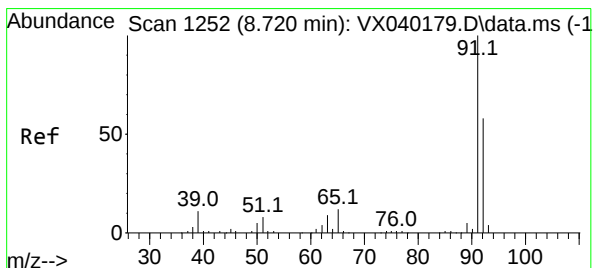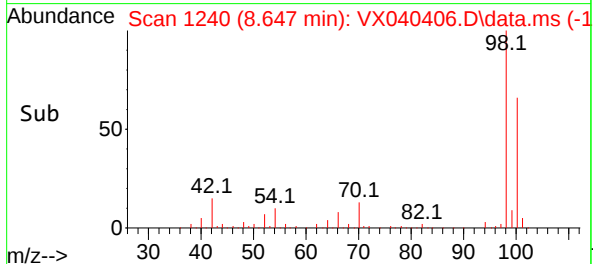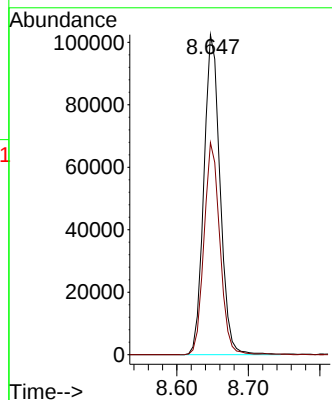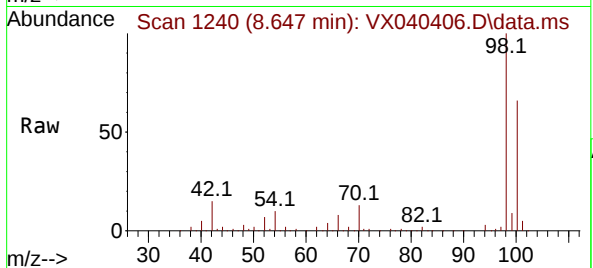

#52
Toluene
Concen: 1.106 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX040406.D
Acq: 22 Feb 2024 16:58

Tgt Ion: 92 Resp: 2604
Ion Ratio Lower Upper
92 100
91 178.3 134.2 201.2


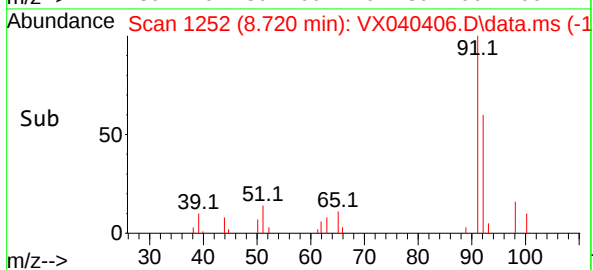
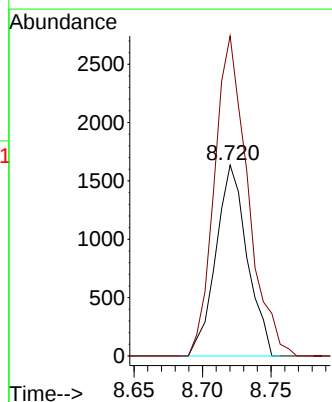
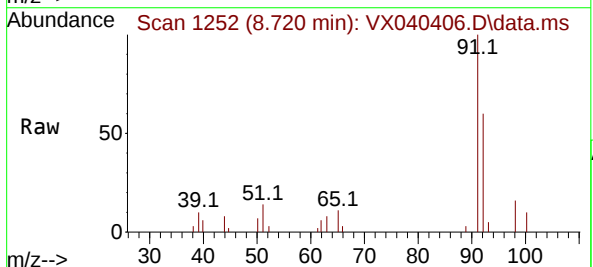


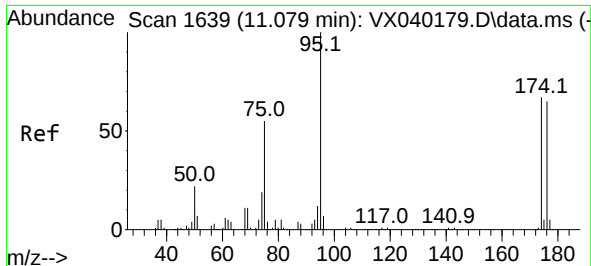

#62
4-Bromofluorobenzene
Concen: 44.249 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX040406.D
Acq: 22 Feb 2024 16:58




Instrument :
MSVOA_X
ClientSampleId :
RE104D3-20240216


Tgt Ion: 95 Resp: 61936
Ion Ratio Lower Upper
95 100
174 74.7 0.0 135.6
176 69.3 0.0 131.0

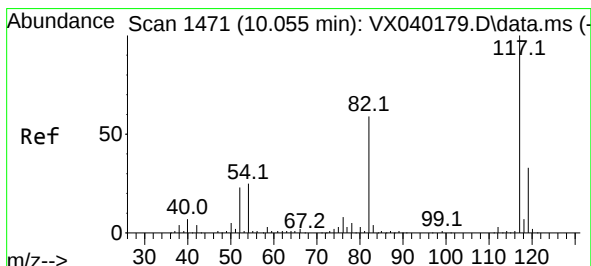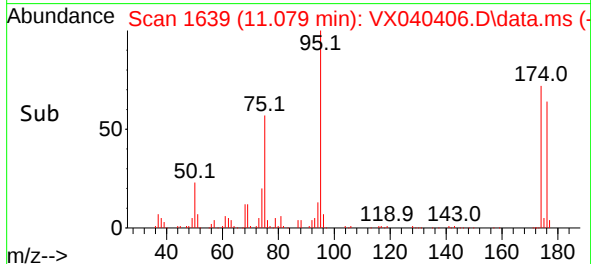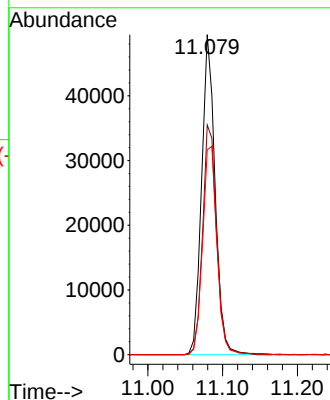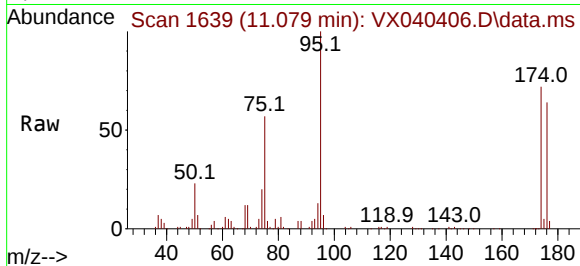

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX040406.D
Acq: 22 Feb 2024 16:58

Tgt Ion: 117 Resp: 126641
Ion Ratio Lower Upper
117 100
82 59.6 46.2 69.4
119 31.5 25.5 38.3

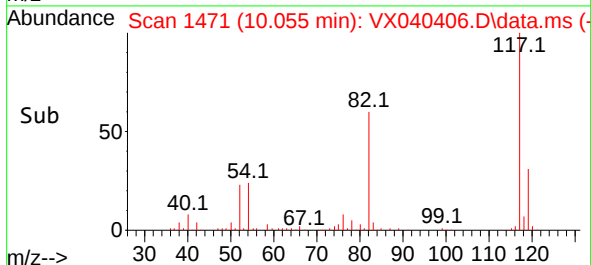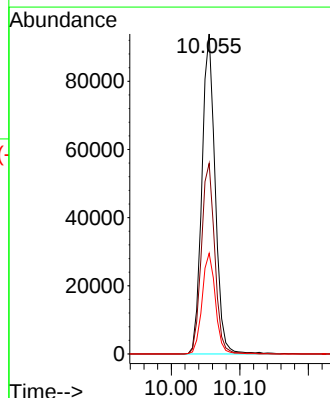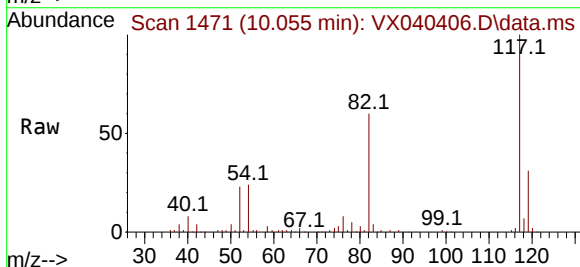

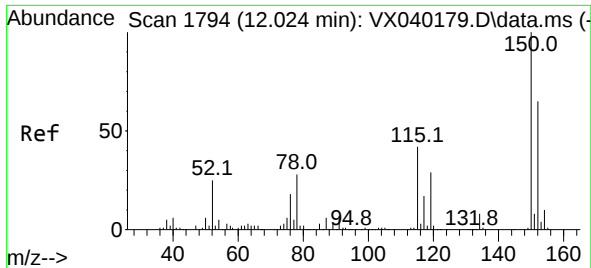

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX040406.D


Acq: 22 Feb 2024 16:58

Instrument :

MSVOA_X

ClientSampleId :

RE104D3-20240216

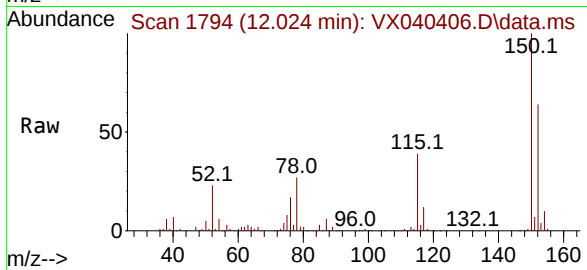

Tgt Ion:152 Resp: 61401

Ion Ratio Lower Upper

152 100

115 62.3 43.3 129.9

150 157.0 0.0 345.0

