



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022224\
Data File : VX040394.D
Acq On : 22 Feb 2024 08:50
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
Title : SW846 8260
Last Update : Mon Feb 12 00:21:14 2024

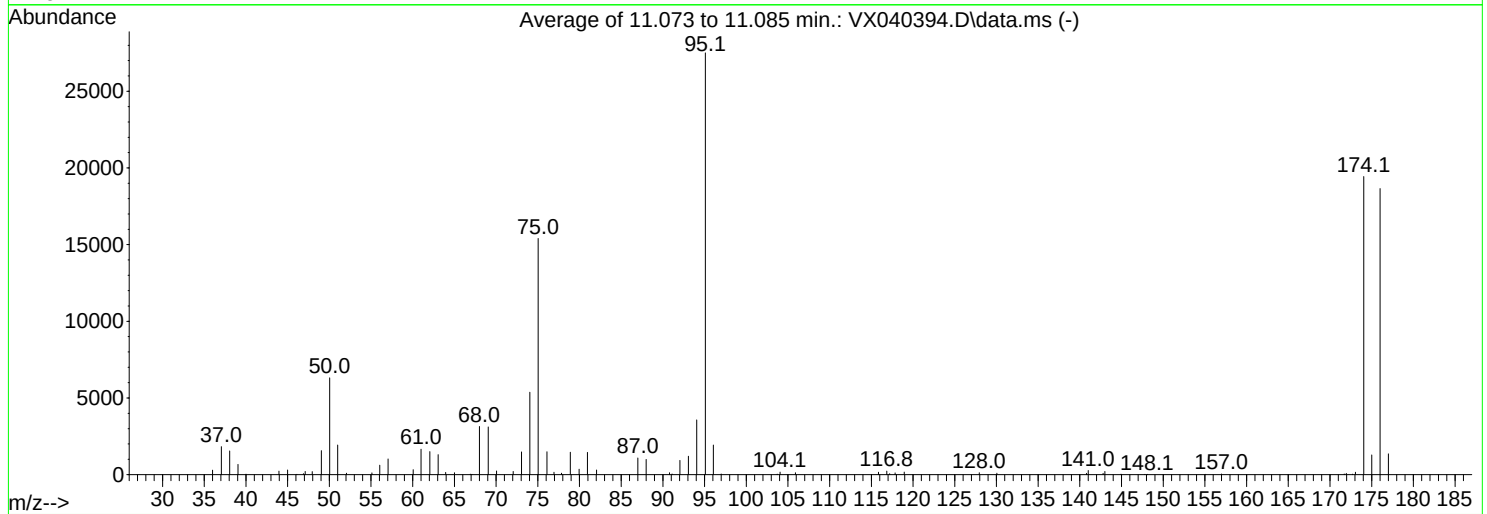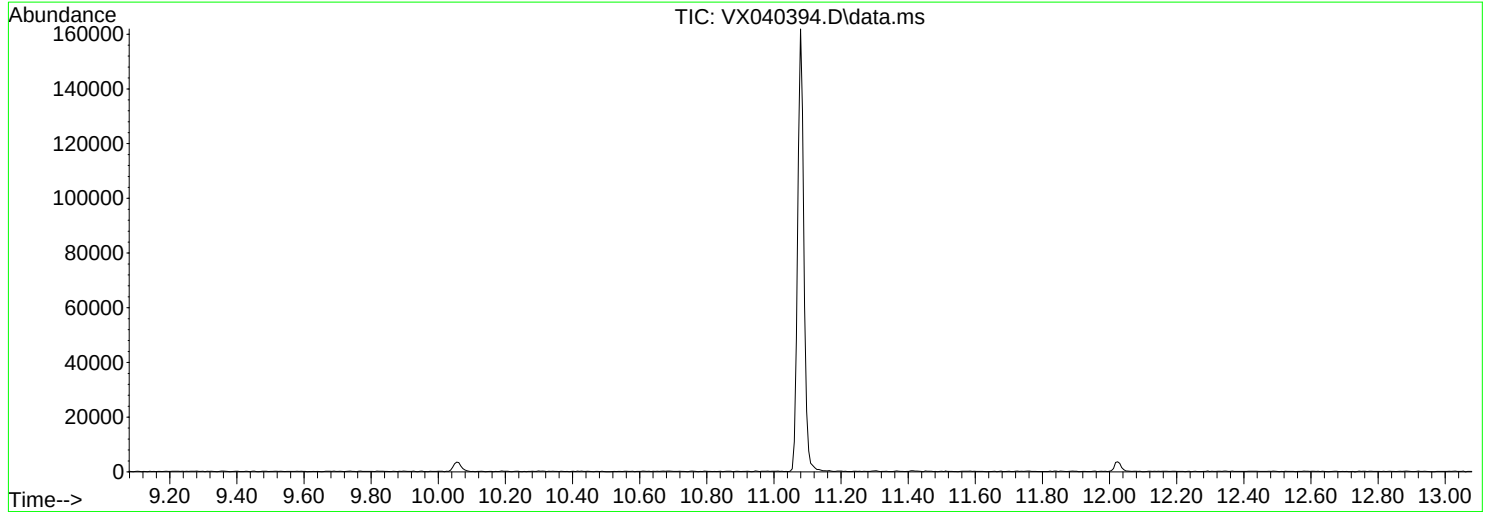

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	6308	PASS
75	95	30	60	56.0	15398	PASS
95	95	100	100	100.0	27507	PASS
96	95	5	9	7.0	1935	PASS
173	174	0.00	2	0.8	161	PASS
174	95	50	100	70.7	19438	PASS
175	174	5	9	6.6	1281	PASS
176	174	95	101	96.0	18661	PASS
177	176	5	9	7.3	1354	PASS