

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022322\
 Data File : VX027143.D
 Acq On : 23 Feb 2022 14:01
 Operator : JC/MD
 Sample : VX0223MBL01
 Misc : 5.00g/10.0mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0223MBL01

Quant Time: Feb 24 03:30:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 23 13:06:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	101162	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	166195	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	150665	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	68660	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	59587	49.044	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.080%
35) Dibromofluoromethane	5.385	113	51440	49.864	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.720%
50) Toluene-d8	8.653	98	190786	49.461	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.920%
62) 4-Bromofluorobenzene	11.079	95	71609	48.364	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022322\
Data File : VX027143.D
Acq On : 23 Feb 2022 14:01
Operator : JC/MD
Sample : VX0223MBL01
Misc : 5.00g/10.0mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0223MBL01

Quant Time: Feb 24 03:30:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 23 13:06:57 2022
Response via : Initial Calibration




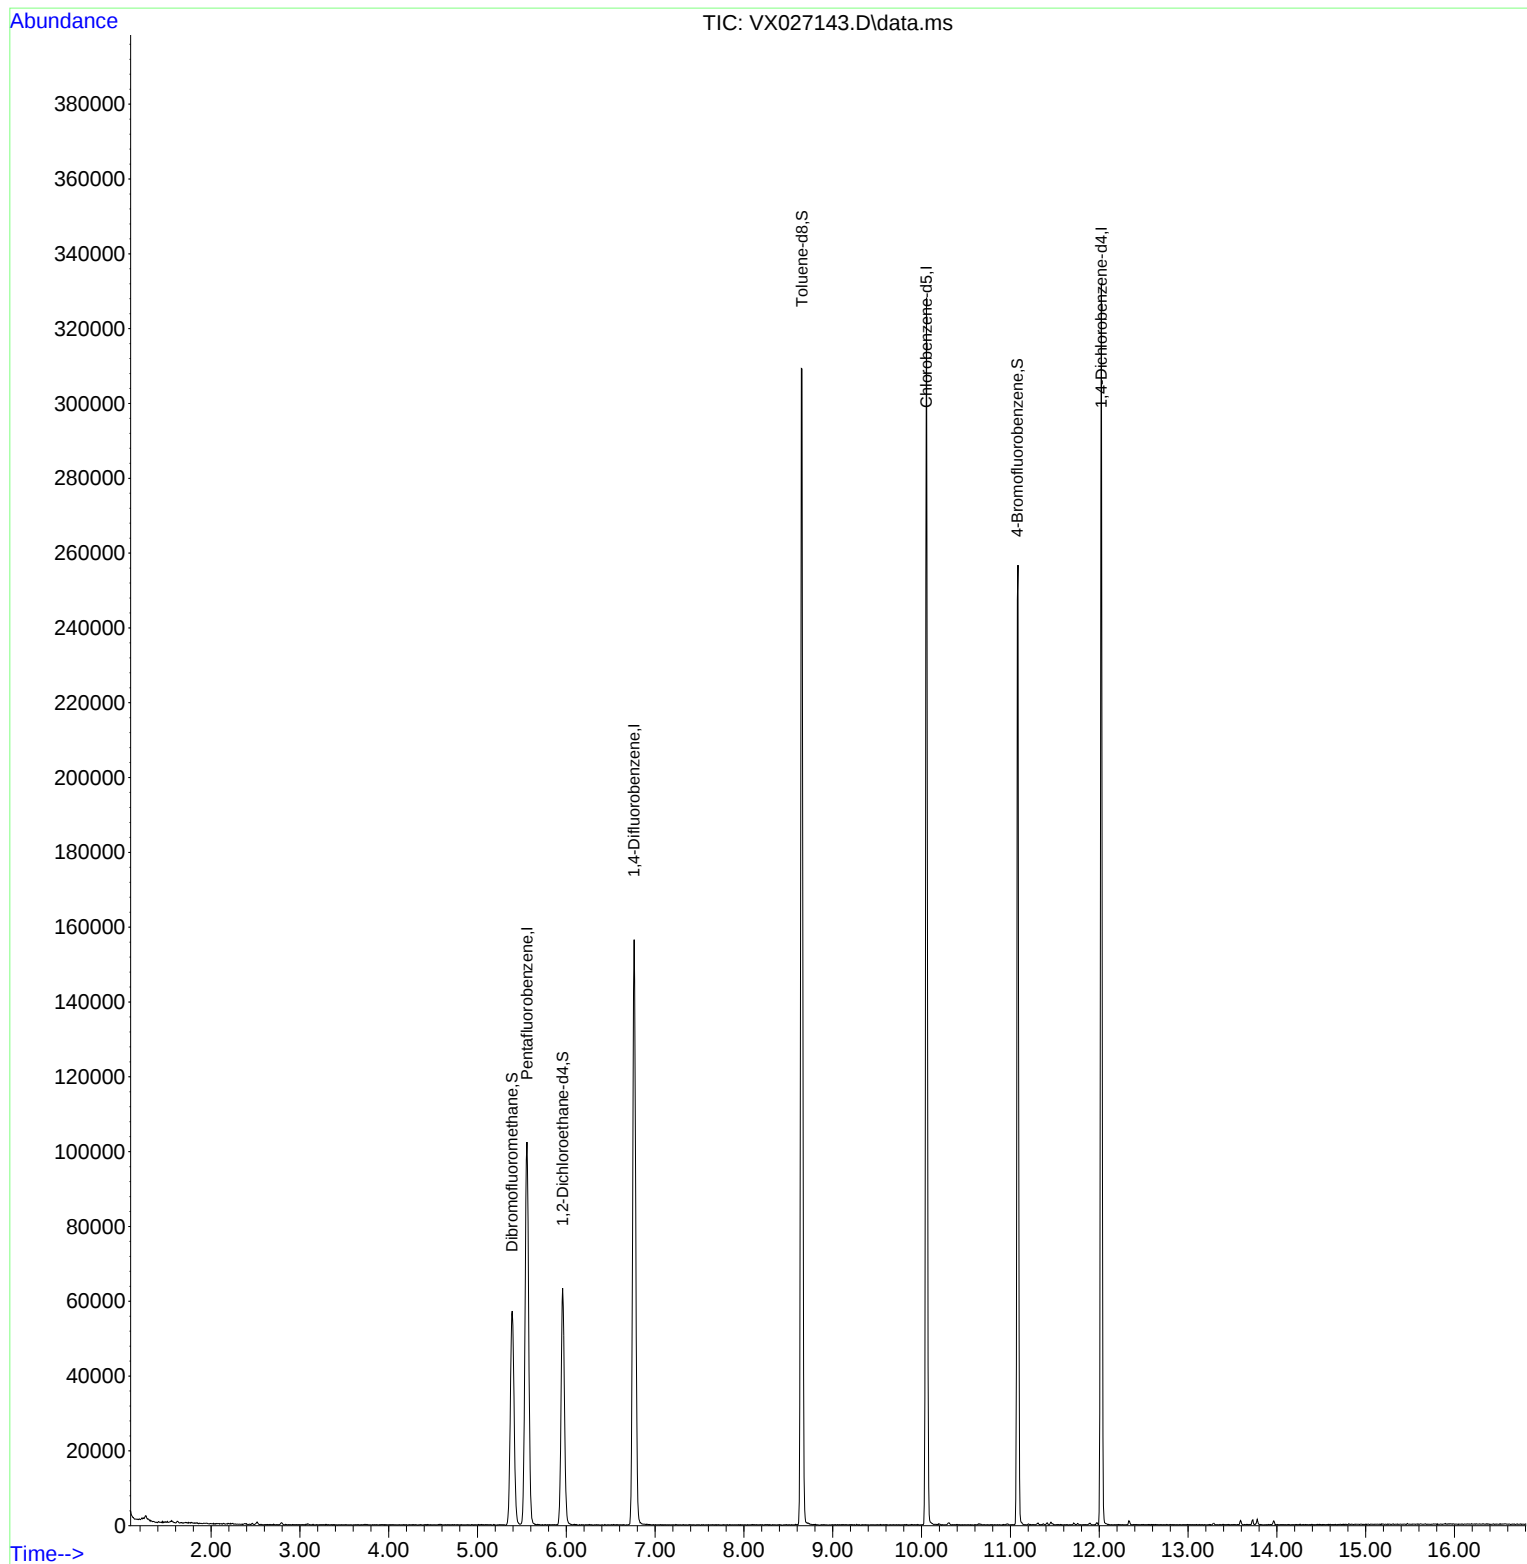


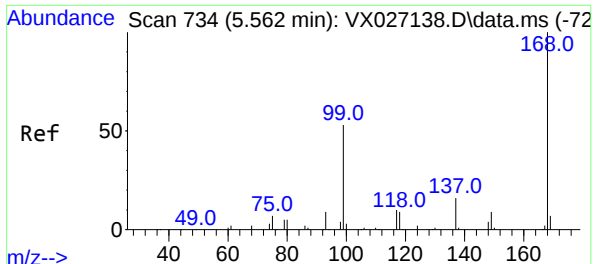

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.006 min
Lab File: VX027143.D
Acq: 23 Feb 2022 14:01




Instrument :
MSVOA_X
ClientSampleId :
VX0223MBL01


Tgt Ion:168 Resp: 101162
Ion Ratio Lower Upper
168 100
99 57.6 50.3 75.5

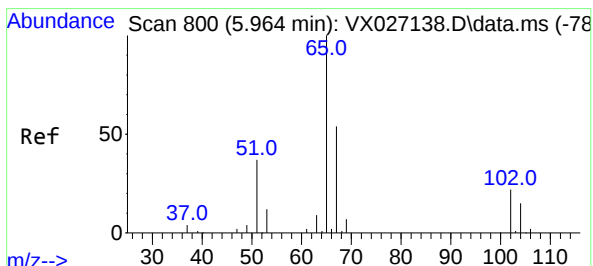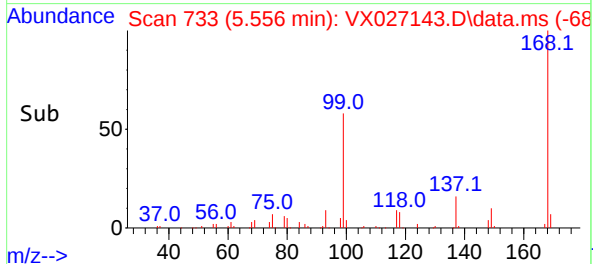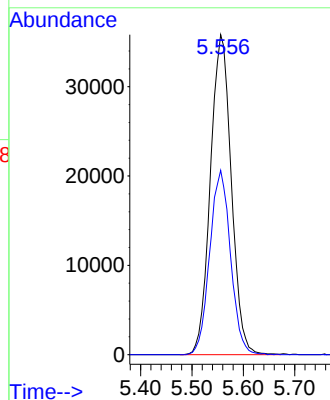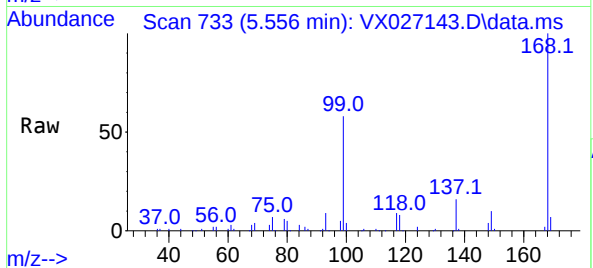

#33
1,2-Dichloroethane-d4
Concen: 49.044 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX027143.D
Acq: 23 Feb 2022 14:01

Tgt Ion: 65 Resp: 59587
Ion Ratio Lower Upper
65 100
67 51.7 0.0 100.8

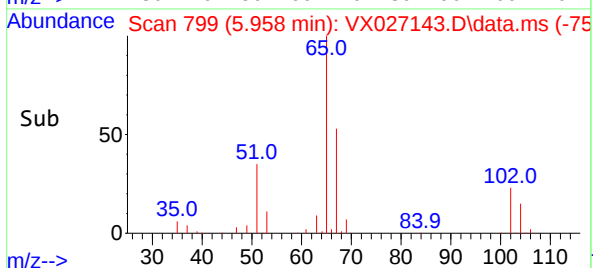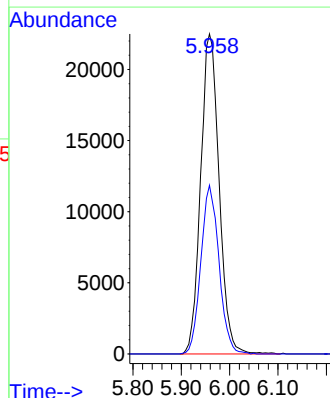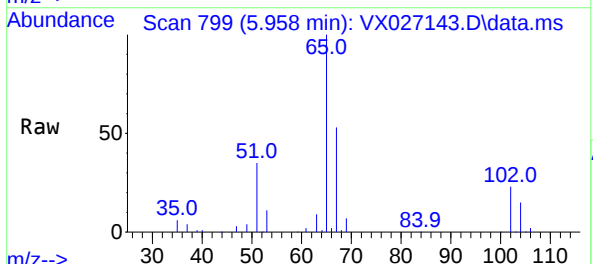

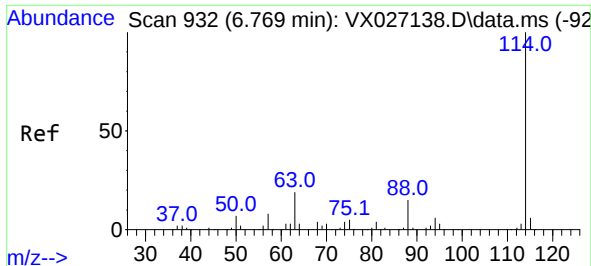

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. -0.006 min

Lab File: VX027143.D

Acq: 23 Feb 2022 14:01

Instrument :

MSVOA_X

ClientSampleId :

VX0223MBL01





Tgt Ion:114 Resp: 166195

Ion Ratio Lower Upper

114 100

63 20.1 0.0 42.8

88 15.7 0.0 33.0

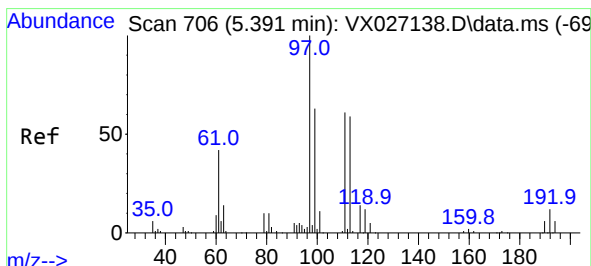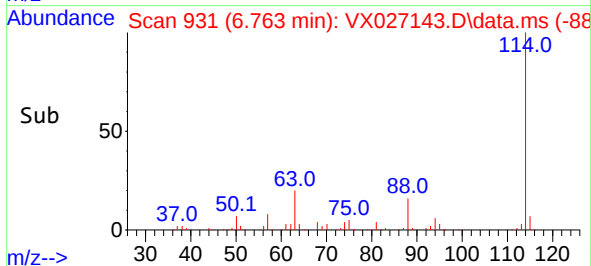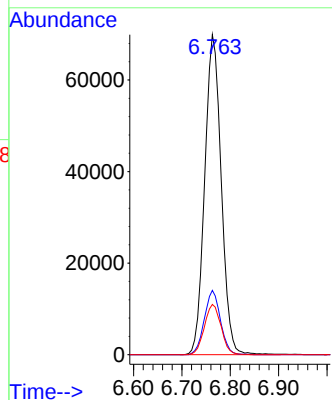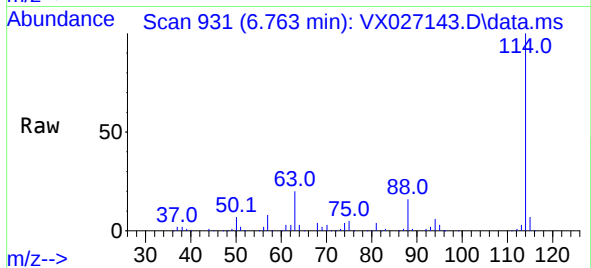

#35

Dibromofluoromethane

Concen: 49.864 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.006 min

Lab File: VX027143.D

Acq: 23 Feb 2022 14:01




Tgt Ion:113 Resp: 51440


Ion Ratio Lower Upper

113 100

111 102.8 81.2 121.8

192 20.6 15.0 22.4


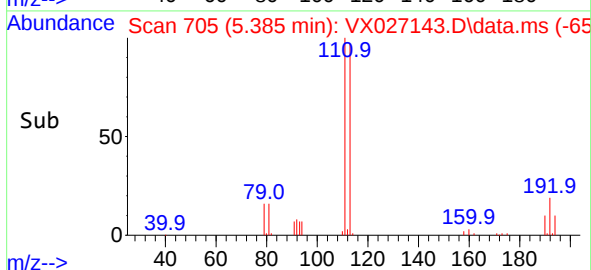
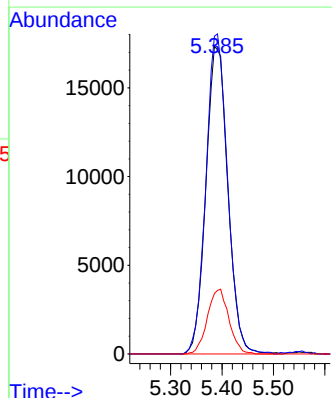
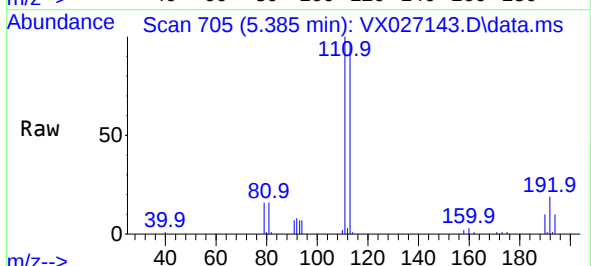


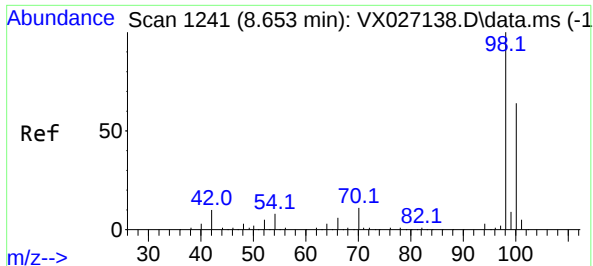

#50
Toluene-d8
Concen: 49.461 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027143.D
Acq: 23 Feb 2022 14:01




Instrument :
MSVOA_X
ClientSampleId :
VX0223MBL01


Tgt Ion: 98 Resp: 190786
Ion Ratio Lower Upper
98 100
100 67.1 53.2 79.8

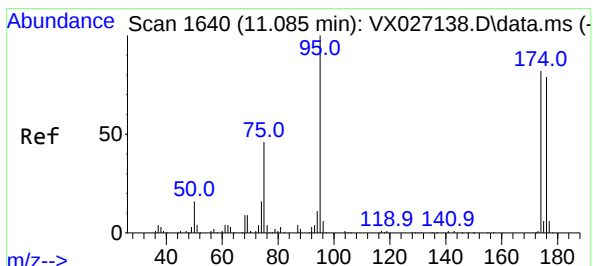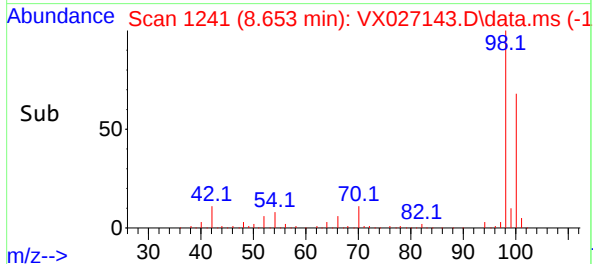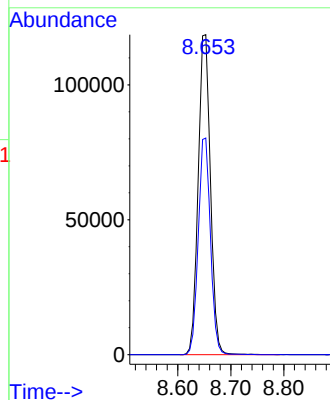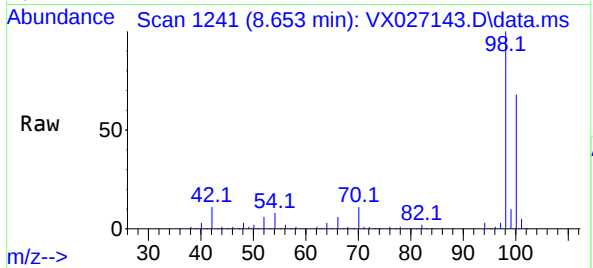

#62
4-Bromofluorobenzene
Concen: 48.364 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX027143.D
Acq: 23 Feb 2022 14:01

Tgt Ion: 95 Resp: 71609
Ion Ratio Lower Upper
95 100
174 78.9 0.0 148.6
176 75.9 0.0 141.4


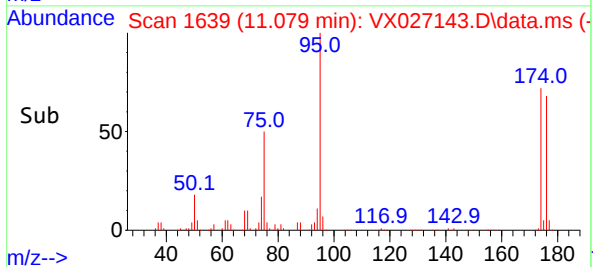
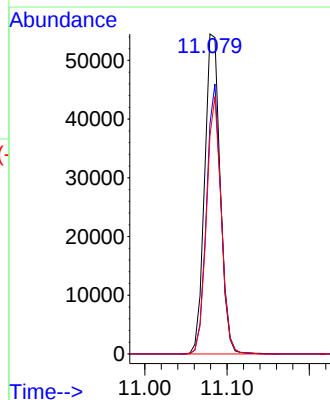
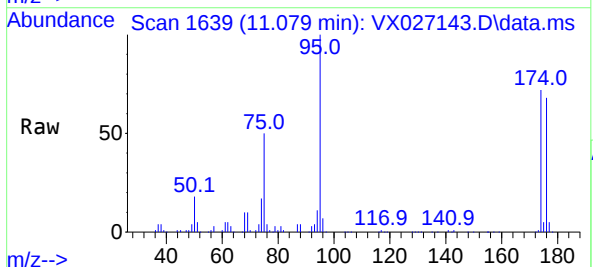


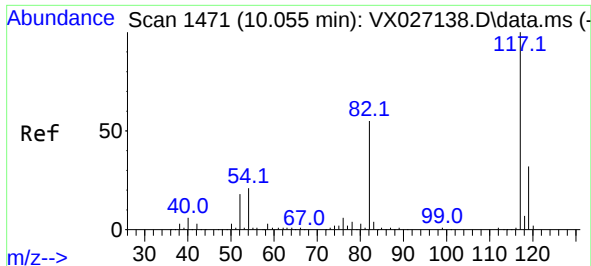

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX027143.D
Acq: 23 Feb 2022 14:01

Instrument :
MSVOA_X
ClientSampleId :
VX0223MBL01

Tgt Ion:117 Resp: 150665
Ion Ratio Lower Upper
117 100
82 54.3 45.2 67.8
119 32.6 26.2 39.2

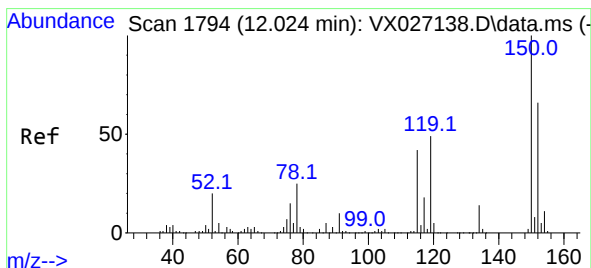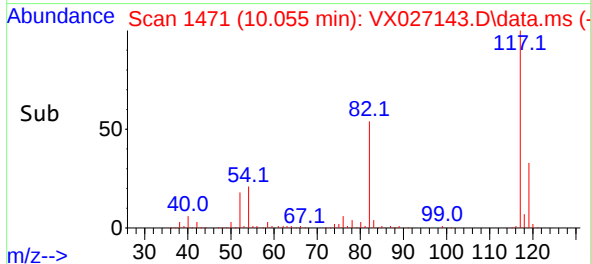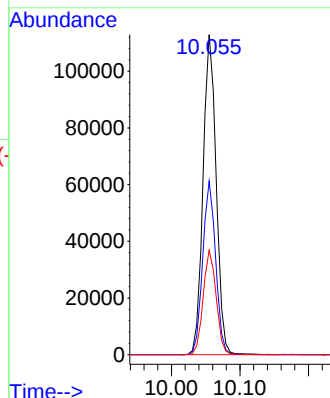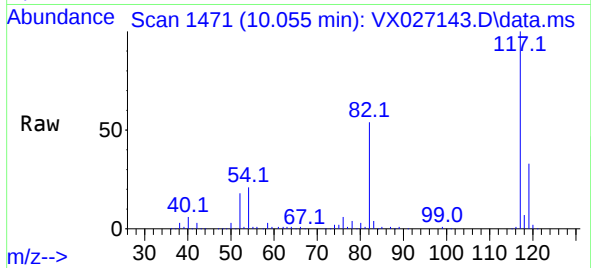

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027143.D
Acq: 23 Feb 2022 14:01

Tgt Ion:152 Resp: 68660
Ion Ratio Lower Upper
152 100
115 59.6 44.2 132.6
150 158.1 0.0 348.2

