

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022322\
 Data File : VX027155.D
 Acq On : 23 Feb 2022 18:56
 Operator : JC/MD
 Sample : N1647-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31382

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Title : SW846 8260

Signal : TIC: VX027155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	695	706	722	rBV	50811	147157	33.43%	5.741%
2	5.556	723	733	745	rVV	90445	253491	57.58%	9.889%
3	5.964	790	800	813	rBV	56339	144641	32.85%	5.642%
4	6.769	922	932	945	rBV	139668	329065	74.75%	12.837%
5	8.653	1234	1241	1249	rBV	284038	440246	100.00%	17.174%
6	8.720	1249	1252	1260	rVB	6731	9976	2.27%	0.389%
7	10.055	1465	1471	1480	rBV	287515	382371	86.85%	14.916%
8	10.305	1506	1512	1519	rBV	5823	8225	1.87%	0.321%
9	11.079	1634	1639	1650	rBV	221201	291360	66.18%	11.366%
10	11.384	1685	1689	1697	rBV	3722	6736	1.53%	0.263%
11	11.756	1745	1750	1756	rVB	11313	13951	3.17%	0.544%
12	12.024	1789	1794	1801	rBV	293039	359159	81.58%	14.011%
13	12.091	1801	1805	1810	rVB	6286	7752	1.76%	0.302%
14	12.244	1826	1830	1833	rBV	5170	7066	1.61%	0.276%
15	12.317	1838	1842	1850	rVB3	3967	5943	1.35%	0.232%
16	12.963	1945	1948	1953	rVB	4826	5360	1.22%	0.209%
17	13.140	1974	1977	1979	rBV2	4888	6064	1.38%	0.237%
18	13.170	1979	1982	1986	rVB2	6660	8136	1.85%	0.317%
19	13.292	1992	2002	2007	rBV3	16718	27578	6.26%	1.076%
20	13.420	2019	2023	2028	rVB	13405	17113	3.89%	0.668%
21	13.585	2046	2050	2055	rVV3	3097	5003	1.14%	0.195%
22	13.664	2060	2063	2068	rVB2	3696	5113	1.16%	0.199%
23	13.853	2088	2094	2100	rVB2	5597	7451	1.69%	0.291%
24	13.926	2100	2106	2111	rBV3	5866	8063	1.83%	0.315%
25	14.079	2128	2131	2135	rBV	4207	4695	1.07%	0.183%
26	14.231	2147	2156	2163	rBV	16129	24860	5.65%	0.970%
27	14.371	2176	2179	2184	rBV3	4348	5320	1.21%	0.208%
28	14.481	2192	2197	2202	rBV2	10650	13527	3.07%	0.528%
29	14.615	2216	2219	2221	rBV2	5813	7077	1.61%	0.276%
30	14.640	2221	2223	2226	rVV2	4532	5490	1.25%	0.214%
31	15.182	2309	2312	2315	rBV2	4146	5454	1.24%	0.213%


Sum of corrected areas: 2563443

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022322\
Data File : VX027155.D
Acq On : 23 Feb 2022 18:56
Operator : JC/MD
Sample : N1647-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31382

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

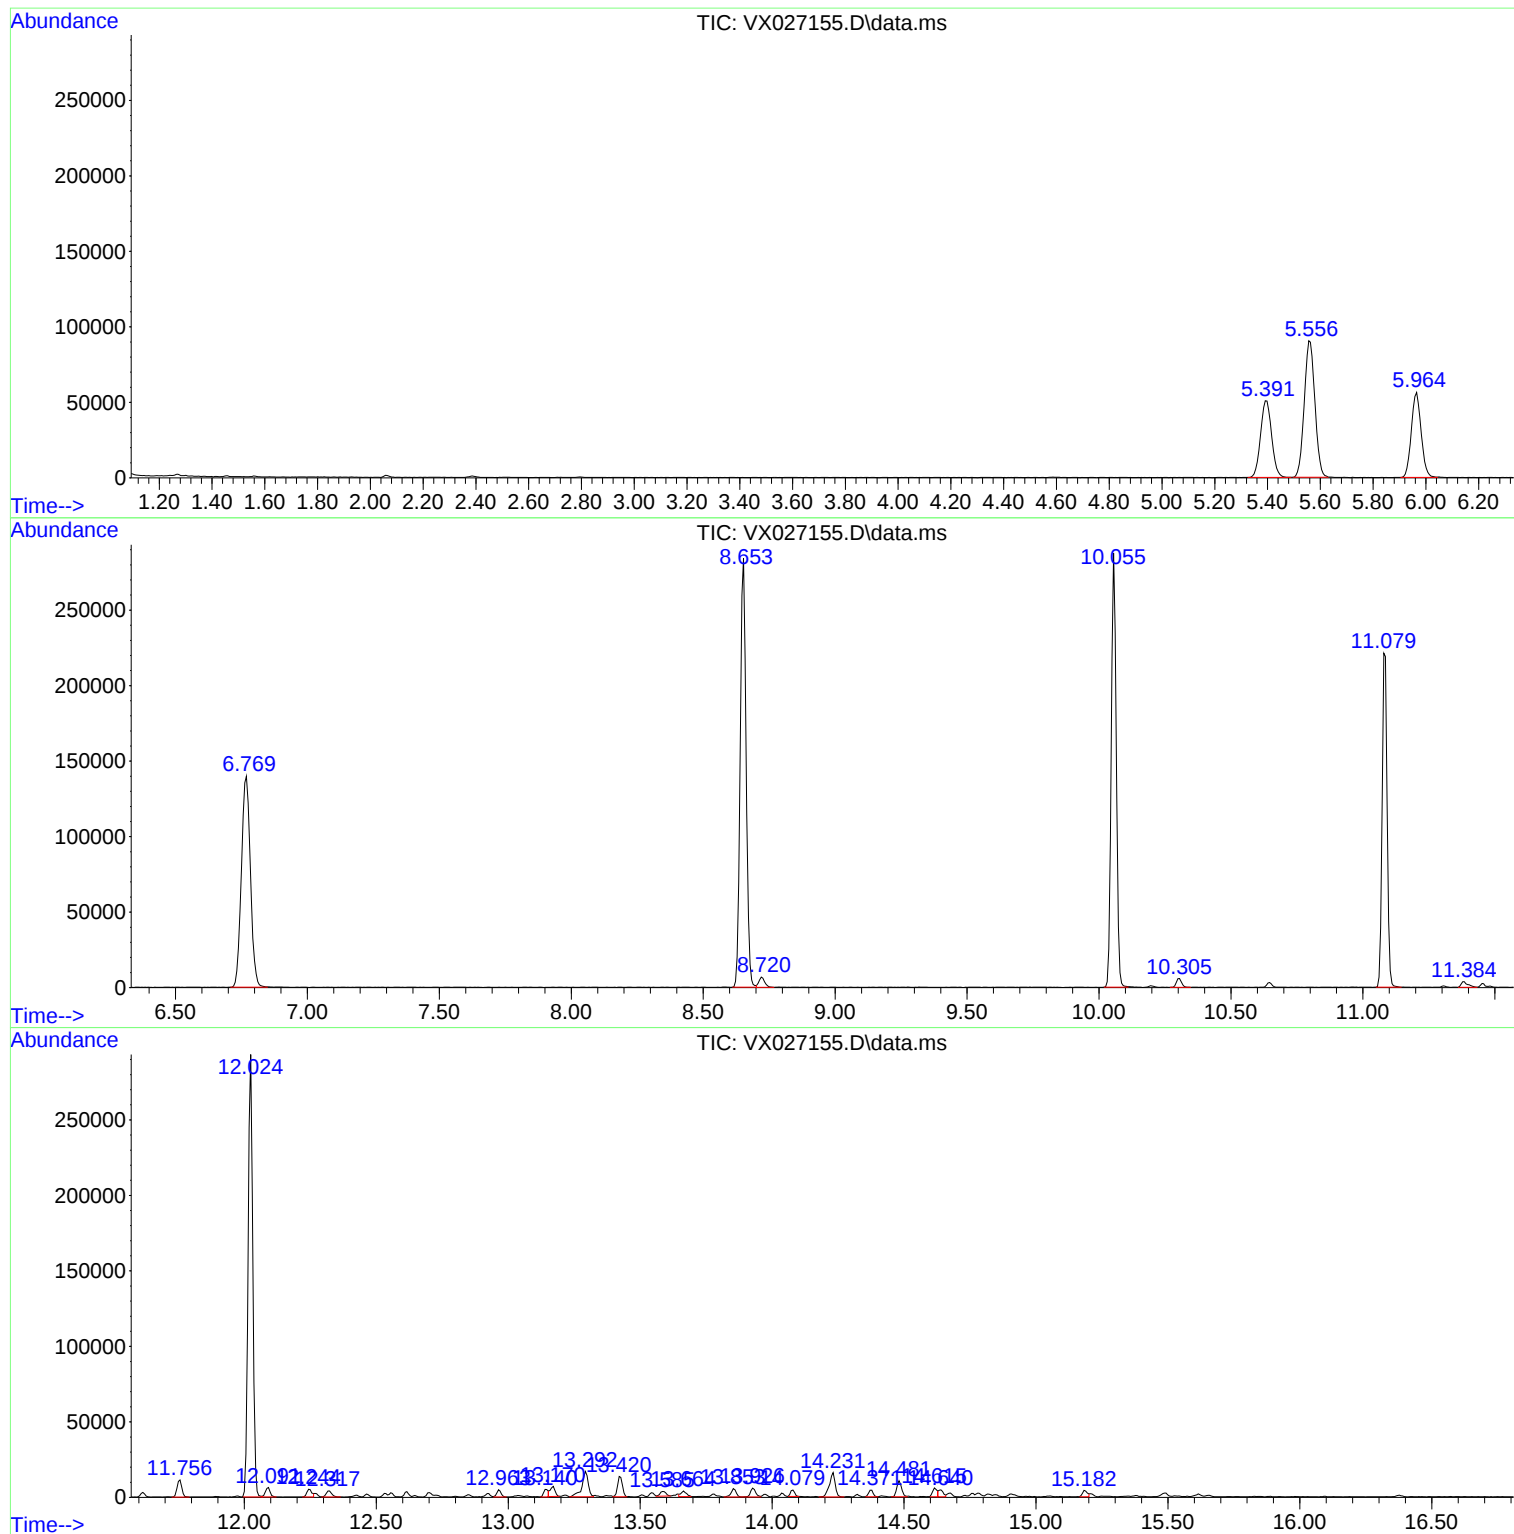

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022322\
Data File : VX027155.D
Acq On : 23 Feb 2022 18:56
Operator : JC/MD
Sample : N1647-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31382

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022322\
Data File : VX027155.D
Acq On : 23 Feb 2022 18:56
Operator : JC/MD
Sample : N1647-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31382

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------