

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022322\
 Data File : VX027156.D
 Acq On : 23 Feb 2022 19:20
 Operator : JC/MD
 Sample : N1647-02 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31415

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Title : SW846 8260

Signal : TIC: VX027156.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	694	707	722	rBV	51522	149434	33.80%	5.829%
2	5.562	723	734	746	rVB	90195	255583	57.80%	9.970%
3	5.964	790	800	818	rVB	54928	145186	32.83%	5.663%
4	6.769	922	932	945	rBV	139747	330212	74.68%	12.881%
5	8.653	1233	1241	1250	rBV	286271	442177	100.00%	17.248%
6	10.055	1465	1471	1483	rBV	294710	390424	88.30%	15.229%
7	11.086	1634	1640	1651	rVB	231995	300286	67.91%	11.713%
8	11.756	1745	1750	1755	rVB	5885	6963	1.57%	0.272%
9	12.024	1789	1794	1801	rBV	314051	373899	84.56%	14.585%
10	12.091	1801	1805	1811	rVB	3601	4859	1.10%	0.190%
11	13.140	1973	1977	1979	rBV2	4929	6710	1.52%	0.262%
12	13.170	1979	1982	1987	rVB2	5524	7413	1.68%	0.289%
13	13.268	1992	1998	1999	rBV4	4992	6840	1.55%	0.267%
14	13.292	1999	2002	2007	rVB2	14033	18908	4.28%	0.738%
15	13.420	2019	2023	2031	rVB	11797	15965	3.61%	0.623%
16	13.585	2046	2050	2054	rBV2	2888	4638	1.05%	0.181%
17	13.664	2060	2063	2070	rVB2	3178	4639	1.05%	0.181%
18	13.853	2088	2094	2100	rVB2	5099	8381	1.90%	0.327%
19	13.926	2100	2106	2111	rBV3	5479	8067	1.82%	0.315%
20	14.036	2120	2124	2128	rBV2	4412	5024	1.14%	0.196%
21	14.073	2128	2130	2137	rVB3	4063	4859	1.10%	0.190%
22	14.231	2148	2156	2162	rVB	15036	24045	5.44%	0.938%
23	14.371	2175	2179	2184	rBV	3678	4898	1.11%	0.191%
24	14.481	2192	2197	2203	rBV	10864	15401	3.48%	0.601%
25	14.615	2215	2219	2221	rBV2	6929	8746	1.98%	0.341%
26	14.634	2221	2222	2226	rVV2	5621	6534	1.48%	0.255%
27	15.188	2306	2313	2315	rBV	4673	7052	1.59%	0.275%
28	15.487	2355	2362	2366	rBV4	4013	6477	1.46%	0.253%


Sum of corrected areas: 2563620

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022322\
Data File : VX027156.D
Acq On : 23 Feb 2022 19:20
Operator : JC/MD
Sample : N1647-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31415

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

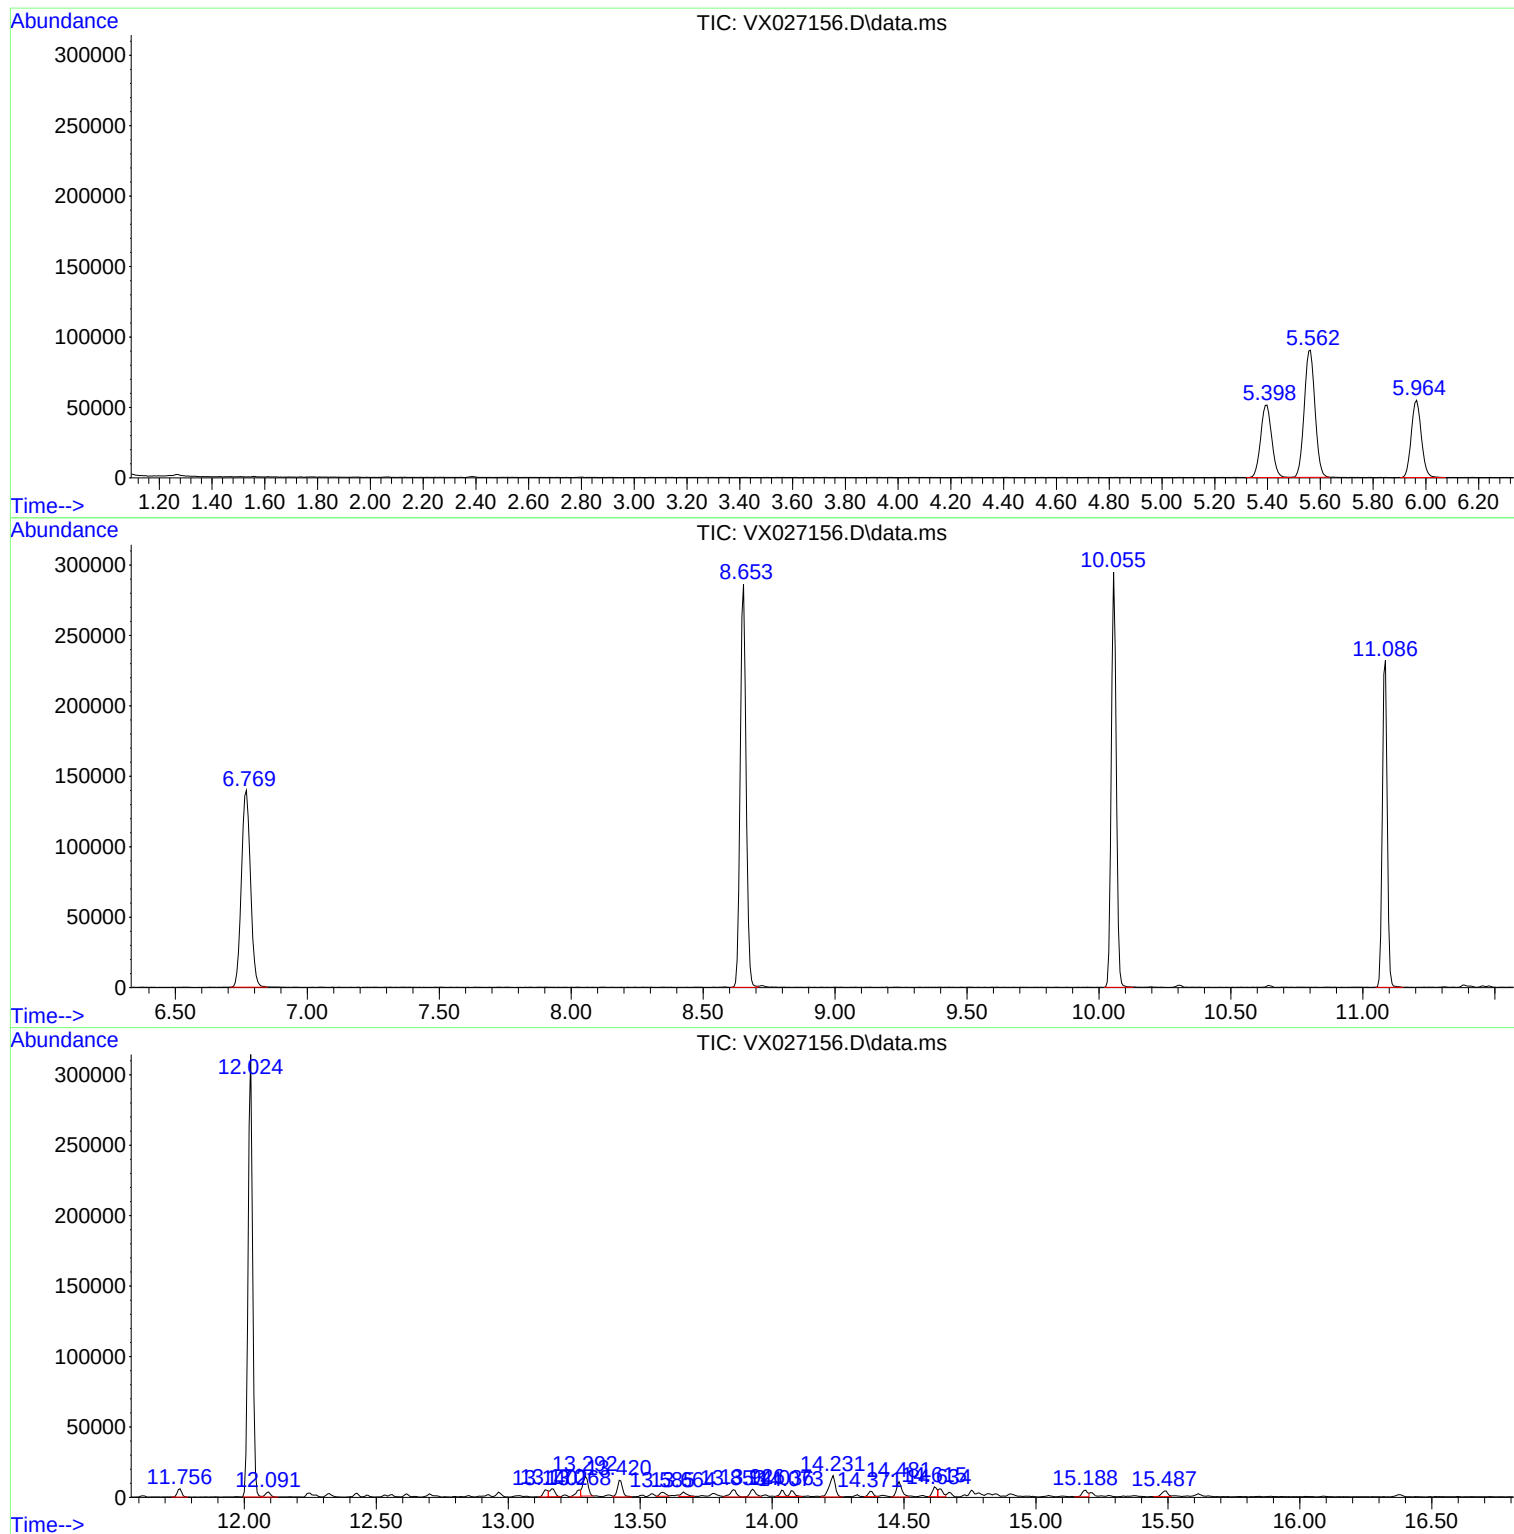

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022322\
Data File : VX027156.D
Acq On : 23 Feb 2022 19:20
Operator : JC/MD
Sample : N1647-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31415

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022322\
Data File : VX027156.D
Acq On : 23 Feb 2022 19:20
Operator : JC/MD
Sample : N1647-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31415

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------