

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022324\
 Data File : VX040432.D
 Acq On : 23 Feb 2024 15:23
 Operator : JC/MD
 Sample : PB159217ZHE#02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB159217ZHE#02

Quant Time: Feb 23 22:20:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022224W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 23 06:47:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	70521	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	127619	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	124922	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	60835	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	56854	49.503	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	99.000%
35) Dibromofluoromethane	5.385	113	42408	49.312	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.620%
50) Toluene-d8	8.647	98	160620	51.706	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	103.420%
62) 4-Bromofluorobenzene	11.079	95	63076	50.672	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	101.340%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.172	85	240	0.282	ug/l	89
3) Chloromethane	1.178	50	697	0.725	ug/l #	65
6) Chloroethane	1.684	64	302	0.523	ug/l #	43
11) Tert butyl alcohol	2.959	59	237	1.068	ug/l #	78
13) Acrolein	2.233	56	196	0.738	ug/l	93
16) Acetone	2.379	43	20941	43.760	ug/l	96
17) Carbon Disulfide	2.514	76	568	0.265	ug/l #	76
18) Methyl Acetate	2.703	43	945	0.762	ug/l #	79
20) Methylene Chloride	2.788	84	5547	5.536	ug/l	93
25) 2-Butanone	4.556	43	512	0.686	ug/l	98
29) Tetrahydrofuran	5.019	42	1593	3.208	ug/l	96
31) Cyclohexane	5.550	56	2032	1.476	ug/l #	33
36) 1,1-Dichloropropene	5.550	75	6713	5.044	ug/l #	51
37) Ethyl Acetate	4.733	43	2332	1.534	ug/l #	81
38) Carbon Tetrachloride	5.550	117	8053	6.540	ug/l #	15
41) Methacrylonitrile	5.019	41	539	0.668	ug/l #	44
43) Isopropyl Acetate	6.342	43	77321	33.139	ug/l	98
48) Methyl methacrylate	7.799	41	68752	59.500	ug/l #	50
49) 1,4-Dioxane	7.805	88	69	2.963	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	60461	38.153	ug/l #	50
53) t-1,3-Dichloropropene	8.958	75	499	0.367	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	23314	16.089	ug/l #	65
56) Ethyl methacrylate	9.244	69	585	0.403	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	3251	1.964	ug/l #	42
59) 2-Hexanone	9.372	43	73429	60.081	ug/l #	26
74) N-amyl acetate	10.817	43	529	0.265	ug/l #	44
76) 1,2,3-Trichloropropane	11.079	75	36126	26.706	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.079	75	36126	92.925	ug/l #	5
88) 1,4-Dichlorobenzene	12.036	146	438	0.210	ug/l #	57
93) 1,2,4-Trichlorobenzene	13.597	180	274	0.219	ug/l #	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022324\
Data File : VX040432.D
Acq On : 23 Feb 2024 15:23
Operator : JC/MD
Sample : PB159217ZHE#02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02

Quant Time: Feb 23 22:20:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022224W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 23 06:47:29 2024
Response via : Initial Calibration




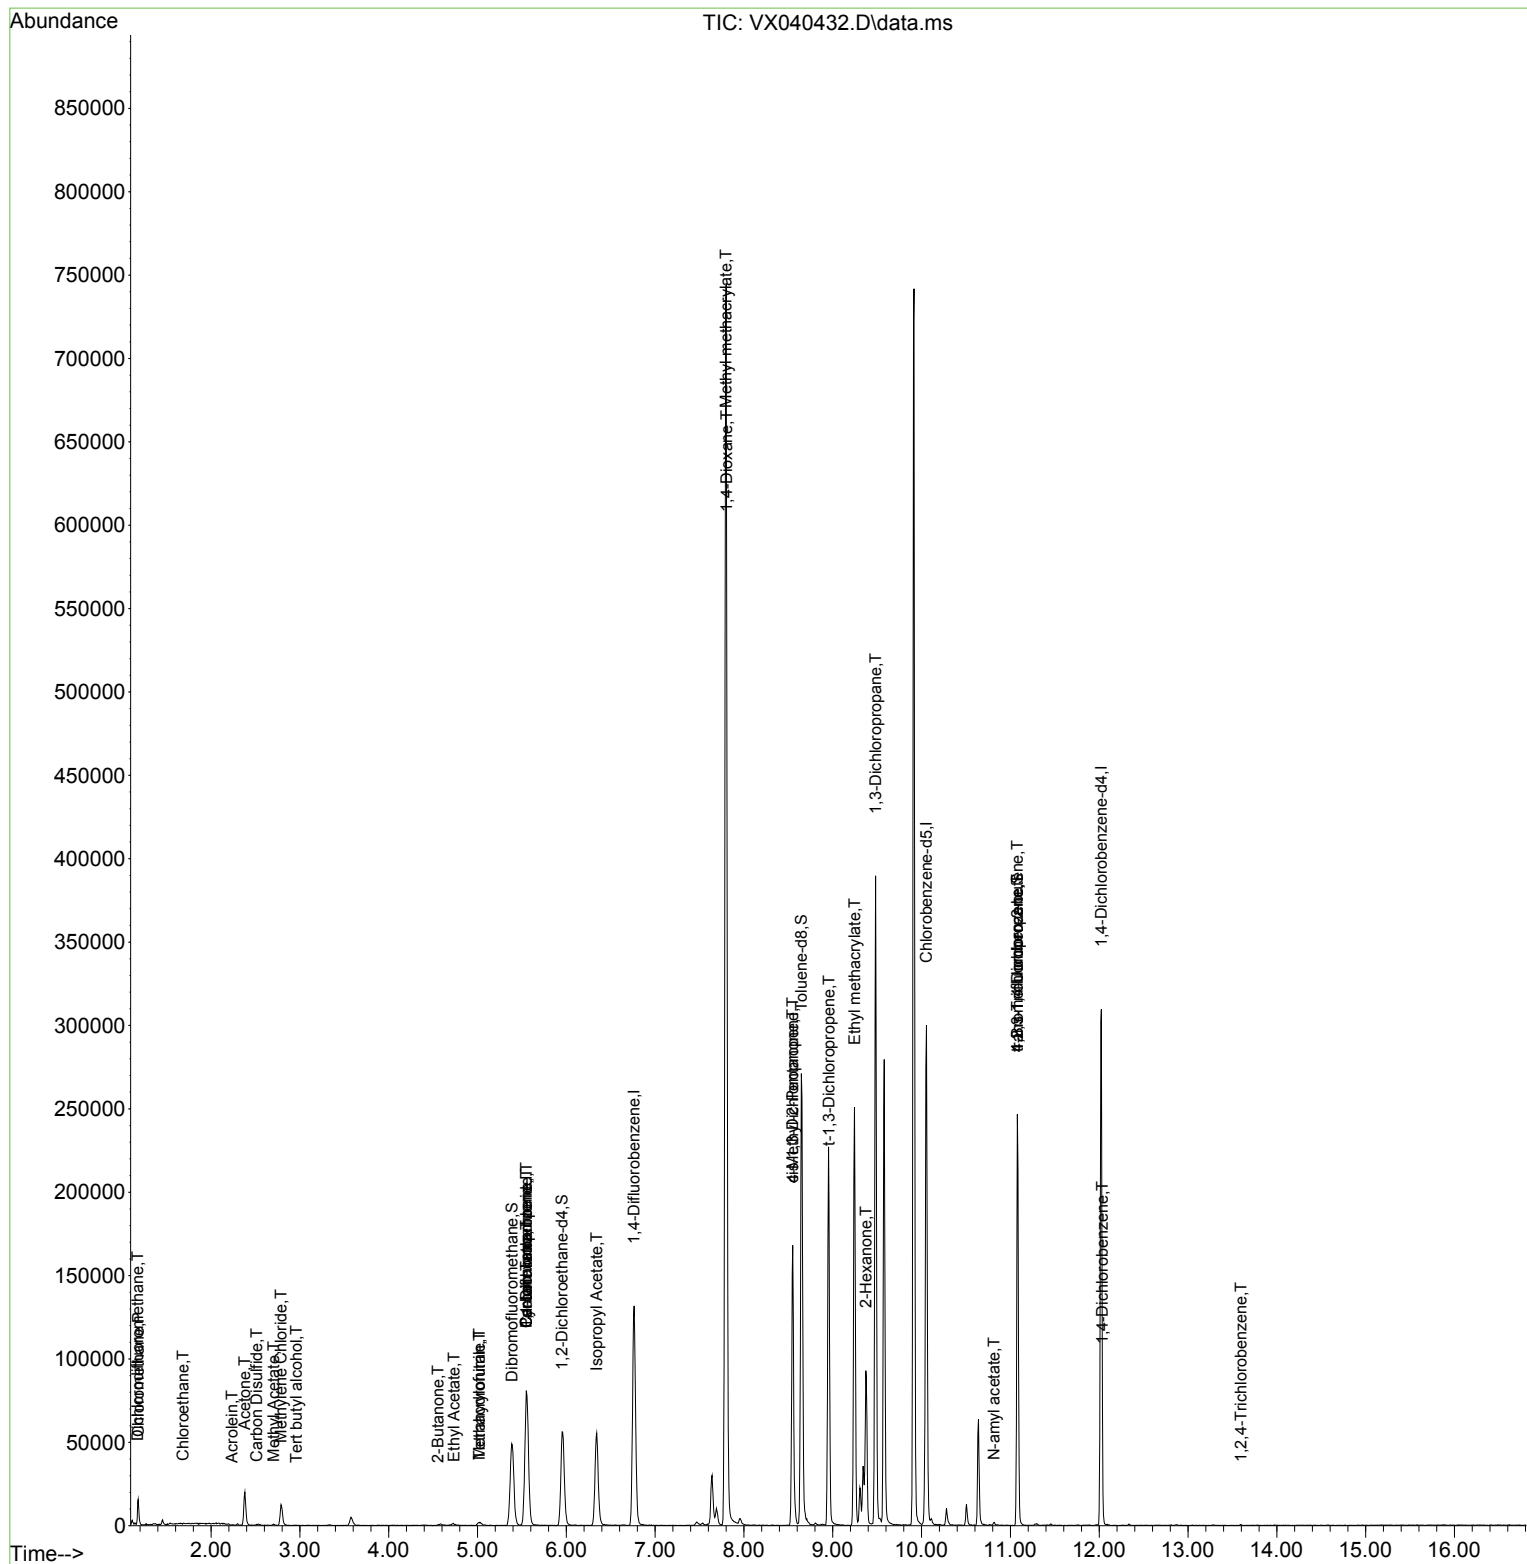




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23




Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02


Tgt Ion:168 Resp: 70521
Ion Ratio Lower Upper
168 100
99 67.5 56.6 85.0

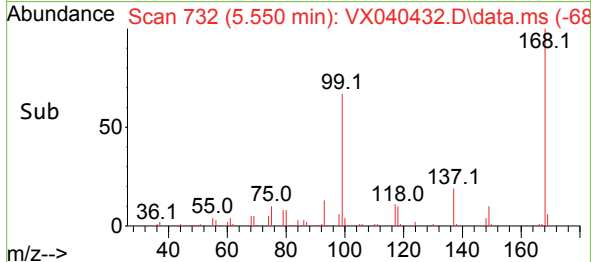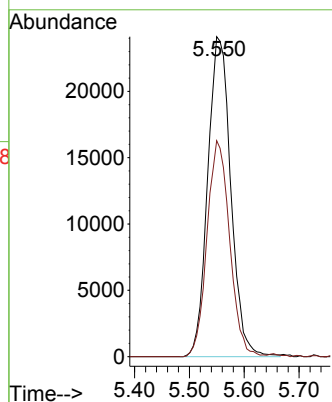

#2
Dichlorodifluoromethane
Concen: 0.282 ug/l
RT: 1.172 min Scan# 14
Delta R.T. 0.006 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion: 85 Resp: 240
Ion Ratio Lower Upper
85 100
87 27.3 16.7 50.1


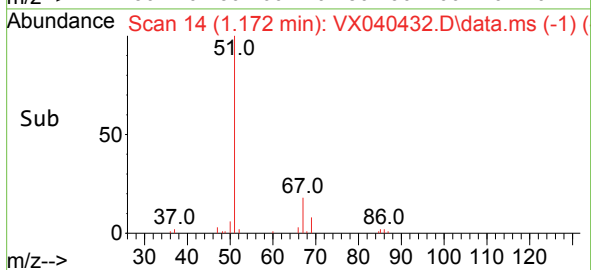




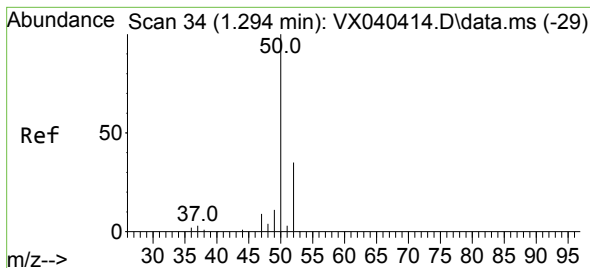

#3
Chloromethane
Concen: 0.725 ug/l
RT: 1.178 min Scan# 11
Delta R.T. -0.116 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23




Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02


Tgt Ion: 50 Resp: 697
Ion Ratio Lower Upper
50 100
52 12.7 25.5 38.3#

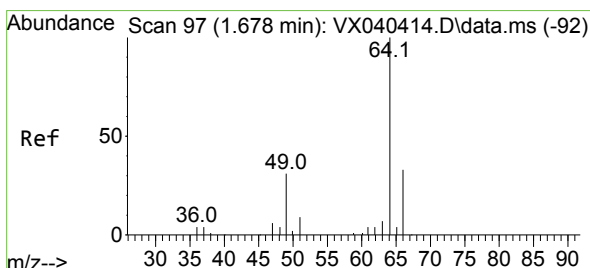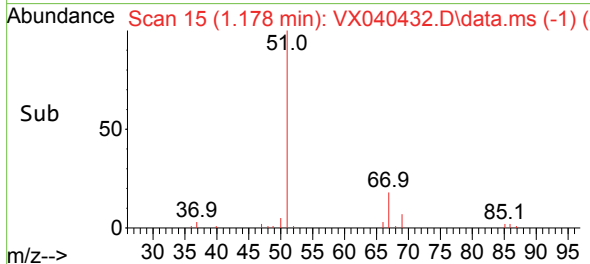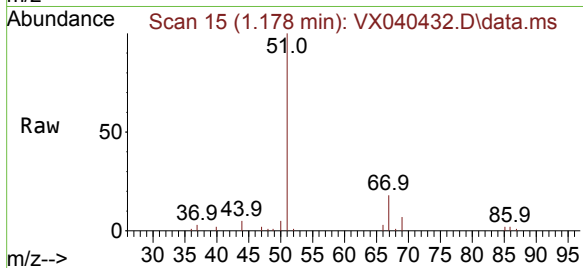

#6
Chloroethane
Concen: 0.523 ug/l
RT: 1.684 min Scan# 98
Delta R.T. 0.006 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion: 64 Resp: 302
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#

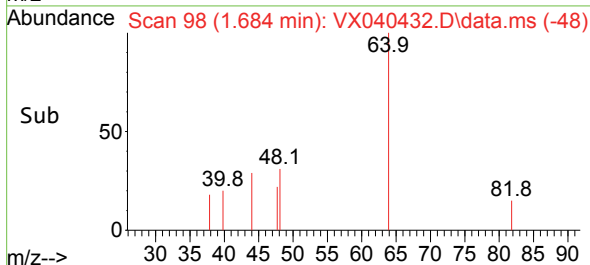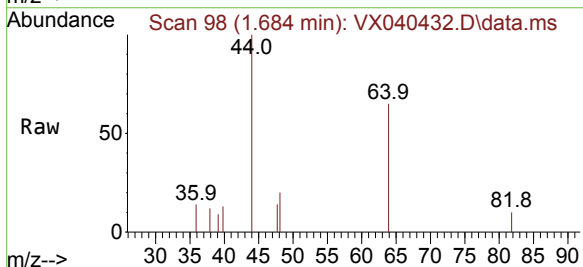



#11

Tert butyl alcohol

Concen: 1.068 ug/l

RT: 2.959 min Scan# 307

Delta R.T. -0.000 min

Lab File: VX040432.D

Acq: 23 Feb 2024 15:23

Instrument :

MSVOA_X

ClientSampleId :





PB159217ZHE#02

Tgt Ion: 59 Resp: 237

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#



#13

Acrolein

Concen: 0.738 ug/l

RT: 2.233 min Scan# 188

Delta R.T. -0.000 min

Lab File: VX040432.D




Acq: 23 Feb 2024 15:23


Tgt Ion: 56 Resp: 196

Ion Ratio Lower Upper

56 100

55 65.3 57.1 85.7


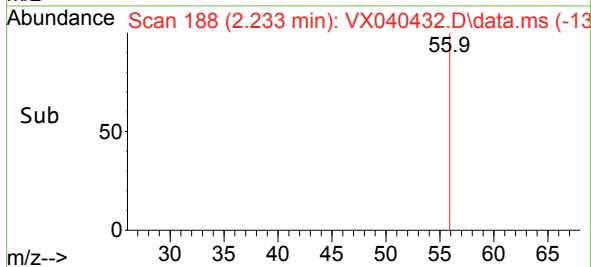

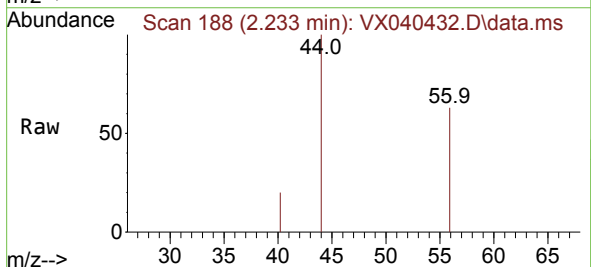




#16
Acetone
Concen: 43.760 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23




Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02


Tgt Ion: 43 Resp: 20941
Ion Ratio Lower Upper
43 100
58 29.7 21.9 32.9

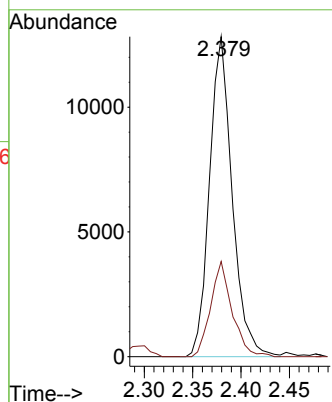

#17
Carbon Disulfide
Concen: 0.265 ug/l
RT: 2.514 min Scan# 234
Delta R.T. 0.006 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23


Tgt Ion: 76 Resp: 568
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.6#

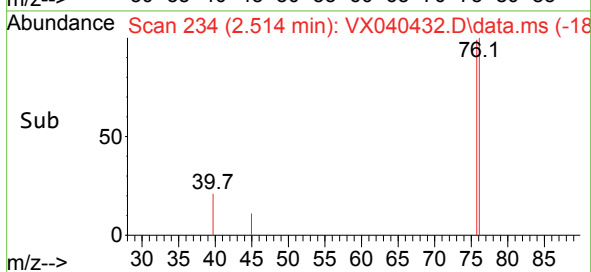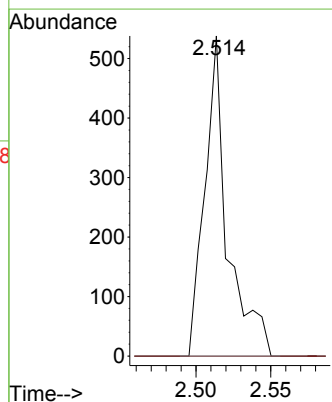






#18
Methyl Acetate
Concen: 0.762 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.000 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23


Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02





Tgt Ion: 43 Resp: 945
Ion Ratio Lower Upper
43 100
74 12.3 17.8 26.8#




#20
Methylene Chloride
Concen: 5.536 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

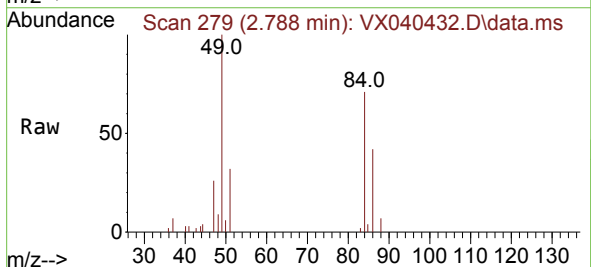

Tgt Ion: 84 Resp: 5547
Ion Ratio Lower Upper
84 100
49 141.3 103.6 155.4
51 45.2 33.8 50.6
86 58.8 49.4 74.0



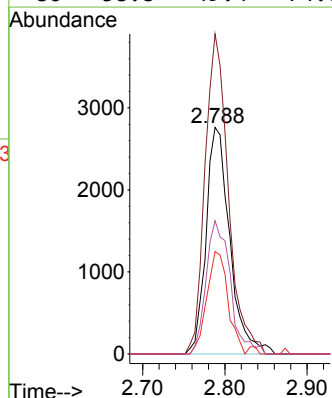
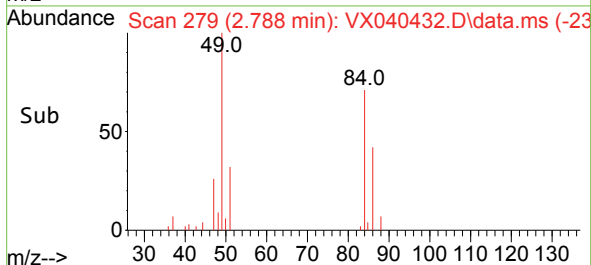




#25
2-Butanone
Concen: 0.686 ug/l
RT: 4.556 min Scan# 512
Delta R.T. 0.006 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23




Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02


Tgt Ion: 43 Resp: 512
Ion Ratio Lower Upper
43 100
72 23.5 19.4 29.2

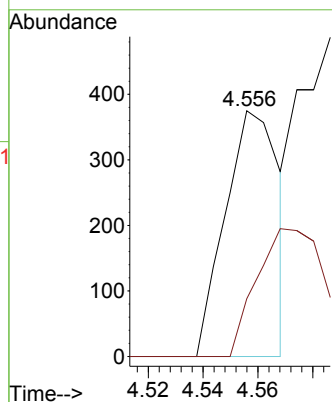

#29
Tetrahydrofuran
Concen: 3.208 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.018 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23


Tgt Ion: 42 Resp: 1593
Ion Ratio Lower Upper
42 100
72 45.5 34.2 51.4
71 42.6 32.2 48.2

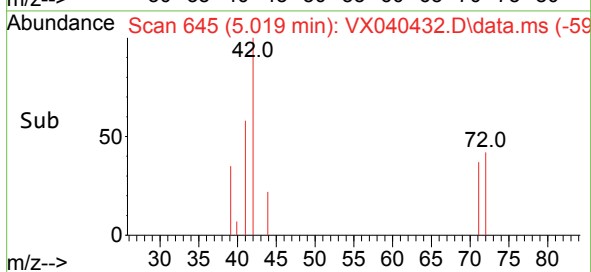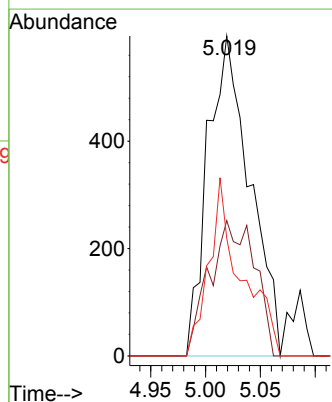



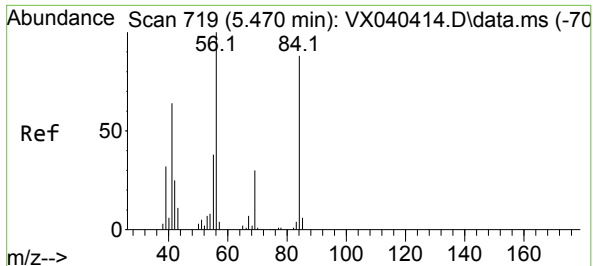


#31
Cyclohexane
Concen: 1.476 ug/l
RT: 5.550 min Scan# 719
Delta R.T. 0.079 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02



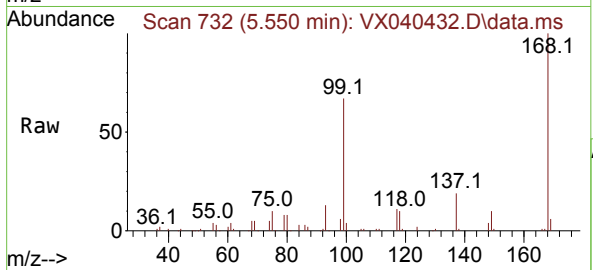



Tgt Ion: 56 Resp: 2032
Ion Ratio Lower Upper
56 100
69 139.1 23.4 35.2#
84 98.2 65.9 98.9

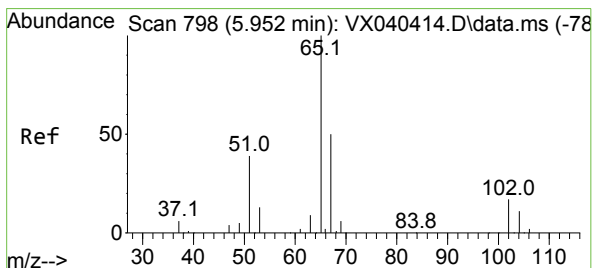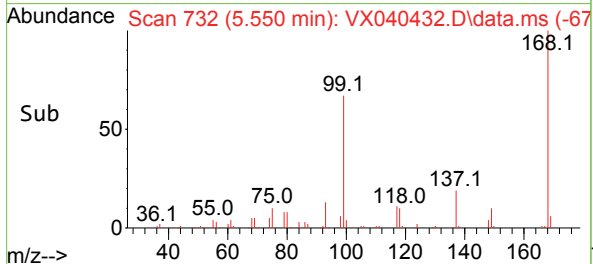

#33
1,2-Dichloroethane-d4
Concen: 49.503 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion: 65 Resp: 56854
Ion Ratio Lower Upper
65 100
67 51.8 0.0 100.2


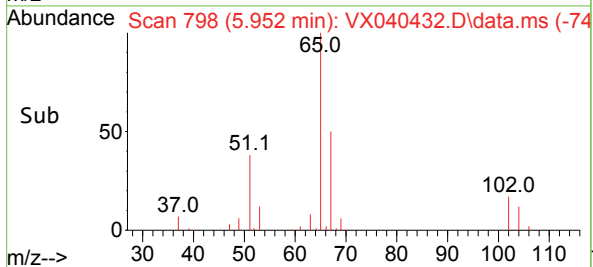

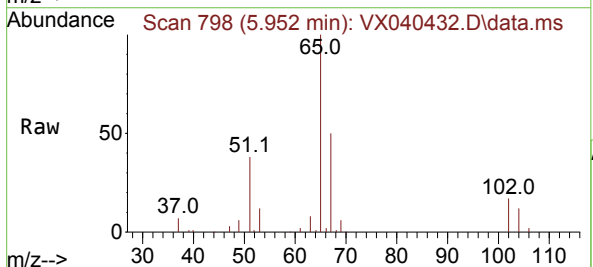


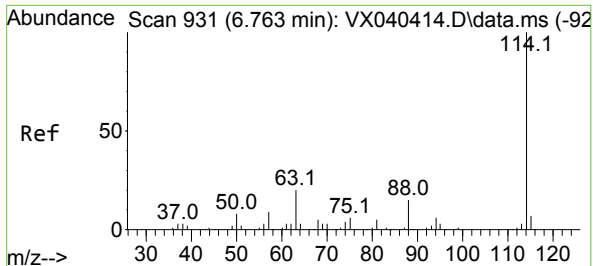

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23




Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02


Tgt Ion:114 Resp: 127619
Ion Ratio Lower Upper
114 100
63 24.0 0.0 45.0
88 16.9 0.0 36.6

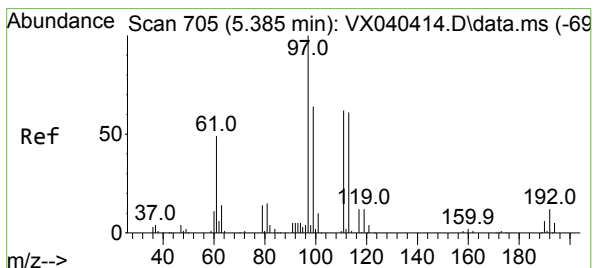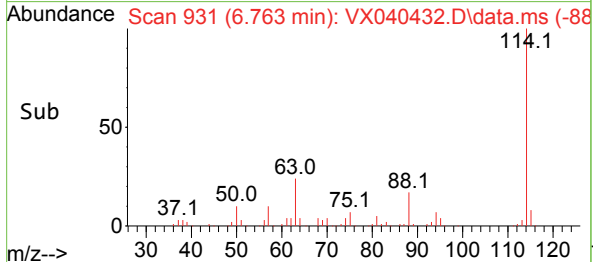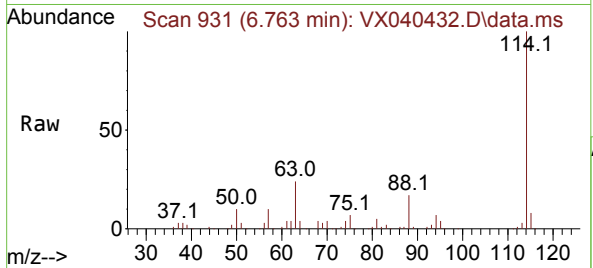

#35
Dibromofluoromethane
Concen: 49.312 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion:113 Resp: 42408
Ion Ratio Lower Upper
113 100
111 100.9 82.9 124.3
192 17.0 13.3 19.9

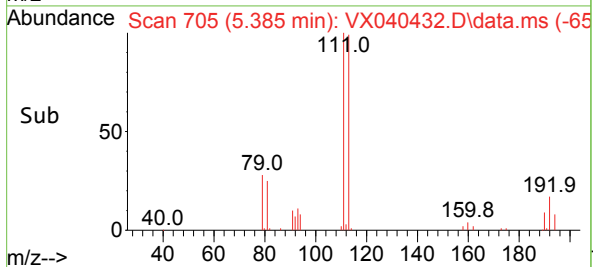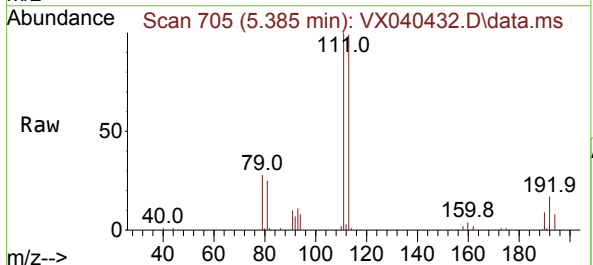



#36

1,1-Dichloropropene

Concen: 5.044 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.140 min

Lab File: VX040432.D

Acq: 23 Feb 2024 15:23

Instrument :

MSVOA_X

ClientSampleId :

PB159217ZHE#02





Tgt Ion: 75 Resp: 6713

Ion Ratio Lower Upper

75 100

110 10.2 17.0 50.9#

77 0.0 24.7 37.1#

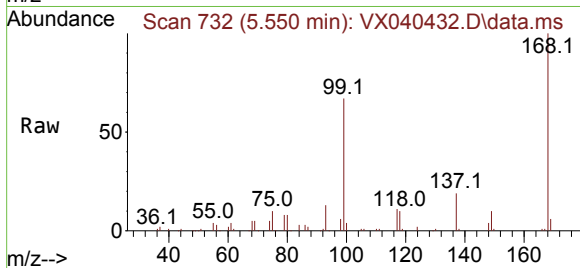

#37

Ethyl Acetate

Concen: 1.534 ug/l

RT: 4.733 min Scan# 598

Delta R.T. 0.018 min

Lab File: VX040432.D

Acq: 23 Feb 2024 15:23




Tgt Ion: 43 Resp: 2332


Ion Ratio Lower Upper

43 100

61 5.7 10.6 16.0#


70 3.5 8.3 12.5#

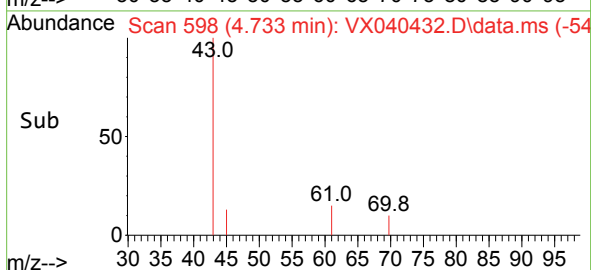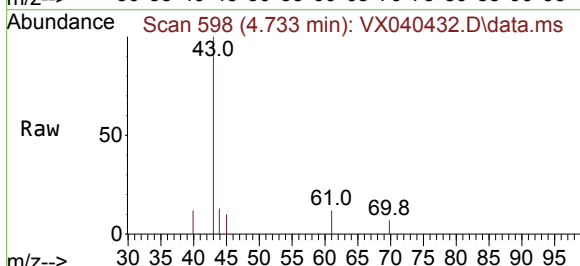






#38
Carbon Tetrachloride
Concen: 6.540 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02







Tgt Ion:117 Resp: 8053
Ion Ratio Lower Upper
117 100
119 4.5 78.2 117.2#
121 0.0 24.4 36.6#



#41
Methacrylonitrile
Concen: 0.668 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.098 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion: 41 Resp: 539
Ion Ratio Lower Upper
41 100
39 74.6 45.2 67.8#
67 0.0 52.6 78.8#
52 0.0 22.7 34.1#



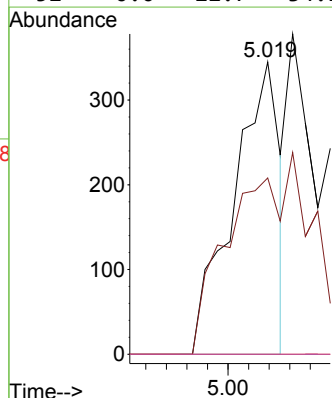





#43
Isopropyl Acetate
Concen: 33.139 ug/l
RT: 6.342 min Scan# 80
Delta R.T. 0.006 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23




Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02


Tgt Ion: 43 Resp: 77321
Ion Ratio Lower Upper
43 100
61 17.6 15.2 22.8
87 12.1 9.8 14.6



#48
Methyl methacrylate
Concen: 59.500 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.110 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion: 41 Resp: 68752
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 56.4 47.7 71.5


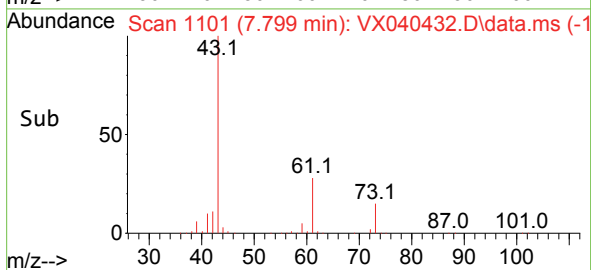






#49
1,4-Dioxane
Concen: 2.963 ug/l
RT: 7.805 min Scan# 1102
Delta R.T. 0.146 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23




Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02


Tgt Ion: 88 Resp: 69
Ion Ratio Lower Upper
88 100
43 1011488.4 0.0 0.0#
58 4402.9 60.1 90.1#

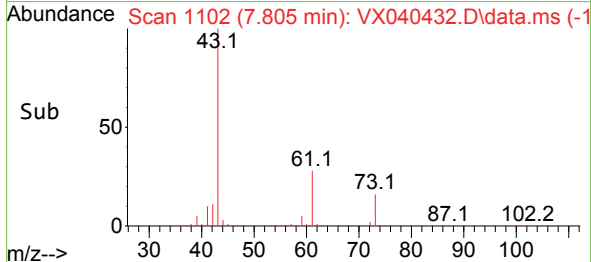

#50
Toluene-d8
Concen: 51.706 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion: 98 Resp: 160620
Ion Ratio Lower Upper
98 100
100 63.9 53.1 79.7

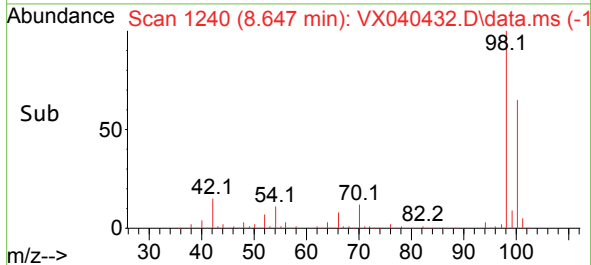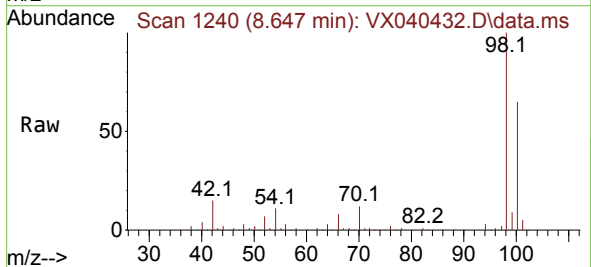



#51

4-Methyl-2-Pentanone

Concen: 38.153 ug/l

RT: 8.549 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX040432.D

Acq: 23 Feb 2024 15:23

Instrument :

MSVOA_X

ClientSampleId :





PB159217ZHE#02

Tgt Ion: 43 Resp: 60461

Ion Ratio Lower Upper

43 100

58 7.6 30.4 45.6#



#53

t-1,3-Dichloropropene

Concen: 0.367 ug/l

RT: 8.958 min Scan# 1291

Delta R.T. -0.018 min

Lab File: VX040432.D




Acq: 23 Feb 2024 15:23


Tgt Ion: 75 Resp: 499

Ion Ratio Lower Upper

75 100

77 0.0 25.7 38.5#









#54
 cis-1,3-Dichloropropene
 Concen: 16.089 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX040432.D
 Acq: 23 Feb 2024 15:23




Instrument :
 MSVOA_X
 ClientSampleId :
 PB159217ZHE#02


Tgt Ion: 75 Resp: 23314
 Ion Ratio Lower Upper
 75 100
 77 0.5 25.3 37.9#
 39 40.7 46.7 70.1#



#56
 Ethyl methacrylate
 Concen: 0.403 ug/l
 RT: 9.244 min Scan# 1338
 Delta R.T. 0.128 min
 Lab File: VX040432.D
 Acq: 23 Feb 2024 15:23

Tgt Ion: 69 Resp: 585
 Ion Ratio Lower Upper
 69 100
 41 7137.9 56.8 85.2#
 39 3286.8 32.0 48.0#

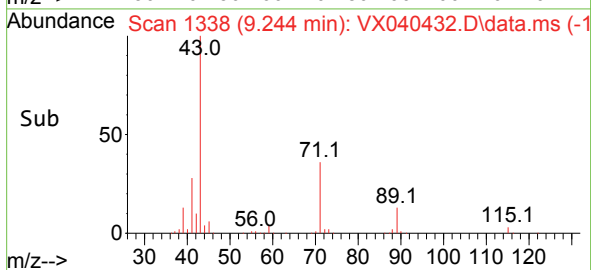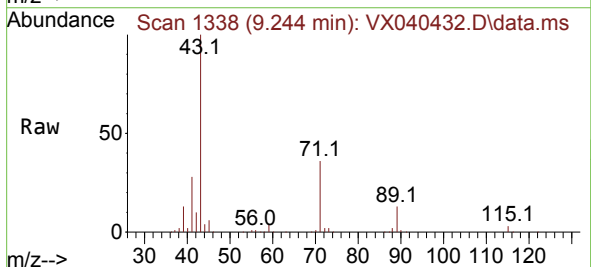



#57

1,3-Dichloropropane

Concen: 1.964 ug/l

RT: 9.482 min Scan# 11

Delta R.T. 0.177 min

Lab File: VX040432.D

Acq: 23 Feb 2024 15:23

Instrument :

MSVOA_X

ClientSampleId :





PB159217ZHE#02

Tgt Ion: 76 Resp: 3251

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

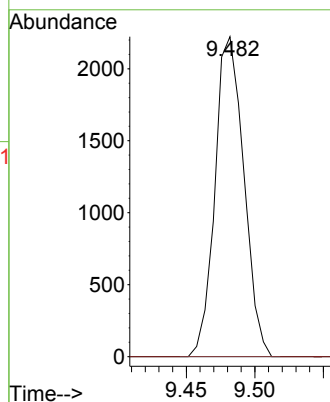

#59

2-Hexanone

Concen: 60.081 ug/l

RT: 9.372 min Scan# 1359

Delta R.T. -0.055 min

Lab File: VX040432.D




Acq: 23 Feb 2024 15:23


Tgt Ion: 43 Resp: 73429

Ion Ratio Lower Upper

43 100

58 0.0 26.2 78.5#


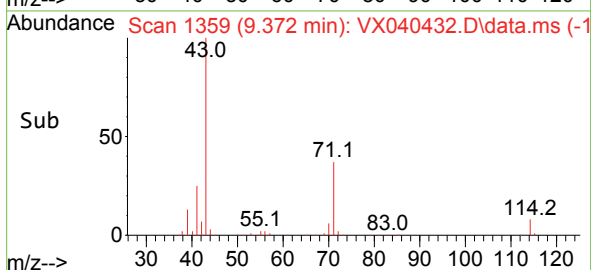






#62
4-Bromofluorobenzene
Concen: 50.672 ug/l
RT: 11.079 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23




Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02


Tgt Ion: 95 Resp: 63076
Ion Ratio Lower Upper
95 100
174 72.7 0.0 135.6
176 68.5 0.0 131.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion: 117 Resp: 124922
Ion Ratio Lower Upper
117 100
82 58.0 46.2 69.4
119 32.4 25.5 38.3



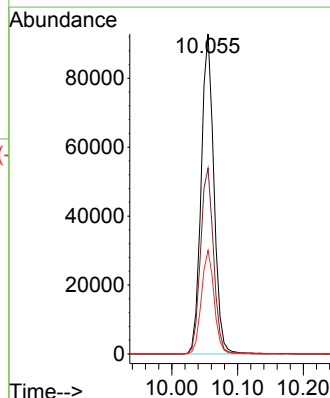





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23




Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02


Tgt Ion:152 Resp: 60835
Ion Ratio Lower Upper
152 100
115 64.1 43.3 129.9
150 161.4 0.0 345.0

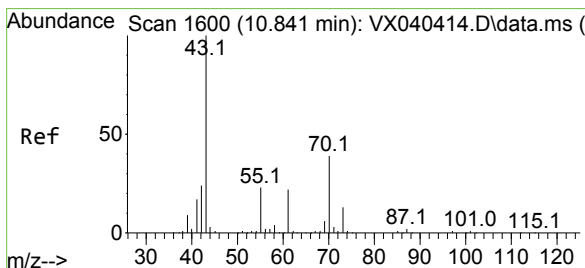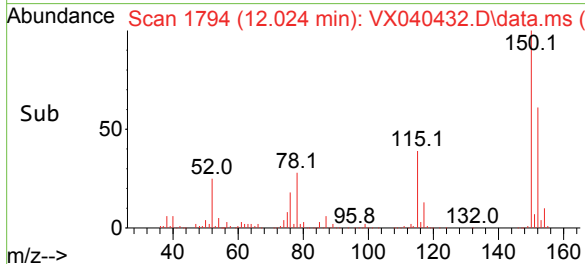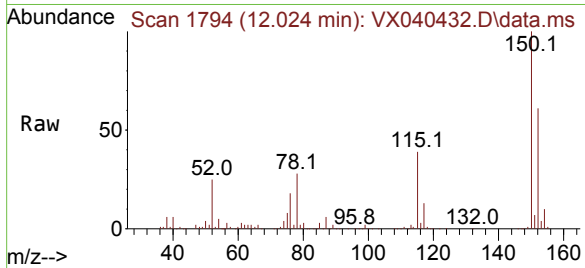

#74
N-ethyl acetate
Concen: 0.265 ug/l
RT: 10.817 min Scan# 1596
Delta R.T. -0.024 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion: 43 Resp: 529
Ion Ratio Lower Upper
43 100
70 0.0 32.9 49.3#
55 0.0 19.3 28.9#
61 0.0 18.8 28.2#


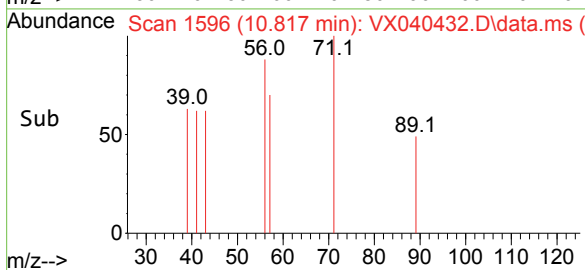

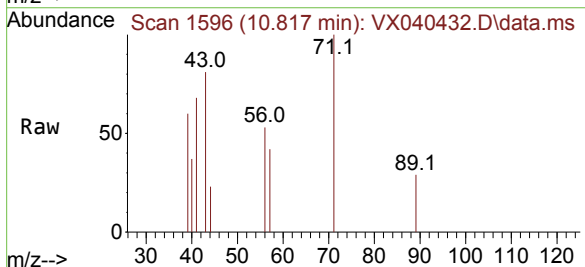




#76
1,2,3-Trichloropropane
Concen: 26.706 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23




Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02


Tgt Ion: 75 Resp: 36126
Ion Ratio Lower Upper
75 100
77 1.2 19.1 57.5#

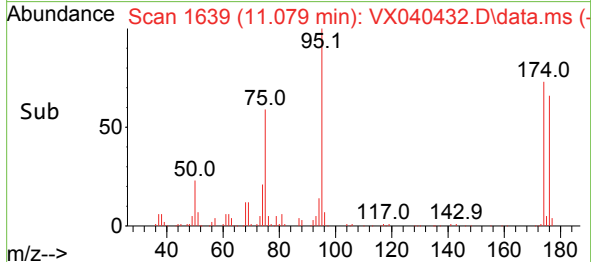

#81
trans-1,4-Dichloro-2-butene
Concen: 92.925 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion: 75 Resp: 36126
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#


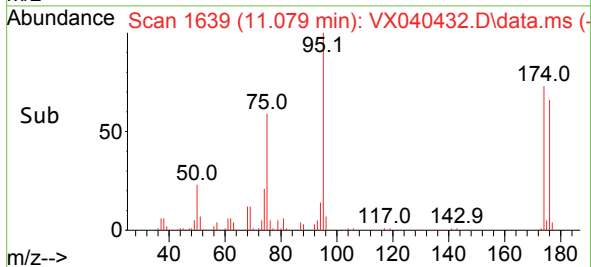

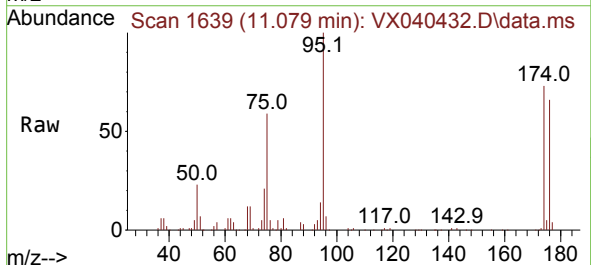




#88
1,4-Dichlorobenzene
Concen: 0.210 ug/l
RT: 12.036 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Instrument :
MSVOA_X
ClientSampleId :
PB159217ZHE#02

Tgt Ion:146 Resp: 438
Ion Ratio Lower Upper
146 100
111 0.0 21.3 63.7#
148 42.0 31.8 95.4

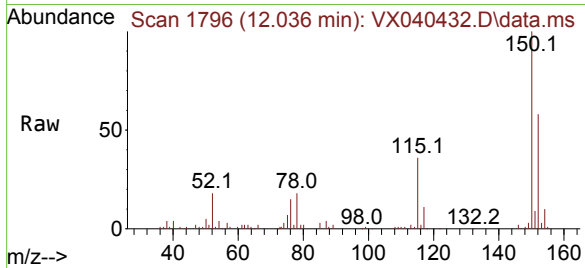

#93
1,2,4-Trichlorobenzene
Concen: 0.219 ug/l
RT: 13.597 min Scan# 2052
Delta R.T. 0.012 min
Lab File: VX040432.D
Acq: 23 Feb 2024 15:23

Tgt Ion:180 Resp: 274
Ion Ratio Lower Upper
180 100
182 64.6 48.3 144.8
145 0.0 18.0 54.0#

