
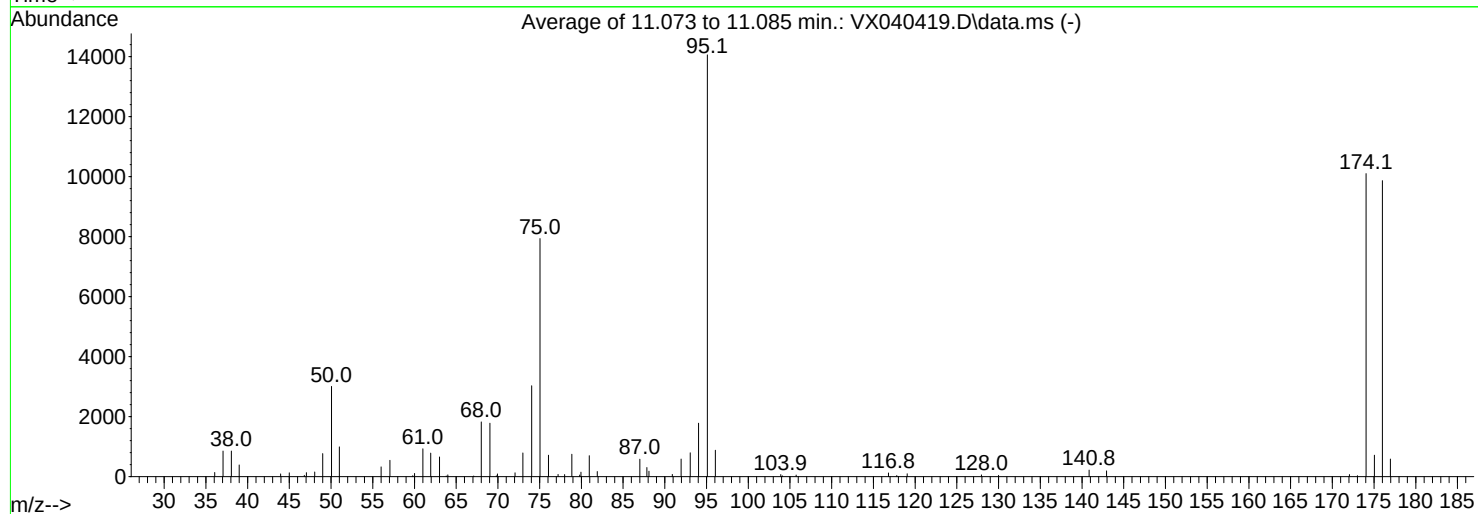


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022324\
Data File : VX040419.D
Acq On : 23 Feb 2024 09:01
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022224W.M
Title : SW846 8260
Last Update : Fri Feb 23 06:47:29 2024

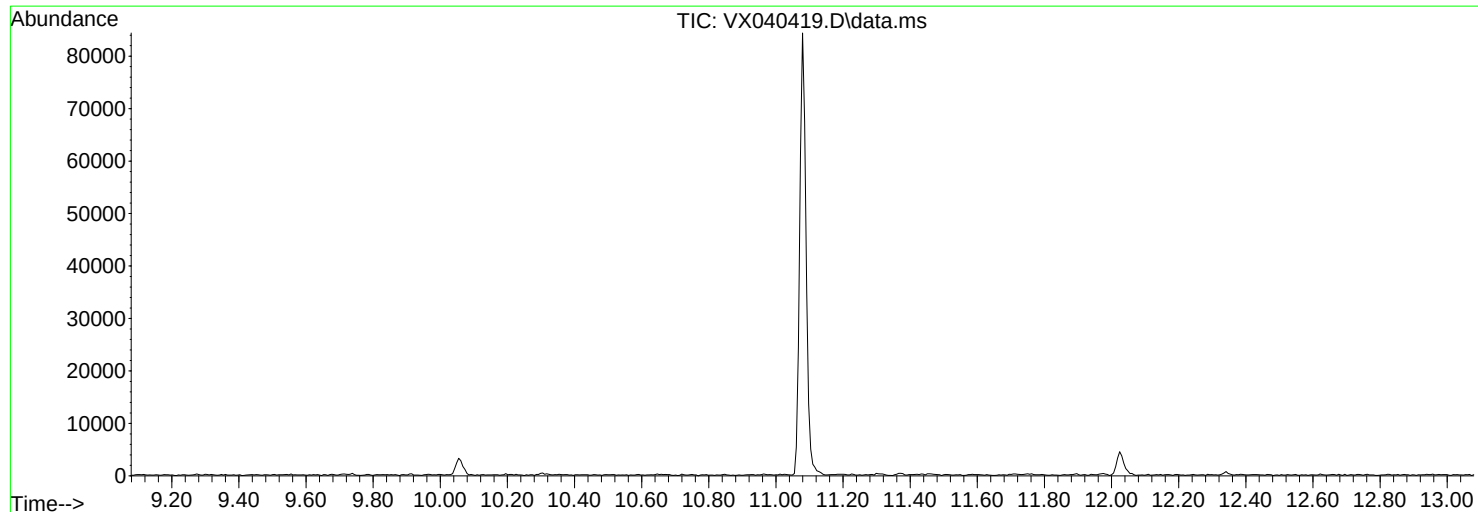

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.4	3006	PASS
75	95	30	60	56.4	7936	PASS
95	95	100	100	100.0	14061	PASS
96	95	5	9	6.3	882	PASS
173	174	0.00	2	0.3	30	PASS
174	95	50	100	71.9	10104	PASS
175	174	5	9	7.1	715	PASS
176	174	95	101	97.7	9870	PASS
177	176	5	9	6.0	588	PASS