


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX022420\
 Data File : VX014997.D
 Acq On : 24 Feb 2020 09:20
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
 Title : SW846 8260
 Last Update : Mon Feb 10 12:09:20 2020

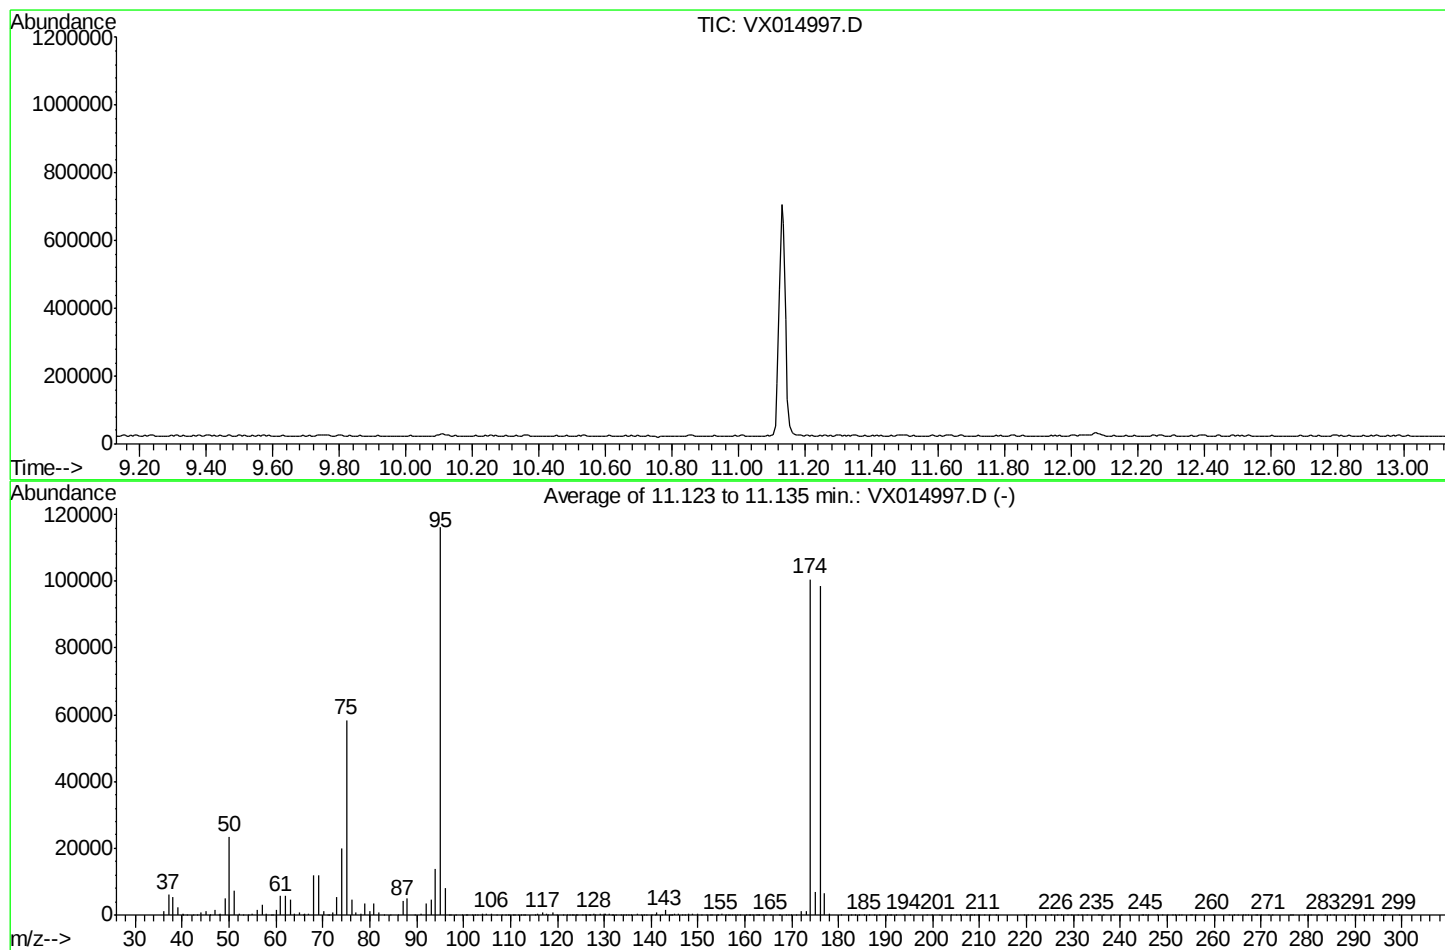

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1670

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	23509	PASS
75	95	30	60	50.4	58504	PASS
95	95	100	100	100.0	116170	PASS
96	95	5	9	6.9	8062	PASS
173	174	0.00	2	1.2	1177	PASS
174	95	50	100	86.6	100594	PASS
175	174	5	9	7.0	7055	PASS
176	174	95	101	97.9	98434	PASS
177	176	5	9	6.7	6593	PASS