


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022421\
Data File : VX020893.D
Acq On : 24 Feb 2021 10:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Title : SW846 8260
Last Update : Wed Feb 24 13:50:55 2021

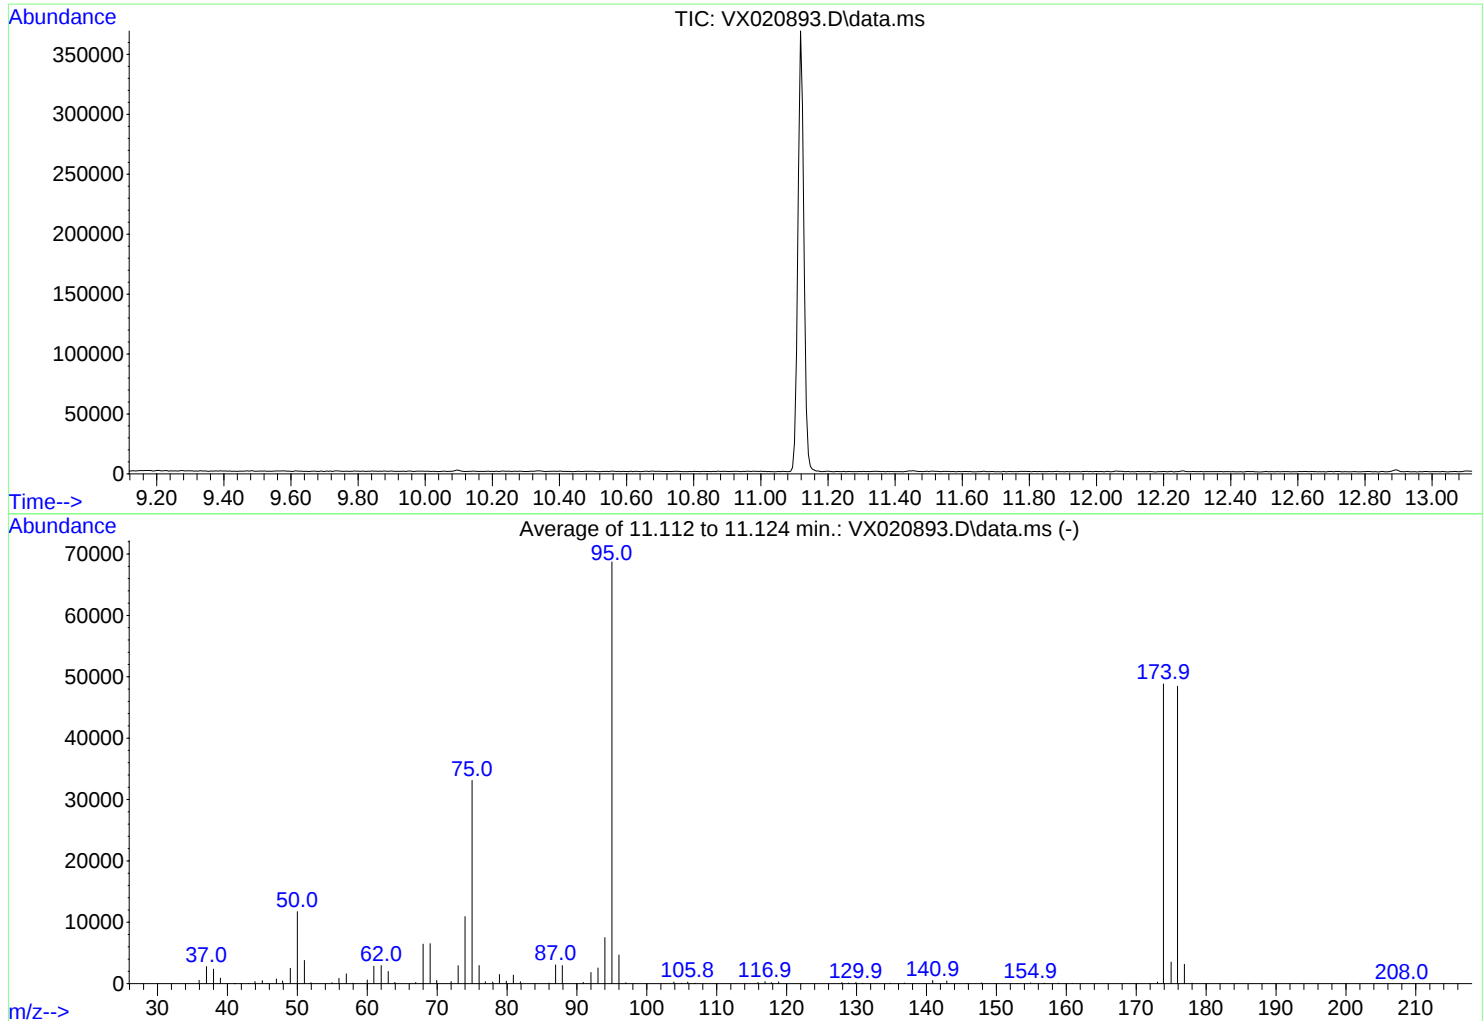

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	11729	PASS
75	95	30	60	48.2	33101	PASS
95	95	100	100	100.0	68728	PASS
96	95	5	9	6.8	4670	PASS
173	174	0.00	2	0.5	254	PASS
174	95	50	100	71.1	48840	PASS
175	174	5	9	7.2	3508	PASS
176	174	95	101	99.3	48475	PASS
177	176	5	9	6.5	3153	PASS