

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022422\
 Data File : VX027168.D
 Acq On : 24 Feb 2022 14:23
 Operator : JC/MD
 Sample : N1659-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-3-MH

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Title : SW846 8260

Signal : TIC: VX027168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.385	207	213	222	rBV	8263	13442	2.97%	0.526%
2	5.391	695	706	720	rBV2	52050	149127	32.99%	5.838%
3	5.556	722	733	747	rBV2	93200	259517	57.41%	10.160%
4	5.964	789	800	819	rVB	56243	146823	32.48%	5.748%
5	6.763	922	931	943	rBV	139059	334088	73.90%	13.079%
6	8.579	1224	1229	1234	rVB2	2832	4552	1.01%	0.178%
7	8.653	1234	1241	1249	rBV	287460	452066	100.00%	17.698%
8	10.055	1465	1471	1485	rBV	305180	401341	88.78%	15.712%
9	11.085	1634	1640	1650	rBV	233969	313900	69.44%	12.289%
10	12.024	1788	1794	1801	rBV	327345	392961	86.93%	15.384%
11	13.170	1975	1982	1984	rBV6	2416	4668	1.03%	0.183%
12	13.292	1989	2002	2013	rVB6	10876	48526	10.73%	1.900%
13	13.511	2031	2038	2040	rBV5	3106	6756	1.49%	0.264%
14	14.231	2144	2156	2160	rBV9	3590	7745	1.71%	0.303%
15	15.334	2332	2337	2339	rBV4	2812	5337	1.18%	0.209%
16	15.487	2357	2362	2368	rBV6	3744	6665	1.47%	0.261%
17	16.377	2501	2508	2513	rBV3	3644	6819	1.51%	0.267%




Sum of corrected areas: 2554333

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022422\
Data File : VX027168.D
Acq On : 24 Feb 2022 14:23
Operator : JC/MD
Sample : N1659-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-3-MH

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

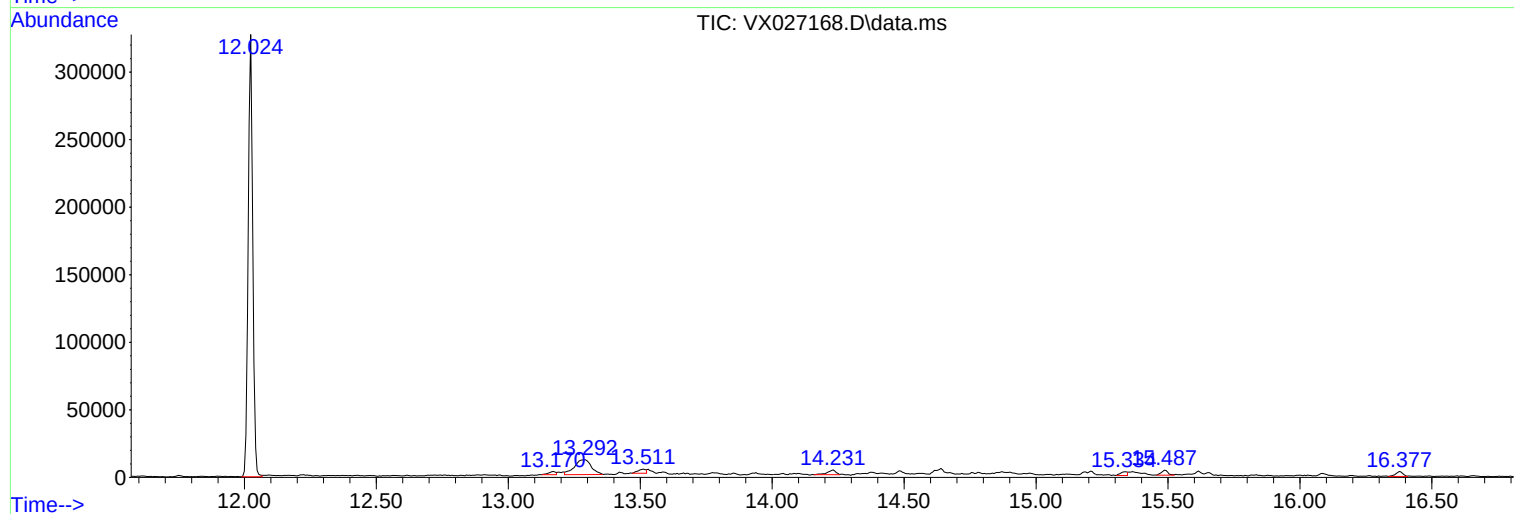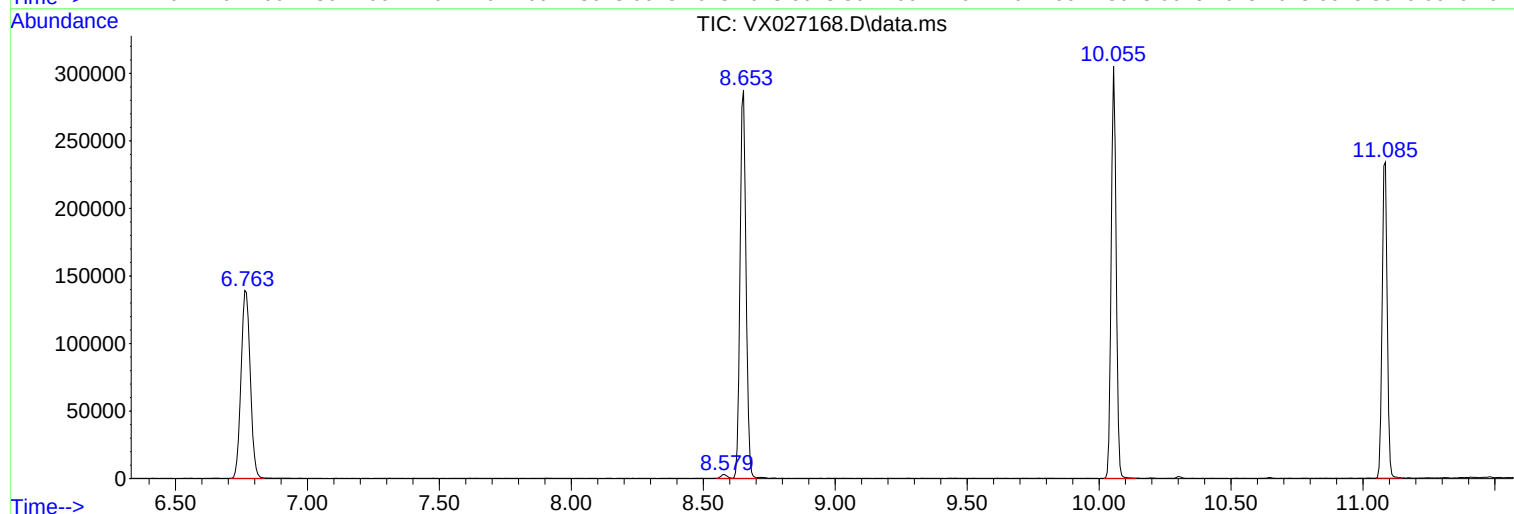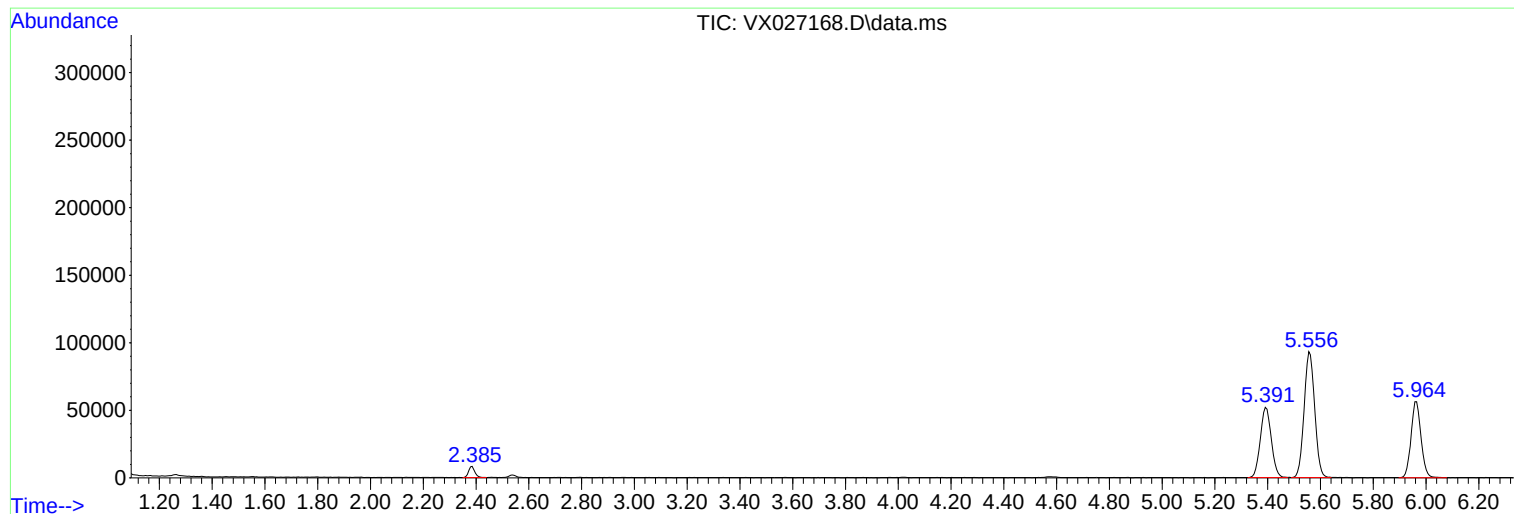

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022422\
Data File : VX027168.D
Acq On : 24 Feb 2022 14:23
Operator : JC/MD
Sample : N1659-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-3-MH










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tridecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.292	6.17 ug/l	48526	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tridecane	184	C13H28	000629-50-5	53
2			Dodecane, 2-methyl-	184	C13H28	001560-97-0	49
3			Tridecane, 1-iodo-	310	C13H27I	035599-77-0	46
4			10-Methylnonadecane	282	C20H42	056862-62-5	46
5			Hexacosane	366	C26H54	000630-01-3	43

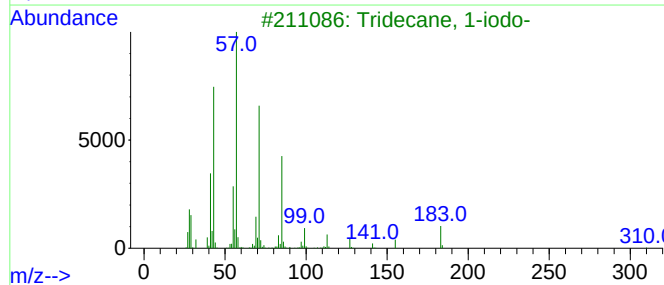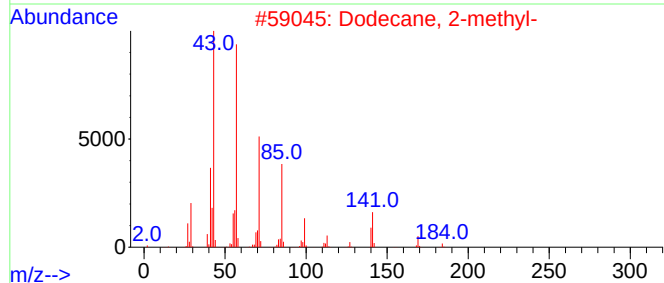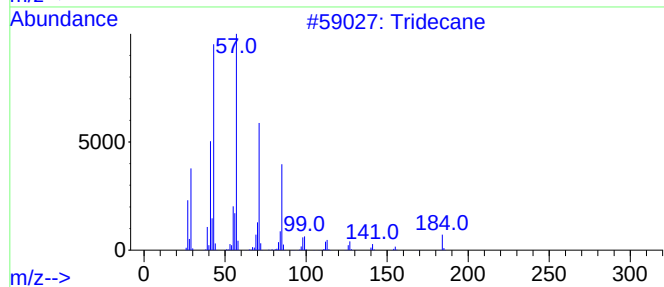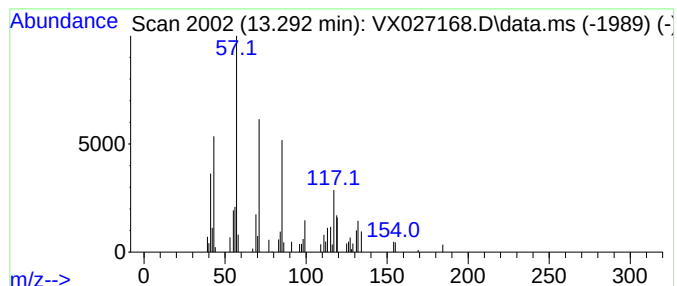

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022422\
Data File : VX027168.D
Acq On : 24 Feb 2022 14:23
Operator : JC/MD
Sample : N1659-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-3-MH

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tridecane	13.292	6.2	ug/l	48526	4	12.024	392961	50.0