

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022422\
 Data File : VX027178.D
 Acq On : 24 Feb 2022 18:23
 Operator : JC/MD
 Sample : N1668-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PURGED-WATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Title : SW846 8260

Signal : TIC: VX027178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.752	105	109	116	rBV	16202	22537	4.78%	0.822%
2	2.386	208	213	221	rVB	9549	15754	3.34%	0.575%
3	2.538	231	238	246	rBV	6162	11357	2.41%	0.414%
4	2.623	246	252	265	rVV	6052	13270	2.81%	0.484%
5	2.788	271	279	282	rBV4	3842	8171	1.73%	0.298%
6	2.867	289	292	300	rVB	4640	8867	1.88%	0.323%
7	3.105	321	331	342	rVB3	7096	19226	4.07%	0.701%
8	4.306	520	528	538	rVB2	8036	22569	4.78%	0.823%
9	5.391	695	706	715	rBV	54307	155372	32.93%	5.667%
10	5.477	715	720	725	rVV	10548	28462	6.03%	1.038%
11	5.556	725	733	752	rVB	96730	273866	58.05%	9.989%
12	5.849	773	781	789	rBV6	1943	5671	1.20%	0.207%
13	5.958	789	799	809	rVV	56930	152720	32.37%	5.570%
14	6.044	809	813	823	rVB	5311	12978	2.75%	0.473%
15	6.251	840	847	858	rVB6	2313	6995	1.48%	0.255%
16	6.361	858	865	872	rBV6	2359	6089	1.29%	0.222%
17	6.763	922	931	944	rBV	145934	346446	73.43%	12.636%
18	7.385	1024	1033	1040	rBV3	9464	22309	4.73%	0.814%
19	8.580	1221	1229	1234	rBV2	4388	9020	1.91%	0.329%
20	8.653	1234	1241	1248	rVV	307116	471809	100.00%	17.209%
21	8.720	1248	1252	1257	rVB	2681	4723	1.00%	0.172%
22	9.037	1299	1304	1311	rBV3	2324	5149	1.09%	0.188%
23	10.055	1463	1471	1479	rBV	312430	408689	86.62%	14.907%
24	11.079	1634	1639	1649	rBV	239227	310985	65.91%	11.343%
25	12.024	1788	1794	1801	rBV	319916	387863	82.21%	14.147%
26	12.244	1827	1830	1834	rVB2	4803	5708	1.21%	0.208%
27	12.701	1900	1905	1912	rVB2	3184	5043	1.07%	0.184%




Sum of corrected areas: 2741648

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022422\
Data File : VX027178.D
Acq On : 24 Feb 2022 18:23
Operator : JC/MD
Sample : N1668-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PURGED-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

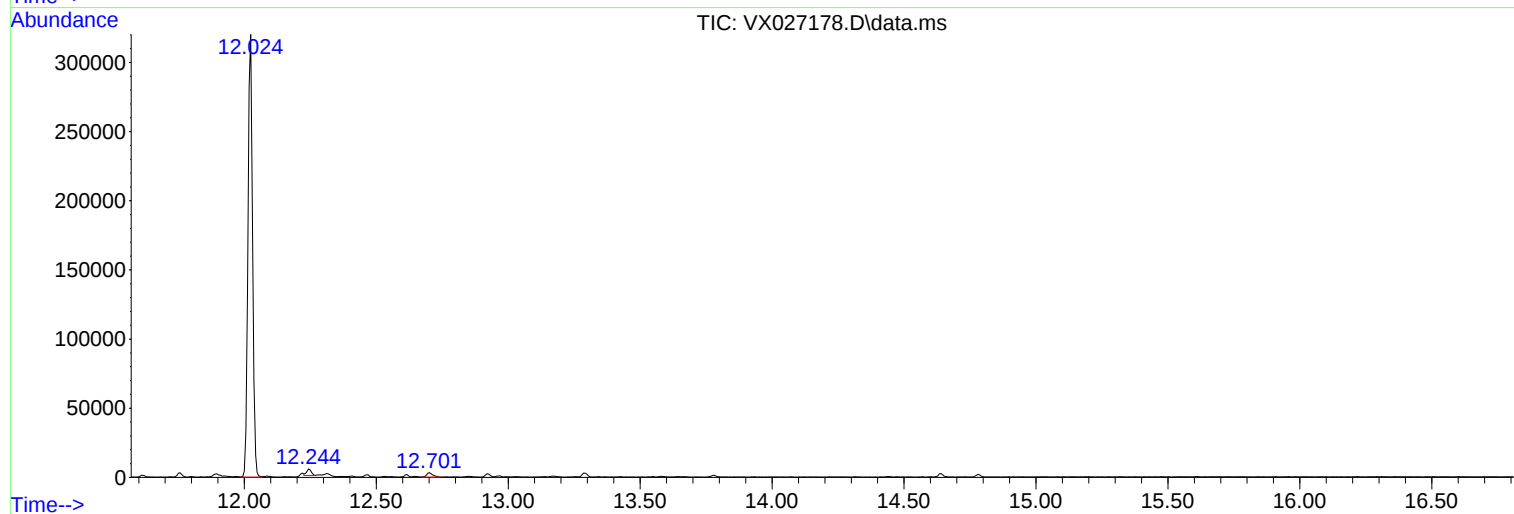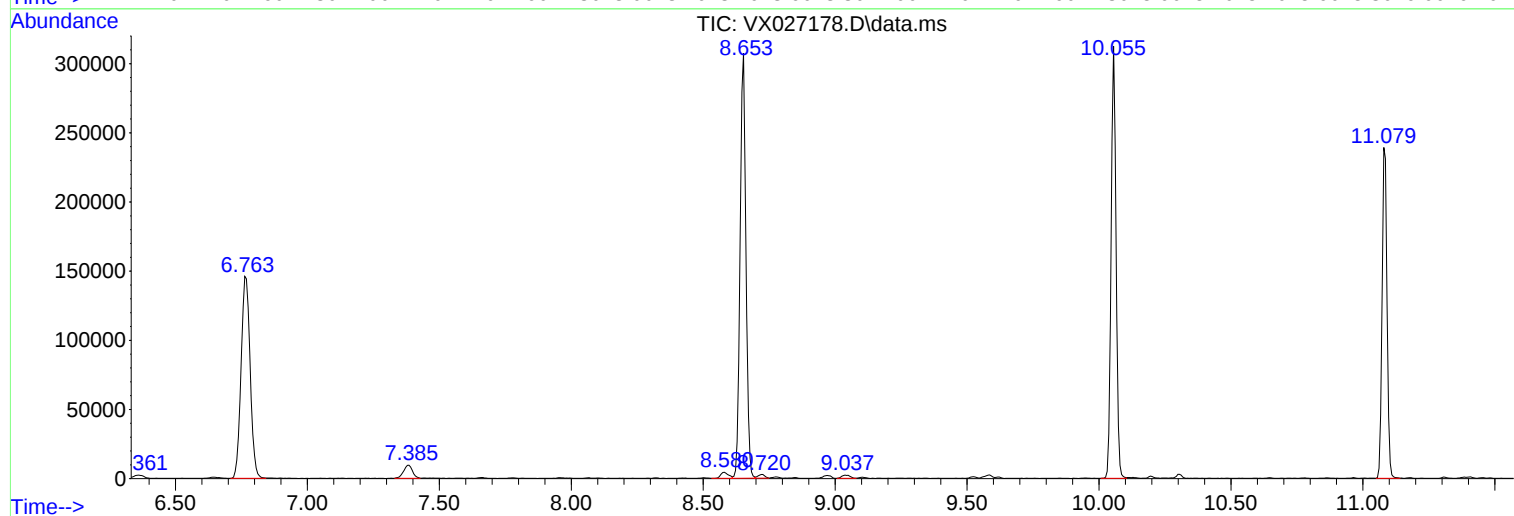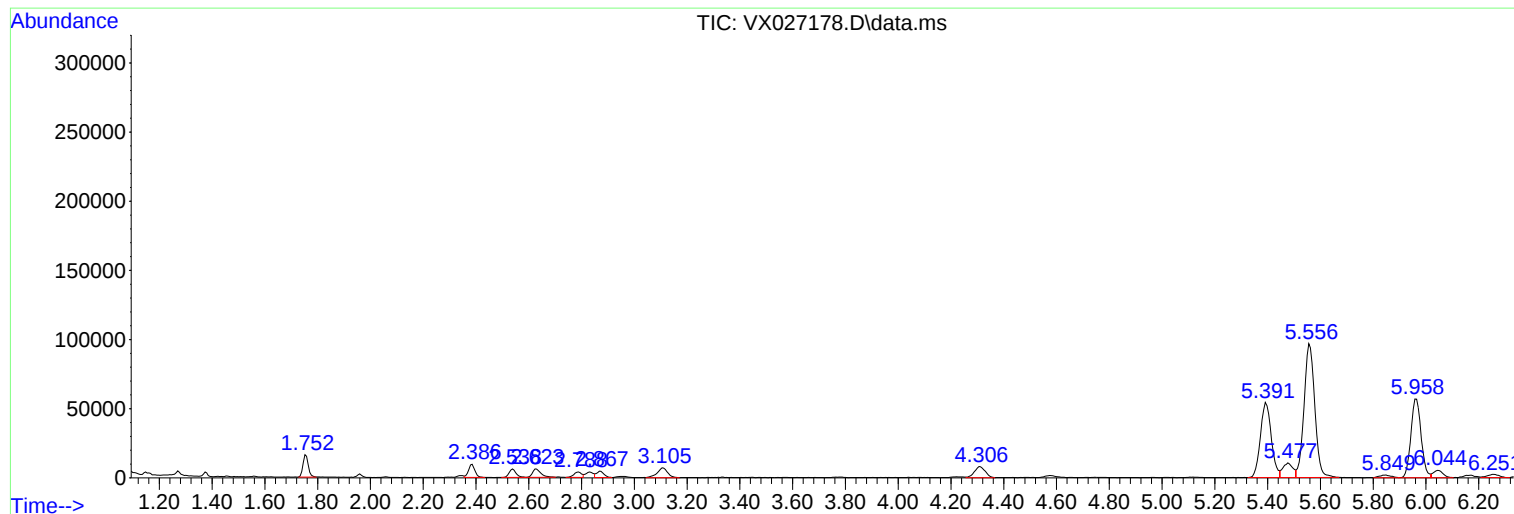

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022422\
Data File : VX027178.D
Acq On : 24 Feb 2022 18:23
Operator : JC/MD
Sample : N1668-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PURGED-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022422\
Data File : VX027178.D
Acq On : 24 Feb 2022 18:23
Operator : JC/MD
Sample : N1668-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PURGED-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------