

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022423\
Data File : VX034256.D
Acq On : 24 Feb 2023 11:12
Operator : JC/MD
Sample : VX0224MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0224MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Title : SW846 8260

Signal : TIC: VX034256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.557	72	77	84	rBV4	8518	15542	1.05%	0.206%
2	4.550	563	568	579	rVB2	4934	14936	1.01%	0.198%
3	5.385	692	705	719	rBV	165388	488340	33.13%	6.470%
4	5.550	721	732	745	rVV	278649	788874	53.52%	10.452%
5	5.952	787	798	810	rBV2	182539	490441	33.27%	6.498%
6	6.757	920	930	949	rBV	444462	1066495	72.35%	14.131%
7	8.647	1233	1240	1260	rBV	963500	1474115	100.00%	19.532%
8	10.055	1465	1471	1487	rBV	851030	1217858	82.62%	16.136%
9	11.079	1634	1639	1650	rBV	697545	908865	61.65%	12.042%
10	12.024	1788	1794	1802	rBV	816156	1081890	73.39%	14.335%




Sum of corrected areas: 7547356

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022423\
Data File : VX034256.D
Acq On : 24 Feb 2023 11:12
Operator : JC/MD
Sample : VX0224MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0224MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

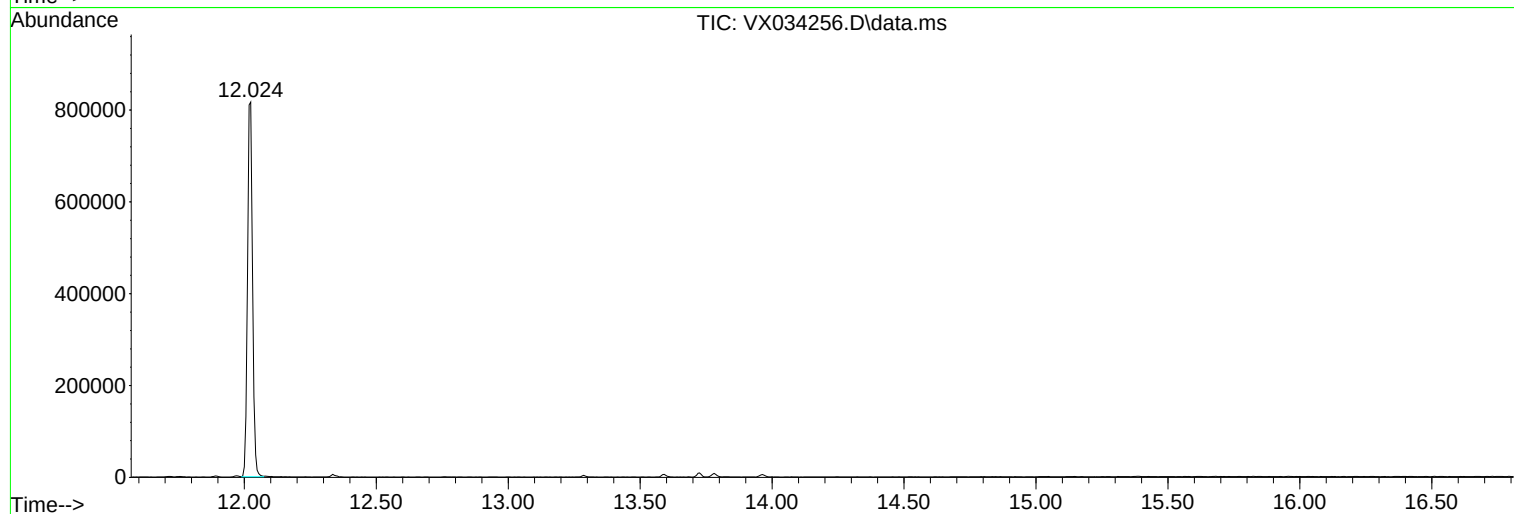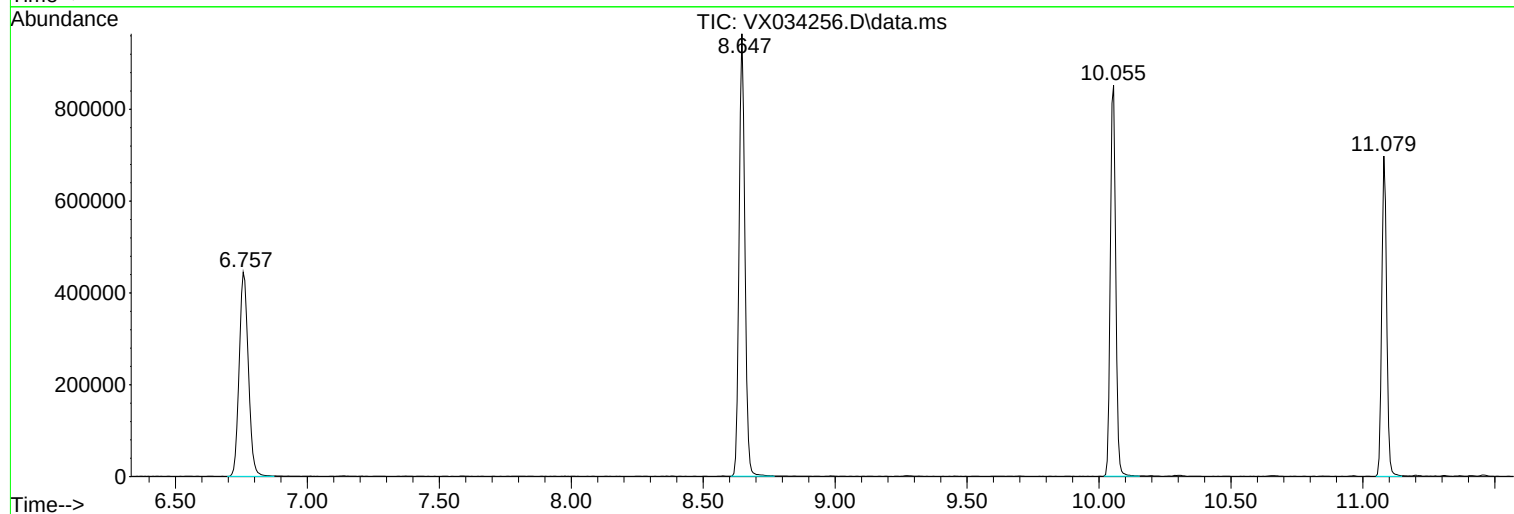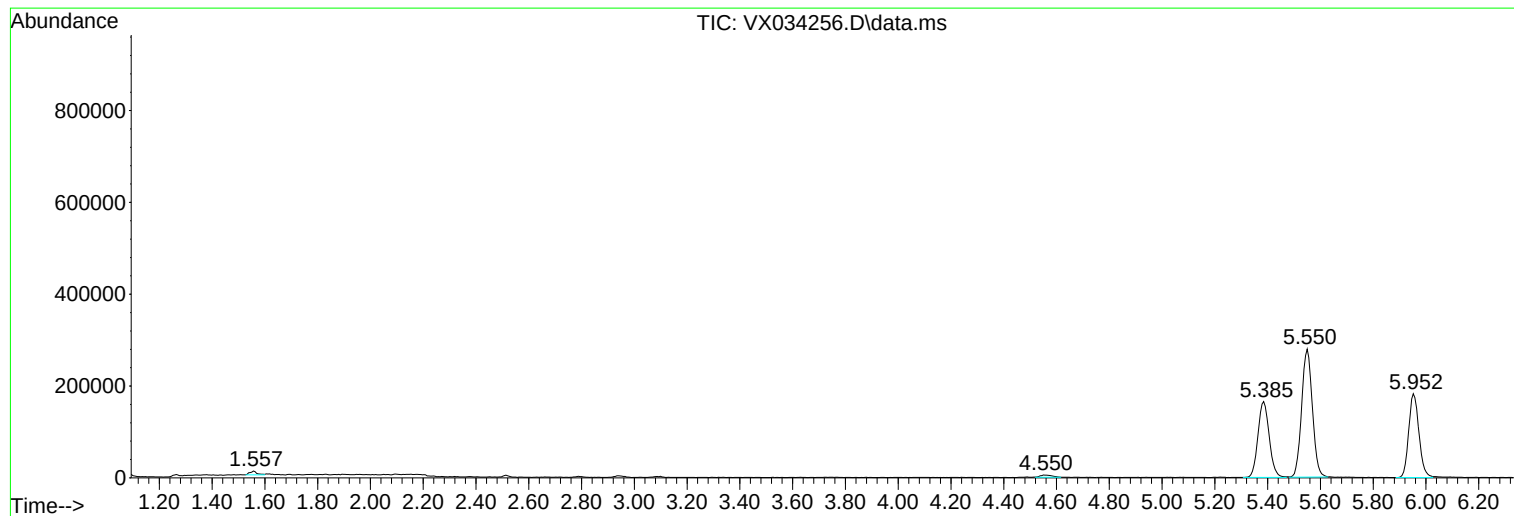

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022423\
Data File : VX034256.D
Acq On : 24 Feb 2023 11:12
Operator : JC/MD
Sample : VX0224MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0224MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022423\
Data File : VX034256.D
Acq On : 24 Feb 2023 11:12
Operator : JC/MD
Sample : VX0224MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0224MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc