



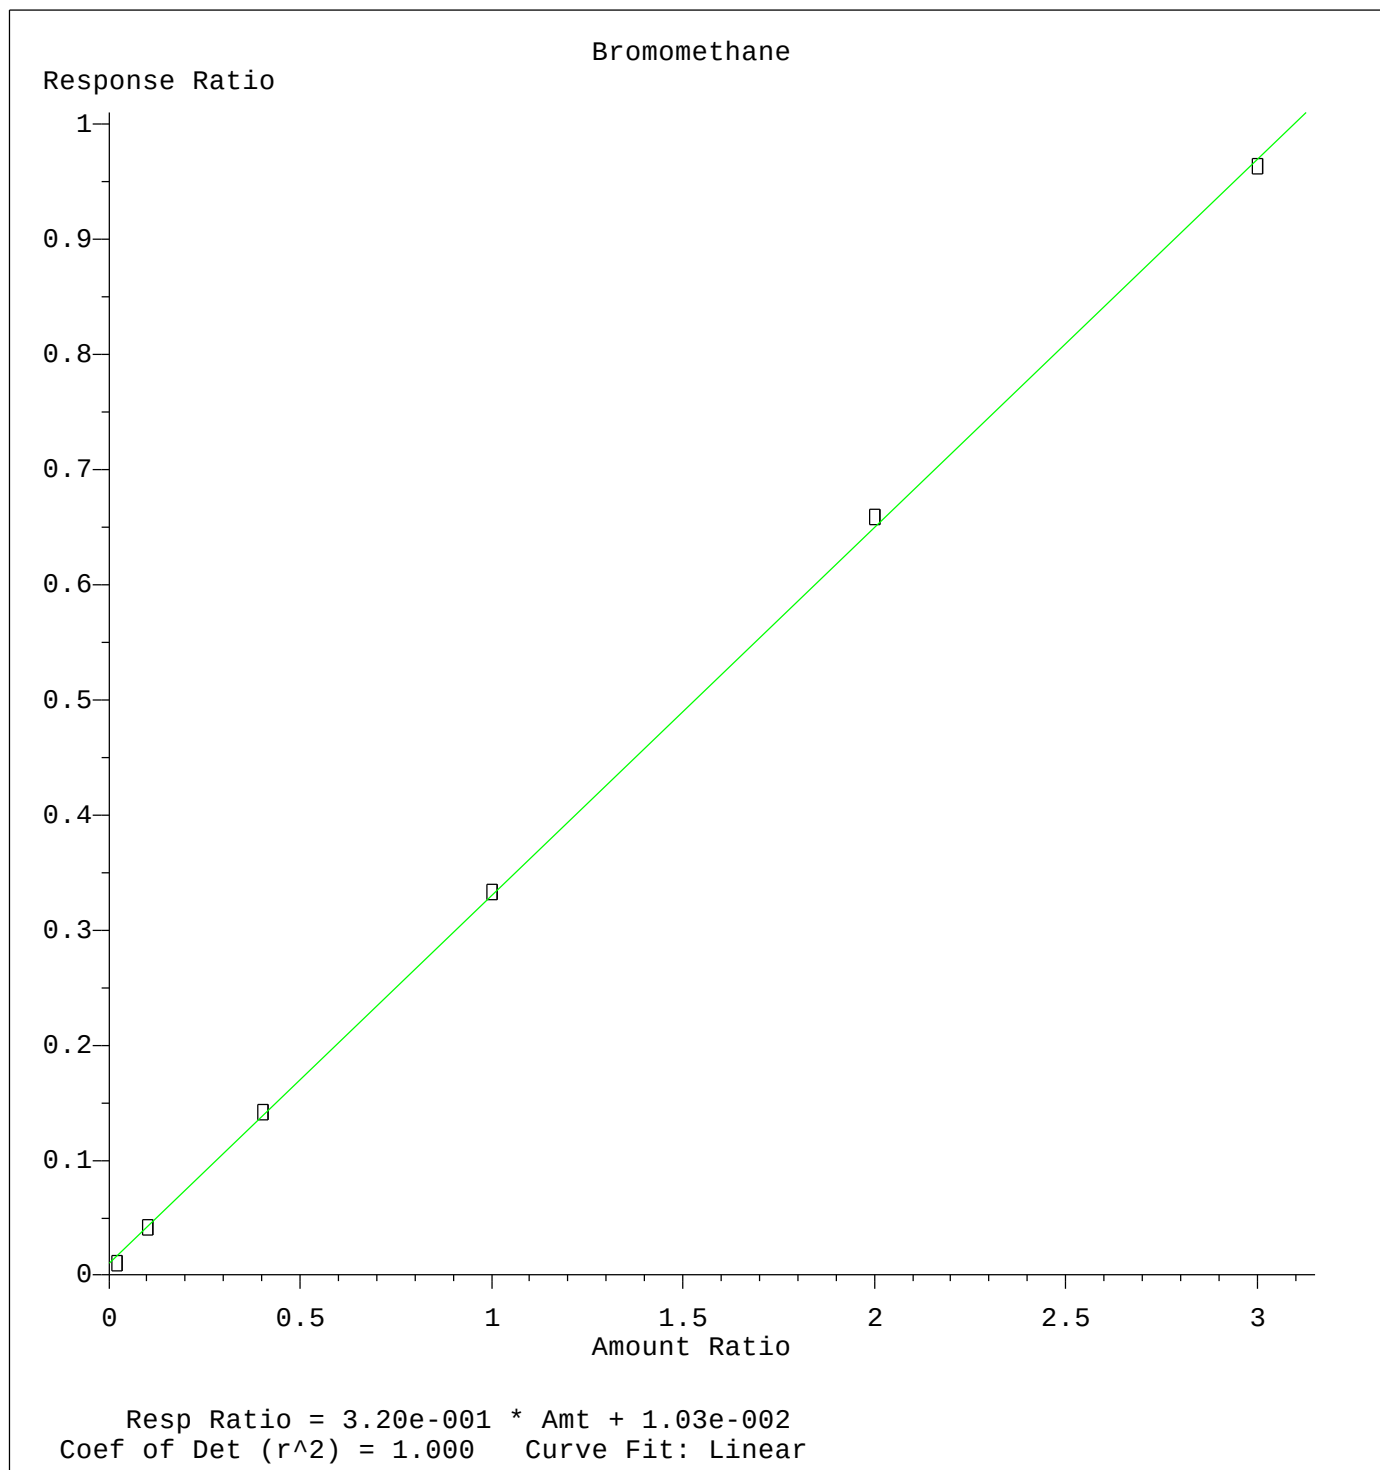

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X022519W.M
Calibration Table Last Updated: Tue Feb 26 01:53:13 2019

t-1,3-Dichloropropene

Response Ratio

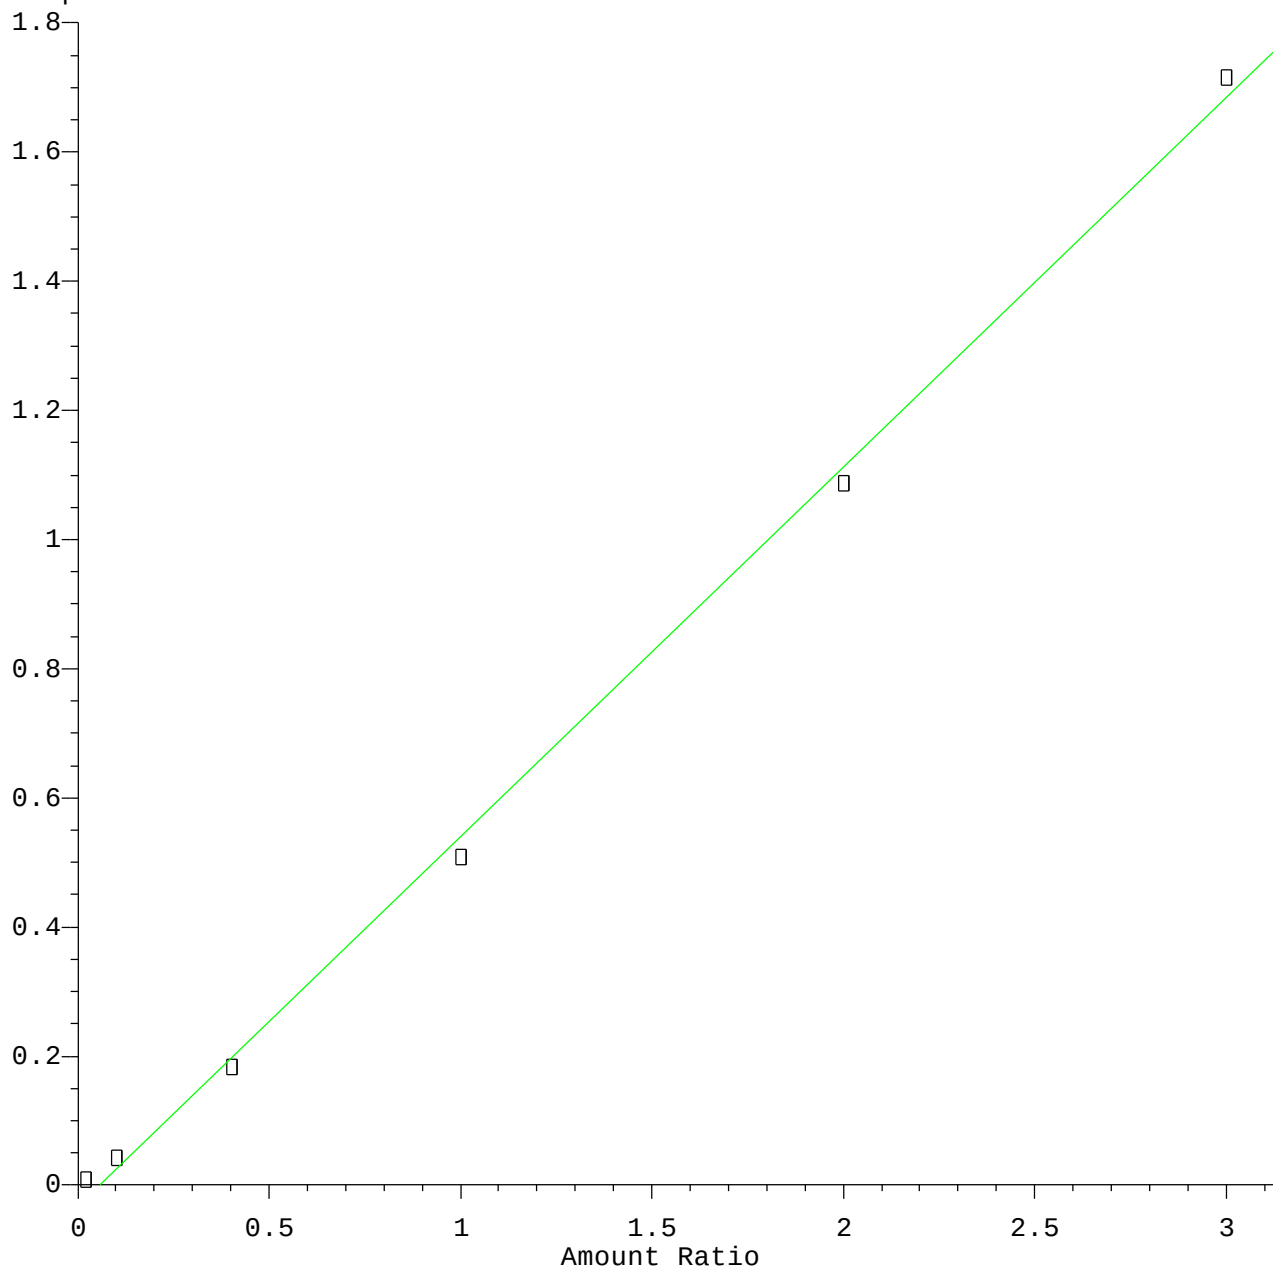


Resp Ratio = 5.72e-001 * Amt - 3.21e-002
Coef of Det (r²) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X022519W.M
Calibration Table Last Updated: Tue Feb 26 01:53:13 2019

trans-1,4-Dichloro-2-butene

Response Ratio

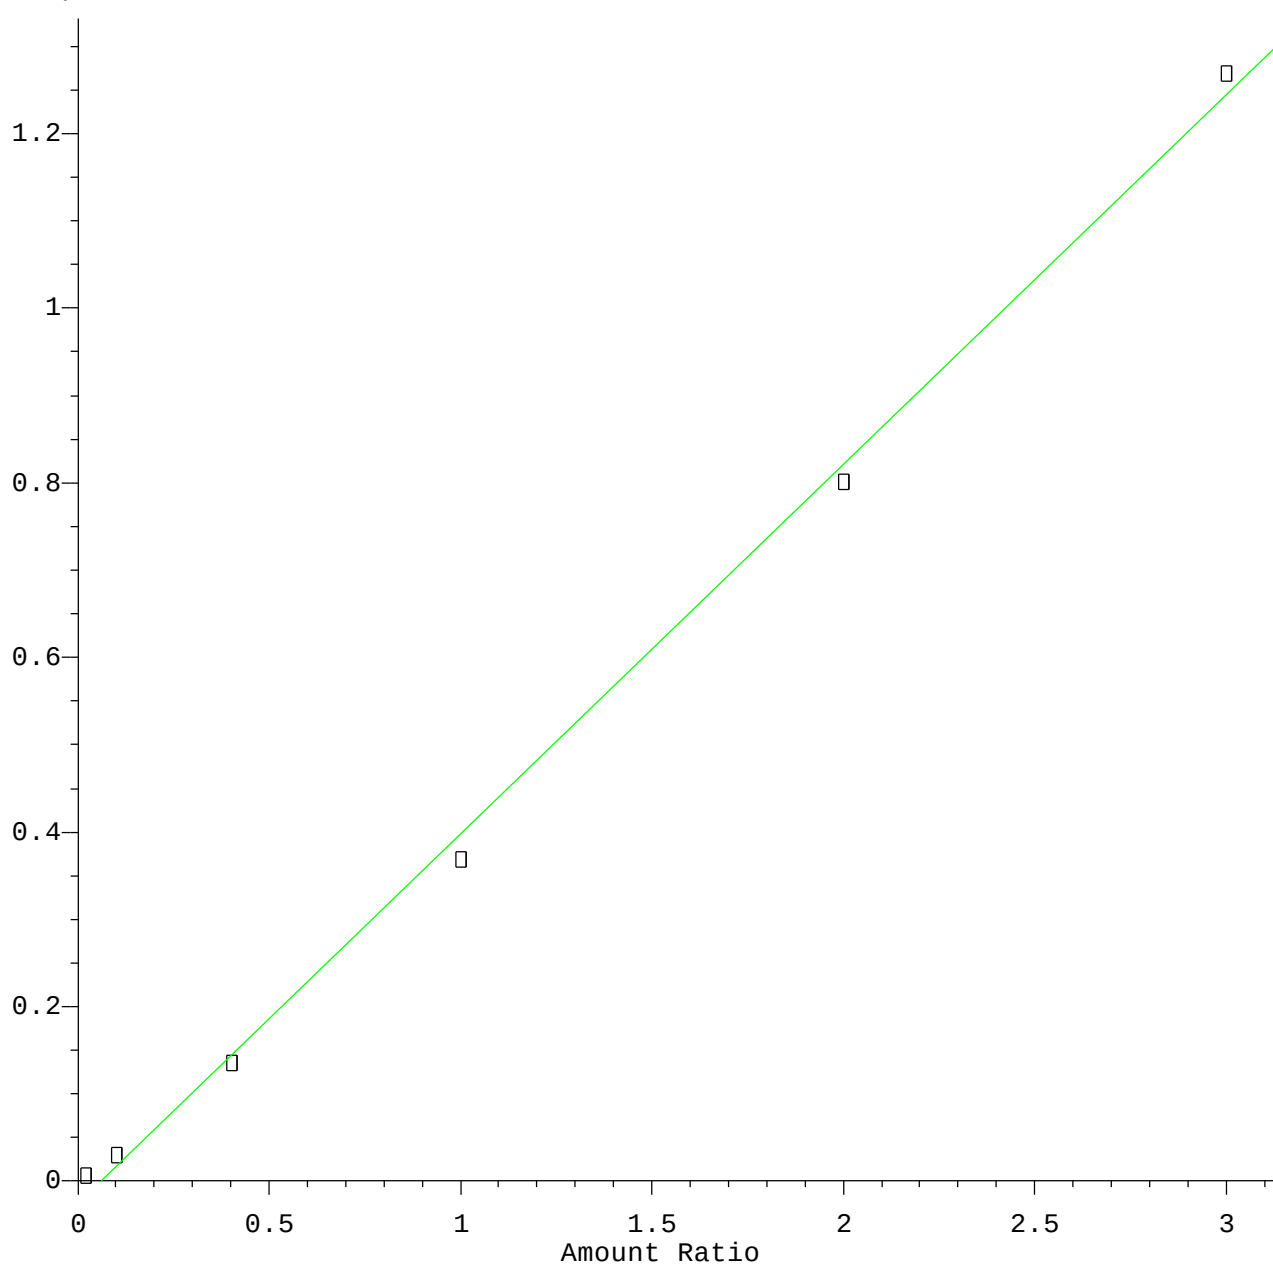

Resp Ratio = $4.23 \times 10^{-1} \times \text{Amt} - 2.55 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X022519W.M
Calibration Table Last Updated: Tue Feb 26 01:53:13 2019