


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX022519\
Data File : VX007661.D
Acq On : 25 Feb 2019 09:09
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X022519W.M
Title : SW846 8260
Last Update : Tue Feb 26 01:53:13 2019

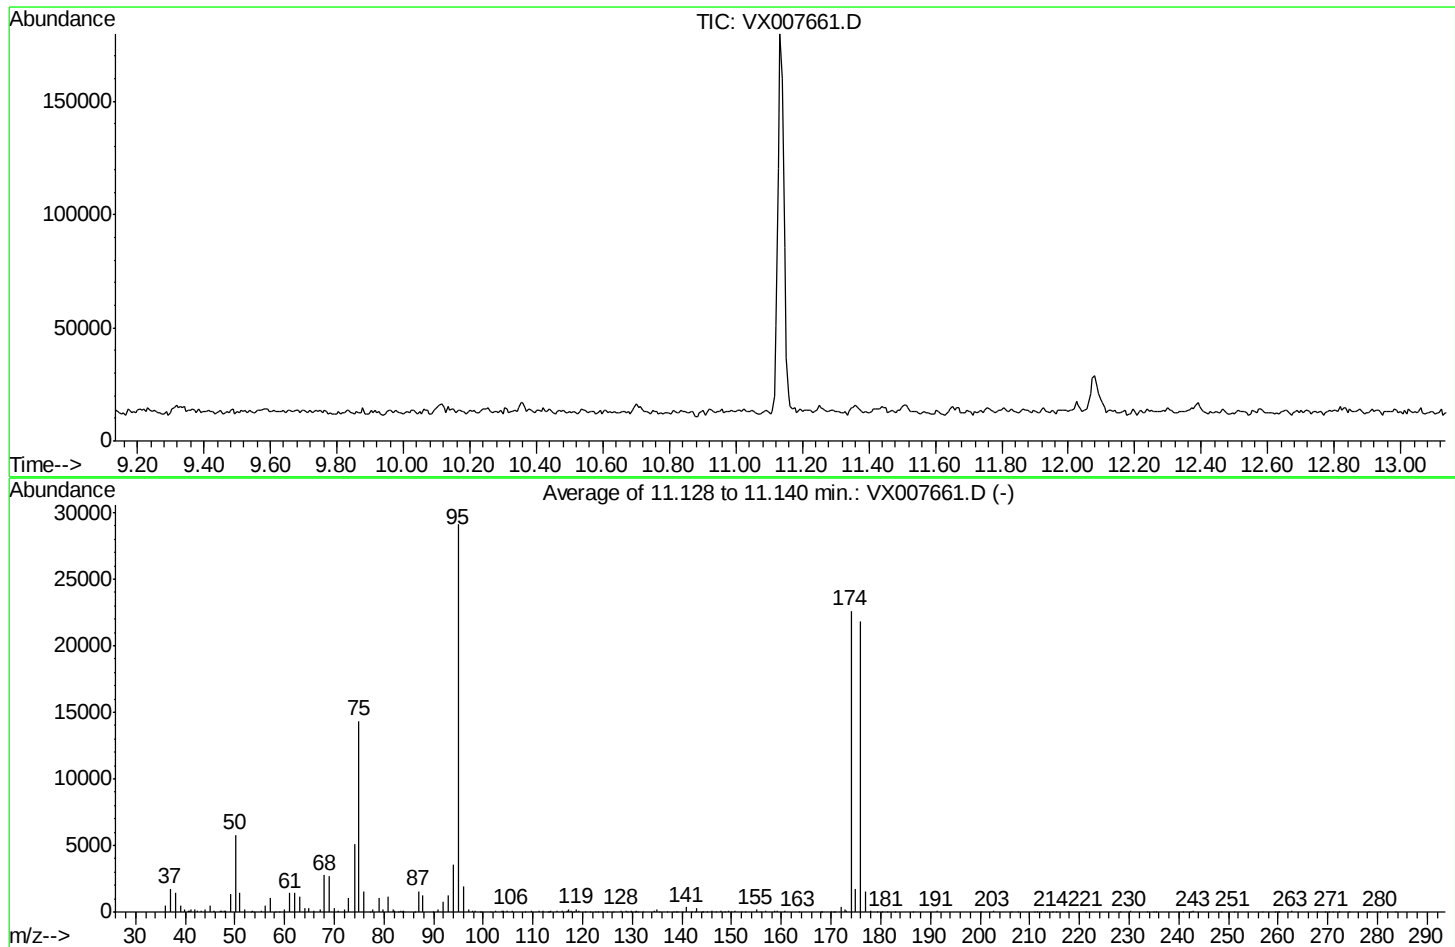

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	5812	PASS
75	95	30	60	49.4	14376	PASS
95	95	100	100	100.0	29122	PASS
96	95	5	9	6.5	1889	PASS
173	174	0.00	2	1.0	233	PASS
174	95	50	100	77.7	22618	PASS
175	174	5	9	7.7	1740	PASS
176	174	95	101	96.6	21851	PASS
177	176	5	9	7.1	1551	PASS