
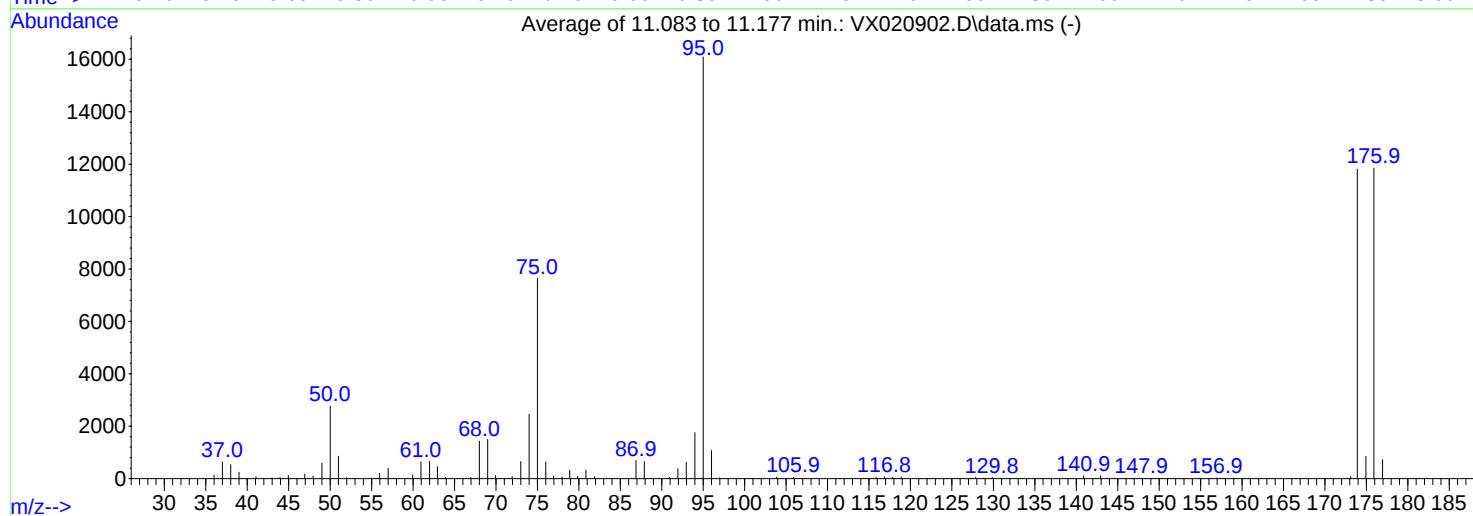


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022521\
 Data File : VX020902.D
 Acq On : 25 Feb 2021 08:51
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X022521W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Feb 25 13:26:35 2021

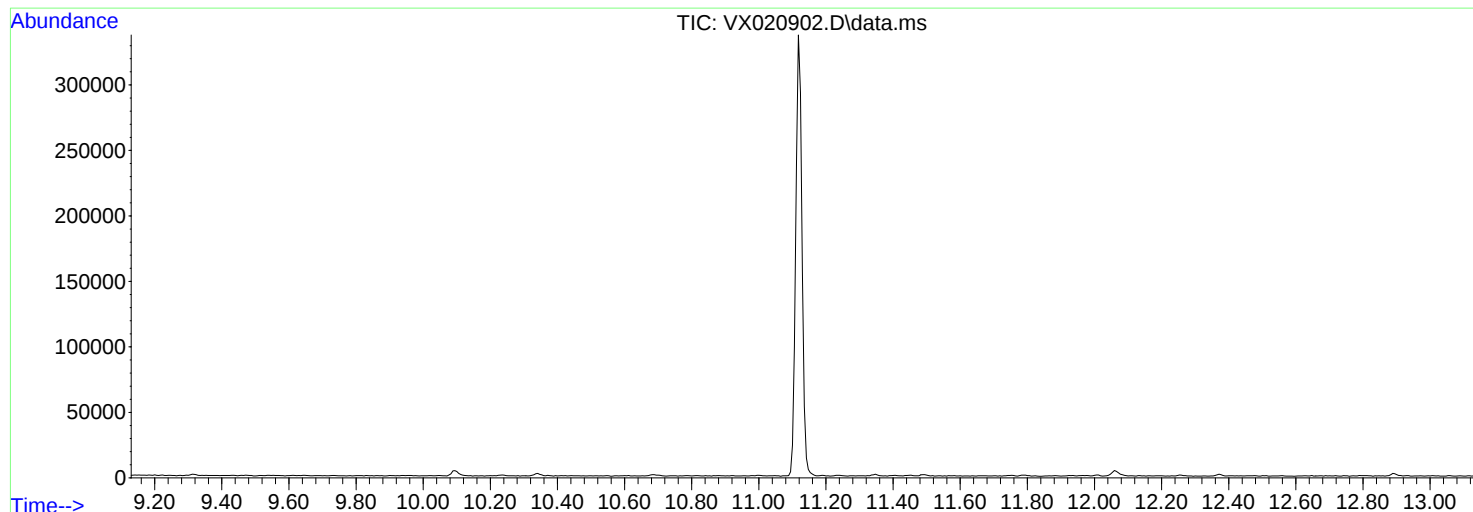

AutoFind: Averaged scan 1699 to 1715; Bkg corrected with scan 1698

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	2768	PASS
75	95	30	60	47.5	7642	PASS
95	95	100	100	100.0	16095	PASS
96	95	5	9	6.7	1074	PASS
173	174	0.00	2	0.7	78	PASS
174	95	50	100	73.4	11815	PASS
175	174	5	9	7.2	849	PASS
176	174	95	101	100.3	11854	PASS
177	176	5	9	6.1	726	PASS