

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022522\
 Data File : VX027213.D
 Acq On : 26 Feb 2022 01:28
 Operator : JC/MD
 Sample : N1584-07ME
 Misc : 5.35g/5.0mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 D13-7.5ME

Quant Time: Feb 26 02:49:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 23 13:06:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	95792	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	160791	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	147042	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	74750	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	57400	49.893	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	99.780%		
35) Dibromofluoromethane	5.397	113	46833	46.924	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	93.840%		
50) Toluene-d8	8.653	98	187557	50.258	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	100.520%		
62) 4-Bromofluorobenzene	11.085	95	73061	51.003	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	102.000%		
Target Compounds					Qvalue	
5) Bromomethane	1.605	94	133	Below Cal		82
11) Tert butyl alcohol	2.947	59	172	0.768 ug/l #		75
14) Allyl chloride	2.770	41	527	0.321 ug/l #		68
16) Acetone	2.416	43	423	0.837 ug/l #		46
18) Methyl Acetate	2.764	43	2575	1.975 ug/l #		53
20) Methylene Chloride	2.788	84	334	0.319 ug/l #		82
25) 2-Butanone	4.611	43	465	0.578 ug/l #		50
30) Chloroform	5.160	83	585	0.311 ug/l #		18
31) Cyclohexane	5.495	56	3355	1.947 ug/l #		49
36) 1,1-Dichloropropene	5.556	75	7108	4.880 ug/l #		51
38) Carbon Tetrachloride	5.556	117	9659	6.358 ug/l #		17
39) Methylcyclohexane	7.373	83	5340	2.947 ug/l		95
43) Isopropyl Acetate	6.239	43	8832	3.590 ug/l #		62
51) 4-Methyl-2-Pentanone	8.616	43	2659	1.663 ug/l #		54
52) Toluene	8.720	92	9940	3.644 ug/l		100
53) t-1,3-Dichloropropene	8.915	75	129	3.045 ug/l #		1
55) 1,1,2-Trichloroethane	9.104	97	2121	1.963 ug/l #		20
56) Ethyl methacrylate	9.104	69	610	0.363 ug/l #		19
59) 2-Hexanone	9.384	43	1450	1.186 ug/l #		25
67) Ethyl Benzene	10.195	91	22494	4.275 ug/l		98
68) m/p-Xylenes	10.305	106	25036	12.376 ug/l		97
69) o-Xylene	10.646	106	8129	4.004 ug/l		99
73) Isopropylbenzene	10.963	105	9569	1.789 ug/l		97
74) N-amyl acetate	10.860	43	664	0.326 ug/l #		1
76) 1,2,3-Trichloropropane	11.317	75	1325	0.880 ug/l #		24
78) n-propylbenzene	11.305	91	24093	3.963 ug/l		98
79) 2-Chlorotoluene	11.378	91	6740	1.809 ug/l #		42
80) 1,3,5-Trimethylbenzene	11.457	105	22060	4.905 ug/l		100
81) trans-1,4-Dichloro-2-b...	11.085	75	35224	66.579 ug/l #		4
82) 4-Chlorotoluene	11.451	91	2411	0.567 ug/l #		46
83) tert-Butylbenzene	11.756	119	6902	1.578 ug/l #		64
84) 1,2,4-Trimethylbenzene	11.756	105	57459	12.843 ug/l		97
85) sec-Butylbenzene	11.890	105	3662	0.668 ug/l		89
86) p-Isopropyltoluene	11.975	119	2180	0.466 ug/l		93
89) n-Butylbenzene	12.335	91	11091	2.839 ug/l #		43
90) Hexachloroethane	12.536	117	1096	1.514 ug/l #		14


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022522\
Data File : VX027213.D
Acq On : 26 Feb 2022 01:28
Operator : JC/MD
Sample : N1584-07ME
Misc : 5.35g/5.0mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME

Quant Time: Feb 26 02:49:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 23 13:06:57 2022
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
92) 1,2-Dibromo-3-Chloropr...	12.927	75	82	0.224	ug/l #	3
95) Naphthalene	13.780	128	10549	2.008	ug/l	99





(#) = qualifier out of range (m) = manual integration (+) = signals summed

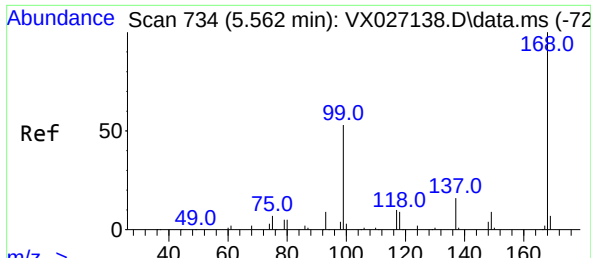

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion:168 Resp: 95792
Ion Ratio Lower Upper
168 100
99 58.0 50.3 75.5

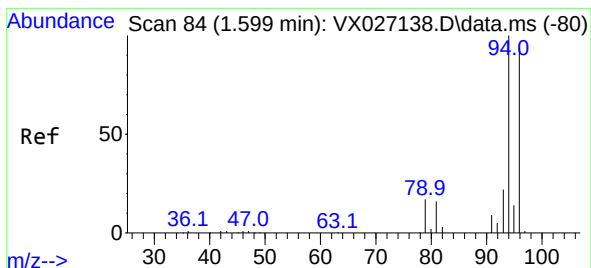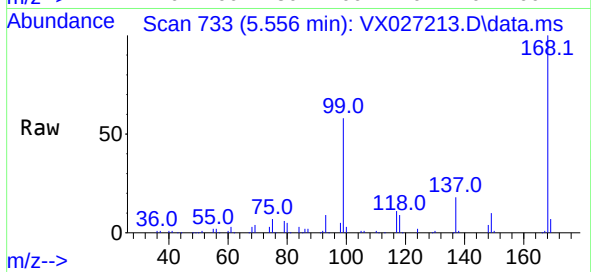

#5
Bromomethane
Concen: Below Cal
RT: 1.605 min Scan# 85
Delta R.T. 0.006 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 94 Resp: 133
Ion Ratio Lower Upper
94 100
96 77.3 75.9 113.9


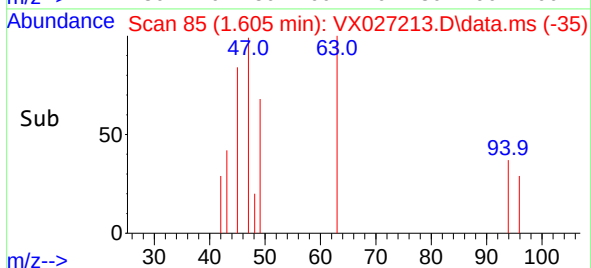
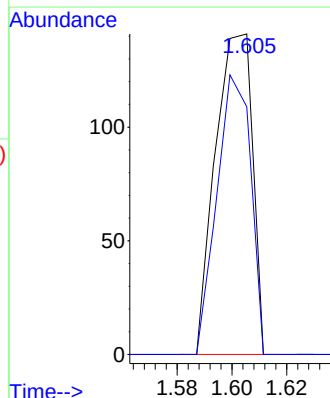
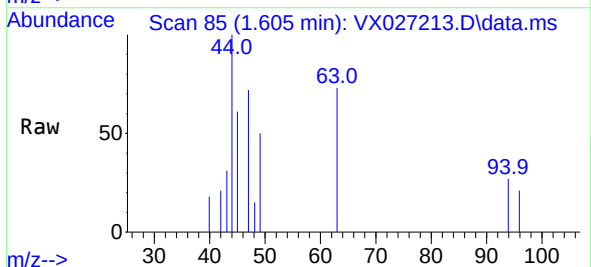




#11
Tert butyl alcohol
Concen: 0.768 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.030 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion: 59 Resp: 172
Ion Ratio Lower Upper
59 100
57 0.0 7.2 10.8#



#14
Allyl chloride
Concen: 0.321 ug/l
RT: 2.770 min Scan# 276
Delta R.T. 0.104 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 41 Resp: 527
Ion Ratio Lower Upper
41 100
39 51.6 54.2 81.4#
76 0.0 25.2 37.8#


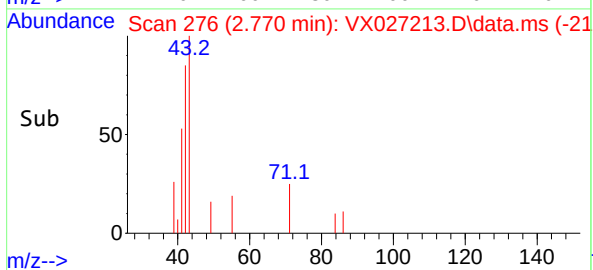






#16
Acetone
Concen: 0.837 ug/l
RT: 2.416 min Scan# 213
Delta R.T. 0.030 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion: 43 Resp: 423
Ion Ratio Lower Upper
43 100
58 0.0 23.0 34.6#



#18
Methyl Acetate
Concen: 1.975 ug/l
RT: 2.764 min Scan# 275
Delta R.T. 0.055 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 43 Resp: 2575
Ion Ratio Lower Upper
43 100
74 0.0 18.3 27.5#


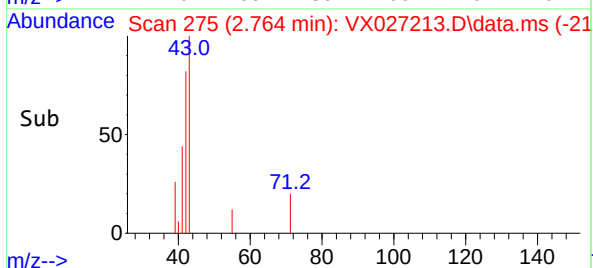






#20
Methylene Chloride
Concen: 0.319 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion:	84	Resp:	334
Ion	Ratio	Lower	Upper
84	100		
49	133.3	101.5	152.3
51	50.0	31.2	46.8#
86	97.8	51.3	76.9#

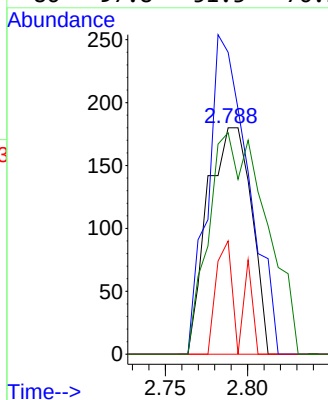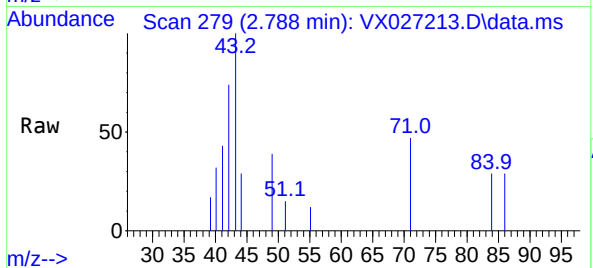

#25
2-Butanone
Concen: 0.578 ug/l
RT: 4.611 min Scan# 578
Delta R.T. 0.049 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion:	43	Resp:	465
Ion	Ratio	Lower	Upper
43	100		
72	0.0	20.4	30.6#

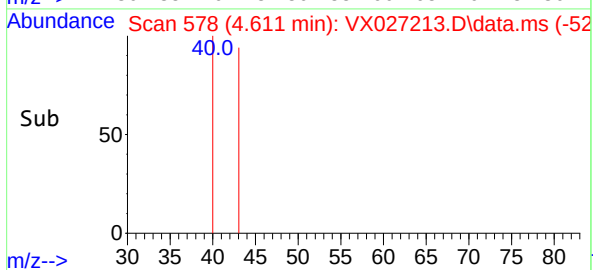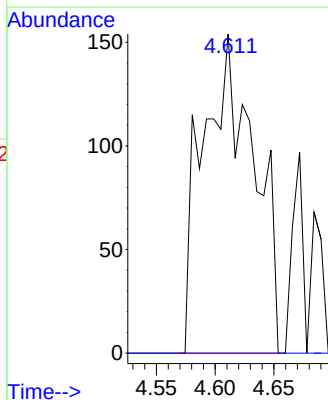



#30

Chloroform

Concen: 0.311 ug/l

RT: 5.160 min Scan# 6

Delta R.T. 0.062 min

Lab File: VX027213.D

Acq: 26 Feb 2022 01:28

Instrument :

MSVOA_X

ClientSampleId :





D13-7.5ME

Tgt Ion: 83 Resp: 585

Ion Ratio Lower Upper

83 100

85 0.0 51.6 77.4#

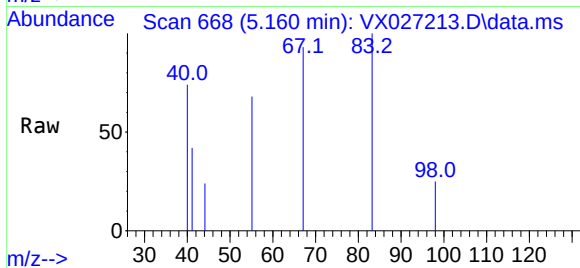

#31

Cyclohexane

Concen: 1.947 ug/l

RT: 5.495 min Scan# 723

Delta R.T. 0.019 min

Lab File: VX027213.D

Acq: 26 Feb 2022 01:28




Tgt Ion: 56 Resp: 3355


Ion Ratio Lower Upper

56 100

69 10.7 25.8 38.6#

84 34.9 68.9 103.3#

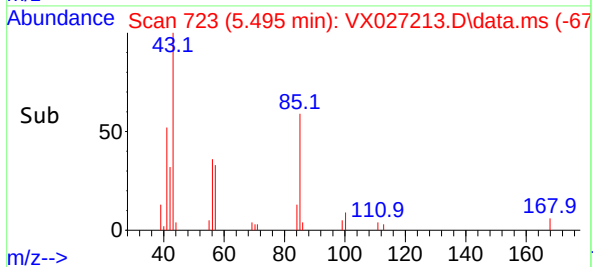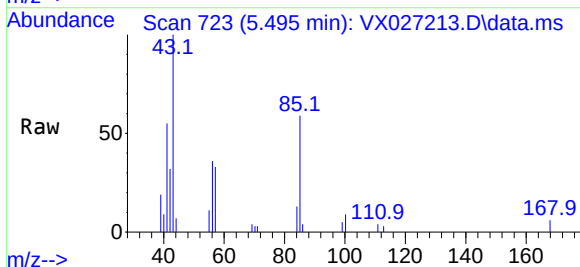



#33

1,2-Dichloroethane-d4

Concen: 49.893 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX027213.D

Acq: 26 Feb 2022 01:28

Instrument :

MSVOA_X

ClientSampleId :





D13-7.5ME

Tgt Ion: 65 Resp: 57400

Ion Ratio Lower Upper

65 100

67 52.2 0.0 100.8

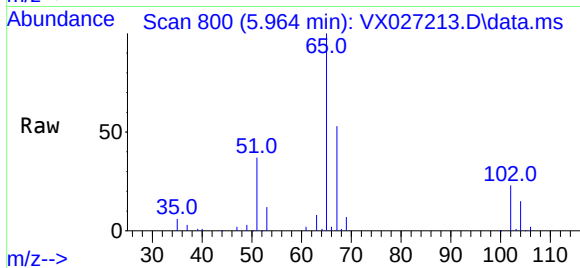

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX027213.D

Acq: 26 Feb 2022 01:28




Tgt Ion: 114 Resp: 160791


Ion Ratio Lower Upper

114 100

63 19.7 0.0 42.8

88 16.4 0.0 33.0

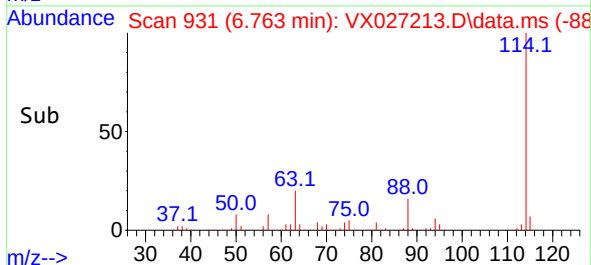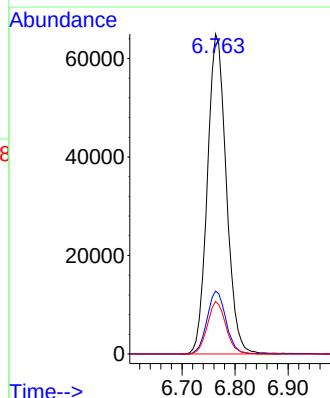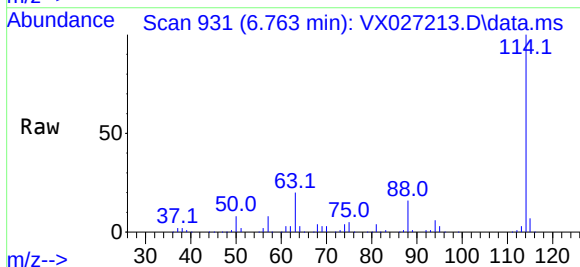

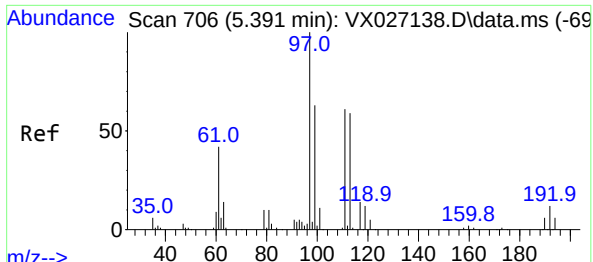

#35

Dibromofluoromethane

Concen: 46.924 ug/l

RT: 5.397 min Scan# 706

Delta R.T. 0.006 min

Lab File: VX027213.D

Acq: 26 Feb 2022 01:28

Instrument :

MSVOA_X

ClientSampleId :

D13-7.5ME





Tgt Ion:113 Resp: 46833

Ion Ratio Lower Upper

113 100

111 103.7 81.2 121.8

192 20.4 15.0 22.4

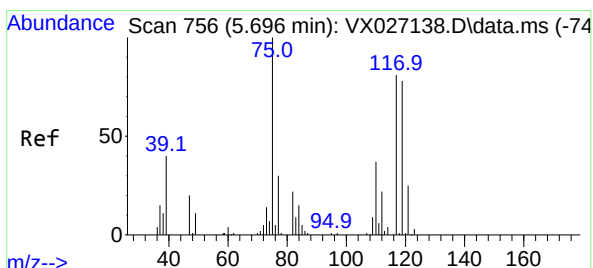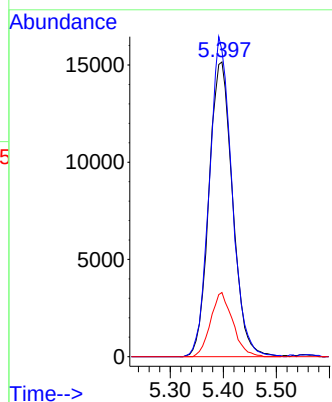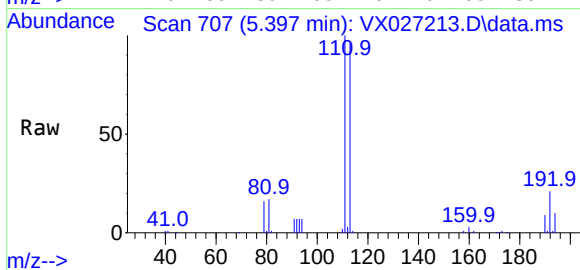

#36

1,1-Dichloropropene

Concen: 4.880 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX027213.D

Acq: 26 Feb 2022 01:28




Tgt Ion: 75 Resp: 7108


Ion Ratio Lower Upper

75 100

110 9.4 17.2 51.6#

77 0.0 24.6 36.8#


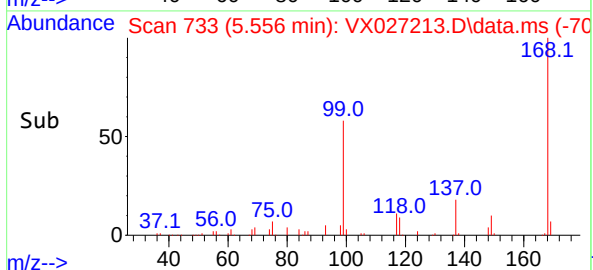

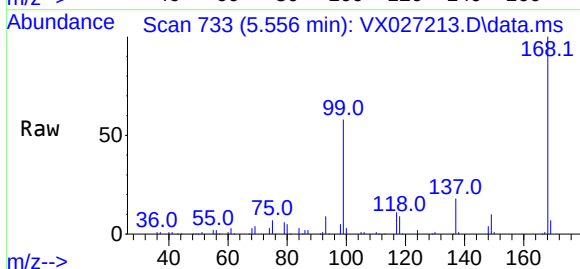




#38
Carbon Tetrachloride
Concen: 6.358 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion:117 Resp: 9659
Ion Ratio Lower Upper
117 100
119 4.5 74.7 112.1#
121 0.0 25.4 38.0#

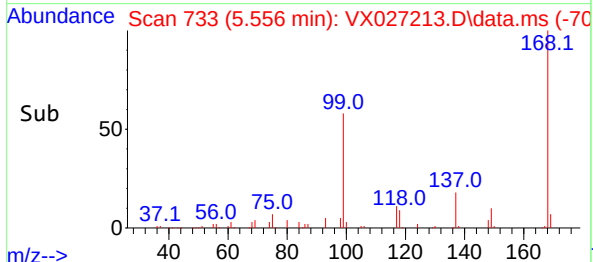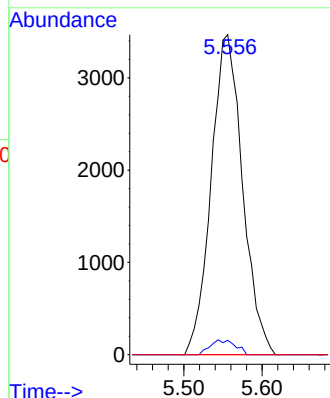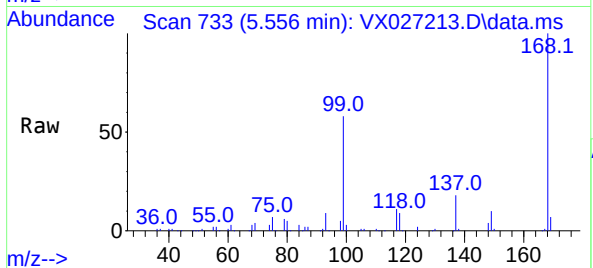

#39
Methylcyclohexane
Concen: 2.947 ug/l
RT: 7.373 min Scan# 1031
Delta R.T. -0.012 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 83 Resp: 5340
Ion Ratio Lower Upper
83 100
55 85.2 63.6 95.4
98 46.0 38.4 57.6


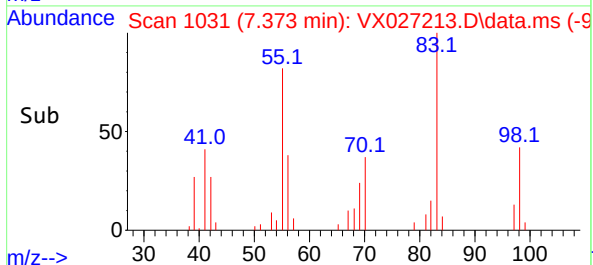
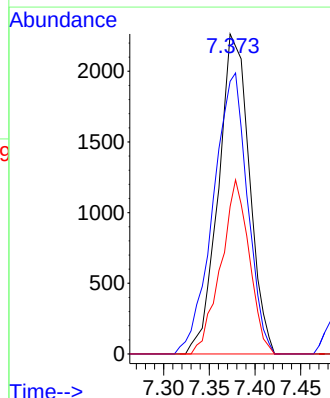
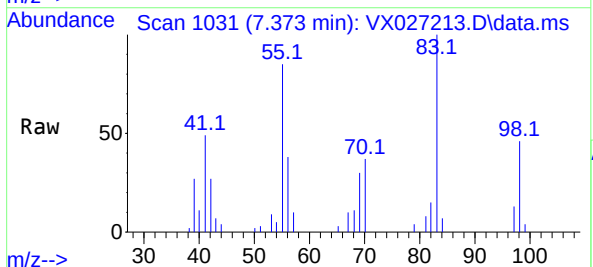




#43
Isopropyl Acetate
Concen: 3.590 ug/l
RT: 6.239 min Scan# 84
Delta R.T. -0.109 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion: 43 Resp: 8832
Ion Ratio Lower Upper
43 100
61 0.0 15.4 23.0#
87 0.0 10.2 15.2#

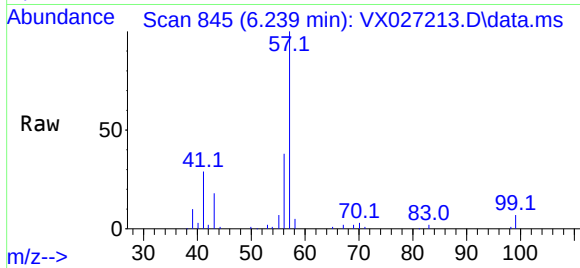

#50
Toluene-d8
Concen: 50.258 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 98 Resp: 187557
Ion Ratio Lower Upper
98 100
100 65.8 53.2 79.8


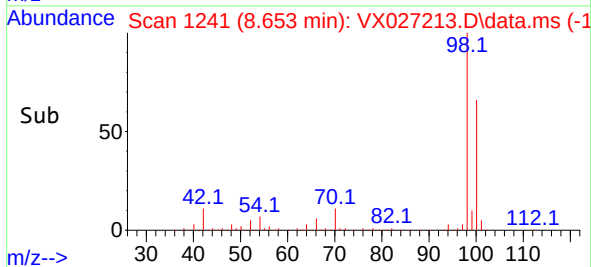

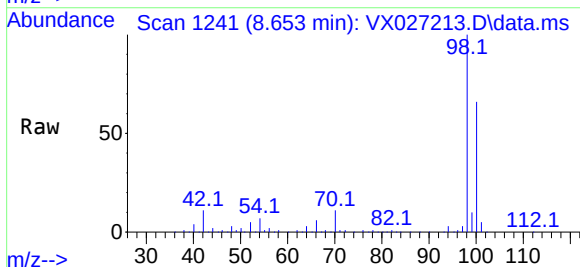




#51
4-Methyl-2-Pentanone
Concen: 1.663 ug/l
RT: 8.616 min Scan# 11
Delta R.T. 0.036 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion: 43 Resp: 2659
Ion Ratio Lower Upper
43 100
58 10.2 30.5 45.7#

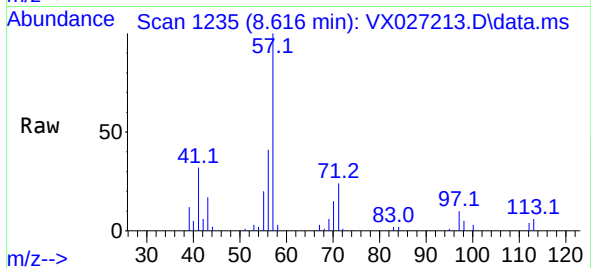

#52
Toluene
Concen: 3.644 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 92 Resp: 9940
Ion Ratio Lower Upper
92 100
91 169.2 135.7 203.5

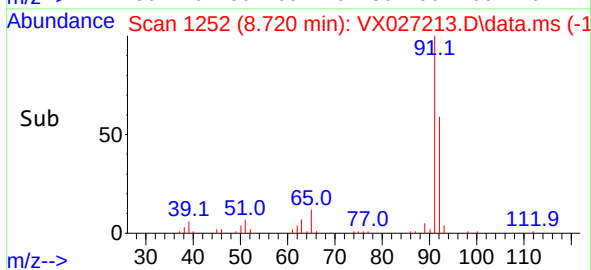



#53

t-1,3-Dichloropropene

Concen: 3.045 ug/l

RT: 8.915 min Scan# 11

Delta R.T. -0.067 min

Lab File: VX027213.D

Acq: 26 Feb 2022 01:28

Instrument :

MSVOA_X

ClientSampleId :


D13-7.5ME

Tgt Ion: 75 Resp: 129




Ion Ratio Lower Upper

75 100

77 89.8 25.7 38.5#

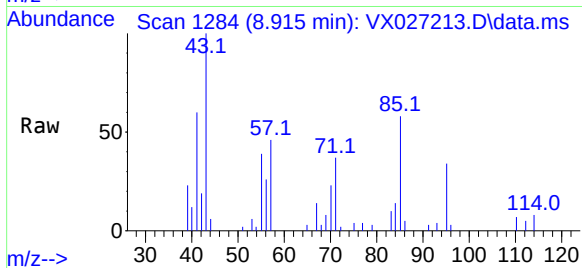

Abundance

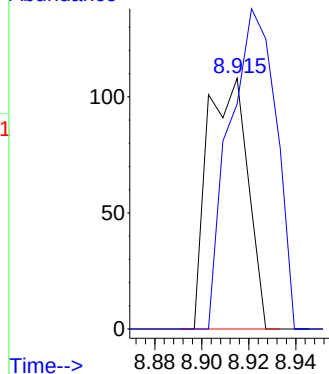

#55

1,1,2-Trichloroethane

Concen: 1.963 ug/l

RT: 9.104 min Scan# 1315

Delta R.T. -0.049 min

Lab File: VX027213.D

Acq: 26 Feb 2022 01:28

Tgt Ion: 97 Resp: 2121


Ion Ratio Lower Upper

97 100



83 9.7 68.4 102.6#


85 0.0 44.0 66.0#

99 0.0 49.8 74.6#

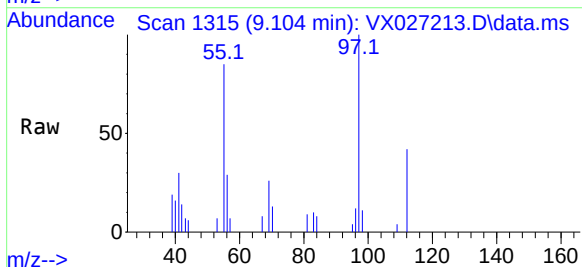

Abundance

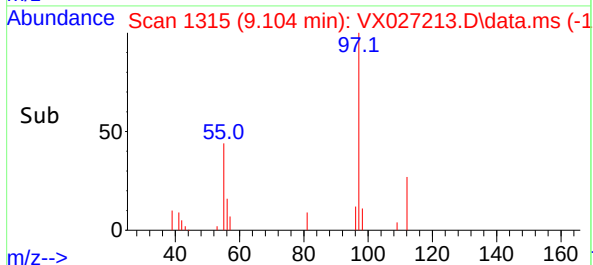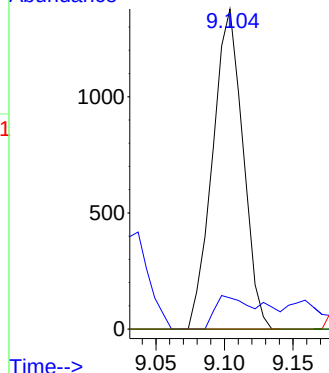



#56

Ethyl methacrylate

Concen: 0.363 ug/l

RT: 9.104 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX027213.D

Acq: 26 Feb 2022 01:28

Instrument :





MSVOA_X

ClientSampleId :

D13-7.5ME

Tgt Ion: 69 Resp: 610

Ion	Ratio	Lower	Upper
69	100		
41	100.2	57.2	85.8#
39	140.2	30.9	46.3#

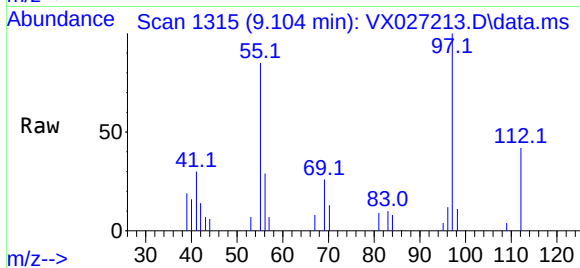

#59

2-Hexanone

Concen: 1.186 ug/l

RT: 9.384 min Scan# 1361




Delta R.T. -0.049 min


Lab File: VX027213.D

Acq: 26 Feb 2022 01:28

Tgt Ion: 43 Resp: 1450

Ion	Ratio	Lower	Upper
43	100		
58	0.0	26.4	79.2#


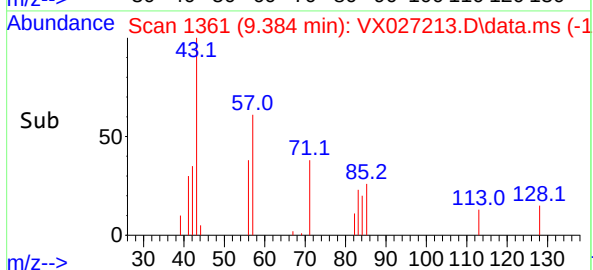
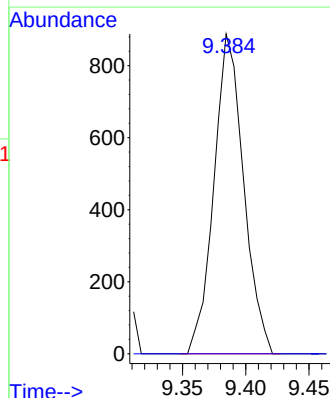
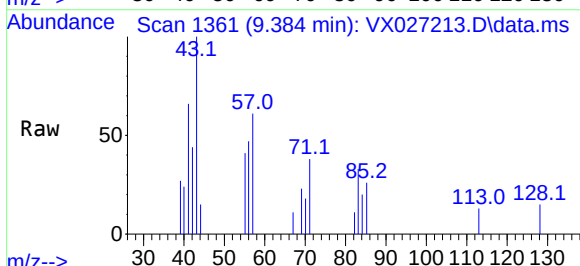




#62
4-Bromofluorobenzene
Concen: 51.003 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion: 95 Resp: 73061
Ion Ratio Lower Upper
95 100
174 76.9 0.0 148.6
176 76.5 0.0 141.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 117 Resp: 147042
Ion Ratio Lower Upper
117 100
82 55.0 45.2 67.8
119 31.8 26.2 39.2


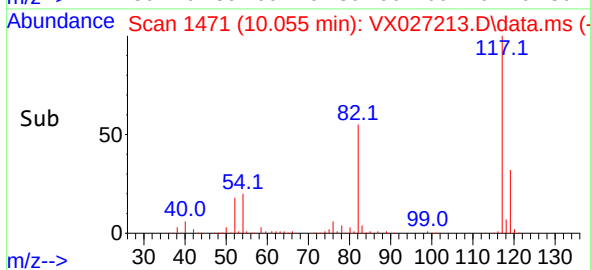






#67
Ethyl Benzene
Concen: 4.275 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion: 91 Resp: 22494
Ion Ratio Lower Upper
91 100
106 32.1 24.7 37.1



#68
m/p-Xylenes
Concen: 12.376 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 106 Resp: 25036
Ion Ratio Lower Upper
106 100
91 201.7 165.3 247.9


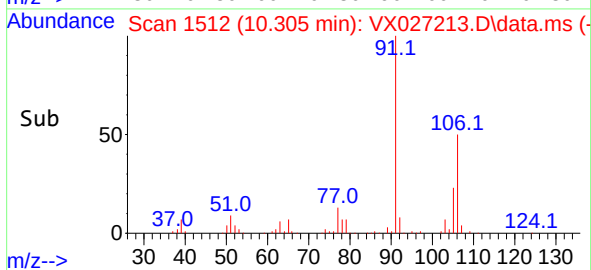






#69
o-Xylene
Concen: 4.004 ug/l
RT: 10.646 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion:106 Resp: 8129
Ion Ratio Lower Upper
106 100
91 217.1 109.7 329.0

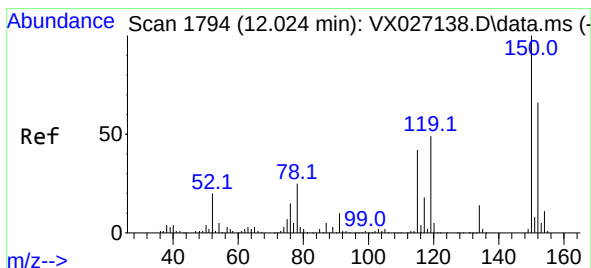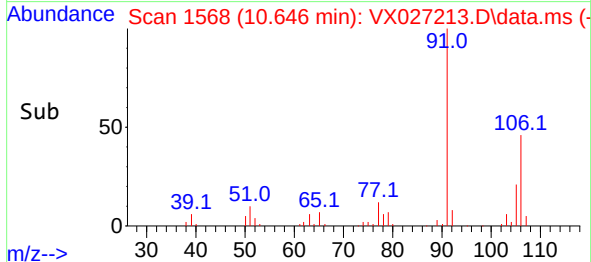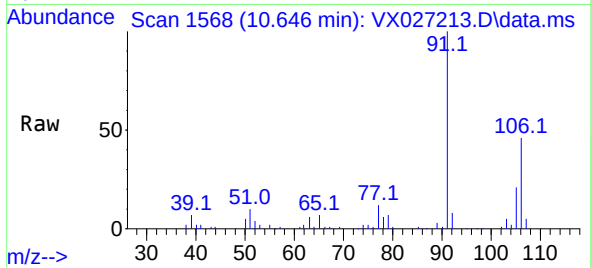

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion:152 Resp: 74750
Ion Ratio Lower Upper
152 100
115 59.1 44.2 132.6
150 156.3 0.0 348.2


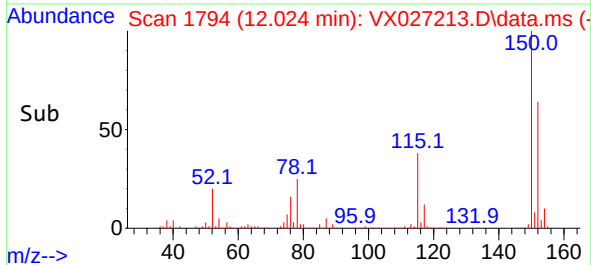

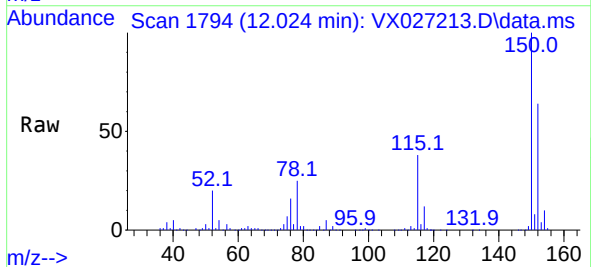




#73
Isopropylbenzene
Concen: 1.789 ug/l
RT: 10.963 min Scan# 1603
Delta R.T. 0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion:105 Resp: 9569
Ion Ratio Lower Upper
105 100
120 27.9 13.1 39.1

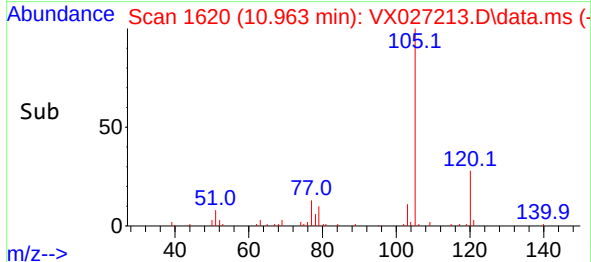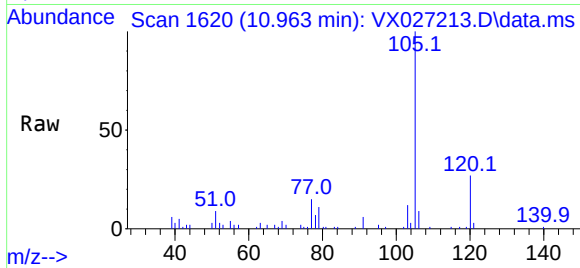

#74
N-ethyl acetate
Concen: 0.326 ug/l
RT: 10.860 min Scan# 1603
Delta R.T. 0.013 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 43 Resp: 664
Ion Ratio Lower Upper
43 100
70 84.5 32.9 49.3#
55 163.3 18.3 27.5#
61 0.0 18.9 28.3#


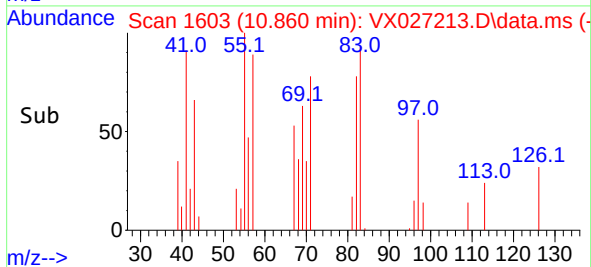

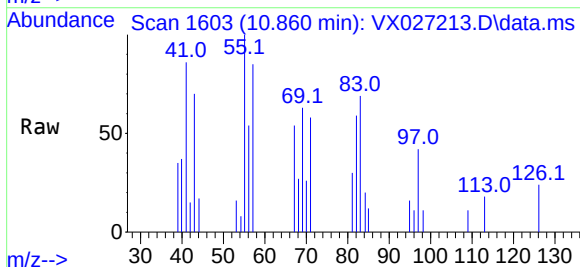




#76
1,2,3-Trichloropropane
Concen: 0.880 ug/l
RT: 11.317 min Scan# 1678
Delta R.T. 0.073 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion: 75 Resp: 1325
Ion Ratio Lower Upper
75 100
77 81.2 18.3 54.8#

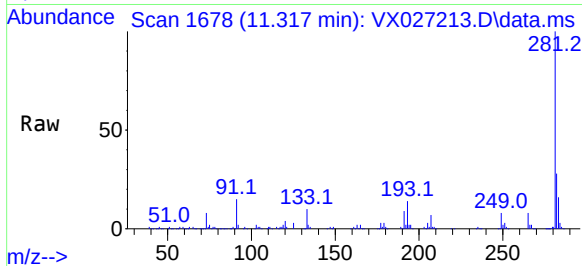

#78
n-propylbenzene
Concen: 3.963 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 91 Resp: 24093
Ion Ratio Lower Upper
91 100
120 24.1 11.6 34.7


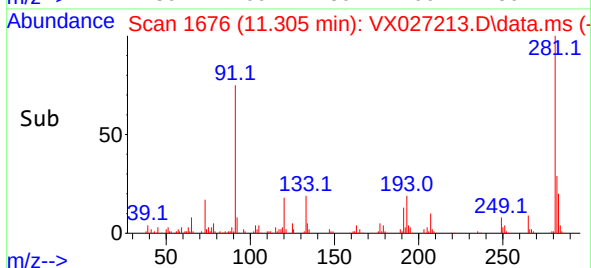

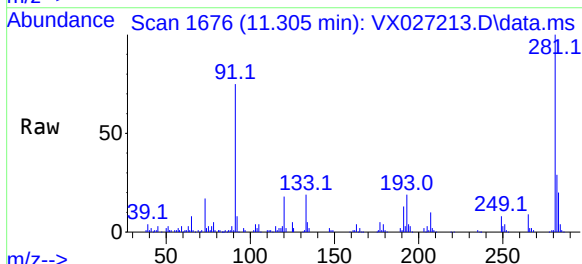




#79
2-Chlorotoluene
Concen: 1.809 ug/l
RT: 11.378 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion: 91 Resp: 6740
Ion Ratio Lower Upper
91 100
126 0.0 16.4 49.2#

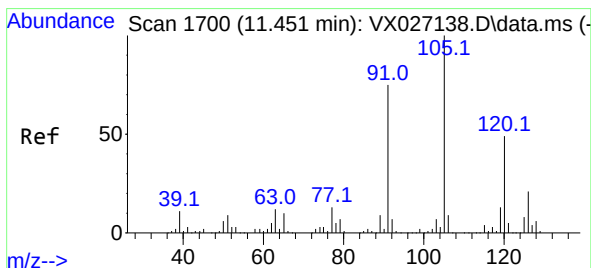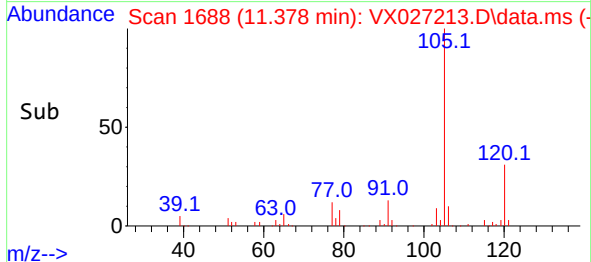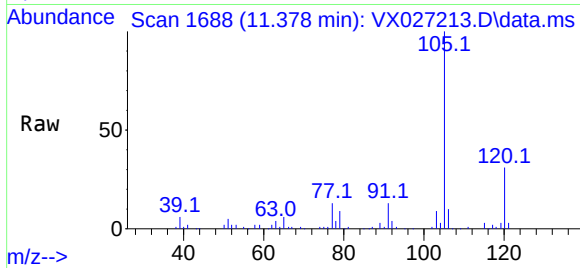

#80
1,3,5-Trimethylbenzene
Concen: 4.905 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 105 Resp: 22060
Ion Ratio Lower Upper
105 100
120 48.3 24.0 72.0


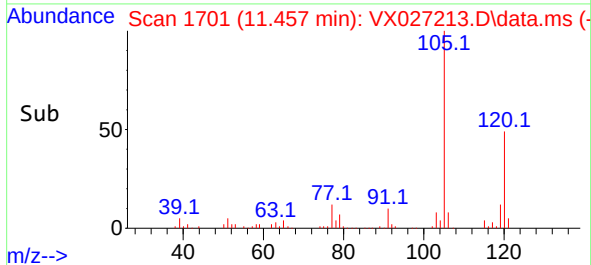

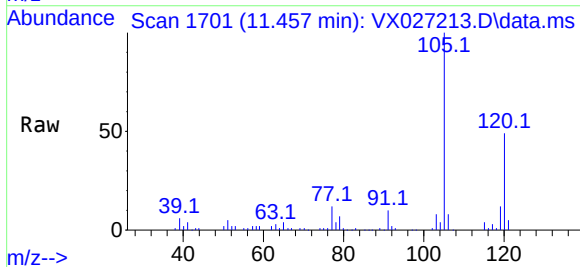




#81
trans-1,4-Dichloro-2-butene
Concen: 66.579 ug/l
RT: 11.085 min Scan# 1100
Delta R.T. 0.061 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion: 75 Resp: 35224
Ion Ratio Lower Upper
75 100
53 0.3 94.0 141.0#
89 0.0 37.0 55.4#

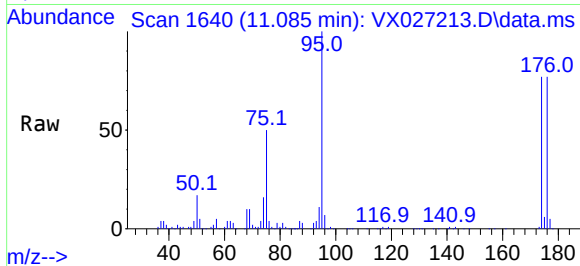

#82
4-Chlorotoluene
Concen: 0.567 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 91 Resp: 2411
Ion Ratio Lower Upper
91 100
126 0.0 14.1 42.4#


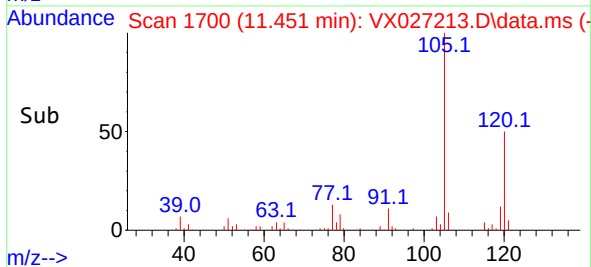

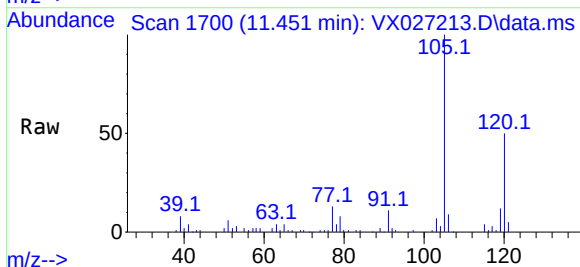




#83
tert-Butylbenzene
Concen: 1.578 ug/l
RT: 11.756 min Scan# 11
Delta R.T. 0.037 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion:119 Resp: 6902
Ion Ratio Lower Upper
119 100
91 87.4 31.4 94.0
134 0.0 11.8 35.3#

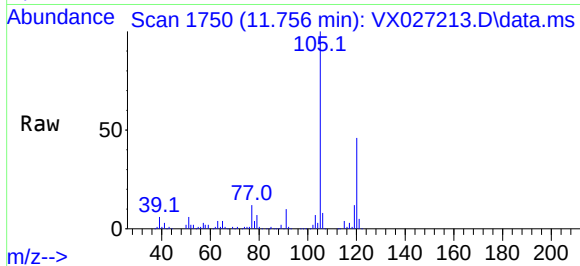

#84
1,2,4-Trimethylbenzene
Concen: 12.843 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion:105 Resp: 57459
Ion Ratio Lower Upper
105 100
120 45.4 21.9 65.5


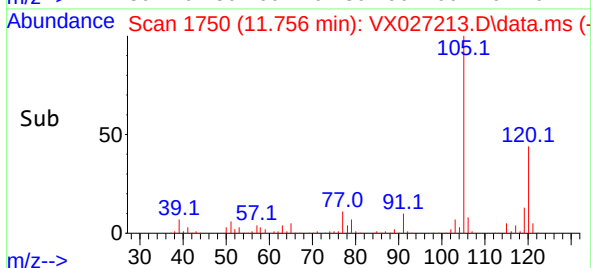
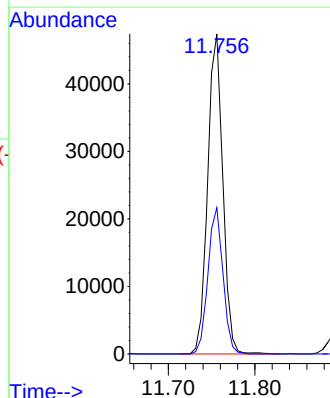
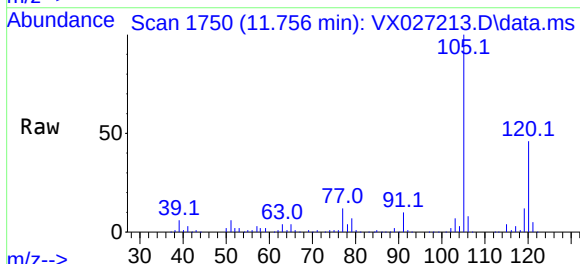




#85
sec-Butylbenzene
Concen: 0.668 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28




Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME


Tgt Ion:105 Resp: 3662
Ion Ratio Lower Upper
105 100
134 15.2 10.1 30.1

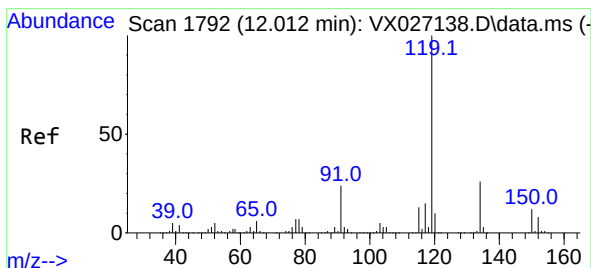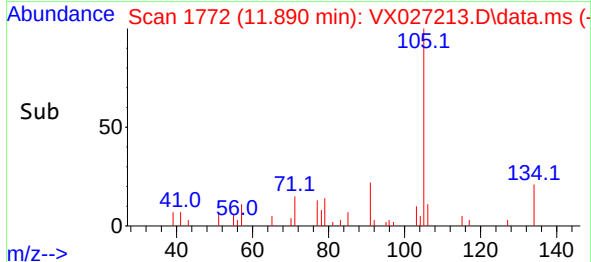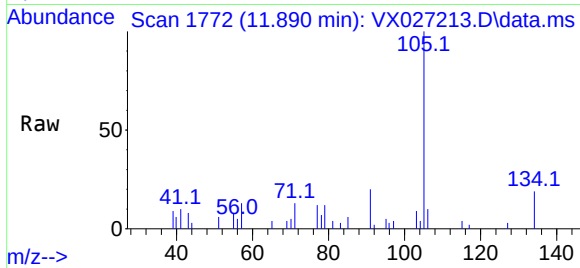

#86
p-Isopropyltoluene
Concen: 0.466 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. -0.037 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion:119 Resp: 2180
Ion Ratio Lower Upper
119 100
134 29.3 13.0 39.0
91 28.8 12.6 37.6

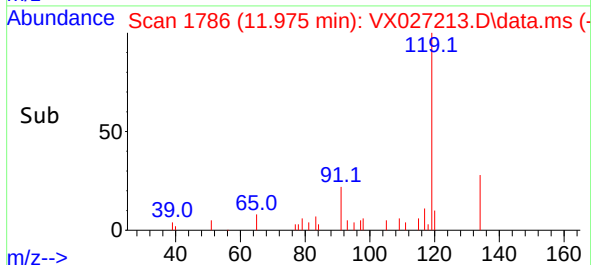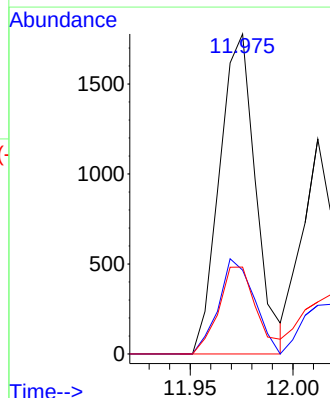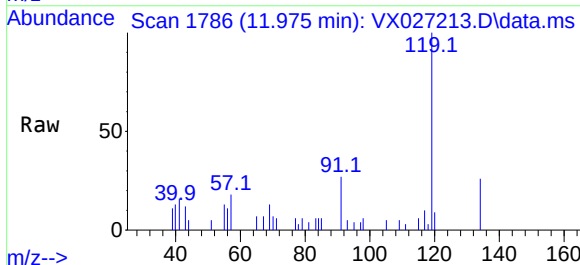



#89

n-Butylbenzene

Concen: 2.839 ug/l

RT: 12.335 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX027213.D

Acq: 26 Feb 2022 01:28

Instrument :

MSVOA_X

ClientSampleId :

D13-7.5ME





Tgt Ion: 91 Resp: 11091

Ion Ratio Lower Upper

91 100

92 35.7 27.2 81.6

134 87.4 13.1 39.1#

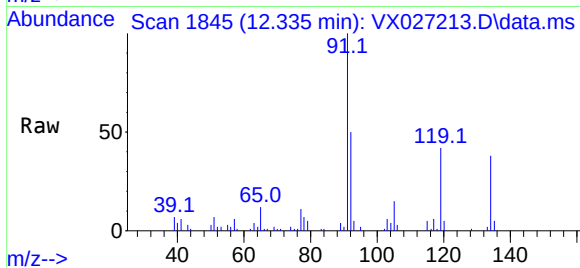

#90

Hexachloroethane

Concen: 1.514 ug/l

RT: 12.536 min Scan# 1878

Delta R.T. -0.006 min

Lab File: VX027213.D




Acq: 26 Feb 2022 01:28


Tgt Ion: 117 Resp: 1096

Ion Ratio Lower Upper

117 100

201 0.0 35.6 106.8#


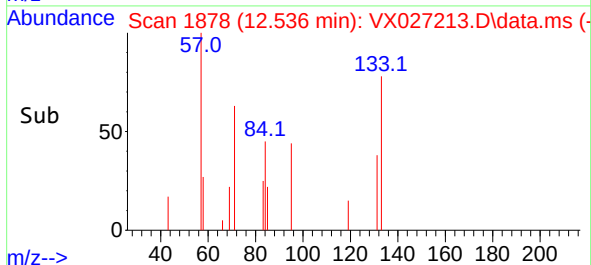
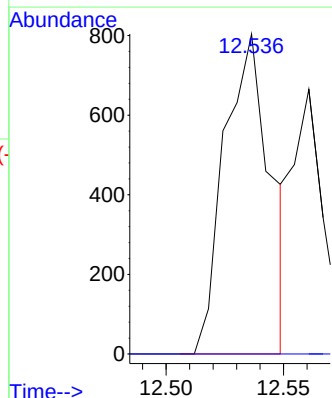
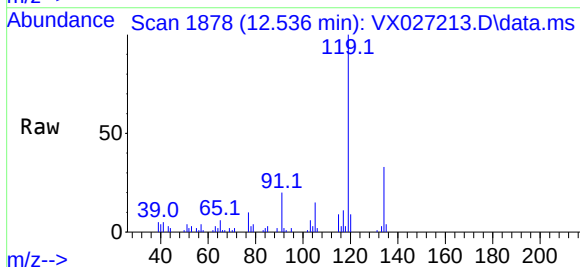




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.224 ug/l
RT: 12.927 min Scan# 1942
Delta R.T. -0.018 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Instrument :
MSVOA_X
ClientSampleId :
D13-7.5ME

Tgt Ion: 75 Resp: 82
Ion Ratio Lower Upper
75 100
155 0.0 40.0 119.9#
157 0.0 51.6 154.8#

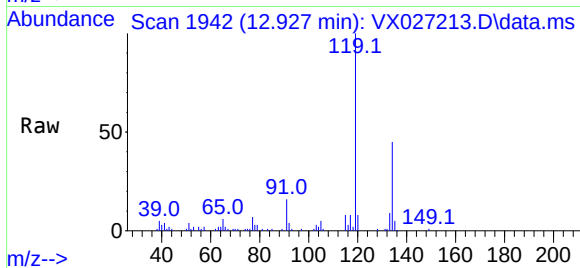

#95
Naphthalene
Concen: 2.008 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX027213.D
Acq: 26 Feb 2022 01:28

Tgt Ion: 128 Resp: 10549
Ion Ratio Lower Upper
128 100
127 13.1 10.3 15.5
129 11.8 8.7 13.1

