

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022525\
 Data File : VX045036.D
 Acq On : 25 Feb 2025 14:07
 Operator : JC/MD
 Sample : Q1423-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-192-TB-20250220

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
 Title : SW846 8260

Signal : TIC: VX045036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	5	9	19	rBV	17071	18636	3.81%	0.713%
2	1.240	21	25	37	rBV	45091	66453	13.57%	2.544%
3	1.368	42	46	50	rVV2	6223	9733	1.99%	0.373%
4	1.447	56	59	65	rBV	5589	6583	1.34%	0.252%
5	1.575	69	80	81	rBV3	4757	10953	2.24%	0.419%
6	1.630	87	89	92	rVB4	5657	5753	1.17%	0.220%
7	2.386	208	213	221	rBV	6690	11545	2.36%	0.442%
8	5.385	695	705	720	rBV	55984	165701	33.83%	6.342%
9	5.544	720	731	753	rVV	76775	222878	45.51%	8.531%
10	5.952	787	798	814	rBV	62787	171734	35.07%	6.573%
11	6.757	920	930	946	rBV	140018	343397	70.12%	13.144%
12	8.647	1232	1240	1263	rBV	298052	489738	100.00%	18.745%
13	9.531	1381	1385	1394	rVB4	3509	7044	1.44%	0.270%
14	10.055	1465	1471	1487	rBV	281395	412419	84.21%	15.786%
15	10.774	1584	1589	1598	rBV	4009	6988	1.43%	0.267%
16	10.860	1600	1603	1609	rBV3	5005	6804	1.39%	0.260%
17	11.079	1634	1639	1650	rBV	220457	289461	59.11%	11.079%
18	11.482	1701	1705	1713	rVB4	4077	6312	1.29%	0.242%
19	11.847	1759	1765	1771	rBV2	4072	6569	1.34%	0.251%
20	11.933	1775	1779	1788	rBV4	5390	8653	1.77%	0.331%
21	12.018	1788	1793	1803	rBV	257442	329692	67.32%	12.619%
22	12.768	1912	1916	1922	rBV4	3464	6125	1.25%	0.234%
23	12.859	1925	1931	1936	rBV3	6415	9466	1.93%	0.362%




Sum of corrected areas: 2612637

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022525\
Data File : VX045036.D
Acq On : 25 Feb 2025 14:07
Operator : JC/MD
Sample : Q1423-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-192-TB-20250220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

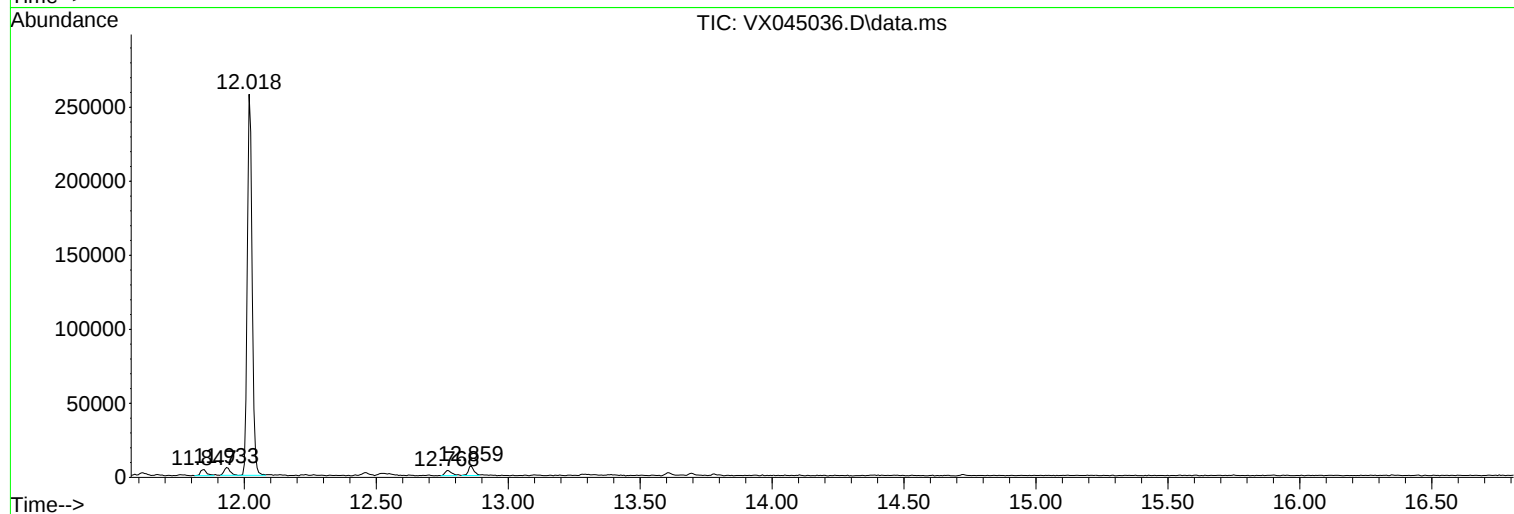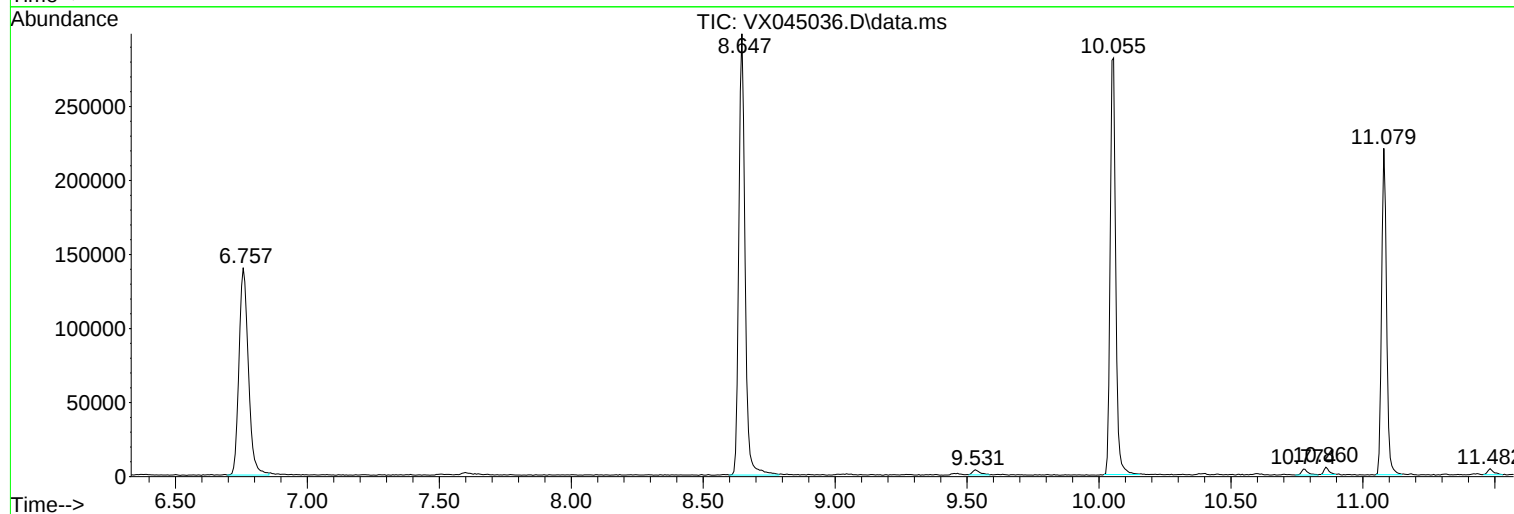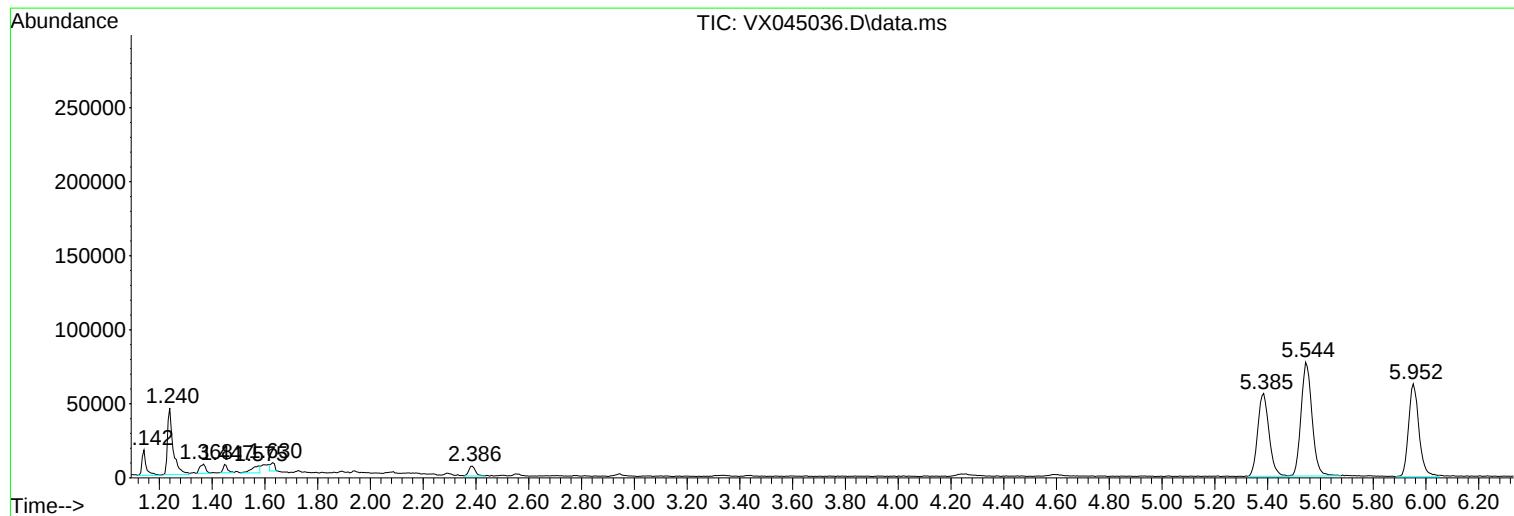

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022525\
Data File : VX045036.D
Acq On : 25 Feb 2025 14:07
Operator : JC/MD
Sample : Q1423-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-192-TB-20250220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022525\
Data File : VX045036.D
Acq On : 25 Feb 2025 14:07
Operator : JC/MD
Sample : Q1423-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-192-TB-20250220

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc