


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX022619\
 Data File : VX007709.D
 Acq On : 26 Feb 2019 12:30
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X022519W.M
 Title : SW846 8260
 Last Update : Tue Feb 26 01:53:13 2019

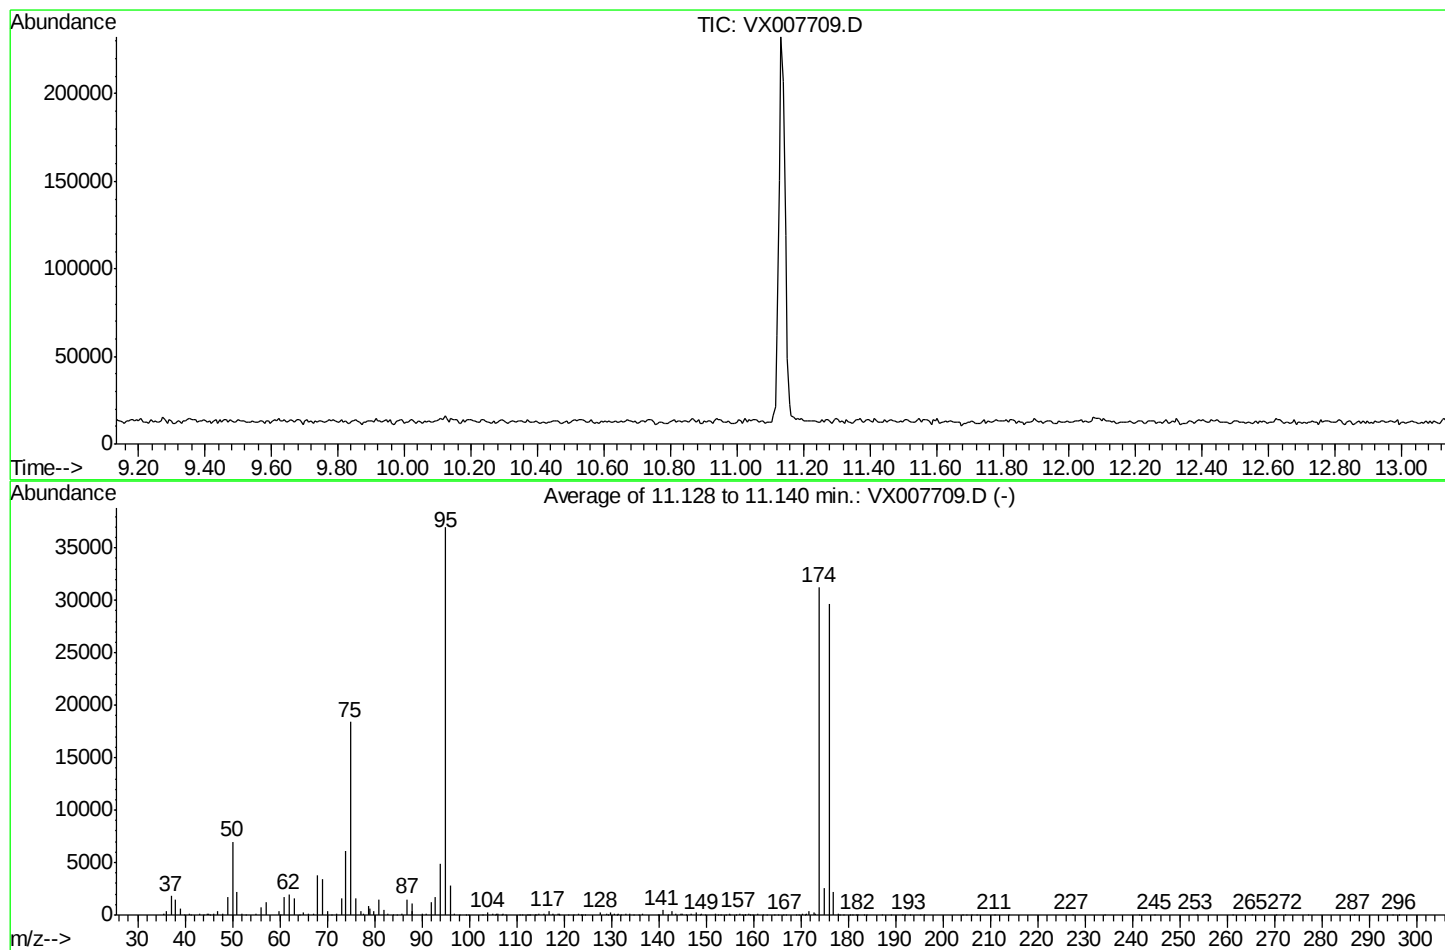

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	7001	PASS
75	95	30	60	49.7	18386	PASS
95	95	100	100	100.0	36960	PASS
96	95	5	9	7.6	2822	PASS
173	174	0.00	2	0.6	202	PASS
174	95	50	100	84.4	31192	PASS
175	174	5	9	8.2	2544	PASS
176	174	95	101	95.0	29642	PASS
177	176	5	9	7.2	2145	PASS