


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX022620\
 Data File : VX015004.D
 Acq On : 26 Feb 2020 08:14
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
 Title : SW846 8260
 Last Update : Mon Feb 10 12:09:20 2020

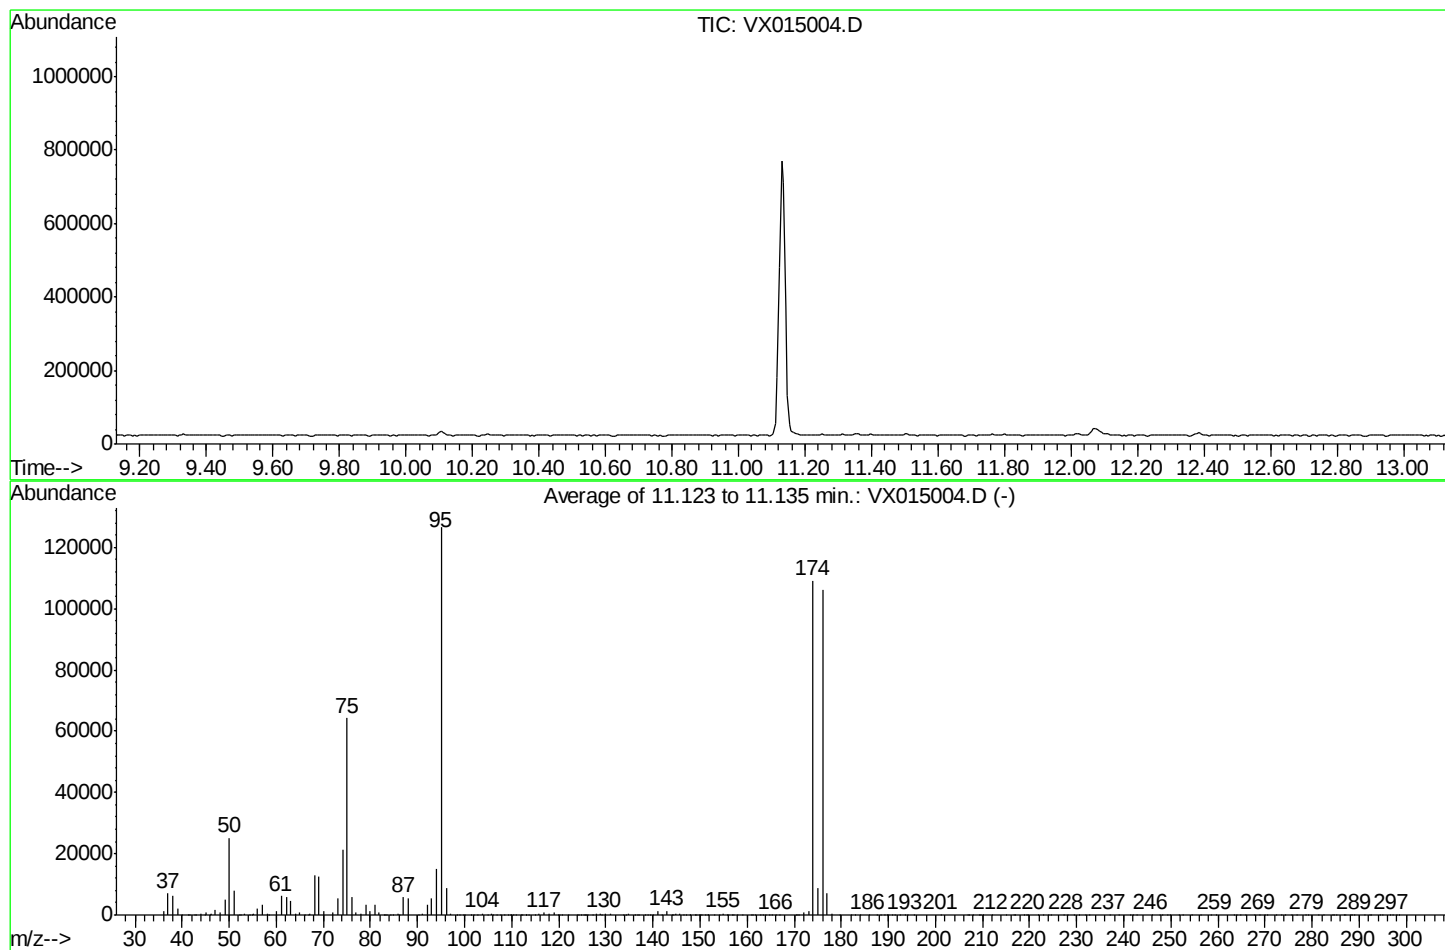

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	25096	PASS
75	95	30	60	50.8	64329	PASS
95	95	100	100	100.0	126573	PASS
96	95	5	9	7.0	8835	PASS
173	174	0.00	2	1.2	1356	PASS
174	95	50	100	86.3	109221	PASS
175	174	5	9	8.0	8745	PASS
176	174	95	101	97.1	106088	PASS
177	176	5	9	6.7	7153	PASS