

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
 Data File : VX020926.D
 Acq On : 26 Feb 2021 14:34
 Operator : JC/MD
 Sample : VX0226WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK404

Quant Time: Feb 27 02:42:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 26 12:33:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.823	114	302451	50.00	ug/L	0.00
28) Chlorobenzene-d5	10.094	117	274547	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.059	152	121613	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.387	65	94092	46.30	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.60%
7) Chloroethane-d5	1.693	69	83814	49.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.26%
11) 1,1-Dichloroethene-d2	2.340	63	137544	35.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.64%
21) 2-Butanone-d5	4.523	46	133881	107.95	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.95%
24) Chloroform-d	5.135	84	195652	51.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.80%
26) 1,2-Dichloroethane-d4	6.029	65	128069	52.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.28%
32) Benzene-d6	6.047	84	405055	49.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.74%
36) 1,2-Dichloropropane-d6	7.365	67	127146	50.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.54%
41) Toluene-d8	8.694	98	358401	49.15	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.30%
43) trans-1,3-Dichloroprop...	8.988	79	65378	50.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.22%
47) 2-Hexanone-d5	9.424	63	103136	101.51	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	101.51%
56) 1,1,2,2-Tetrachloroeth...	11.230	84	153063	49.23	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.46%
66) 1,2-Dichlorobenzene-d4	12.359	152	125602	53.95	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.90%
Target Compounds						
16) Methylene chloride	2.835	84	2249	0.99	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
Data File : VX020926.D
Acq On : 26 Feb 2021 14:34
Operator : JC/MD
Sample : VX0226WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK404


Quant Time: Feb 27 02:42:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM022621WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 26 12:33:14 2021
Response via : Initial Calibration

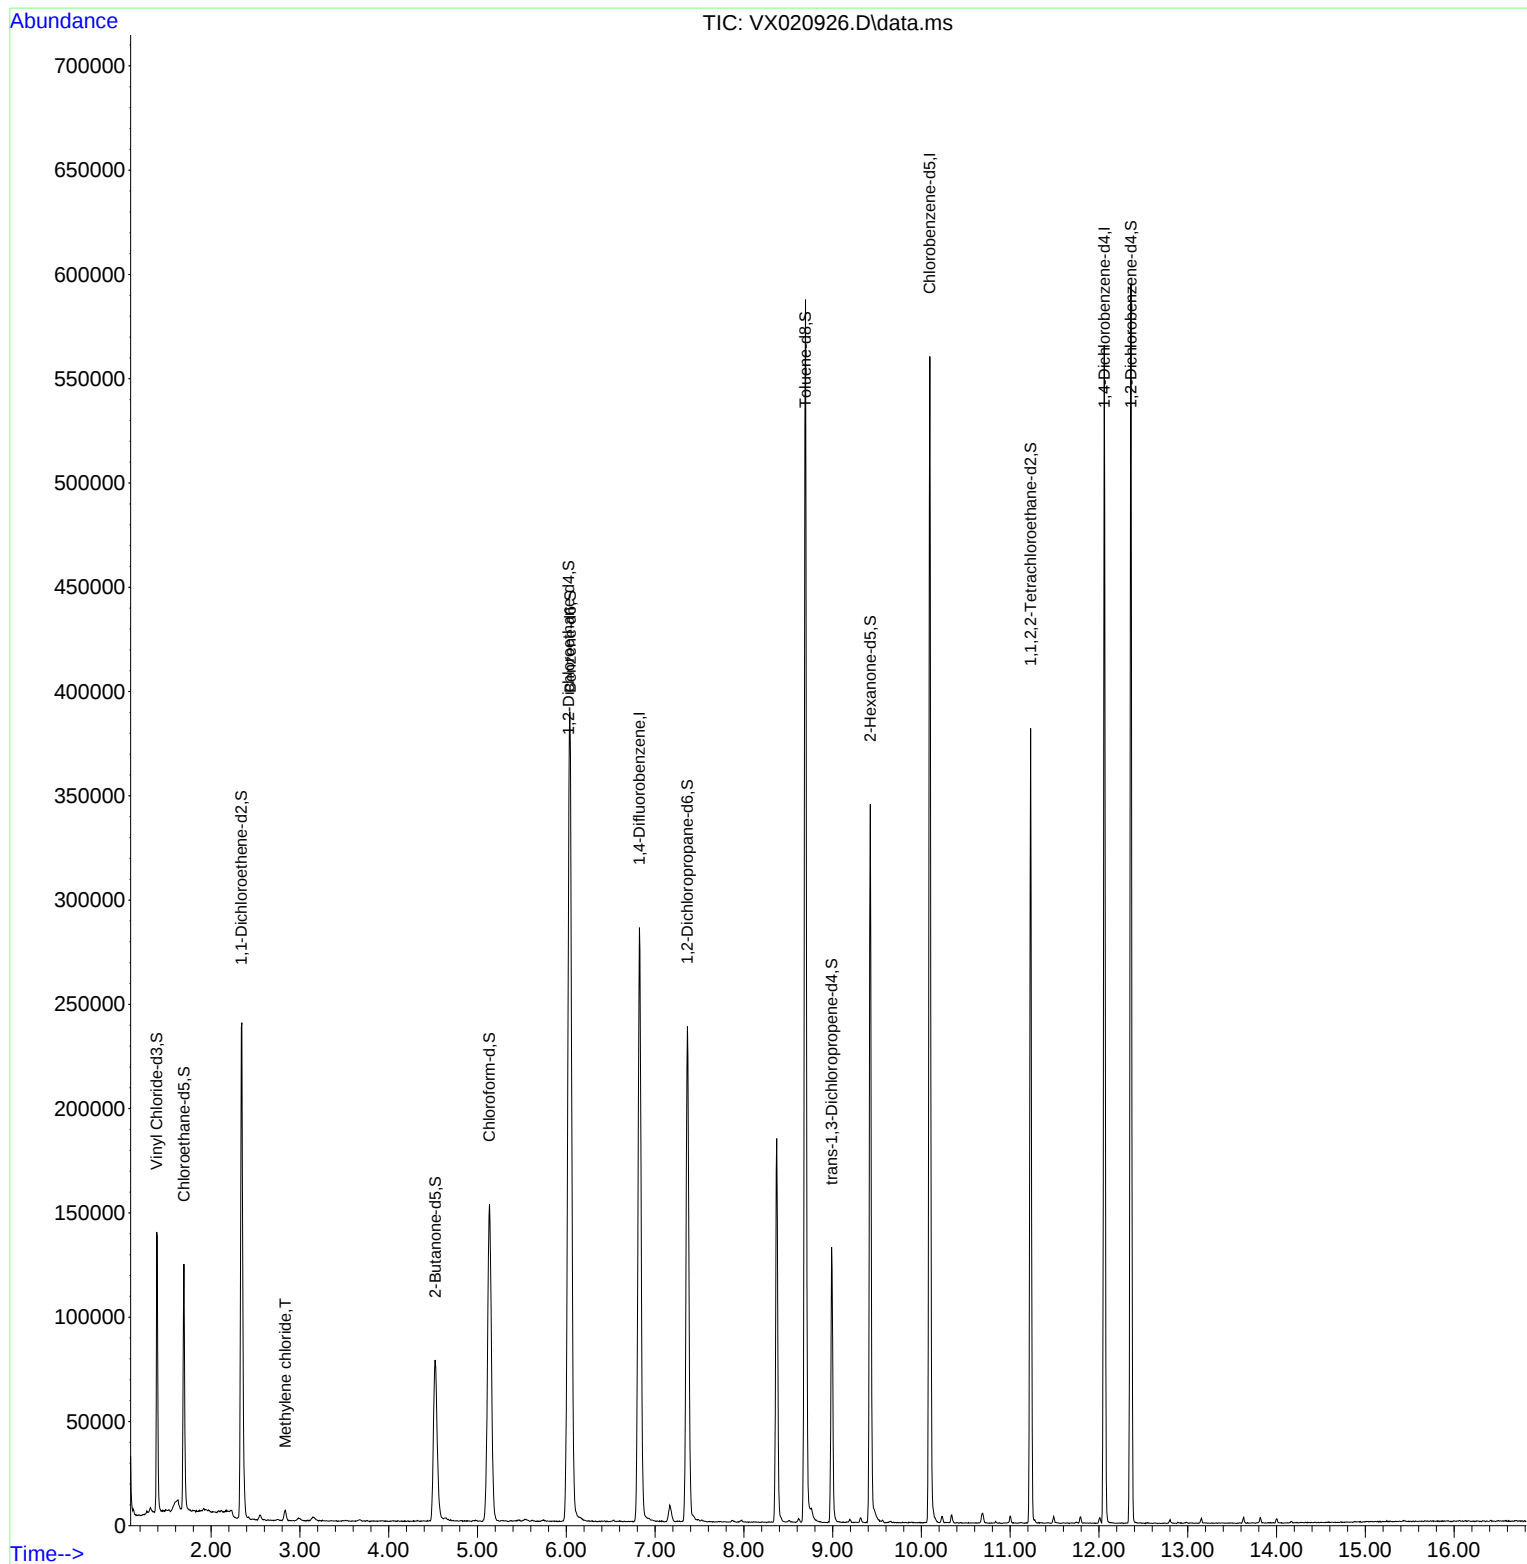

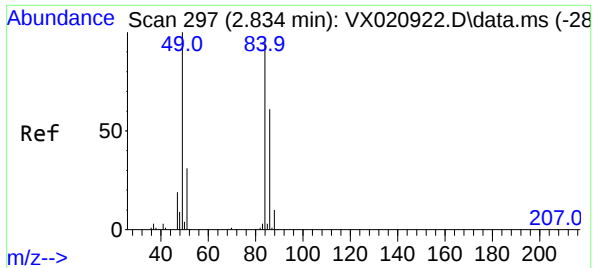

#16
Methylene chloride
Concen: 0.99 ug/L
RT: 2.835 min Scan# 297
Delta R.T. 0.000 min
Lab File: VX020926.D
Acq: 26 Feb 2021 14:34

Instrument :
MSVOA_X
ClientSampleId :
VBLK404

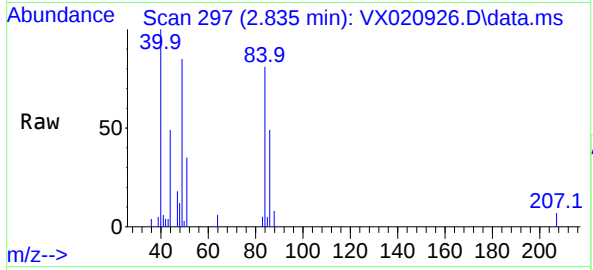

Tgt Ion: 84 Resp: 2249

Ion	Ratio	Lower	Upper
84	100		
86	61.0	44.2	82.0
49	105.4	77.8	144.6

