

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
 Data File : VX020926.D
 Acq On : 26 Feb 2021 14:34
 Operator : JC/MD
 Sample : VX0226WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK404

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M

Title : VOC Analysis

Signal : TIC: VX020926.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.387	48	51	60	rVB	133960	147437	12.74%	1.735%
2	1.693	98	103	113	rVB	117995	145887	12.61%	1.716%
3	2.346	207	214	226	rVB	237278	399967	34.57%	4.705%
4	2.552	244	249	255	rBV	2383	4392	0.38%	0.052%
5	2.835	291	297	304	rVB2	5098	9667	0.84%	0.114%
6	3.088	338	340	341	rBV2	450	263	0.02%	0.003%
7	3.105	341	343	344	rVV	441	257	0.02%	0.003%
8	3.146	345	350	361	rVB6	1955	5511	0.48%	0.065%
9	3.252	366	368	369	rBV	515	334	0.03%	0.004%
10	4.523	575	584	600	rBV	77183	225527	19.49%	2.653%
11	4.852	637	640	641	rBV2	458	369	0.03%	0.004%
12	5.135	675	688	707	rBV	152090	458372	39.62%	5.393%
13	5.511	750	752	753	rBV	467	382	0.03%	0.004%
14	5.529	753	755	756	rVV2	597	384	0.03%	0.005%
15	6.041	829	842	859	rBV2	388165	1157020	100.00%	13.612%
16	6.653	944	946	948	rBV2	352	273	0.02%	0.003%
17	6.823	963	975	990	rBV	285033	675246	58.36%	7.944%
18	7.165	1027	1033	1044	rVB5	7977	18032	1.56%	0.212%
19	7.365	1058	1067	1084	rBV	237268	522788	45.18%	6.150%
20	7.865	1150	1152	1156	rBV2	648	854	0.07%	0.010%
21	7.976	1165	1171	1175	rBV4	937	1469	0.13%	0.017%
22	8.206	1208	1210	1213	rBV2	334	357	0.03%	0.004%
23	8.271	1219	1221	1222	rBV2	276	264	0.02%	0.003%
24	8.371	1231	1238	1255	rBV	183944	297832	25.74%	3.504%
25	8.512	1258	1262	1265	rVV3	824	1197	0.10%	0.014%
26	8.541	1265	1267	1269	rVB2	339	250	0.02%	0.003%
27	8.618	1276	1280	1284	rVB4	1787	2345	0.20%	0.028%
28	8.694	1285	1293	1303	rBV	586227	936206	80.92%	11.014%
29	8.953	1335	1337	1338	rBV	364	286	0.02%	0.003%
30	8.988	1338	1343	1354	rVV	131948	194364	16.80%	2.287%
31	9.159	1370	1372	1374	rBV2	343	278	0.02%	0.003%
32	9.194	1374	1378	1381	rVB3	1427	1696	0.15%	0.020%
33	9.253	1386	1388	1391	rBV	292	345	0.03%	0.004%
34	9.312	1394	1398	1402	rBV3	2191	2887	0.25%	0.034%
35	9.424	1411	1417	1435	rVV	344466	489813	42.33%	5.762%
36	9.559	1438	1440	1445	rVB3	1328	1653	0.14%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
 Data File : VX020926.D
 Acq On : 26 Feb 2021 14:34
 Operator : JC/MD
 Sample : VX0226WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK404

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Title : VOC Analysis

37	9.600	1445	1447	1450	rBV	257	301	0.03%	0.004%
38	9.647	1452	1455	1459	rVB4	648	899	0.08%	0.011%
39	9.688	1459	1462	1463	rVB2	300	236	0.02%	0.003%
40	9.700	1463	1464	1468	rVB3	223	245	0.02%	0.003%
41	9.818	1482	1484	1487	rVB3	233	258	0.02%	0.003%
42	9.859	1490	1491	1493	rBV2	433	281	0.02%	0.003%
43	10.094	1525	1531	1548	rBV	559187	789253	68.21%	9.285%
44	10.236	1550	1555	1559	rVB3	3053	4194	0.36%	0.049%
45	10.341	1569	1573	1578	rVB	3948	5317	0.46%	0.063%
46	10.400	1581	1583	1587	rVB2	378	421	0.04%	0.005%
47	10.441	1587	1590	1591	rBV2	329	348	0.03%	0.004%
48	10.689	1625	1632	1638	rVB4	4673	8416	0.73%	0.099%
49	10.836	1654	1657	1661	rVB2	875	782	0.07%	0.009%
50	10.924	1669	1672	1675	rBV	287	461	0.04%	0.005%
51	11.000	1679	1685	1690	rVB2	3362	4457	0.39%	0.052%
52	11.183	1713	1716	1718	rBV2	463	453	0.04%	0.005%
53	11.230	1718	1724	1731	rBV	380973	490629	42.40%	5.772%
54	11.318	1738	1739	1741	rVB	476	326	0.03%	0.004%
55	11.489	1763	1768	1771	rBV3	3295	3901	0.34%	0.046%
56	11.595	1782	1786	1789	rBV2	294	472	0.04%	0.006%
57	11.647	1791	1795	1798	rVB2	364	552	0.05%	0.006%
58	11.689	1798	1802	1803	rBV2	368	452	0.04%	0.005%
59	11.747	1808	1812	1816	rVV3	556	796	0.07%	0.009%
60	11.789	1816	1819	1824	rVB	3117	3919	0.34%	0.046%
61	11.830	1824	1826	1828	rBV2	292	253	0.02%	0.003%
62	12.006	1851	1856	1860	rBV3	2701	3842	0.33%	0.045%
63	12.059	1860	1865	1876	rVB	564615	704696	60.91%	8.291%
64	12.359	1910	1916	1924	rVV	594409	742079	64.14%	8.730%
65	12.530	1944	1945	1947	rBV2	422	334	0.03%	0.004%
66	12.548	1947	1948	1950	rVV2	460	312	0.03%	0.004%
67	12.624	1958	1961	1967	rVB3	309	694	0.06%	0.008%
68	12.683	1967	1971	1973	rBV2	264	364	0.03%	0.004%
69	12.801	1984	1991	1996	rBV2	1845	2493	0.22%	0.029%
70	12.889	2003	2006	2008	rBV2	694	703	0.06%	0.008%
71	12.983	2016	2022	2027	rVB5	600	1256	0.11%	0.015%
72	13.030	2027	2030	2031	rBV2	364	421	0.04%	0.005%
73	13.154	2047	2051	2055	rVV	2434	2765	0.24%	0.033%
74	13.324	2076	2080	2082	rVB2	301	365	0.03%	0.004%
75	13.348	2082	2084	2087	rBV2	319	338	0.03%	0.004%
76	13.630	2128	2132	2138	rVB2	2900	3459	0.30%	0.041%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
 Data File : VX020926.D
 Acq On : 26 Feb 2021 14:34
 Operator : JC/MD
 Sample : VX0226WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK404

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Title : VOC Analysis

77	13.724	2145	2148	2150	rBV3	216	248	0.02%	0.003%
78	13.783	2155	2158	2159	rBV3	252	297	0.03%	0.003%
79	13.818	2160	2164	2167	rVV	2725	3291	0.28%	0.039%
80	13.907	2176	2179	2182	rVV2	283	327	0.03%	0.004%
81	14.001	2192	2195	2199	rVV4	1971	2637	0.23%	0.031%
82	14.054	2201	2204	2205	rVB2	387	305	0.03%	0.004%
83	14.171	2221	2224	2226	rVB4	727	867	0.07%	0.010%
84	14.265	2238	2240	2242	rVV2	315	265	0.02%	0.003%
85	14.324	2248	2250	2253	rVV2	330	347	0.03%	0.004%
86	14.442	2266	2270	2272	rVB4	309	370	0.03%	0.004%
87	14.501	2277	2280	2281	rBV4	286	264	0.02%	0.003%
88	14.589	2294	2295	2298	rVB	470	236	0.02%	0.003%
89	14.718	2315	2317	2319	rVB2	271	238	0.02%	0.003%
90	14.883	2341	2345	2347	rBV3	541	765	0.07%	0.009%
91	15.166	2391	2393	2395	rBV2	498	387	0.03%	0.005%
92	15.189	2395	2397	2400	rBV2	361	456	0.04%	0.005%
93	15.242	2404	2406	2408	rVB2	594	347	0.03%	0.004%
94	15.266	2408	2410	2411	rBV3	401	272	0.02%	0.003%
95	15.542	2454	2457	2459	rBV2	480	508	0.04%	0.006%
96	15.566	2459	2461	2463	rBV2	395	354	0.03%	0.004%
97	15.830	2504	2506	2507	rVB	367	244	0.02%	0.003%
98	16.319	2587	2589	2590	rBV	392	297	0.03%	0.003%
99	16.478	2614	2616	2617	rBV2	381	341	0.03%	0.004%
100	16.683	2649	2651	2653	rBV2	424	410	0.04%	0.005%


Sum of corrected areas: 8500020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
Data File : VX020926.D
Acq On : 26 Feb 2021 14:34
Operator : JC/MD
Sample : VX0226WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK404

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

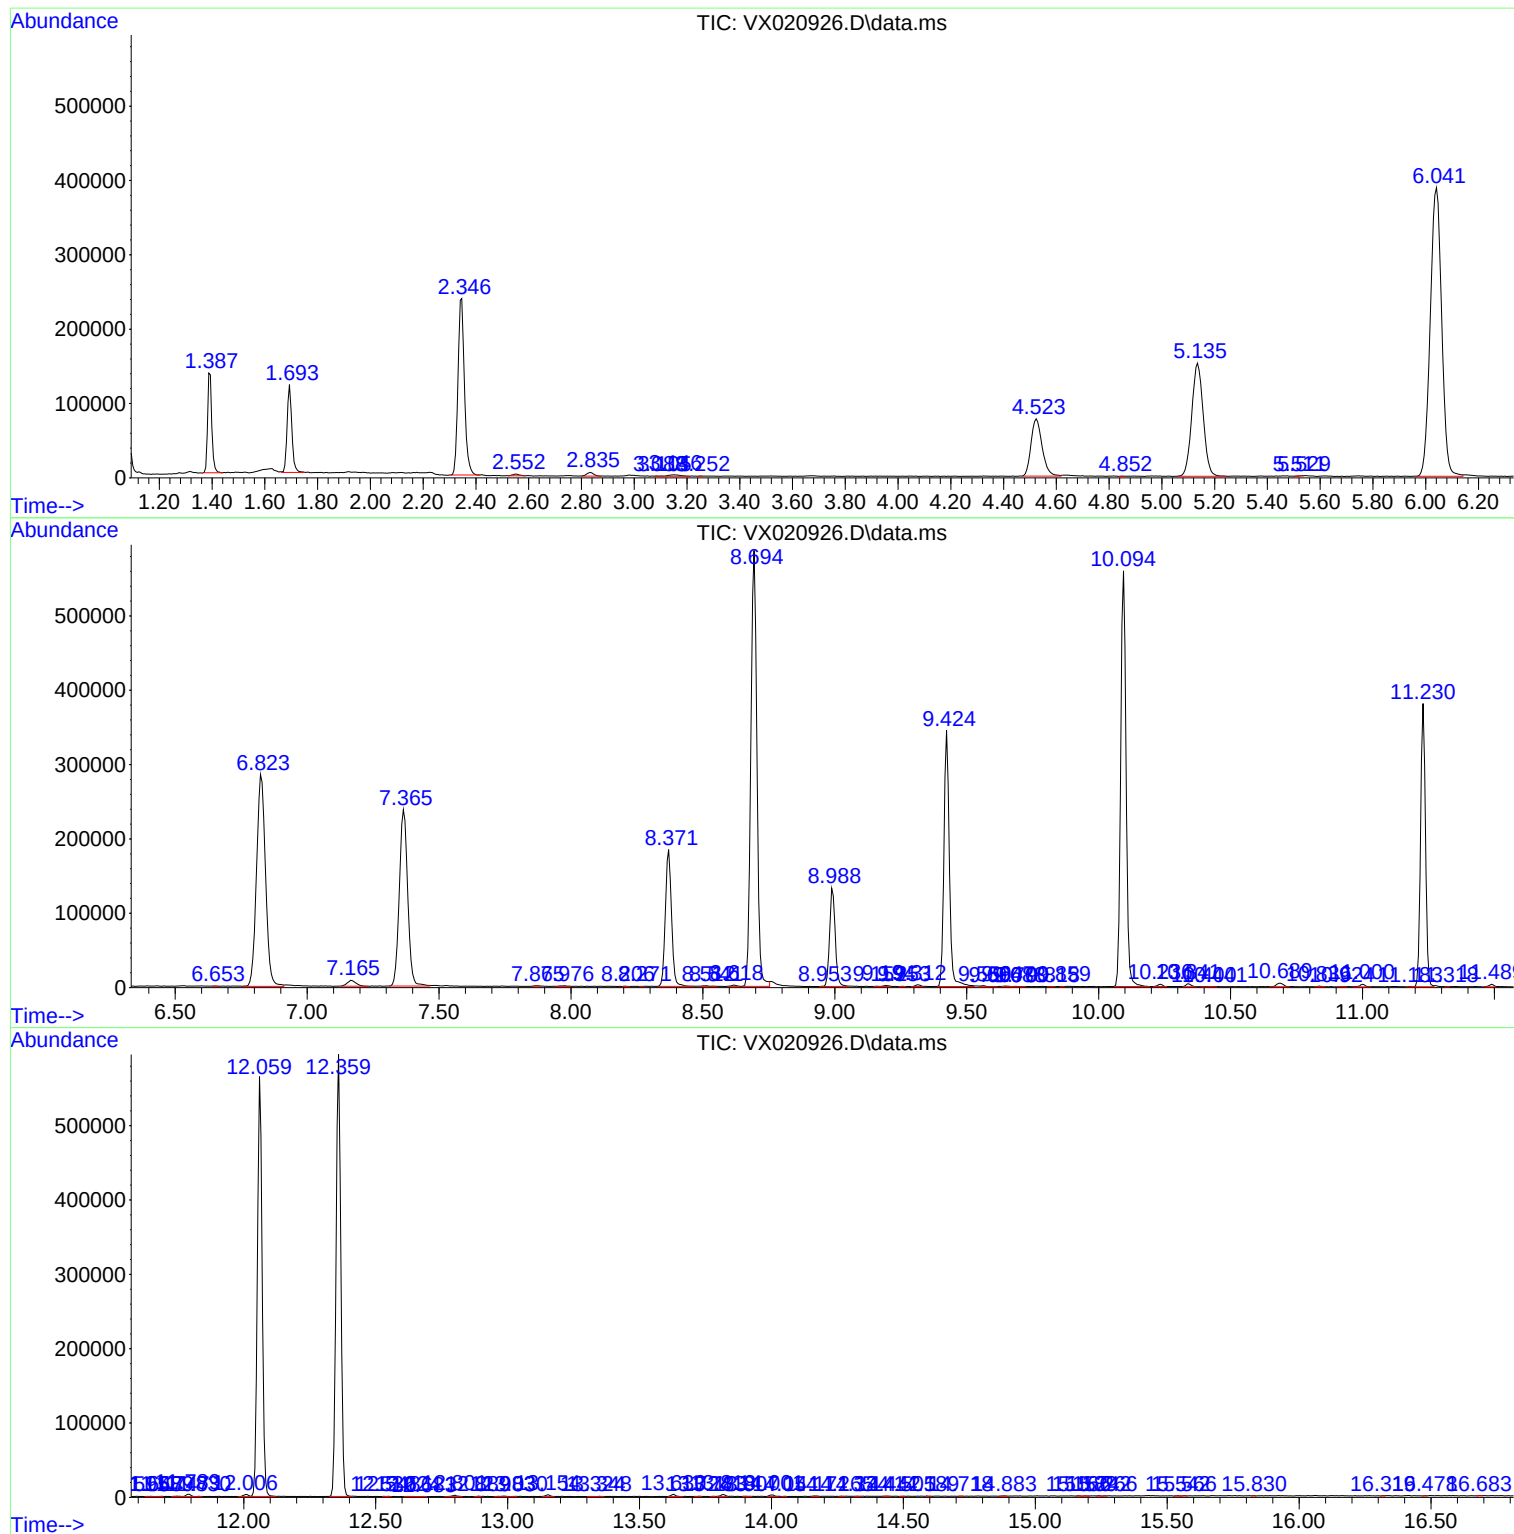

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
Data File : VX020926.D
Acq On : 26 Feb 2021 14:34
Operator : JC/MD
Sample : VX0226WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK404

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
Data File : VX020926.D
Acq On : 26 Feb 2021 14:34
Operator : JC/MD
Sample : VX0226WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK404

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
