

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
 Data File : VX020927.D
 Acq On : 26 Feb 2021 14:57
 Operator : JC/MD
 Sample : VX0226MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK405

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M

Title : VOC Analysis

Signal : TIC: VX020927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	30	32	35	rBV	1941	1650	0.14%	0.019%
2	1.393	48	52	62	rVB	146110	159423	13.33%	1.844%
3	1.693	99	103	114	rVB	130411	158289	13.24%	1.831%
4	2.346	207	214	227	rVB	261083	428531	35.83%	4.957%
5	2.675	268	270	272	rBV3	415	297	0.02%	0.003%
6	2.834	291	297	305	rBV3	4182	7878	0.66%	0.091%
7	2.917	309	311	315	rBV3	665	954	0.08%	0.011%
8	3.446	399	401	406	rBV3	503	703	0.06%	0.008%
9	3.511	410	412	416	rVB4	684	815	0.07%	0.009%
10	4.034	499	501	502	rVB	485	275	0.02%	0.003%
11	4.052	502	504	505	rBV	342	290	0.02%	0.003%
12	4.523	575	584	601	rBV	76222	223205	18.66%	2.582%
13	5.140	677	689	704	rBV	157080	470639	39.35%	5.445%
14	5.405	732	734	738	rBV3	398	531	0.04%	0.006%
15	6.046	830	843	863	rBV2	398873	1195983	100.00%	13.836%
16	6.594	933	936	939	rBV3	405	472	0.04%	0.005%
17	6.623	939	941	943	rVB2	497	255	0.02%	0.003%
18	6.829	965	976	990	rBV	274756	653856	54.67%	7.564%
19	7.170	1026	1034	1043	rVB3	7861	15884	1.33%	0.184%
20	7.276	1050	1052	1056	rVB4	542	560	0.05%	0.006%
21	7.364	1058	1067	1081	rBV	245291	535748	44.80%	6.198%
22	7.535	1094	1096	1099	rVB4	944	848	0.07%	0.010%
23	7.623	1109	1111	1113	rBV2	380	416	0.03%	0.005%
24	7.741	1127	1131	1135	rBV2	372	603	0.05%	0.007%
25	7.917	1158	1161	1163	rBV2	418	450	0.04%	0.005%
26	8.294	1223	1225	1228	rVB2	453	471	0.04%	0.005%
27	8.370	1231	1238	1251	rVV	190919	302752	25.31%	3.502%
28	8.694	1285	1293	1315	rBV	639829	1007029	84.20%	11.650%
29	8.994	1337	1344	1357	rVV	134993	199791	16.71%	2.311%
30	9.135	1364	1368	1373	rBV3	569	610	0.05%	0.007%
31	9.318	1395	1399	1402	rVV2	953	1185	0.10%	0.014%
32	9.423	1411	1417	1446	rVB	355673	503588	42.11%	5.826%
33	9.653	1451	1456	1459	rVB3	461	678	0.06%	0.008%
34	9.694	1459	1463	1465	rVB4	286	357	0.03%	0.004%
35	9.788	1475	1479	1482	rBV3	352	541	0.05%	0.006%
36	9.882	1491	1495	1497	rBV3	575	615	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
 Data File : VX020927.D
 Acq On : 26 Feb 2021 14:57
 Operator : JC/MD
 Sample : VX0226MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK405

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Title : VOC Analysis

37	10.006	1514	1516	1519	rVB2	490	338	0.03%	0.004%
38	10.094	1525	1531	1548	rBV	580296	772938	64.63%	8.942%
39	10.235	1550	1555	1557	rBV4	1051	1166	0.10%	0.013%
40	10.306	1564	1567	1568	rVB2	415	284	0.02%	0.003%
41	10.341	1568	1573	1577	rBV4	1647	2329	0.19%	0.027%
42	10.429	1586	1588	1591	rBV	358	300	0.03%	0.003%
43	10.494	1596	1599	1601	rVV3	236	280	0.02%	0.003%
44	10.518	1601	1603	1608	rVV2	293	349	0.03%	0.004%
45	10.688	1626	1632	1638	rBV6	1593	2894	0.24%	0.033%
46	11.006	1682	1686	1690	rVB4	796	1021	0.09%	0.012%
47	11.077	1694	1698	1700	rBV2	236	353	0.03%	0.004%
48	11.118	1703	1705	1708	rVB3	481	449	0.04%	0.005%
49	11.230	1718	1724	1737	rVB	399966	508055	42.48%	5.877%
50	11.347	1742	1744	1749	rVB2	588	677	0.06%	0.008%
51	11.394	1749	1752	1756	rVB3	401	424	0.04%	0.005%
52	11.488	1764	1768	1771	rBV3	859	1203	0.10%	0.014%
53	11.630	1790	1792	1796	rVV3	275	335	0.03%	0.004%
54	11.747	1810	1812	1816	rVB3	509	550	0.05%	0.006%
55	11.788	1816	1819	1824	rVB3	756	967	0.08%	0.011%
56	11.918	1839	1841	1848	rBV3	173	398	0.03%	0.005%
57	12.006	1852	1856	1860	rBV3	968	1162	0.10%	0.013%
58	12.059	1860	1865	1874	rBV	552973	680060	56.86%	7.867%
59	12.165	1881	1883	1888	rVB2	538	537	0.04%	0.006%
60	12.253	1896	1898	1901	rVB2	279	272	0.02%	0.003%
61	12.359	1910	1916	1923	rBV	637169	769559	64.35%	8.903%
62	12.500	1936	1940	1943	rBV3	337	661	0.06%	0.008%
63	12.553	1945	1949	1950	rVV3	419	469	0.04%	0.005%
64	12.600	1956	1957	1960	rVV	281	315	0.03%	0.004%
65	12.706	1974	1975	1977	rVV2	322	263	0.02%	0.003%
66	12.759	1983	1984	1986	rVV	403	271	0.02%	0.003%
67	12.800	1986	1991	1995	rVV2	1540	2277	0.19%	0.026%
68	12.841	1997	1998	2003	rVV4	262	370	0.03%	0.004%
69	12.894	2003	2007	2009	rVV4	625	652	0.05%	0.008%
70	12.953	2015	2017	2020	rVB3	228	265	0.02%	0.003%
71	13.024	2026	2029	2033	rBV3	377	536	0.04%	0.006%
72	13.153	2045	2051	2054	rBV3	1026	1264	0.11%	0.015%
73	13.224	2061	2063	2066	rVB	346	255	0.02%	0.003%
74	13.330	2079	2081	2083	rBV	415	274	0.02%	0.003%
75	13.500	2109	2110	2113	rBV2	302	274	0.02%	0.003%
76	13.530	2113	2115	2117	rBV2	341	263	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
 Data File : VX020927.D
 Acq On : 26 Feb 2021 14:57
 Operator : JC/MD
 Sample : VX0226MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK405

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Title : VOC Analysis

77	13.571	2121	2122	2125	rVB	366	303	0.03%	0.004%
78	13.630	2128	2132	2136	rVB4	1261	1597	0.13%	0.018%
79	13.665	2136	2138	2141	rBV2	369	385	0.03%	0.004%
80	13.812	2161	2163	2167	rVV2	1221	1166	0.10%	0.013%
81	13.942	2183	2185	2189	rBV2	375	330	0.03%	0.004%
82	14.000	2192	2195	2198	rBV4	1032	1177	0.10%	0.014%
83	14.071	2206	2207	2210	rVB2	587	518	0.04%	0.006%
84	14.095	2210	2211	2212	rBV	443	254	0.02%	0.003%
85	14.142	2216	2219	2220	rBV	400	337	0.03%	0.004%
86	14.165	2220	2223	2229	rVB2	776	1375	0.11%	0.016%
87	14.459	2270	2273	2275	rBV2	355	343	0.03%	0.004%
88	14.477	2275	2276	2279	rBV2	265	255	0.02%	0.003%
89	14.765	2324	2325	2328	rBV3	436	364	0.03%	0.004%
90	15.001	2363	2365	2367	rBV2	469	365	0.03%	0.004%
91	15.130	2383	2387	2388	rVB3	514	465	0.04%	0.005%
92	15.142	2388	2389	2391	rBV2	520	387	0.03%	0.004%
93	15.195	2396	2398	2400	rBV2	387	364	0.03%	0.004%
94	15.324	2417	2420	2421	rBV3	409	407	0.03%	0.005%
95	15.342	2421	2423	2425	rBV	431	366	0.03%	0.004%
96	15.830	2505	2506	2508	rBV	465	292	0.02%	0.003%
97	15.895	2516	2517	2519	rVB2	584	270	0.02%	0.003%
98	16.536	2625	2626	2629	rBV2	545	549	0.05%	0.006%
99	16.671	2647	2649	2653	rBV3	457	548	0.05%	0.006%
100	16.736	2659	2660	2662	rBV2	616	381	0.03%	0.004%


Sum of corrected areas: 8644279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
Data File : VX020927.D
Acq On : 26 Feb 2021 14:57
Operator : JC/MD
Sample : VX0226MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK405

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

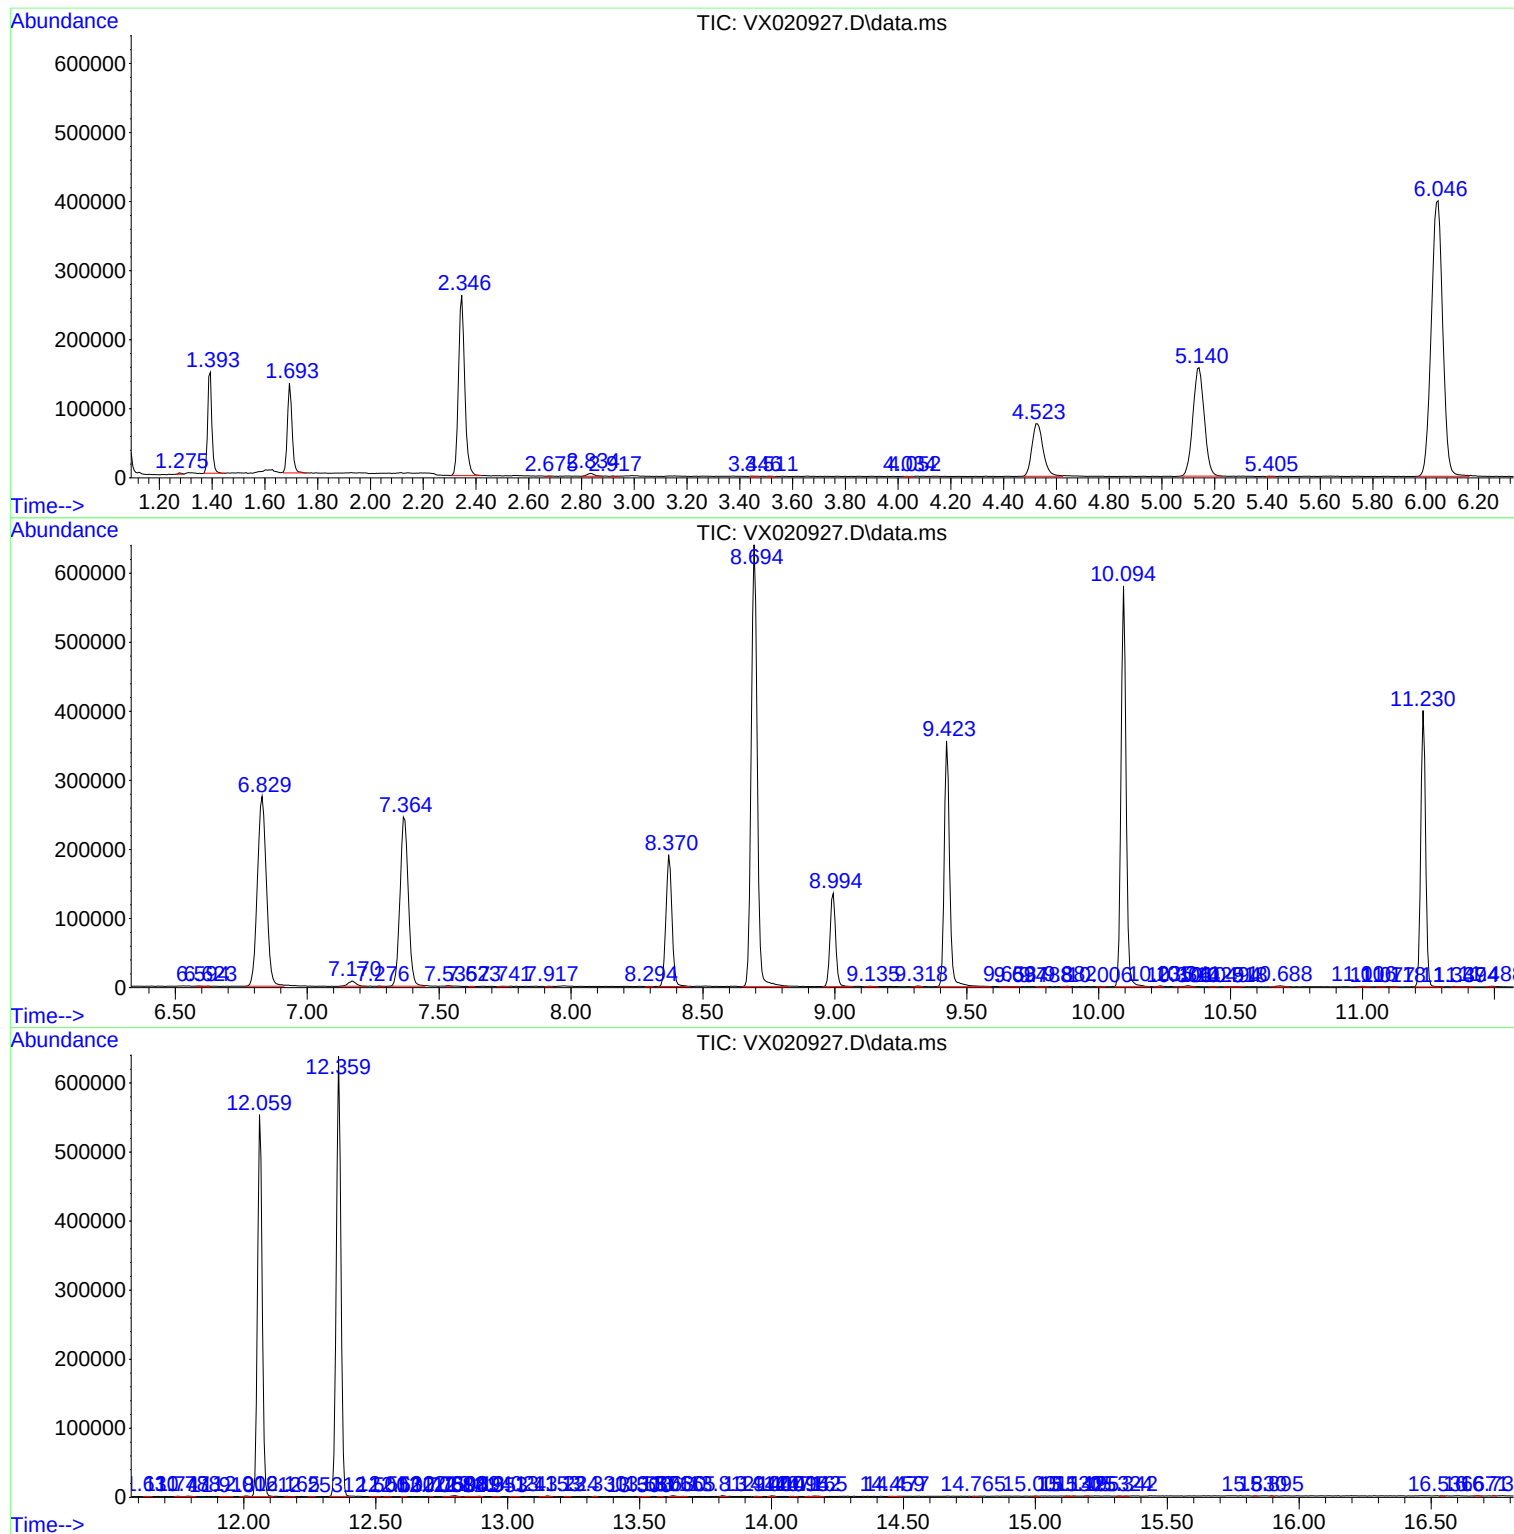

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
Data File : VX020927.D
Acq On : 26 Feb 2021 14:57
Operator : JC/MD
Sample : VX0226MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK405

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
Data File : VX020927.D
Acq On : 26 Feb 2021 14:57
Operator : JC/MD
Sample : VX0226MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK405

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
