


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022621\
 Data File : VX020919.D
 Acq On : 26 Feb 2021 09:17
 Operator : JC/MD
 Sample : BFB67
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB67

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM022621WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 03 01:05:22 2021

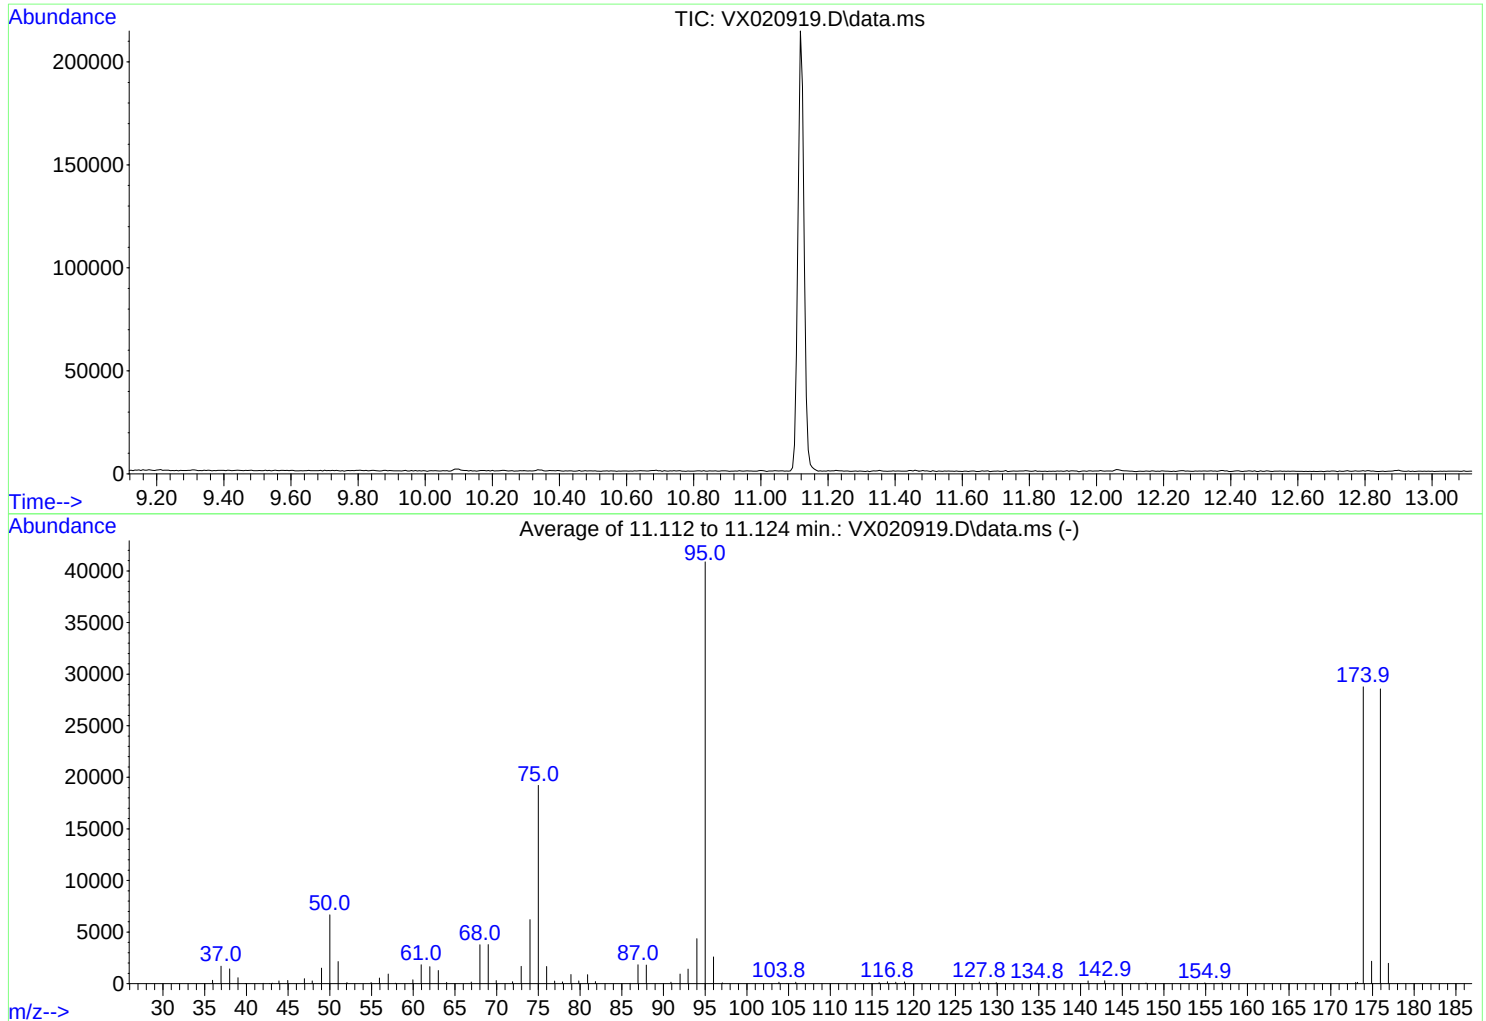

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1699

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	6669	PASS
75	95	30	80	47.0	19211	PASS
95	95	100	100	100.0	40885	PASS
96	95	5	9	6.4	2599	PASS
173	174	0.00	2	0.5	131	PASS
174	95	50	120	70.4	28771	PASS
175	174	5	9	7.6	2175	PASS
176	174	95	101	99.3	28563	PASS
177	176	5	9	6.9	1969	PASS

m/z	Abundance
36.00	336.0
36.90	1554.0
38.00	1407.0
39.00	532.0
39.90	538.0
41.10	63.0
43.10	65.0
43.90	843.0
44.90	253.0
47.00	486.0
47.90	214.0
49.00	1336.0
50.00	5783.0
51.00	1854.0
52.10	79.0
55.00	105.0
56.00	462.0
57.00	838.0
57.90	65.0
59.90	306.0
60.90	1526.0
62.00	1331.0
63.00	1156.0
64.00	121.0
66.90	155.0
68.00	3148.0
69.00	3449.0
69.90	273.0
71.90	164.0
73.00	1513.0
74.00	5468.0
75.00	16560.0
76.00	1484.0
77.00	207.0
77.90	139.0
78.90	721.0
79.90	269.0
80.90	674.0
81.80	176.0
86.90	1557.0
87.90	1349.0
90.90	123.0
92.00	845.0
92.90	1099.0
94.00	3736.0
95.00	32520.0
96.00	2268.0
97.00	79.0
103.90	107.0
105.80	89.0
115.80	72.0
116.90	135.0
117.90	98.0
118.90	123.0
128.00	101.0
129.90	102.0
134.80	65.0
140.90	205.0
142.90	191.0
147.90	62.0
154.90	72.0
156.90	85.0
173.00	138.0
173.90	18904.0
174.90	1651.0
175.90	19064.0
176.90	1433.0
207.00	130.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67

m/z	Abundance
36.00	377.0
37.00	2043.0
38.00	1643.0
39.00	658.0
39.90	556.0
41.10	60.0
42.80	58.0
43.90	969.0
45.00	399.0
47.00	486.0
47.90	346.0
49.00	1767.0
50.00	8025.0
51.00	2591.0
52.00	165.0
55.00	109.0
56.00	656.0
57.00	1133.0
57.90	87.0
60.00	447.0
61.00	2115.0
62.00	2075.0
63.00	1467.0
63.90	150.0
66.90	186.0
68.00	4523.0
69.00	4262.0
70.00	325.0
71.80	223.0
73.00	2038.0
74.00	7276.0
75.00	22856.0
76.00	2041.0
76.90	292.0
77.80	177.0
78.90	1084.0
79.90	305.0
80.90	1038.0
81.90	230.0
86.00	93.0
87.00	2152.0
87.90	2473.0
90.80	161.0
92.00	974.0
93.00	1624.0
94.00	5274.0
95.00	49256.0
96.00	2944.0
97.10	99.0
103.80	194.0
104.80	57.0
105.90	201.0
115.80	157.0
116.80	203.0
117.80	182.0
118.90	209.0
127.80	193.0
128.90	54.0
130.00	127.0
134.80	72.0
137.00	52.0
140.90	307.0
142.90	347.0
147.80	66.0
154.90	102.0
157.00	54.0
173.00	256.0
173.90	33664.0
174.90	2430.0
176.00	33408.0
176.90	2255.0
207.00	90.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67

m/z	Abundance
35.90	261.0
37.00	1456.0
38.00	1230.0
39.00	534.0
39.90	536.0
41.10	80.0
42.00	72.0
43.10	74.0
44.00	911.0
45.00	299.0
46.90	461.0
47.90	244.0
49.00	1406.0
50.00	6199.0
51.00	1990.0
52.00	81.0
54.90	138.0
55.90	491.0
57.00	847.0
59.90	353.0
61.00	1831.0
62.00	1544.0
63.00	1178.0
64.10	116.0
67.00	142.0
68.00	3614.0
69.00	3656.0
69.90	293.0
72.00	192.0
72.90	1476.0
74.00	5852.0
75.00	18216.0
76.00	1460.0
76.90	257.0
78.00	188.0
78.90	857.0
79.80	220.0
80.90	880.0
81.90	196.0
86.90	1792.0
88.00	1591.0
91.00	131.0
92.00	986.0
93.00	1529.0
94.00	4089.0
95.00	40880.0
96.00	2585.0
97.00	75.0
103.90	128.0
104.80	57.0
105.90	116.0
115.90	118.0
116.90	213.0
117.80	134.0
118.90	178.0
127.90	175.0
128.80	75.0
129.80	102.0
134.80	76.0
140.90	283.0
142.90	301.0
147.80	84.0
154.90	81.0
157.00	61.0
171.90	63.0
173.20	391.0
173.90	33744.0
174.90	2444.0
175.90	33216.0
176.90	2218.0
207.00	110.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67

Scan 1699 (11.083 min): VX020919.D\data.ms
BFB67

m/z	Abundance
39.90	525.0
41.00	70.0
43.90	643.0
207.00	110.0

Instrument :
MSVOA_X
ClientSampleId :
BFB67