


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX022719\
Data File : VX007729.D
Acq On : 27 Feb 2019 12:06
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X022519W.M
Title : SW846 8260
Last Update : Tue Feb 26 01:53:13 2019

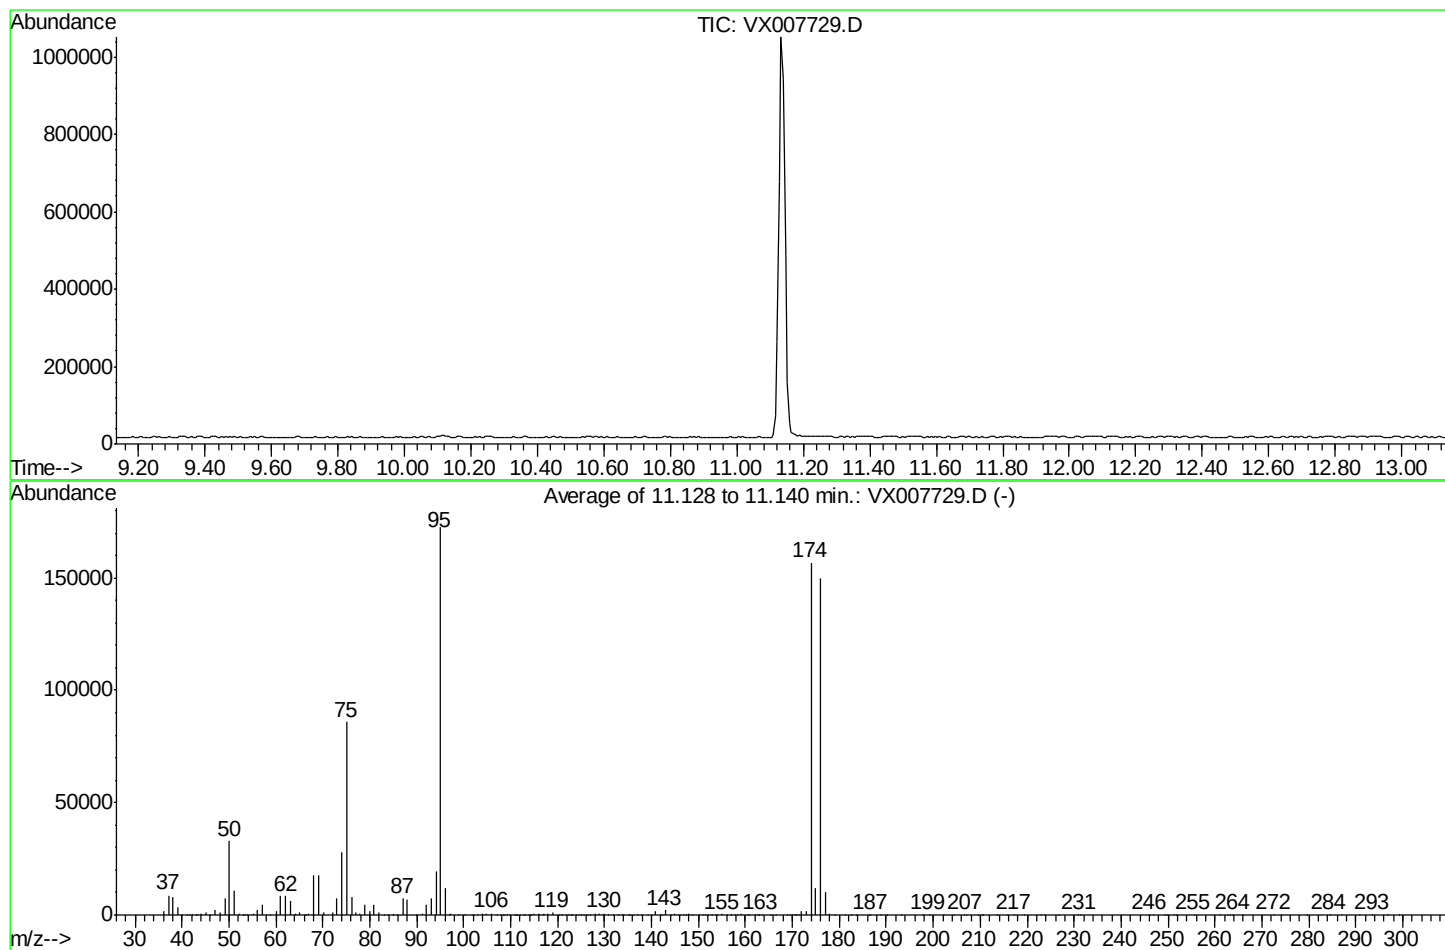

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	32913	PASS
75	95	30	60	49.8	85914	PASS
95	95	100	100	100.0	172526	PASS
96	95	5	9	6.8	11803	PASS
173	174	0.00	2	1.2	1840	PASS
174	95	50	100	90.9	156842	PASS
175	174	5	9	7.5	11750	PASS
176	174	95	101	95.7	150111	PASS
177	176	5	9	6.7	10084	PASS