

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\WX022720\
 Data File : VX015038.D
 Acq On : 27 Feb 2020 11:28
 Operator : JC/SP
 Sample : L1694-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VOC-TRIP-BLANK

Quant Time: Feb 27 15:47:57 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 10 12:09:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	456631	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	718372	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	672999	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	332819	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.05	65	253770	49.24	ug/l	0.00
Spiked Amount			Recovery	=	98.48%	
35) Dibromofluoromethane	5.49	113	218388	49.45	ug/l	0.00
Spiked Amount			Recovery	=	98.90%	
50) Toluene-d8	8.71	98	863166	51.20	ug/l	0.00
Spiked Amount			Recovery	=	102.40%	
62) 4-Bromofluorobenzene	11.13	95	307358	50.61	ug/l	0.00
Spiked Amount			Recovery	=	101.22%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.66	94	1708	0.50	ug/l	86
10) Methyl Iodide	2.52	142	2091	4.77	ug/l #	89
11) Tert butyl alcohol	3.02	59	945	1.04	ug/l #	54
13) Acrolein	2.24	56	472	0.68	ug/l	98
16) Acetone	2.43	43	1541	Below Cal	#	45
17) Carbon Disulfide	2.57	76	3112	0.27	ug/l #	79
18) Methyl Acetate	2.76	43	2754	0.53	ug/l #	80
20) Methylene Chloride	2.86	84	1108	0.22	ug/l #	71
21) trans-1,2-Dichloroethene	3.16	96	1081	0.23	ug/l #	64
29) Tetrahydrofuran	5.11	42	508	0.25	ug/l #	48
36) 1,1-Dichloropropene	5.65	75	30080	4.68	ug/l #	52
38) Carbon Tetrachloride	5.65	117	37819	6.04	ug/l #	16
42) 1,2-Dichloroethane	6.18	62	1501	0.22	ug/l	100
44) Trichloroethene	7.20	130	1959	0.35	ug/l	71
49) 1,4-Dioxane	7.74	88	289	2.84	ug/l #	6
68) m/p-Xylenes	10.35	106	2018	0.23	ug/l #	54
76) 1,2,3-Trichloropropane	11.13	75	147997	24.59	ug/l #	41
81) trans-1,4-Dichloro-2-buten	11.13	75	147997	62.94	ug/l #	12
87) 1,3-Dichlorobenzene	12.02	146	2575	0.25	ug/l	90
88) 1,4-Dichlorobenzene	12.02	146	2575	0.24	ug/l	91
89) n-Butylbenzene	12.39	91	5142	0.30	ug/l	94
91) 1,2-Dichlorobenzene	12.39	146	2178	0.21	ug/l	96
93) 1,2,4-Trichlorobenzene	13.64	180	3219	0.43	ug/l	95
94) Hexachlorobutadiene	13.78	225	1663	0.45	ug/l	88
95) Naphthalene	13.83	128	6697	0.33	ug/l #	88
96) 1,2,3-Trichlorobenzene	14.02	180	2946	0.40	ug/l	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX022720\
Data File : VX015038.D
Acq On : 27 Feb 2020 11:28
Operator : JC/SP
Sample : L1694-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VOC-TRIP-BLANK

Quant Time: Feb 27 15:47:57 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 10 12:09:20 2020
Response via : Initial Calibration

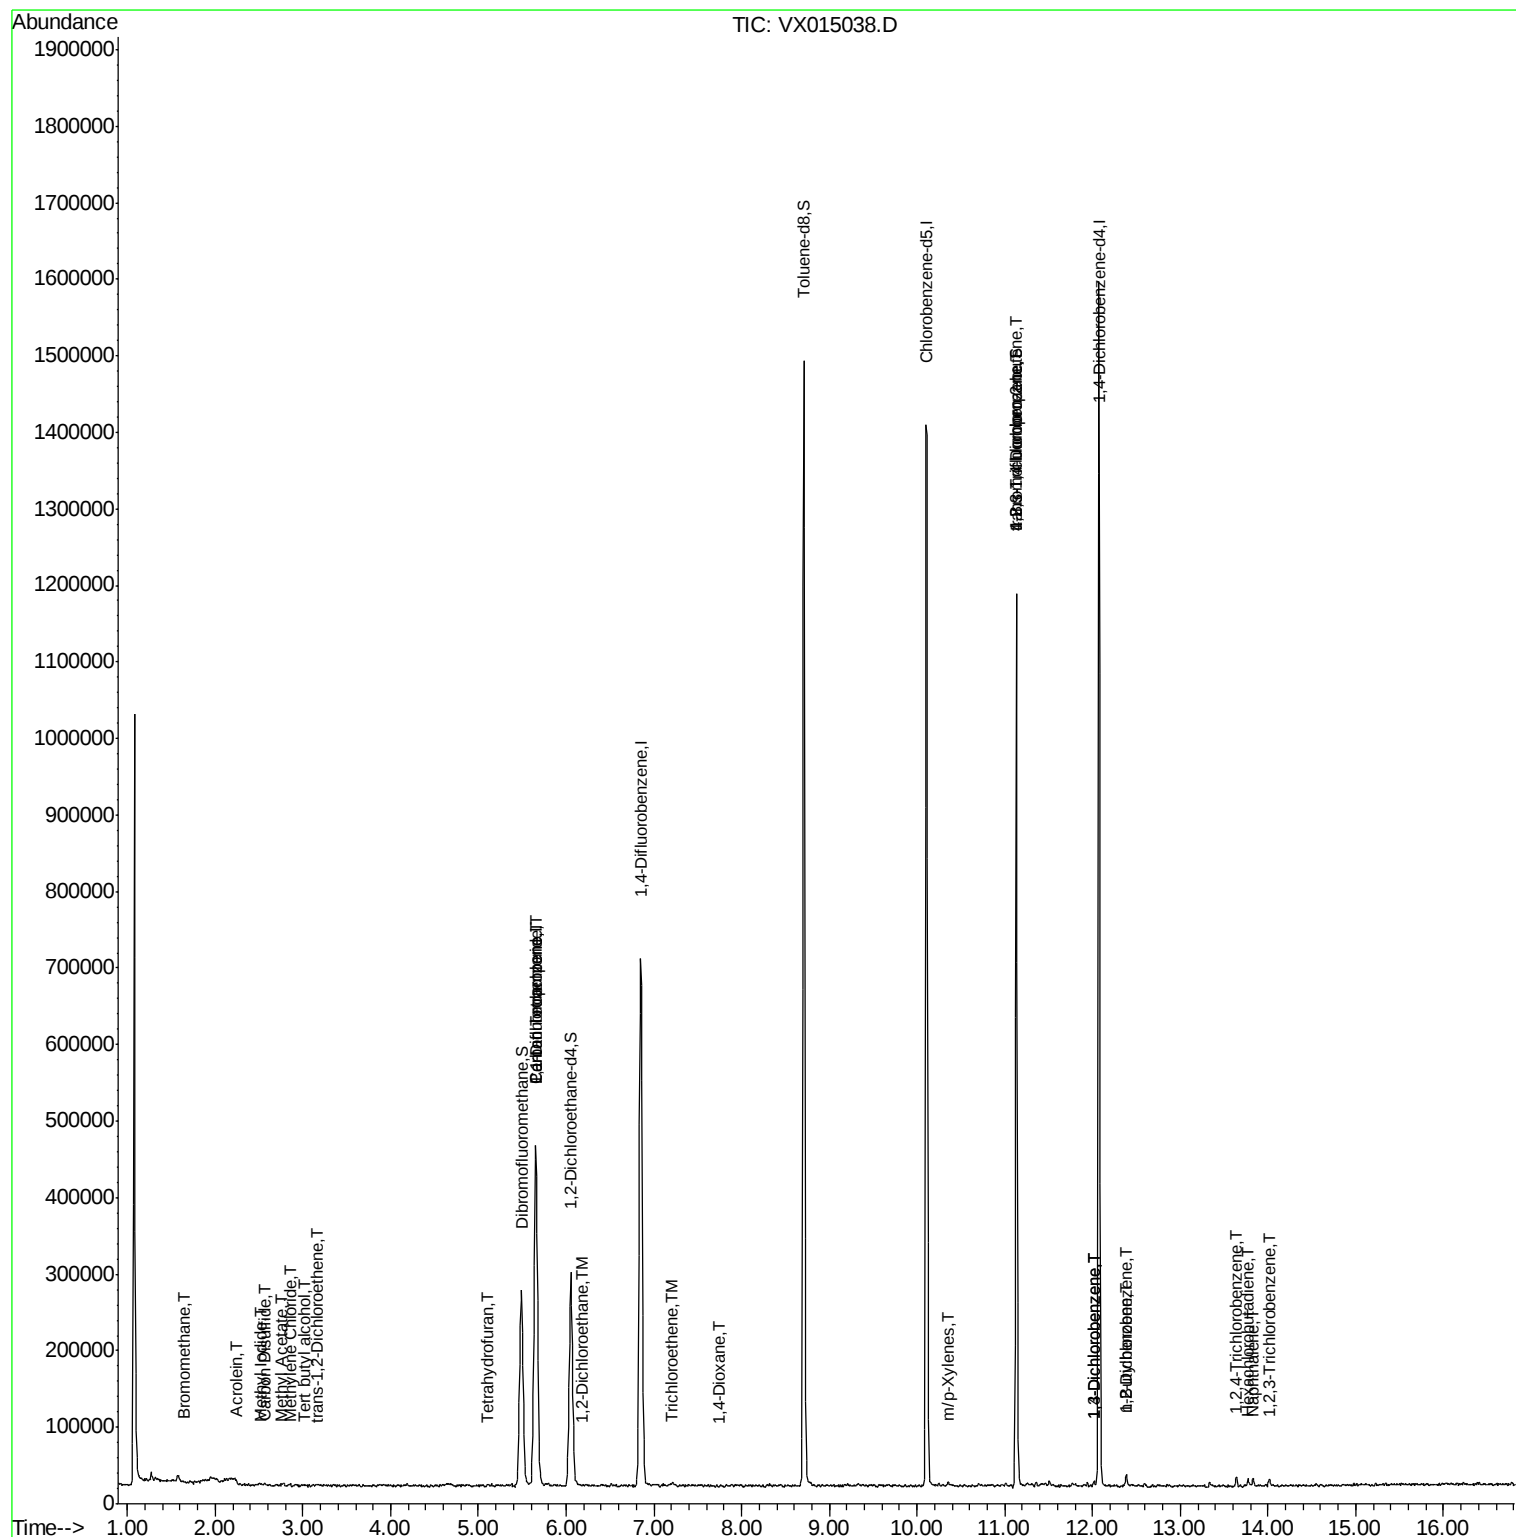

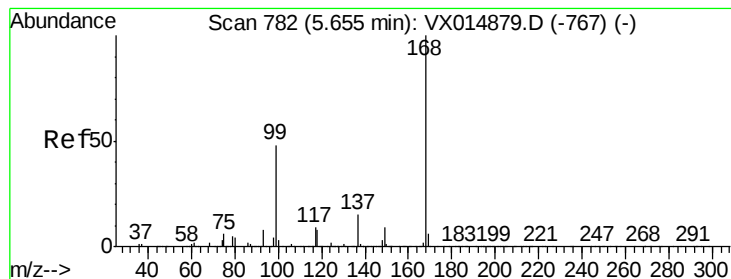

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.65 min Scan# 782

Delta R.T. -0.00 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28

Instrument :

MSVOA_X

ClientSampleId :


VOC-TRIP-BLANK

Tgt Ion: 168 Resp: 456631

Ion Ratio Lower Upper

168 100

99 48.7 38.7 58.1



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80



#5

Bromomethane

Concen: 0.50 ug/l

RT: 1.66 min Scan# 126

Delta R.T. 0.02 min

Lab File: VX015038.D


Acq: 27 Feb 2020 11:28

Tgt Ion: 94 Resp: 1708

Ion Ratio Lower Upper

94 100

96 105.8 73.7 110.5



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1000

800

600


400


200

0

Time-->

1.60 1.65 1.70







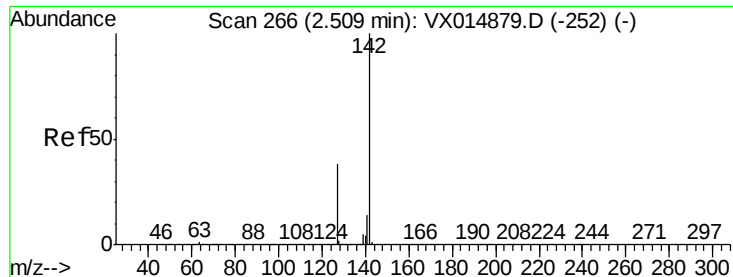

#10
Methyl Iodide
Concen: 4.77 ug/l
RT: 2.52 min Scan# 268
Delta R.T. 0.01 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28




Instrument :
MSVOA_X
ClientSampleId :
VOC-TRIP-BLANK


Tgt Ion: 142 Resp: 2091
Ion Ratio Lower Upper
142 100
127 32.8 31.1 46.7
141 20.0 11.3 16.9#

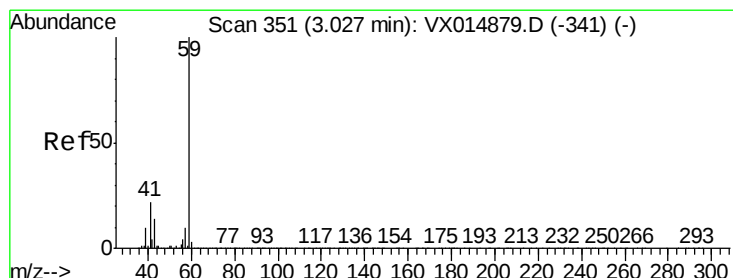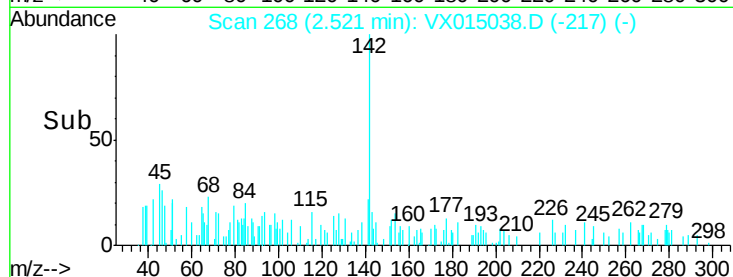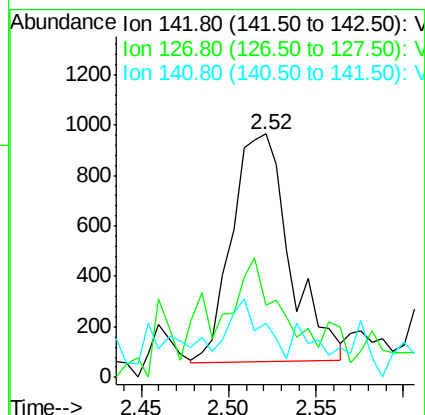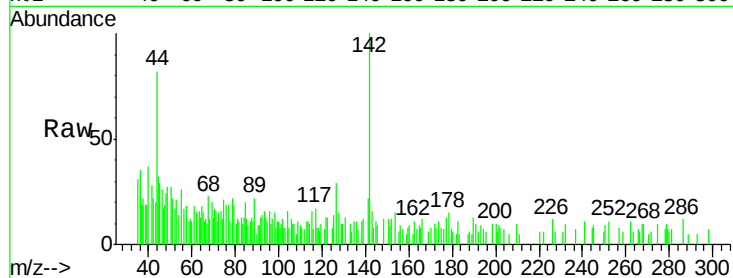

#11
Tert butyl alcohol
Concen: 1.04 ug/l
RT: 3.02 min Scan# 350
Delta R.T. -0.01 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28

Tgt Ion: 59 Resp: 945
Ion Ratio Lower Upper
59 100
57 27.4 8.2 12.4#

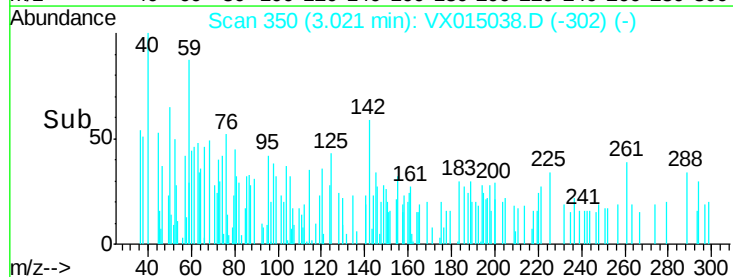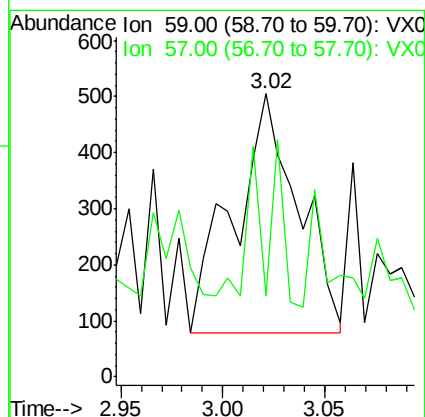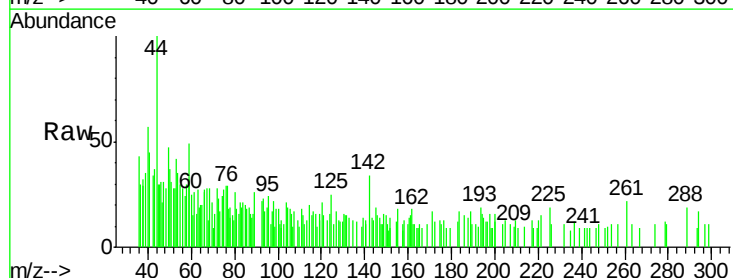



#13

Acrolein

Concen: 0.68 ug/l

RT: 2.24 min Scan# 222

Delta R.T. -0.05 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28

Instrument :

MSVOA_X

ClientSampleId :


VOC-TRIP-BLANK

Tgt Ion: 56 Resp: 472

Ion Ratio Lower Upper




56 100

55 67.2 55.0 82.4



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

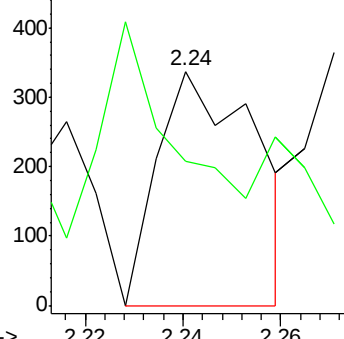

#16

Acetone

Concen: Below Cal

RT: 2.43 min Scan# 253

Delta R.T. 0.00 min

Lab File: VX015038.D


Acq: 27 Feb 2020 11:28

Tgt Ion: 43 Resp: 1541

Ion Ratio Lower Upper



43 100


58 0.0 24.1 36.1#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

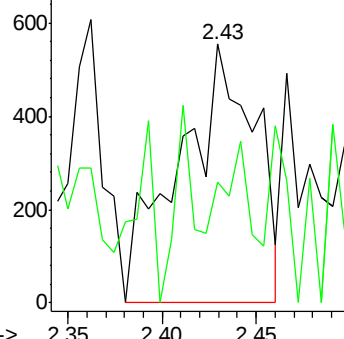

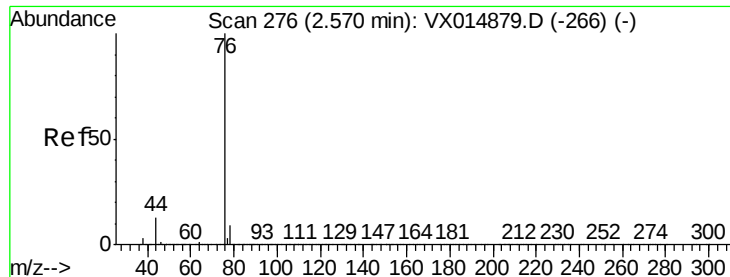

#17

Carbon Disulfide

Concen: 0.27 ug/l

RT: 2.57 min Scan# 276

Delta R.T. -0.00 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28

Instrument :

MSVOA_X

ClientSampleId :


VOC-TRIP-BLANK

Tgt Ion: 76 Resp: 3112

Ion Ratio Lower Upper




76 100

78 1.4 7.4 11.0#

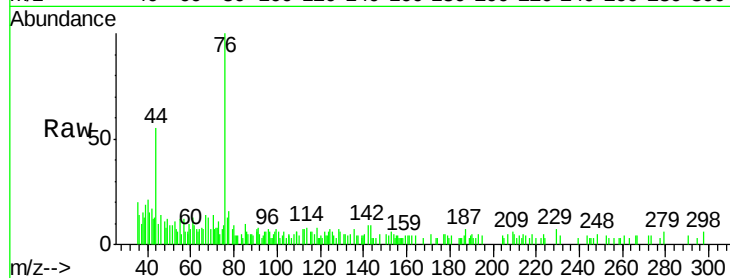

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

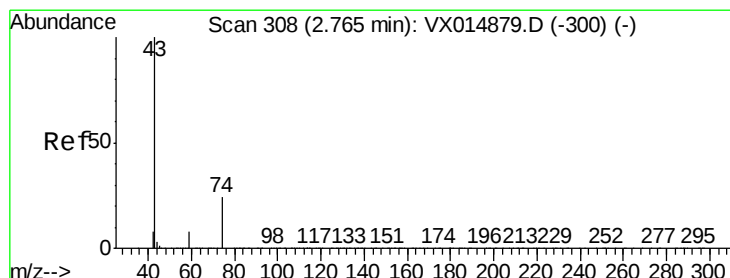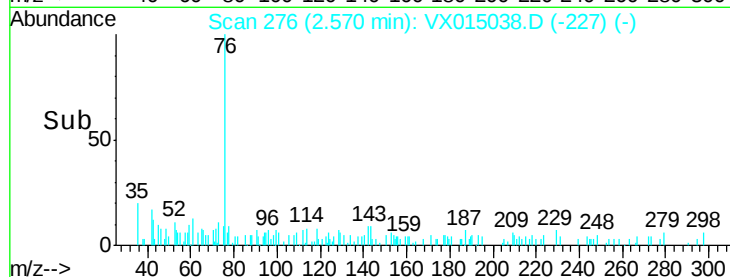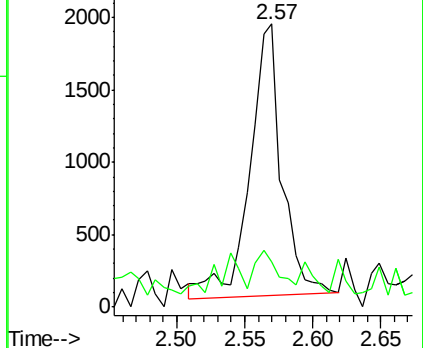

#18

Methyl Acetate

Concen: 0.53 ug/l

RT: 2.76 min Scan# 308

Delta R.T. -0.00 min

Lab File: VX015038.D


Acq: 27 Feb 2020 11:28

Tgt Ion: 43 Resp: 2754

Ion Ratio Lower Upper



43 100


74 14.1 19.4 29.0#

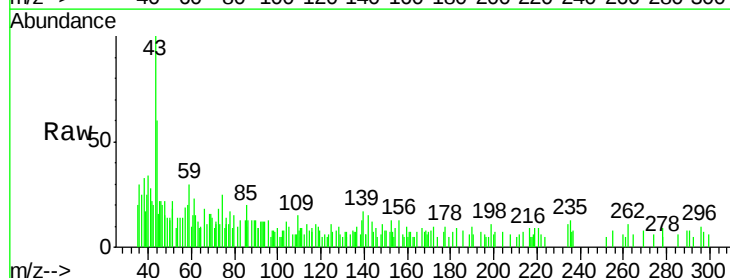

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0



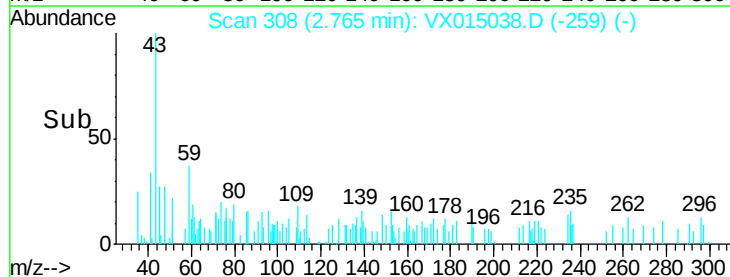
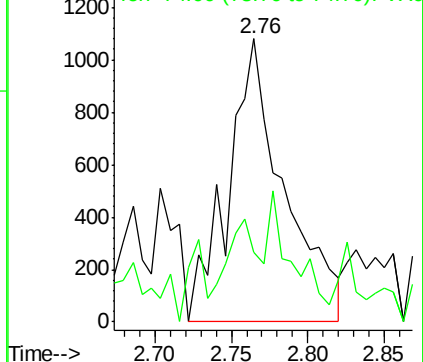




#20
Methylene Chloride
Concen: 0.22 ug/l
RT: 2.86 min Scan# 324
Delta R.T. 0.01 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28




Instrument :
MSVOA_X
ClientSampleId :
VOC-TRIP-BLANK


Tgt Ion: 84 Resp: 1108
Ion Ratio Lower Upper
84 100
49 101.3 95.6 143.4
51 8.3 29.0 43.6#
86 31.1 51.4 77.0#

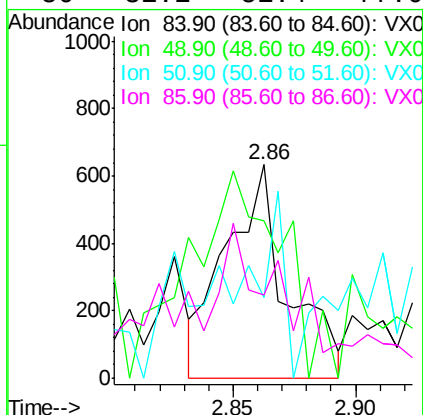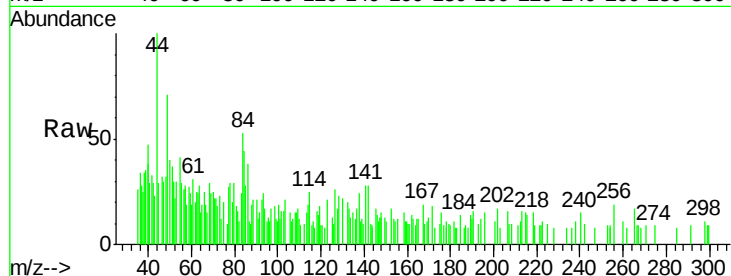

#21
trans-1,2-Dichloroethene
Concen: 0.23 ug/l
RT: 3.16 min Scan# 373
Delta R.T. -0.00 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28

Tgt Ion: 96 Resp: 1081
Ion Ratio Lower Upper
96 100
61 73.3 106.9 160.3#
98 66.8 50.7 76.1


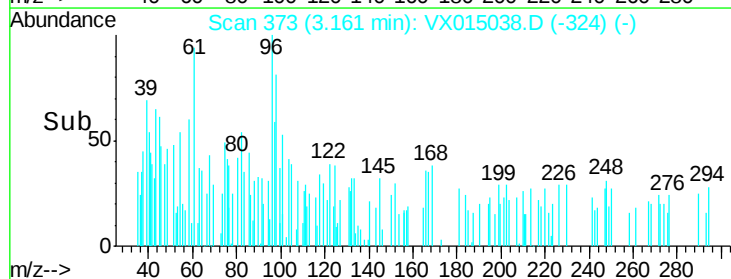
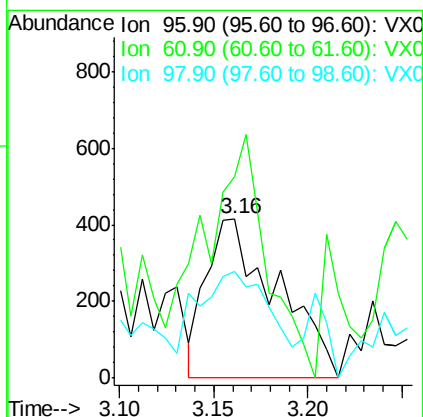



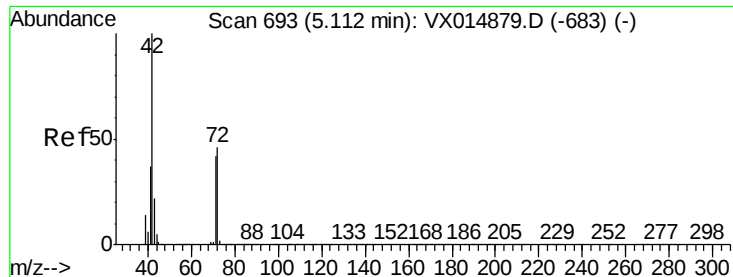

#29
Tetrahydrofuran
Concen: 0.25 ug/l
RT: 5.11 min Scan# 692
Delta R.T. -0.01 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28




Instrument :
MSVOA_X
ClientSampleId :
VOC-TRIP-BLANK


Tgt Ion: 42 Resp: 508
Ion Ratio Lower Upper
42 100
72 21.1 36.9 55.3#
71 0.0 34.1 51.1#

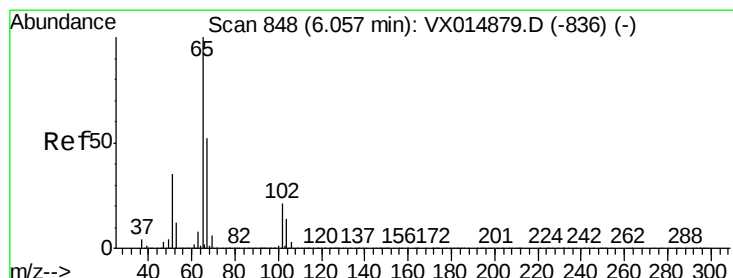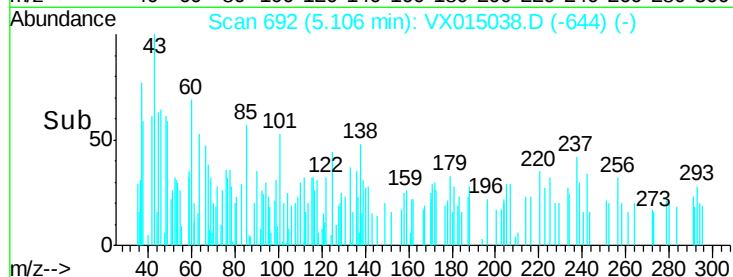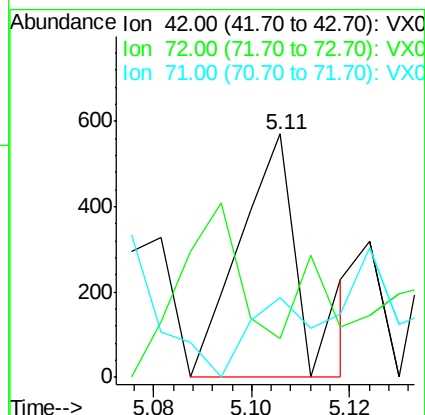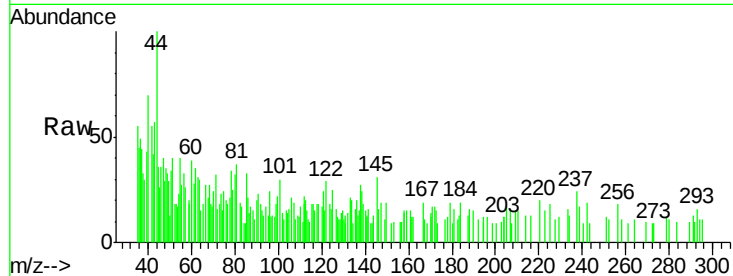

#33
1,2-Dichloroethane-d4
Concen: 49.24 ug/l
RT: 6.05 min Scan# 847
Delta R.T. -0.01 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28

Tgt Ion: 65 Resp: 253770
Ion Ratio Lower Upper
65 100
67 53.0 0.0 103.0

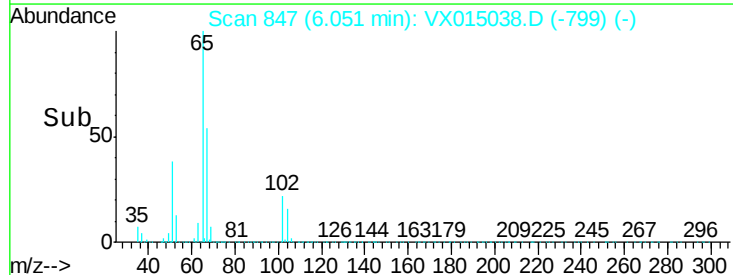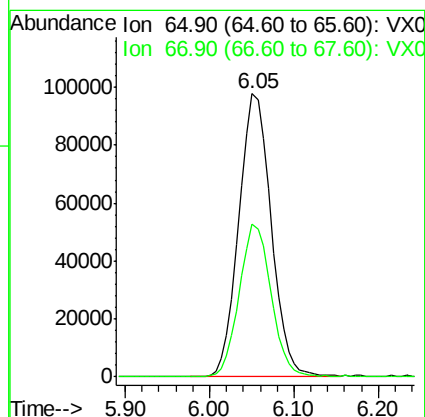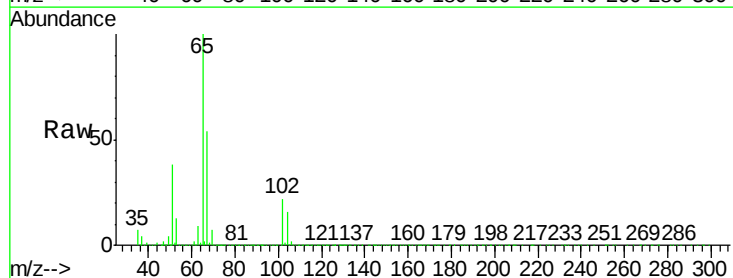



#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.85 min Scan# 978

Delta R.T. -0.00 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28

Instrument :

MSVOA_X

ClientSampleId :

VOC-TRIP-BLANK


Tgt Ion:114 Resp: 718372

Ion Ratio Lower Upper

114 100

63 20.3 0.0 39.2




88 15.9 0.0 32.0

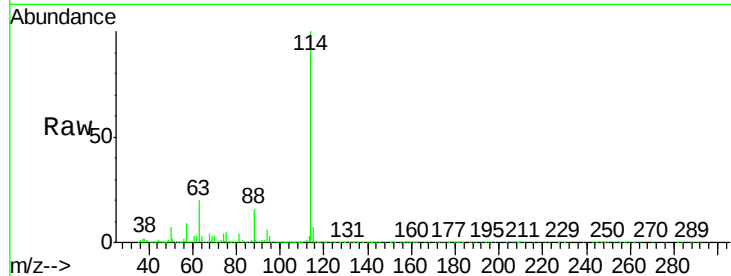

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

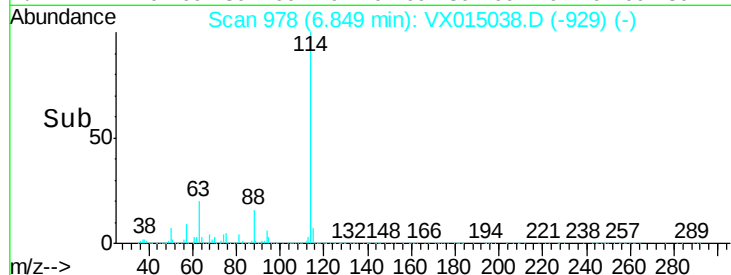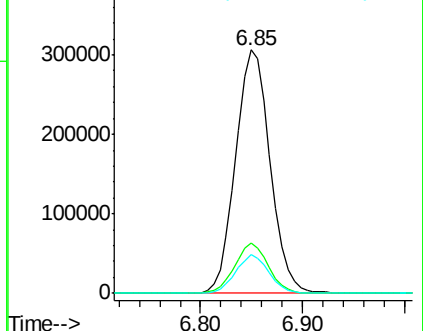

#35

Dibromofluoromethane

Concen: 49.45 ug/l

RT: 5.49 min Scan# 755

Delta R.T. -0.00 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28


Tgt Ion:113 Resp: 218388

Ion Ratio Lower Upper

113 100

111 103.0 82.4 123.6



192 24.1 19.1 28.7

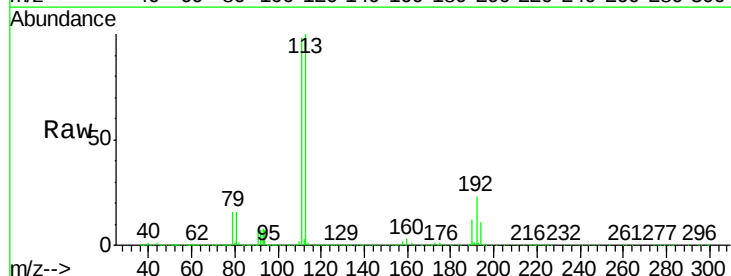


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V




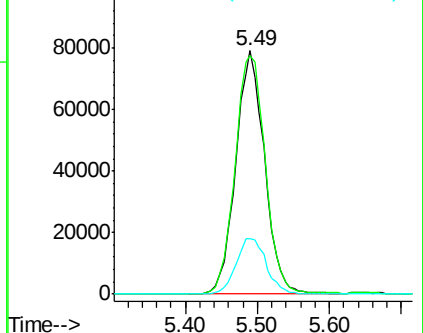


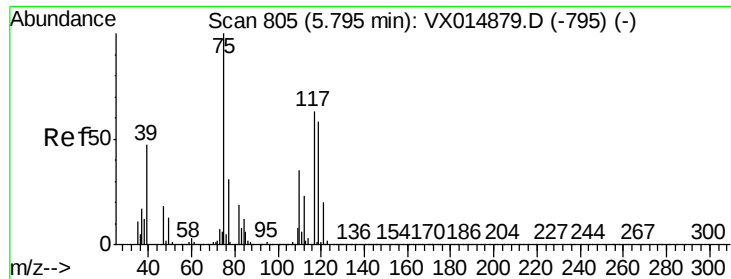

#36
 1,1-Dichloropropene
 Concen: 4.68 ug/l
 RT: 5.65 min Scan# 782
 Delta R.T. -0.14 min
 Lab File: VX015038.D
 Acq: 27 Feb 2020 11:28




Instrument :
 MSVOA_X
 ClientSampleId :
 VOC-TRIP-BLANK


Tgt Ion	Ratio	Lower	Upper
75	100		
110	11.0	18.3	54.8#
77	0.7	24.6	36.8#

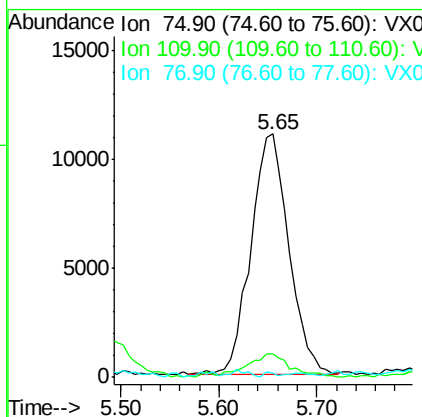

#38
 Carbon Tetrachloride
 Concen: 6.04 ug/l
 RT: 5.65 min Scan# 781
 Delta R.T. -0.13 min
 Lab File: VX015038.D
 Acq: 27 Feb 2020 11:28

Tgt Ion	Ratio	Lower	Upper
117	100		
119	4.7	76.0	114.0#
121	0.2	25.4	38.2#

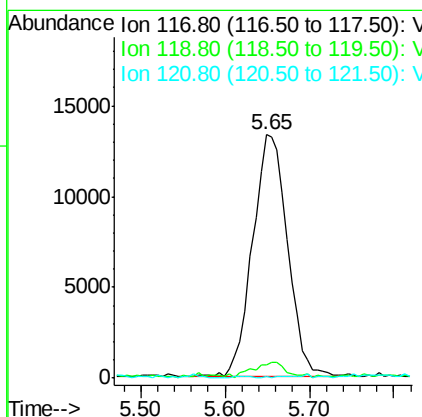

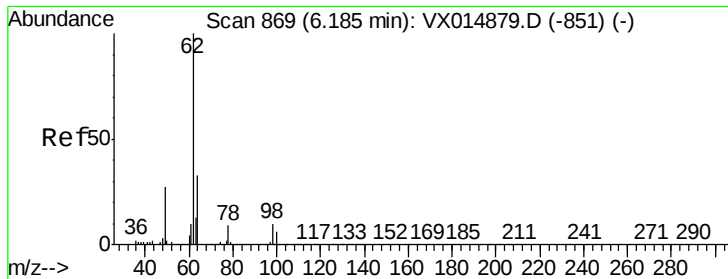

#42

1,2-Dichloroethane

Concen: 0.22 ug/l

RT: 6.18 min Scan# 868

Delta R.T. -0.01 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28

Instrument :

MSVOA_X

ClientSampleId :


VOC-TRIP-BLANK

Tgt Ion: 62 Resp: 1501

Ion Ratio Lower Upper


62 100

98 9.7 0.0 19.2


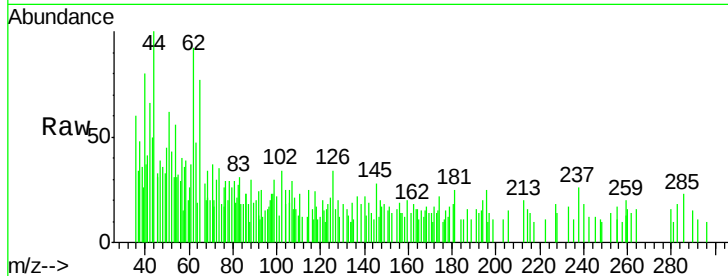


Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

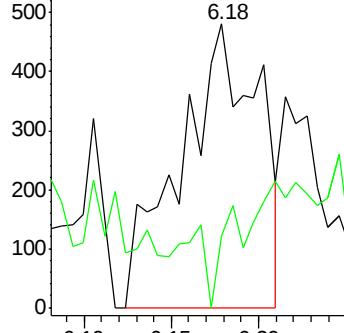

Time-->

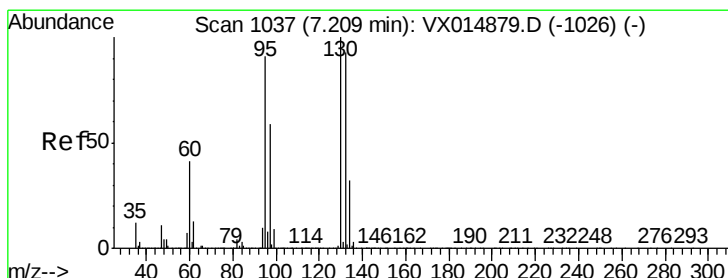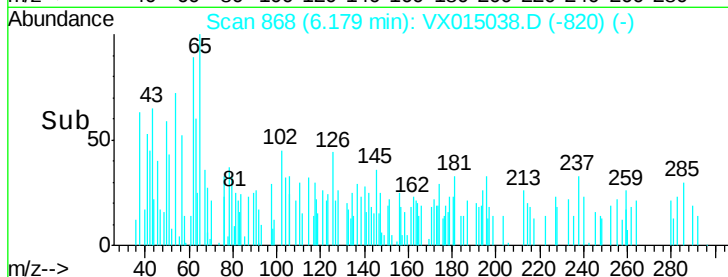

#44

Trichloroethene

Concen: 0.35 ug/l

RT: 7.20 min Scan# 1036

Delta R.T. -0.01 min

Lab File: VX015038.D


Acq: 27 Feb 2020 11:28

Tgt Ion: 130 Resp: 1959

Ion Ratio Lower Upper


130 100

95 63.7 0.0 182.6

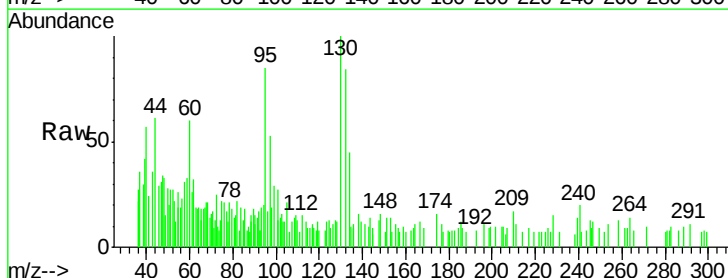



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

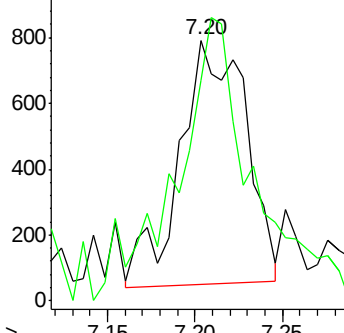

Time-->

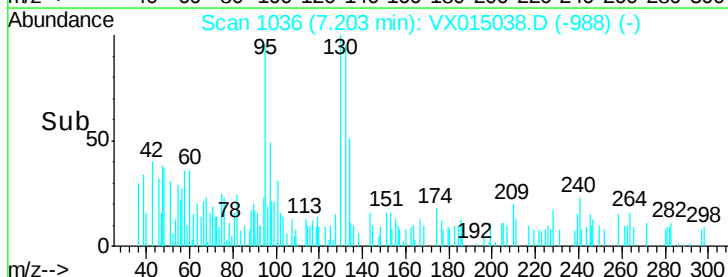

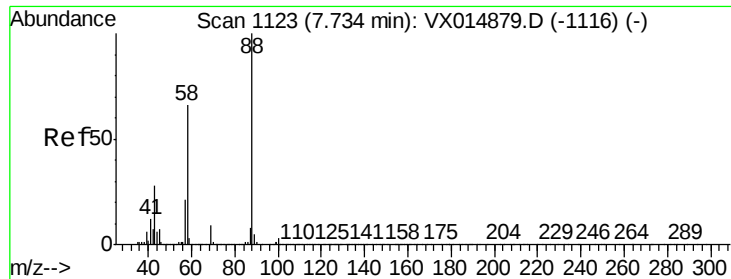

#49

1,4-Dioxane

Concen: 2.84 ug/l

RT: 7.74 min Scan# 1124

Delta R.T. 0.01 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28

Instrument :

MSVOA_X

ClientSampleId :

VOC-TRIP-BLANK


Tgt Ion: 88 Resp: 289

Ion Ratio Lower Upper

88 100

43 168.2 27.0 40.4#




58 84.1 53.2 79.8#

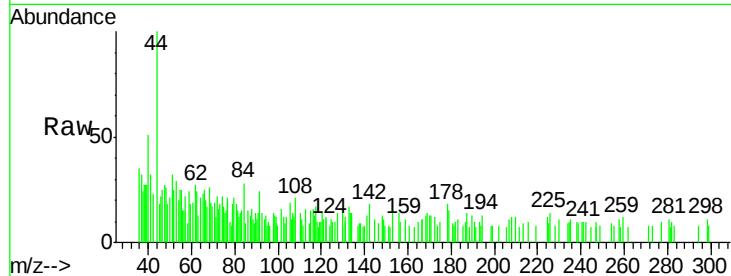

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

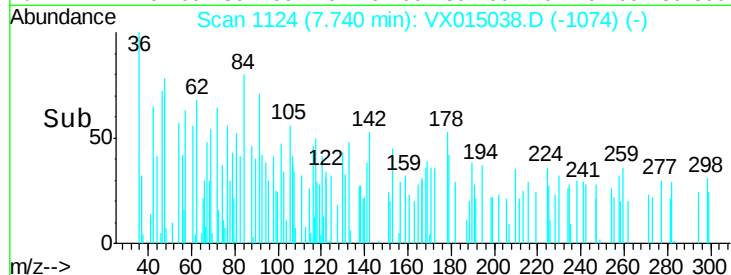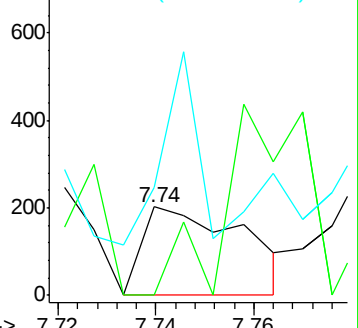

#50

Toluene-d8

Concen: 51.20 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. -0.00 min

Lab File: VX015038.D


Acq: 27 Feb 2020 11:28

Tgt Ion: 98 Resp: 863166

Ion Ratio Lower Upper



98 100


100 65.7 52.4 78.6



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0




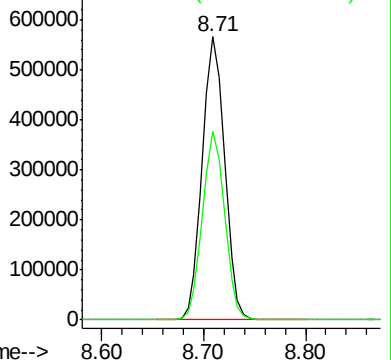


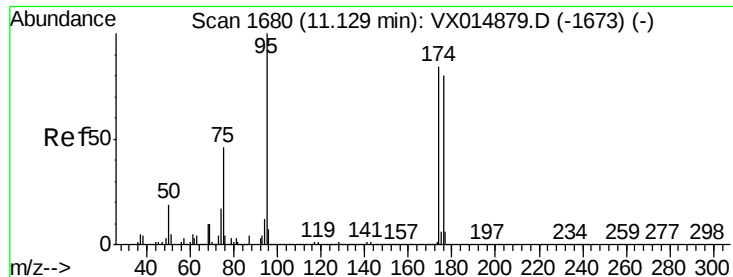

#62
4-Bromofluorobenzene
Concen: 50.61 ug/l
RT: 11.13 min Scan# 1680
Delta R.T. -0.00 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28




Instrument :
MSVOA_X
ClientSampleId :
VOC-TRIP-BLANK


Tgt Ion: 95 Resp: 307358
Ion Ratio Lower Upper
95 100
174 89.6 0.0 183.0
176 87.0 0.0 178.0

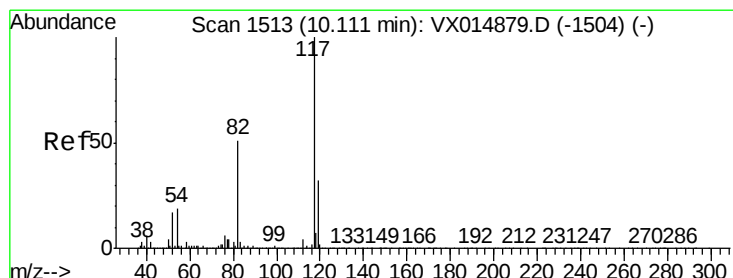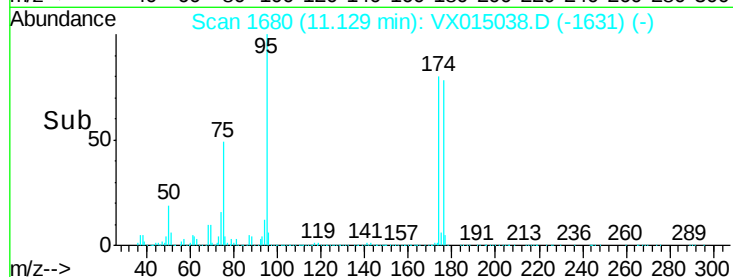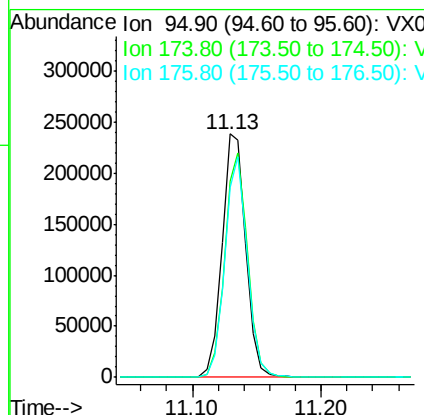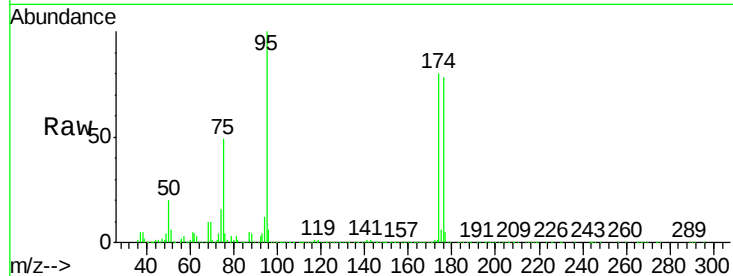

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.11 min Scan# 1513
Delta R.T. -0.00 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28

Tgt Ion: 117 Resp: 672999
Ion Ratio Lower Upper
117 100
82 51.0 40.5 60.7
119 31.5 25.8 38.6

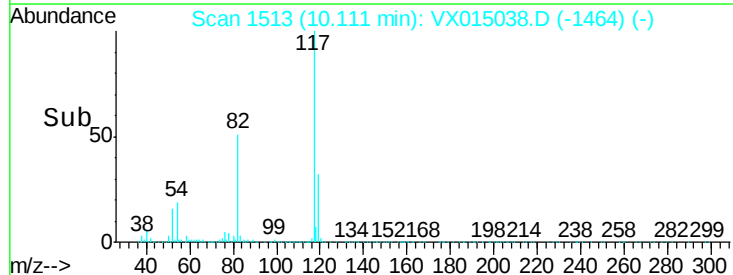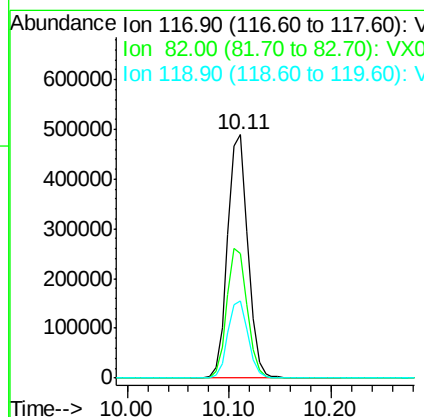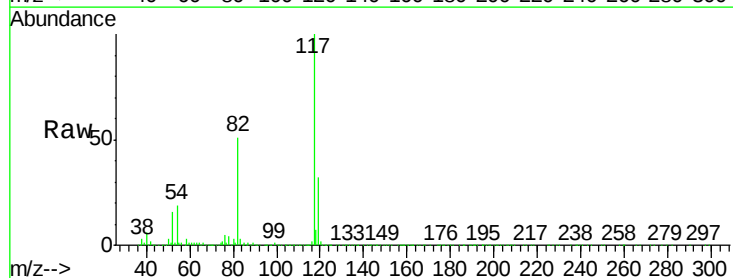

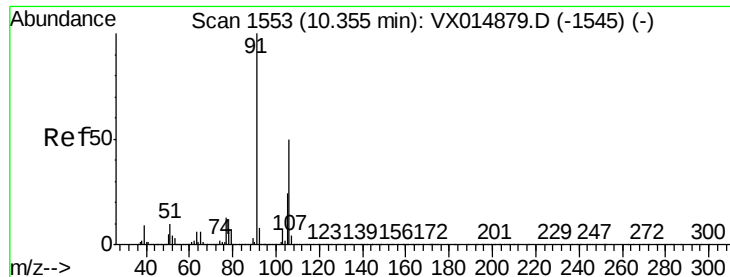

#68

m/p-Xylenes

Concen: 0.23 ug/l

RT: 10.35 min Scan# 1553

Delta R.T. -0.00 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28

Instrument :

MSVOA_X

ClientSampleId :


VOC-TRIP-BLANK

Tgt Ion:106 Resp: 2018

Ion Ratio Lower Upper




106 100

91 131.2 160.6 240.8#

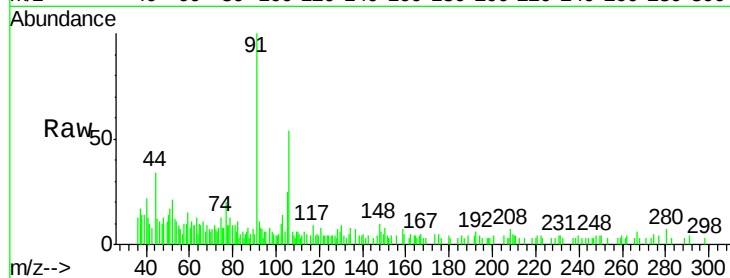

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VX0

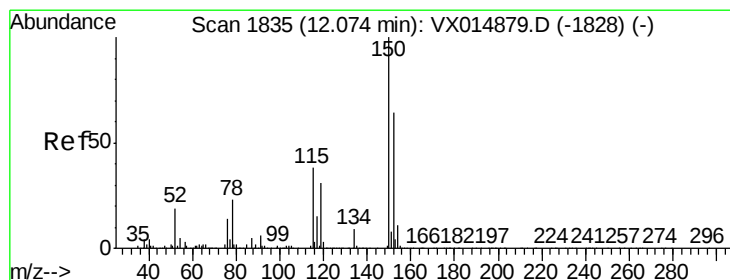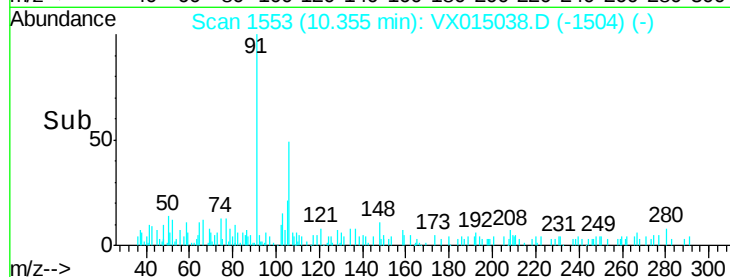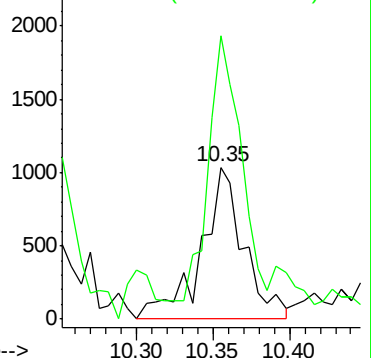

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.07 min Scan# 1835

Delta R.T. -0.00 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28


Tgt Ion:152 Resp: 332819

Ion Ratio Lower Upper

152 100

115 53.6 38.6 116.0



150 153.5 0.0 349.0

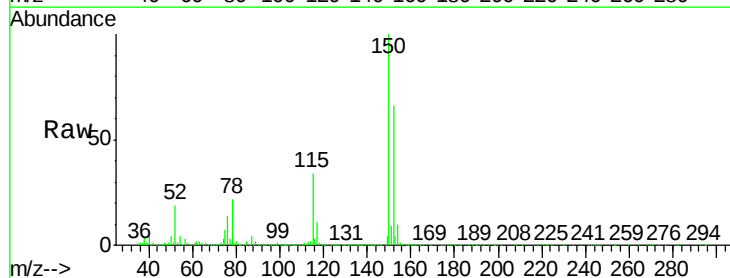


Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

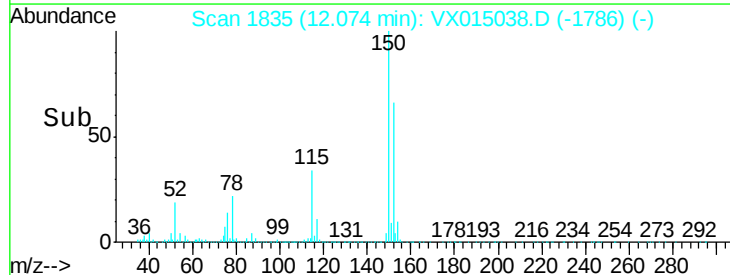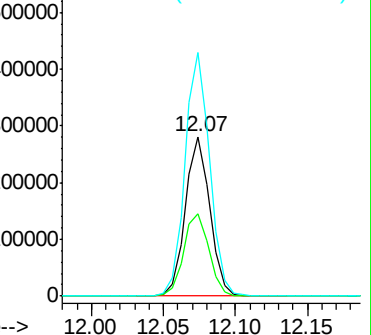



#76

1,2,3-Trichloropropane

Concen: 24.59 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.16 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28

Instrument :

MSVOA_X

ClientSampleId :


VOC-TRIP-BLANK

Tgt Ion: 75 Resp: 147997

Ion Ratio Lower Upper




75 100

77 1.5 18.4 55.0#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

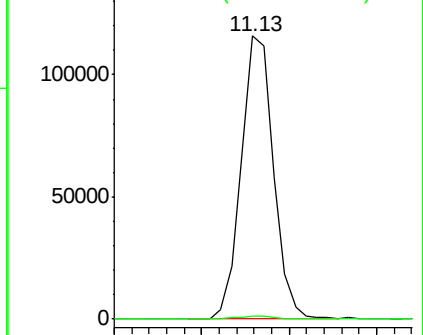

#81

trans-1,4-Dichloro-2-butene

Concen: 62.94 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. 0.06 min

Lab File: VX015038.D

Acq: 27 Feb 2020 11:28


Tgt Ion: 75 Resp: 147997

Ion Ratio Lower Upper

75 100

53 0.3 76.2 114.2#



89 0.1 35.8 53.6#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0




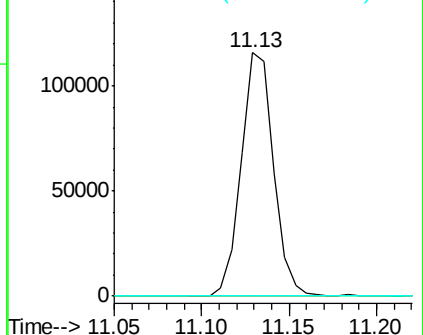




#87
 1,3-Dichlorobenzene
 Concen: 0.25 ug/l
 RT: 12.02 min Scan# 1826
 Delta R.T. -0.00 min
 Lab File: VX015038.D
 Acq: 27 Feb 2020 11:28




Instrument :
 MSVOA_X
 ClientSampleId :
 VOC-TRIP-BLANK


Tgt Ion:146 Resp: 2575
 Ion Ratio Lower Upper
 146 100
 111 38.5 18.6 56.0
 148 74.9 31.8 95.4

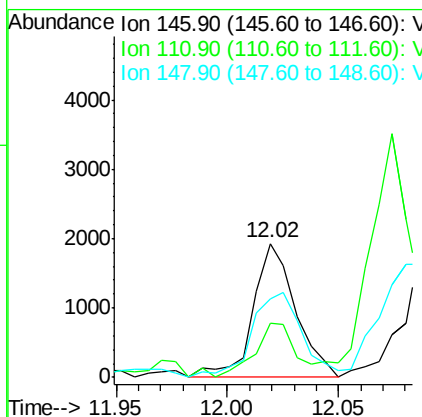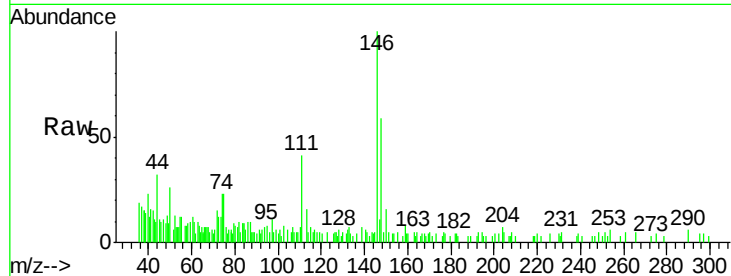

#88
 1,4-Dichlorobenzene
 Concen: 0.24 ug/l
 RT: 12.02 min Scan# 1826
 Delta R.T. -0.07 min
 Lab File: VX015038.D
 Acq: 27 Feb 2020 11:28

Tgt Ion:146 Resp: 2575
 Ion Ratio Lower Upper
 146 100
 111 38.5 18.6 55.6
 148 74.9 32.4 97.0


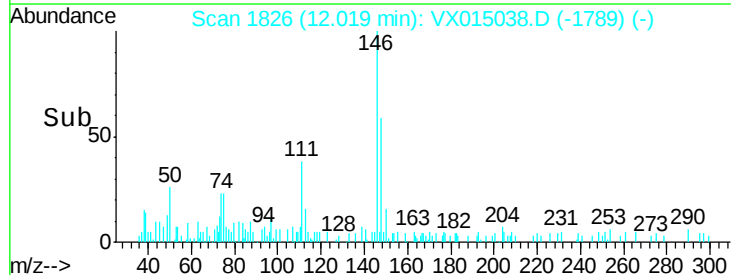
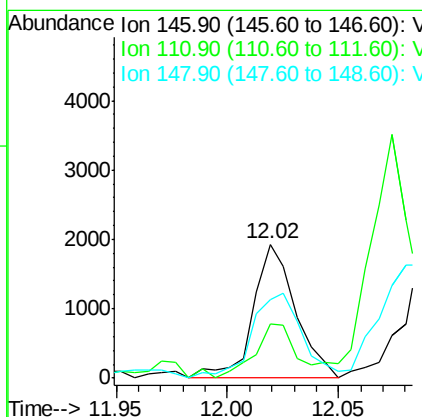



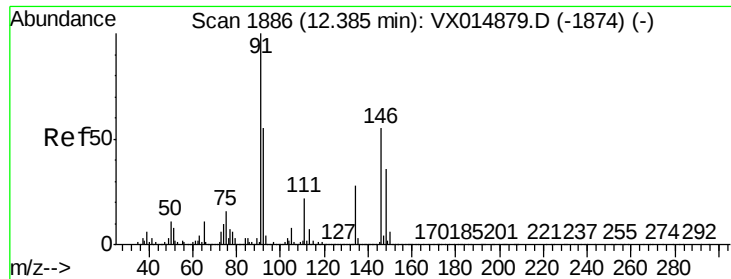

#89
n-Butylbenzene
Concen: 0.30 ug/l
RT: 12.39 min Scan# 1886
Delta R.T. -0.00 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28




Instrument :
MSVOA_X
ClientSampleId :
VOC-TRIP-BLANK


Tgt Ion: 91 Resp: 5142
Ion Ratio Lower Upper
91 100
92 51.5 27.3 81.8
134 33.1 13.8 41.4

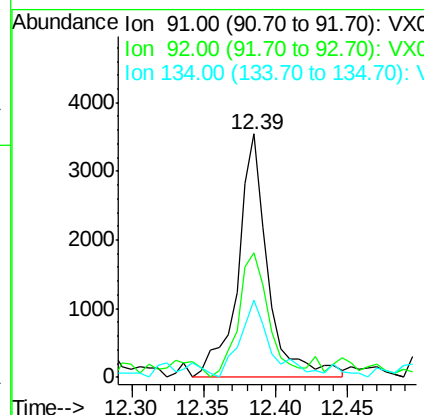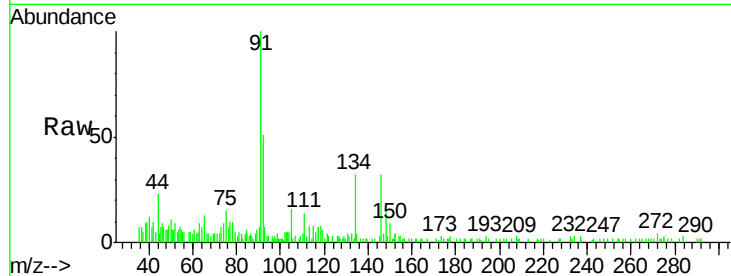

#91
1,2-Dichlorobenzene
Concen: 0.21 ug/l
RT: 12.39 min Scan# 1887
Delta R.T. 0.01 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28

Tgt Ion: 146 Resp: 2178
Ion Ratio Lower Upper
146 100
111 44.1 19.8 59.3
148 63.4 32.4 97.2


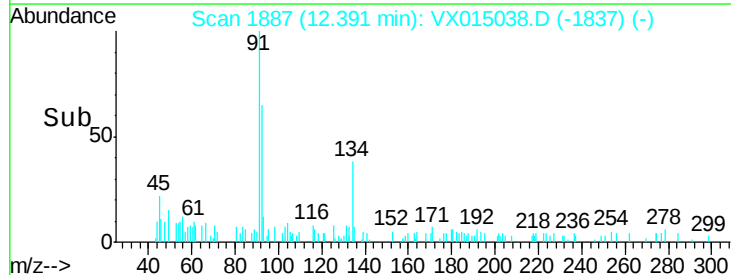
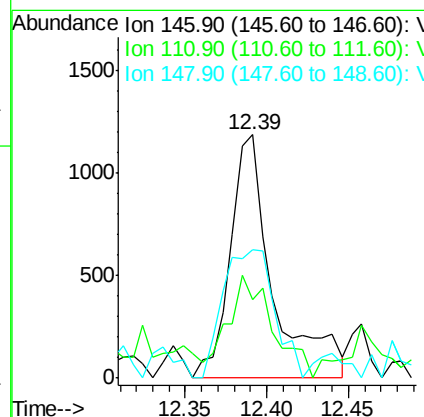





#93
 1,2,4-Trichlorobenzene
 Concen: 0.43 ug/l
 RT: 13.64 min Scan# 2092
 Delta R.T. -0.00 min
 Lab File: VX015038.D
 Acq: 27 Feb 2020 11:28




Instrument :
 MSVOA_X
 ClientSampleId :
 VOC-TRIP-BLANK


Tgt Ion:180 Resp: 3219
 Ion Ratio Lower Upper
 180 100
 182 100.2 48.4 145.3
 145 33.3 14.1 42.4

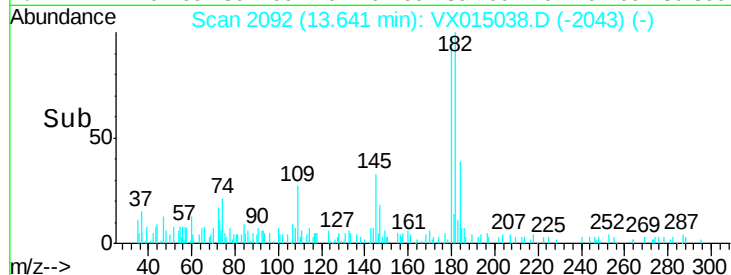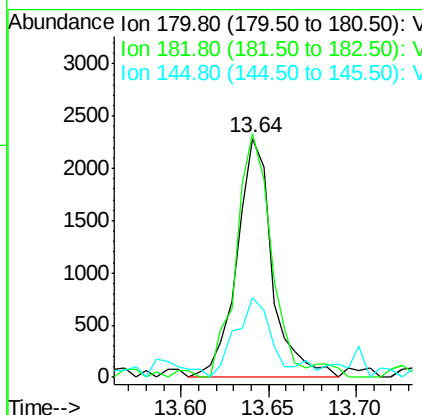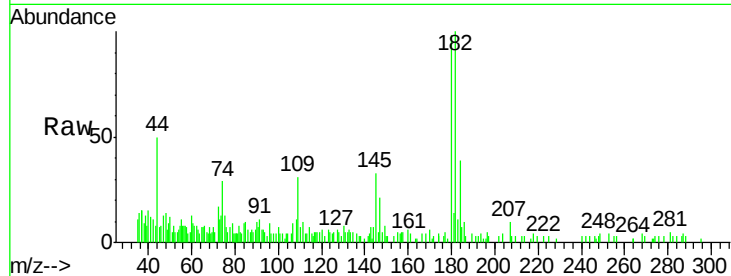

#94
 Hexachlorobutadiene
 Concen: 0.45 ug/l
 RT: 13.78 min Scan# 2114
 Delta R.T. -0.00 min
 Lab File: VX015038.D
 Acq: 27 Feb 2020 11:28

Tgt Ion:225 Resp: 1663
 Ion Ratio Lower Upper
 225 100
 223 73.2 31.1 93.2
 227 69.6 30.9 92.5


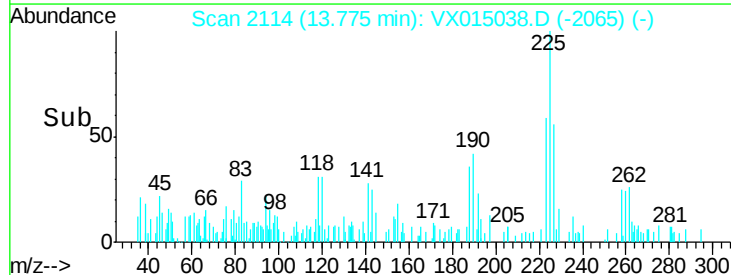
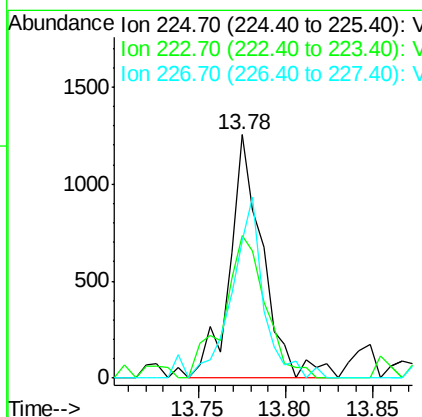



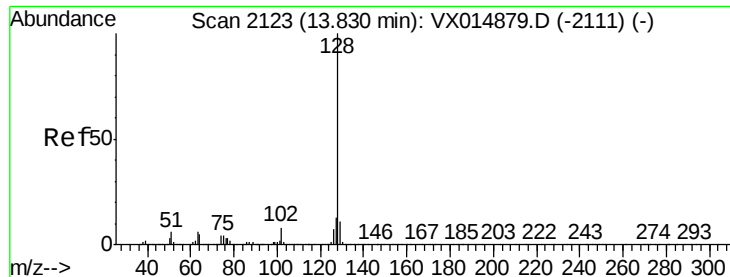

#95
Naphthalene
Concen: 0.33 ug/l
RT: 13.83 min Scan# 2123
Delta R.T. -0.00 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28

Instrument :
MSVOA_X
ClientSampleId :
VOC-TRIP-BLANK

Tgt Ion	Ratio	Lower	Upper
128	100		
127	16.6	10.4	15.6#
129	16.9	8.6	13.0#

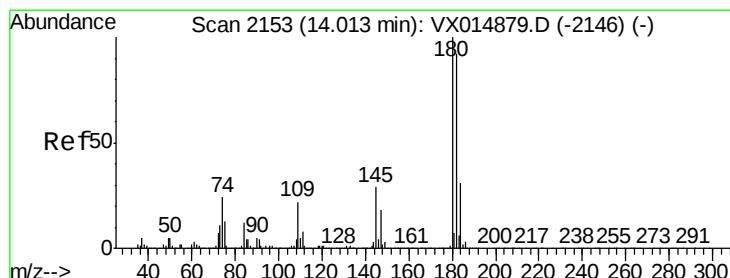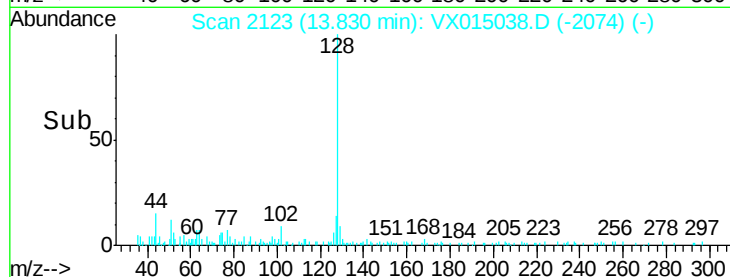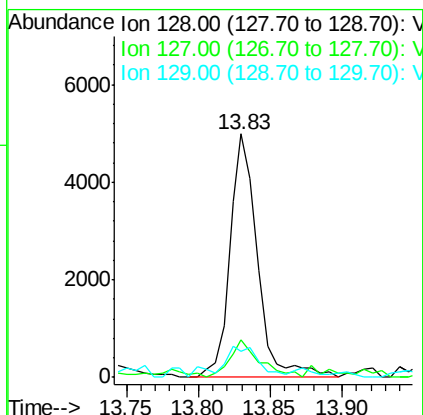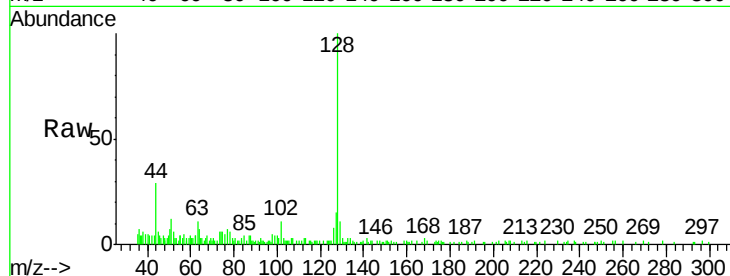

#96
1,2,3-Trichlorobenzene
Concen: 0.40 ug/l
RT: 14.02 min Scan# 2154
Delta R.T. 0.01 min
Lab File: VX015038.D
Acq: 27 Feb 2020 11:28

Tgt Ion	Ratio	Lower	Upper
180	100		
182	102.6	47.5	142.6
145	40.4	14.5	43.5

