

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022822\
 Data File : VX027223.D
 Acq On : 28 Feb 2022 16:25
 Operator : JC/MD
 Sample : N1688-08 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Mar 01 00:44:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 23 13:06:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	95203	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	156647	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	145304	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	70697	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	58139	50.848	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 101.700%	
35) Dibromofluoromethane	5.391	113	49923	51.343	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.680%	
50) Toluene-d8	8.653	98	184037	50.620	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 101.240%	
62) 4-Bromofluorobenzene	11.079	95	72364	51.853	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 103.700%	
Target Compounds						
					Qvalue	
5) Bromomethane	1.612	94	130	Below Cal	#	75
11) Tert butyl alcohol	2.959	59	393	1.767	ug/l #	75
13) Acrolein	2.221	56	386	1.877	ug/l #	1
14) Allyl chloride	2.758	41	754	0.462	ug/l #	34
15) Acrylonitrile	3.111	53	150	0.263	ug/l #	9
16) Acetone	2.386	43	646	1.287	ug/l	95
19) Methyl tert-butyl Ether	3.117	73	15515	4.878	ug/l	95
31) Cyclohexane	5.483	56	3969	2.318	ug/l	94
36) 1,1-Dichloropropene	5.556	75	7036	4.958	ug/l #	50
38) Carbon Tetrachloride	5.556	117	9535	6.442	ug/l #	17
39) Methylcyclohexane	7.379	83	817	0.463	ug/l #	79
40) Benzene	6.044	78	57764	13.920	ug/l	99
41) Methacrylonitrile	5.196	41	627	0.734	ug/l #	1
51) 4-Methyl-2-Pentanone	8.647	43	786	0.505	ug/l #	1
52) Toluene	8.720	92	106766	40.179	ug/l	100
53) t-1,3-Dichloropropene	8.720	75	1140	3.638	ug/l #	1
67) Ethyl Benzene	10.195	91	191006	36.734	ug/l	98
68) m/p-Xylenes	10.305	106	108723	54.390	ug/l	96
69) o-Xylene	10.640	106	76606	38.184	ug/l	97
70) Styrene	10.640	104	3984	1.214	ug/l #	1
73) Isopropylbenzene	10.964	105	6338	1.253	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	34637	24.324	ug/l #	40
78) n-propylbenzene	11.305	91	16375	2.848	ug/l	99
79) 2-Chlorotoluene	11.378	91	7663	2.175	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	18498	4.349	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	34637	69.024	ug/l #	3
82) 4-Chlorotoluene	11.451	91	2041	0.507	ug/l #	46
83) tert-Butylbenzene	11.756	119	16360	3.955	ug/l #	62
84) 1,2,4-Trimethylbenzene	11.756	105	136696	32.307	ug/l	97
85) sec-Butylbenzene	11.756	105	136696	26.357	ug/l #	56
89) n-Butylbenzene	12.323	91	2214	0.599	ug/l #	23
90) Hexachloroethane	12.646	117	3392	4.953	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	12.963	75	93	0.268	ug/l #	3
95) Naphthalene	13.780	128	88957	17.907	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022822\
Data File : VX027223.D
Acq On : 28 Feb 2022 16:25
Operator : JC/MD
Sample : N1688-08 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Mar 01 00:44:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 23 13:06:57 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022822\
Data File : VX027223.D
Acq On : 28 Feb 2022 16:25
Operator : JC/MD
Sample : N1688-08 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Mar 01 00:44:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 23 13:06:57 2022
Response via : Initial Calibration

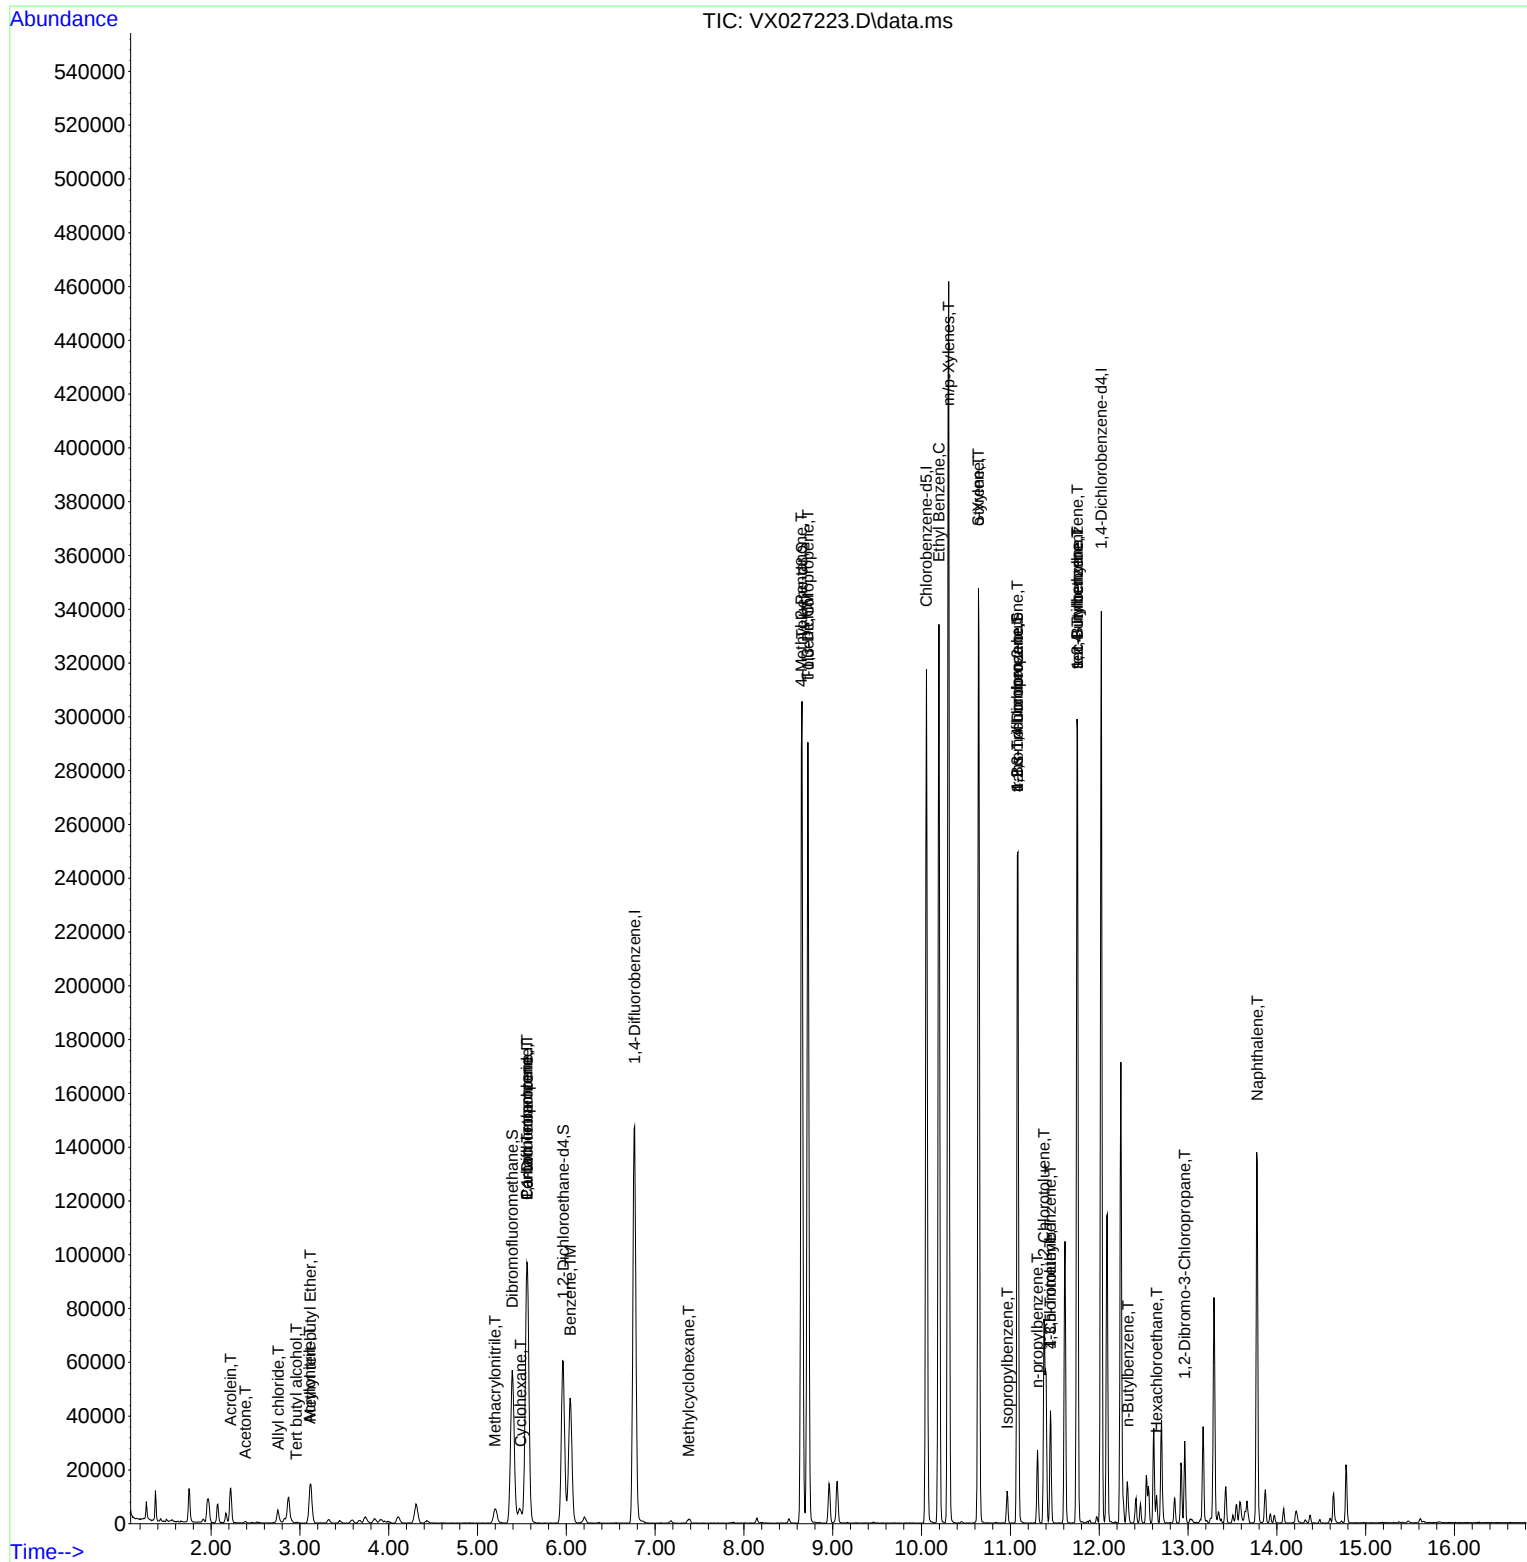






#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.556 min Scan# 71
 Delta R.T. -0.006 min
 Lab File: VX027223.D
 Acq: 28 Feb 2022 16:25

Instrument :
 MSVOA_X
 ClientSampleId :







Tgt Ion:168 Resp: 95203
 Ion Ratio Lower Upper
 168 100
 99 58.2 50.3 75.5

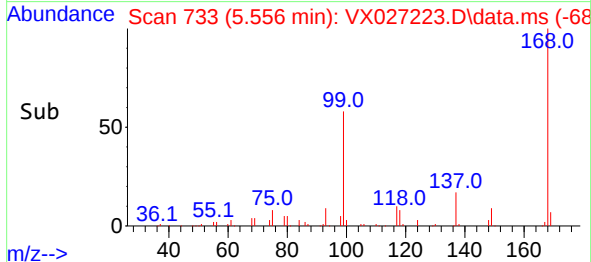

#5
 Bromomethane
 Concen: Below Cal
 RT: 1.612 min Scan# 86
 Delta R.T. 0.013 min
 Lab File: VX027223.D
 Acq: 28 Feb 2022 16:25

Tgt Ion: 94 Resp: 130
 Ion Ratio Lower Upper
 94 100
 96 71.1 75.9 113.9#

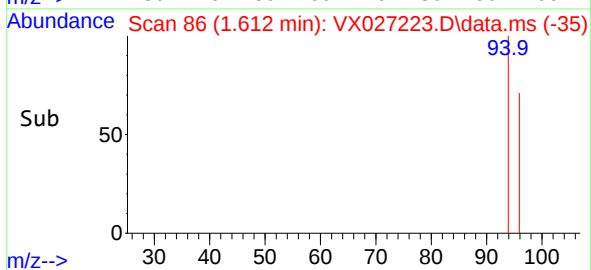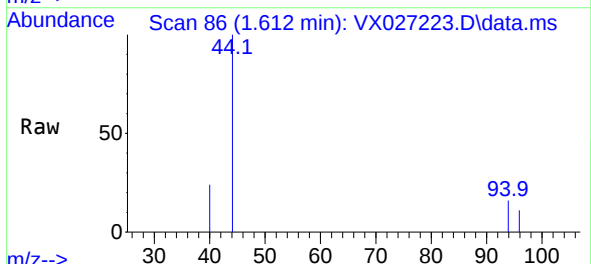



#11

Tert butyl alcohol

Concen: 1.767 ug/l

RT: 2.959 min Scan# 30

Delta R.T. -0.018 min

Lab File: VX027223.D

Acq: 28 Feb 2022 16:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 59 Resp: 393

Ion Ratio Lower Upper

59 100

57 0.0 7.2 10.8#

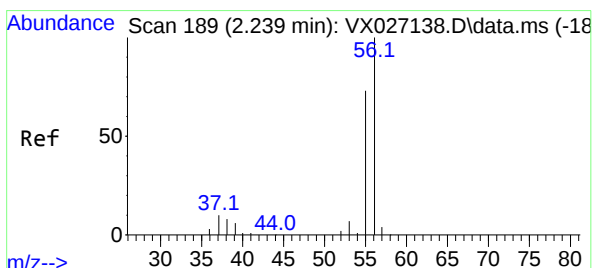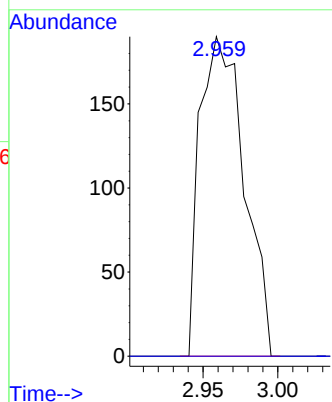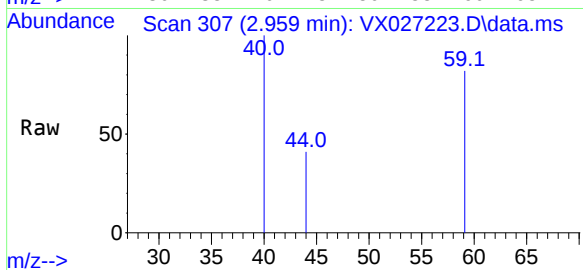

#13

Acrolein

Concen: 1.877 ug/l

RT: 2.221 min Scan# 186

Delta R.T. -0.018 min

Lab File: VX027223.D




Acq: 28 Feb 2022 16:25


Tgt Ion: 56 Resp: 386

Ion Ratio Lower Upper

56 100


55 1891.2 56.9 85.3#

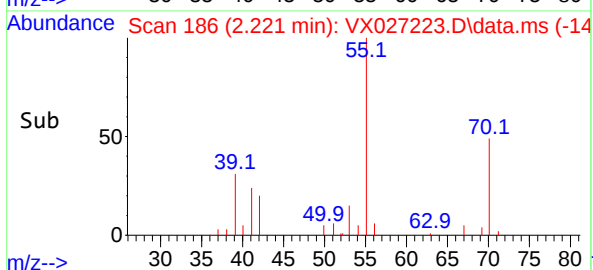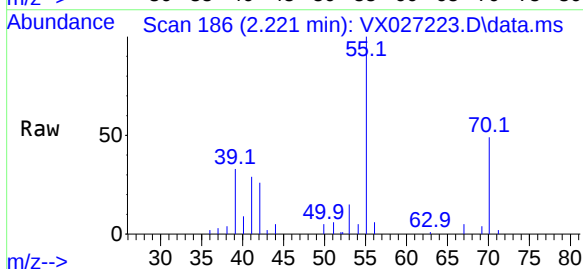






#14
 Allyl chloride
 Concen: 0.462 ug/l
 RT: 2.758 min Scan# 21
 Delta R.T. 0.092 min
 Lab File: VX027223.D
 Acq: 28 Feb 2022 16:25

Instrument :
 MSVOA_X
 ClientSampleId :



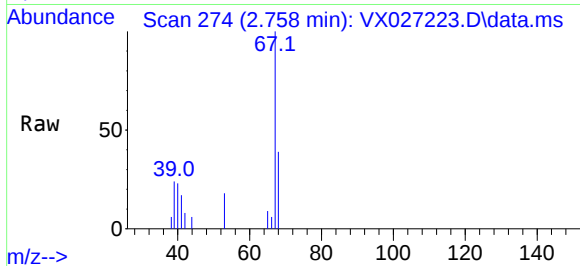



Tgt Ion: 41 Resp: 754
 Ion Ratio Lower Upper
 41 100
 39 124.5 54.2 81.4#
 76 0.0 25.2 37.8#

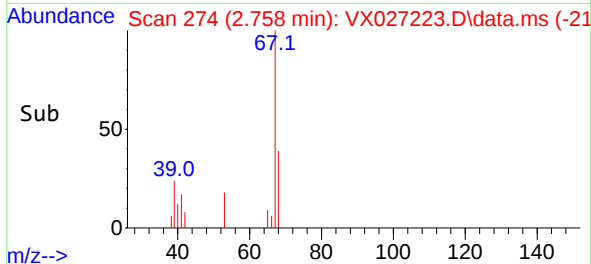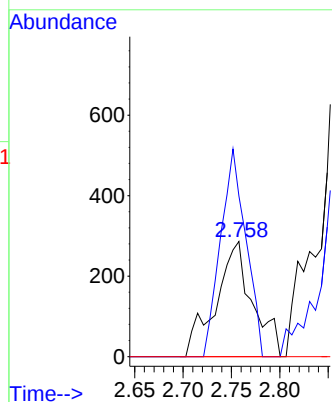

#15
 Acrylonitrile
 Concen: 0.263 ug/l
 RT: 3.111 min Scan# 332
 Delta R.T. 0.043 min
 Lab File: VX027223.D
 Acq: 28 Feb 2022 16:25

Tgt Ion: 53 Resp: 150
 Ion Ratio Lower Upper
 53 100
 52 0.0 66.6 100.0#
 51 89.3 29.5 44.3#


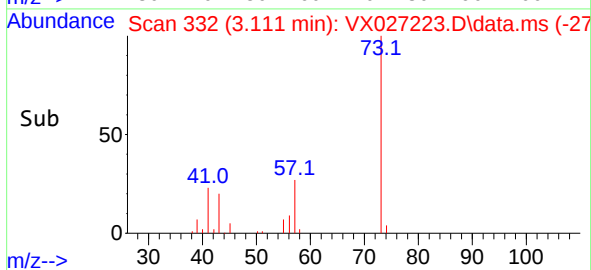

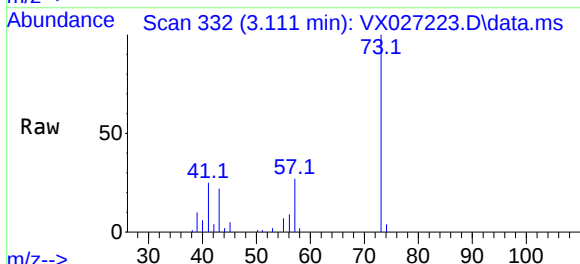




#16
Acetone
Concen: 1.287 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 646
Ion Ratio Lower Upper
43 100
58 26.2 23.0 34.6

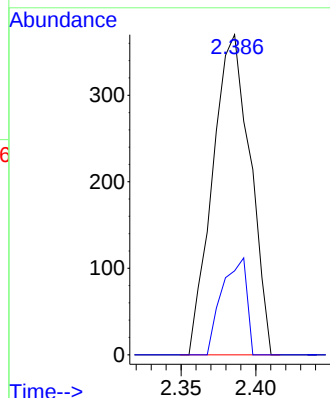

#19
Methyl tert-butyl Ether
Concen: 4.878 ug/l
RT: 3.117 min Scan# 333
Delta R.T. 0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25


Tgt Ion: 73 Resp: 15515
Ion Ratio Lower Upper
73 100
57 24.2 17.4 26.2

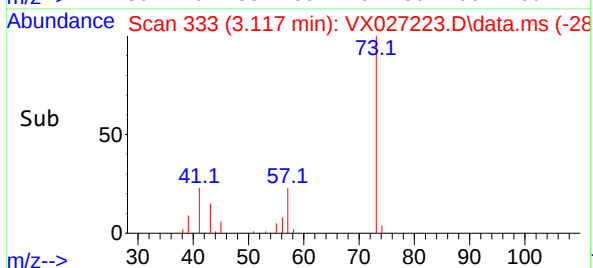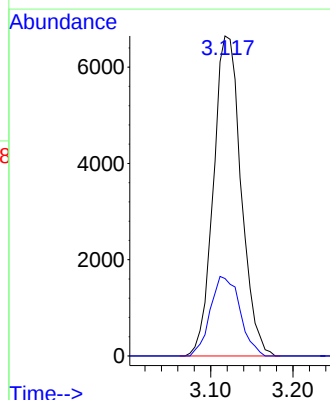






#31
Cyclohexane
Concen: 2.318 ug/l
RT: 5.483 min Scan# 720
Delta R.T. 0.007 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Instrument :
MSVOA_X
ClientSampleId :



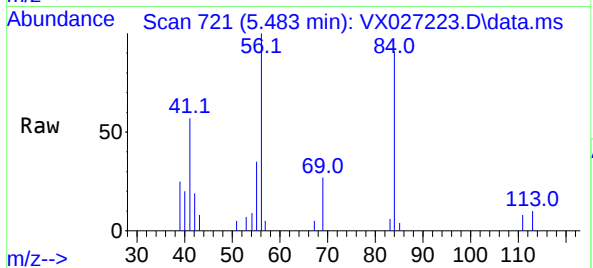



Tgt Ion: 56 Resp: 3969
Ion Ratio Lower Upper
56 100
69 27.3 25.8 38.6
84 90.8 68.9 103.3



#33
1,2-Dichloroethane-d4
Concen: 50.848 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25


Tgt Ion: 65 Resp: 58139
Ion Ratio Lower Upper
65 100
67 51.4 0.0 100.8

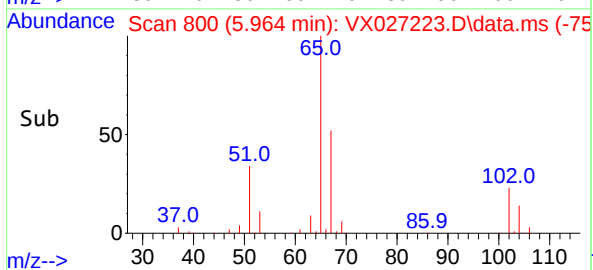






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:114 Resp: 156647
Ion Ratio Lower Upper
114 100
63 19.4 0.0 42.8
88 16.5 0.0 33.0

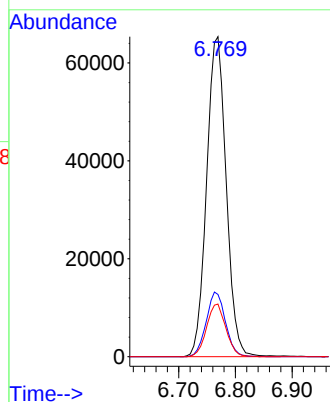

#35
Dibromofluoromethane
Concen: 51.343 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25


Tgt Ion:113 Resp: 49923
Ion Ratio Lower Upper
113 100
111 102.1 81.2 121.8
192 20.3 15.0 22.4

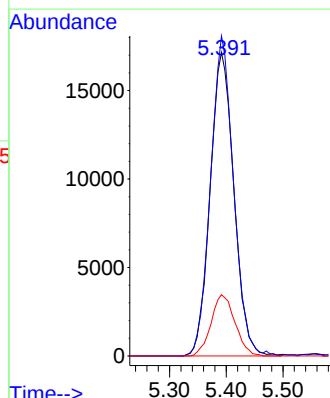






#36
1,1-Dichloropropene
Concen: 4.958 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.140 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25


Instrument :
MSVOA_X
ClientSampleId :

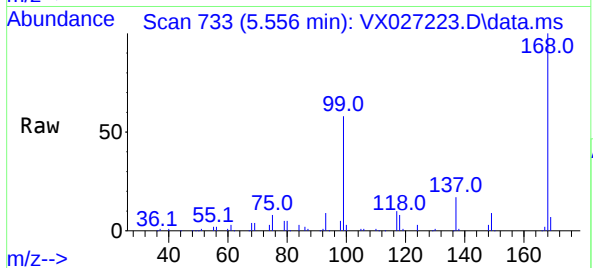



Tgt Ion: 75 Resp: 7036
Ion Ratio Lower Upper
75 100
110 8.6 17.2 51.6#
77 0.0 24.6 36.8#

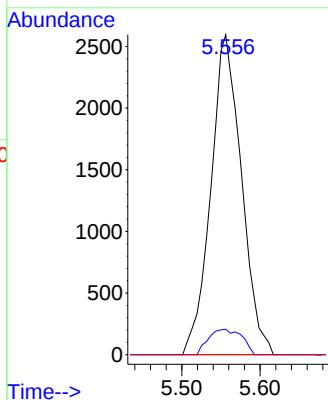


#38
Carbon Tetrachloride
Concen: 6.442 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.128 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

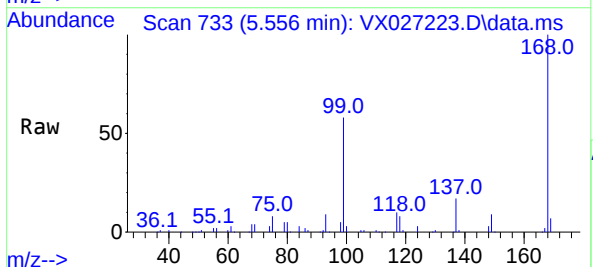

Tgt Ion: 117 Resp: 9535
Ion Ratio Lower Upper
117 100
119 5.5 74.7 112.1#
121 0.0 25.4 38.0#

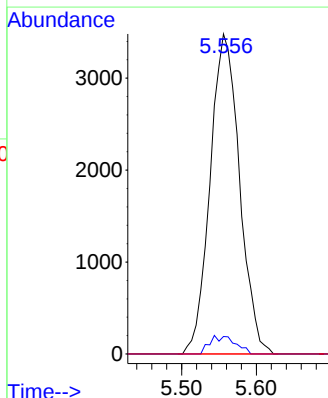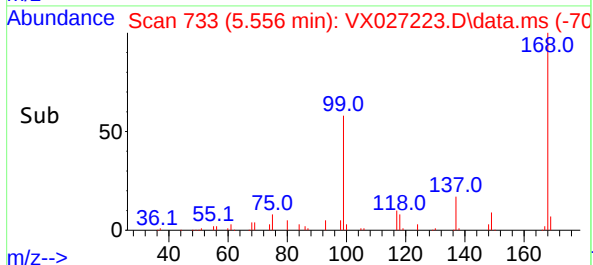



#39

Methylcyclohexane

Concen: 0.463 ug/l

RT: 7.379 min Scan# 10

Delta R.T. -0.006 min

Lab File: VX027223.D

Acq: 28 Feb 2022 16:25

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 83 Resp: 817

Ion Ratio Lower Upper

83 100

55 101.7 63.6 95.4#

98 38.6 38.4 57.6

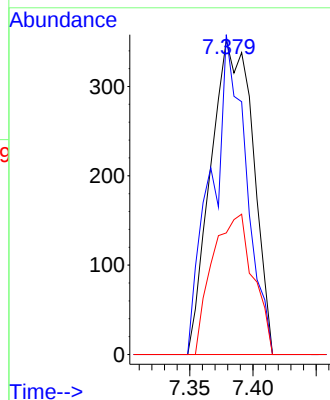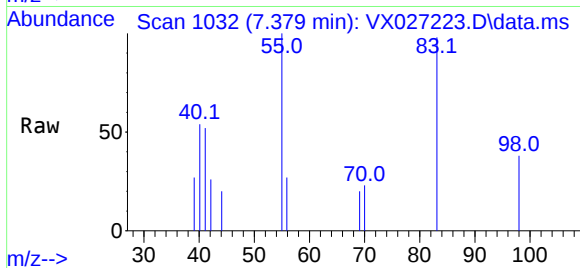

#40

Benzene

Concen: 13.920 ug/l

RT: 6.044 min Scan# 813

Delta R.T. 0.001 min

Lab File: VX027223.D




Acq: 28 Feb 2022 16:25


Tgt Ion: 78 Resp: 57764

Ion Ratio Lower Upper

78 100


77 24.0 18.9 28.3

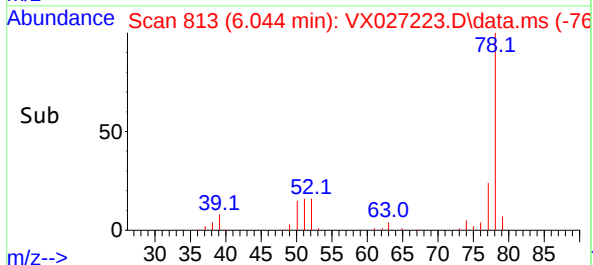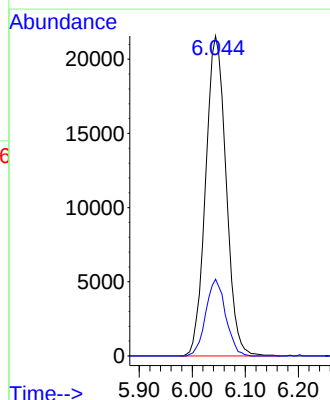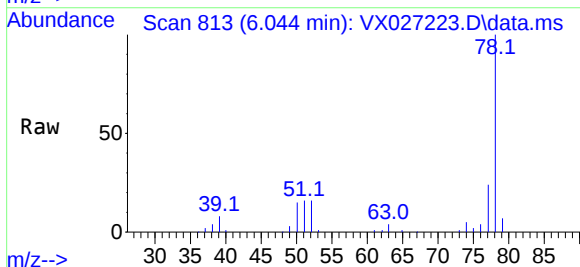






#41
Methacrylonitrile
Concen: 0.734 ug/l
RT: 5.196 min Scan# 61
Delta R.T. 0.268 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Instrument :
MSVOA_X
ClientSampleId :



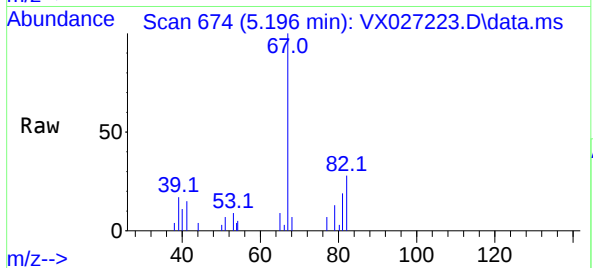



Tgt Ion: 41 Resp: 627
Ion Ratio Lower Upper
41 100
39 85.0 45.4 68.0#
67 595.9 53.2 79.8#
52 6.7 23.0 34.6#



#50
Toluene-d8
Concen: 50.620 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Tgt Ion: 98 Resp: 184037
Ion Ratio Lower Upper
98 100
100 67.1 53.2 79.8

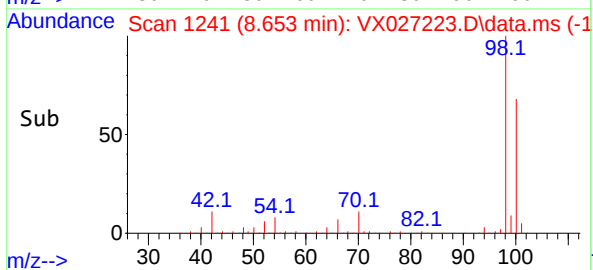



#51

4-Methyl-2-Pentanone

Concen: 0.505 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.067 min

Lab File: VX027223.D

Acq: 28 Feb 2022 16:25

Instrument :

MSVOA_X


ClientSampleId :

Tgt Ion: 43 Resp: 786


Ion Ratio Lower Upper

43 100



58 190.5 30.5 45.7#

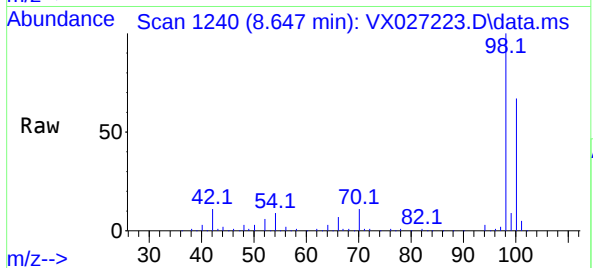

Abundance

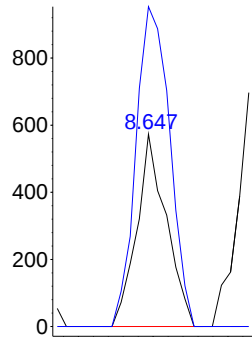

Time-->

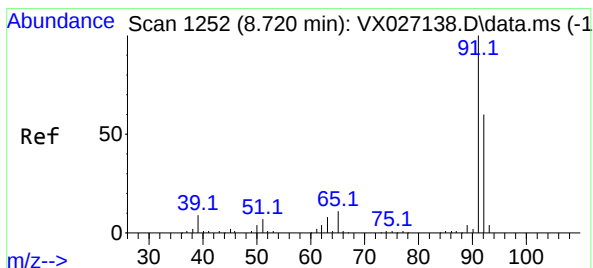

#52

Toluene

Concen: 40.179 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. 0.000 min

Lab File: VX027223.D


Acq: 28 Feb 2022 16:25

Tgt Ion: 92 Resp: 106766


Ion Ratio Lower Upper

92 100


91 169.1 135.7 203.5

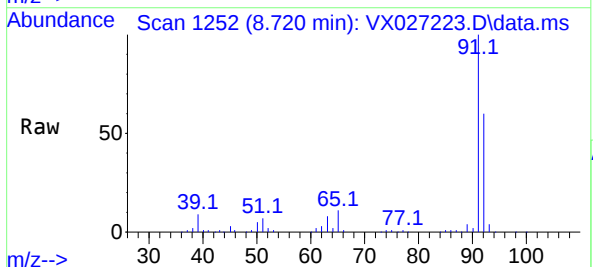


Abundance

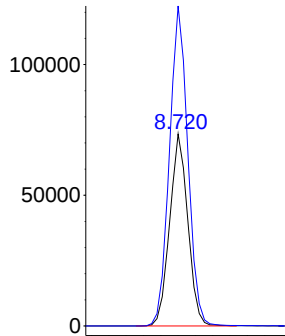

Time-->

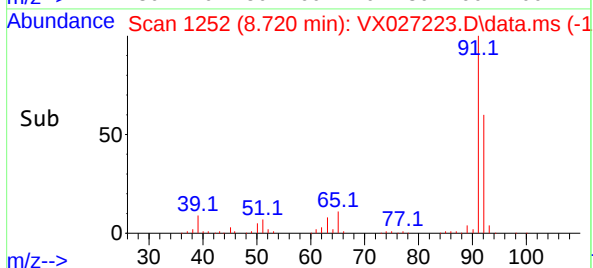



#53

t-1,3-Dichloropropene

Concen: 3.638 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.262 min

Lab File: VX027223.D

Acq: 28 Feb 2022 16:25

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 1140

Ion Ratio Lower Upper

75 100

77 180.7 25.7 38.5#

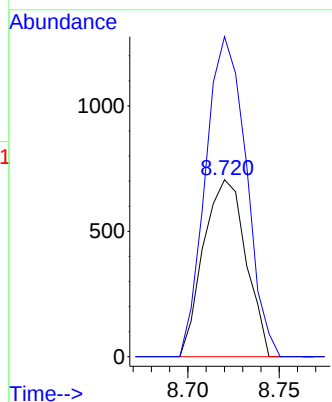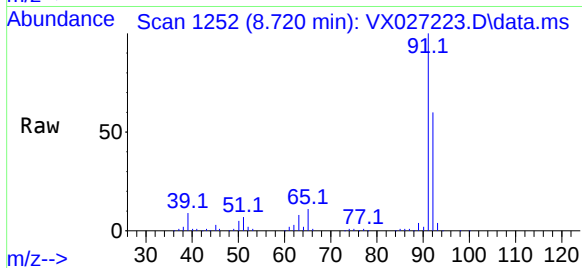

#62

4-Bromofluorobenzene

Concen: 51.853 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.006 min

Lab File: VX027223.D

Acq: 28 Feb 2022 16:25




Tgt Ion: 95 Resp: 72364


Ion Ratio Lower Upper

95 100

174 76.7 0.0 148.6


176 74.3 0.0 141.4

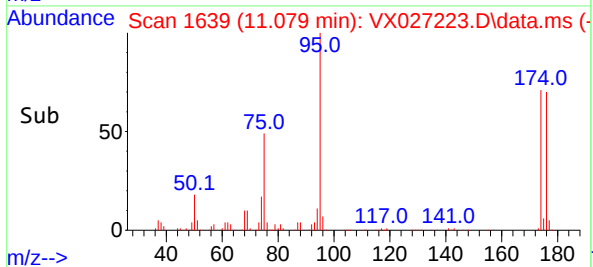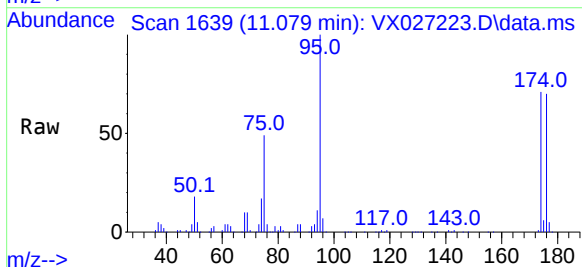






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 145304
Ion Ratio Lower Upper
117 100
82 54.3 45.2 67.8
119 32.2 26.2 39.2

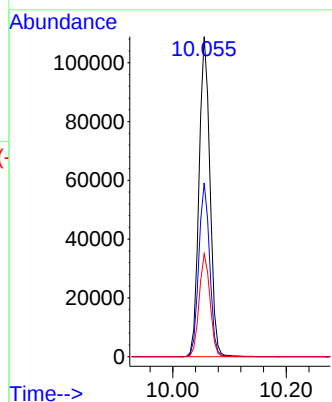

#67
Ethyl Benzene
Concen: 36.734 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Tgt Ion: 91 Resp: 191006
Ion Ratio Lower Upper
91 100
106 32.0 24.7 37.1




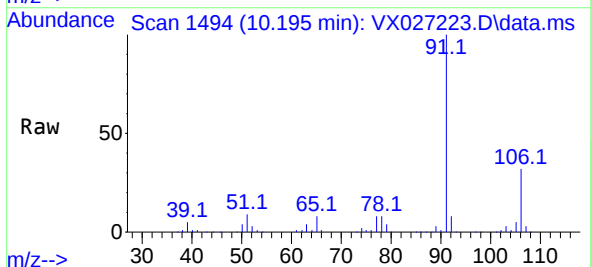




#68
m/p-Xylenes
Concen: 54.390 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 108723
Ion Ratio Lower Upper
106 100
91 201.1 165.3 247.9

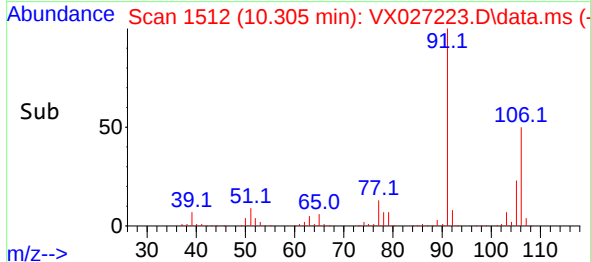

#69
o-Xylene
Concen: 38.184 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.006 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25


Tgt Ion:106 Resp: 76606
Ion Ratio Lower Upper
106 100
91 213.7 109.7 329.0

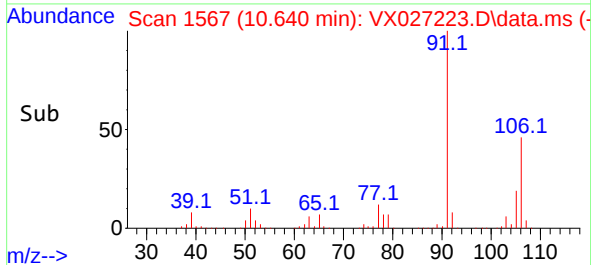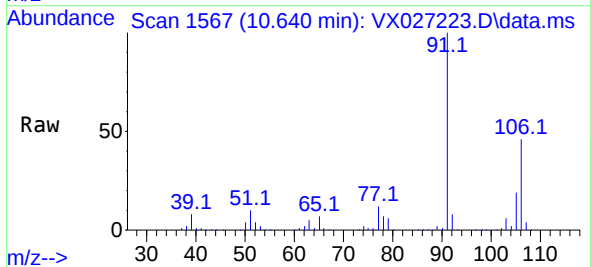






#70
Styrene
Concen: 1.214 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:104 Resp: 3984
Ion Ratio Lower Upper
104 100
78 288.1 42.5 63.7#
103 263.0 43.3 64.9#

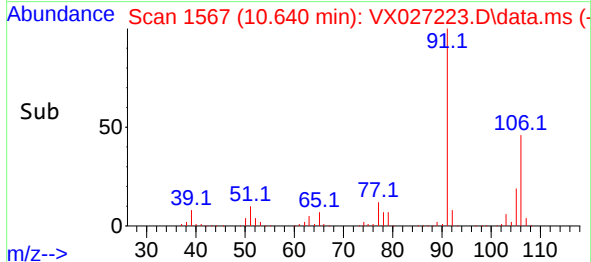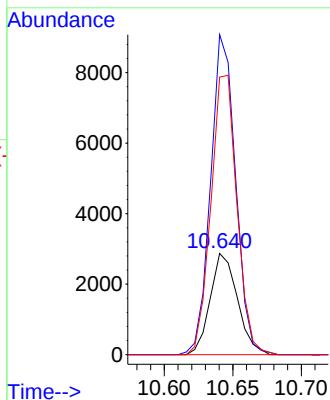

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25


Tgt Ion:152 Resp: 70697
Ion Ratio Lower Upper
152 100
115 59.8 44.2 132.6
150 155.7 0.0 348.2

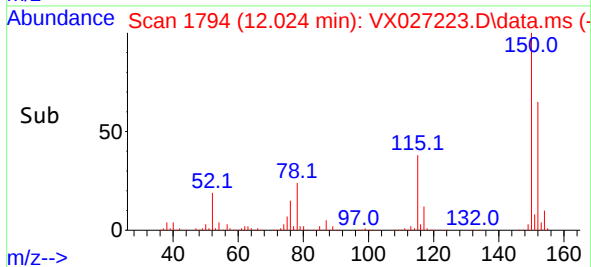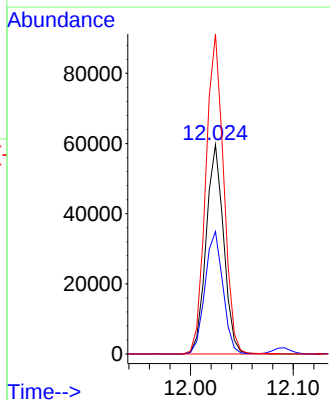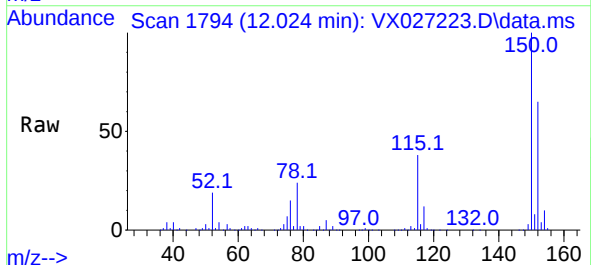






#73
Isopropylbenzene
Concen: 1.253 ug/l
RT: 10.964 min Scan# 1639
Delta R.T. 0.001 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Instrument :
MSVOA_X
ClientSampleId :



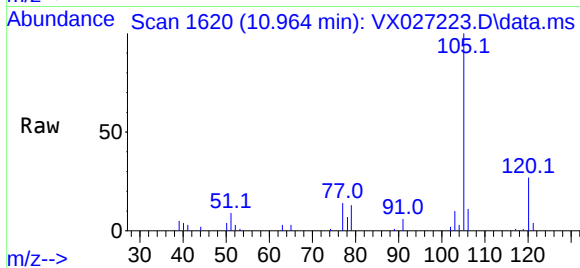



Tgt Ion:105 Resp: 6338
Ion Ratio Lower Upper
105 100
120 25.7 13.1 39.1

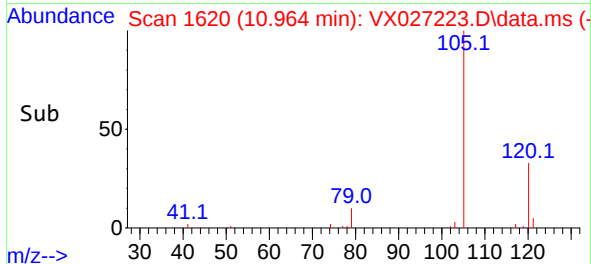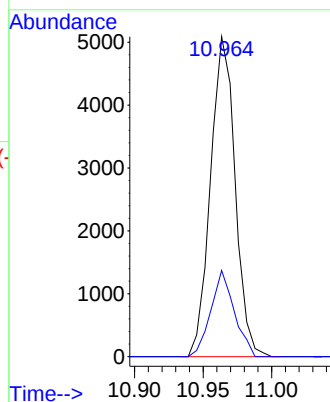

#76
1,2,3-Trichloropropane
Concen: 24.324 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Tgt Ion: 75 Resp: 34637
Ion Ratio Lower Upper
75 100
77 1.2 18.3 54.8#


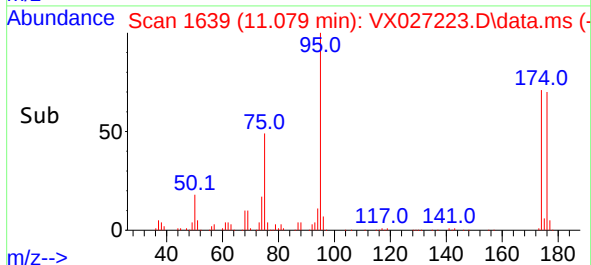
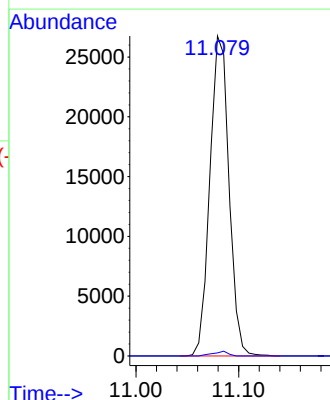
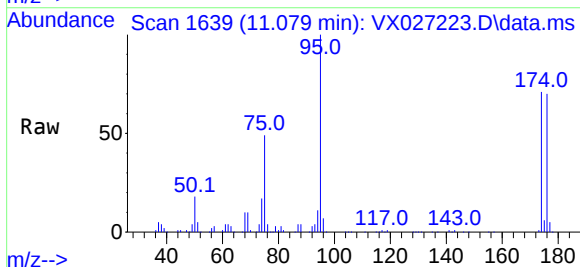




#78
n-propylbenzene
Concen: 2.848 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 16375
Ion Ratio Lower Upper
91 100
120 22.6 11.6 34.7

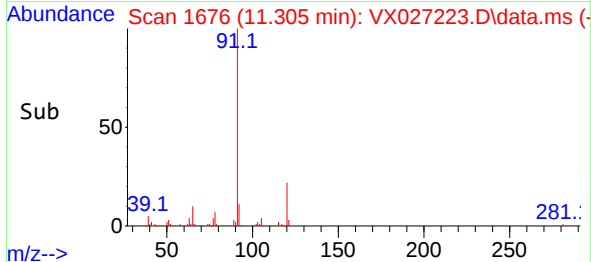

#79
2-Chlorotoluene
Concen: 2.175 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Tgt Ion: 91 Resp: 7663
Ion Ratio Lower Upper
91 100
126 0.0 16.4 49.2#


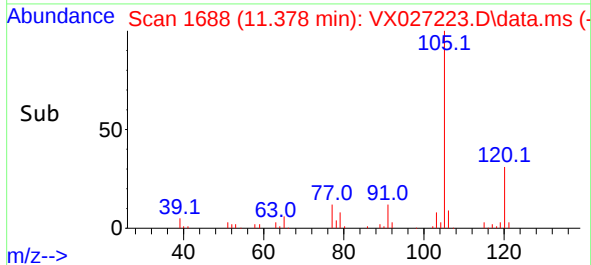

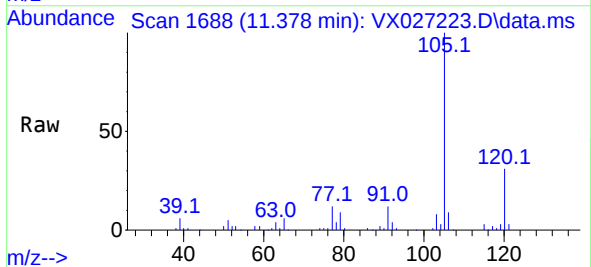




#80
1,3,5-Trimethylbenzene
Concen: 4.349 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 18498
Ion Ratio Lower Upper
105 100
120 49.2 24.0 72.0

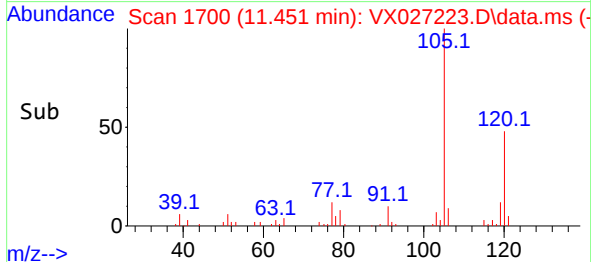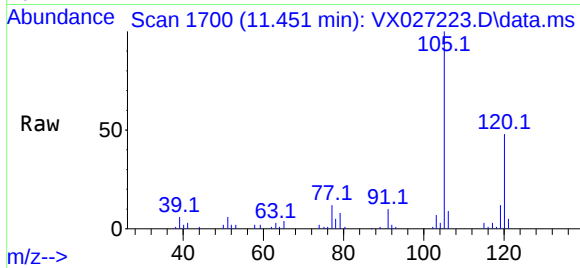

#81
trans-1,4-Dichloro-2-butene
Concen: 69.024 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.055 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25


Tgt Ion: 75 Resp: 34637
Ion Ratio Lower Upper
75 100
53 0.0 94.0 141.0#
89 0.0 37.0 55.4#

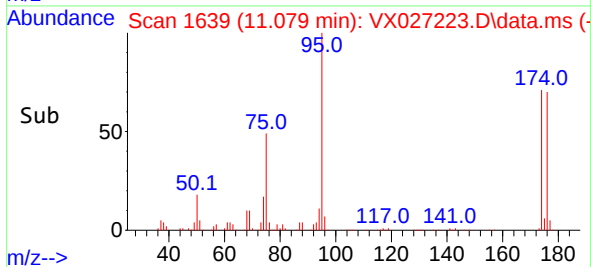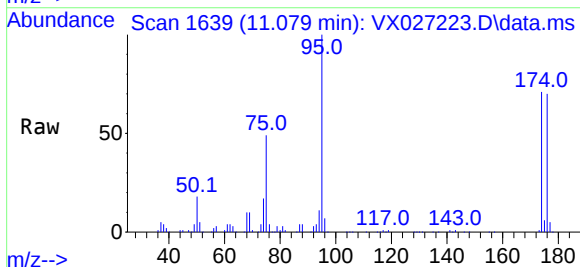






#82
4-Chlorotoluene
Concen: 0.507 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Instrument :
MSVOA_X
ClientSampleId :



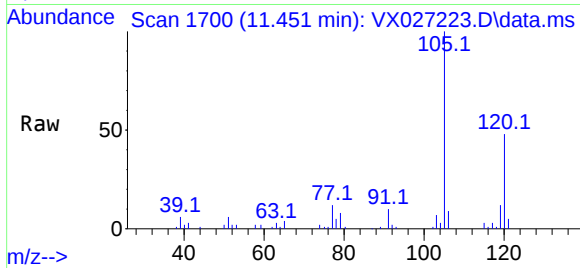



Tgt Ion: 91 Resp: 2041
Ion Ratio Lower Upper
91 100
126 0.0 14.1 42.4#

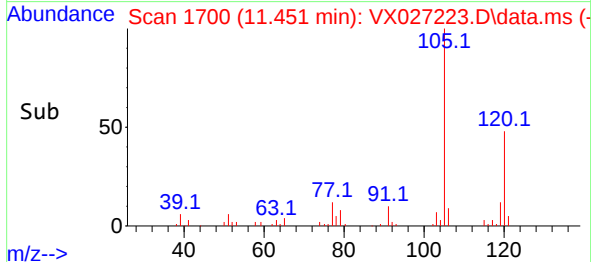

#83
tert-Butylbenzene
Concen: 3.955 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Tgt Ion: 119 Resp: 16360
Ion Ratio Lower Upper
119 100
91 89.0 31.4 94.0
134 0.0 11.8 35.3#


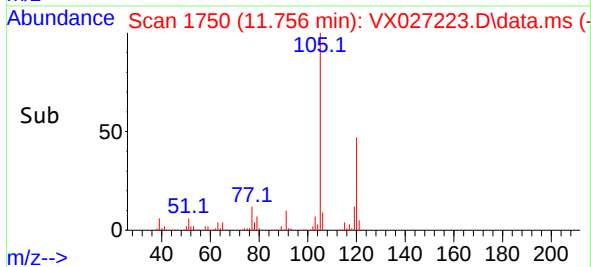

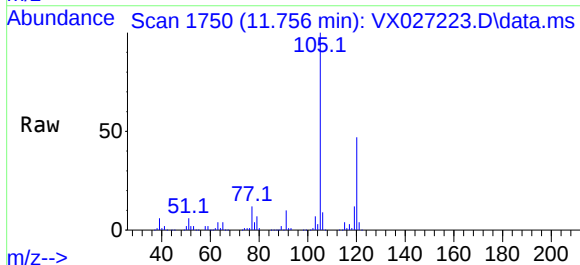




#84
1,2,4-Trimethylbenzene
Concen: 32.307 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 136696
Ion Ratio Lower Upper
105 100
120 45.8 21.9 65.5

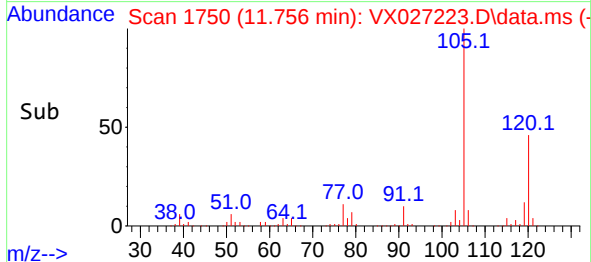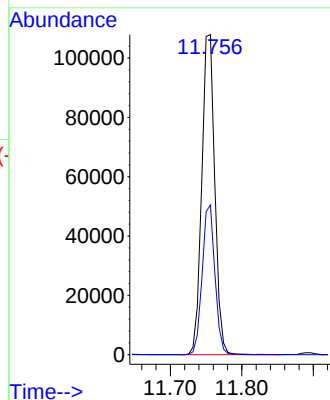

#85
sec-Butylbenzene
Concen: 26.357 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX027223.D
Acq: 28 Feb 2022 16:25

Tgt Ion:105 Resp: 136696
Ion Ratio Lower Upper
105 100
134 0.0 10.1 30.1#

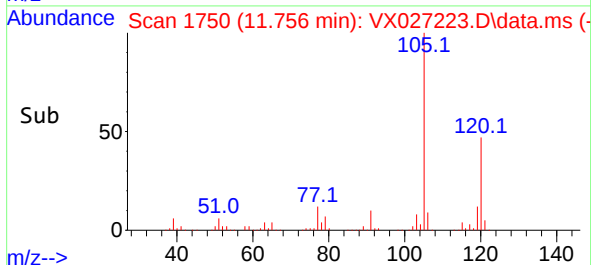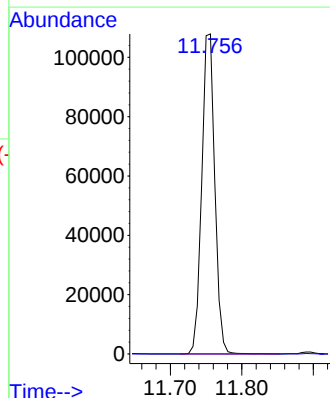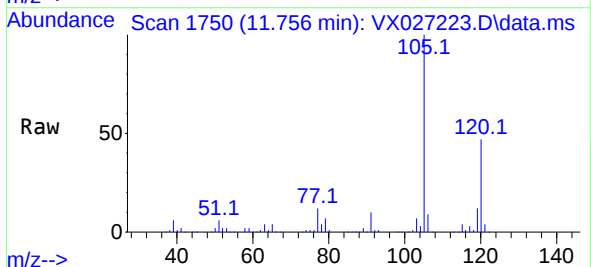

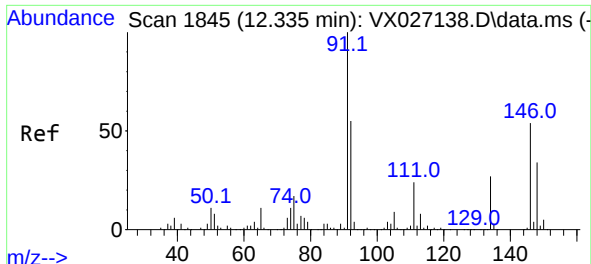

#89

n-Butylbenzene

Concen: 0.599 ug/l

RT: 12.323 min Scan# 1843

Delta R.T. -0.012 min

Lab File: VX027223.D

Acq: 28 Feb 2022 16:25

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 91 Resp: 2214

Ion Ratio Lower Upper

91 100

92 30.4 27.2 81.6

134 111.9 13.1 39.1#

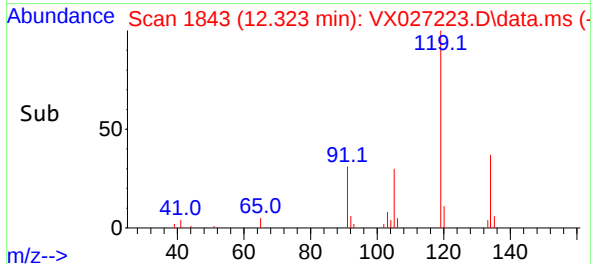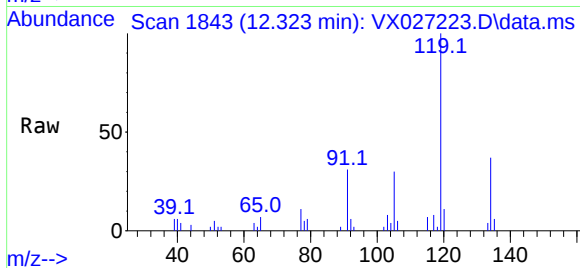

#90

Hexachloroethane

Concen: 4.953 ug/l

RT: 12.646 min Scan# 1896

Delta R.T. 0.104 min

Lab File: VX027223.D




Acq: 28 Feb 2022 16:25


Tgt Ion: 117 Resp: 3392

Ion Ratio Lower Upper

117 100

201 0.0 35.6 106.8#

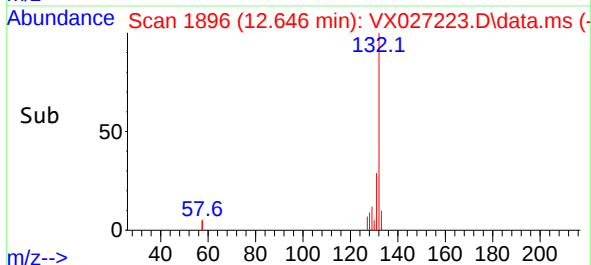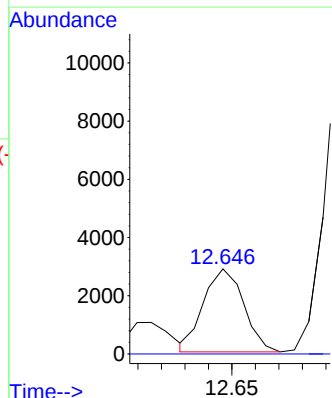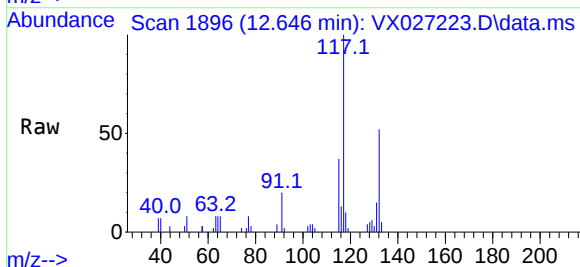



#92

1,2-Dibromo-3-Chloropropane

Concen: 0.268 ug/l

RT: 12.963 min Scan# 1948

Delta R.T. 0.018 min


Lab File: VX027223.D

Acq: 28 Feb 2022 16:25

Instrument :

MSVOA_X

ClientSampleId :

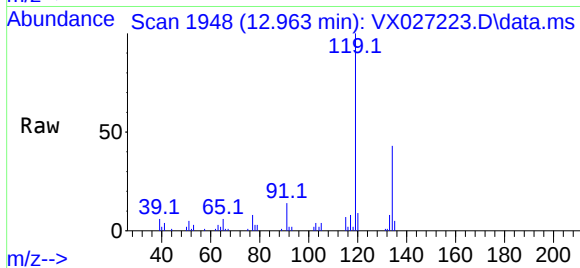




Tgt Ion: 75 Resp: 93

Ion Ratio Lower Upper

75 100

155 0.0 40.0 119.9#

157 0.0 51.6 154.8#

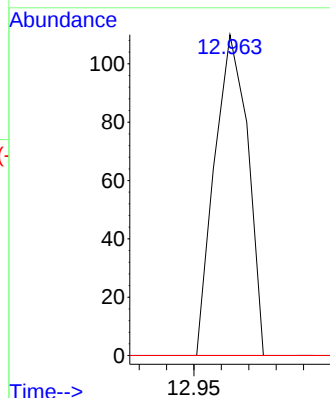

#95

Naphthalene

Concen: 17.907 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.000 min

Lab File: VX027223.D

Acq: 28 Feb 2022 16:25

Tgt Ion: 128 Resp: 88957

Ion Ratio Lower Upper

128 100

127 12.8 10.3 15.5

129 11.1 8.7 13.1

