

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022822\
 Data File : VX027228.D
 Acq On : 28 Feb 2022 18:23
 Operator : JC/MD
 Sample : N1688-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Mar 01 00:45:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 23 13:06:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	93168	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	155087	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	141316	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	65896	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	56561	50.548	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 101.100%	
35) Dibromofluoromethane	5.397	113	48240	50.112	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.220%	
50) Toluene-d8	8.653	98	181999	50.563	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 101.120%	
62) 4-Bromofluorobenzene	11.079	95	67820	49.086	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 98.180%	


Target Compounds				Qvalue		
5) Bromomethane	1.618	94	97	Below Cal	#	68
11) Tert butyl alcohol	2.965	59	30710	141.059	ug/l	97
13) Acrolein	2.215	56	228	1.133	ug/l #	1
14) Allyl chloride	2.776	41	1311	0.821	ug/l #	25
15) Acrylonitrile	3.123	53	359	0.643	ug/l #	24
16) Acetone	2.386	43	682	1.388	ug/l	93
18) Methyl Acetate	2.788	43	2144	1.691	ug/l #	53
19) Methyl tert-butyl Ether	3.117	73	30566	9.821	ug/l	98
22) Diisopropyl ether	3.770	45	5984	1.922	ug/l #	76
23) Vinyl Acetate	3.770	43	3006	1.143	ug/l #	73
29) Tetrahydrofuran	5.026	42	245	0.468	ug/l #	34
31) Cyclohexane	5.483	56	3674	2.192	ug/l	98
36) 1,1-Dichloropropene	5.562	75	6633	4.721	ug/l #	51
38) Carbon Tetrachloride	5.562	117	9249	6.312	ug/l #	17
39) Methylcyclohexane	7.385	83	692	0.396	ug/l	90
40) Benzene	6.044	78	351015	85.436	ug/l	100
42) 1,2-Dichloroethane	6.044	62	2995	2.055	ug/l #	75
43) Isopropyl Acetate	6.348	43	638	0.269	ug/l #	30
48) Methyl methacrylate	7.897	41	345	0.300	ug/l #	26
52) Toluene	8.720	92	1770	0.673	ug/l	90
59) 2-Hexanone	9.452	43	813	0.690	ug/l	87
67) Ethyl Benzene	10.195	91	17289	3.419	ug/l	97
68) m/p-Xylenes	10.305	106	765	0.393	ug/l	92
73) Isopropylbenzene	10.963	105	7215	1.530	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	33307	25.094	ug/l #	40
78) n-propylbenzene	11.305	91	6737	1.257	ug/l	97
79) 2-Chlorotoluene	11.305	91	6737	2.051	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.616	105	809	0.204	ug/l	82
81) trans-1,4-Dichloro-2-b...	11.079	75	33307	71.051	ug/l #	3
82) 4-Chlorotoluene	11.305	91	6737	1.796	ug/l #	46
90) Hexachloroethane	12.646	117	973	1.524	ug/l #	14
95) Naphthalene	13.780	128	3517	0.760	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022822\
Data File : VX027228.D
Acq On : 28 Feb 2022 18:23
Operator : JC/MD
Sample : N1688-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Mar 01 00:45:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 23 13:06:57 2022
Response via : Initial Calibration

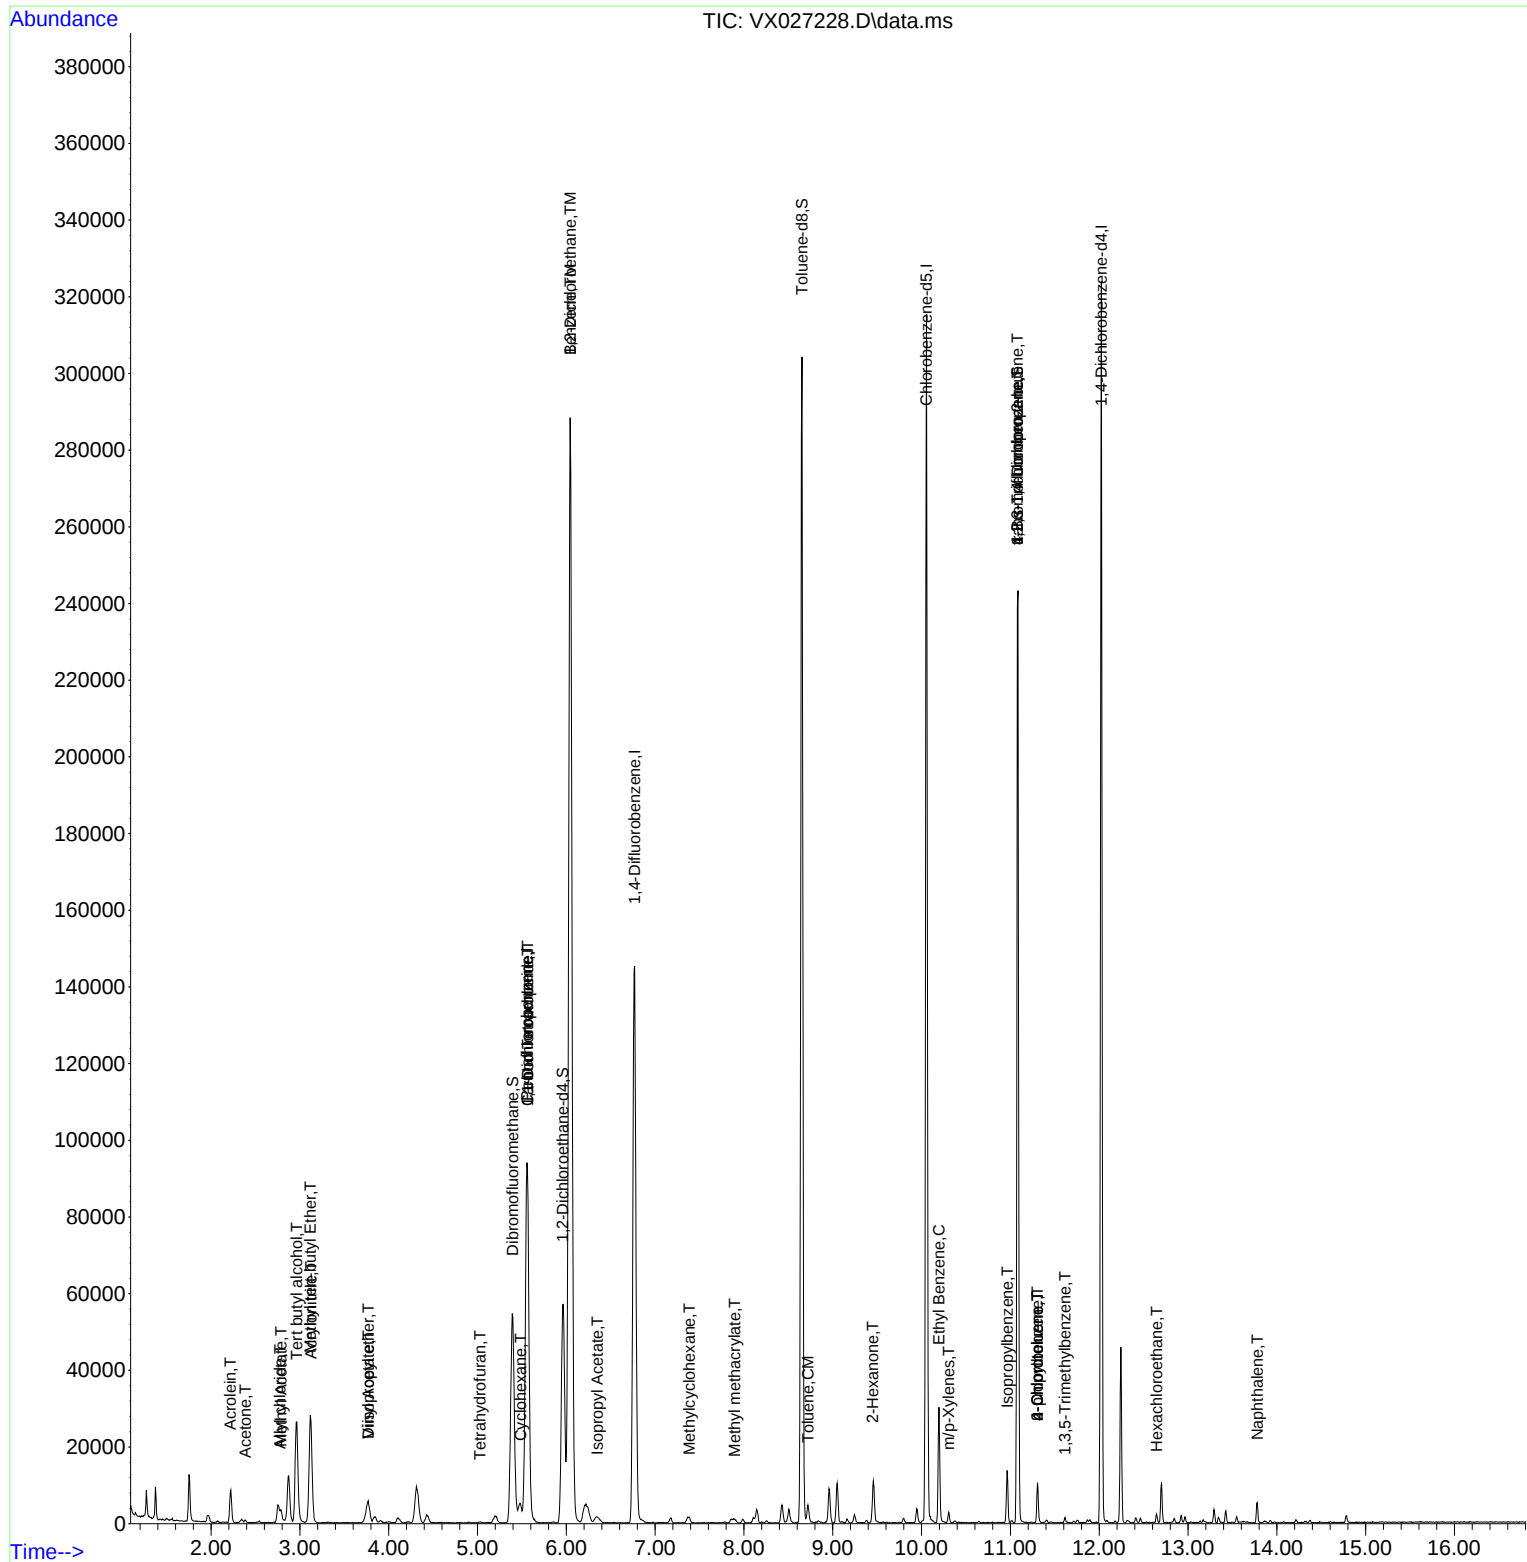






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Instrument :
MSVOA_X
ClientSampleId :



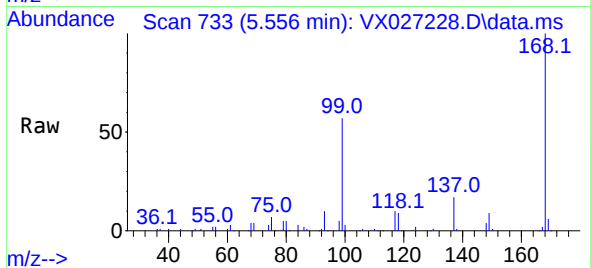



Tgt Ion:168 Resp: 93168
Ion Ratio Lower Upper
168 100
99 56.9 50.3 75.5

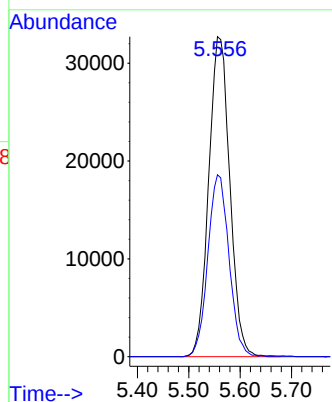

#5
Bromomethane
Concen: Below Cal
RT: 1.618 min Scan# 87
Delta R.T. 0.019 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Tgt Ion: 94 Resp: 97
Ion Ratio Lower Upper
94 100
96 63.7 75.9 113.9#

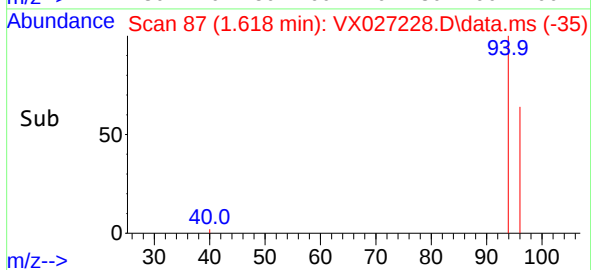



#11

Tert butyl alcohol

Concen: 141.059 ug/l

RT: 2.965 min Scan# 30

Delta R.T. -0.012 min

Lab File: VX027228.D

Acq: 28 Feb 2022 18:23

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 59 Resp: 30710

Ion Ratio Lower Upper

59 100

57 10.2 7.2 10.8

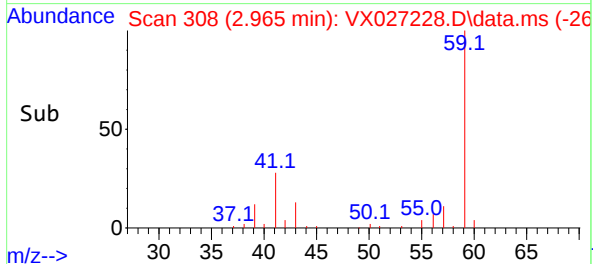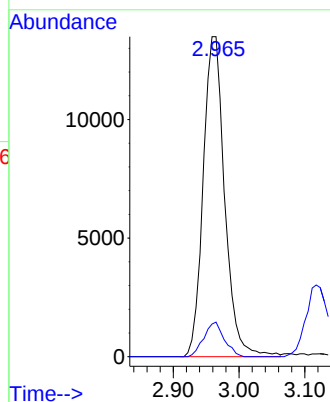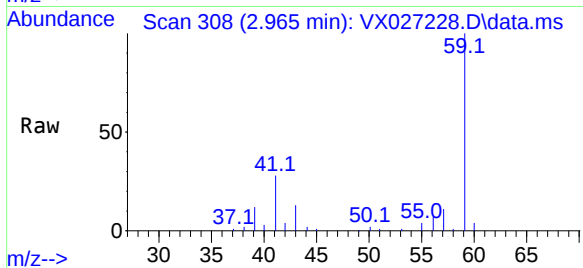

#13

Acrolein

Concen: 1.133 ug/l

RT: 2.215 min Scan# 185

Delta R.T. -0.024 min

Lab File: VX027228.D




Acq: 28 Feb 2022 18:23


Tgt Ion: 56 Resp: 228

Ion Ratio Lower Upper

56 100


55 2109.6 56.9 85.3#

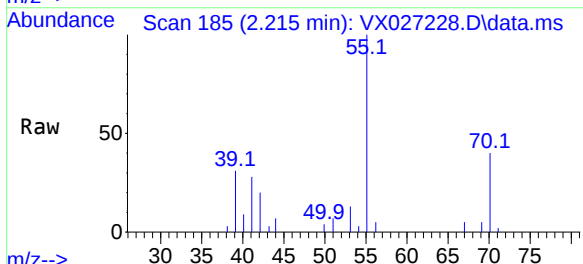






#14
 Allyl chloride
 Concen: 0.821 ug/l
 RT: 2.776 min Scan# 21
 Delta R.T. 0.110 min
 Lab File: VX027228.D
 Acq: 28 Feb 2022 18:23

Instrument :
 MSVOA_X
 ClientSampleId :







Tgt Ion: 41 Resp: 1311
 Ion Ratio Lower Upper
 41 100
 39 0.0 54.2 81.4#
 76 0.0 25.2 37.8#

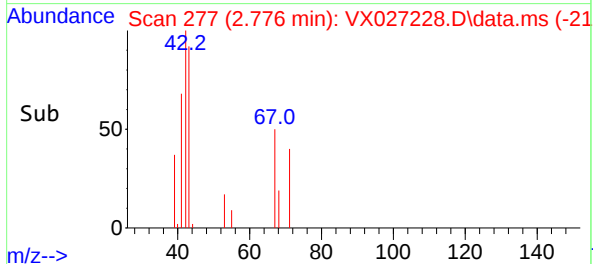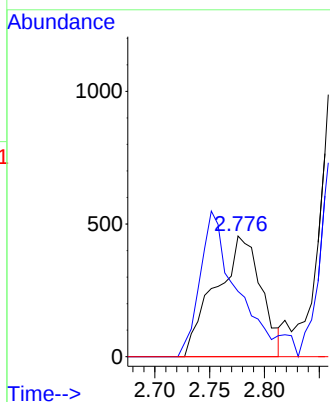

#15
 Acrylonitrile
 Concen: 0.643 ug/l
 RT: 3.123 min Scan# 334
 Delta R.T. 0.055 min
 Lab File: VX027228.D
 Acq: 28 Feb 2022 18:23

Tgt Ion: 53 Resp: 359
 Ion Ratio Lower Upper
 53 100
 52 0.0 66.6 100.0#
 51 61.0 29.5 44.3#


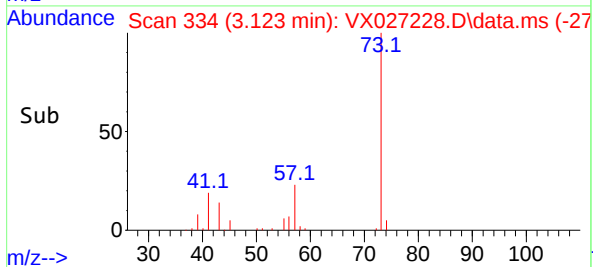

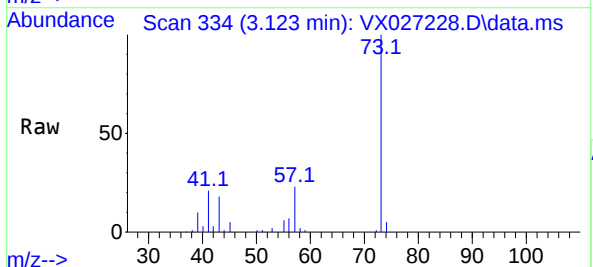




#16
Acetone
Concen: 1.388 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 682
Ion Ratio Lower Upper
43 100
58 24.9 23.0 34.6



#18
Methyl Acetate
Concen: 1.691 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.079 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Tgt Ion: 43 Resp: 2144
Ion Ratio Lower Upper
43 100
74 0.0 18.3 27.5#


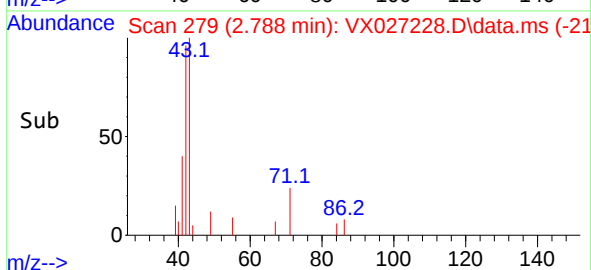






#19
Methyl tert-butyl Ether
Concen: 9.821 ug/l
RT: 3.117 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 73 Resp: 30566
Ion Ratio Lower Upper
73 100
57 22.6 17.4 26.2

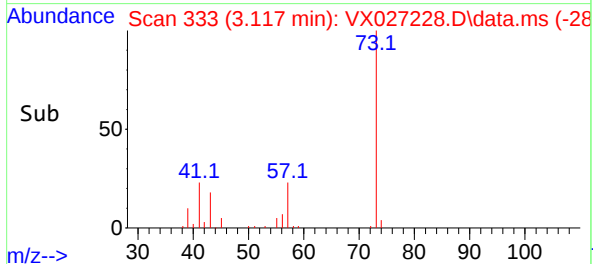

#22
Diisopropyl ether
Concen: 1.922 ug/l
RT: 3.770 min Scan# 440
Delta R.T. 0.001 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Tgt Ion: 45 Resp: 5984
Ion Ratio Lower Upper
45 100
43 46.5 60.6 91.0#
87 26.0 22.0 33.0
59 13.9 9.0 13.4#



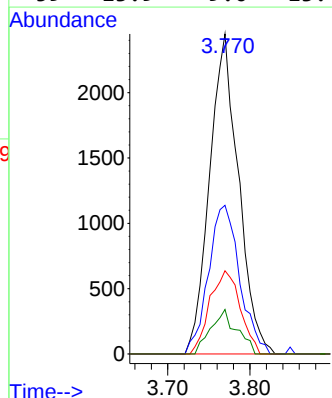
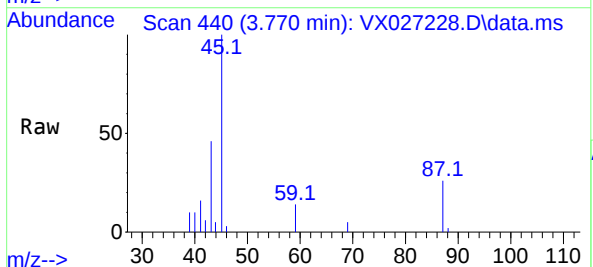


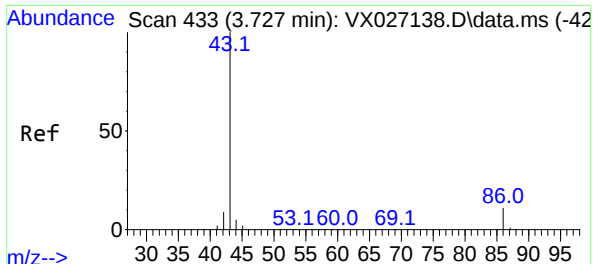

#23
 Vinyl Acetate
 Concen: 1.143 ug/l
 RT: 3.770 min Scan# 44
 Delta R.T. 0.043 min
 Lab File: VX027228.D
 Acq: 28 Feb 2022 18:23




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 43 Resp: 3006
 Ion Ratio Lower Upper
 43 100
 86 0.0 8.1 12.1#

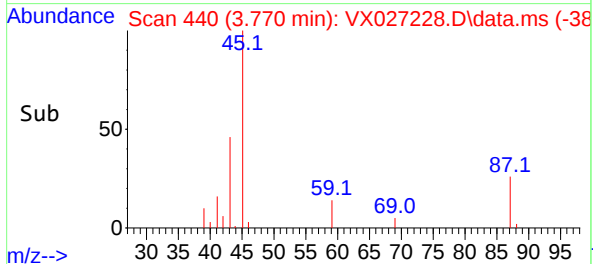

#29
 Tetrahydrofuran
 Concen: 0.468 ug/l
 RT: 5.026 min Scan# 646
 Delta R.T. 0.019 min
 Lab File: VX027228.D
 Acq: 28 Feb 2022 18:23


Tgt Ion: 42 Resp: 245
 Ion Ratio Lower Upper
 42 100
 72 0.0 34.6 52.0#
 71 0.0 31.8 47.8#

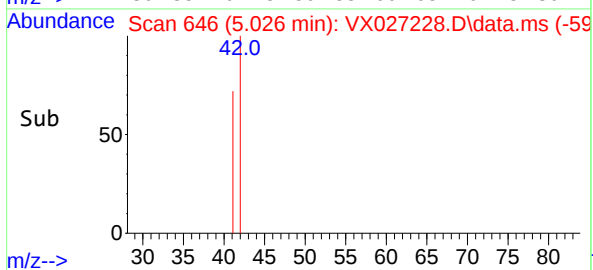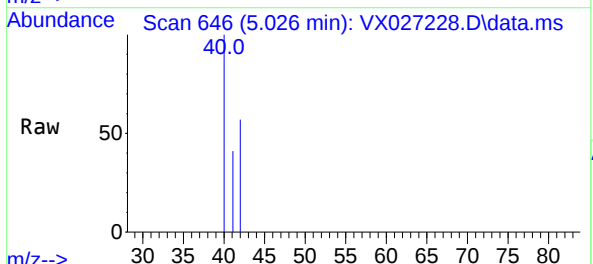






#31
Cyclohexane
Concen: 2.192 ug/l
RT: 5.483 min Scan# 719
Delta R.T. 0.007 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Instrument :
MSVOA_X
ClientSampleId :



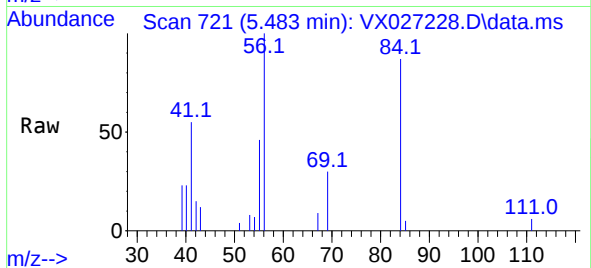



Tgt Ion: 56 Resp: 3674
Ion Ratio Lower Upper
56 100
69 30.4 25.8 38.6
84 87.1 68.9 103.3



#33
1,2-Dichloroethane-d4
Concen: 50.548 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Tgt Ion: 65 Resp: 56561
Ion Ratio Lower Upper
65 100
67 52.6 0.0 100.8

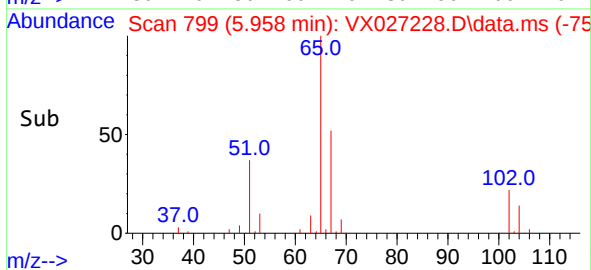



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 91

Delta R.T. 0.000 min

Lab File: VX027228.D

Acq: 28 Feb 2022 18:23

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:114 Resp: 155087

Ion Ratio Lower Upper

114 100

63 19.1 0.0 42.8

88 16.1 0.0 33.0

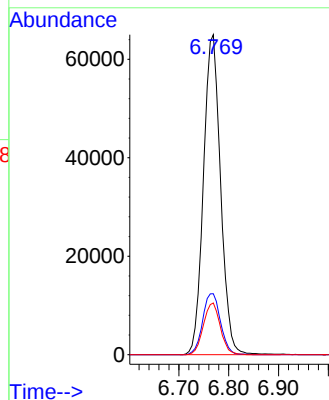

#35

Dibromofluoromethane

Concen: 50.112 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.006 min

Lab File: VX027228.D

Acq: 28 Feb 2022 18:23




Tgt Ion:113 Resp: 48240


Ion Ratio Lower Upper

113 100

111 102.5 81.2 121.8


192 19.8 15.0 22.4

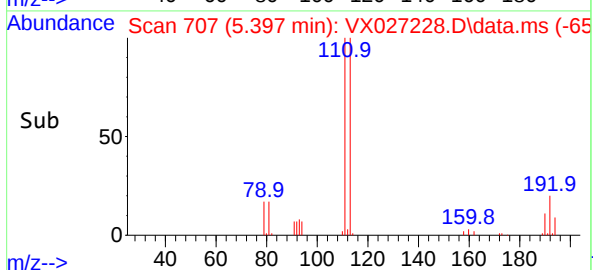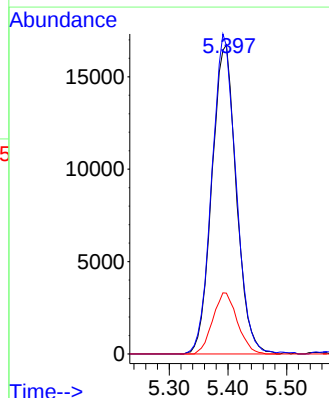



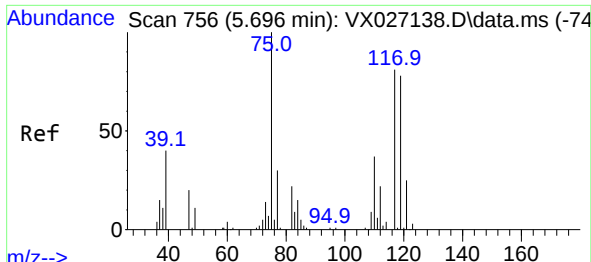


#36
1,1-Dichloropropene
Concen: 4.721 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Instrument :
MSVOA_X
ClientSampleId :



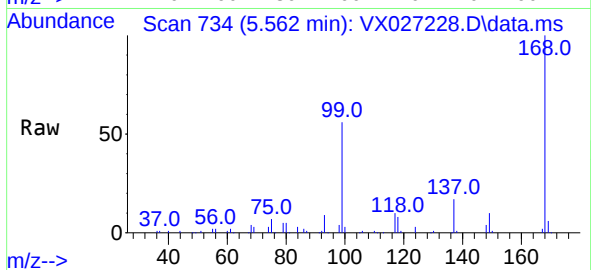



Tgt Ion: 75 Resp: 6633
Ion Ratio Lower Upper
75 100
110 9.6 17.2 51.6#
77 0.0 24.6 36.8#

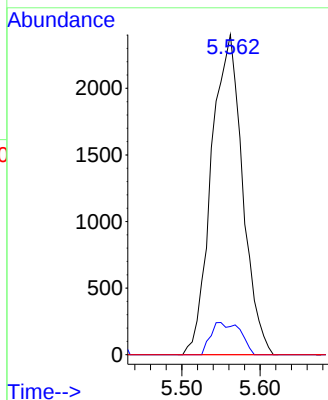

#38
Carbon Tetrachloride
Concen: 6.312 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.122 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Tgt Ion: 117 Resp: 9249
Ion Ratio Lower Upper
117 100
119 5.6 74.7 112.1#
121 0.0 25.4 38.0#

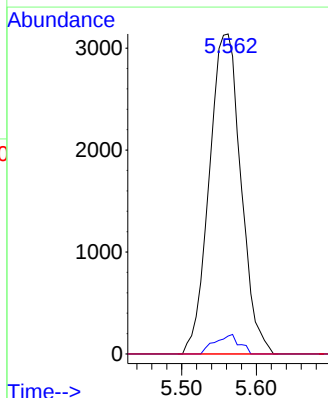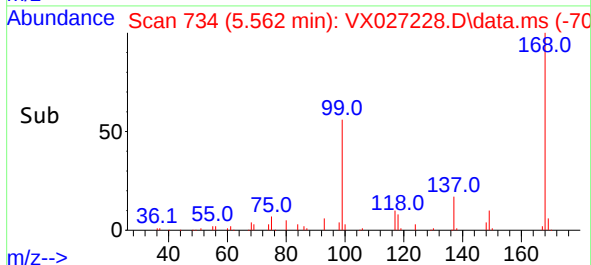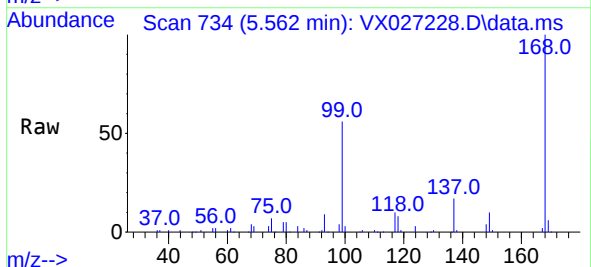



#39

Methylcyclohexane

Concen: 0.396 ug/l

RT: 7.385 min Scan# 1033

Delta R.T. -0.000 min

Lab File: VX027228.D

Acq: 28 Feb 2022 18:23

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 83 Resp: 692

Ion Ratio Lower Upper

83 100

55 90.7 63.6 95.4

98 51.5 38.4 57.6

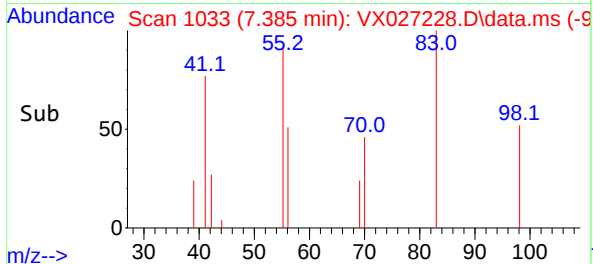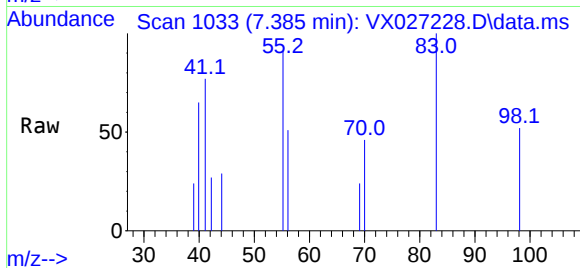

#40

Benzene

Concen: 85.436 ug/l

RT: 6.044 min Scan# 813

Delta R.T. 0.001 min

Lab File: VX027228.D




Acq: 28 Feb 2022 18:23


Tgt Ion: 78 Resp: 351015

Ion Ratio Lower Upper

78 100

77 23.6 18.9 28.3

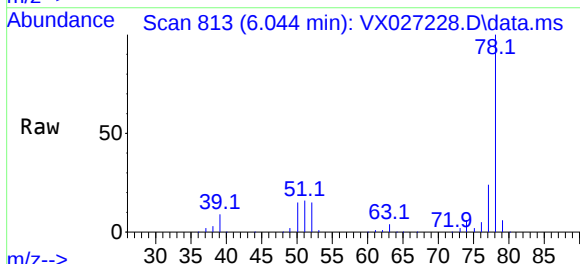



#42

1,2-Dichloroethane

Concen: 2.055 ug/l

RT: 6.044 min Scan# 813

Delta R.T. -0.048 min

Lab File: VX027228.D

Acq: 28 Feb 2022 18:23

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 62 Resp: 2995

Ion Ratio Lower Upper

62 100

98 0.0 0.0 17.8

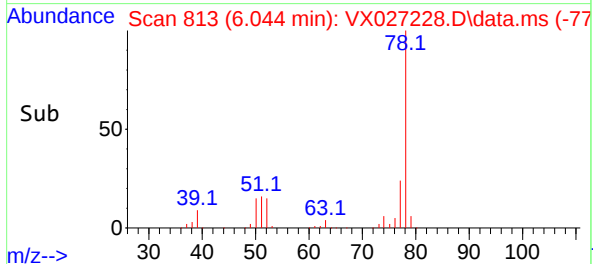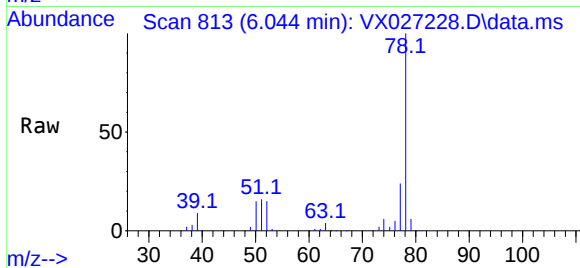

#43

Isopropyl Acetate

Concen: 0.269 ug/l

RT: 6.348 min Scan# 863

Delta R.T. 0.000 min

Lab File: VX027228.D

Acq: 28 Feb 2022 18:23




Tgt Ion: 43 Resp: 638


Ion Ratio Lower Upper

43 100

61 0.0 15.4 23.0#

87 56.7 10.2 15.2#

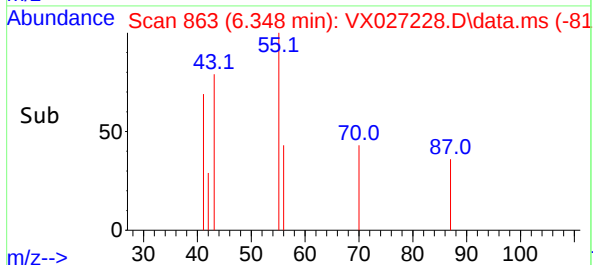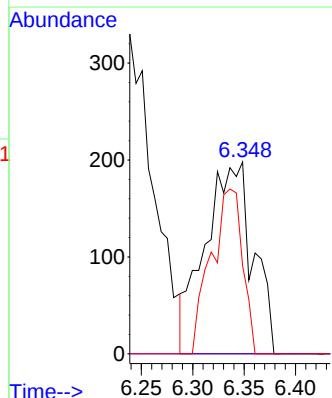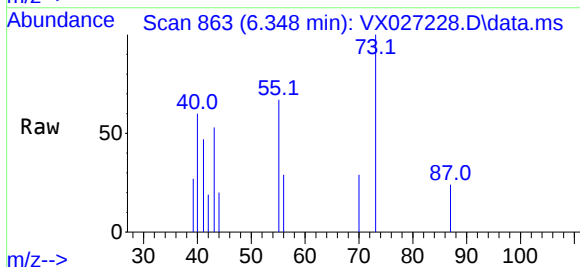



#48

Methyl methacrylate

Concen: 0.300 ug/l

RT: 7.897 min Scan# 1117

Delta R.T. 0.201 min

Lab File: VX027228.D





Acq: 28 Feb 2022 18:23

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 41	Resp: 345
Ion Ratio	Lower Upper
41	100
69	0.0 62.2 93.4#
39	95.9 45.4 68.0#



#50

Toluene-d8

Concen: 50.563 ug/l




RT: 8.653 min Scan# 1241


Delta R.T. -0.000 min

Lab File: VX027228.D

Acq: 28 Feb 2022 18:23

Tgt Ion: 98	Resp: 181999
Ion Ratio	Lower Upper
98	100
100	67.4 53.2 79.8



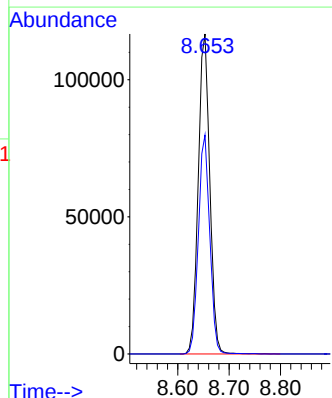
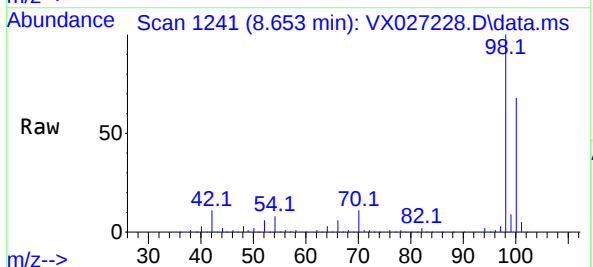




#52
Toluene
Concen: 0.673 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 1770
Ion Ratio Lower Upper
92 100
91 156.6 135.7 203.5

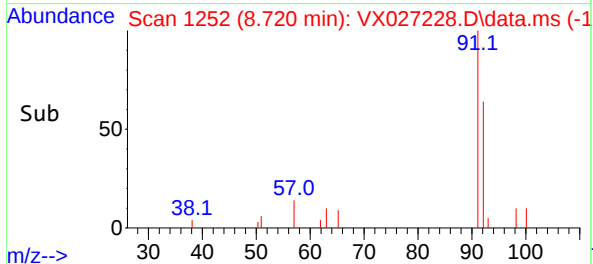

#59
2-Hexanone
Concen: 0.690 ug/l
RT: 9.452 min Scan# 1372
Delta R.T. 0.019 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Tgt Ion: 43 Resp: 813
Ion Ratio Lower Upper
43 100
58 43.9 26.4 79.2


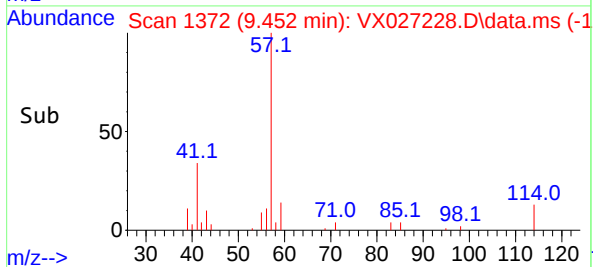

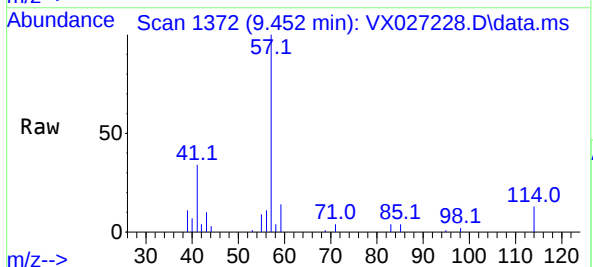




#62
4-Bromofluorobenzene
Concen: 49.086 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 67820
Ion Ratio Lower Upper
95 100
174 78.8 0.0 148.6
176 76.1 0.0 141.4

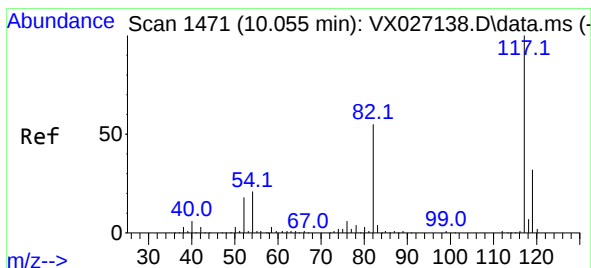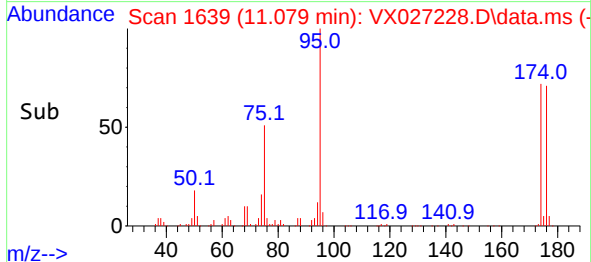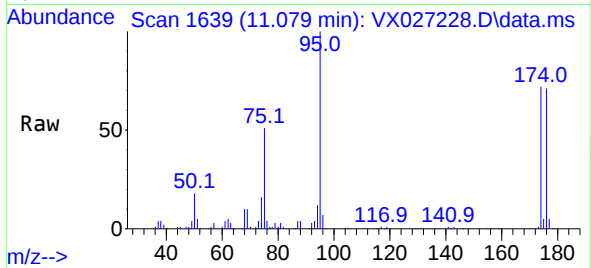

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Tgt Ion: 117 Resp: 141316
Ion Ratio Lower Upper
117 100
82 54.8 45.2 67.8
119 32.4 26.2 39.2


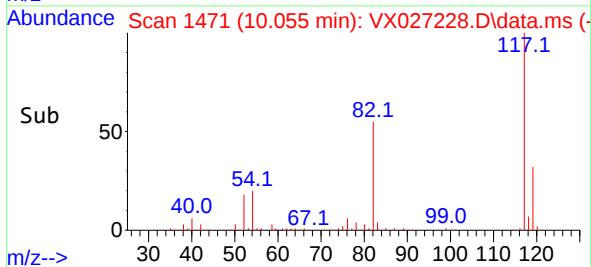

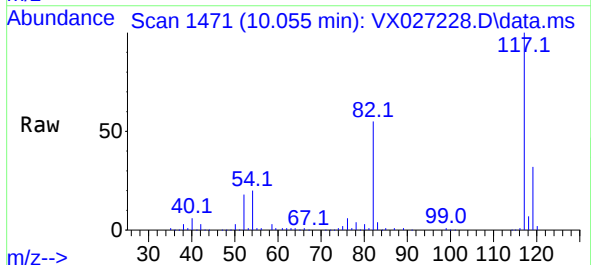




#67
Ethyl Benzene
Concen: 3.419 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 17289
Ion Ratio Lower Upper
91 100
106 32.6 24.7 37.1

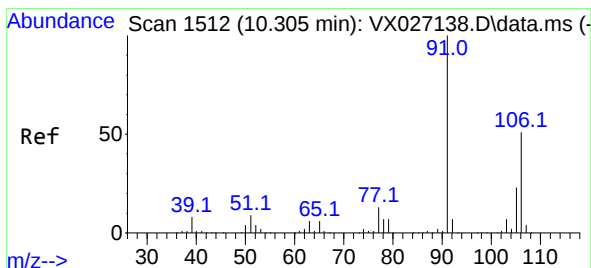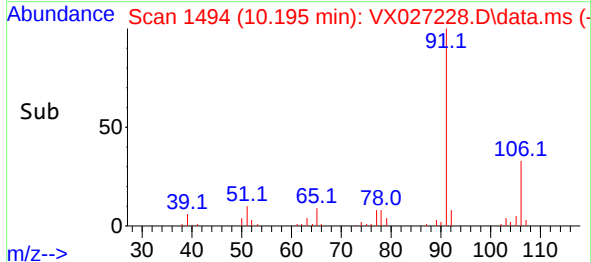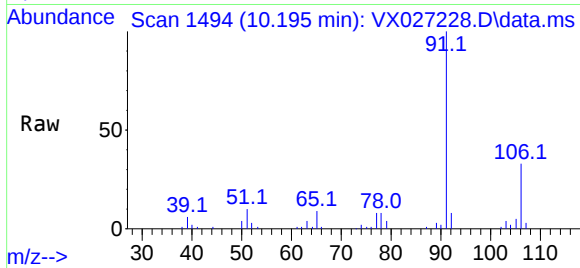

#68
m/p-Xylenes
Concen: 0.393 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23


Tgt Ion: 106 Resp: 765
Ion Ratio Lower Upper
106 100
91 194.2 165.3 247.9

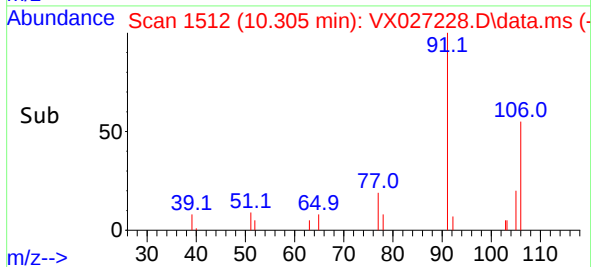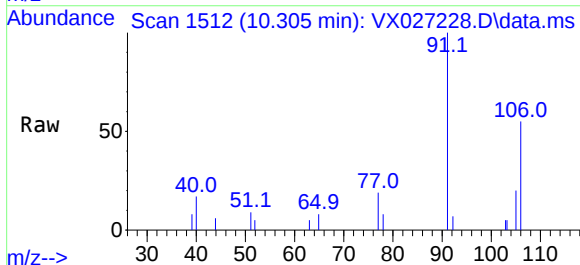






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23


Instrument :
MSVOA_X
ClientSampleId :

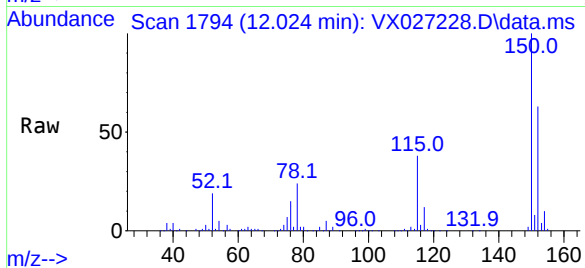



Tgt Ion:152 Resp: 65896
Ion Ratio Lower Upper
152 100
115 59.5 44.2 132.6
150 157.7 0.0 348.2

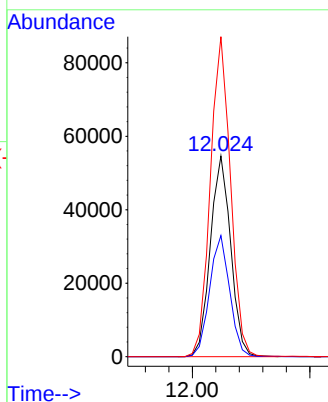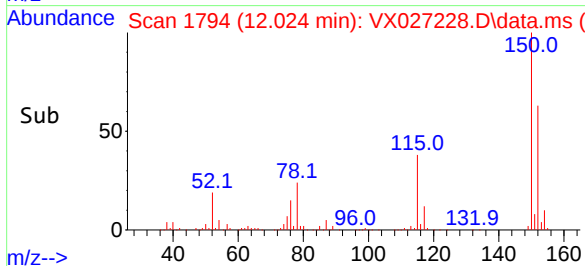


#73
Isopropylbenzene
Concen: 1.530 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

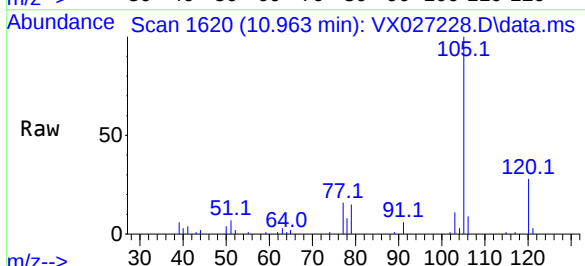


Tgt Ion:105 Resp: 7215
Ion Ratio Lower Upper
105 100
120 27.4 13.1 39.1

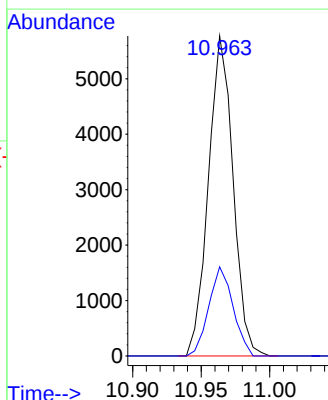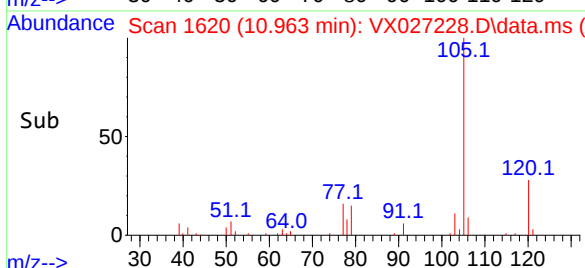






#76
1,2,3-Trichloropropane
Concen: 25.094 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Instrument :
MSVOA_X
ClientSampleId :



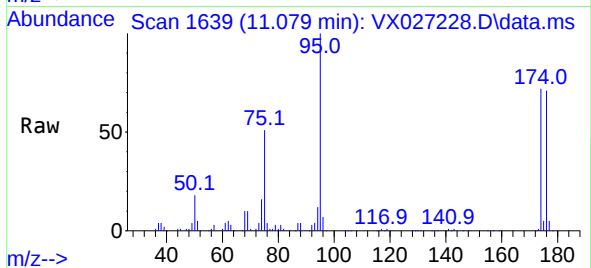



Tgt Ion: 75 Resp: 33307
Ion Ratio Lower Upper
75 100
77 1.2 18.3 54.8#

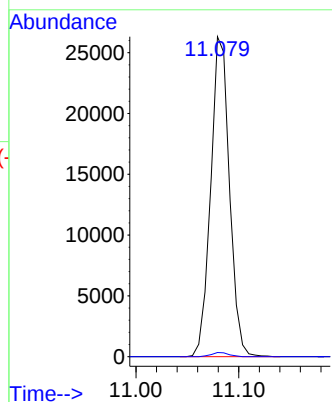

#78
n-propylbenzene
Concen: 1.257 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Tgt Ion: 91 Resp: 6737
Ion Ratio Lower Upper
91 100
120 21.7 11.6 34.7

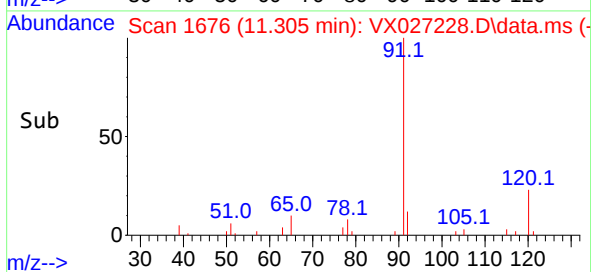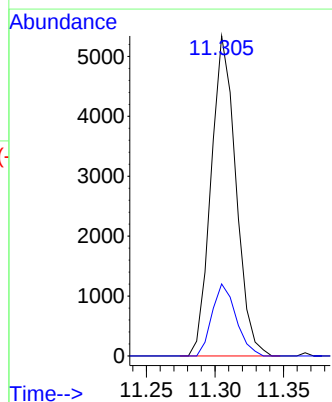



#79

2-Chlorotoluene

Concen: 2.051 ug/l

RT: 11.305 min Scan# 1

Delta R.T. -0.061 min

Lab File: VX027228.D

Acq: 28 Feb 2022 18:23

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 6737

Ion Ratio Lower Upper

91 100

126 0.0 16.4 49.2#

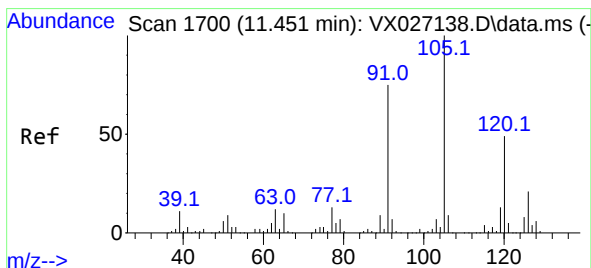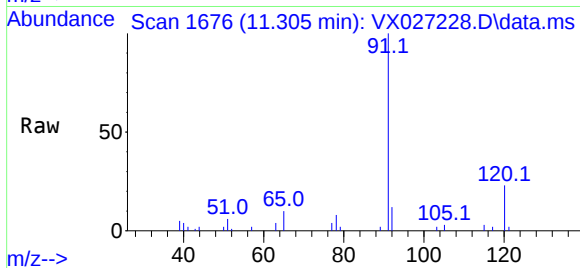

#80

1,3,5-Trimethylbenzene

Concen: 0.204 ug/l

RT: 11.616 min Scan# 1727

Delta R.T. 0.165 min

Lab File: VX027228.D




Acq: 28 Feb 2022 18:23


Tgt Ion:105 Resp: 809

Ion Ratio Lower Upper

105 100

120 36.0 24.0 72.0


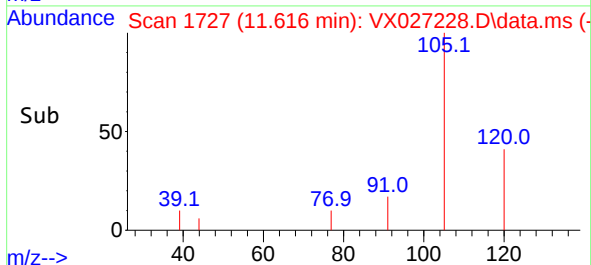
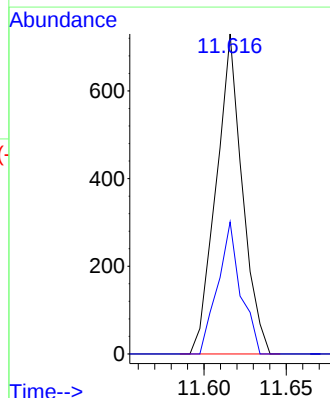
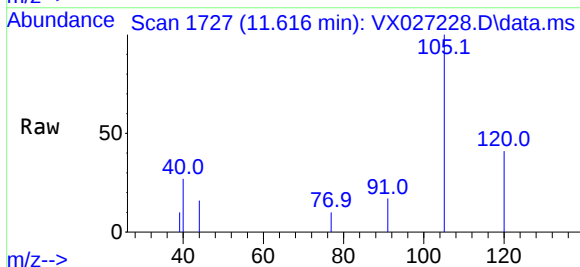




#81
trans-1,4-Dichloro-2-butene
Concen: 71.051 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.055 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 33307
Ion Ratio Lower Upper
75 100
53 0.0 94.0 141.0#
89 0.0 37.0 55.4#

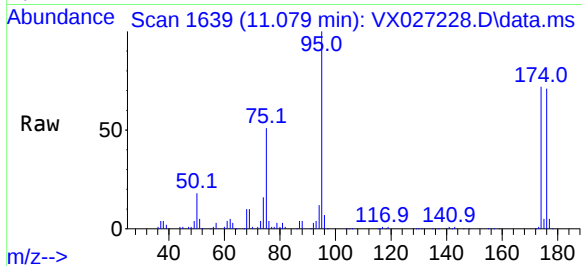

#82
4-Chlorotoluene
Concen: 1.796 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.152 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Tgt Ion: 91 Resp: 6737
Ion Ratio Lower Upper
91 100
126 0.0 14.1 42.4#


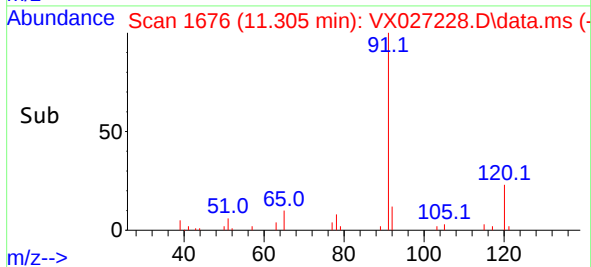

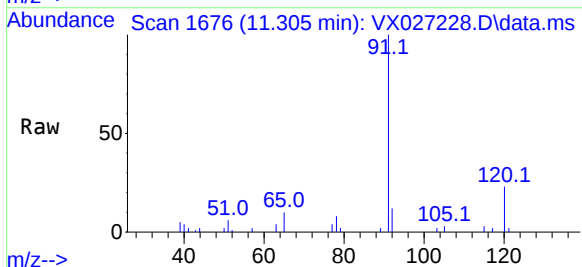




#90
Hexachloroethane
Concen: 1.524 ug/l
RT: 12.646 min Scan# 1879
Delta R.T. 0.104 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:117 Resp: 973
Ion Ratio Lower Upper
117 100
201 0.0 35.6 106.8#

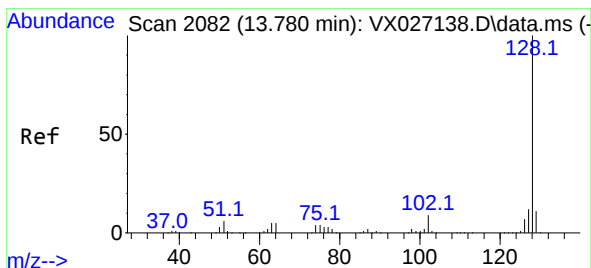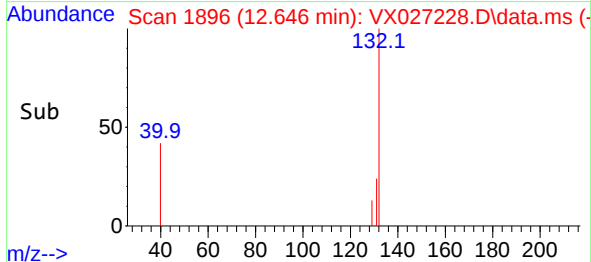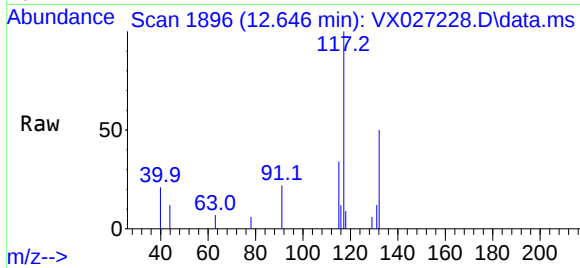

#95
Naphthalene
Concen: 0.760 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX027228.D
Acq: 28 Feb 2022 18:23

Tgt Ion:128 Resp: 3517
Ion Ratio Lower Upper
128 100
127 12.5 10.3 15.5
129 10.9 8.7 13.1

