

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022822\
 Data File : VX027225.D
 Acq On : 28 Feb 2022 17:12
 Operator : JC/MD
 Sample : N1688-10DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-27DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Title : SW846 8260

Signal : TIC: VX027225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	695	706	718	rBV	53447	153790	33.19%	5.506%
2	5.556	723	733	747	rVB	93611	263509	56.87%	9.433%
3	5.958	790	799	807	rBV	56523	150925	32.57%	5.403%
4	6.043	807	813	827	rVB	40797	106725	23.03%	3.821%
5	6.763	921	931	946	rBV	144946	343147	74.05%	12.284%
6	8.653	1234	1241	1248	rBV	298438	463378	100.00%	16.589%
7	8.720	1248	1252	1258	rVB	4037	6416	1.38%	0.230%
8	10.055	1465	1471	1482	rBV	308355	406611	87.75%	14.556%
9	10.195	1489	1494	1502	rVB	39295	49828	10.75%	1.784%
10	10.305	1507	1512	1521	rBV	24890	31342	6.76%	1.122%
11	10.640	1563	1567	1574	rBV	21177	27774	5.99%	0.994%
12	11.079	1634	1639	1651	rVB	237645	312950	67.54%	11.203%
13	11.305	1672	1676	1681	rBV	4175	5446	1.18%	0.195%
14	11.402	1684	1692	1696	rBV	3917	6093	1.31%	0.218%
15	11.616	1722	1727	1733	rVB	9114	11189	2.41%	0.401%
16	11.750	1745	1749	1756	rVB	16660	21016	4.54%	0.752%
17	12.024	1789	1794	1800	rBV	324577	389119	83.97%	13.930%
18	12.091	1800	1805	1810	rVB	8935	11367	2.45%	0.407%
19	12.244	1825	1830	1835	rBV	10599	12345	2.66%	0.442%
20	13.292	1997	2002	2008	rVB3	4434	5765	1.24%	0.206%
21	13.780	2076	2082	2086	rBV	5993	7594	1.64%	0.272%
22	14.780	2239	2246	2252	rVB	5122	7008	1.51%	0.251%


Sum of corrected areas: 2793337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022822\
Data File : VX027225.D
Acq On : 28 Feb 2022 17:12
Operator : JC/MD
Sample : N1688-10DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

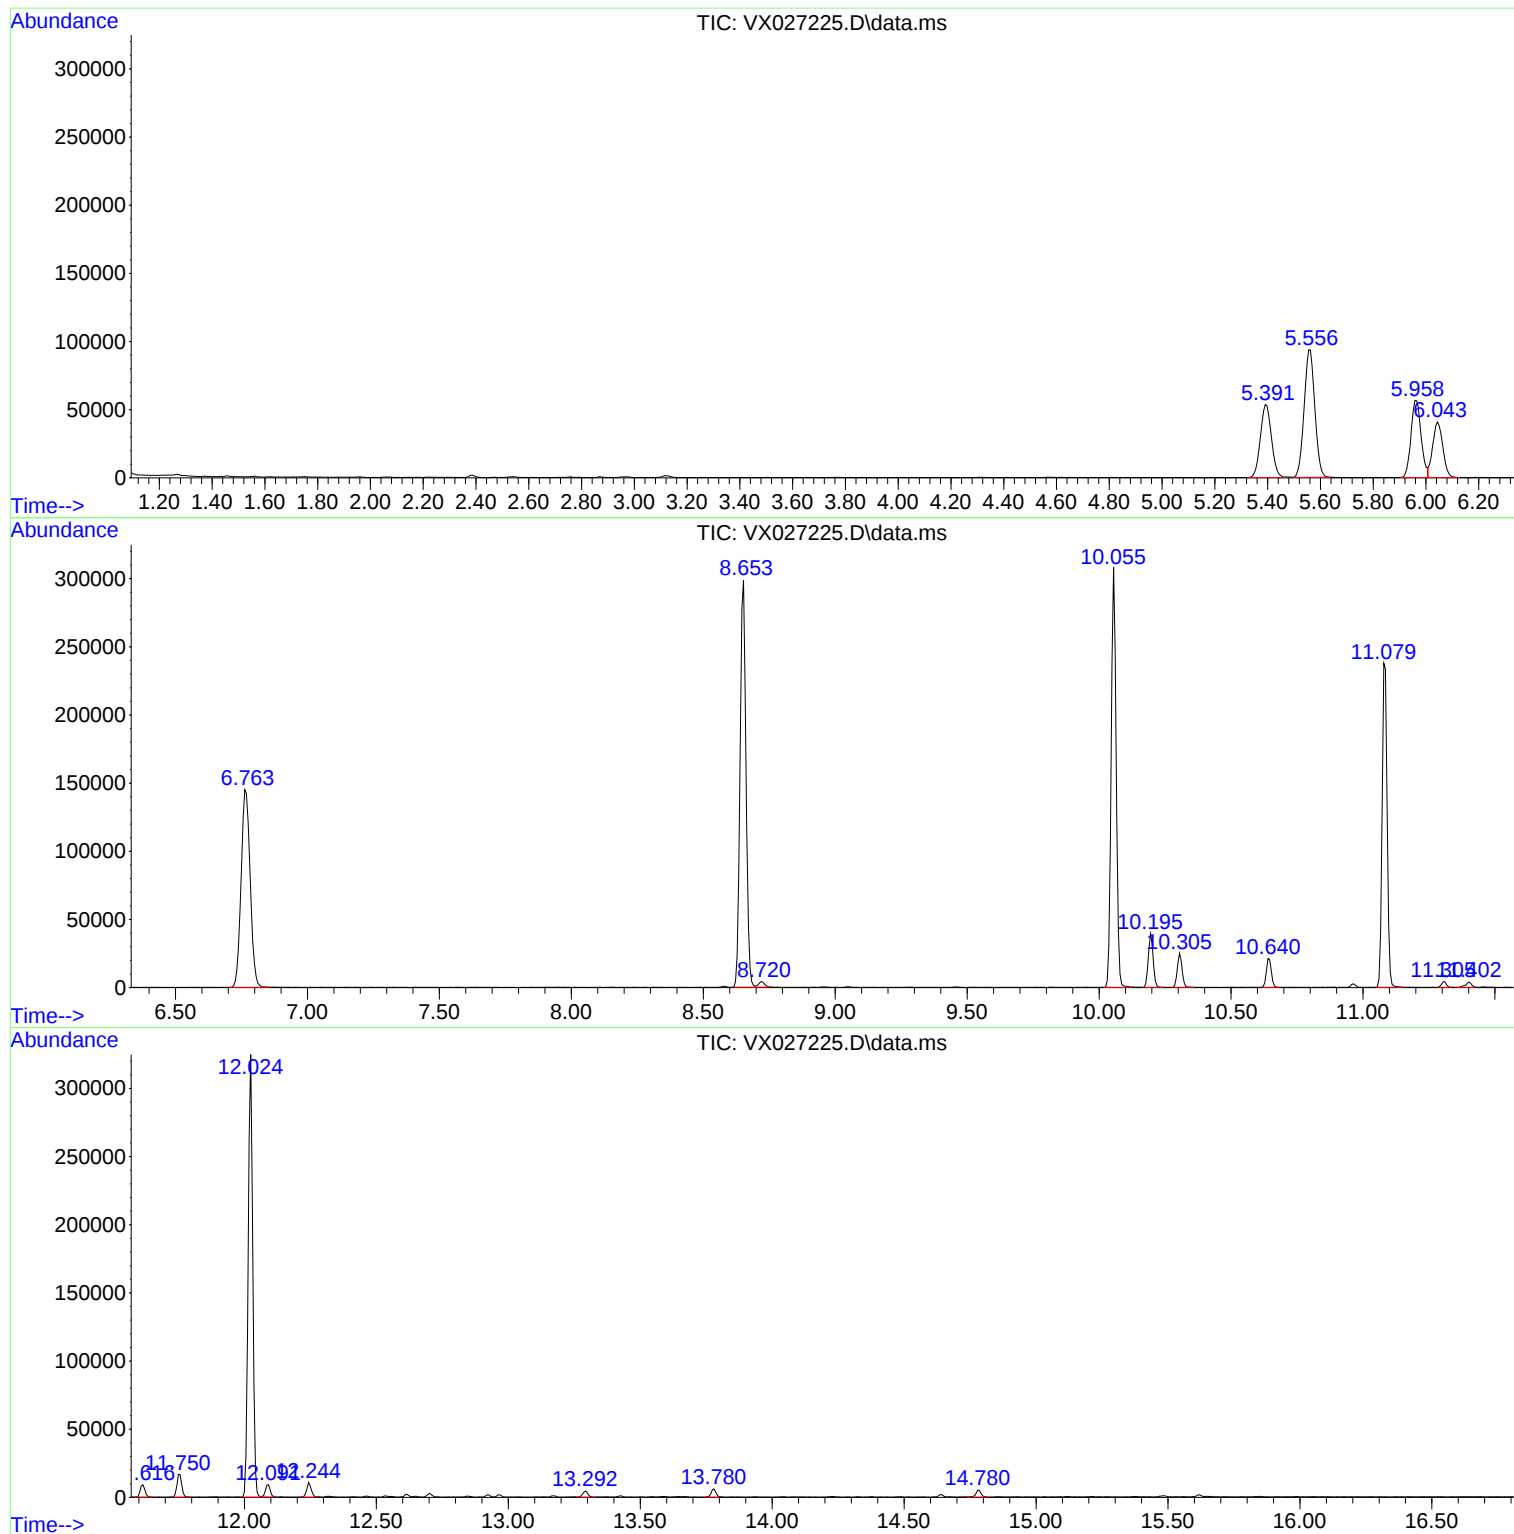

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022822\
Data File : VX027225.D
Acq On : 28 Feb 2022 17:12
Operator : JC/MD
Sample : N1688-10DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022822\
Data File : VX027225.D
Acq On : 28 Feb 2022 17:12
Operator : JC/MD
Sample : N1688-10DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------