
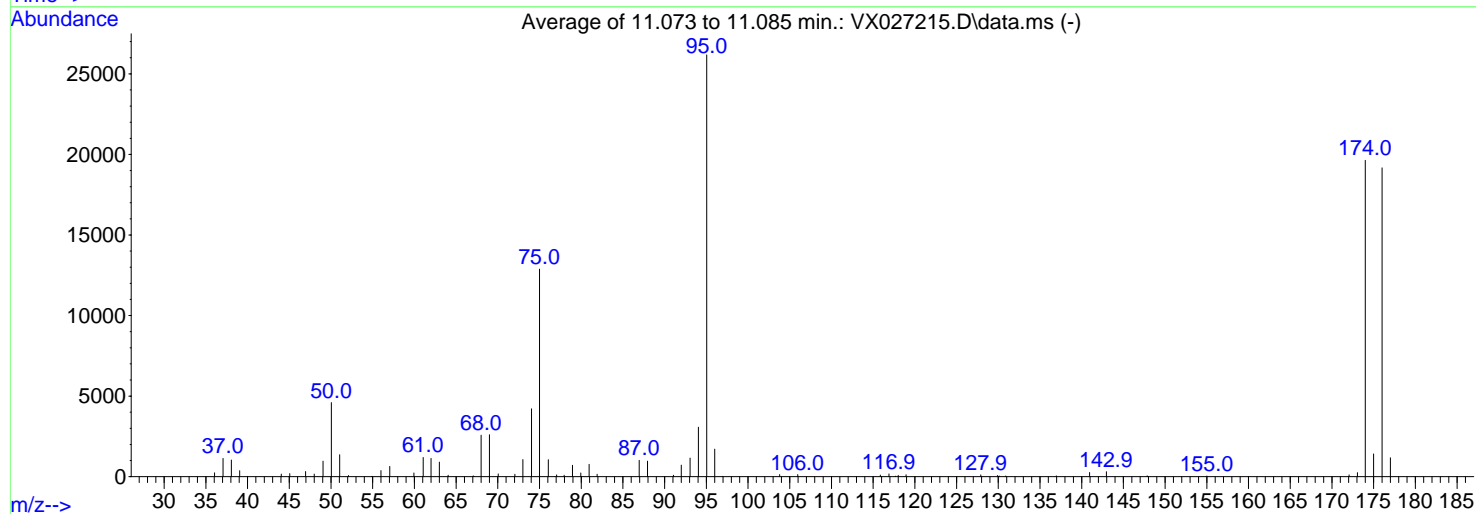


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022822\
 Data File : VX027215.D
 Acq On : 28 Feb 2022 09:43
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Title : SW846 8260
 Last Update : Wed Feb 23 13:06:57 2022

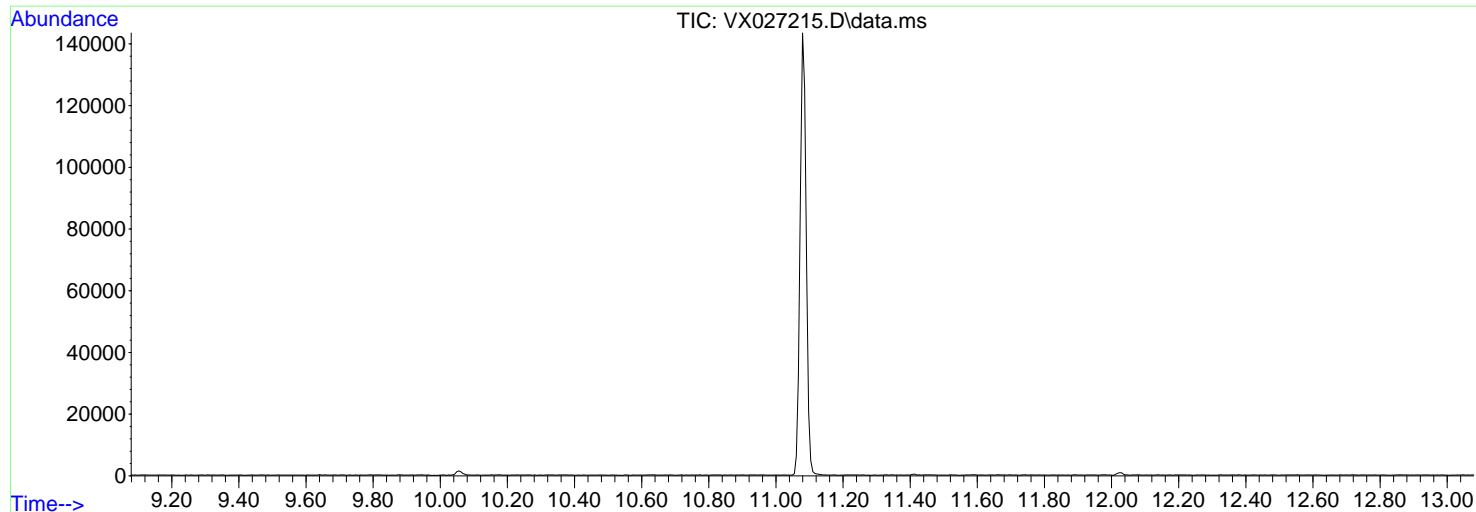

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	4602	PASS
75	95	30	60	49.2	12883	PASS
95	95	100	100	100.0	26181	PASS
96	95	5	9	6.5	1708	PASS
173	174	0.00	2	1.3	250	PASS
174	95	50	100	75.0	19636	PASS
175	174	5	9	7.2	1411	PASS
176	174	95	101	97.6	19163	PASS
177	176	5	9	6.1	1171	PASS