

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022824\
 Data File : VX040514.D
 Acq On : 28 Feb 2024 16:26
 Operator : JC/MD
 Sample : P1613-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1847

Quant Time: Feb 29 03:52:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 27 05:01:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	75573	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	132767	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	129141	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	65883	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	62396	49.364	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.720%
35) Dibromofluoromethane	5.385	113	44560	48.264	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.520%
50) Toluene-d8	8.647	98	161519	48.196	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.400%
62) 4-Bromofluorobenzene	11.079	95	66428	51.999	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	104.000%
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.959	59	1360	6.400	ug/l #	92
16) Acetone	2.380	43	22248	53.972	ug/l	95
25) 2-Butanone	4.586	43	1470	2.047	ug/l #	84
52) Toluene	8.720	92	1172	0.496	ug/l	80
68) m/p-Xylenes	10.305	106	1009	0.537	ug/l	90
69) o-Xylene	10.646	106	389	0.217	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022824\
Data File : VX040514.D
Acq On : 28 Feb 2024 16:26
Operator : JC/MD
Sample : P1613-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1847

Quant Time: Feb 29 03:52:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 27 05:01:33 2024
Response via : Initial Calibration




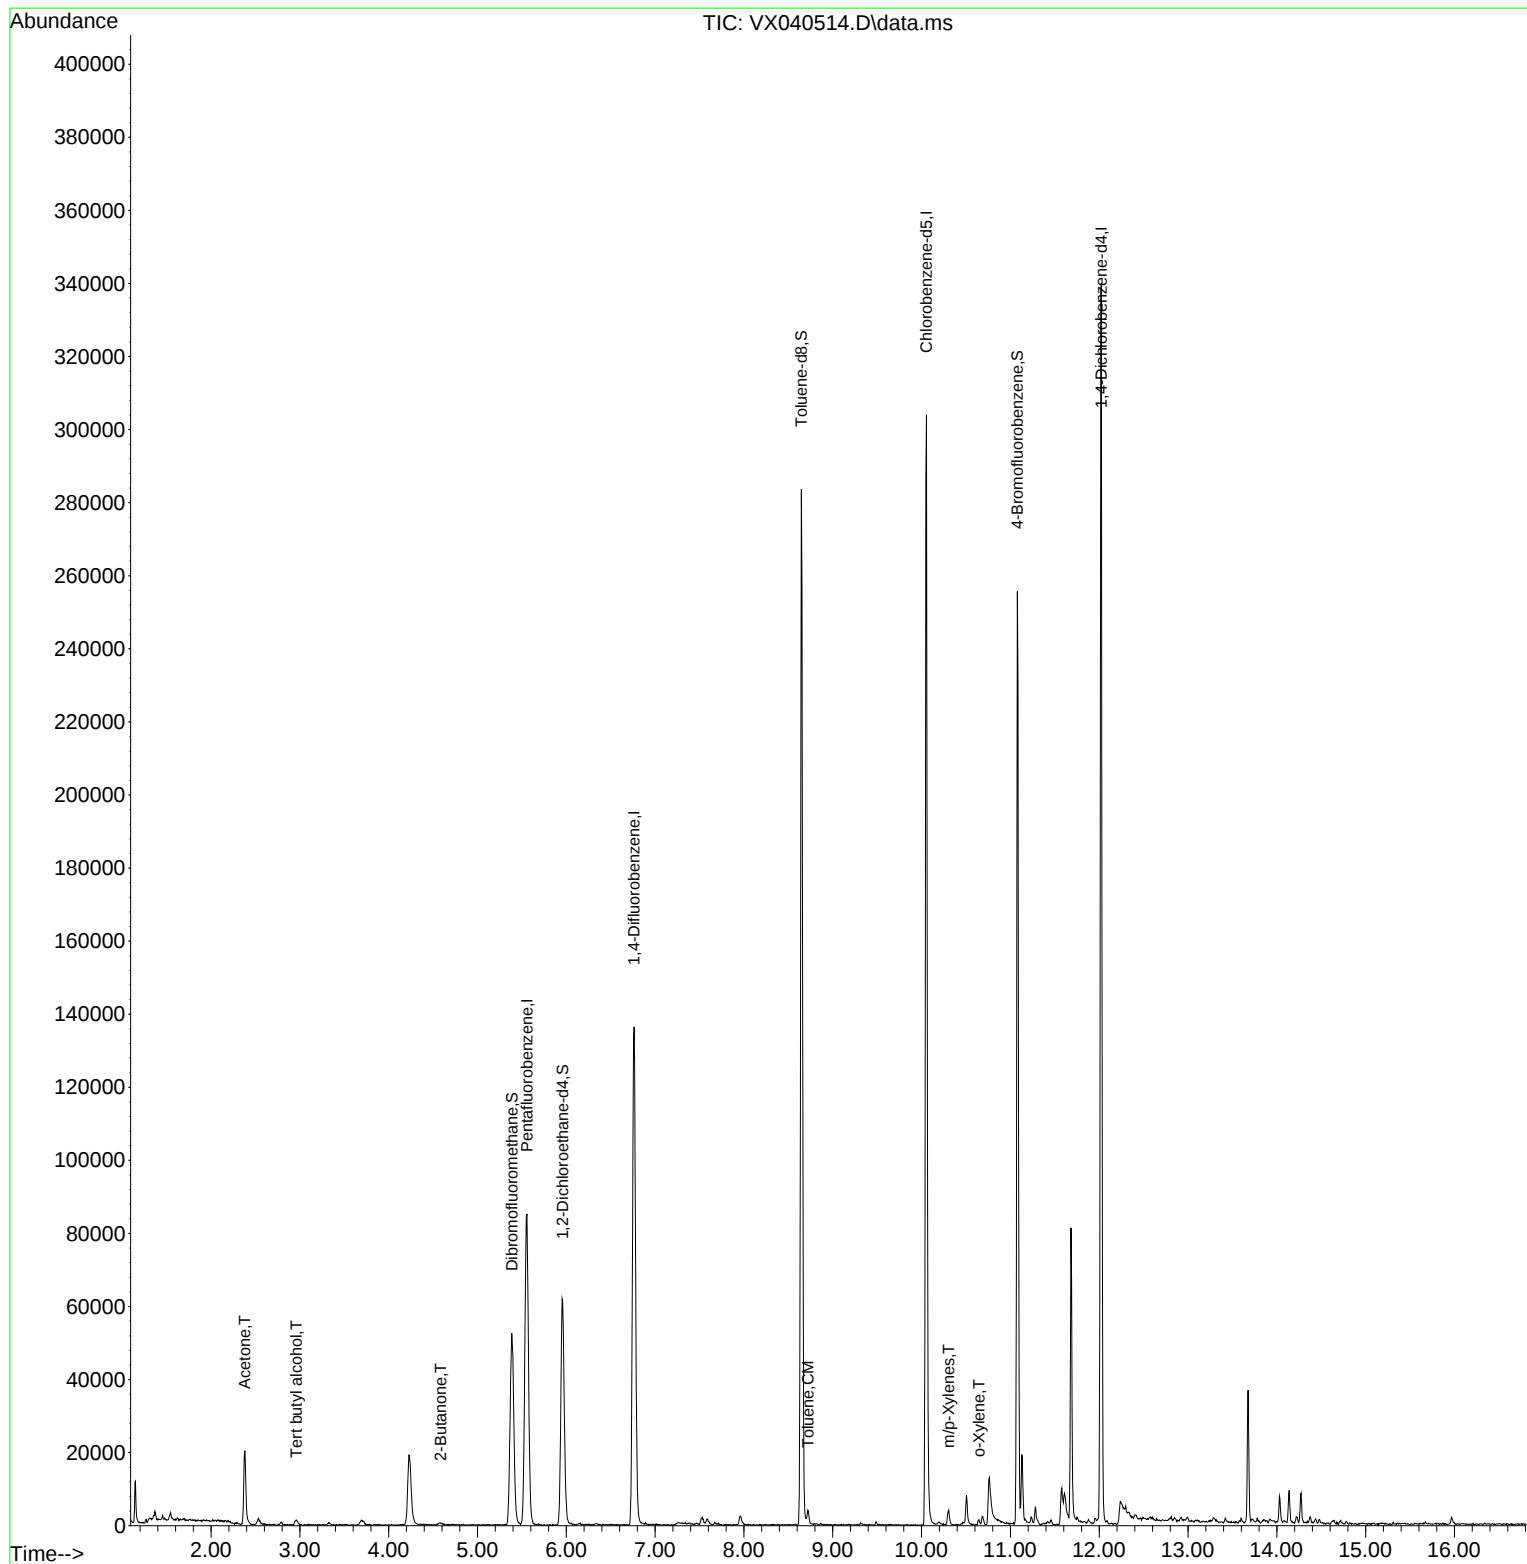


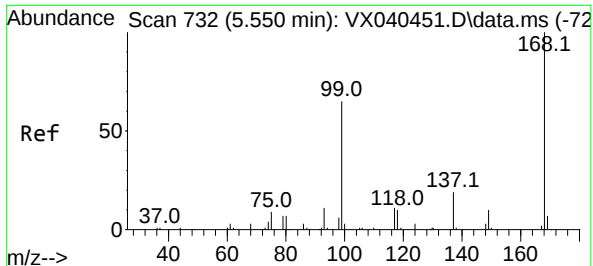

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX040514.D
Acq: 28 Feb 2024 16:26




Instrument :
MSVOA_X
ClientSampleId :
1847


Tgt Ion:168 Resp: 75573
Ion Ratio Lower Upper
168 100
99 65.4 56.6 85.0

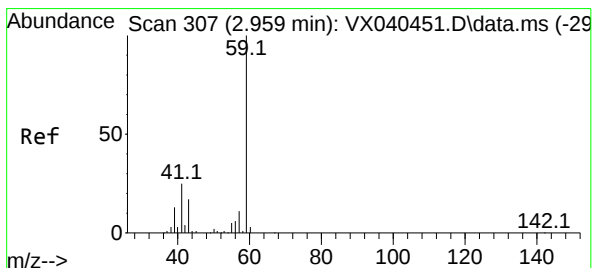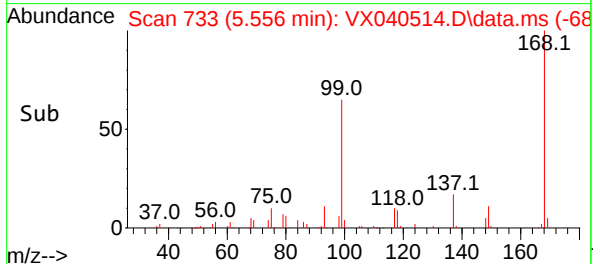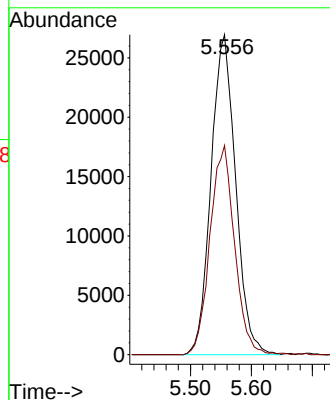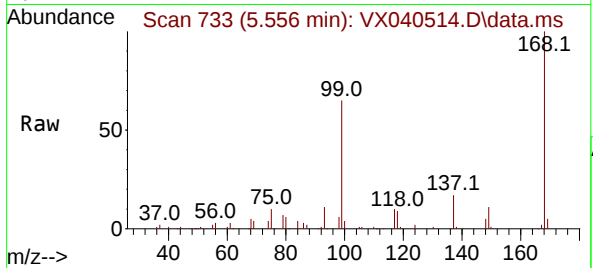

#11
Tert butyl alcohol
Concen: 6.400 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.000 min
Lab File: VX040514.D
Acq: 28 Feb 2024 16:26

Tgt Ion: 59 Resp: 1360
Ion Ratio Lower Upper
59 100
57 4.6 6.0 9.0#


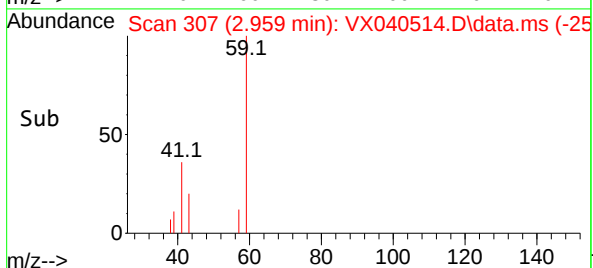
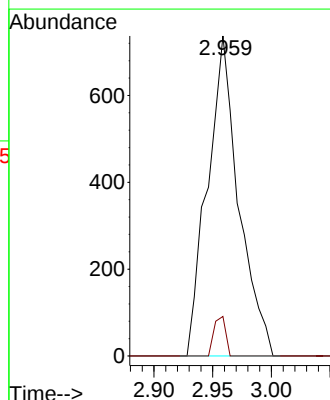
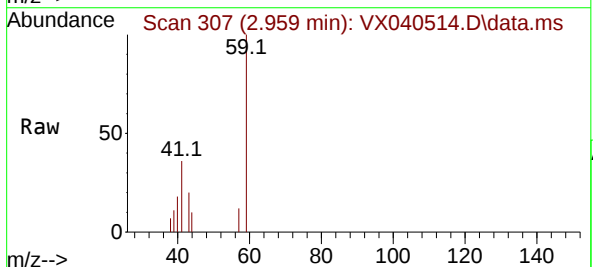


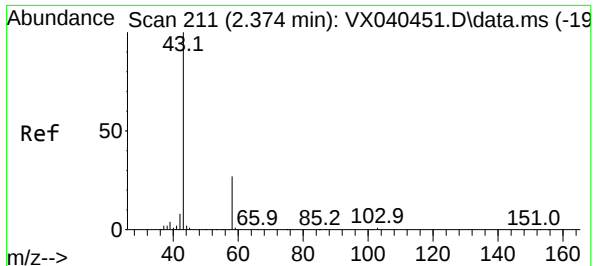

#16
Acetone
Concen: 53.972 ug/l
RT: 2.380 min Scan# 211
Delta R.T. 0.006 min
Lab File: VX040514.D
Acq: 28 Feb 2024 16:26




Instrument :
MSVOA_X
ClientSampleId :
1847


Tgt Ion: 43 Resp: 22248
Ion Ratio Lower Upper
43 100
58 24.8 21.9 32.9

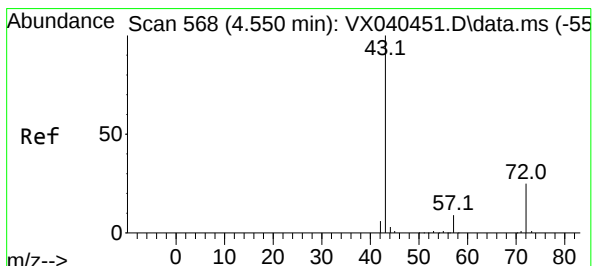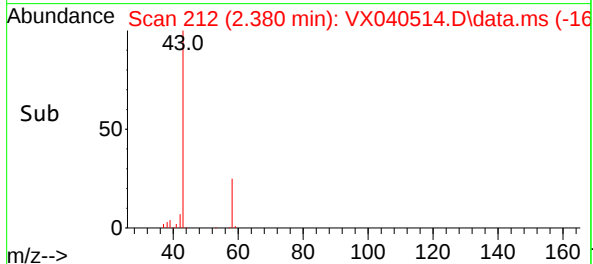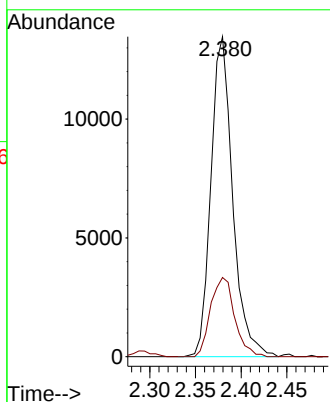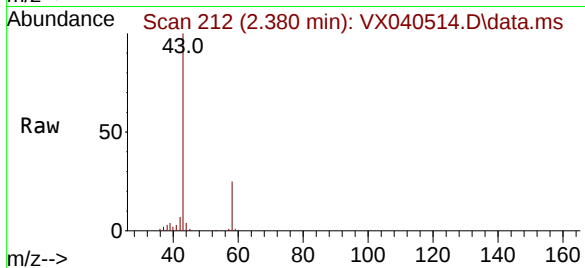

#25
2-Butanone
Concen: 2.047 ug/l
RT: 4.586 min Scan# 574
Delta R.T. 0.036 min
Lab File: VX040514.D
Acq: 28 Feb 2024 16:26

Tgt Ion: 43 Resp: 1470
Ion Ratio Lower Upper
43 100
72 16.4 19.4 29.2#

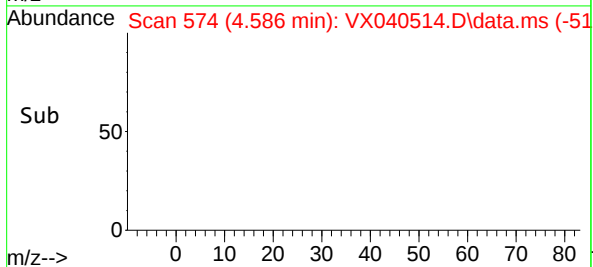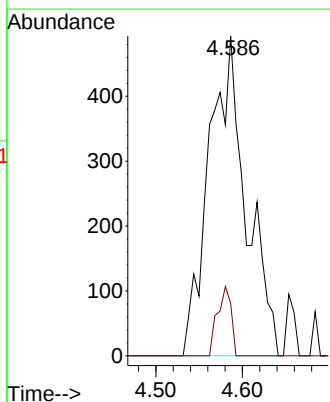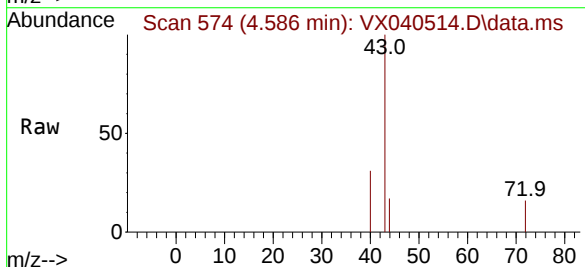

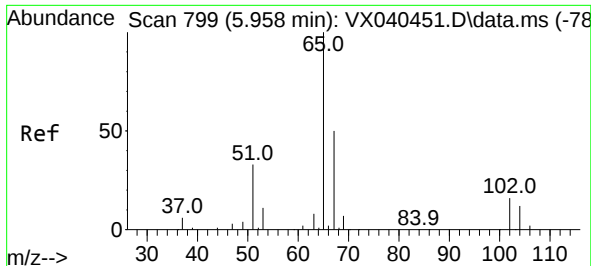

#33

1,2-Dichloroethane-d4

Concen: 49.364 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX040514.D

Acq: 28 Feb 2024 16:26

Instrument :

MSVOA_X

ClientSampleId :





1847

Tgt Ion: 65 Resp: 62396

Ion Ratio Lower Upper

65 100

67 50.2 0.0 100.2

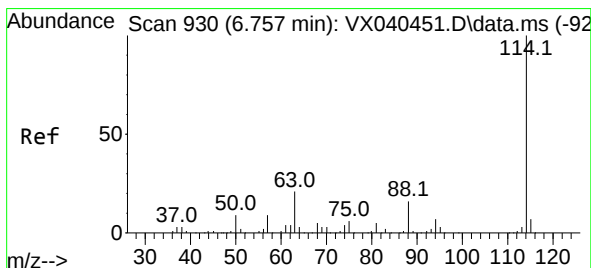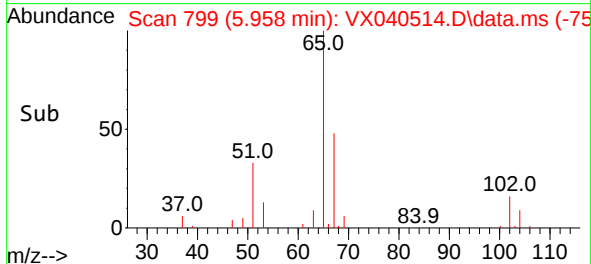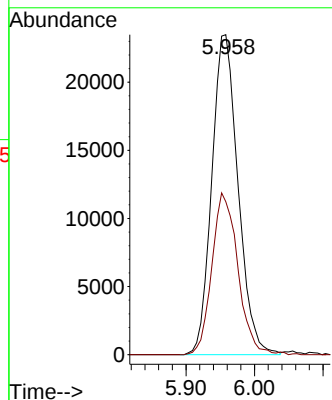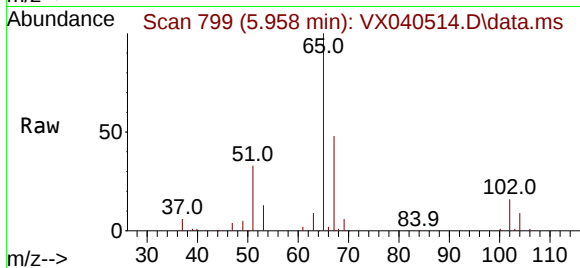

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX040514.D

Acq: 28 Feb 2024 16:26




Tgt Ion: 114 Resp: 132767


Ion Ratio Lower Upper

114 100

63 22.0 0.0 45.0

88 16.1 0.0 36.6

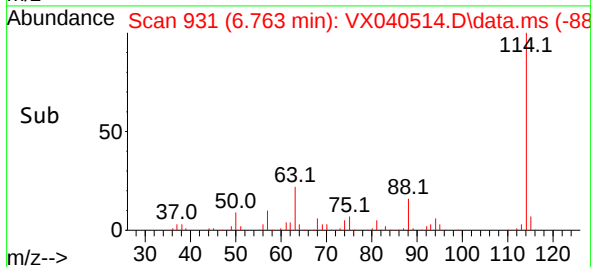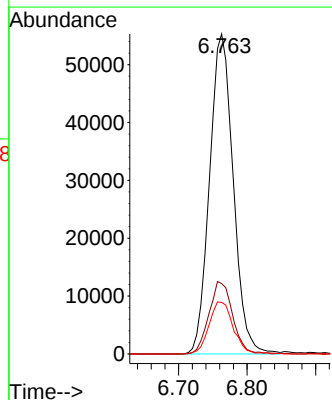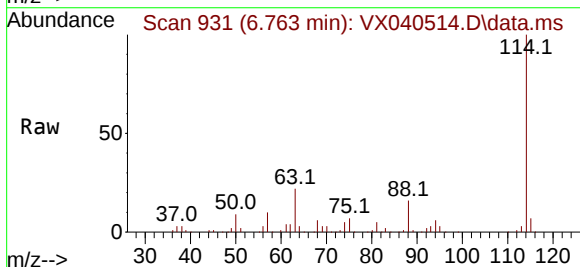

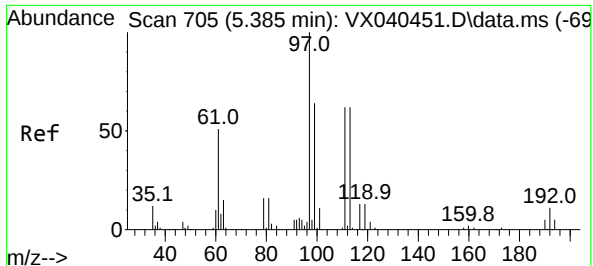

#35

Dibromofluoromethane

Concen: 48.264 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.000 min

Lab File: VX040514.D


Acq: 28 Feb 2024 16:26

Instrument :

MSVOA_X

ClientSampleId :

1847

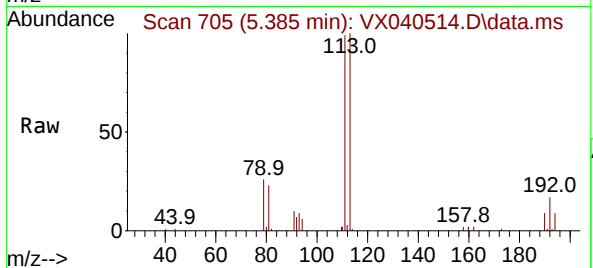




Tgt Ion:113 Resp: 44560

Ion Ratio Lower Upper

113 100

111 104.0 82.9 124.3

192 18.1 13.3 19.9

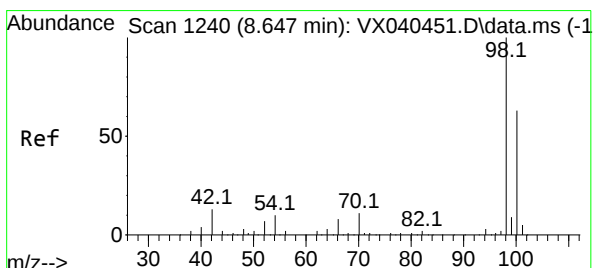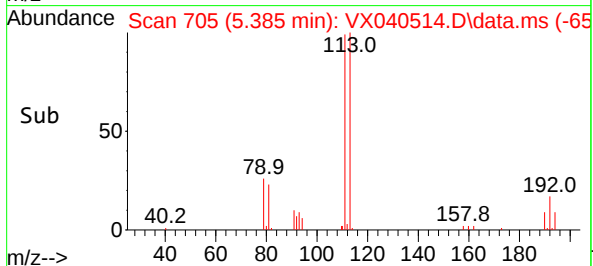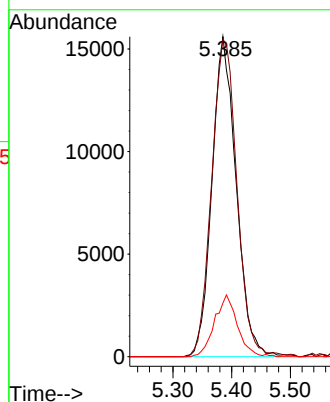

#50

Toluene-d8

Concen: 48.196 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX040514.D




Acq: 28 Feb 2024 16:26


Tgt Ion: 98 Resp: 161519

Ion Ratio Lower Upper

98 100

100 63.7 53.1 79.7

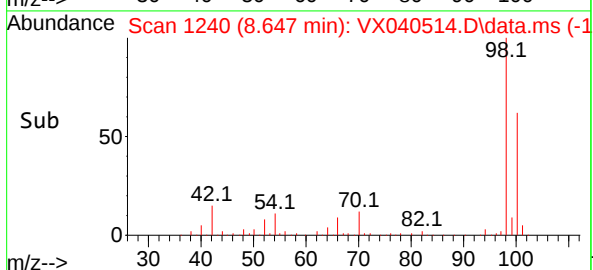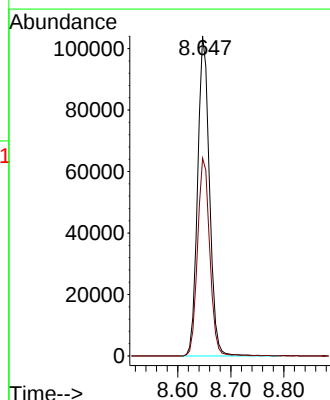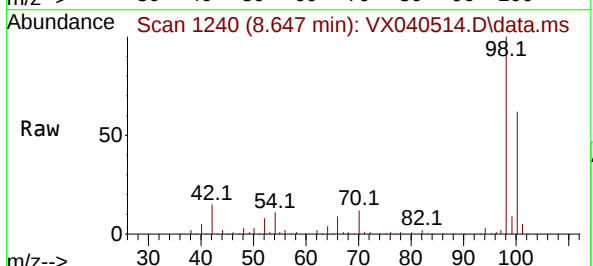

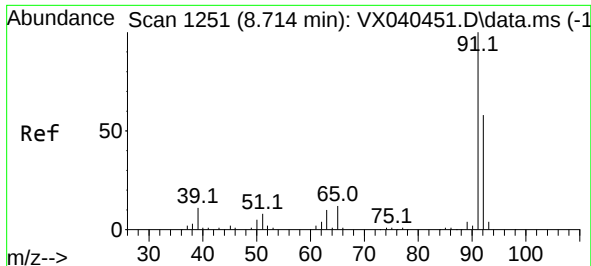

#52

Toluene

Concen: 0.496 ug/l

RT: 8.720 min Scan# 1172

Delta R.T. 0.006 min

Lab File: VX040514.D

Acq: 28 Feb 2024 16:26

Instrument :

MSVOA_X

ClientSampleId :





1847

Tgt Ion: 92 Resp: 1172

Ion Ratio Lower Upper

92 100

91 195.0 134.2 201.2

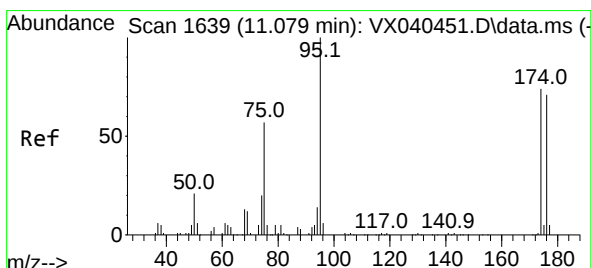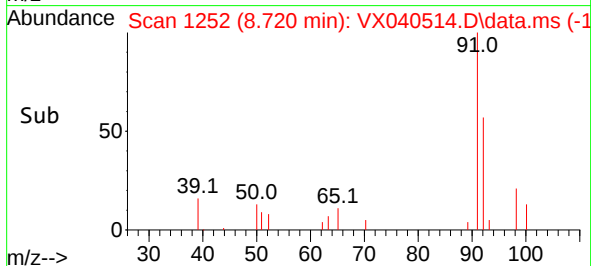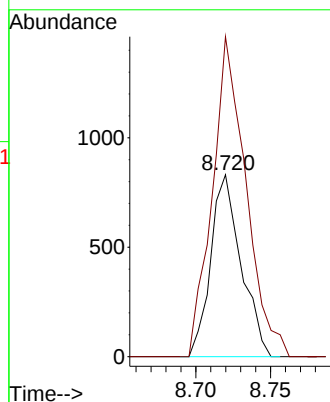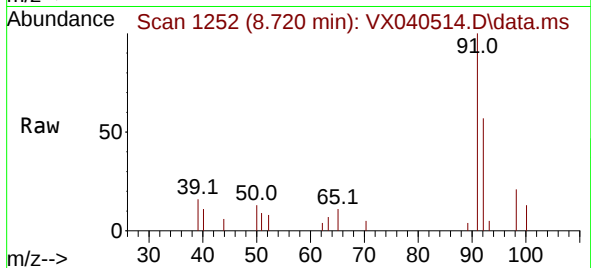

#62

4-Bromofluorobenzene

Concen: 51.999 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX040514.D

Acq: 28 Feb 2024 16:26




Tgt Ion: 95 Resp: 66428


Ion Ratio Lower Upper

95 100

174 74.2 0.0 135.6

176 71.4 0.0 131.0


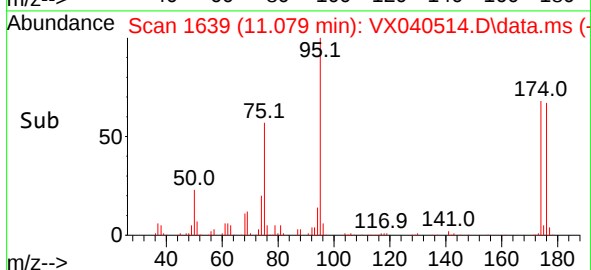
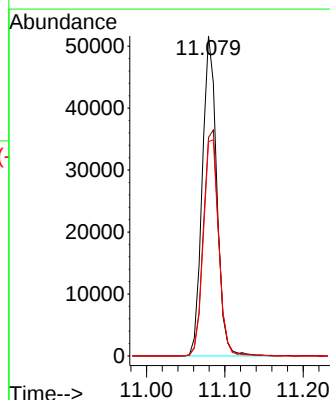
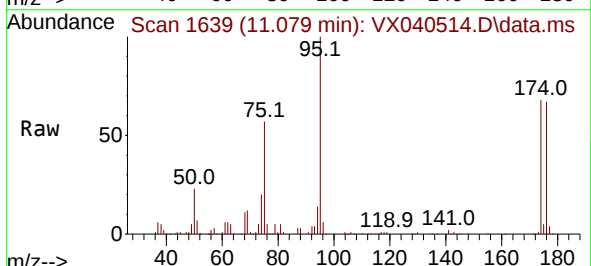


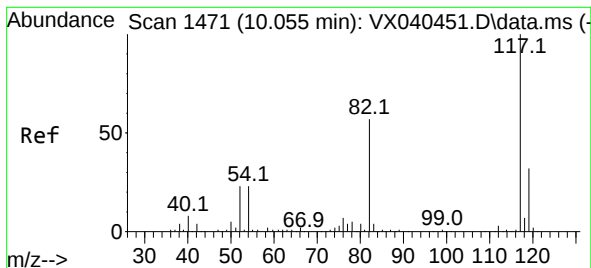

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX040514.D
Acq: 28 Feb 2024 16:26




Instrument :
MSVOA_X
ClientSampleId :
1847


Tgt Ion:117 Resp: 129141
Ion Ratio Lower Upper
117 100
82 56.7 46.2 69.4
119 32.3 25.5 38.3

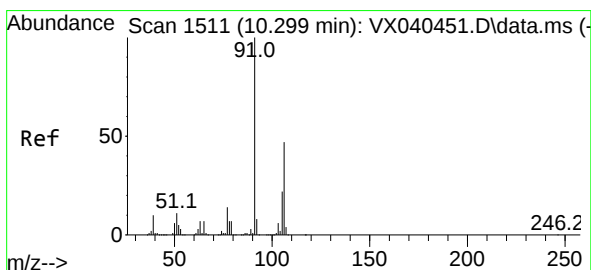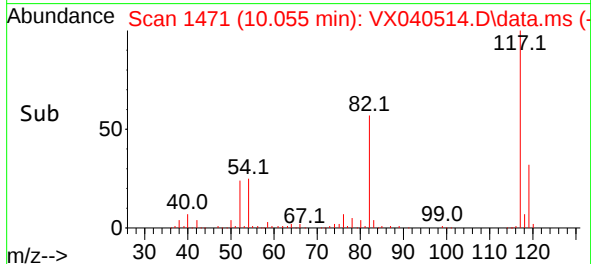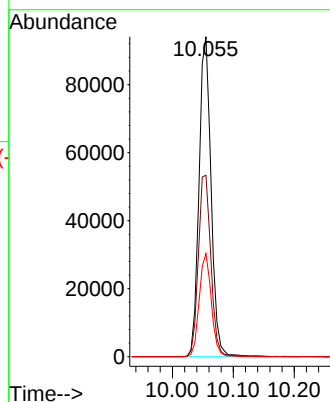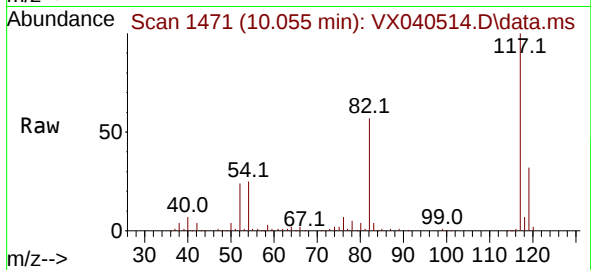

#68
m/p-Xylenes
Concen: 0.537 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX040514.D
Acq: 28 Feb 2024 16:26

Tgt Ion:106 Resp: 1009
Ion Ratio Lower Upper
106 100
91 222.7 165.5 248.3


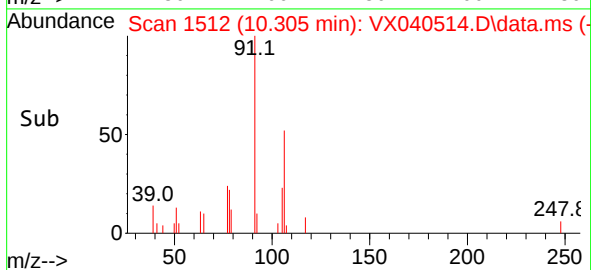
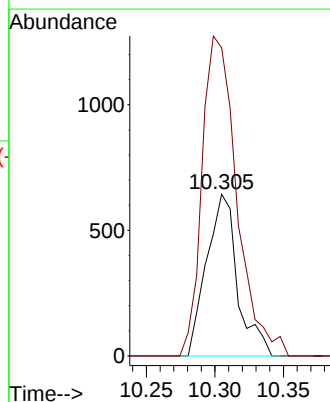
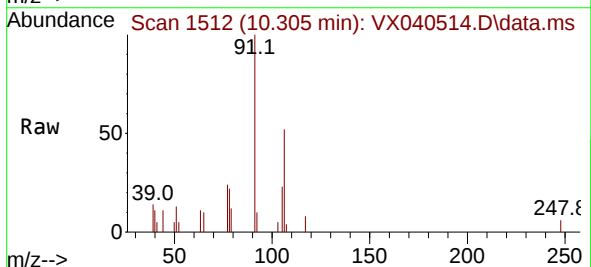


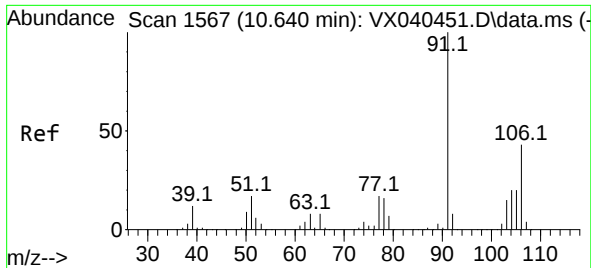

#69
o-Xylene
Concen: 0.217 ug/l
RT: 10.646 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX040514.D
Acq: 28 Feb 2024 16:26

Instrument :
MSVOA_X
ClientSampleId :
1847

Tgt Ion:106 Resp: 389
Ion Ratio Lower Upper
106 100
91 229.0 108.9 326.8

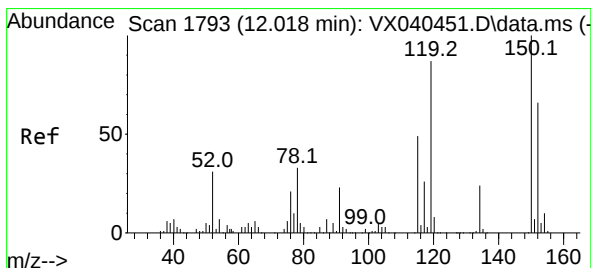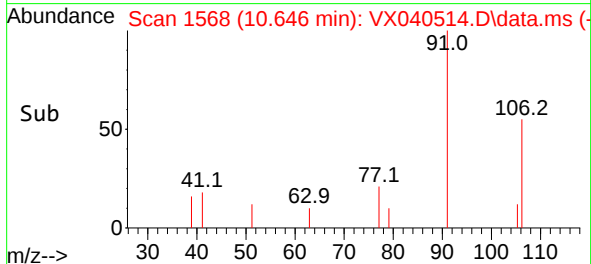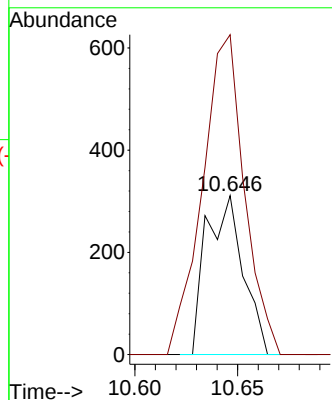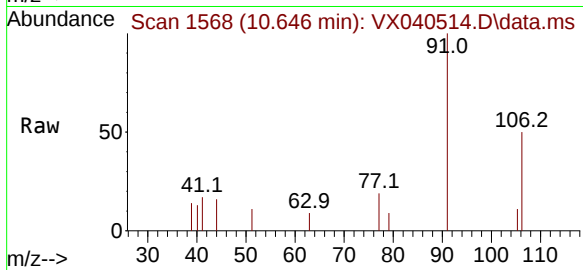

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX040514.D
Acq: 28 Feb 2024 16:26

Tgt Ion:152 Resp: 65883
Ion Ratio Lower Upper
152 100
115 62.2 43.3 129.9
150 157.7 0.0 345.0

