

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022824\
 Data File : VX040523.D
 Acq On : 28 Feb 2024 19:52
 Operator : JC/MD
 Sample : P1615-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GM38-RW3-MW1-20240226

Quant Time: Feb 29 03:55:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 27 05:01:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	73400	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	130582	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	126910	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	65670	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	61716	50.271	ug/l	0.00
Spiked Amount	50.000	Range 78 - 117	Recovery	= 100.540%		
35) Dibromofluoromethane	5.385	113	43476	47.878	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	= 95.760%		
50) Toluene-d8	8.647	98	159908	48.514	ug/l	0.00
Spiked Amount	50.000	Range 92 - 112	Recovery	= 97.020%		
62) 4-Bromofluorobenzene	11.079	95	63567	50.592	ug/l	0.00
Spiked Amount	50.000	Range 83 - 123	Recovery	= 101.180%		
Target Compounds						
					Qvalue	
9) 1,1,2-Trichlorotrifluo...	2.331	101	524	0.629	ug/l	91
16) Acetone	2.380	43	808	2.018	ug/l #	81
30) Chloroform	5.105	83	610	0.335	ug/l #	82
44) Trichloroethene	7.129	130	18342	18.006	ug/l	93
52) Toluene	8.720	92	3086	1.328	ug/l	91
64) Tetrachloroethene	9.275	164	1291	1.449	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022824\
Data File : VX040523.D
Acq On : 28 Feb 2024 19:52
Operator : JC/MD
Sample : P1615-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GM38-RW3-MW1-20240226

Quant Time: Feb 29 03:55:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 27 05:01:33 2024
Response via : Initial Calibration




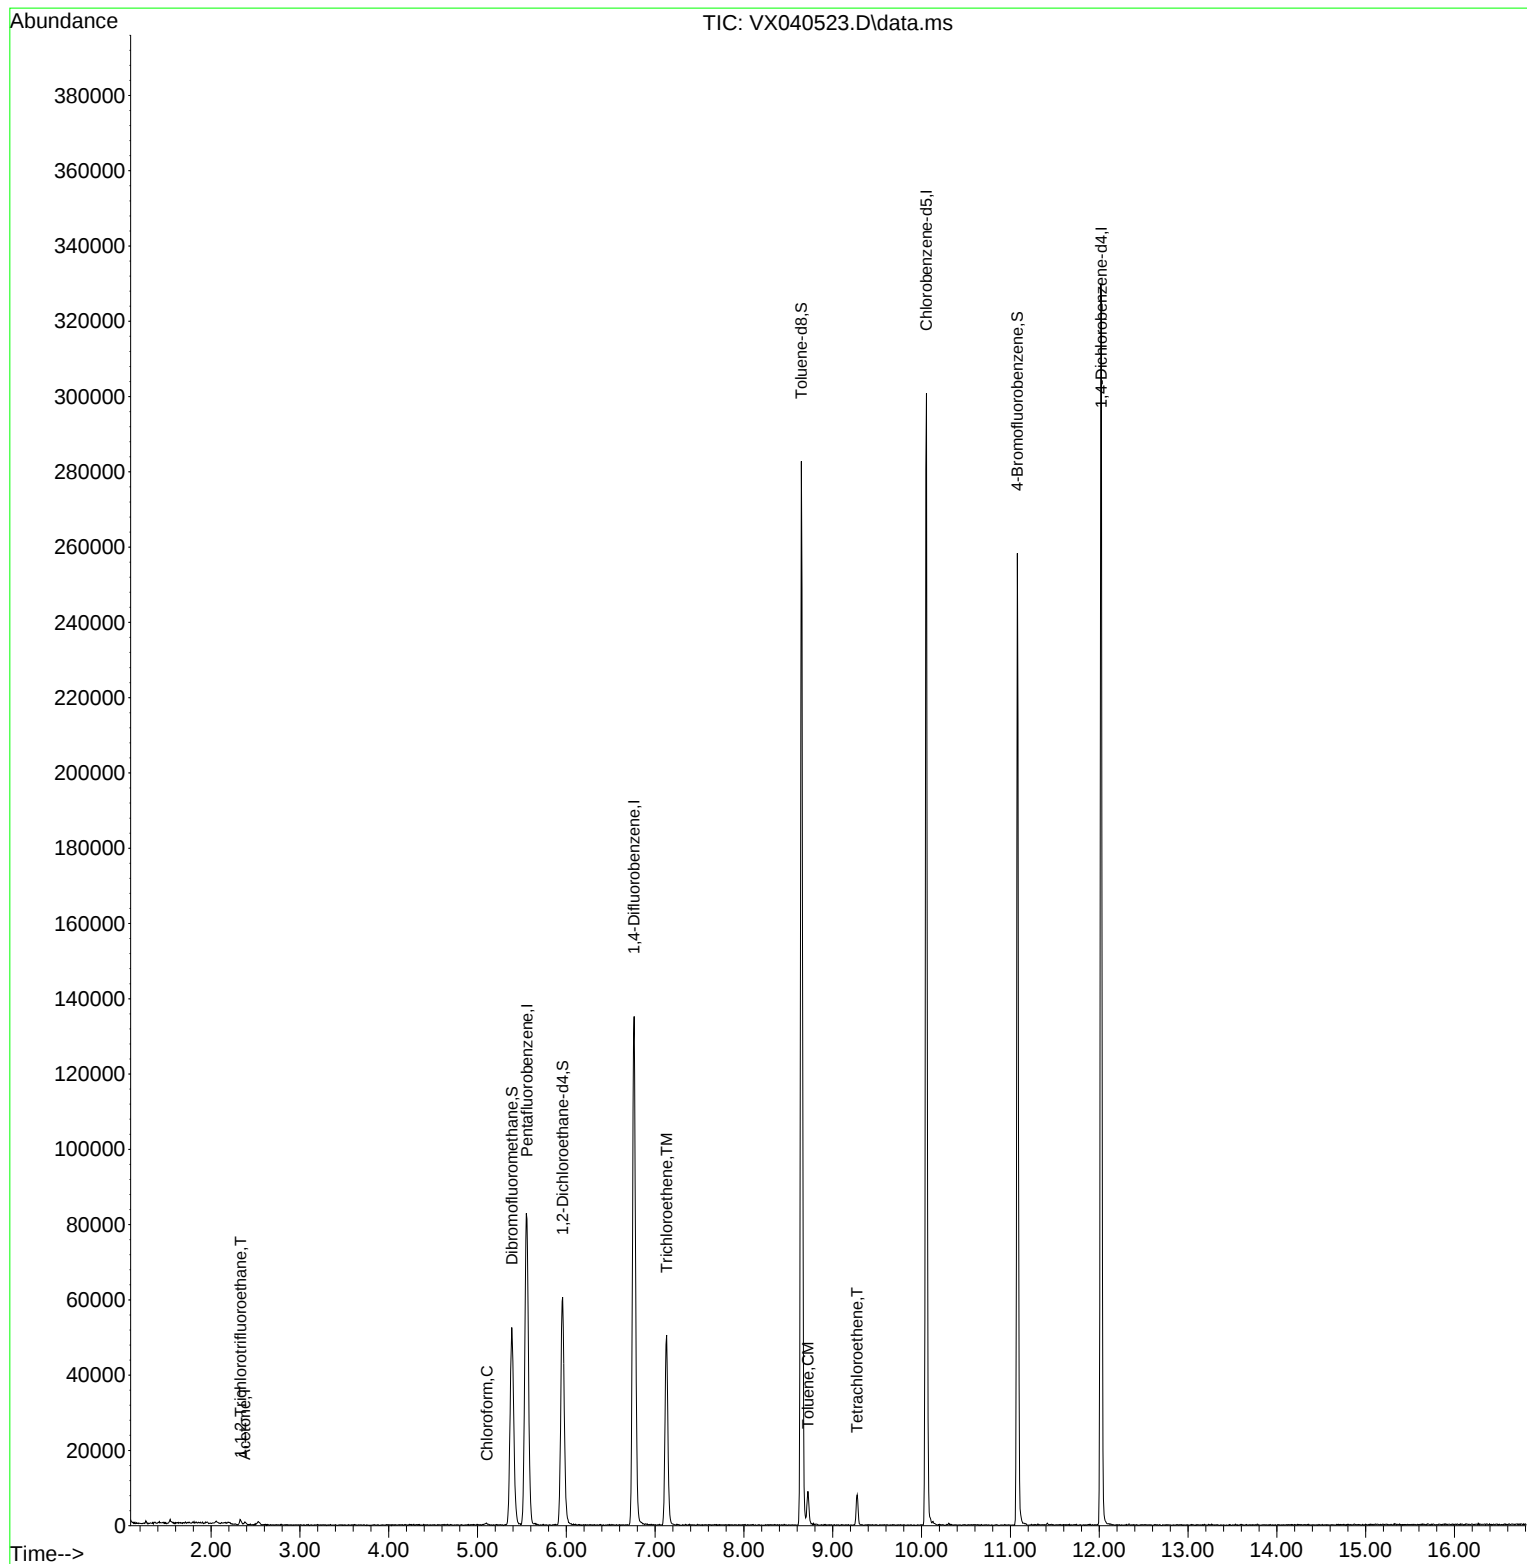


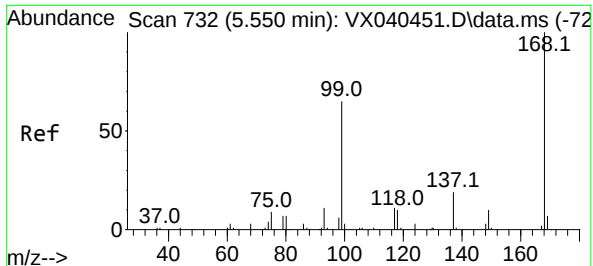

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. 0.006 min
Lab File: VX040523.D
Acq: 28 Feb 2024 19:52




Instrument :
MSVOA_X
ClientSampleId :
GM38-RW3-MW1-20240226


Tgt Ion:168 Resp: 73400
Ion Ratio Lower Upper
168 100
99 67.9 56.6 85.0

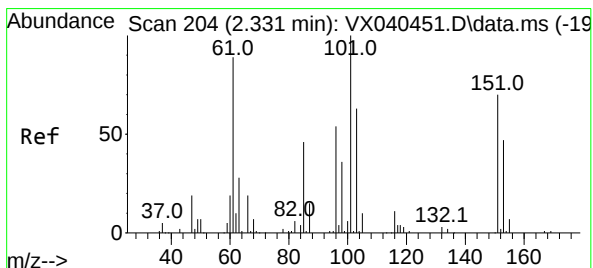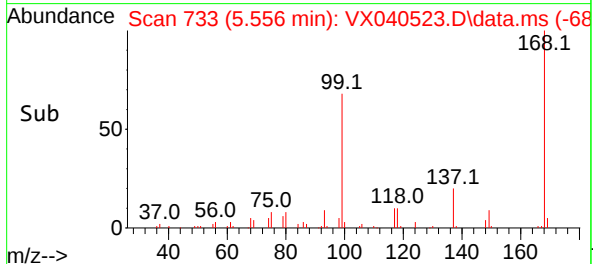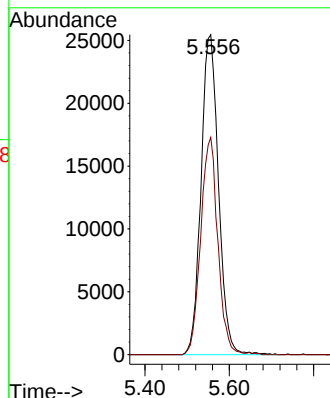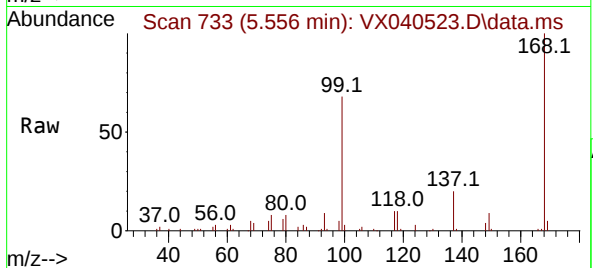

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.629 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX040523.D
Acq: 28 Feb 2024 19:52

Tgt Ion:101 Resp: 524
Ion Ratio Lower Upper
101 100
85 48.5 37.0 55.6
151 84.0 58.6 87.8


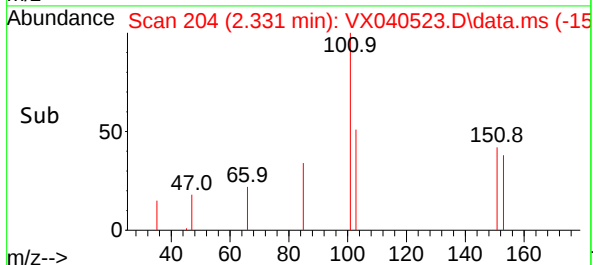
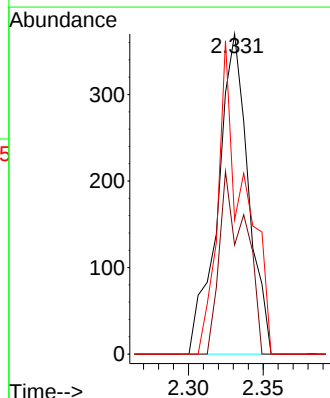
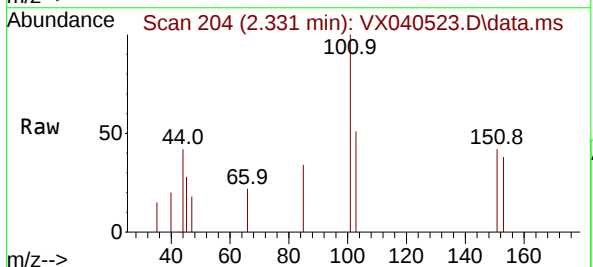


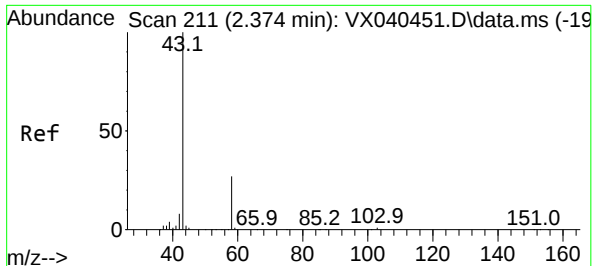

#16
Acetone
Concen: 2.018 ug/l
RT: 2.380 min Scan# 211
Delta R.T. 0.006 min
Lab File: VX040523.D
Acq: 28 Feb 2024 19:52




Instrument :
MSVOA_X
ClientSampleId :
GM38-RW3-MW1-20240226


Tgt Ion: 43 Resp: 808
Ion Ratio Lower Upper
43 100
58 37.5 21.9 32.9#

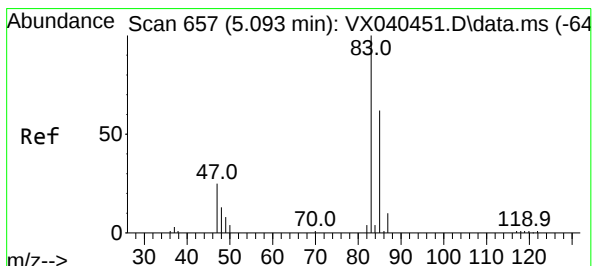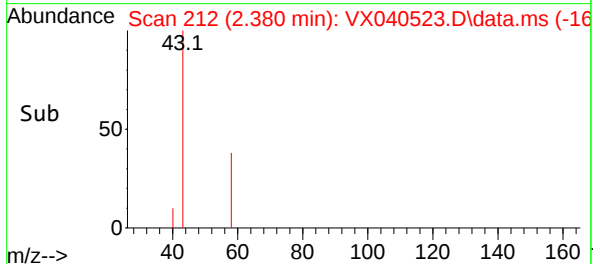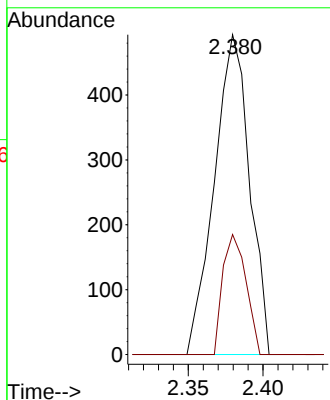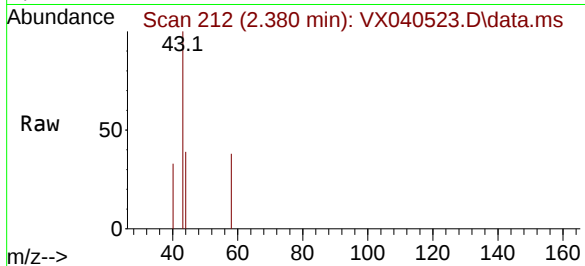

#30
Chloroform
Concen: 0.335 ug/l
RT: 5.105 min Scan# 659
Delta R.T. 0.012 min
Lab File: VX040523.D
Acq: 28 Feb 2024 19:52

Tgt Ion: 83 Resp: 610
Ion Ratio Lower Upper
83 100
85 48.8 50.3 75.5#

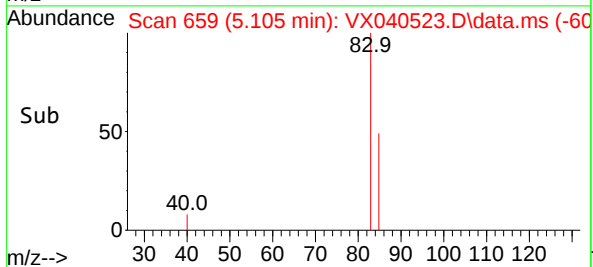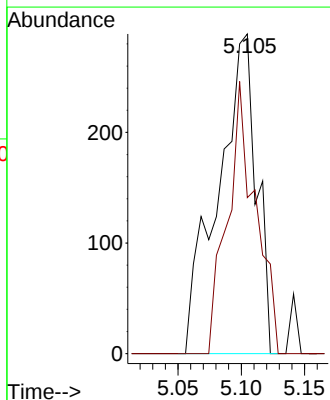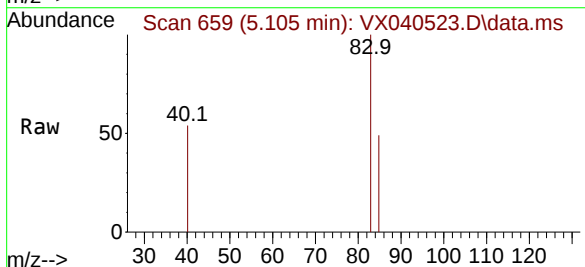

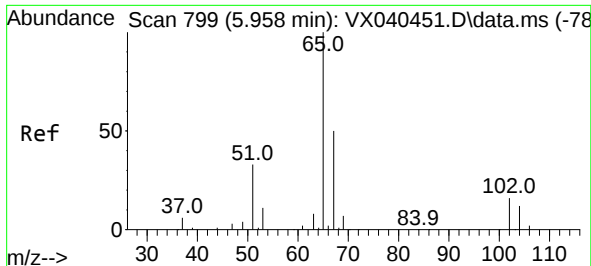

#33

1,2-Dichloroethane-d4

Concen: 50.271 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX040523.D

Acq: 28 Feb 2024 19:52

Instrument :

MSVOA_X

ClientSampleId :





GM38-RW3-MW1-20240226

Tgt Ion: 65 Resp: 61716

Ion Ratio Lower Upper

65 100

67 49.2 0.0 100.2

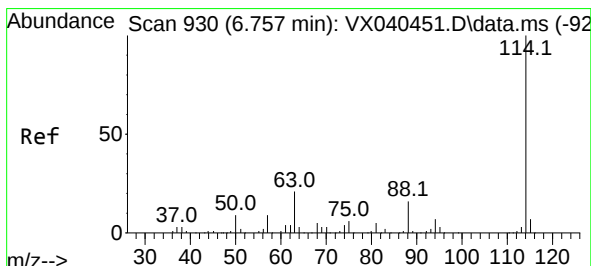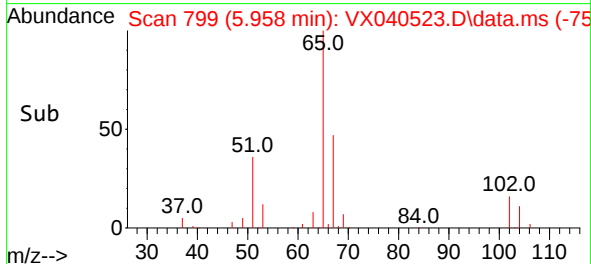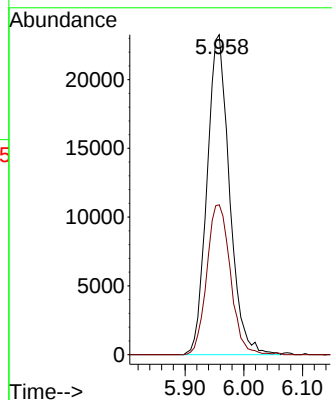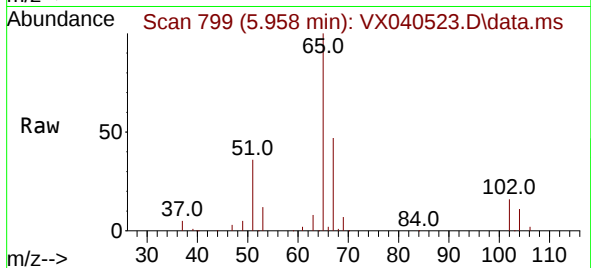

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX040523.D

Acq: 28 Feb 2024 19:52




Tgt Ion: 114 Resp: 130582


Ion Ratio Lower Upper

114 100

63 22.6 0.0 45.0

88 15.9 0.0 36.6


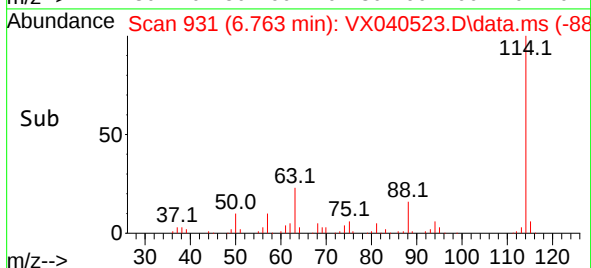
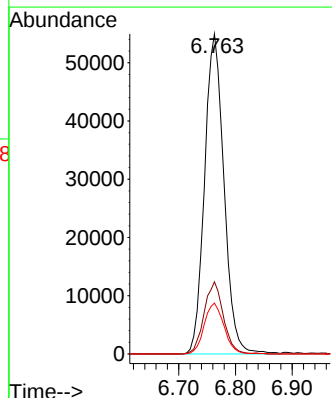
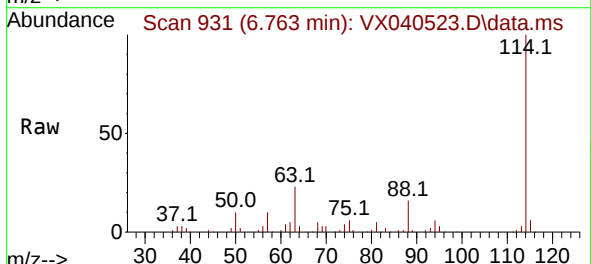


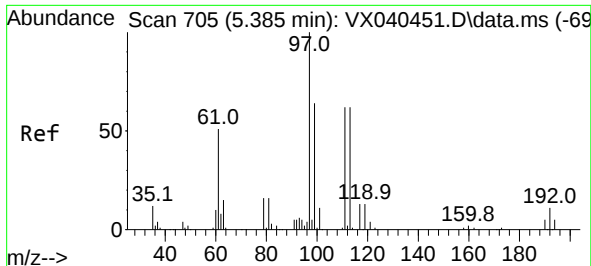

#35
Dibromofluoromethane
Concen: 47.878 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX040523.D
Acq: 28 Feb 2024 19:52




Instrument :
MSVOA_X
ClientSampleId :
GM38-RW3-MW1-20240226


Tgt Ion:113 Resp: 43476
Ion Ratio Lower Upper
113 100
111 103.5 82.9 124.3
192 17.5 13.3 19.9

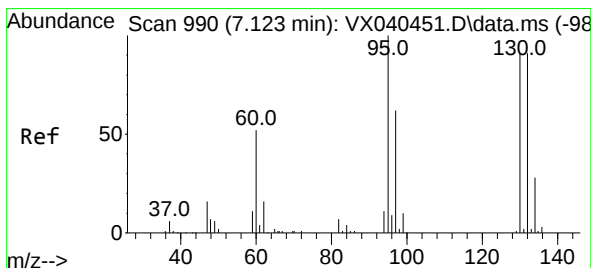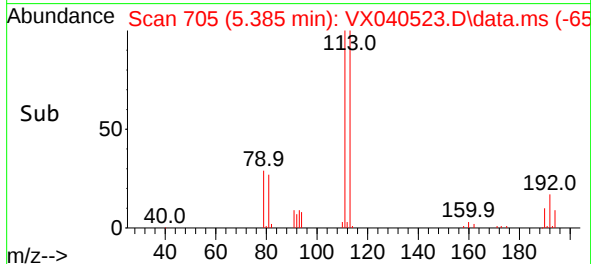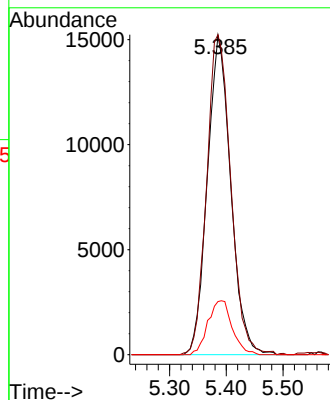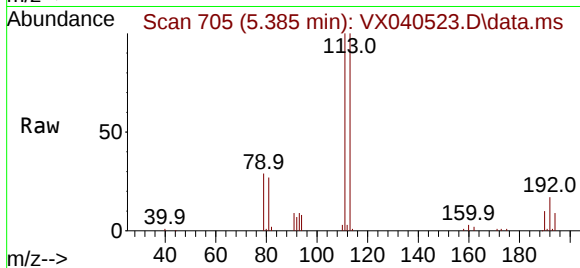

#44
Trichloroethene
Concen: 18.006 ug/l
RT: 7.129 min Scan# 991
Delta R.T. 0.006 min
Lab File: VX040523.D
Acq: 28 Feb 2024 19:52

Tgt Ion:130 Resp: 18342
Ion Ratio Lower Upper
130 100
95 109.6 0.0 204.4


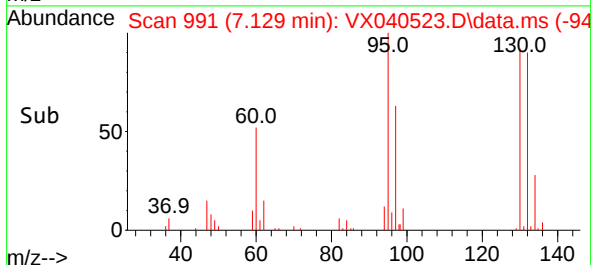
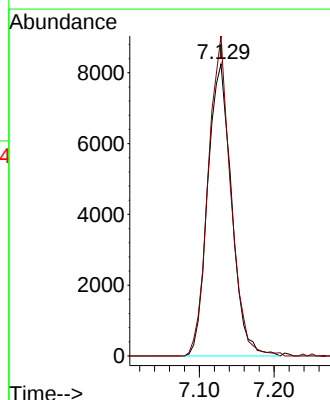
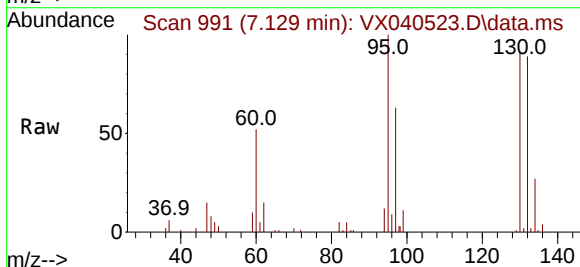


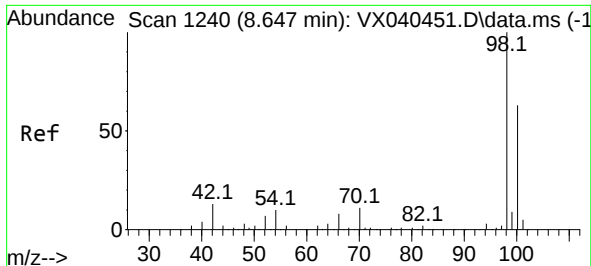

#50
Toluene-d8
Concen: 48.514 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX040523.D
Acq: 28 Feb 2024 19:52




Instrument :
MSVOA_X
ClientSampleId :
GM38-RW3-MW1-20240226


Tgt Ion: 98 Resp: 159908
Ion Ratio Lower Upper
98 100
100 62.9 53.1 79.7

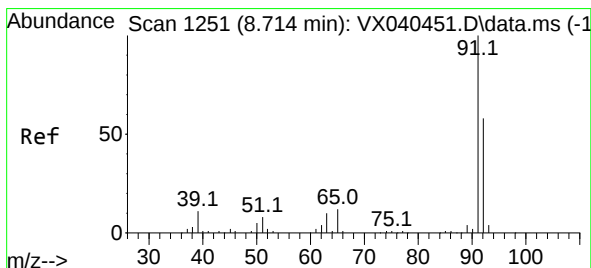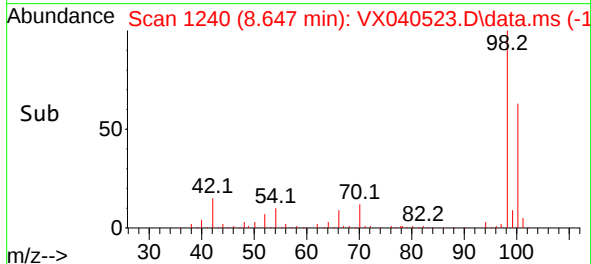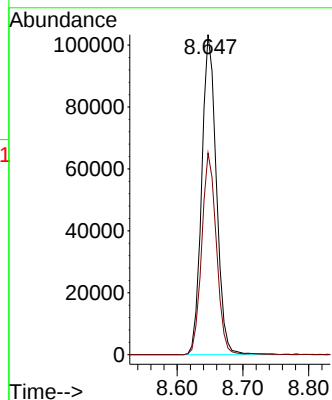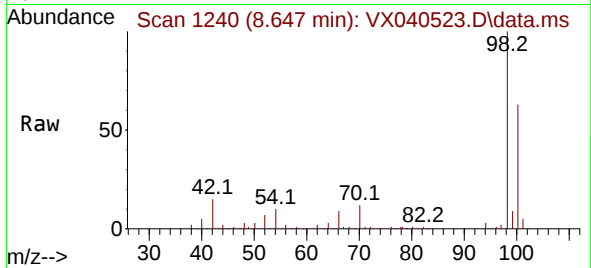

#52
Toluene
Concen: 1.328 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.006 min
Lab File: VX040523.D
Acq: 28 Feb 2024 19:52

Tgt Ion: 92 Resp: 3086
Ion Ratio Lower Upper
92 100
91 180.2 134.2 201.2

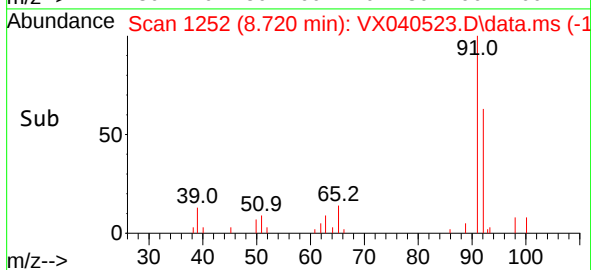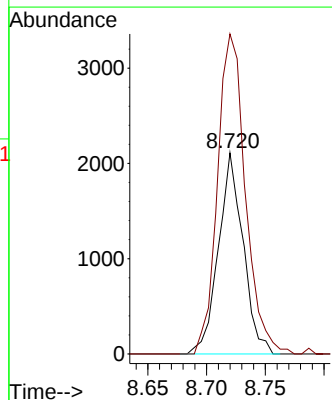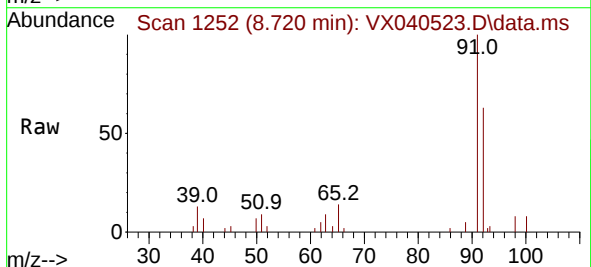

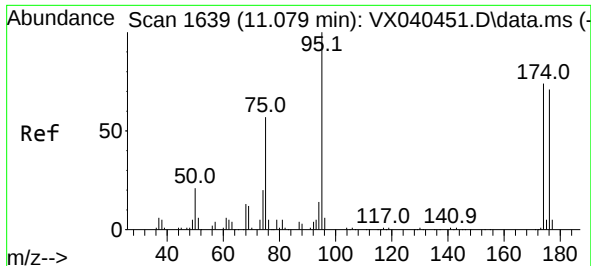

#62

4-Bromofluorobenzene

Concen: 50.592 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX040523.D

Acq: 28 Feb 2024 19:52

Instrument :

MSVOA_X

ClientSampleId :

GM38-RW3-MW1-20240226





Tgt Ion: 95 Resp: 63567

Ion Ratio Lower Upper

95 100

174 75.5 0.0 135.6

176 73.2 0.0 131.0

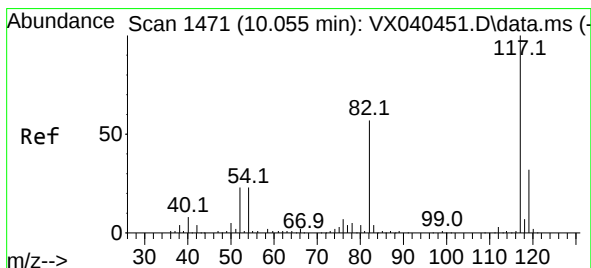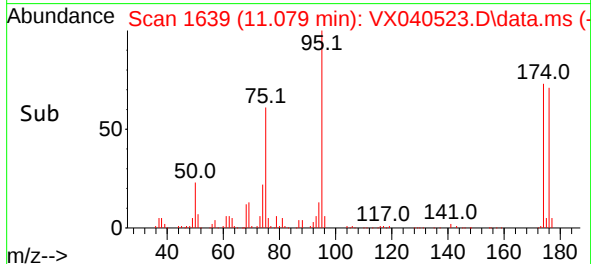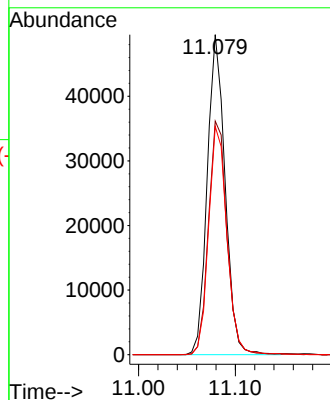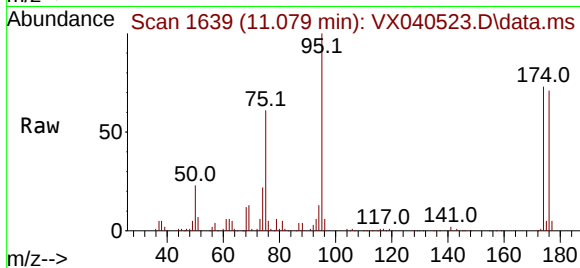

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX040523.D

Acq: 28 Feb 2024 19:52




Tgt Ion: 117 Resp: 126910


Ion Ratio Lower Upper

117 100

82 59.6 46.2 69.4

119 32.1 25.5 38.3

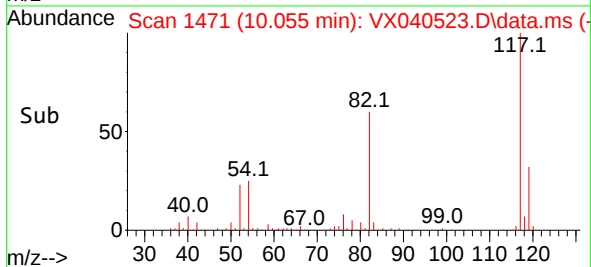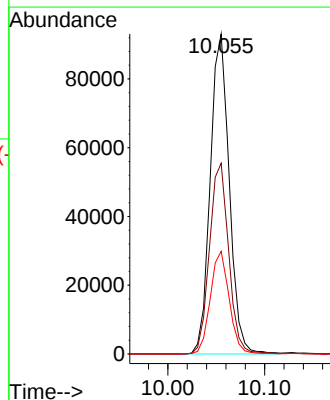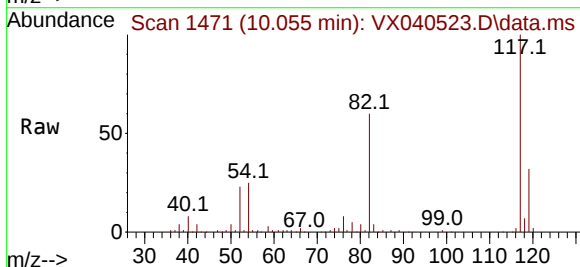




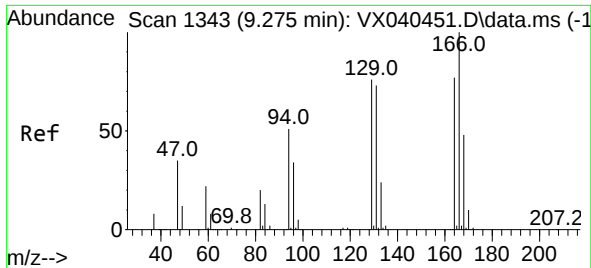


#64
Tetrachloroethene
Concen: 1.449 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX040523.D
Acq: 28 Feb 2024 19:52

Instrument :
MSVOA_X
ClientSampleId :
GM38-RW3-MW1-20240226

Tgt Ion:164 Resp: 1291

Ion	Ratio	Lower	Upper
164	100		
166	126.3	102.7	154.1
129	87.9	80.4	120.6
131	92.5	76.5	114.7

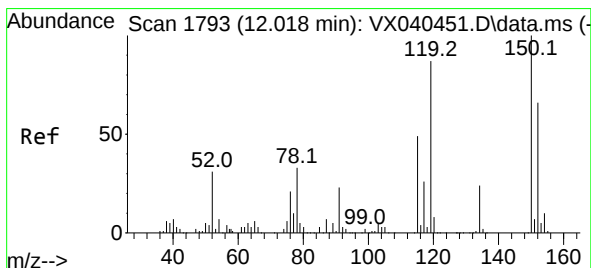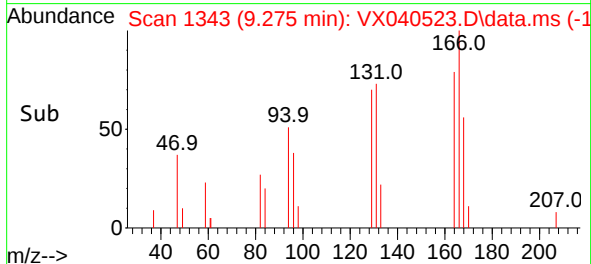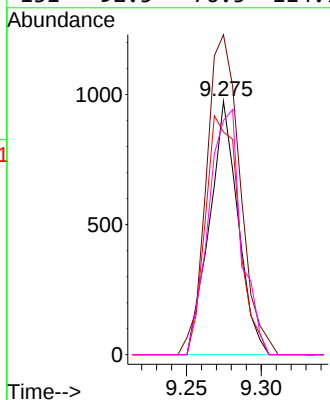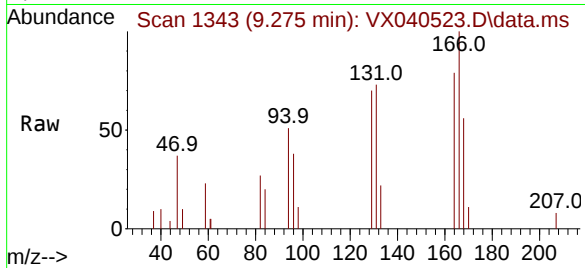

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX040523.D
Acq: 28 Feb 2024 19:52

Tgt Ion:152 Resp: 65670

Ion	Ratio	Lower	Upper
152	100		
115	63.1	43.3	129.9
150	154.5	0.0	345.0

