
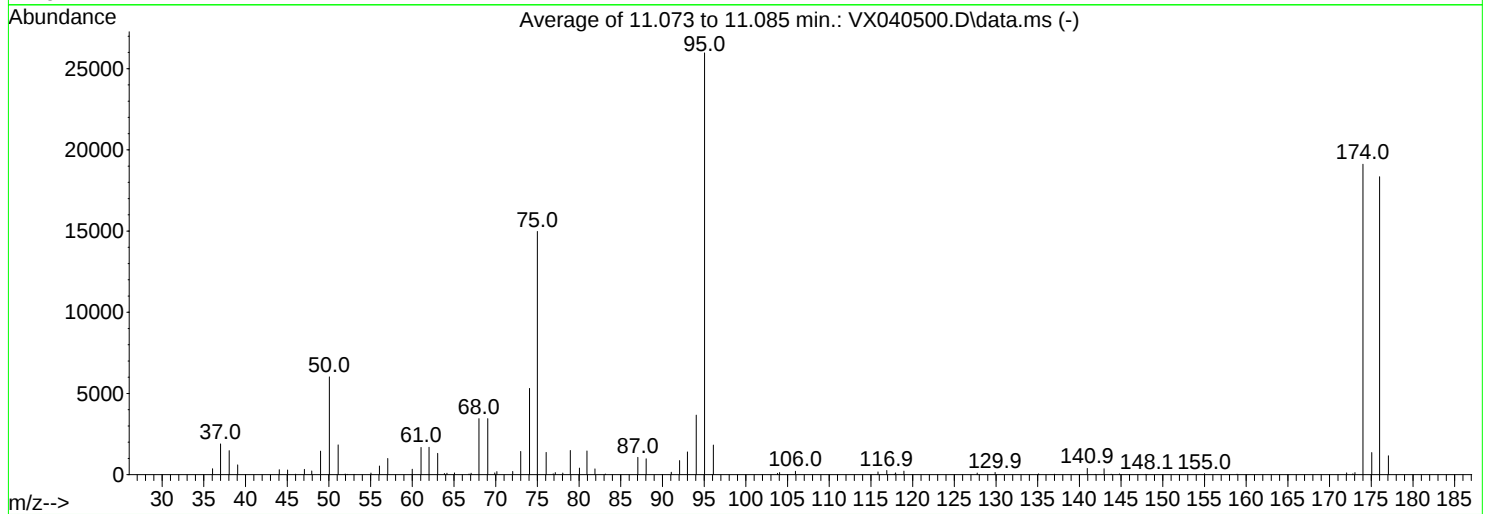


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022824\
Data File : VX040500.D
Acq On : 28 Feb 2024 09:29
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
Title : SW846 8260
Last Update : Tue Feb 27 05:01:33 2024

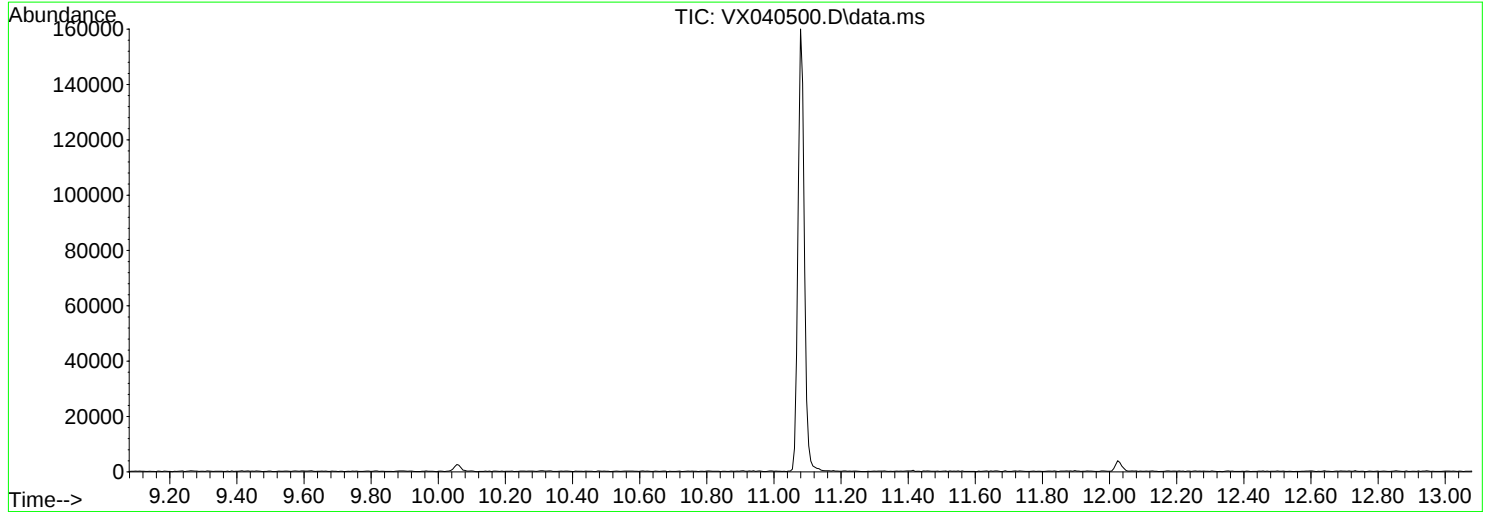

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	6025	PASS
75	95	30	60	57.7	14974	PASS
95	95	100	100	100.0	25973	PASS
96	95	5	9	7.0	1827	PASS
173	174	0.00	2	0.7	128	PASS
174	95	50	100	73.6	19110	PASS
175	174	5	9	7.1	1358	PASS
176	174	95	101	96.0	18344	PASS
177	176	5	9	6.3	1159	PASS